

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
 Data File : PP052241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 19:35
 Operator : YP\AJ
 Sample : N5098-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 250FERRYBLVD-PCB-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 05:40:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 12 05:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.423	3.673	23819270	18028036	15.154	15.736
2) SA Decachlor...	10.239	8.767	159.4E6	115.6E6	114.825	103.433
Target Compounds						
3) L1 AR-1016-1	5.596	4.777	1176753	3777746	25.877	84.939 #
4) L1 AR-1016-2	5.620	4.795	5814476	2931967	88.323	46.077 #
5) L1 AR-1016-3	5.683	4.976	4604269	3989980	110.639	120.034
6) L1 AR-1016-4	5.761f	5.017	28232876	15517198	777.023	569.329 #
8) L2 AR-1221-1	4.632	3.893	3897303	5734189	188.601	366.741 #
9) L2 AR-1221-2	4.716	3.979	5338207	11593161	348.827	966.677 #
10) L2 AR-1221-3	4.795	4.055	6939628	14889695	148.210	393.958 #
11) L3 AR-1232-1	4.795	4.055	6939628	14889695	192.624	513.759 #
12) L3 AR-1232-2	5.311f	4.795	25846504	2931967	1273.870	97.879 #
13) L3 AR-1232-3	5.620	4.976	5814476	3989980	193.070	261.168 #
14) L3 AR-1232-4	5.761f	5.060	28232876	7685558	1692.853	542.745 #
15) L3 AR-1232-5	5.873	5.234	19094931	2745696	1273.189	173.446 #
16) L4 AR-1242-1	5.596	4.777	1176753	3777746	33.829	108.499 #
17) L4 AR-1242-2	5.620	4.795	5814476	2931967	117.449	59.434 #
18) L4 AR-1242-3	5.683	4.976	4604269	3989980	145.211	152.850
19) L4 AR-1242-4	5.761f	5.060	28232876	7685558	1033.586	282.557 #
20) L4 AR-1242-5	6.524	5.594	34703331	81317338	933.446	2412.972 #
21) L5 AR-1248-1	5.596	4.777	1176753	3777746	43.774	139.341 #
22) L5 AR-1248-2	5.873	5.017	19094931	15517198	410.800	417.079
23) L5 AR-1248-3	6.077	5.060	-9639966	7685558	N.D.	201.740 #
24) L5 AR-1248-4	6.458f	5.234	125.1E6	2745696	1970.946	59.257 #
25) L5 AR-1248-5	6.524	5.634	34703331	13581862	560.319	322.968 #
26) L6 AR-1254-1	6.458	5.594	125.1E6	81317338	1757.857	1162.297 #
27) L6 AR-1254-2	6.677	5.742	143.8E6	74783135	1347.978	1193.576
28) L6 AR-1254-3	7.045	6.165f	120.1E6	260.8E6	1142.403	2636.770 #
29) L6 AR-1254-4	7.330	6.382	104.5E6	73441974	1430.481	1228.594
30) L6 AR-1254-5	7.747	6.804	390.9E6	208.6E6	4710.836	2353.146 #
31) L7 AR-1260-1	7.209	6.283	227.4E6	188.6E6	2743.137	2737.859
32) L7 AR-1260-2	7.466	6.472	403.0E6	328.8E6	4269.411	3972.389
33) L7 AR-1260-3	7.828	6.632	1336.2E6	326.2E6	22248.619	4224.778 #
34) L7 AR-1260-4	8.055	7.104	600.7E6	769.5E6	7831.985	13688.821 #
35) L7 AR-1260-5	8.378	7.348	1864.8E6	1644.2E6	13603.800	12467.809
36) L8 AR-1262-1	7.828	6.896	1336.2E6	409.9E6	13780.660	11395.681
37) L8 AR-1262-2	8.378	7.104	1864.8E6	769.5E6	11581.827	9718.027
38) L8 AR-1262-3	8.694	7.634	2344.8E6	1766.4E6	21336.083	28605.189 #
39) L8 AR-1262-4	8.790	7.699	2646.1E6	2253.6E6	51763.084	19740.016 #
40) L8 AR-1262-5	9.460	8.200	1634.2E6	1230.8E6	25960.658	24215.021
41) L9 AR-1268-1	8.694	7.634	2344.8E6	1766.4E6	11843.844	9737.218
42) L9 AR-1268-2	8.790	7.699	2646.1E6	2253.6E6	14410.352	13792.926

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
 Data File : PP052241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 19:35
 Operator : YP\AJ
 Sample : N5098-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 250FERRYBLVD-PCB-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 05:40:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 12 05:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	9.024	7.908	498.6E6	367.5E6	3058.905	2613.545
44) L9	AR-1268-4	9.460	8.200	1634.2E6	1230.8E6	22397.959	21779.982
45) L9	AR-1268-5	9.888	8.501	2349.4E6	1736.8E6	4505.611	4128.634



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
Data File : PP052241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 19:35
Operator : YP\AJ
Sample : N5098-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 05:40:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

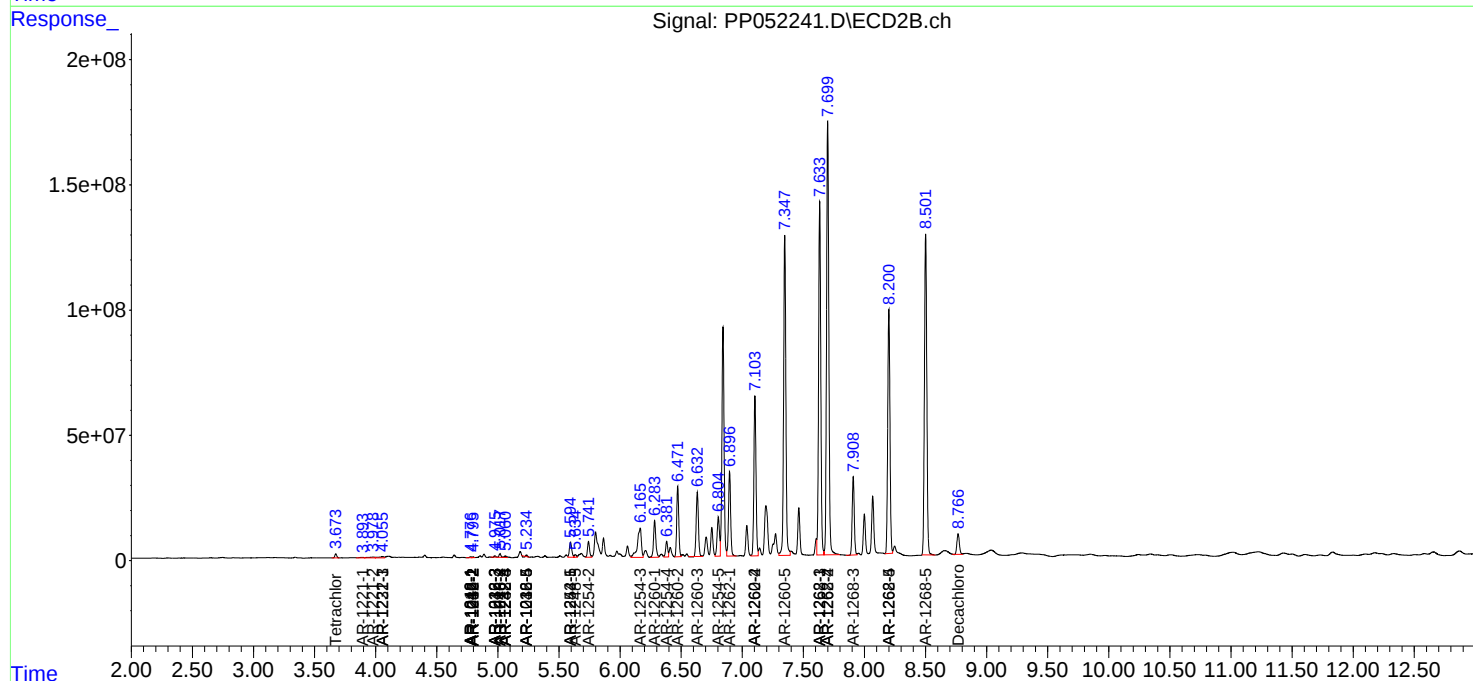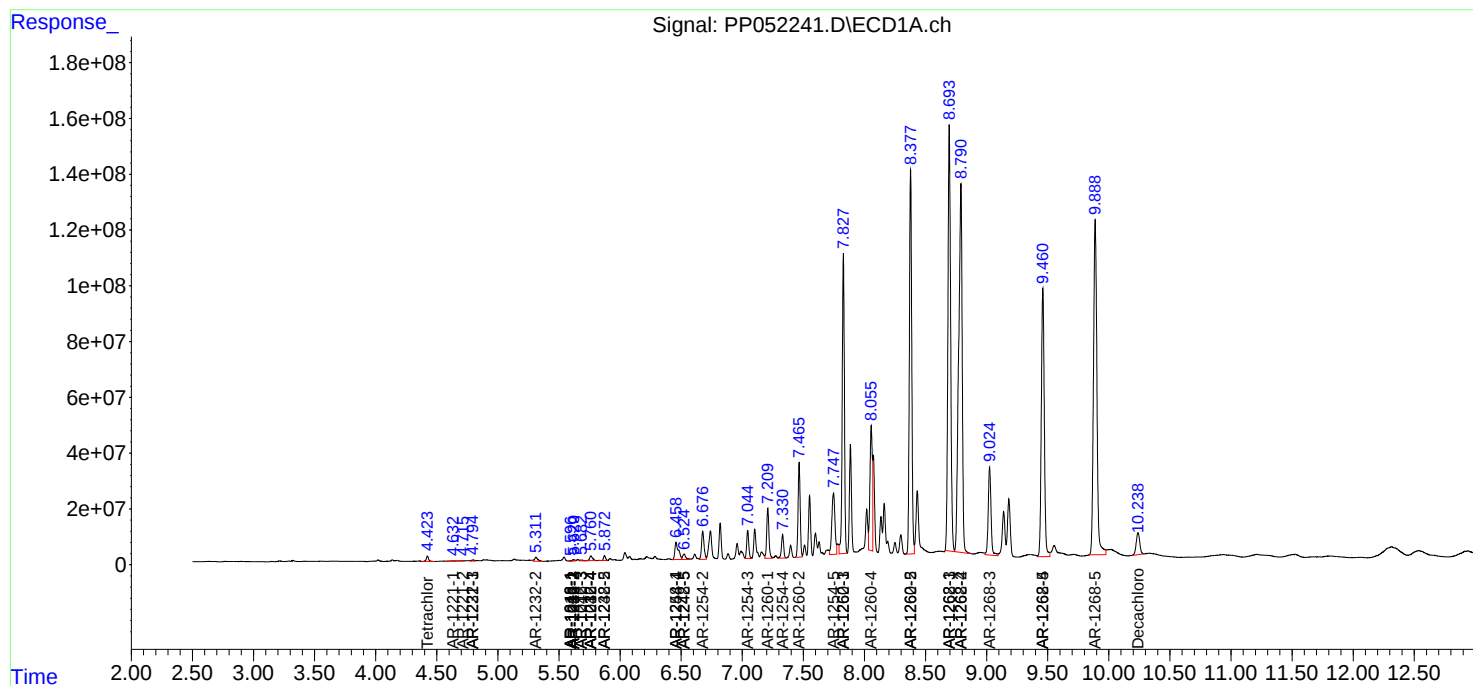


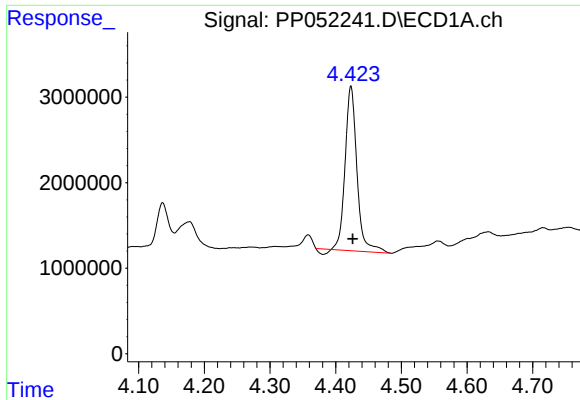

#1 Tetrachloro-m-xylene


R.T.: 4.423 min
Delta R.T.: -0.003 min
Response: 23819270
Conc: 15.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

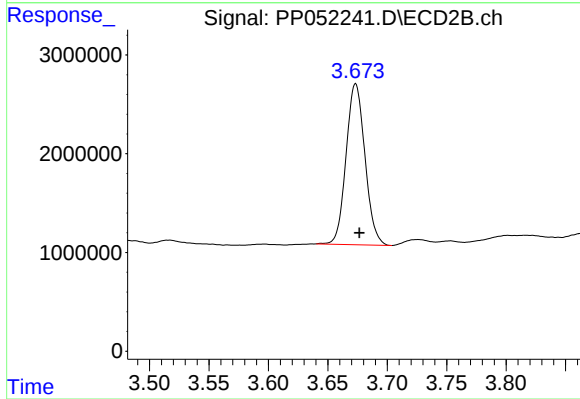


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: -0.003 min
Response: 18028036
Conc: 15.74 ng/ml

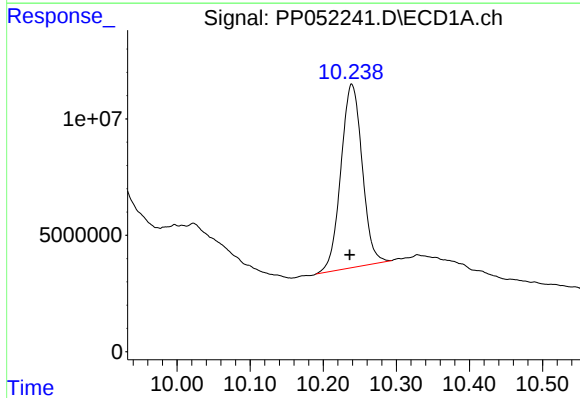


#2 Decachlorobiphenyl

R.T.: 10.239 min
Delta R.T.: 0.003 min
Response: 159359468
Conc: 114.83 ng/ml

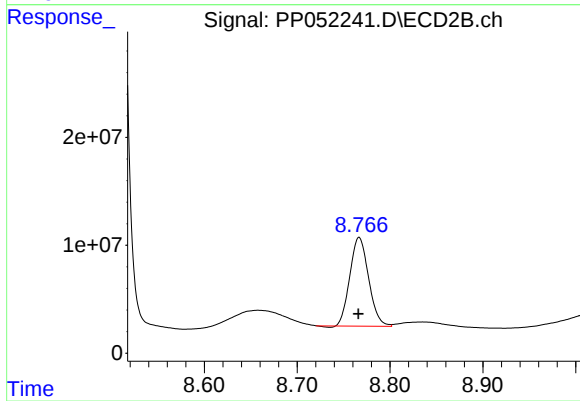

#2 Decachlorobiphenyl


R.T.: 8.767 min
Delta R.T.: 0.000 min
Response: 115571915
Conc: 103.43 ng/ml

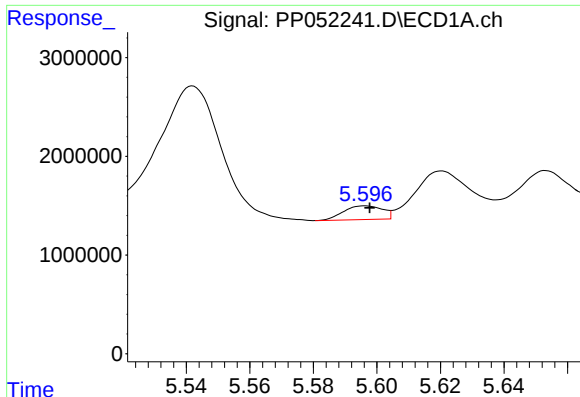

#3 AR-1016-1


R.T.: 5.596 min
Delta R.T.: -0.001 min
Response: 1176753
Conc: 25.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

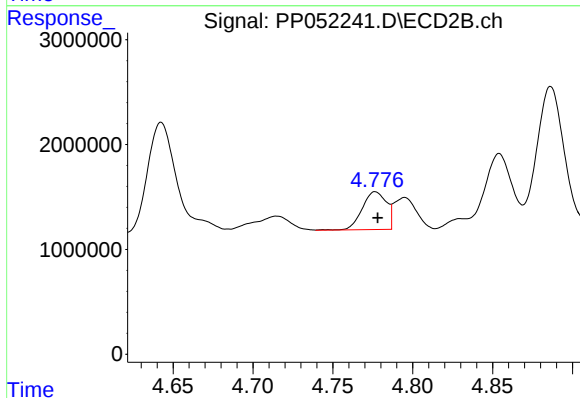


#3 AR-1016-1

R.T.: 4.777 min
Delta R.T.: -0.002 min
Response: 3777746
Conc: 84.94 ng/ml

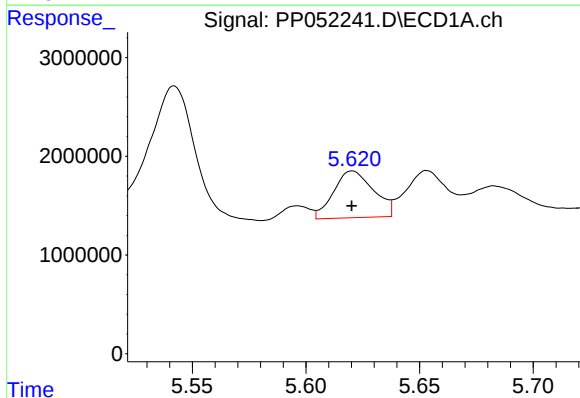


#4 AR-1016-2

R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 5814476
Conc: 88.32 ng/ml

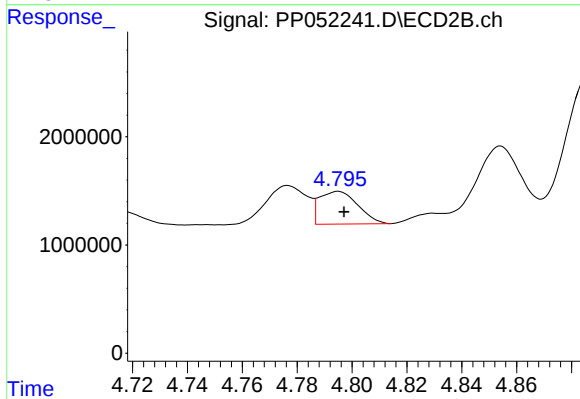

#4 AR-1016-2


R.T.: 4.795 min
Delta R.T.: -0.002 min
Response: 2931967
Conc: 46.08 ng/ml

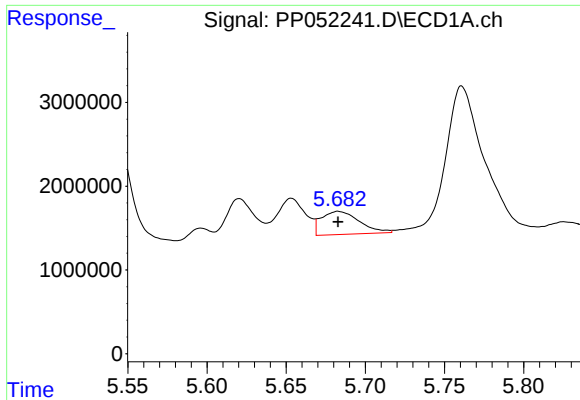

#5 AR-1016-3


R.T.: 5.683 min
Delta R.T.: 0.000 min
Response: 4604269
Conc: 110.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

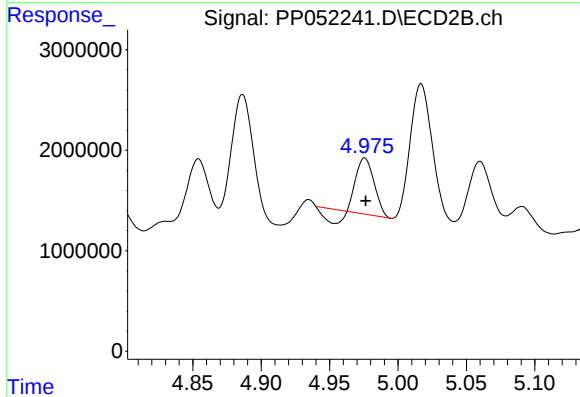


#5 AR-1016-3

R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 3989980
Conc: 120.03 ng/ml

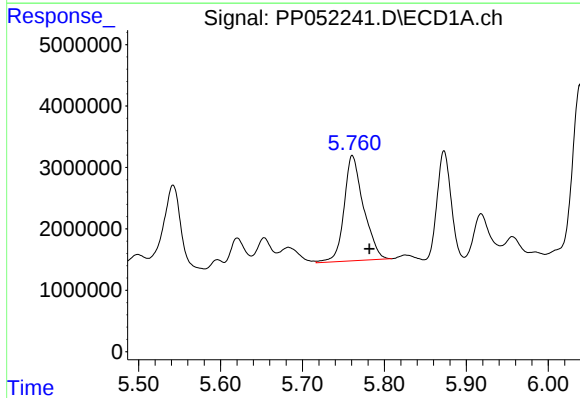


#6 AR-1016-4

R.T.: 5.761 min
Delta R.T.: -0.021 min
Response: 28232876
Conc: 777.02 ng/ml

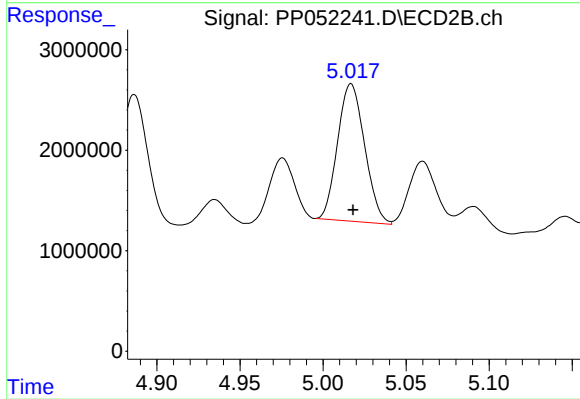

#6 AR-1016-4


R.T.: 5.017 min
Delta R.T.: -0.001 min
Response: 15517198
Conc: 569.33 ng/ml

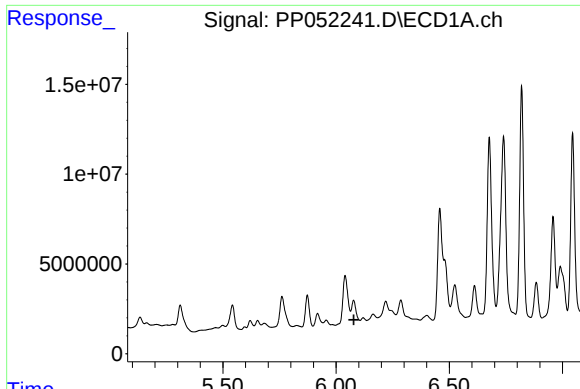

#7 AR-1016-5


R.T.: 6.077 min
Delta R.T.: -0.001 min
Response: -9639966
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

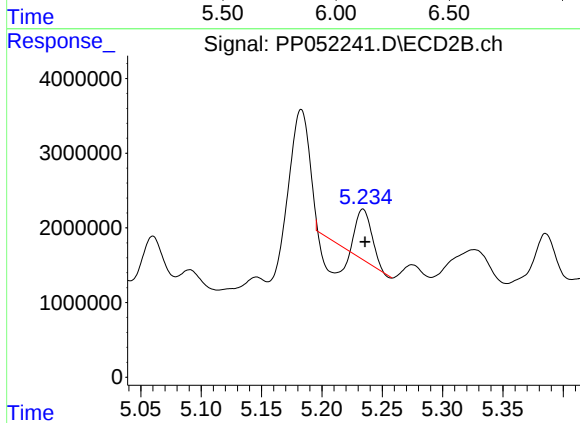


#7 AR-1016-5

R.T.: 5.234 min
Delta R.T.: -0.002 min
Response: 2745696
Conc: 77.61 ng/ml

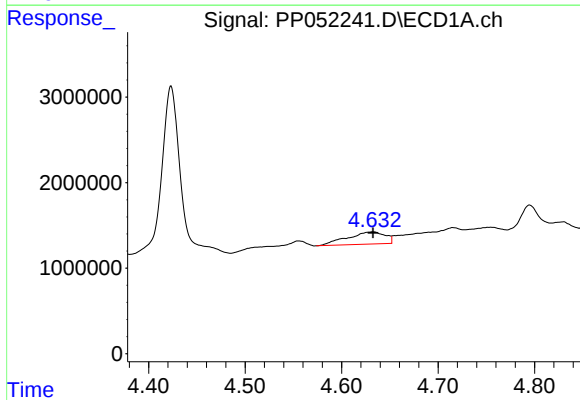


#8 AR-1221-1

R.T.: 4.632 min
Delta R.T.: 0.000 min
Response: 3897303
Conc: 188.60 ng/ml

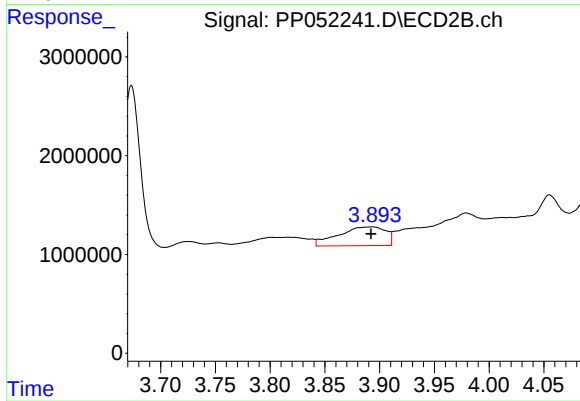

#8 AR-1221-1


R.T.: 3.893 min
Delta R.T.: 0.000 min
Response: 5734189
Conc: 366.74 ng/ml

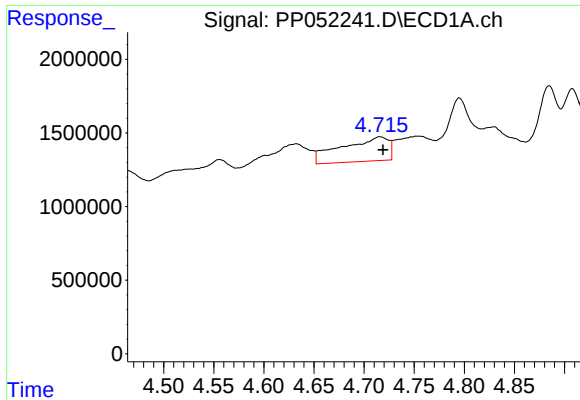

#9 AR-1221-2


R.T.: 4.716 min
Delta R.T.: -0.003 min
Response: 5338207
Conc: 348.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

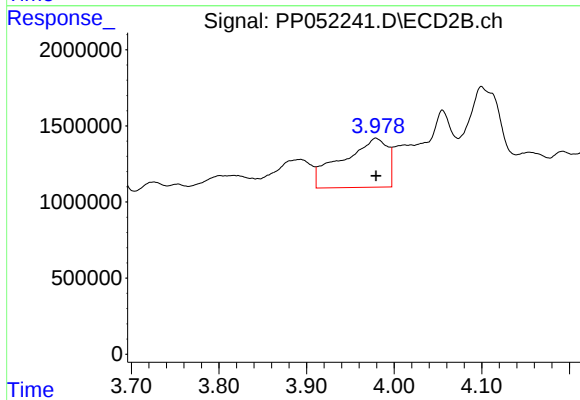


#9 AR-1221-2

R.T.: 3.979 min
Delta R.T.: 0.000 min
Response: 11593161
Conc: 966.68 ng/ml

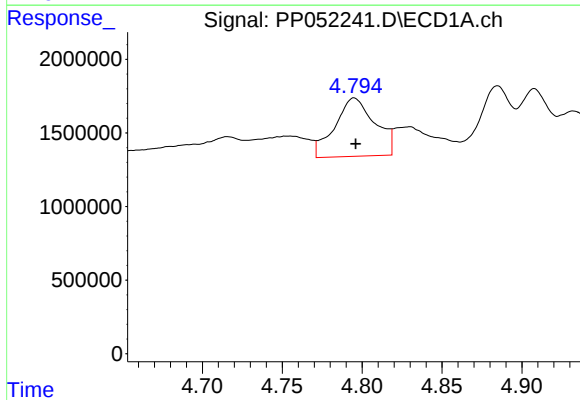


#10 AR-1221-3

R.T.: 4.795 min
Delta R.T.: 0.000 min
Response: 6939628
Conc: 148.21 ng/ml

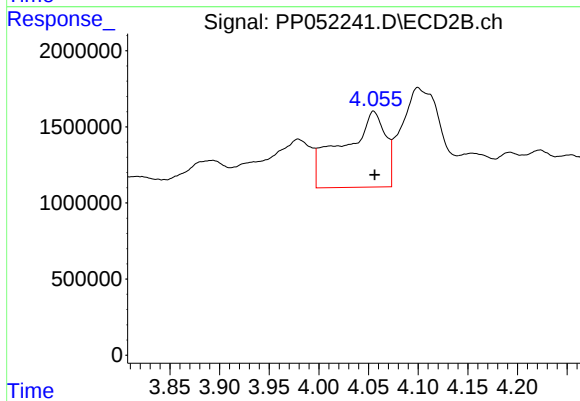

#10 AR-1221-3


R.T.: 4.055 min
Delta R.T.: -0.001 min
Response: 14889695
Conc: 393.96 ng/ml

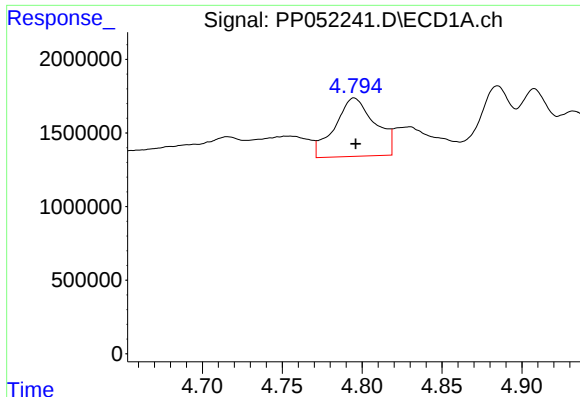

#11 AR-1232-1


R.T.: 4.795 min
Delta R.T.: 0.000 min
Response: 6939628
Conc: 192.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

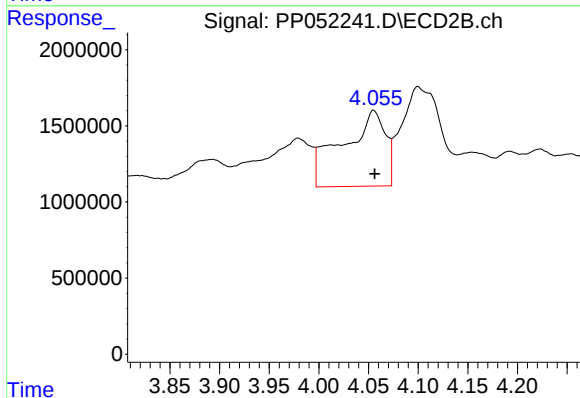


#11 AR-1232-1

R.T.: 4.055 min
Delta R.T.: -0.001 min
Response: 14889695
Conc: 513.76 ng/ml

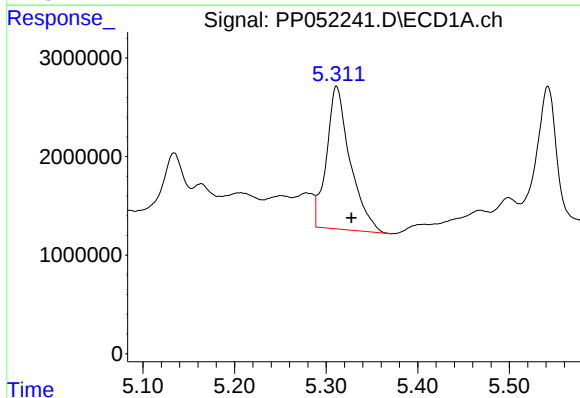


#12 AR-1232-2

R.T.: 5.311 min
Delta R.T.: -0.016 min
Response: 25846504
Conc: 1273.87 ng/ml

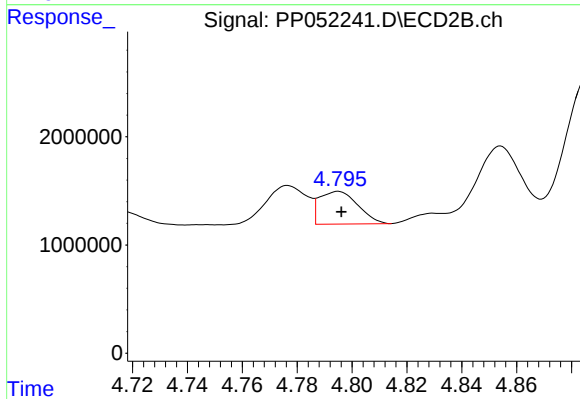

#12 AR-1232-2


R.T.: 4.795 min
Delta R.T.: -0.001 min
Response: 2931967
Conc: 97.88 ng/ml

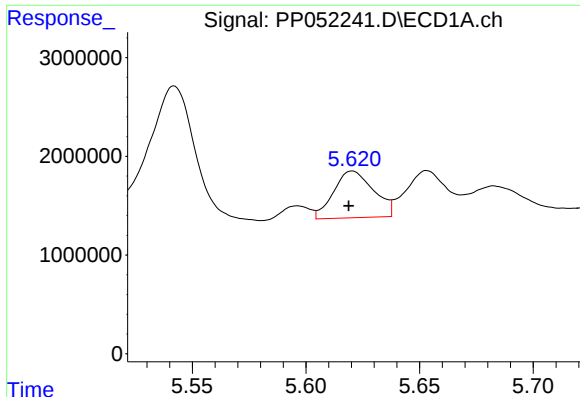

#13 AR-1232-3


R.T.: 5.620 min
Delta R.T.: 0.002 min
Response: 5814476
Conc: 193.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

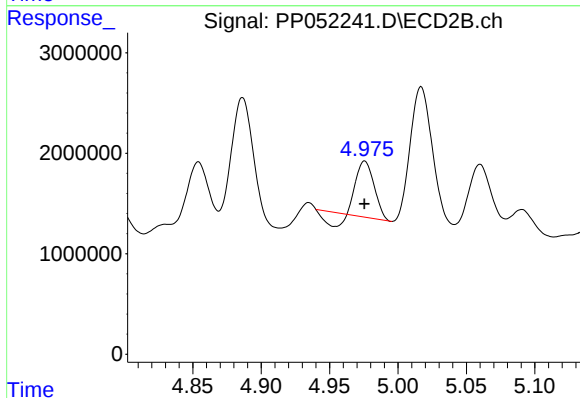


#13 AR-1232-3

R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 3989980
Conc: 261.17 ng/ml

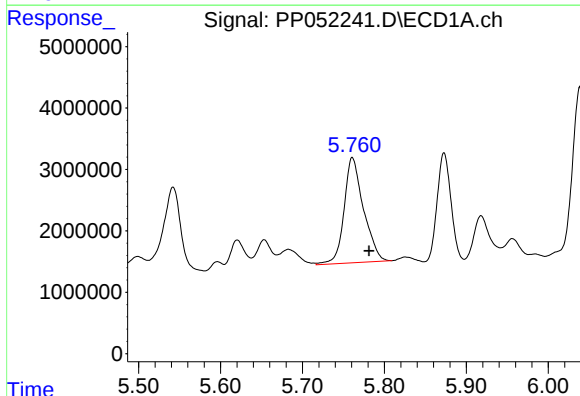


#14 AR-1232-4

R.T.: 5.761 min
Delta R.T.: -0.020 min
Response: 28232876
Conc: 1692.85 ng/ml

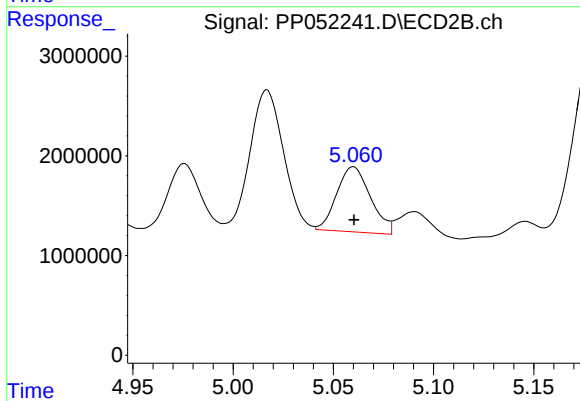

#14 AR-1232-4


R.T.: 5.060 min
Delta R.T.: 0.000 min
Response: 7685558
Conc: 542.74 ng/ml

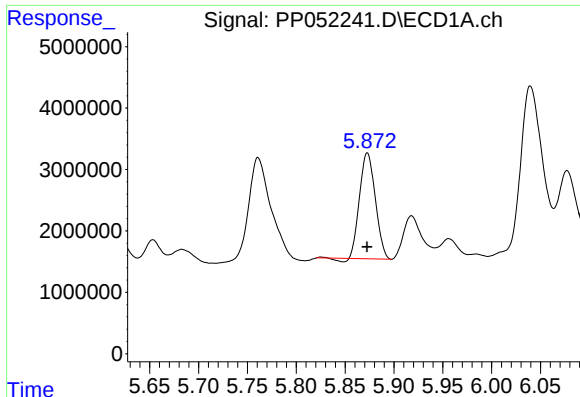

#15 AR-1232-5


R.T.: 5.873 min
Delta R.T.: 0.000 min
Response: 19094931
Conc: 1273.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

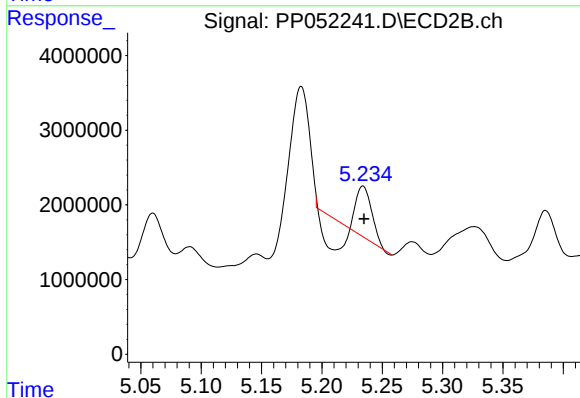


#15 AR-1232-5

R.T.: 5.234 min
Delta R.T.: 0.000 min
Response: 2745696
Conc: 173.45 ng/ml

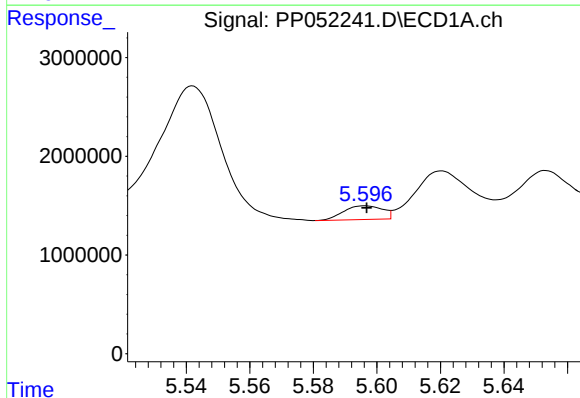


#16 AR-1242-1

R.T.: 5.596 min
Delta R.T.: 0.000 min
Response: 1176753
Conc: 33.83 ng/ml

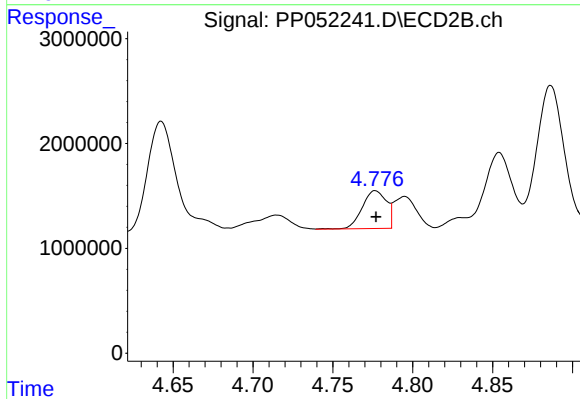

#16 AR-1242-1


R.T.: 4.777 min
Delta R.T.: 0.000 min
Response: 3777746
Conc: 108.50 ng/ml

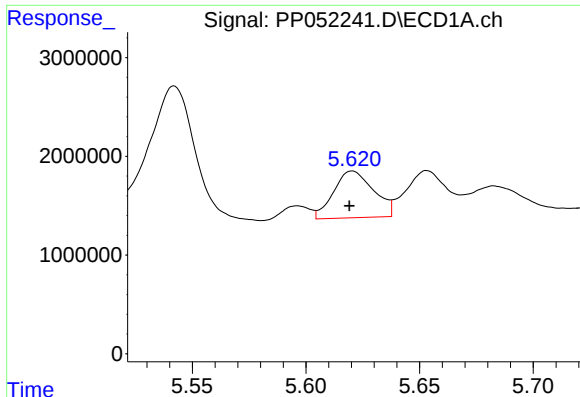

#17 AR-1242-2


R.T.: 5.620 min
Delta R.T.: 0.001 min
Response: 5814476
Conc: 117.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

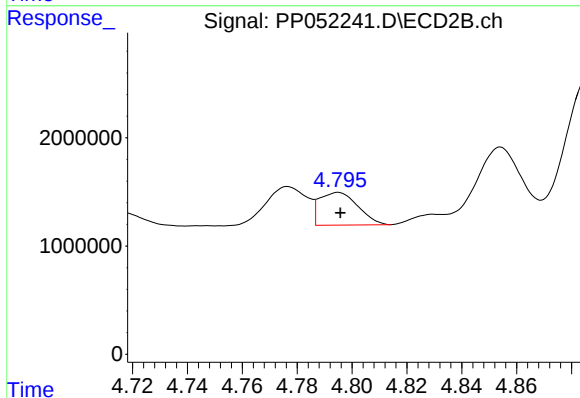


#17 AR-1242-2

R.T.: 4.795 min
Delta R.T.: 0.000 min
Response: 2931967
Conc: 59.43 ng/ml

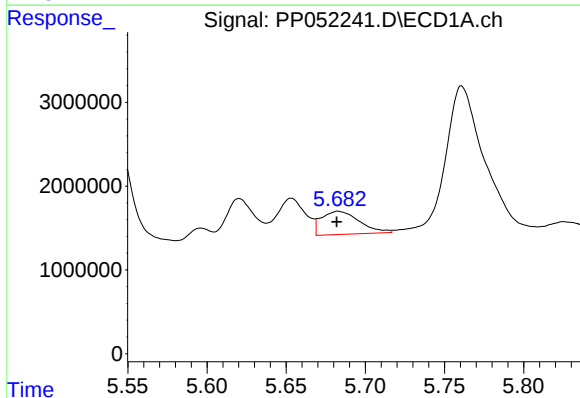


#18 AR-1242-3

R.T.: 5.683 min
Delta R.T.: 0.000 min
Response: 4604269
Conc: 145.21 ng/ml

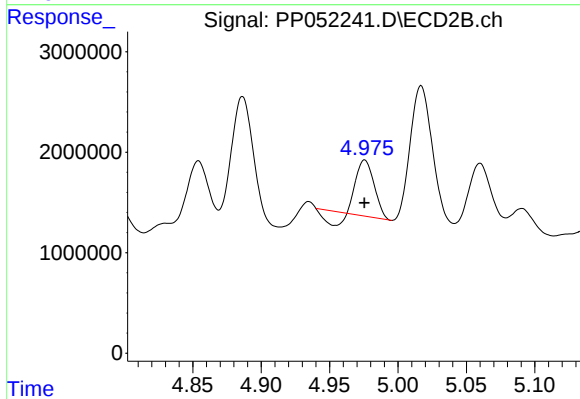

#18 AR-1242-3


R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 3989980
Conc: 152.85 ng/ml

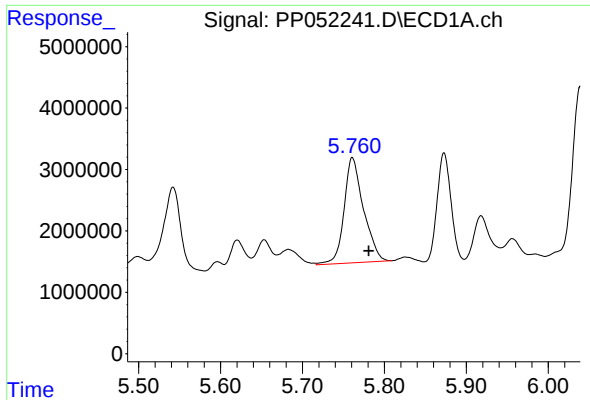

#19 AR-1242-4


R.T.: 5.761 min
Delta R.T.: -0.020 min
Response: 28232876
Conc: 1033.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

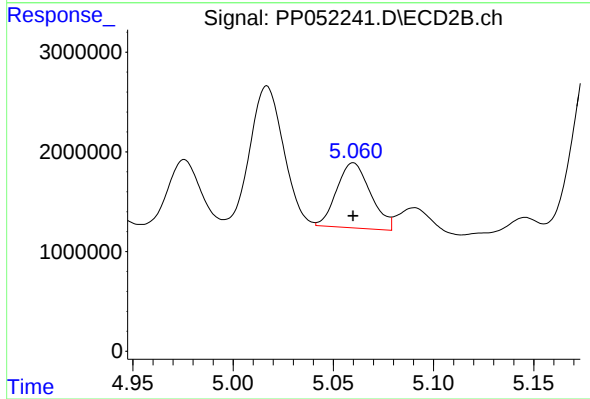


#19 AR-1242-4

R.T.: 5.060 min
Delta R.T.: 0.000 min
Response: 7685558
Conc: 282.56 ng/ml

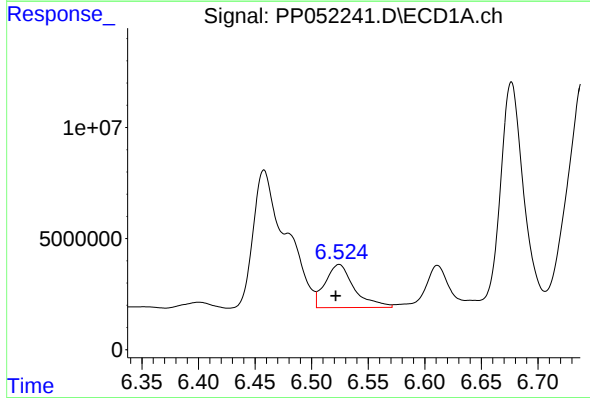


#20 AR-1242-5

R.T.: 6.524 min
Delta R.T.: 0.003 min
Response: 34703331
Conc: 933.45 ng/ml

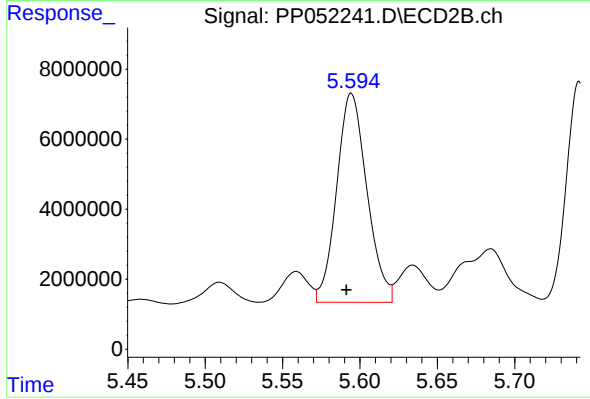

#20 AR-1242-5


R.T.: 5.594 min
Delta R.T.: 0.003 min
Response: 81317338
Conc: 2412.97 ng/ml

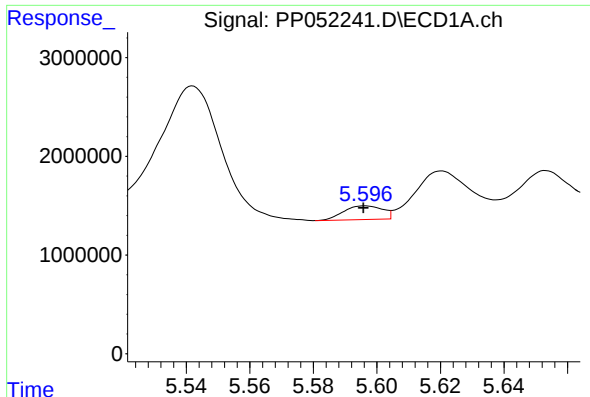

#21 AR-1248-1


R.T.: 5.596 min
Delta R.T.: 0.000 min
Response: 1176753
Conc: 43.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

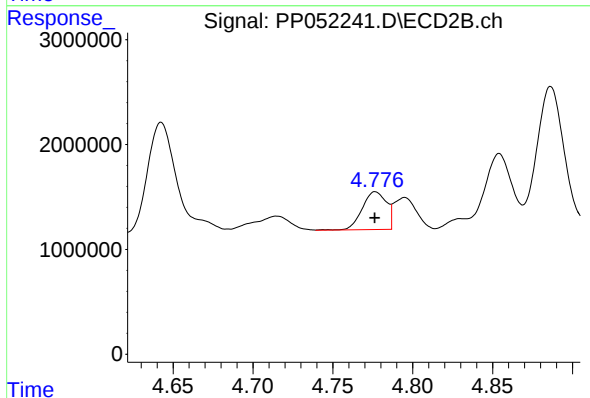


#21 AR-1248-1

R.T.: 4.777 min
Delta R.T.: 0.000 min
Response: 3777746
Conc: 139.34 ng/ml

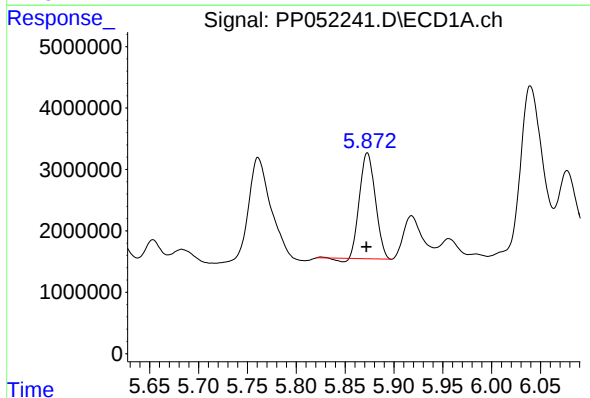


#22 AR-1248-2

R.T.: 5.873 min
Delta R.T.: 0.000 min
Response: 19094931
Conc: 410.80 ng/ml

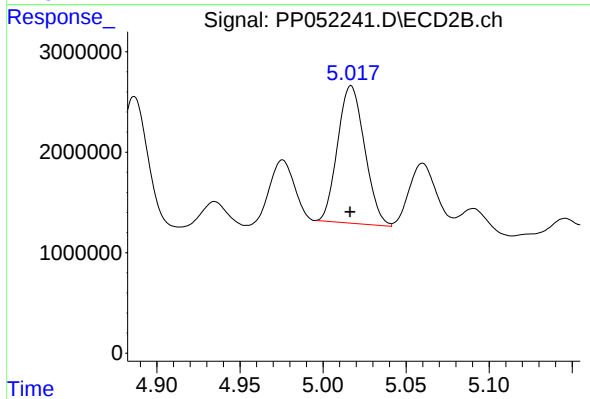

#22 AR-1248-2


R.T.: 5.017 min
Delta R.T.: 0.000 min
Response: 15517198
Conc: 417.08 ng/ml

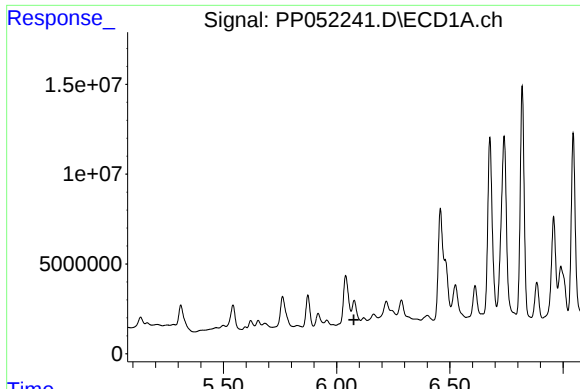

#23 AR-1248-3


R.T.: 6.077 min
Delta R.T.: 0.001 min
Response: -9639966
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

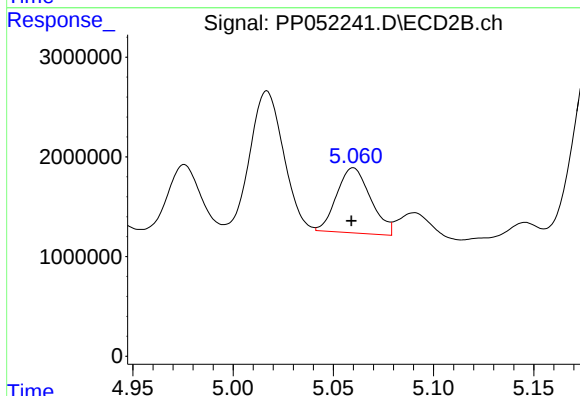


#23 AR-1248-3

R.T.: 5.060 min
Delta R.T.: 0.000 min
Response: 7685558
Conc: 201.74 ng/ml

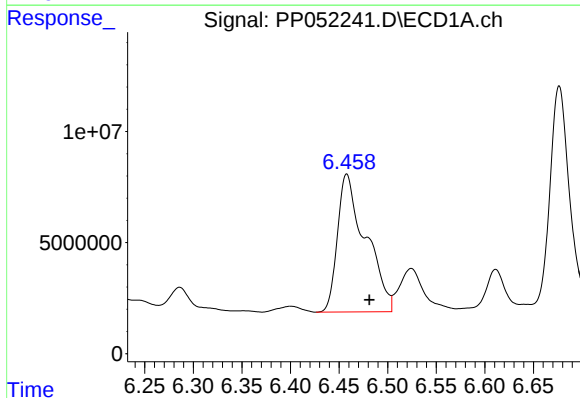


#24 AR-1248-4

R.T.: 6.458 min
Delta R.T.: -0.023 min
Response: 125141079
Conc: 1970.95 ng/ml

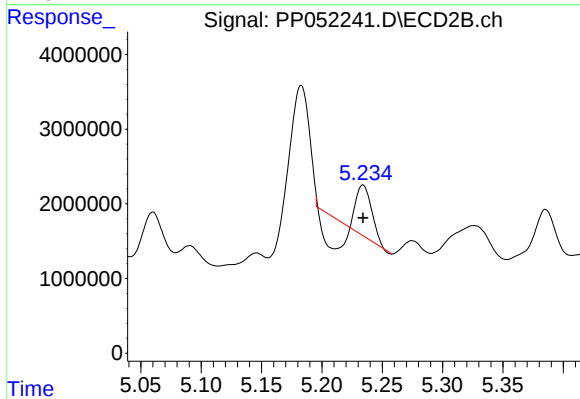

#24 AR-1248-4


R.T.: 5.234 min
Delta R.T.: 0.000 min
Response: 2745696
Conc: 59.26 ng/ml

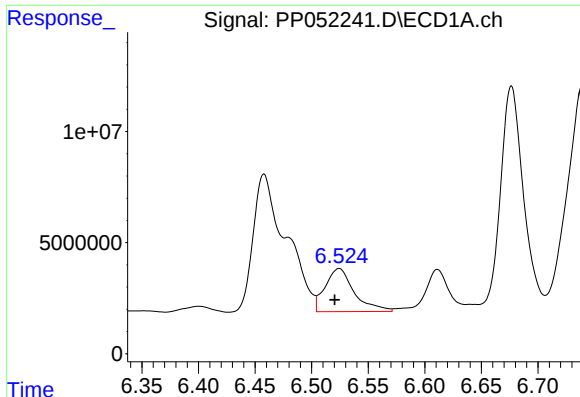

#25 AR-1248-5


R.T.: 6.524 min
Delta R.T.: 0.004 min
Response: 34703331
Conc: 560.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

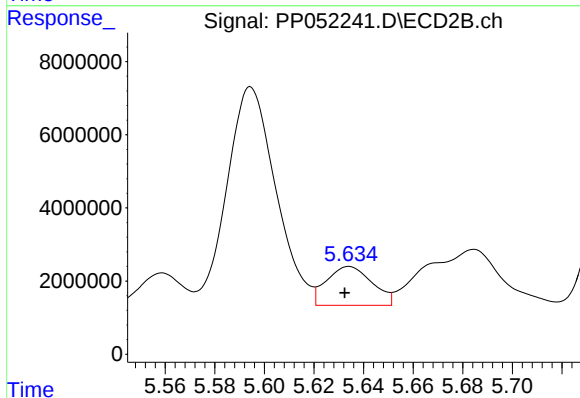


#25 AR-1248-5

R.T.: 5.634 min
Delta R.T.: 0.002 min
Response: 13581862
Conc: 322.97 ng/ml

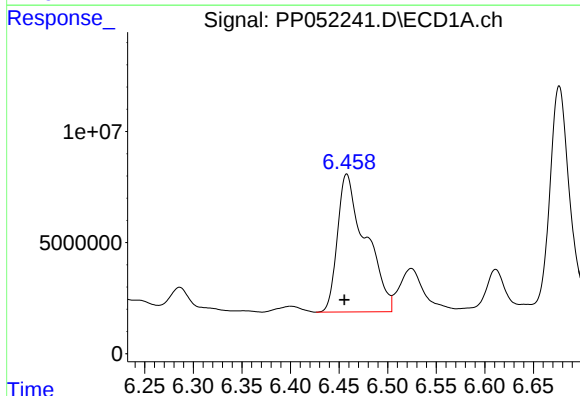


#26 AR-1254-1

R.T.: 6.458 min
Delta R.T.: 0.002 min
Response: 125141079
Conc: 1757.86 ng/ml

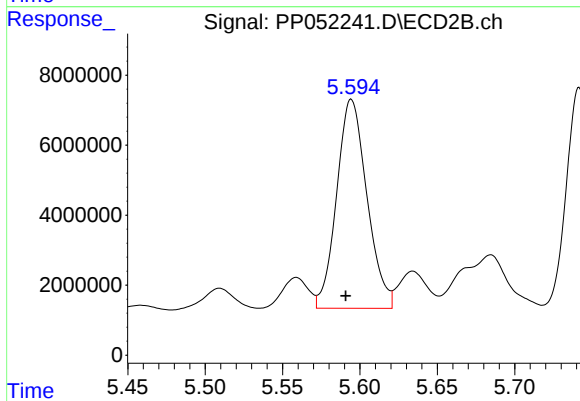

#26 AR-1254-1


R.T.: 5.594 min
Delta R.T.: 0.004 min
Response: 81317338
Conc: 1162.30 ng/ml

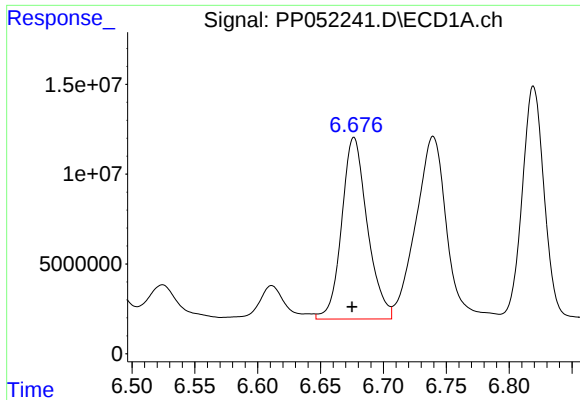

#27 AR-1254-2


R.T.: 6.677 min
Delta R.T.: 0.002 min
Response: 143764180
Conc: 1347.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

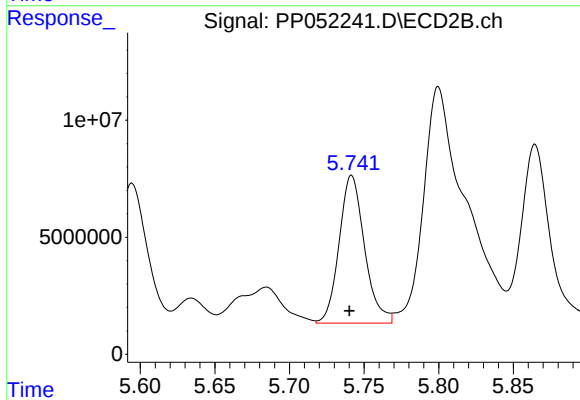


#27 AR-1254-2

R.T.: 5.742 min
Delta R.T.: 0.002 min
Response: 74783135
Conc: 1193.58 ng/ml

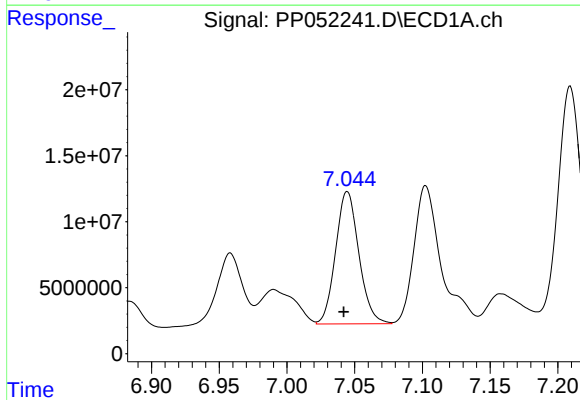


#28 AR-1254-3

R.T.: 7.045 min
Delta R.T.: 0.003 min
Response: 120066459
Conc: 1142.40 ng/ml

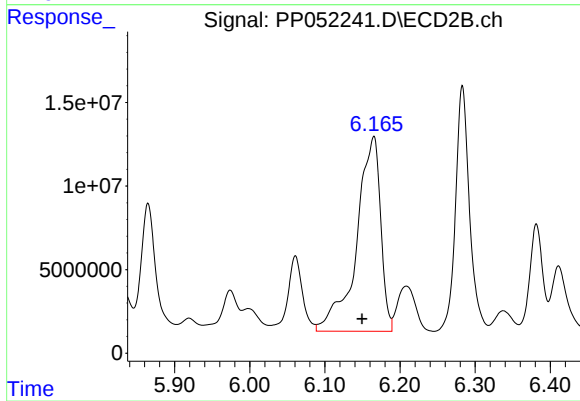

#28 AR-1254-3


R.T.: 6.165 min
Delta R.T.: 0.015 min
Response: 260828628
Conc: 2636.77 ng/ml

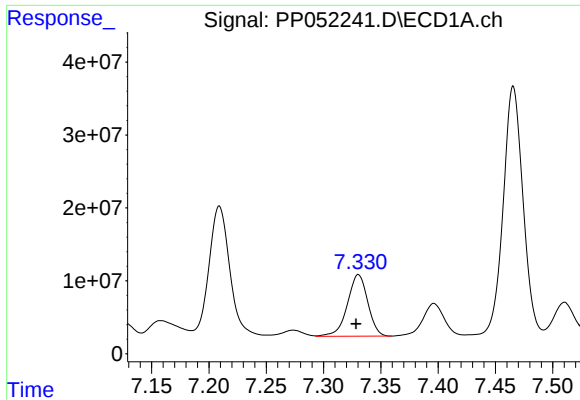

#29 AR-1254-4


R.T.: 7.330 min
Delta R.T.: 0.002 min
Response: 104522896
Conc: 1430.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

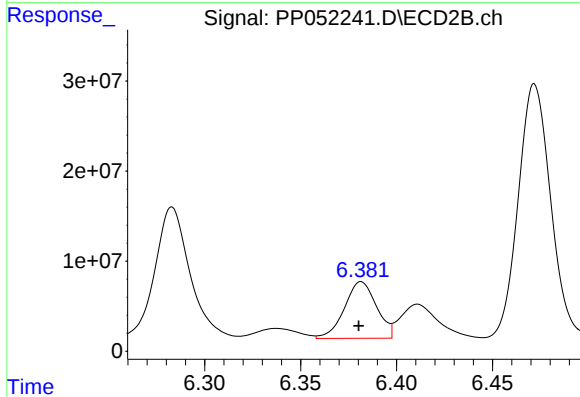


#29 AR-1254-4

R.T.: 6.382 min
Delta R.T.: 0.001 min
Response: 73441974
Conc: 1228.59 ng/ml

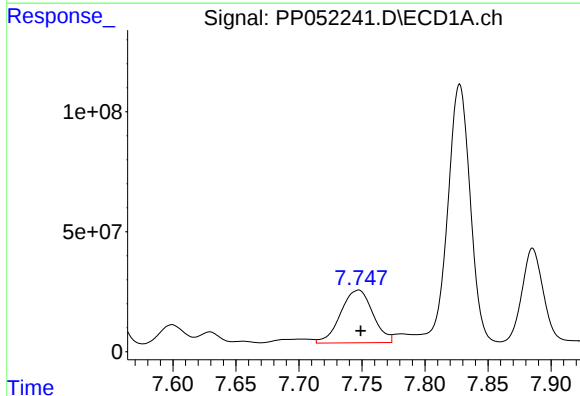


#30 AR-1254-5

R.T.: 7.747 min
Delta R.T.: -0.002 min
Response: 390874744
Conc: 4710.84 ng/ml

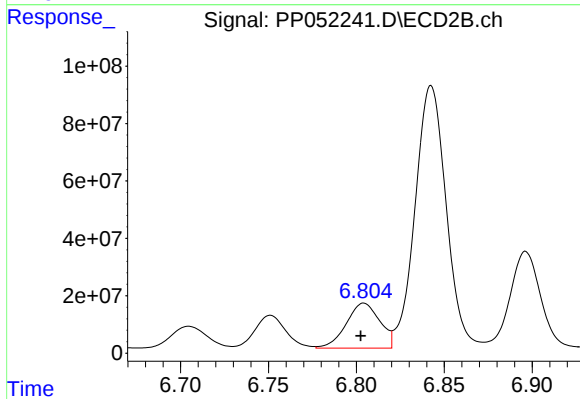

#30 AR-1254-5


R.T.: 6.804 min
Delta R.T.: 0.002 min
Response: 208616305
Conc: 2353.15 ng/ml

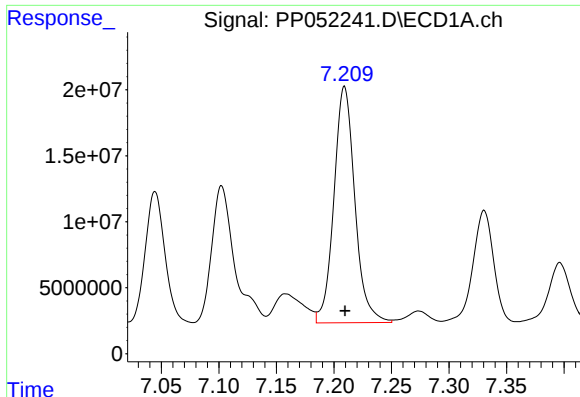

#31 AR-1260-1


R.T.: 7.209 min
Delta R.T.: 0.000 min
Response: 227367035
Conc: 2743.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

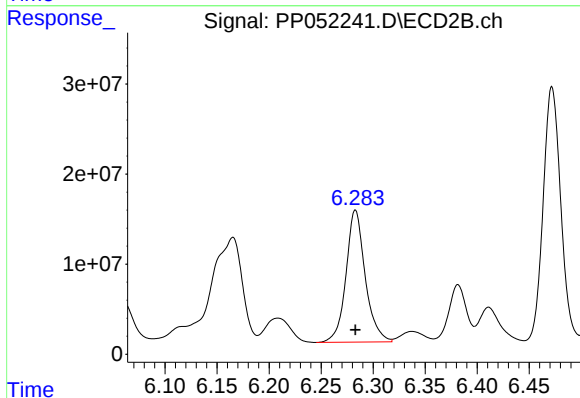


#31 AR-1260-1

R.T.: 6.283 min
Delta R.T.: 0.000 min
Response: 188590947
Conc: 2737.86 ng/ml

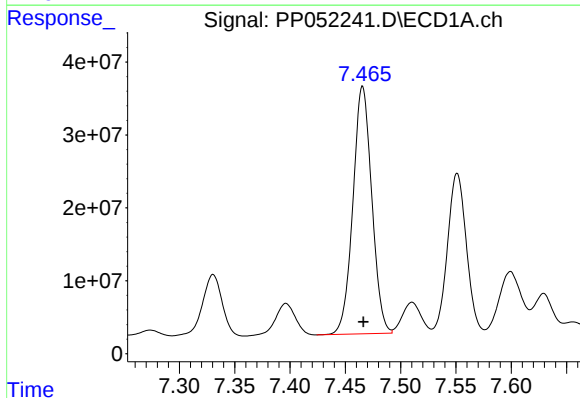


#32 AR-1260-2

R.T.: 7.466 min
Delta R.T.: 0.000 min
Response: 402968293
Conc: 4269.41 ng/ml

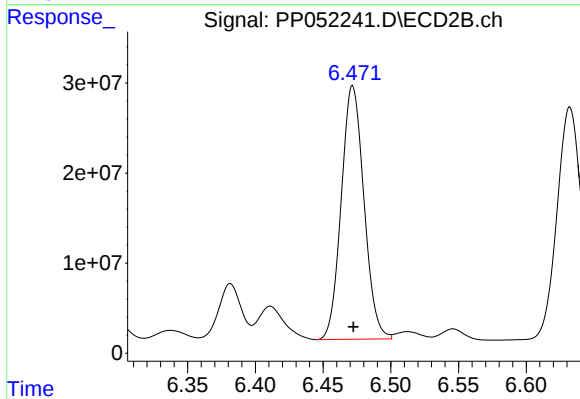

#32 AR-1260-2


R.T.: 6.472 min
Delta R.T.: 0.000 min
Response: 328779523
Conc: 3972.39 ng/ml

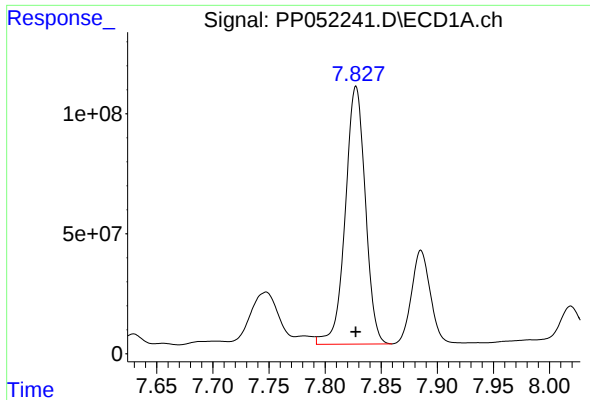

#33 AR-1260-3


R.T.: 7.828 min
Delta R.T.: 0.000 min
Response: 1336228729
Conc: 22248.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

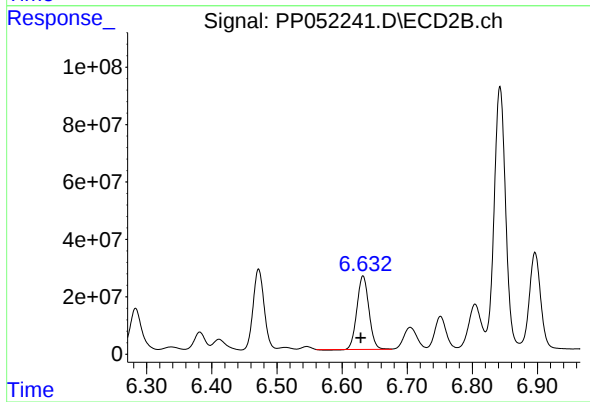


#33 AR-1260-3

R.T.: 6.632 min
Delta R.T.: 0.004 min
Response: 326185300
Conc: 4224.78 ng/ml

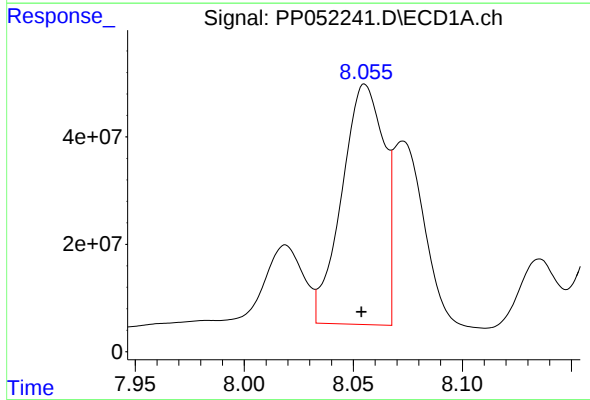


#34 AR-1260-4

R.T.: 8.055 min
Delta R.T.: 0.002 min
Response: 600665250
Conc: 7831.99 ng/ml

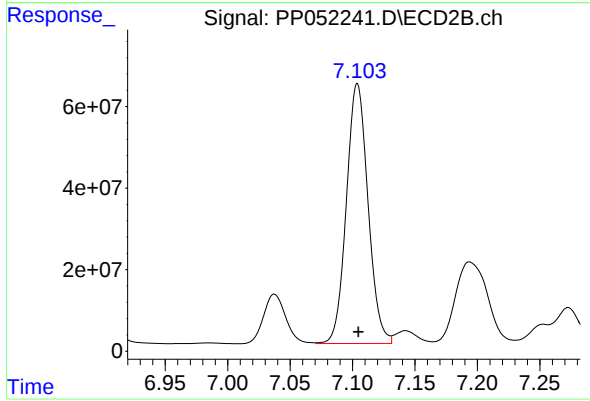

#34 AR-1260-4


R.T.: 7.104 min
Delta R.T.: 0.000 min
Response: 769510978
Conc: 13688.82 ng/ml

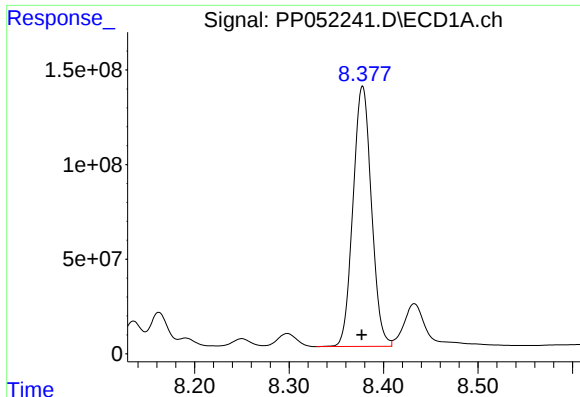

#35 AR-1260-5


R.T.: 8.378 min
Delta R.T.: 0.000 min
Response: 1864782584
Conc: 13603.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

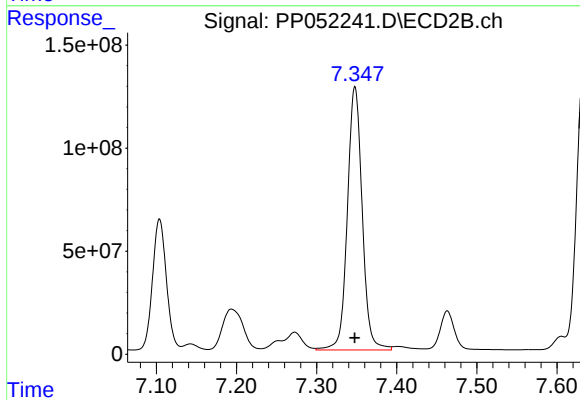


#35 AR-1260-5

R.T.: 7.348 min
Delta R.T.: 0.000 min
Response: 1644218614
Conc: 12467.81 ng/ml

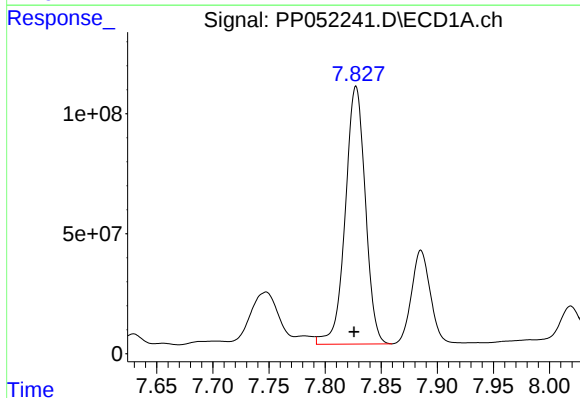


#36 AR-1262-1

R.T.: 7.828 min
Delta R.T.: 0.002 min
Response: 1336228729
Conc: 13780.66 ng/ml

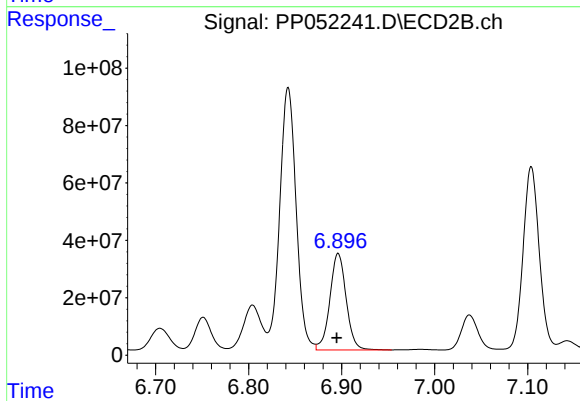

#36 AR-1262-1


R.T.: 6.896 min
Delta R.T.: 0.002 min
Response: 409920530
Conc: 11395.68 ng/ml

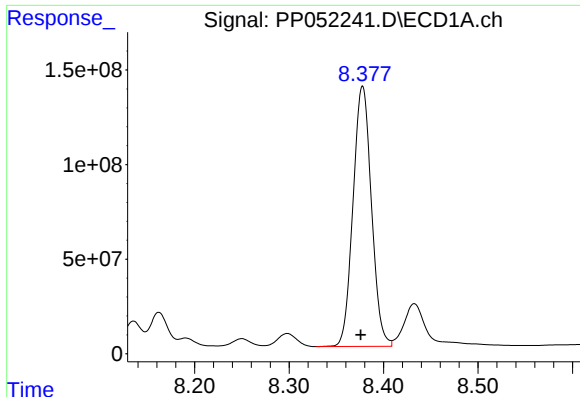

#37 AR-1262-2


R.T.: 8.378 min
Delta R.T.: 0.002 min
Response: 1864782584
Conc: 11581.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

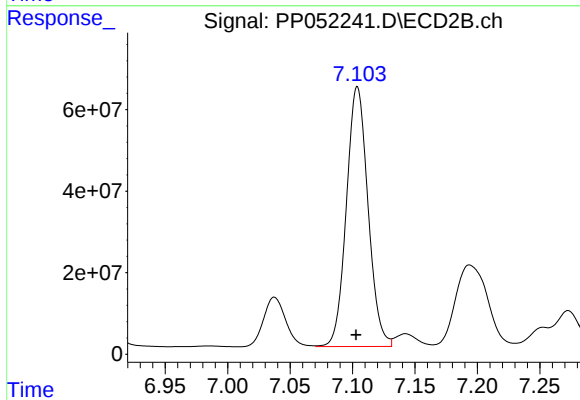


#37 AR-1262-2

R.T.: 7.104 min
Delta R.T.: 0.001 min
Response: 769510978
Conc: 9718.03 ng/ml

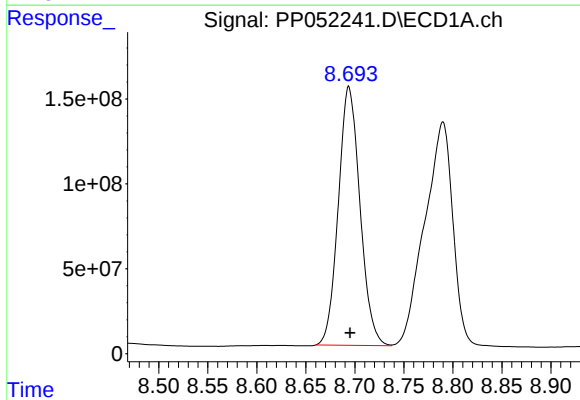


#38 AR-1262-3

R.T.: 8.694 min
Delta R.T.: -0.001 min
Response: 2344831472
Conc: 21336.08 ng/ml

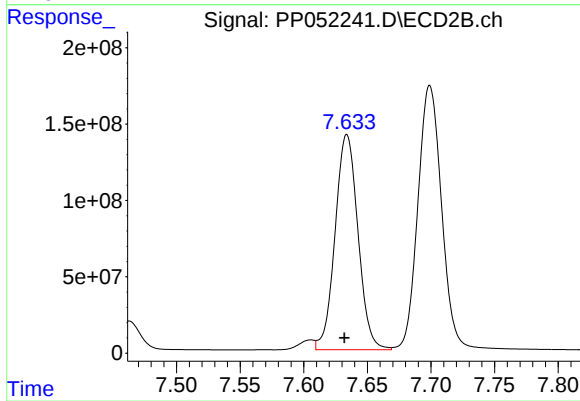

#38 AR-1262-3


R.T.: 7.634 min
Delta R.T.: 0.002 min
Response: 1766430034
Conc: 28605.19 ng/ml

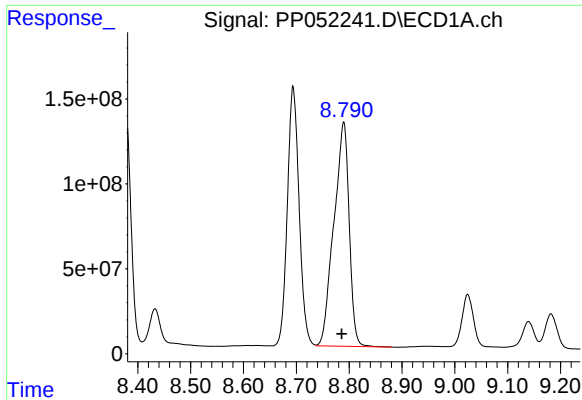

#39 AR-1262-4


R.T.: 8.790 min
Delta R.T.: 0.004 min
Response: 2646060168
Conc: 51763.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

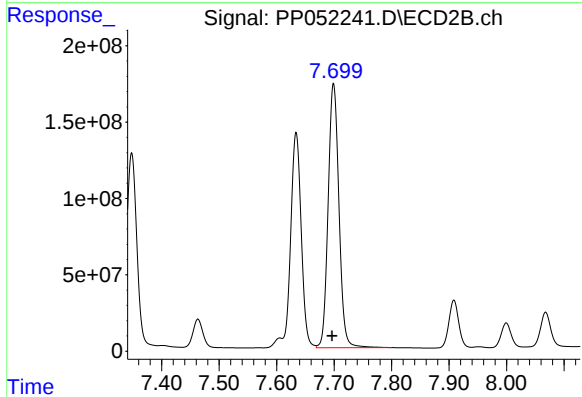


#39 AR-1262-4

R.T.: 7.699 min
Delta R.T.: 0.003 min
Response: 2253585687
Conc: 19740.02 ng/ml

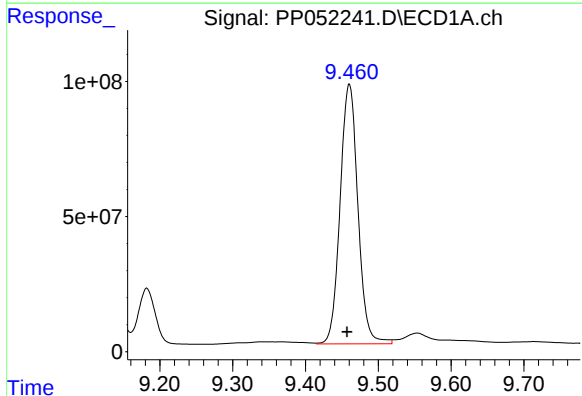


#40 AR-1262-5

R.T.: 9.460 min
Delta R.T.: 0.003 min
Response: 1634197836
Conc: 25960.66 ng/ml

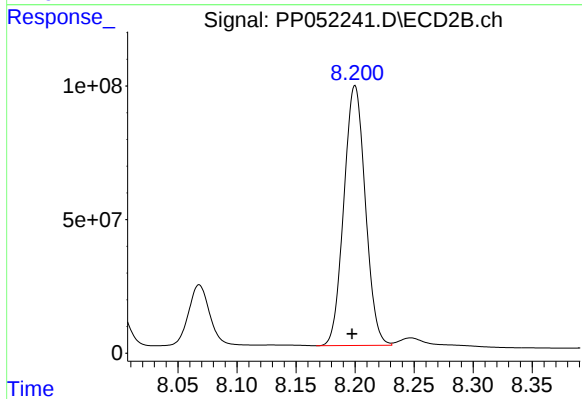

#40 AR-1262-5


R.T.: 8.200 min
Delta R.T.: 0.003 min
Response: 1230815446
Conc: 24215.02 ng/ml

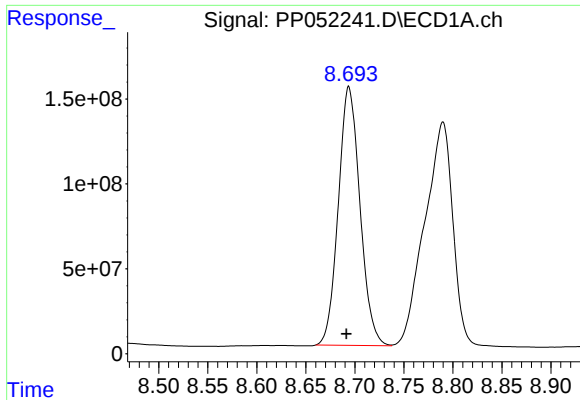

#41 AR-1268-1


R.T.: 8.694 min
Delta R.T.: 0.002 min
Response: 2344831472
Conc: 11843.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

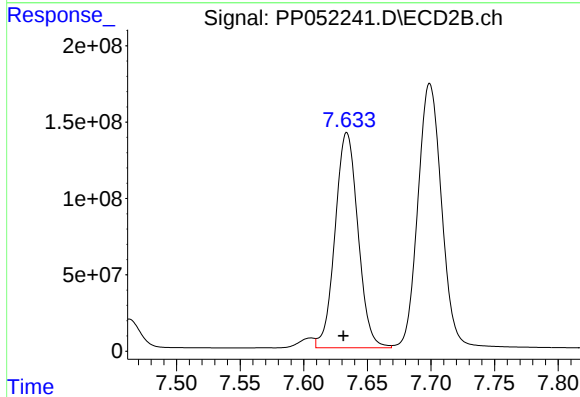


#41 AR-1268-1

R.T.: 7.634 min
Delta R.T.: 0.003 min
Response: 1766430034
Conc: 9737.22 ng/ml

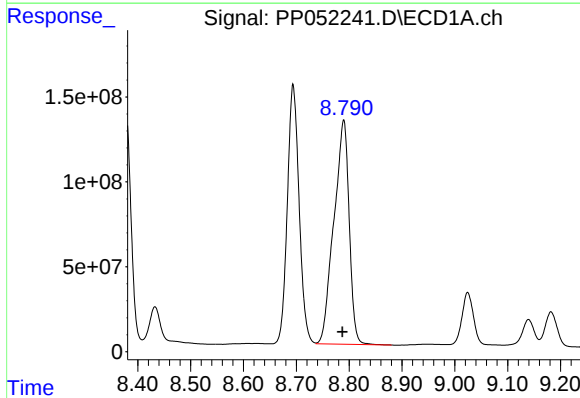


#42 AR-1268-2

R.T.: 8.790 min
Delta R.T.: 0.002 min
Response: 2646060168
Conc: 14410.35 ng/ml

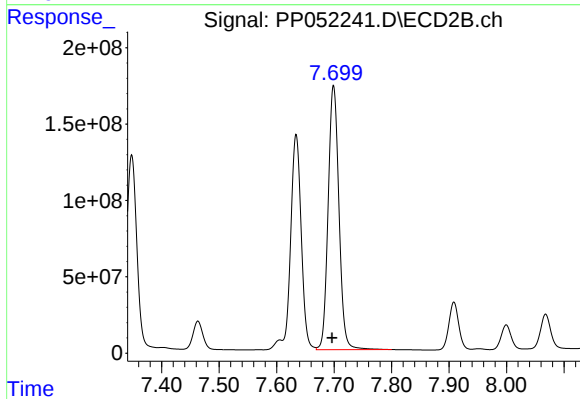

#42 AR-1268-2


R.T.: 7.699 min
Delta R.T.: 0.003 min
Response: 2253585687
Conc: 13792.93 ng/ml

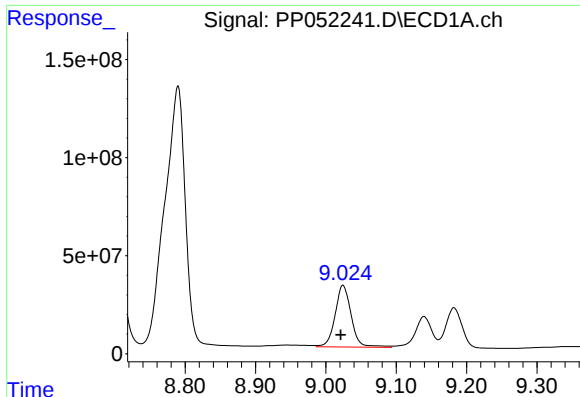

#43 AR-1268-3


R.T.: 9.024 min
Delta R.T.: 0.003 min
Response: 498643009
Conc: 3058.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

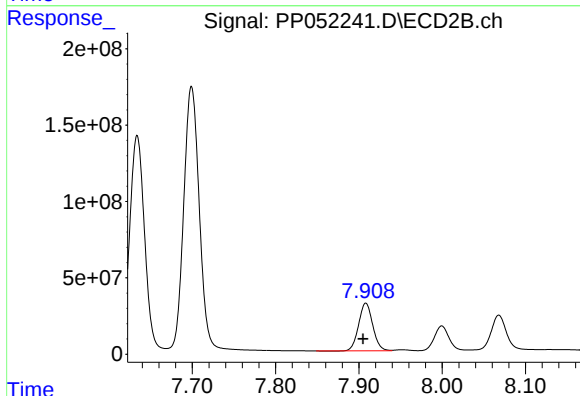


#43 AR-1268-3

R.T.: 7.908 min
Delta R.T.: 0.003 min
Response: 367523141
Conc: 2613.55 ng/ml

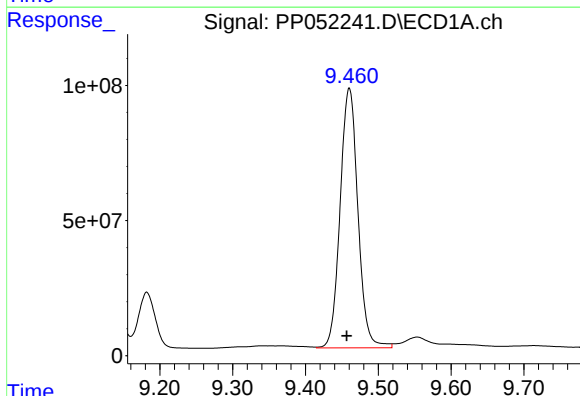


#44 AR-1268-4

R.T.: 9.460 min
Delta R.T.: 0.004 min
Response: 1634197836
Conc: 22397.96 ng/ml

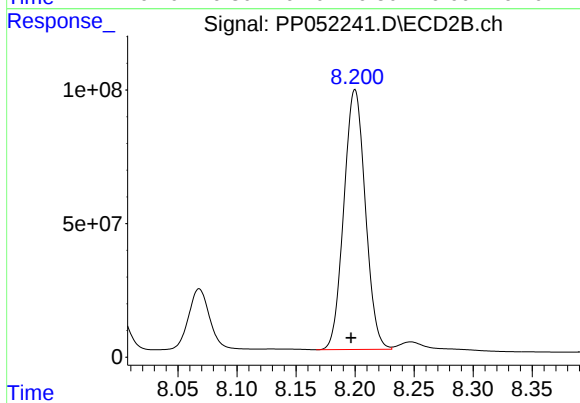

#44 AR-1268-4


R.T.: 8.200 min
Delta R.T.: 0.003 min
Response: 1230815446
Conc: 21779.98 ng/ml

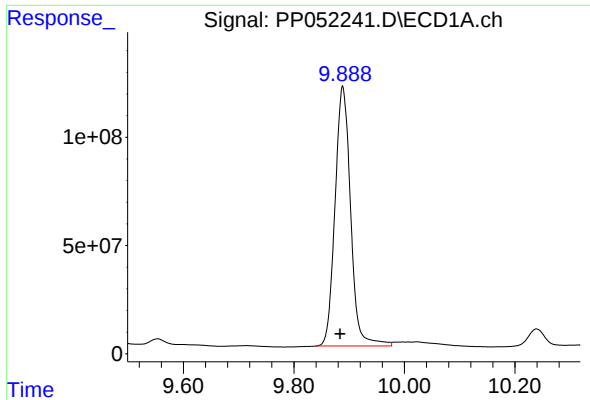

#45 AR-1268-5

R.T.: 9.888 min
Delta R.T.: 0.004 min
Response: 2349419496
Conc: 4505.61 ng/m

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3

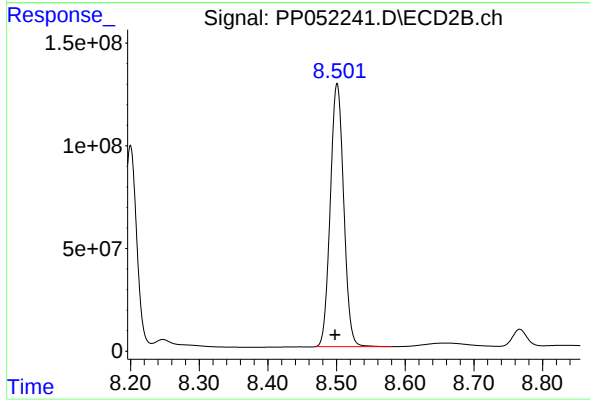

#45 AR-1268-5

R.T.: 8.501 min
Delta R.T.: 0.003 min
Response: 1736750312
Conc: 4128.63 ng/ml