

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
 Data File : PP052242.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 19:52
 Operator : YP\AJ
 Sample : N5098-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 250FERRYBLVD-PCB-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 05:41:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 12 05:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.423	3.673	29890116	22541477	19.016	19.676
2)	SA Decachlor...	10.237	8.767	408.2E6	316.2E6	294.144	282.966
Target Compounds							
3)	L1 AR-1016-1	5.598	4.776	1552139	4306479	34.132	96.827 #
4)	L1 AR-1016-2	5.620	4.794	5763099	3474025	87.542	54.595 #
5)	L1 AR-1016-3	5.682	4.976	3337494	7006287	80.199	210.777 #
6)	L1 AR-1016-4	5.764f	5.017	14796816	10052006	407.237	368.810
8)	L2 AR-1221-1	4.631	3.893	2148956	2972997	103.994	190.143 #
9)	L2 AR-1221-2	4.720	3.978	4395216	5409093	287.207	451.028 #
10)	L2 AR-1221-3	4.794	4.055	4392790	6104198	93.817	161.508 #
11)	L3 AR-1232-1	4.794	4.055	4392790	6104198	121.931	210.621 #
12)	L3 AR-1232-2	5.312f	4.794	14948859	3474025	736.769	115.975 #
13)	L3 AR-1232-3	5.620	4.976	5763099	7006287	191.364	458.604 #
14)	L3 AR-1232-4	5.764f	5.060	14796816	5783313	887.222	408.411 #
15)	L3 AR-1232-5	5.872	5.234	10102823	2080370	673.624	131.417 #
16)	L4 AR-1242-1	5.598	4.776	1552139	4306479	44.620	123.685 #
17)	L4 AR-1242-2	5.620	4.794	5763099	3474025	116.411	70.422 #
18)	L4 AR-1242-3	5.682	4.976	3337494	7006287	105.259	268.401 #
19)	L4 AR-1242-4	5.764f	5.060	14796816	5783313	541.701	212.622 #
20)	L4 AR-1242-5	6.524	5.593	18868605	25685237	507.526	762.171 #
21)	L5 AR-1248-1	5.598	4.776	1552139	4306479	57.738	158.844 #
22)	L5 AR-1248-2	5.872	5.017	10102823	10052006	217.347	270.183
23)	L5 AR-1248-3	6.077	5.060	-5029011	5783313	N.D.	151.807 #
24)	L5 AR-1248-4	6.457f	5.234	40049194	2080370	630.766	44.898 #
25)	L5 AR-1248-5	6.524	5.634	18868605	6191190	304.652	147.222 #
26)	L6 AR-1254-1	6.457	5.593	40049194	25685237	562.571	367.128 #
27)	L6 AR-1254-2	6.676	5.742	55968509	33315834	524.778	531.737
28)	L6 AR-1254-3	7.046	6.133f	36122753	25038380	343.699	253.118 #
29)	L6 AR-1254-4	7.329	6.381	28156781	16654415	385.348	278.608 #
30)	L6 AR-1254-5	7.741	6.805	362.0E6	132.4E6	4362.571	1493.751 #
31)	L7 AR-1260-1	7.209	6.283	222.8E6	180.5E6	2688.608	2620.015
32)	L7 AR-1260-2	7.466	6.472	481.5E6	374.6E6	5101.665	4526.390
33)	L7 AR-1260-3	7.828	6.633	2084.5E6	395.8E6	34707.723	5126.240 #
34)	L7 AR-1260-4	8.056	7.104	736.2E6	1234.3E6	9598.865	21957.489 #
35)	L7 AR-1260-5	8.377	7.348	2801.3E6	2369.0E6	20435.619	17963.543
36)	L8 AR-1262-1	7.828	6.896	2084.5E6	546.1E6	21497.753	15180.620 #
37)	L8 AR-1262-2	8.377	7.104	2801.3E6	1234.3E6	17398.212	15588.156
38)	L8 AR-1262-3	8.694	7.634	4181.4E6	3160.6E6	38047.800	51182.145 #
39)	L8 AR-1262-4	8.789	7.700	4810.2E6	3803.3E6	94099.035	33314.493 #
40)	L8 AR-1262-5	9.460	8.200	2979.3E6	2251.1E6	47328.152	44288.766
41)	L9 AR-1268-1	8.694	7.634	4181.4E6	3160.6E6	21120.662	17422.423
42)	L9 AR-1268-2	8.789	7.700	4810.2E6	3803.3E6	26196.279	23277.811

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
 Data File : PP052242.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 19:52
 Operator : YP\AJ
 Sample : N5098-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 250FERRYBLVD-PCB-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 05:41:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 12 05:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	9.024	7.909	1118.3E6	859.2E6	6860.350	6110.160
44) L9	AR-1268-4	9.460	8.200	2979.3E6	2251.1E6	40833.094	39835.131
45) L9	AR-1268-5	9.888	8.502	5126.4E6	3738.8E6	9831.096	8888.042



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
Data File : PP052242.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 19:52
Operator : YP\AJ
Sample : N5098-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 05:41:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

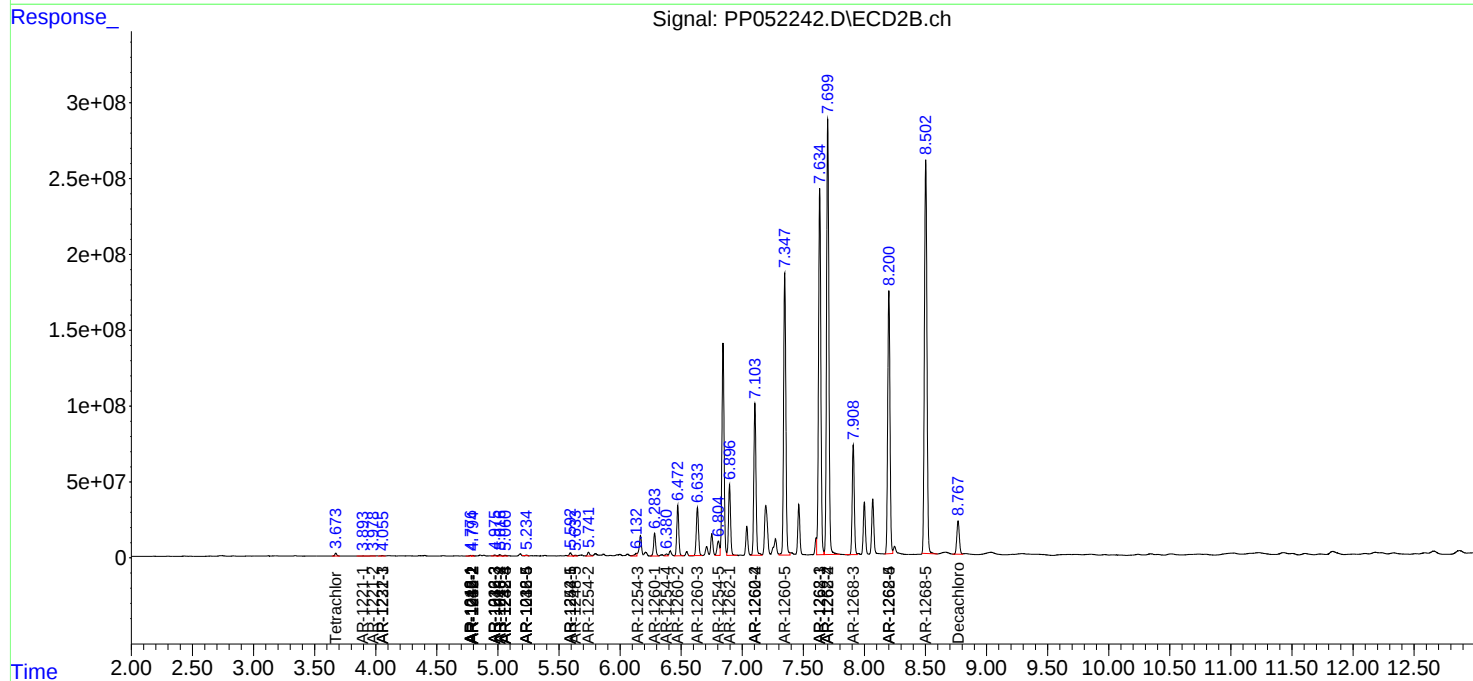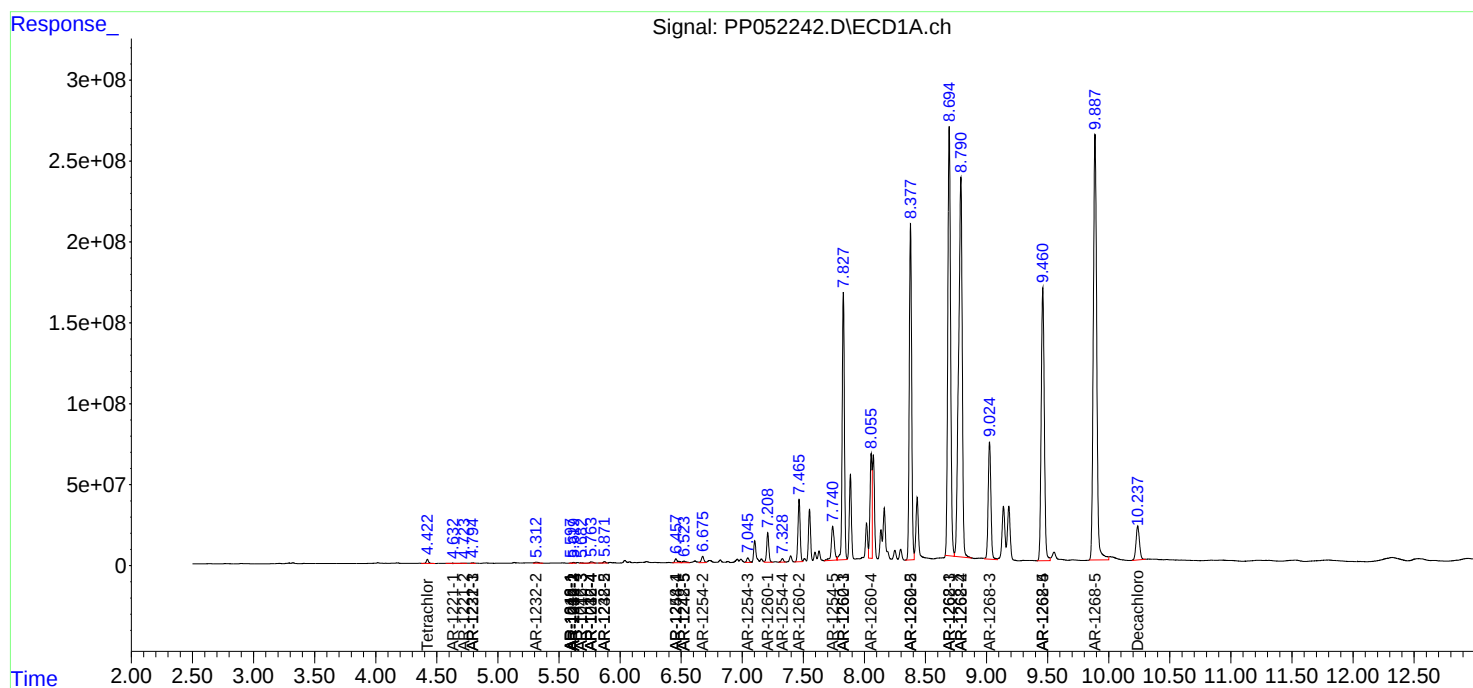


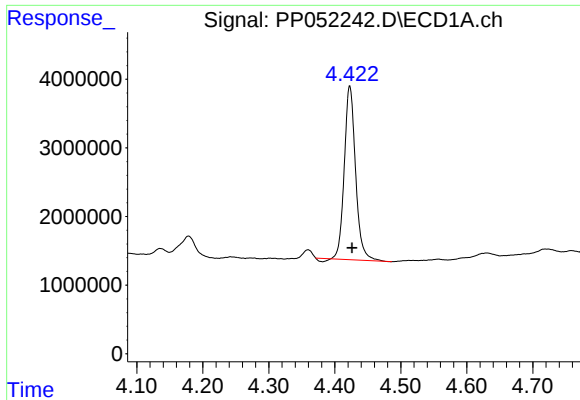

#1 Tetrachloro-m-xylene


R.T.: 4.423 min
Delta R.T.: -0.003 min
Response: 29890116
Conc: 19.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

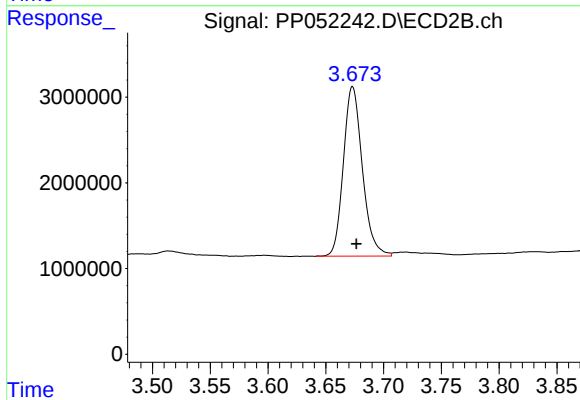


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: -0.003 min
Response: 22541477
Conc: 19.68 ng/ml

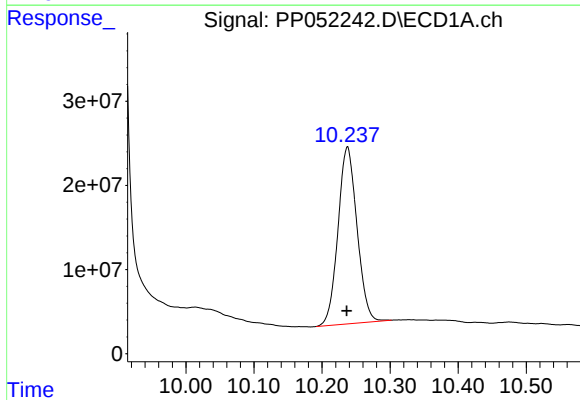


#2 Decachlorobiphenyl

R.T.: 10.237 min
Delta R.T.: 0.000 min
Response: 408226353
Conc: 294.14 ng/ml

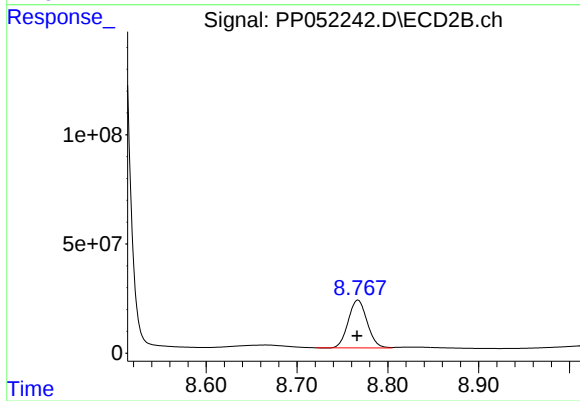

#2 Decachlorobiphenyl


R.T.: 8.767 min
Delta R.T.: 0.001 min
Response: 316175379
Conc: 282.97 ng/ml

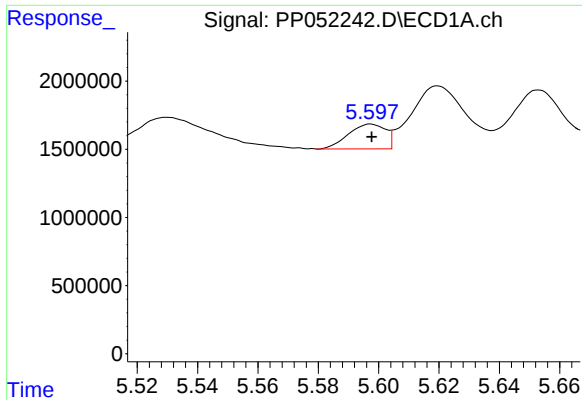

#3 AR-1016-1


R.T.: 5.598 min
Delta R.T.: 0.000 min
Response: 1552139
Conc: 34.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

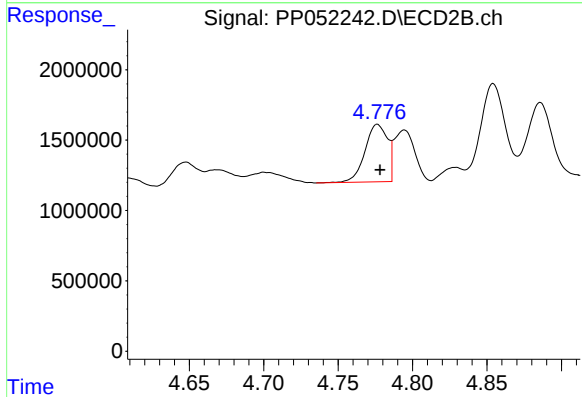


#3 AR-1016-1

R.T.: 4.776 min
Delta R.T.: -0.002 min
Response: 4306479
Conc: 96.83 ng/ml

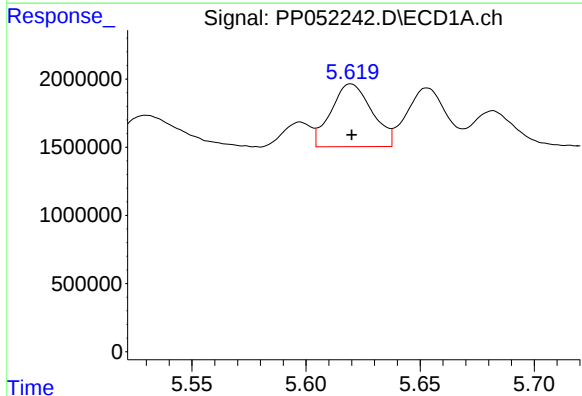


#4 AR-1016-2

R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 5763099
Conc: 87.54 ng/ml

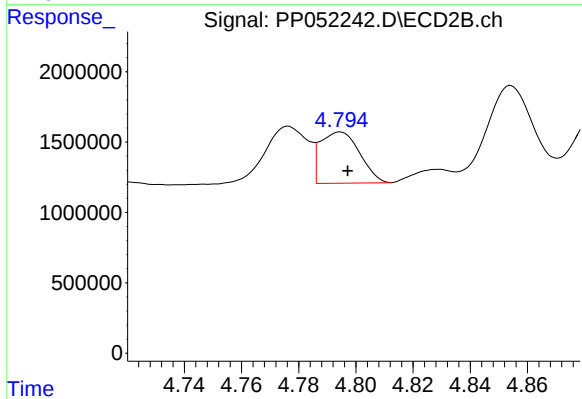

#4 AR-1016-2


R.T.: 4.794 min
Delta R.T.: -0.003 min
Response: 3474025
Conc: 54.60 ng/ml

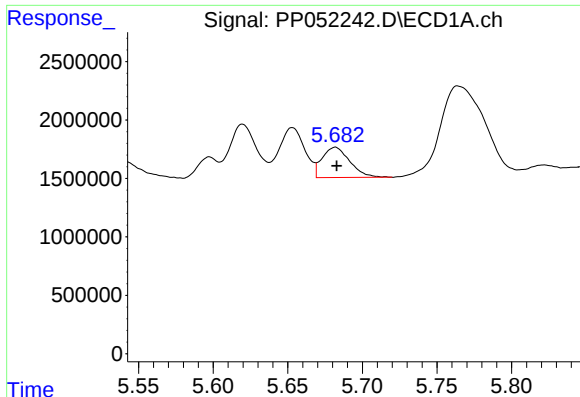

#5 AR-1016-3


R.T.: 5.682 min
Delta R.T.: 0.000 min
Response: 3337494
Conc: 80.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

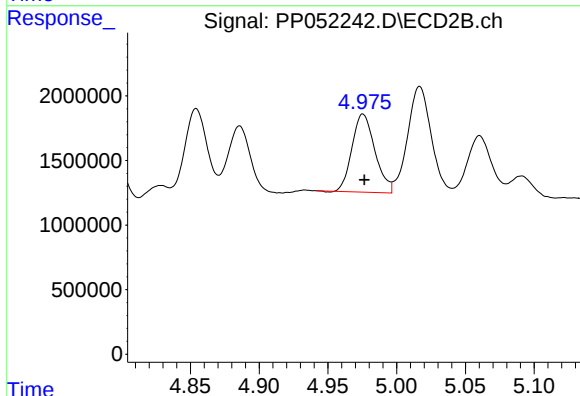


#5 AR-1016-3

R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 7006287
Conc: 210.78 ng/ml

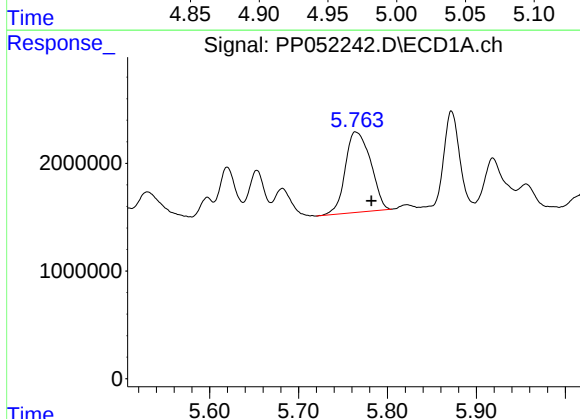


#6 AR-1016-4

R.T.: 5.764 min
Delta R.T.: -0.018 min
Response: 14796816
Conc: 407.24 ng/ml

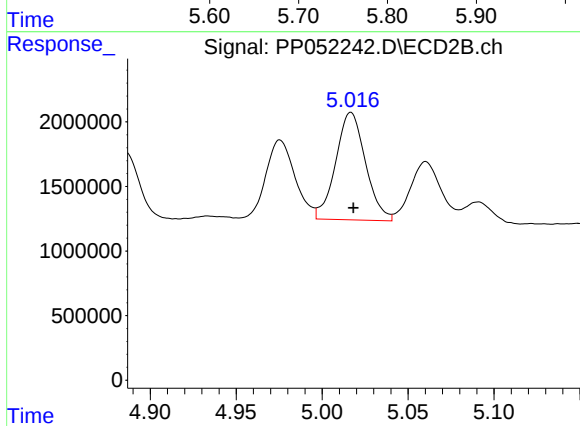

#6 AR-1016-4


R.T.: 5.017 min
Delta R.T.: -0.001 min
Response: 10052006
Conc: 368.81 ng/ml

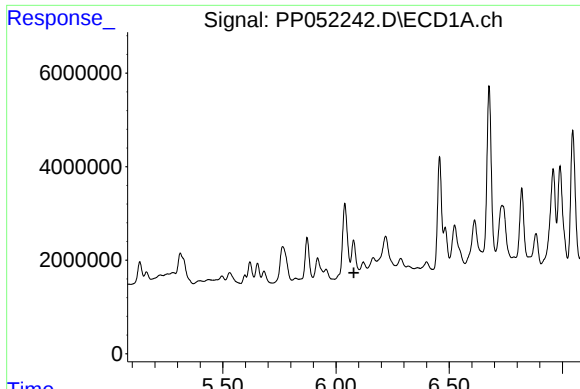

#7 AR-1016-5


R.T.: 6.077 min
Delta R.T.: -0.001 min
Response: -5029011
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

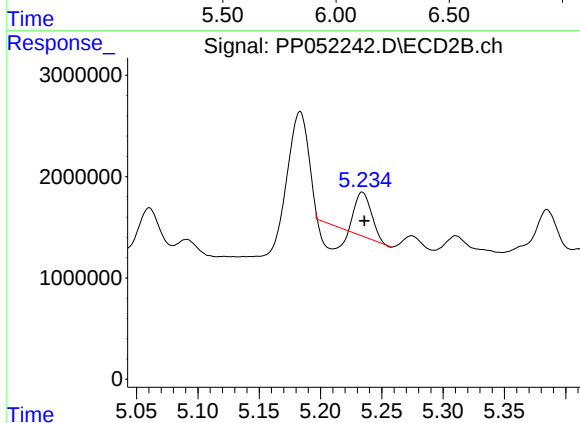


#7 AR-1016-5

R.T.: 5.234 min
Delta R.T.: -0.002 min
Response: 2080370
Conc: 58.80 ng/ml

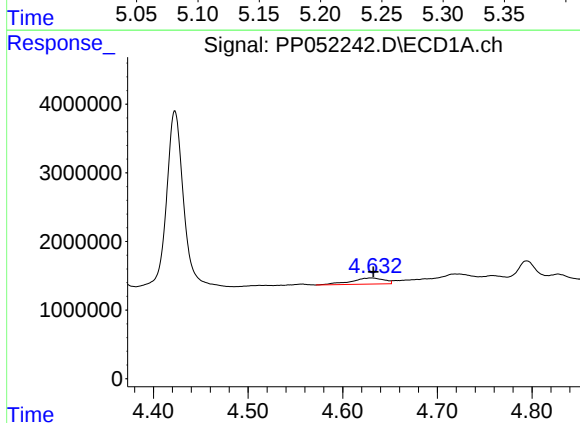


#8 AR-1221-1

R.T.: 4.631 min
Delta R.T.: -0.002 min
Response: 2148956
Conc: 103.99 ng/ml

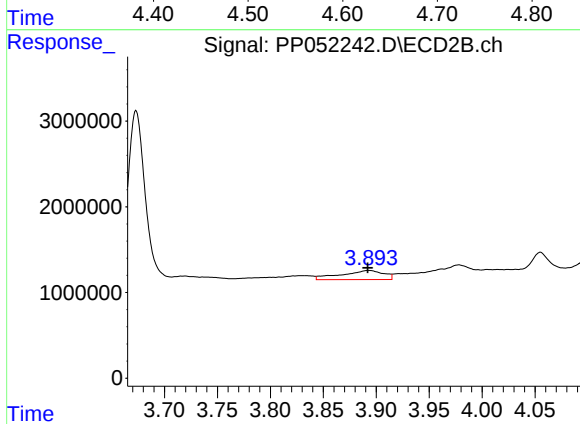

#8 AR-1221-1


R.T.: 3.893 min
Delta R.T.: 0.000 min
Response: 2972997
Conc: 190.14 ng/ml

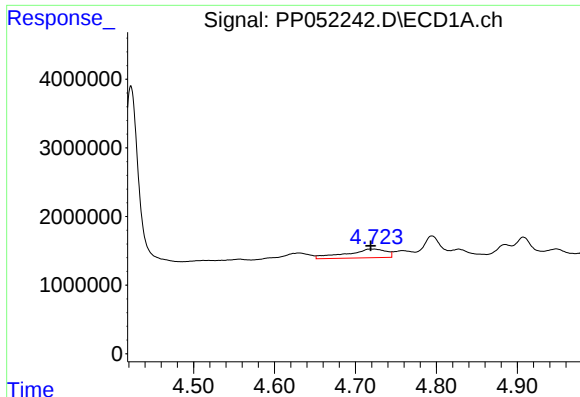

#9 AR-1221-2


R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 4395216
Conc: 287.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

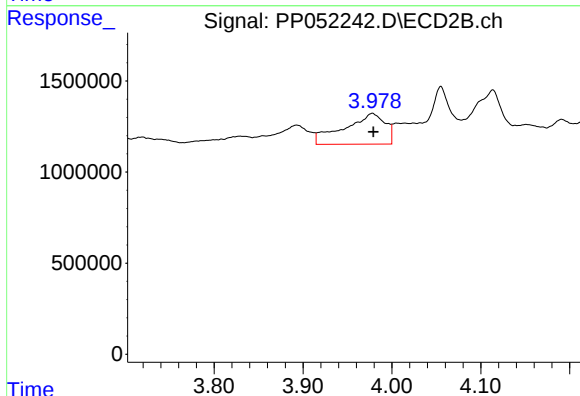


#9 AR-1221-2

R.T.: 3.978 min
Delta R.T.: -0.001 min
Response: 5409093
Conc: 451.03 ng/ml

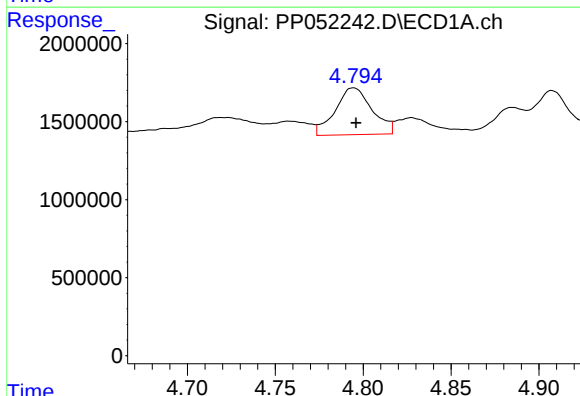


#10 AR-1221-3

R.T.: 4.794 min
Delta R.T.: -0.002 min
Response: 4392790
Conc: 93.82 ng/ml

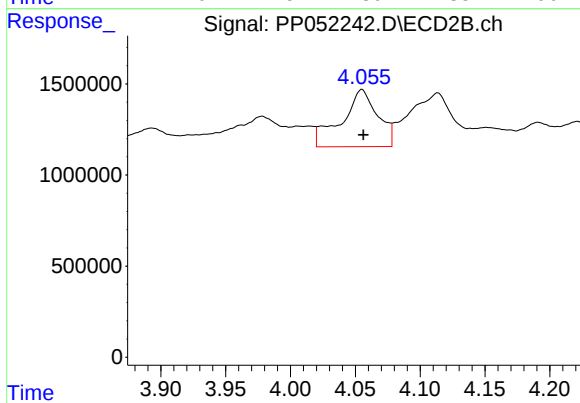

#10 AR-1221-3


R.T.: 4.055 min
Delta R.T.: -0.001 min
Response: 6104198
Conc: 161.51 ng/ml

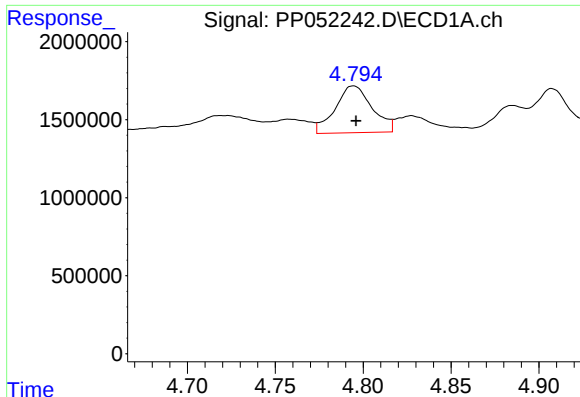

#11 AR-1232-1


R.T.: 4.794 min
Delta R.T.: -0.001 min
Response: 4392790
Conc: 121.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

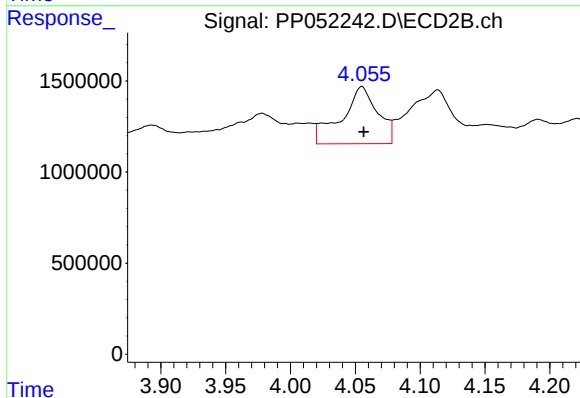


#11 AR-1232-1

R.T.: 4.055 min
Delta R.T.: -0.001 min
Response: 6104198
Conc: 210.62 ng/ml

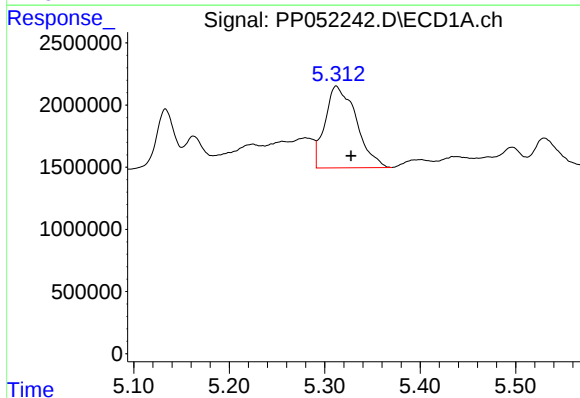


#12 AR-1232-2

R.T.: 5.312 min
Delta R.T.: -0.016 min
Response: 14948859
Conc: 736.77 ng/ml

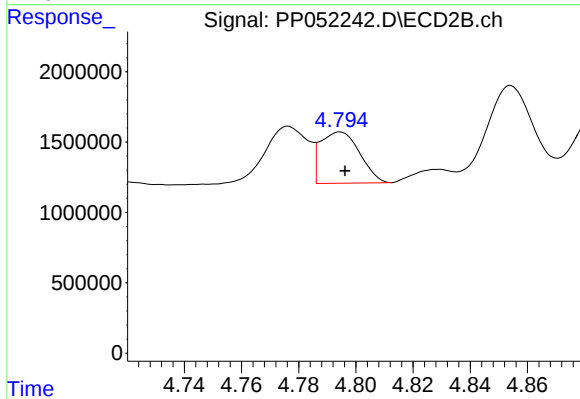

#12 AR-1232-2


R.T.: 4.794 min
Delta R.T.: -0.002 min
Response: 3474025
Conc: 115.97 ng/ml

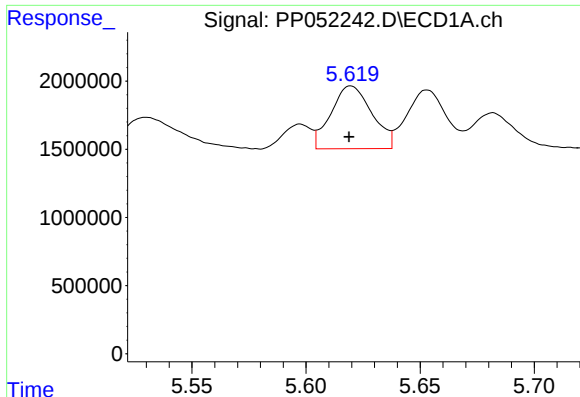

#13 AR-1232-3


R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 5763099
Conc: 191.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

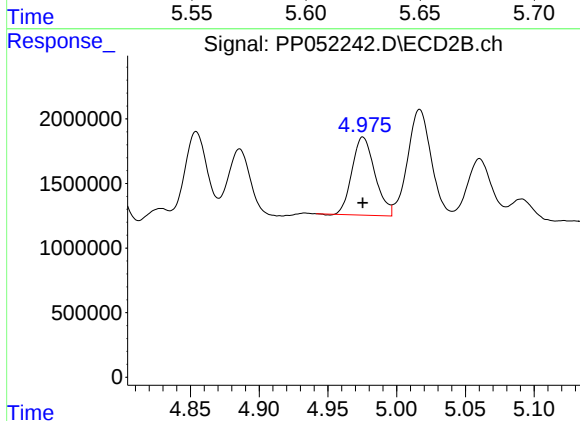


#13 AR-1232-3

R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 7006287
Conc: 458.60 ng/ml

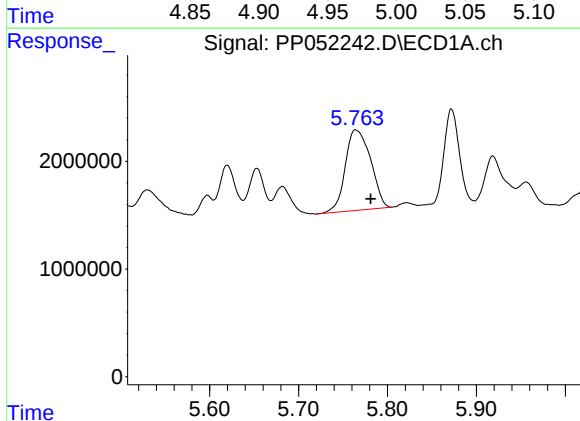


#14 AR-1232-4

R.T.: 5.764 min
Delta R.T.: -0.017 min
Response: 14796816
Conc: 887.22 ng/ml

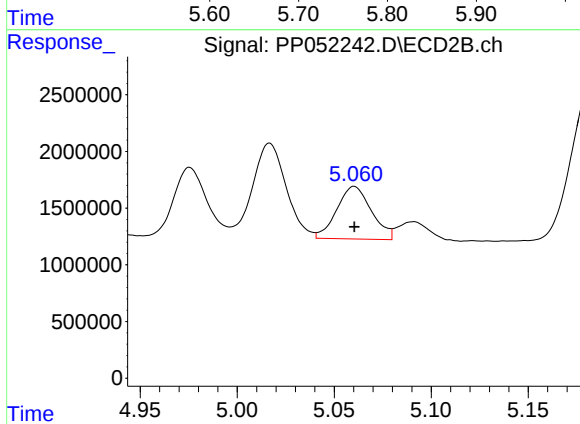

#14 AR-1232-4


R.T.: 5.060 min
Delta R.T.: 0.000 min
Response: 5783313
Conc: 408.41 ng/ml

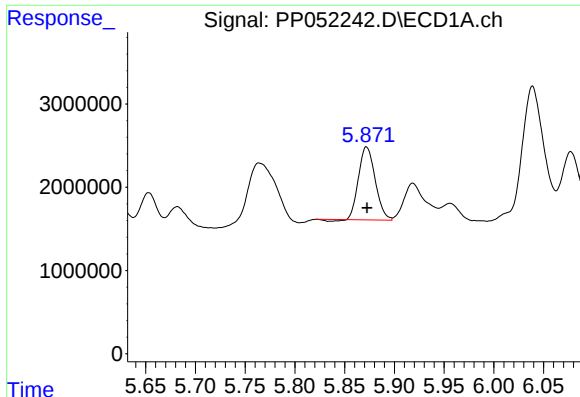

#15 AR-1232-5


R.T.: 5.872 min
Delta R.T.: 0.000 min
Response: 10102823
Conc: 673.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

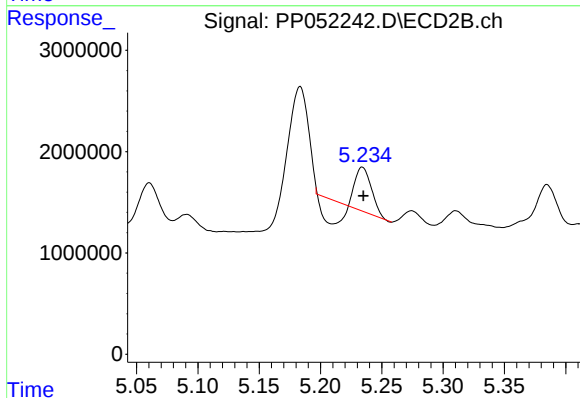


#15 AR-1232-5

R.T.: 5.234 min
Delta R.T.: 0.000 min
Response: 2080370
Conc: 131.42 ng/ml

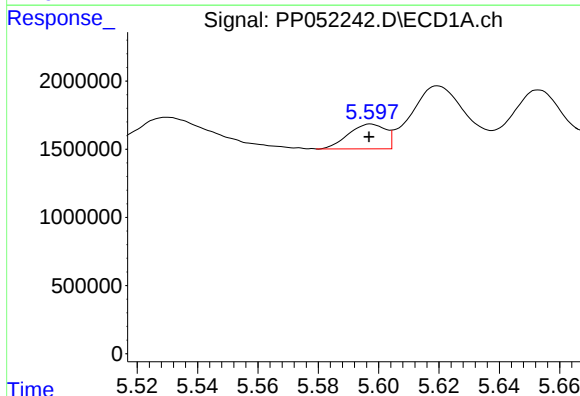


#16 AR-1242-1

R.T.: 5.598 min
Delta R.T.: 0.000 min
Response: 1552139
Conc: 44.62 ng/ml

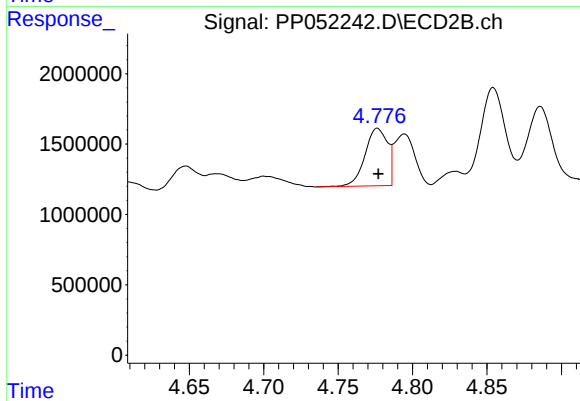

#16 AR-1242-1


R.T.: 4.776 min
Delta R.T.: 0.000 min
Response: 4306479
Conc: 123.68 ng/ml

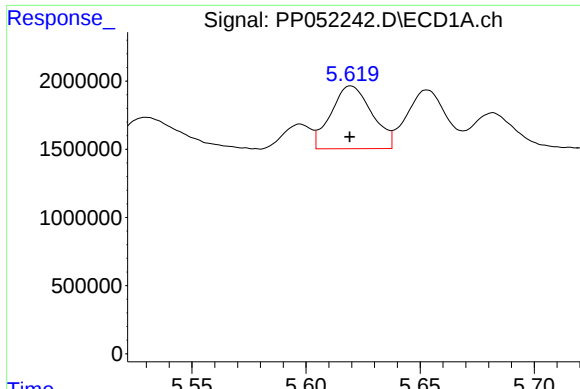

#17 AR-1242-2


R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 5763099
Conc: 116.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

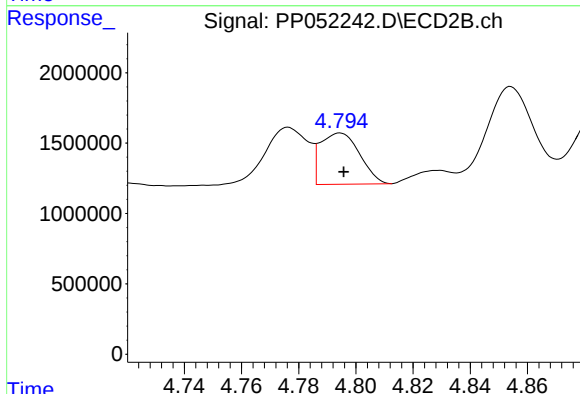


#17 AR-1242-2

R.T.: 4.794 min
Delta R.T.: -0.001 min
Response: 3474025
Conc: 70.42 ng/ml

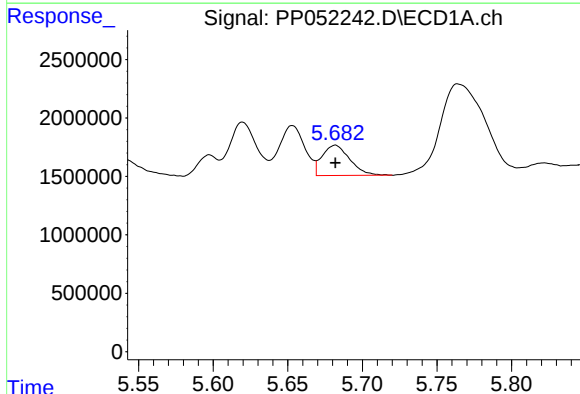


#18 AR-1242-3

R.T.: 5.682 min
Delta R.T.: 0.000 min
Response: 3337494
Conc: 105.26 ng/ml

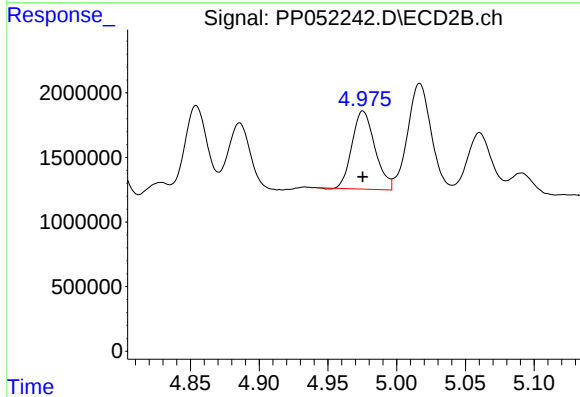

#18 AR-1242-3


R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 7006287
Conc: 268.40 ng/ml

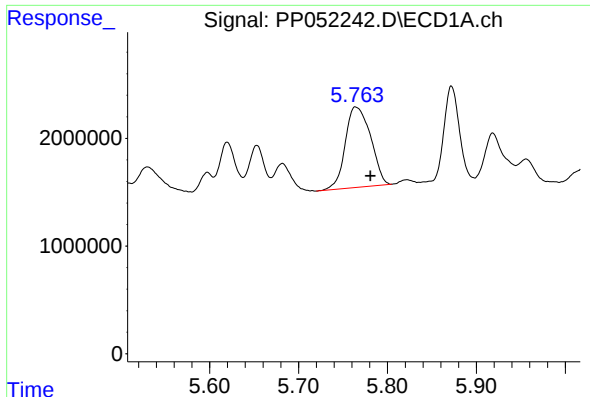

#19 AR-1242-4


R.T.: 5.764 min
Delta R.T.: -0.016 min
Response: 14796816
Conc: 541.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

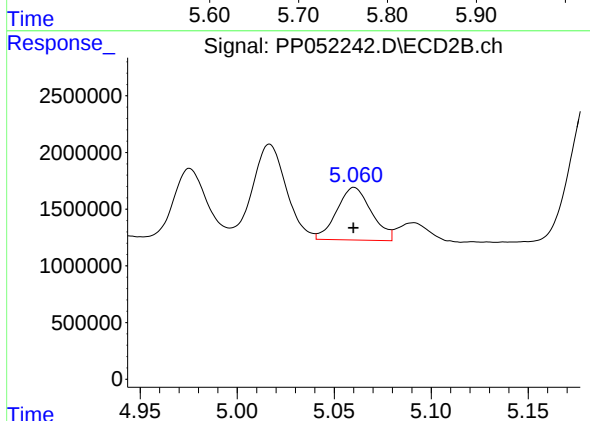


#19 AR-1242-4

R.T.: 5.060 min
Delta R.T.: 0.000 min
Response: 5783313
Conc: 212.62 ng/ml

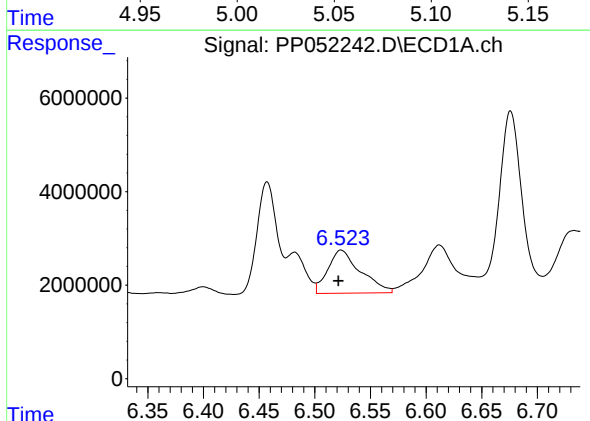


#20 AR-1242-5

R.T.: 6.524 min
Delta R.T.: 0.002 min
Response: 18868605
Conc: 507.53 ng/ml

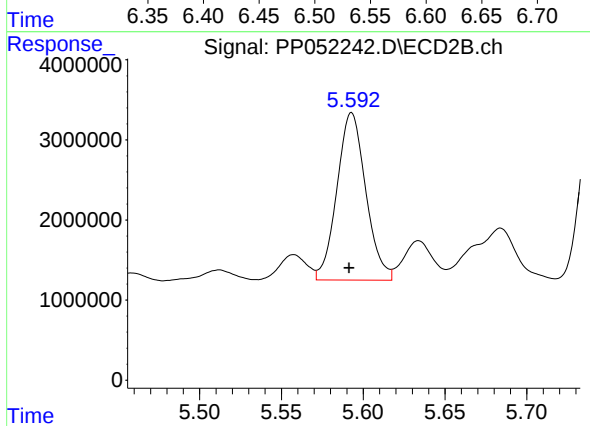

#20 AR-1242-5


R.T.: 5.593 min
Delta R.T.: 0.002 min
Response: 25685237
Conc: 762.17 ng/ml

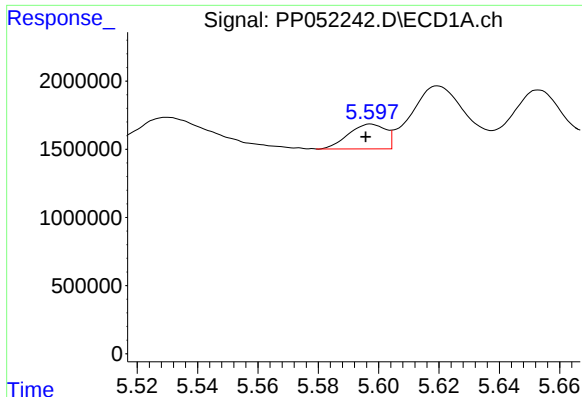

#21 AR-1248-1


R.T.: 5.598 min
Delta R.T.: 0.002 min
Response: 1552139
Conc: 57.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

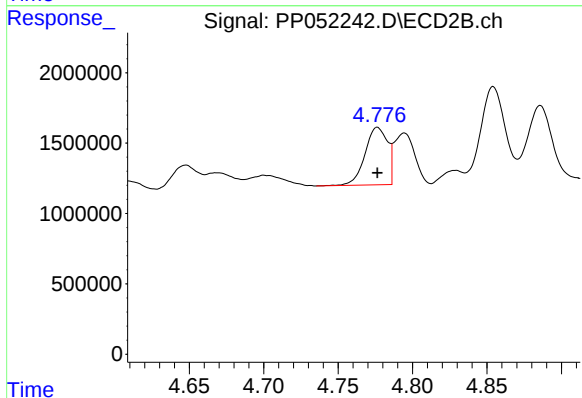


#21 AR-1248-1

R.T.: 4.776 min
Delta R.T.: 0.000 min
Response: 4306479
Conc: 158.84 ng/ml

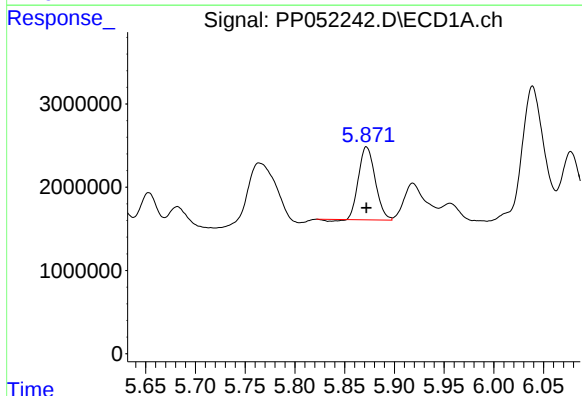


#22 AR-1248-2

R.T.: 5.872 min
Delta R.T.: 0.000 min
Response: 10102823
Conc: 217.35 ng/ml

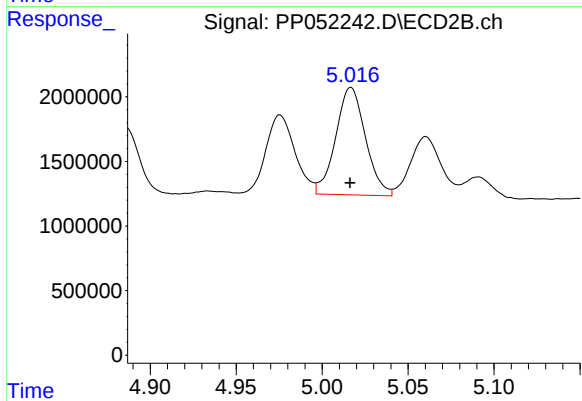

#22 AR-1248-2


R.T.: 5.017 min
Delta R.T.: 0.000 min
Response: 10052006
Conc: 270.18 ng/ml

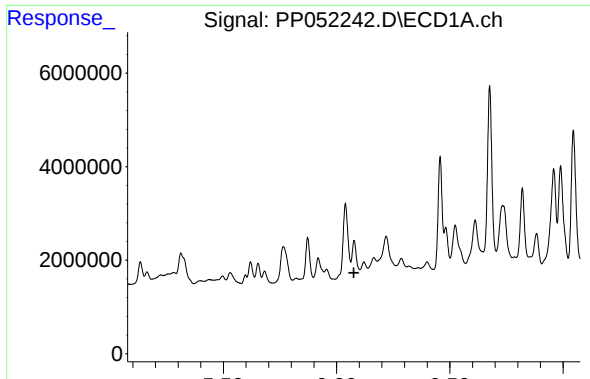

#23 AR-1248-3


R.T.: 6.077 min
Delta R.T.: 0.001 min
Response: -5029011
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

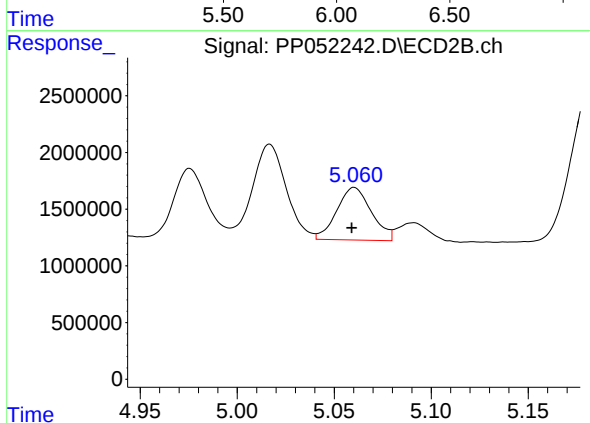


#23 AR-1248-3

R.T.: 5.060 min
Delta R.T.: 0.001 min
Response: 5783313
Conc: 151.81 ng/ml

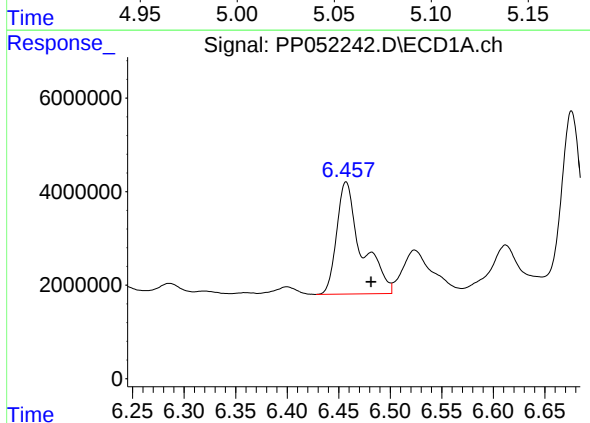


#24 AR-1248-4

R.T.: 6.457 min
Delta R.T.: -0.024 min
Response: 40049194
Conc: 630.77 ng/ml

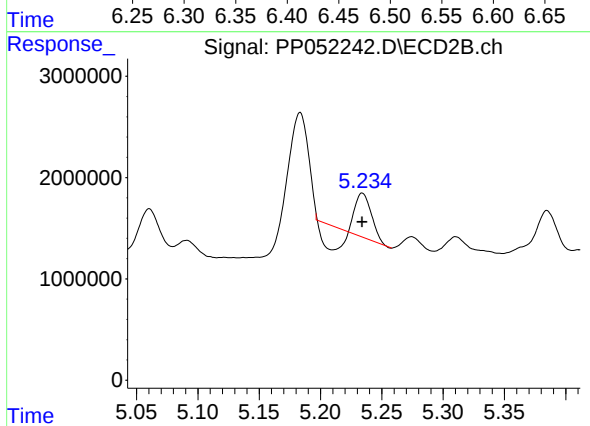

#24 AR-1248-4


R.T.: 5.234 min
Delta R.T.: 0.000 min
Response: 2080370
Conc: 44.90 ng/ml

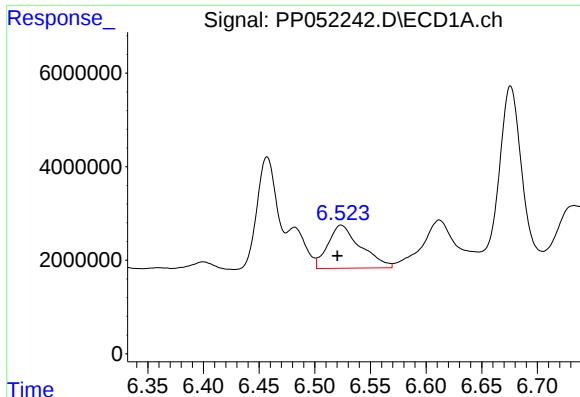

#25 AR-1248-5


R.T.: 6.524 min
Delta R.T.: 0.003 min
Response: 18868605
Conc: 304.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

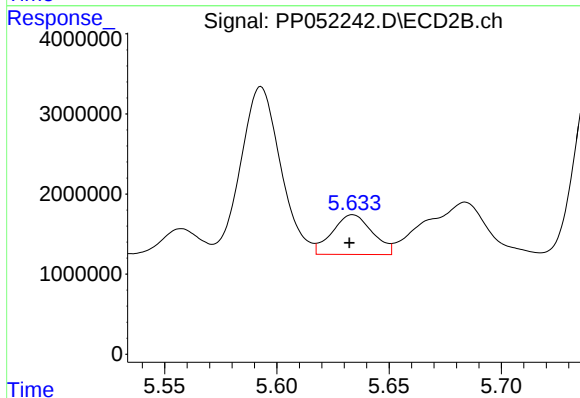


#25 AR-1248-5

R.T.: 5.634 min
Delta R.T.: 0.002 min
Response: 6191190
Conc: 147.22 ng/ml

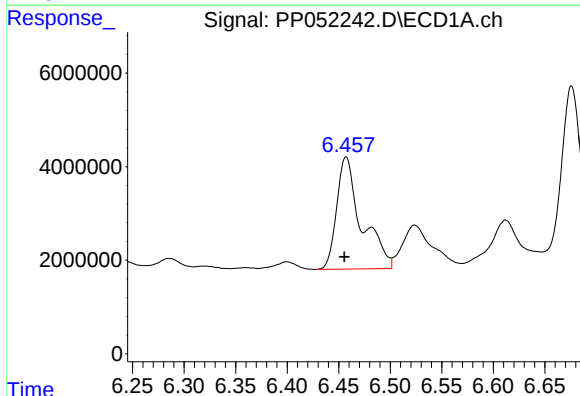


#26 AR-1254-1

R.T.: 6.457 min
Delta R.T.: 0.002 min
Response: 40049194
Conc: 562.57 ng/ml

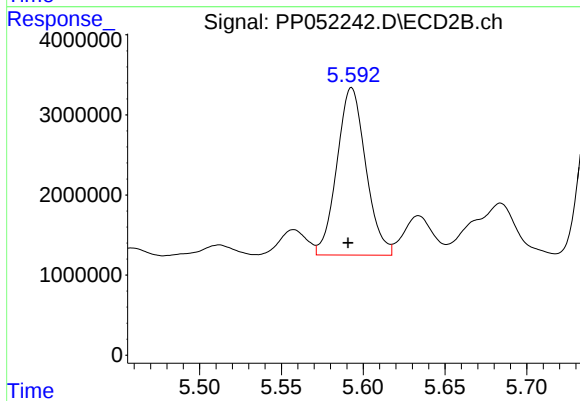

#26 AR-1254-1


R.T.: 5.593 min
Delta R.T.: 0.002 min
Response: 25685237
Conc: 367.13 ng/ml

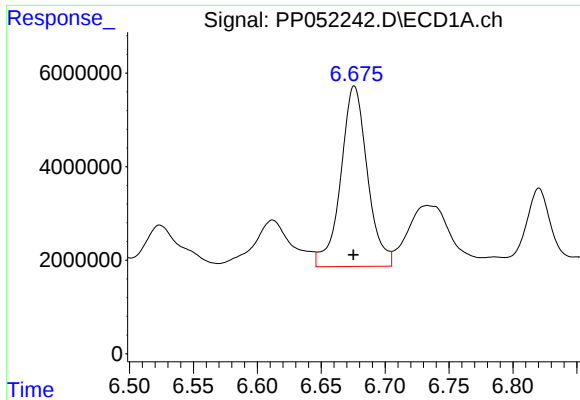

#27 AR-1254-2


R.T.: 6.676 min
Delta R.T.: 0.000 min
Response: 55968509
Conc: 524.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

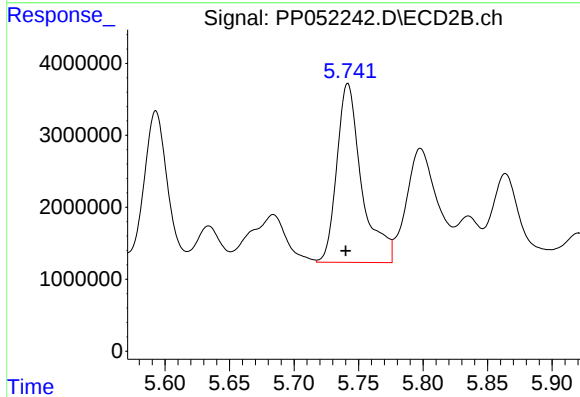


#27 AR-1254-2

R.T.: 5.742 min
Delta R.T.: 0.002 min
Response: 33315834
Conc: 531.74 ng/ml

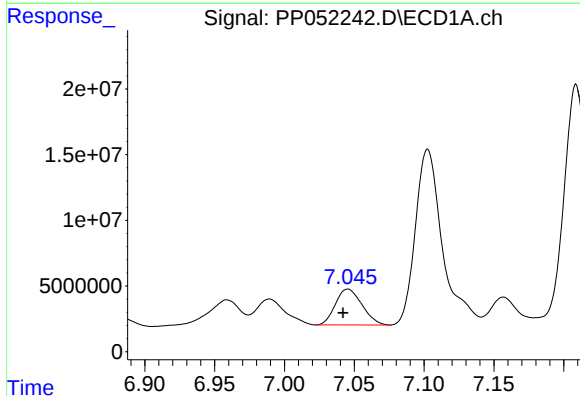


#28 AR-1254-3

R.T.: 7.046 min
Delta R.T.: 0.004 min
Response: 36122753
Conc: 343.70 ng/ml

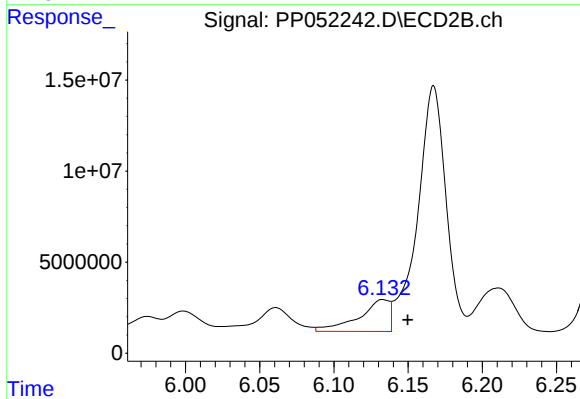

#28 AR-1254-3


R.T.: 6.133 min
Delta R.T.: -0.017 min
Response: 25038380
Conc: 253.12 ng/ml

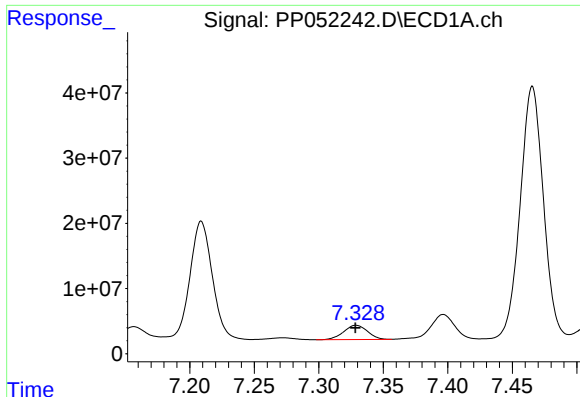

#29 AR-1254-4


R.T.: 7.329 min
Delta R.T.: 0.000 min
Response: 28156781
Conc: 385.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

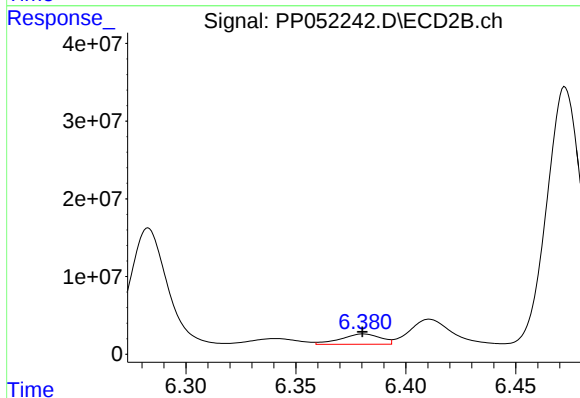


#29 AR-1254-4

R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 16654415
Conc: 278.61 ng/ml

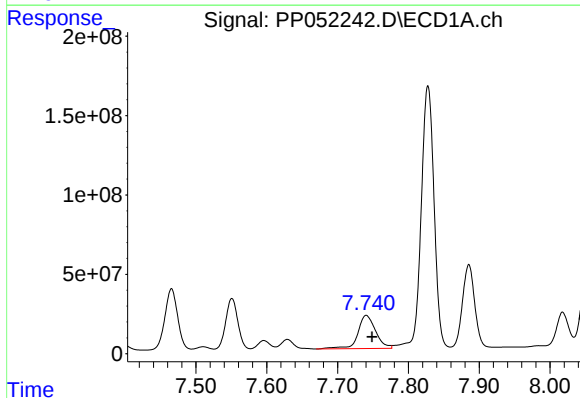


#30 AR-1254-5

R.T.: 7.741 min
Delta R.T.: -0.008 min
Response: 361978007
Conc: 4362.57 ng/ml

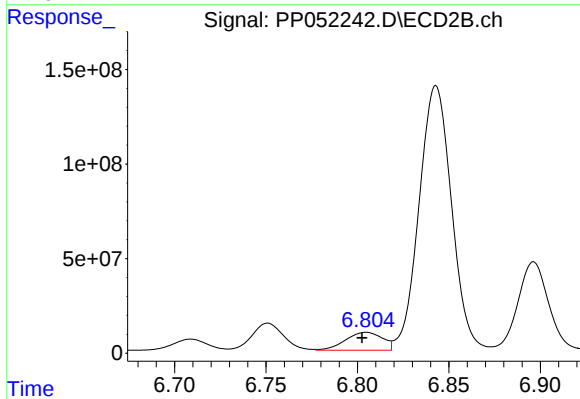

#30 AR-1254-5


R.T.: 6.805 min
Delta R.T.: 0.002 min
Response: 132427314
Conc: 1493.75 ng/ml

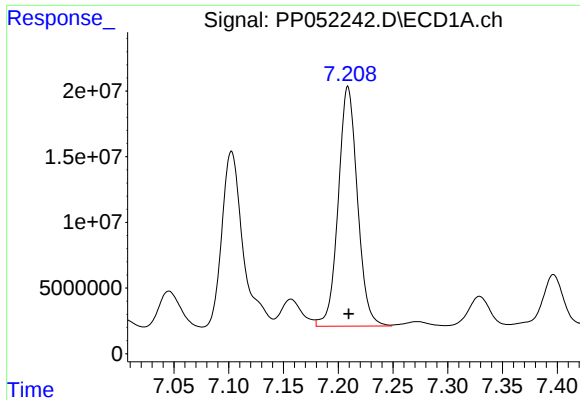

#31 AR-1260-1


R.T.: 7.209 min
Delta R.T.: 0.000 min
Response: 222847316
Conc: 2688.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

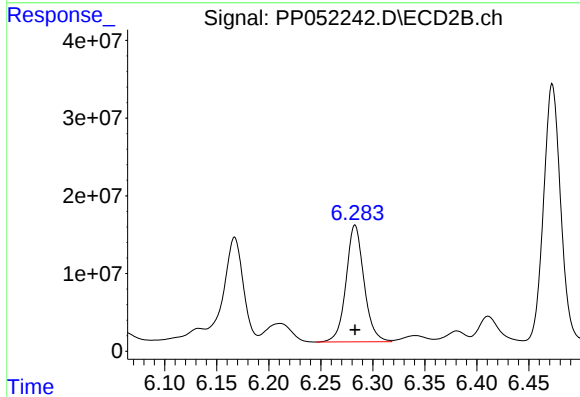


#31 AR-1260-1

R.T.: 6.283 min
Delta R.T.: 0.000 min
Response: 180473576
Conc: 2620.02 ng/ml

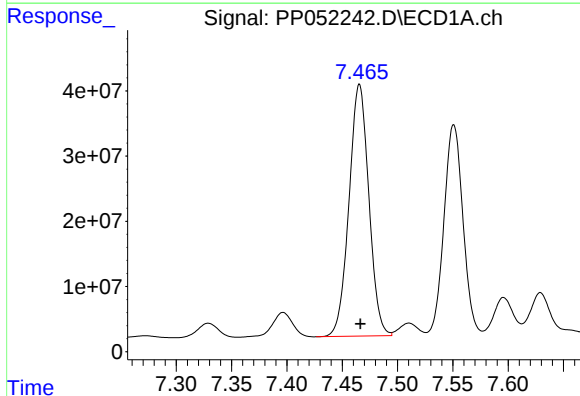


#32 AR-1260-2

R.T.: 7.466 min
Delta R.T.: 0.000 min
Response: 481520579
Conc: 5101.66 ng/ml

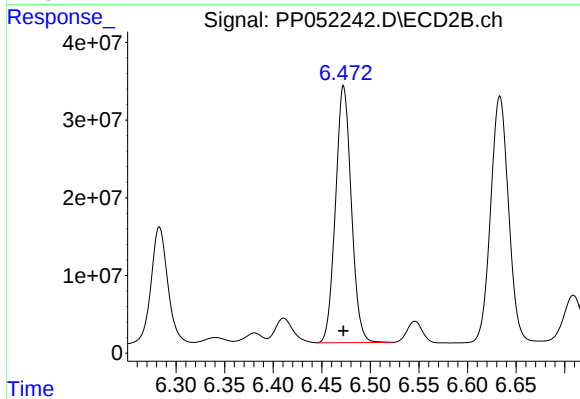

#32 AR-1260-2


R.T.: 6.472 min
Delta R.T.: 0.000 min
Response: 374632122
Conc: 4526.39 ng/ml

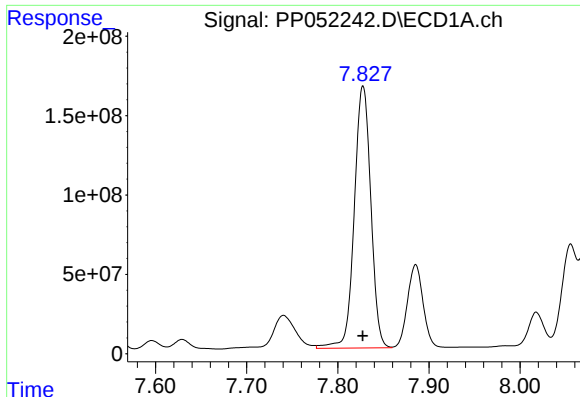

#33 AR-1260-3


R.T.: 7.828 min
Delta R.T.: 0.000 min
Response: 2084509413
Conc: 34707.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

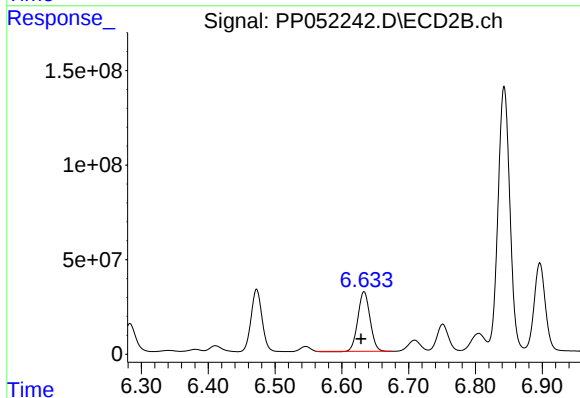


#33 AR-1260-3

R.T.: 6.633 min
Delta R.T.: 0.005 min
Response: 395785108
Conc: 5126.24 ng/ml

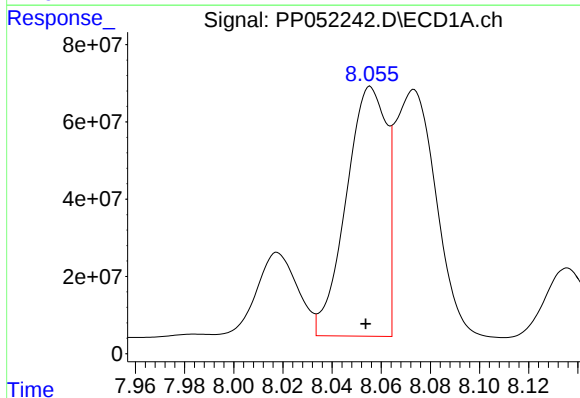


#34 AR-1260-4

R.T.: 8.056 min
Delta R.T.: 0.002 min
Response: 736174076
Conc: 9598.86 ng/ml

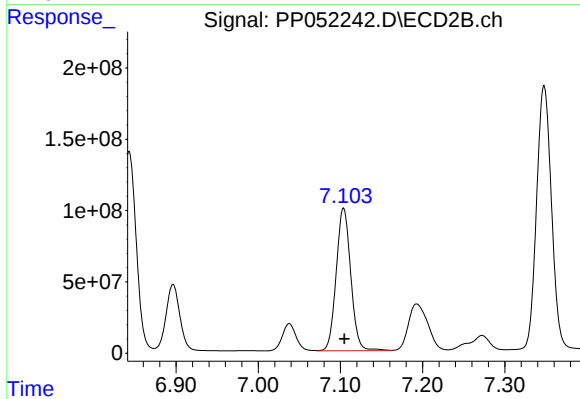

#34 AR-1260-4


R.T.: 7.104 min
Delta R.T.: 0.000 min
Response: 1234330491
Conc: 21957.49 ng/ml

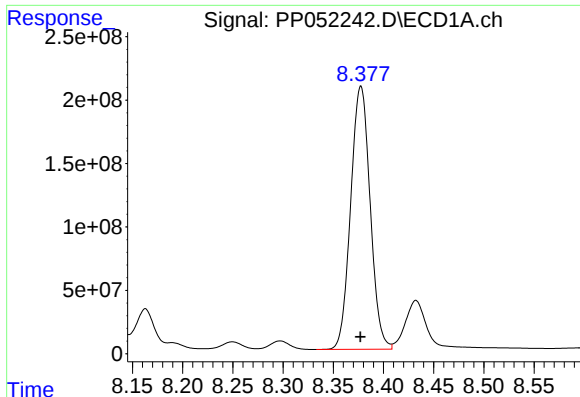

#35 AR-1260-5


R.T.: 8.377 min
Delta R.T.: 0.000 min
Response: 2801275146
Conc: 20435.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

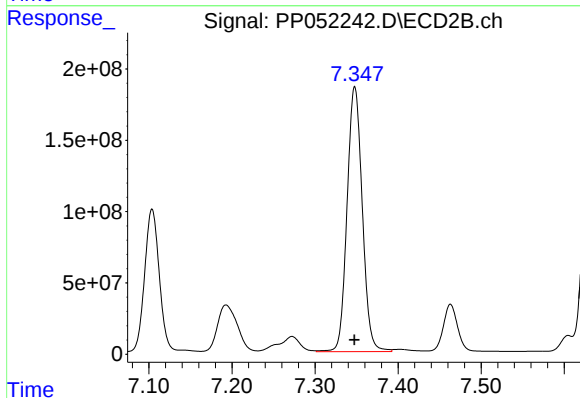


#35 AR-1260-5

R.T.: 7.348 min
Delta R.T.: 0.000 min
Response: 2368980025
Conc: 17963.54 ng/ml

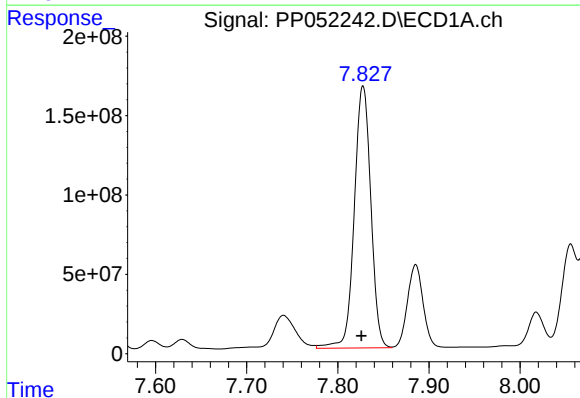


#36 AR-1262-1

R.T.: 7.828 min
Delta R.T.: 0.002 min
Response: 2084509413
Conc: 21497.75 ng/ml

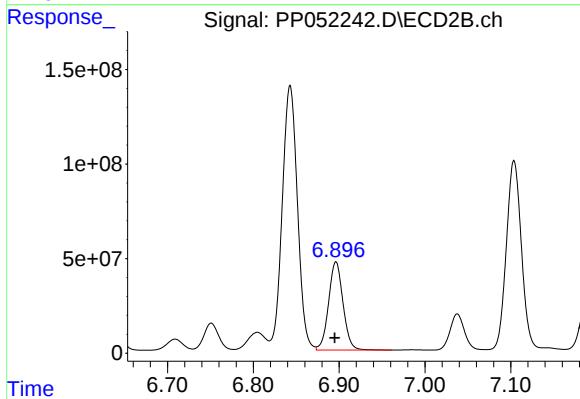

#36 AR-1262-1


R.T.: 6.896 min
Delta R.T.: 0.002 min
Response: 546070735
Conc: 15180.62 ng/ml

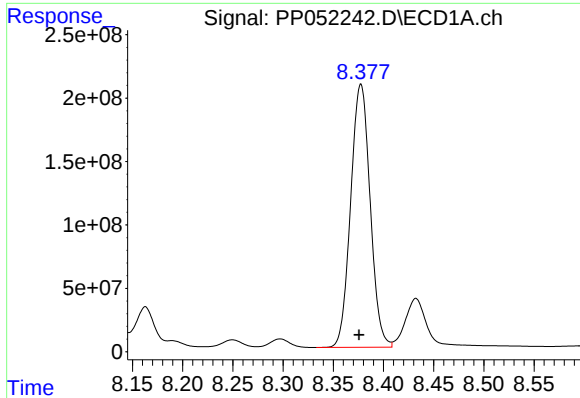

#37 AR-1262-2


R.T.: 8.377 min
Delta R.T.: 0.002 min
Response: 2801275146
Conc: 17398.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

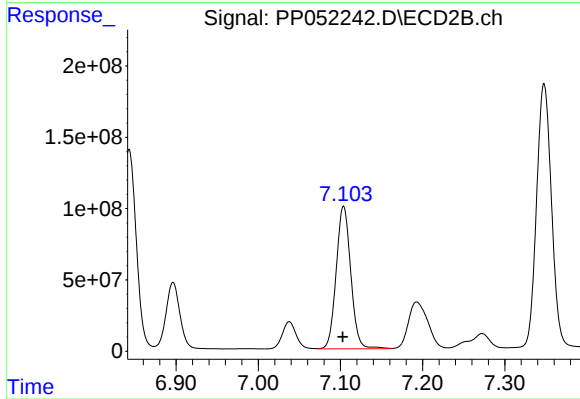


#37 AR-1262-2

R.T.: 7.104 min
Delta R.T.: 0.000 min
Response: 1234330491
Conc: 15588.16 ng/ml

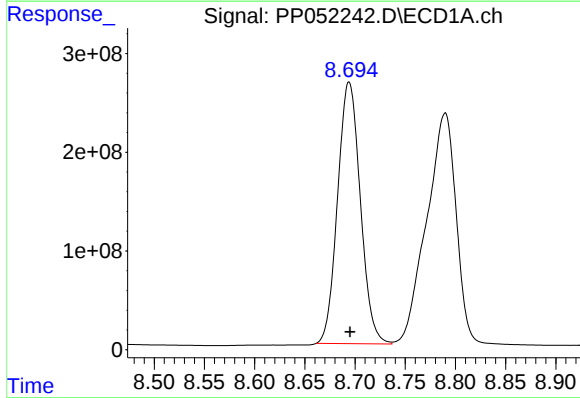


#38 AR-1262-3

R.T.: 8.694 min
Delta R.T.: 0.000 min
Response: 4181445991
Conc: 38047.80 ng/ml

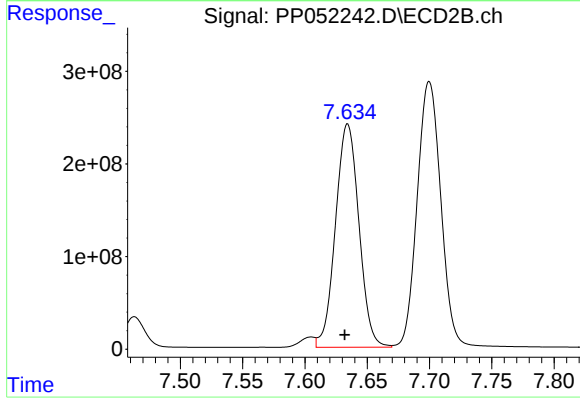

#38 AR-1262-3


R.T.: 7.634 min
Delta R.T.: 0.002 min
Response: 3160604053
Conc: 51182.14 ng/ml

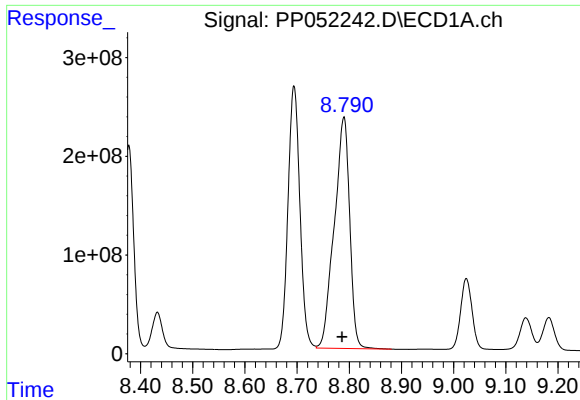

#39 AR-1262-4


R.T.: 8.789 min
Delta R.T.: 0.003 min
Response: 481021777
Conc: 94099.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

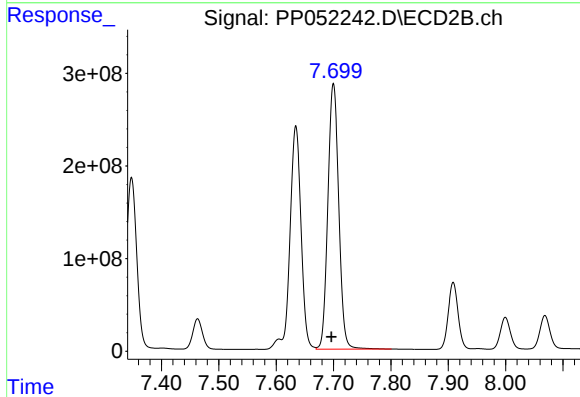


#39 AR-1262-4

R.T.: 7.700 min
Delta R.T.: 0.003 min
Response: 3803293088
Conc: 33314.49 ng/ml

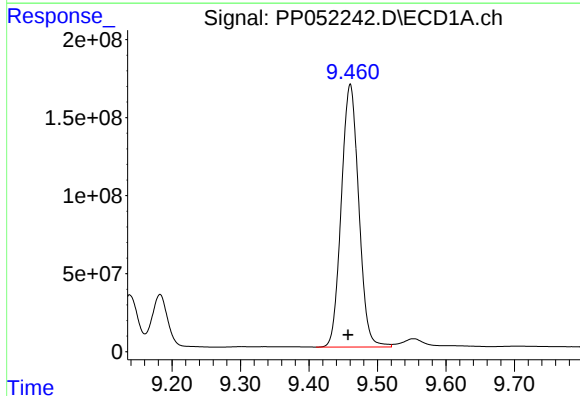


#40 AR-1262-5

R.T.: 9.460 min
Delta R.T.: 0.003 min
Response: 2979260540
Conc: 47328.15 ng/ml

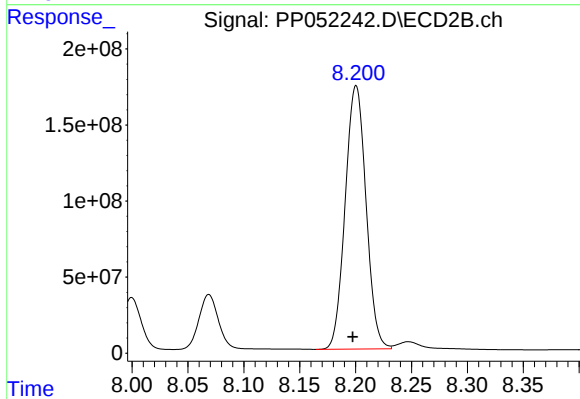

#40 AR-1262-5


R.T.: 8.200 min
Delta R.T.: 0.003 min
Response: 2251135690
Conc: 44288.77 ng/ml

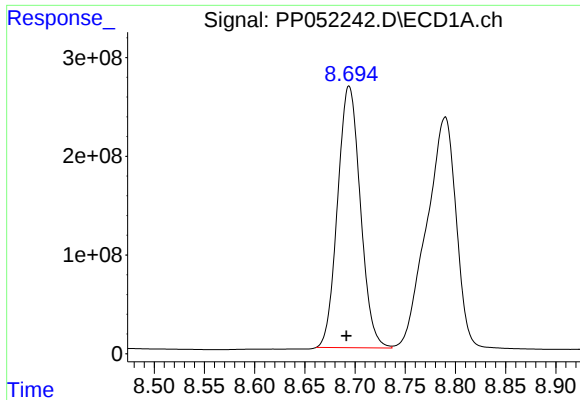

#41 AR-1268-1


R.T.: 8.694 min
Delta R.T.: 0.003 min
Response: 4181445991
Conc: 21120.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

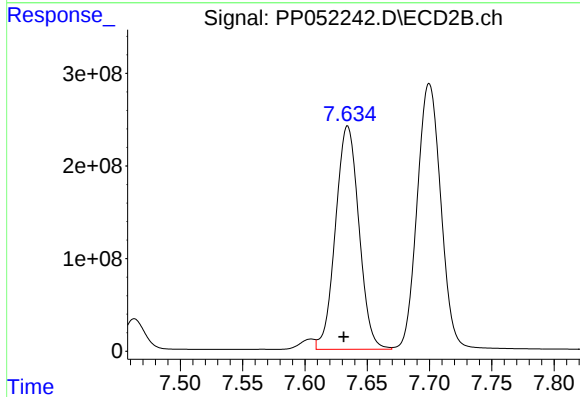


#41 AR-1268-1

R.T.: 7.634 min
Delta R.T.: 0.003 min
Response: 3160604053
Conc: 17422.42 ng/ml

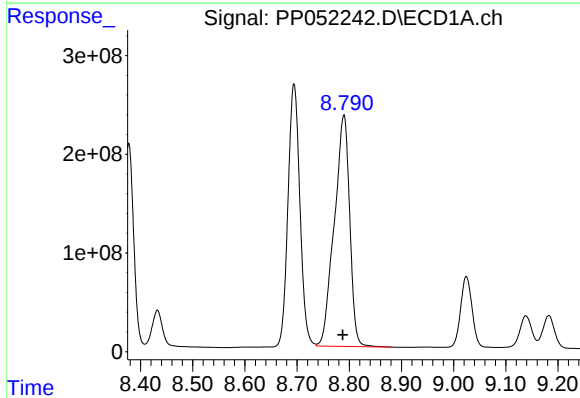


#42 AR-1268-2

R.T.: 8.789 min
Delta R.T.: 0.002 min
Response: 4810217777
Conc: 26196.28 ng/ml

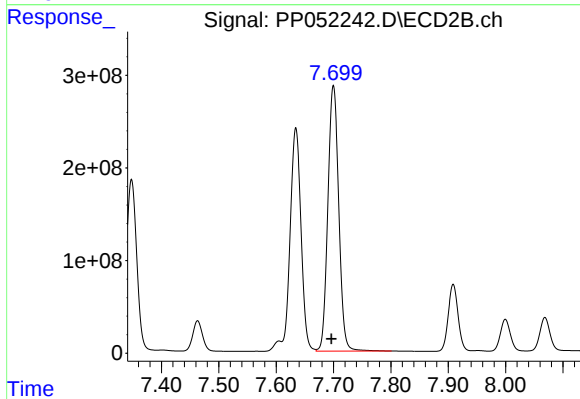

#42 AR-1268-2


R.T.: 7.700 min
Delta R.T.: 0.003 min
Response: 3803293088
Conc: 23277.81 ng/ml

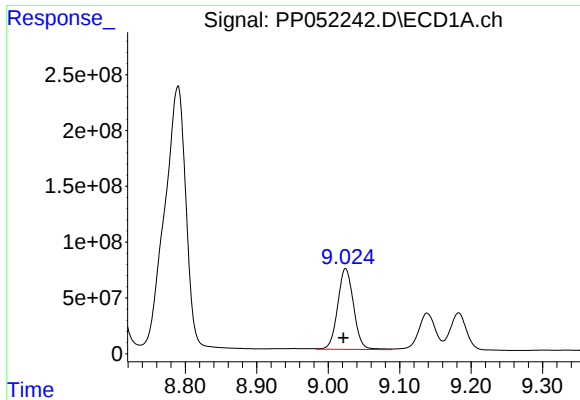

#43 AR-1268-3


R.T.: 9.024 min
Delta R.T.: 0.003 min
Response: 1118330109
Conc: 6860.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

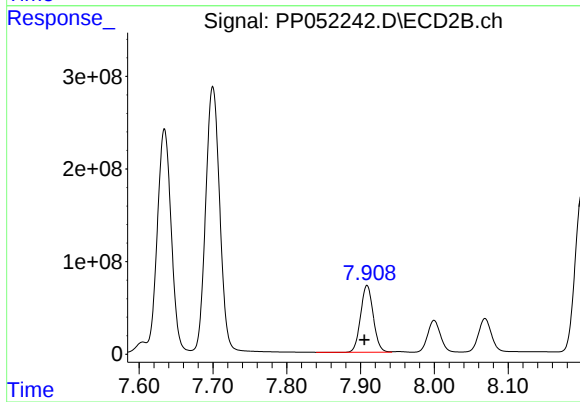


#43 AR-1268-3

R.T.: 7.909 min
Delta R.T.: 0.004 min
Response: 859225710
Conc: 6110.16 ng/ml

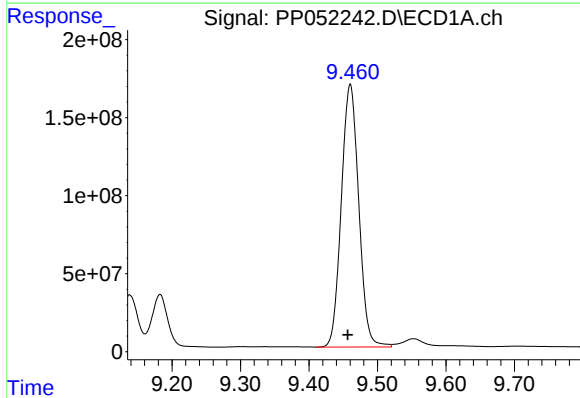


#44 AR-1268-4

R.T.: 9.460 min
Delta R.T.: 0.004 min
Response: 2979260540
Conc: 40833.09 ng/ml

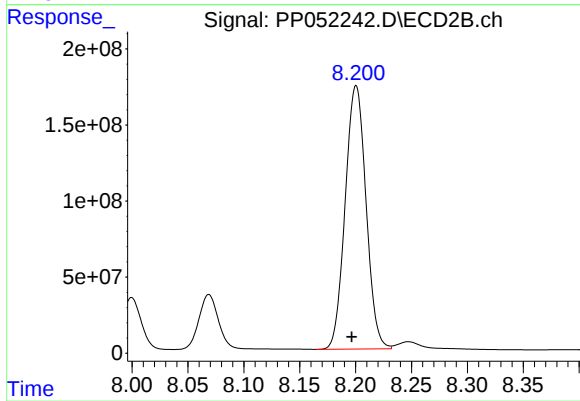

#44 AR-1268-4


R.T.: 8.200 min
Delta R.T.: 0.004 min
Response: 2251135690
Conc: 39835.13 ng/ml

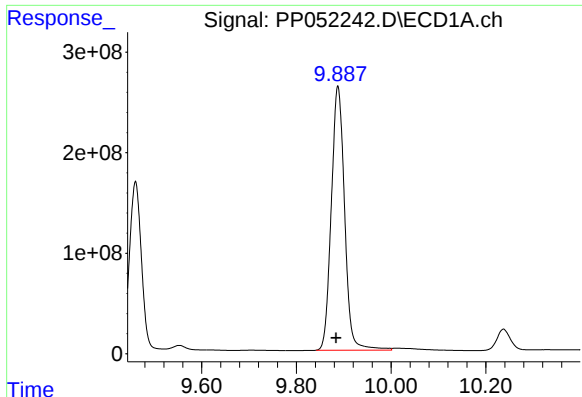

#45 AR-1268-5

R.T.: 9.888 min
Delta R.T.: 0.004 min
Response: 5126356948
Conc: 9831.10 ng/m

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-4

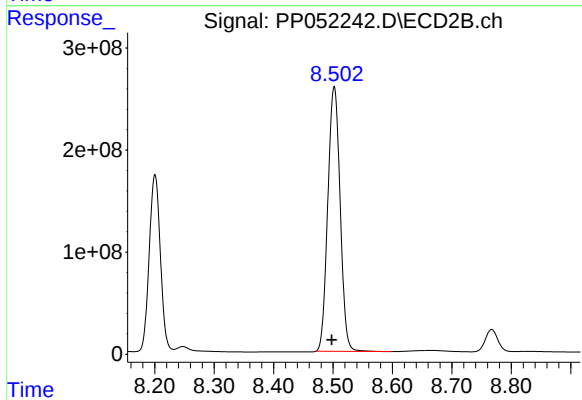

#45 AR-1268-5

R.T.: 8.502 min
Delta R.T.: 0.004 min
Response: 3738841466
Conc: 8888.04 ng/ml