

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
 Data File : PP052243.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 20:08
 Operator : YP\AJ
 Sample : N5059-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RB10622-01-BASEMENT-BATHROOM-SINK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 05:42:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 12 05:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.422	3.673	37695331	28563080	23.981	24.932
2)	SA Decachlor...	10.239	8.766	30978740	15685764	22.321	14.038 #
Target Compounds							
3)	L1 AR-1016-1	5.618f	4.797f	110216	362334	2.424	8.147 #
4)	L1 AR-1016-2	5.618	4.797	110216	362334	1.674	5.694 #
5)	L1 AR-1016-3	0.000	4.974	0	666860	N.D.	20.062 #
6)	L1 AR-1016-4	5.795	5.018	1046230	2350292	28.794	86.233 #
7)	L1 AR-1016-5	0.000	5.235	0	2171808	N.D.	61.387 #
8)	L2 AR-1221-1	4.629	3.913f	554203	14162993	26.819	905.820 #
9)	L2 AR-1221-2	4.725	3.983	704581	2345221	46.041	195.552 #
10)	L2 AR-1221-3	4.786	4.062	548610	1961718	11.717	51.904 #
11)	L3 AR-1232-1	4.786	4.062	548610	1961718	15.228	67.688 #
12)	L3 AR-1232-2	0.000	4.797	0	362334	N.D.	12.096 #
13)	L3 AR-1232-3	5.618	4.974	110216	666860	3.660	43.650 #
14)	L3 AR-1232-4	5.795	0.000	1046230	0	62.732	N.D. #
15)	L3 AR-1232-5	5.878	5.235	1968143	2171808	131.229	137.194
16)	L4 AR-1242-1	5.618f	4.797f	110216	362334	3.168	10.406 #
17)	L4 AR-1242-2	5.618	4.797	110216	362334	2.226	7.345 #
18)	L4 AR-1242-3	0.000	4.974	0	666860	N.D.	25.546 #
19)	L4 AR-1242-4	5.795	0.000	1046230	0	38.302	N.D. #
20)	L4 AR-1242-5	6.524	5.597	1537252	1626068	41.349	48.251
21)	L5 AR-1248-1	5.618f	4.797f	110216	362334	4.100	13.365 #
22)	L5 AR-1248-2	5.878	5.018	1968143	2350292	42.342	63.172 #
24)	L5 AR-1248-4	6.489	5.235	2168117	2171808	34.147	46.872 #
25)	L5 AR-1248-5	6.524	0.000	1537252	0	24.820	N.D. #
26)	L6 AR-1254-1	0.000	5.597	0	1626068	N.D.	23.242 #
27)	L6 AR-1254-2	6.676	0.000	7102940	0	66.599	N.D. #
28)	L6 AR-1254-3	7.032	0.000	3600673	0	34.260	N.D. #
29)	L6 AR-1254-4	0.000	6.361f	0	6356276	N.D.	106.333 #
30)	L6 AR-1254-5	7.755	6.776f	26533649	10884778	319.784	122.778 #
31)	L7 AR-1260-1	7.213	0.000	418239	0	5.046	N.D. #
32)	L7 AR-1260-2	7.451f	0.000	423823	0	4.490	N.D. #
34)	L7 AR-1260-4	8.051	7.105	-495002	11872706	N.D.	211.203 #
35)	L7 AR-1260-5	0.000	7.363f	0	99929838	N.D.	757.750 #
36)	L8 AR-1262-1	0.000	6.886	0	12165852	N.D.	338.207 #
37)	L8 AR-1262-2	0.000	7.105	0	11872706	N.D.	149.938 #
39)	L8 AR-1262-4	8.782	7.712f	17197937	99021652	336.432	867.368 #
40)	L8 AR-1262-5	9.452	0.000	27309670	0	433.838	N.D. #
42)	L9 AR-1268-2	8.782	7.712f	17197937	99021652	93.659	606.056 #
44)	L9 AR-1268-4	9.452	0.000	27309670	0	374.300	N.D. #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
Data File : PP052243.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 20:08
Operator : YP\AJ
Sample : N5059-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 05:42:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.						


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
Data File : PP052243.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 20:08
Operator : YP\AJ
Sample : N5059-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 05:42:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

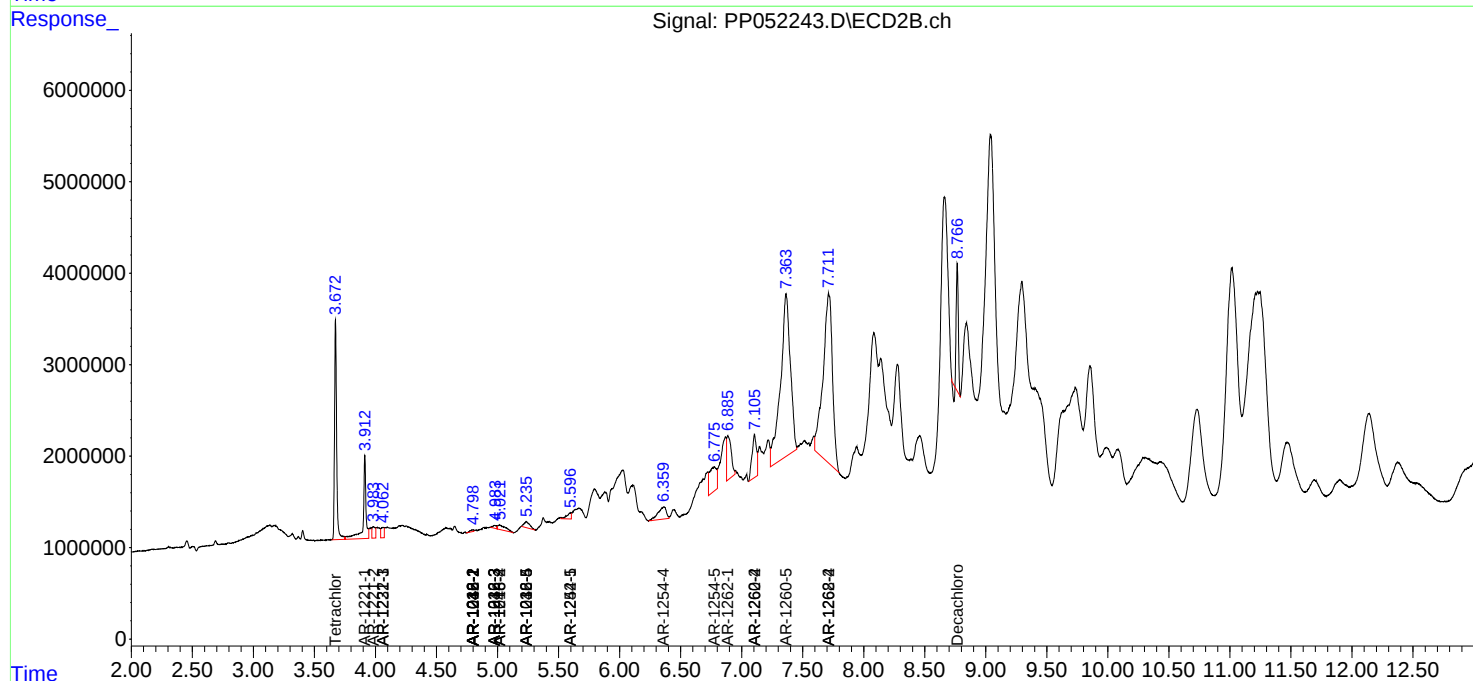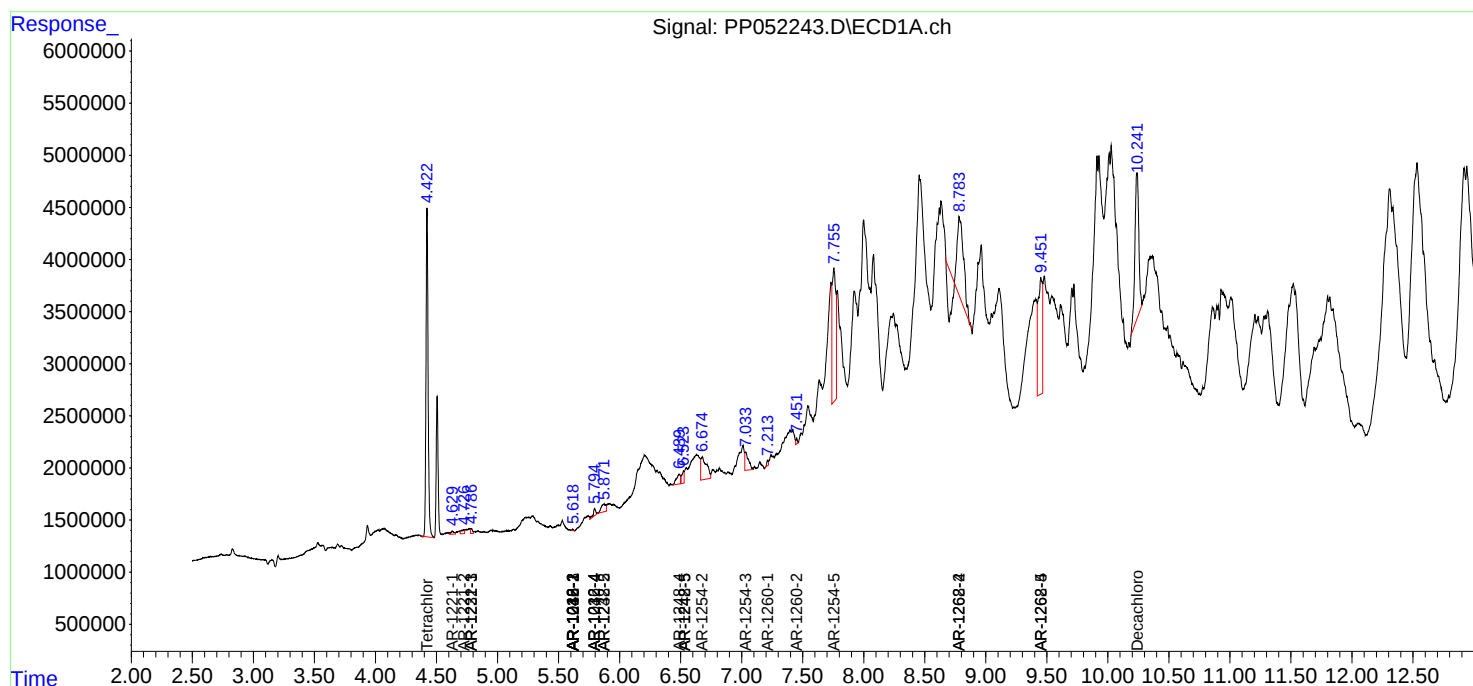

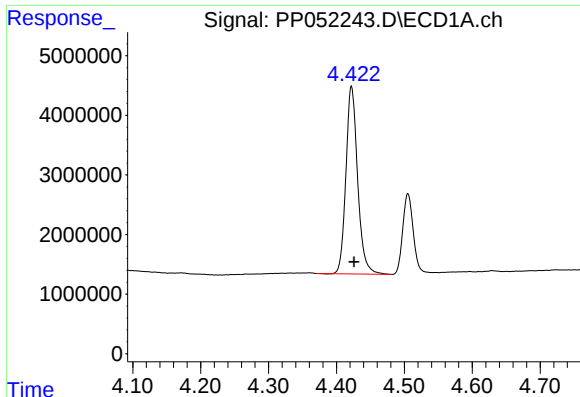

#1 Tetrachloro-m-xylene


R.T.: 4.422 min
Delta R.T.: -0.004 min
Response: 37695331
Conc: 23.98 ng/ml

Instrument :

ECD_P


ClientSampleId :

RB10622-01-BASEMENT-BATHROOM-SINK

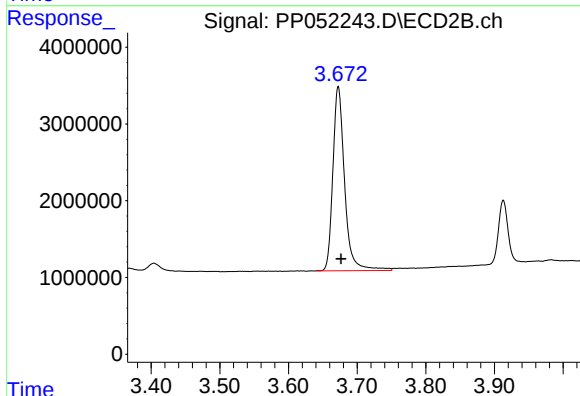


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: -0.004 min
Response: 28563080
Conc: 24.93 ng/ml

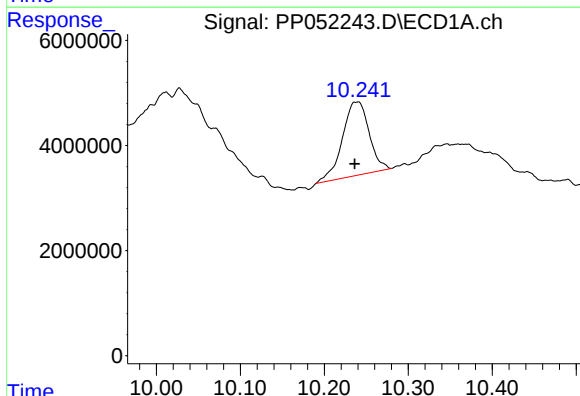


#2 Decachlorobiphenyl

R.T.: 10.239 min
Delta R.T.: 0.002 min
Response: 30978740
Conc: 22.32 ng/ml

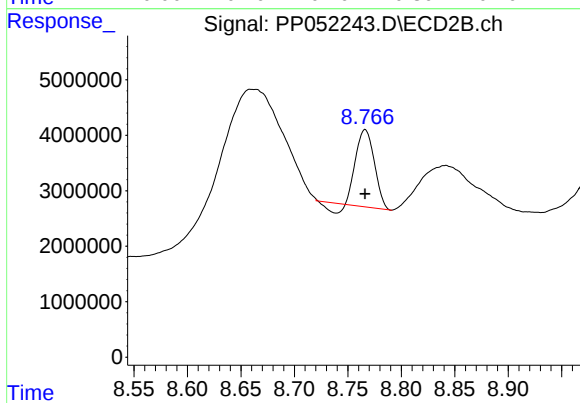

#2 Decachlorobiphenyl


R.T.: 8.766 min
Delta R.T.: 0.000 min
Response: 15685764
Conc: 14.04 ng/ml

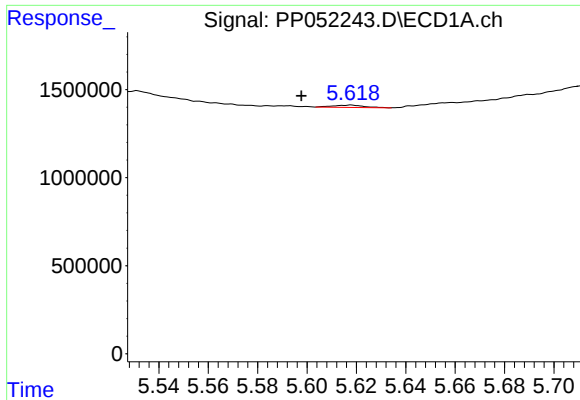

#3 AR-1016-1


R.T.: 5.618 min
Delta R.T.: 0.020 min
Response: 110216
Conc: 2.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

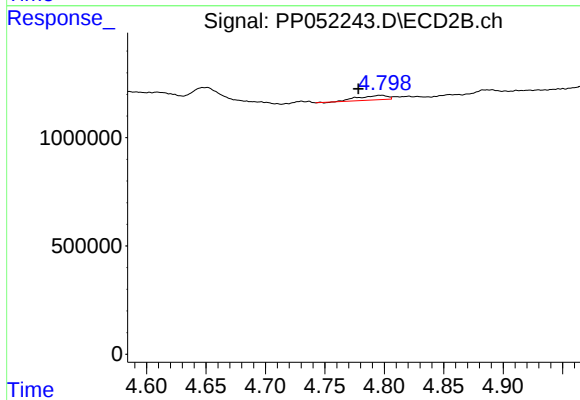


#3 AR-1016-1

R.T.: 4.797 min
Delta R.T.: 0.019 min
Response: 362334
Conc: 8.15 ng/ml

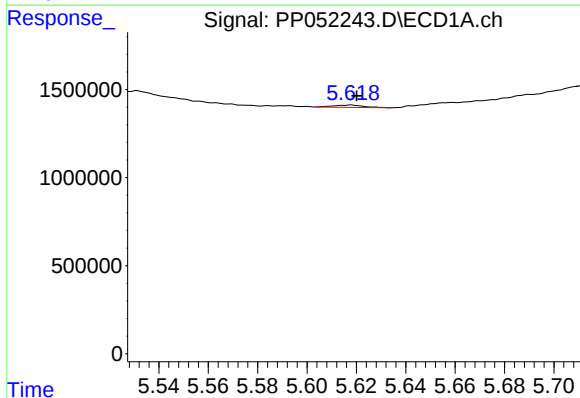


#4 AR-1016-2

R.T.: 5.618 min
Delta R.T.: -0.002 min
Response: 110216
Conc: 1.67 ng/ml

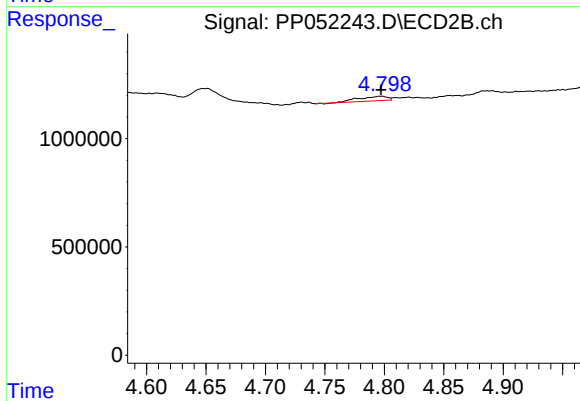

#4 AR-1016-2


R.T.: 4.797 min
Delta R.T.: 0.000 min
Response: 362334
Conc: 5.69 ng/ml

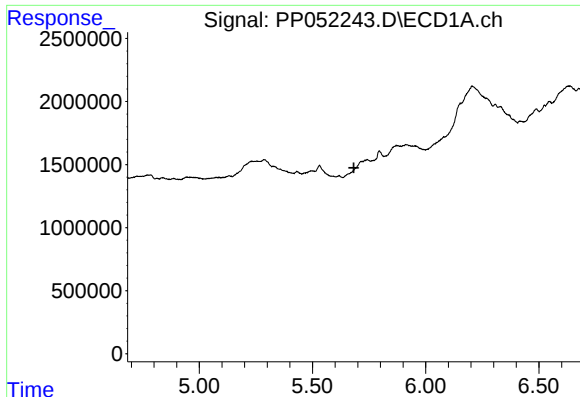

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.683 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

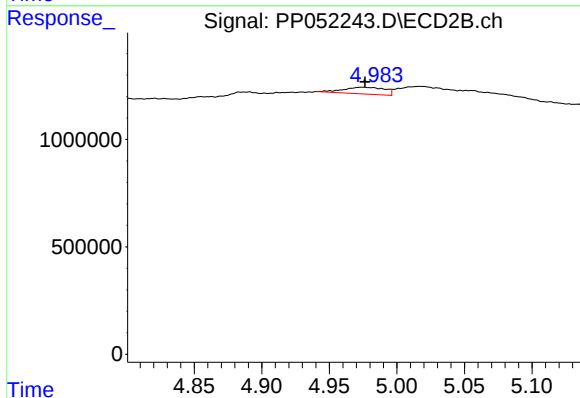


#5 AR-1016-3

R.T.: 4.974 min
Delta R.T.: -0.002 min
Response: 666860
Conc: 20.06 ng/ml

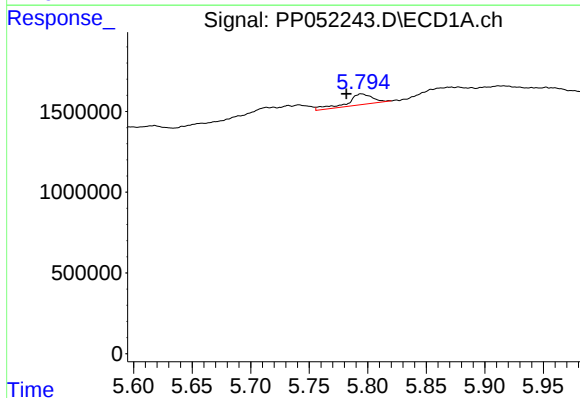


#6 AR-1016-4

R.T.: 5.795 min
Delta R.T.: 0.013 min
Response: 1046230
Conc: 28.79 ng/ml

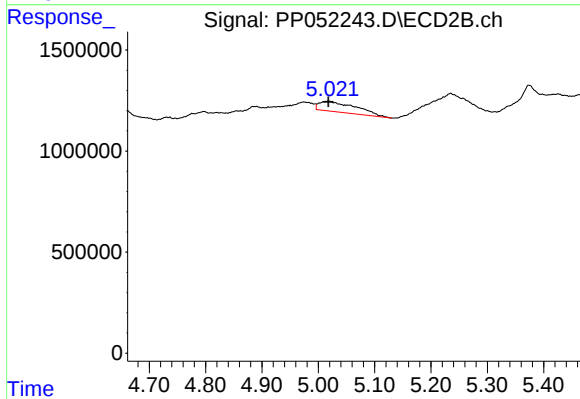

#6 AR-1016-4


R.T.: 5.018 min
Delta R.T.: 0.000 min
Response: 2350292
Conc: 86.23 ng/ml

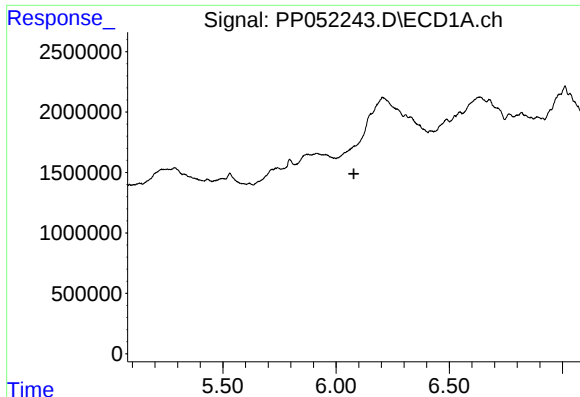

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

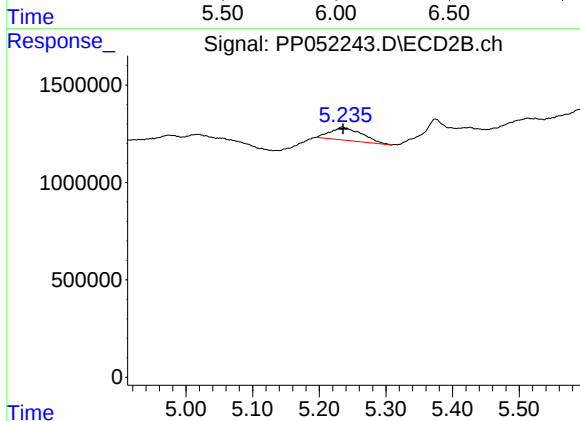


#7 AR-1016-5

R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 2171808
Conc: 61.39 ng/ml

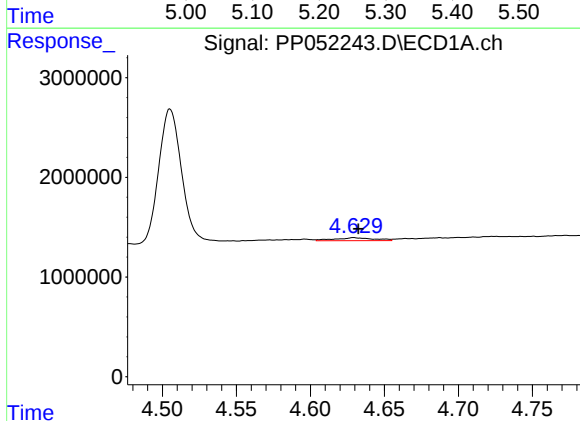


#8 AR-1221-1

R.T.: 4.629 min
Delta R.T.: -0.003 min
Response: 554203
Conc: 26.82 ng/ml

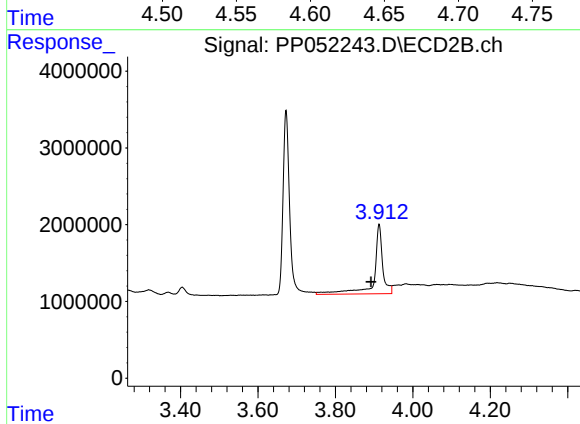

#8 AR-1221-1


R.T.: 3.913 min
Delta R.T.: 0.021 min
Response: 14162993
Conc: 905.82 ng/ml

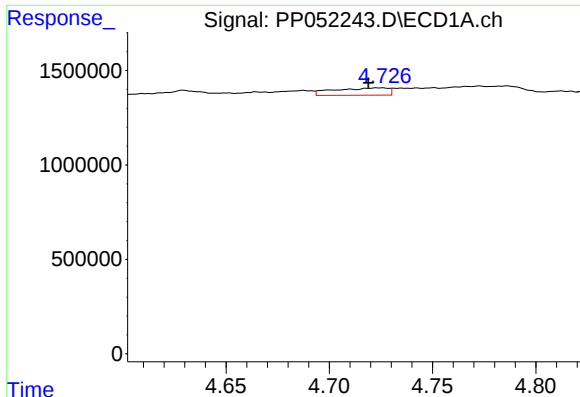

#9 AR-1221-2


R.T.: 4.725 min
Delta R.T.: 0.006 min
Response: 704581
Conc: 46.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

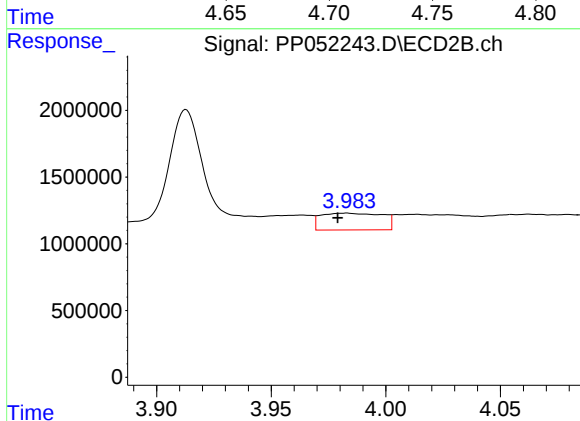


#9 AR-1221-2

R.T.: 3.983 min
Delta R.T.: 0.003 min
Response: 2345221
Conc: 195.55 ng/ml

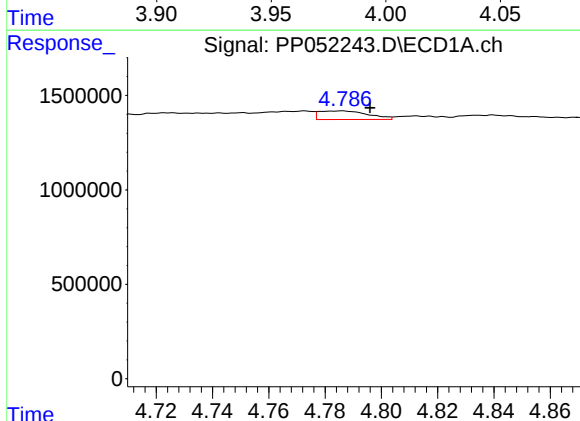


#10 AR-1221-3

R.T.: 4.786 min
Delta R.T.: -0.010 min
Response: 548610
Conc: 11.72 ng/ml

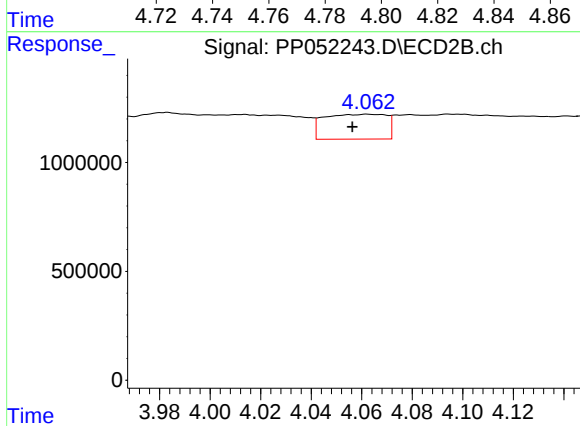

#10 AR-1221-3


R.T.: 4.062 min
Delta R.T.: 0.006 min
Response: 1961718
Conc: 51.90 ng/ml

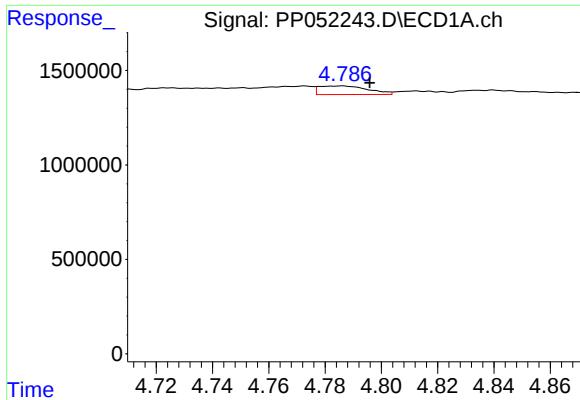

#11 AR-1232-1


R.T.: 4.786 min
Delta R.T.: -0.010 min
Response: 548610
Conc: 15.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

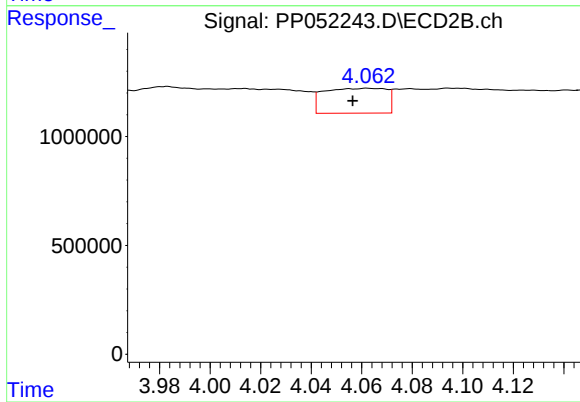


#11 AR-1232-1

R.T.: 4.062 min
Delta R.T.: 0.006 min
Response: 1961718
Conc: 67.69 ng/ml

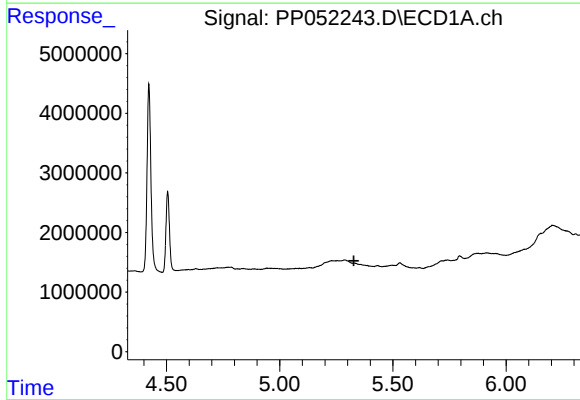


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

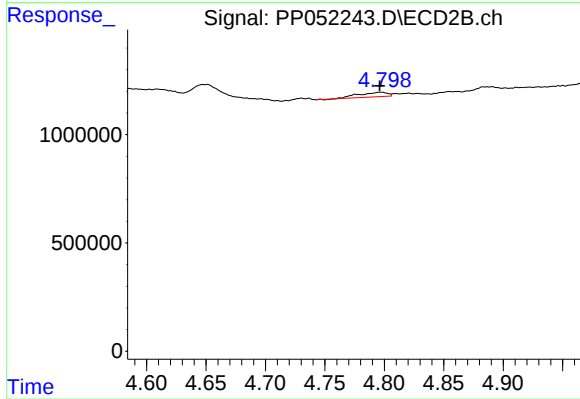

#12 AR-1232-2


R.T.: 4.797 min
Delta R.T.: 0.000 min
Response: 362334
Conc: 12.10 ng/ml

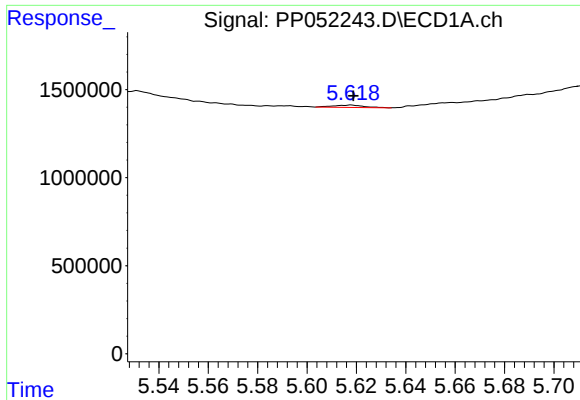

#13 AR-1232-3


R.T.: 5.618 min
Delta R.T.: -0.001 min
Response: 110216
Conc: 3.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

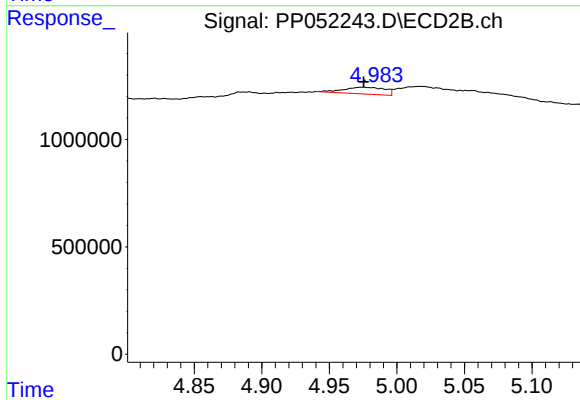


#13 AR-1232-3

R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 666860
Conc: 43.65 ng/ml

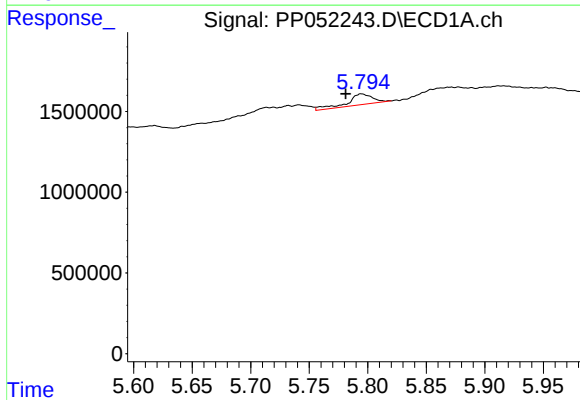


#14 AR-1232-4

R.T.: 5.795 min
Delta R.T.: 0.014 min
Response: 1046230
Conc: 62.73 ng/ml

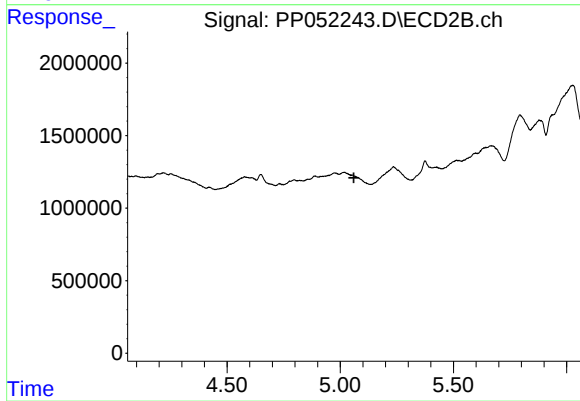

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 5.060 min
Response: 0
Conc: N.D.

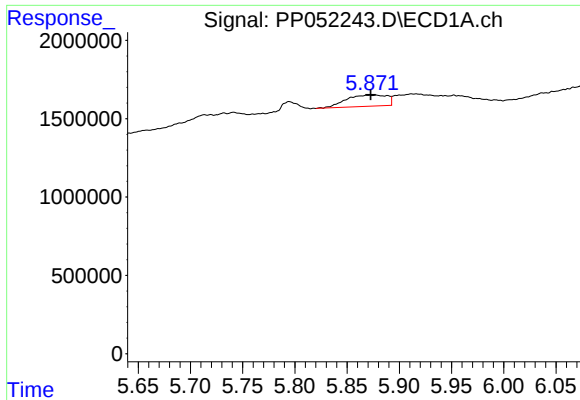

#15 AR-1232-5


R.T.: 5.878 min
Delta R.T.: 0.005 min
Response: 1968143
Conc: 131.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

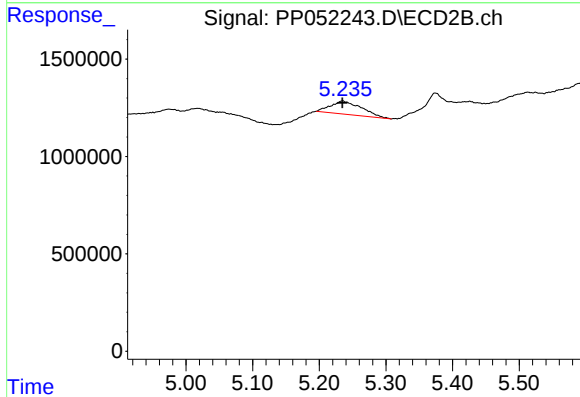


#15 AR-1232-5

R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 2171808
Conc: 137.19 ng/ml

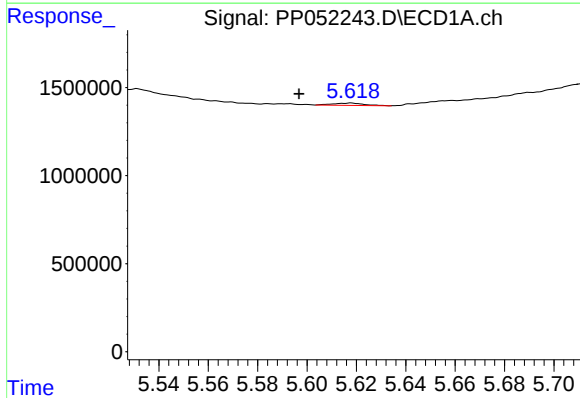


#16 AR-1242-1

R.T.: 5.618 min
Delta R.T.: 0.021 min
Response: 110216
Conc: 3.17 ng/ml

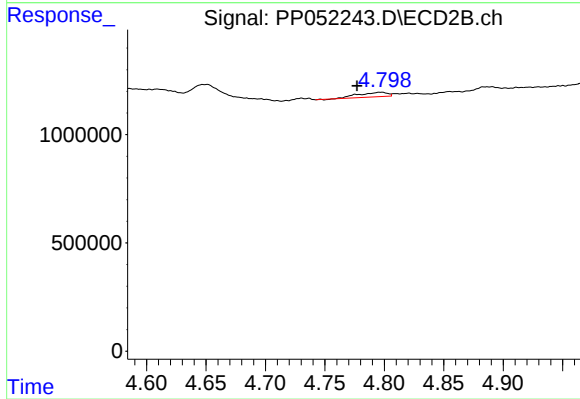

#16 AR-1242-1

R.T.: 4.797 min
Delta R.T.: 0.020 min
Response: 362334
Conc: 10.41 ng/ml

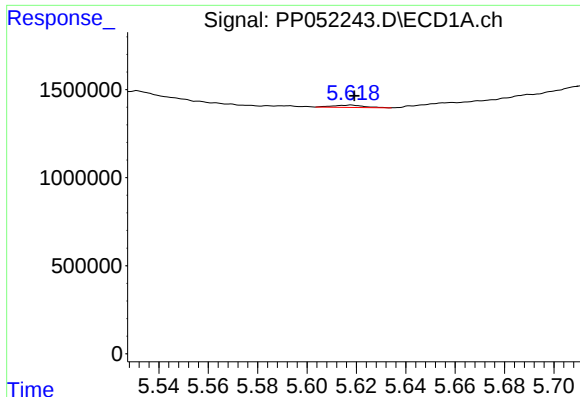

#17 AR-1242-2


R.T.: 5.618 min
Delta R.T.: -0.001 min
Response: 110216
Conc: 2.23 ng/ml

Instrument :

ECD_P


ClientSampleId :

RB10622-01-BASEMENT-BATHROOM-SINK

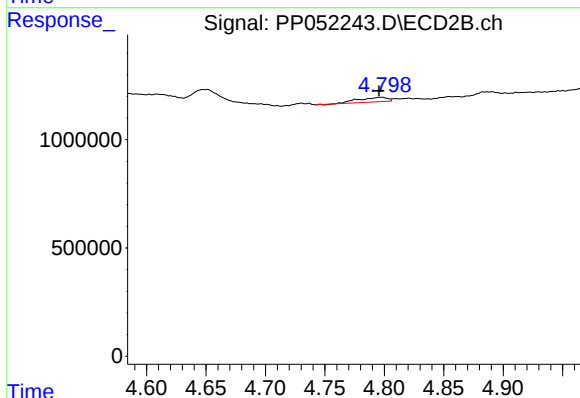


#17 AR-1242-2

R.T.: 4.797 min
Delta R.T.: 0.001 min
Response: 362334
Conc: 7.34 ng/ml

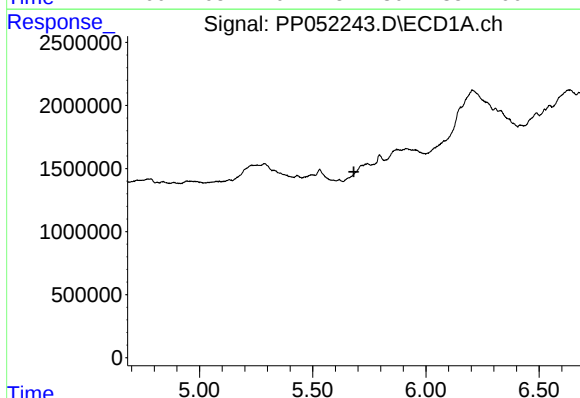


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T. : 5.682 min
Response: 0
Conc: N.D.

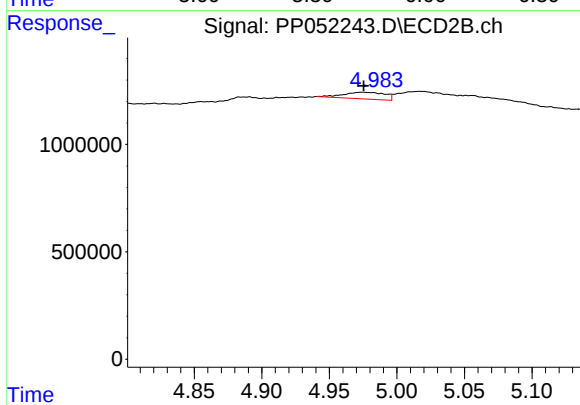

#18 AR-1242-3


R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 666860
Conc: 25.55 ng/ml

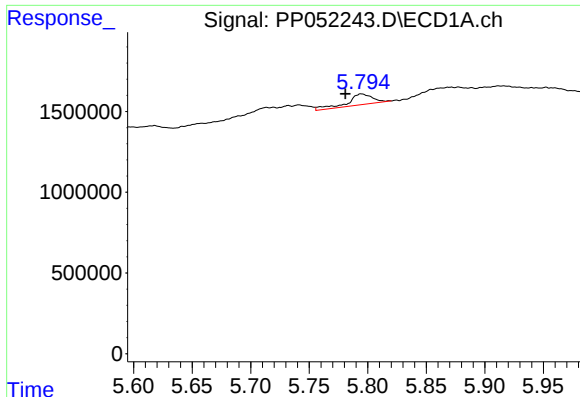

#19 AR-1242-4


R.T.: 5.795 min
Delta R.T.: 0.014 min
Response: 1046230
Conc: 38.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

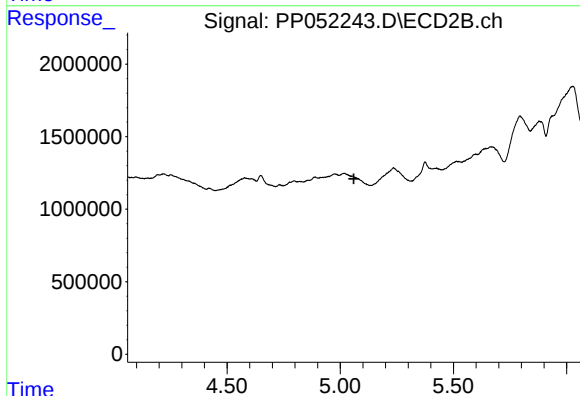


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.060 min
Response: 0
Conc: N.D.

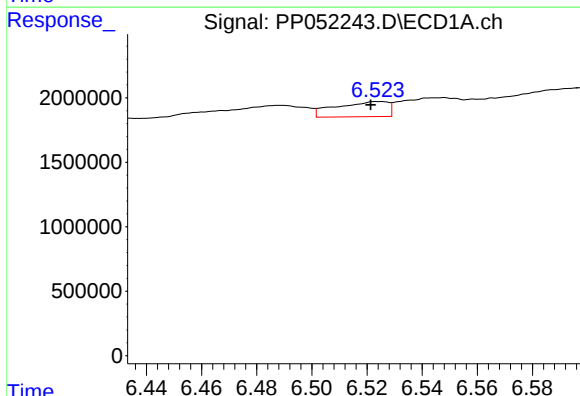


#20 AR-1242-5

R.T.: 6.524 min
Delta R.T.: 0.003 min
Response: 1537252
Conc: 41.35 ng/ml

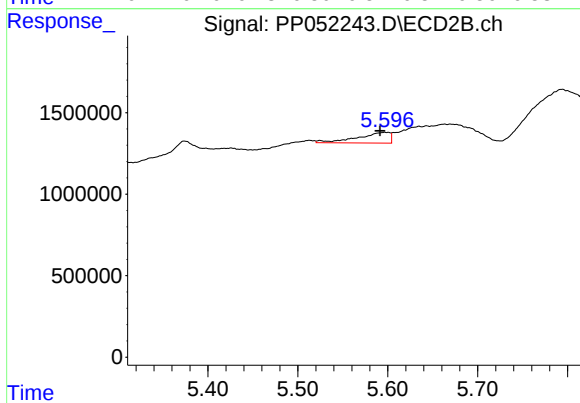

#20 AR-1242-5


R.T.: 5.597 min
Delta R.T.: 0.006 min
Response: 1626068
Conc: 48.25 ng/ml

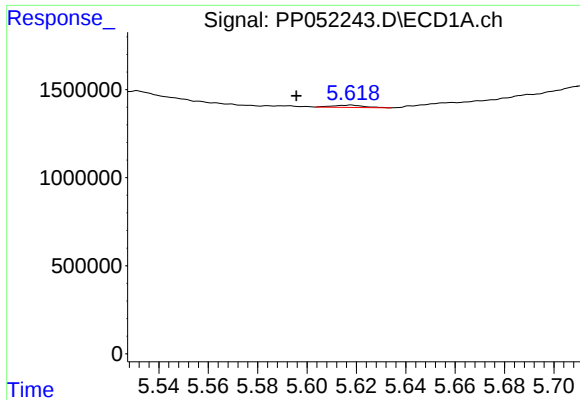

#21 AR-1248-1


R.T.: 5.618 min
Delta R.T.: 0.022 min
Response: 110216
Conc: 4.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

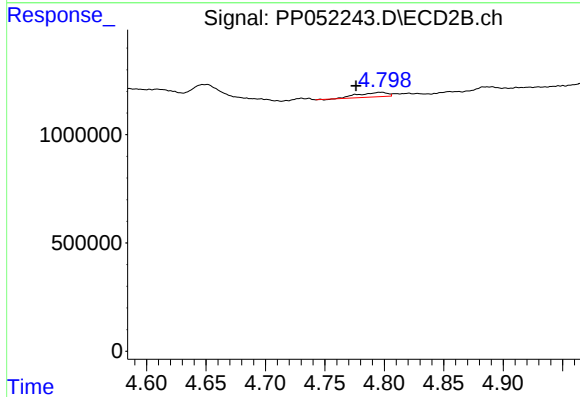


#21 AR-1248-1

R.T.: 4.797 min
Delta R.T.: 0.021 min
Response: 362334
Conc: 13.36 ng/ml

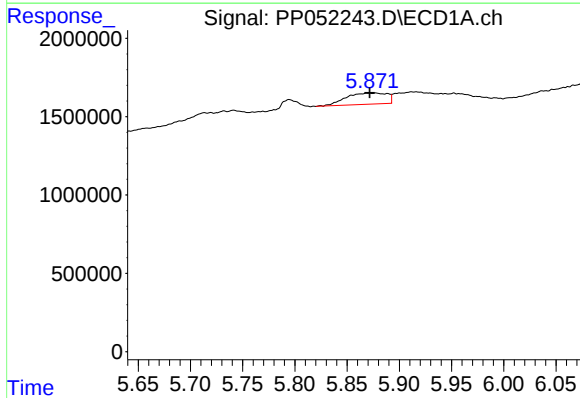


#22 AR-1248-2

R.T.: 5.878 min
Delta R.T.: 0.006 min
Response: 1968143
Conc: 42.34 ng/ml

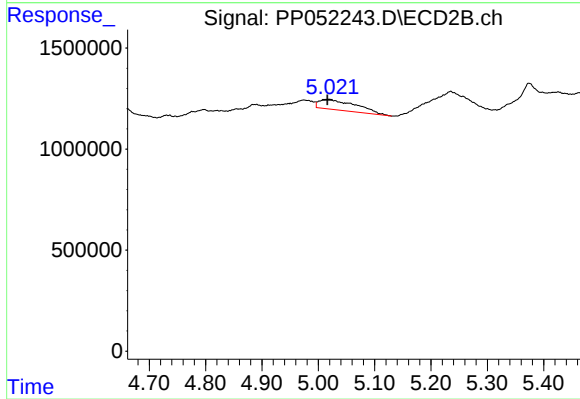

#22 AR-1248-2


R.T.: 5.018 min
Delta R.T.: 0.001 min
Response: 2350292
Conc: 63.17 ng/ml

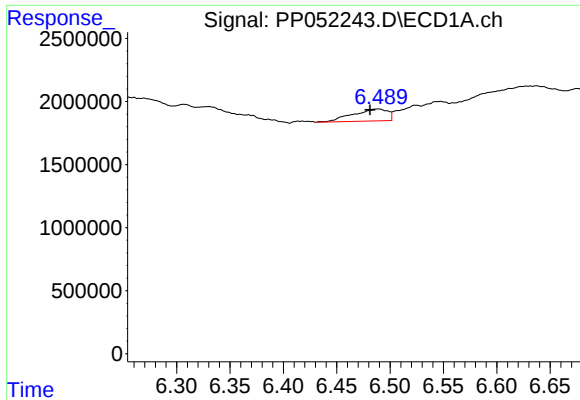

#24 AR-1248-4


R.T.: 6.489 min
Delta R.T.: 0.007 min
Response: 2168117
Conc: 34.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

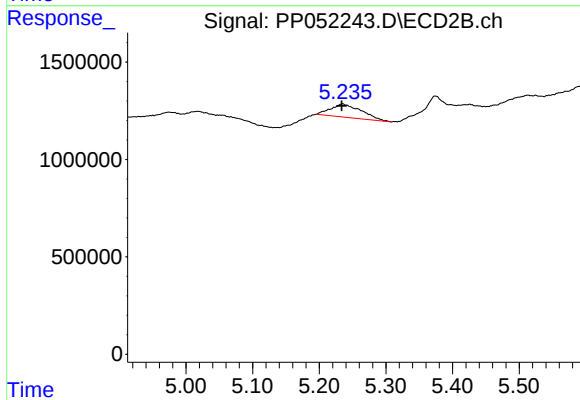


#24 AR-1248-4

R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 2171808
Conc: 46.87 ng/ml

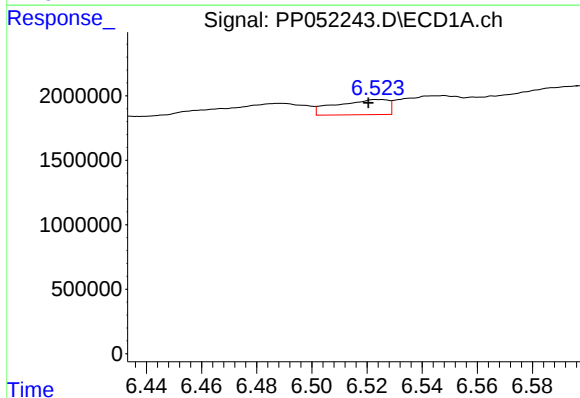


#25 AR-1248-5

R.T.: 6.524 min
Delta R.T.: 0.004 min
Response: 1537252
Conc: 24.82 ng/ml

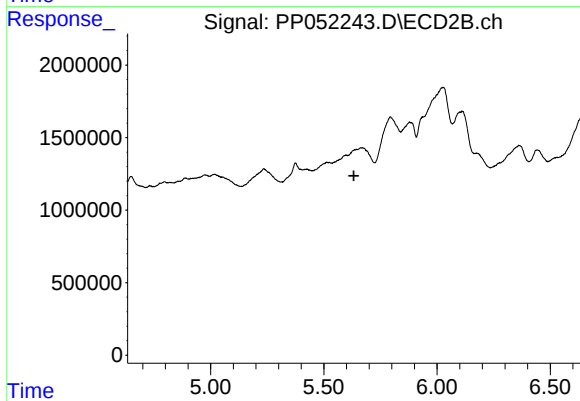

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 5.632 min
Response: 0
Conc: N.D.

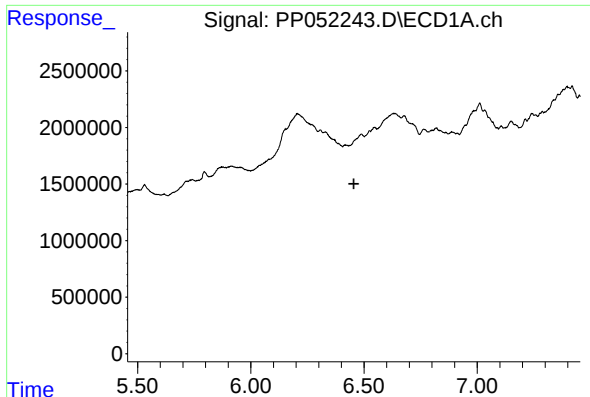

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

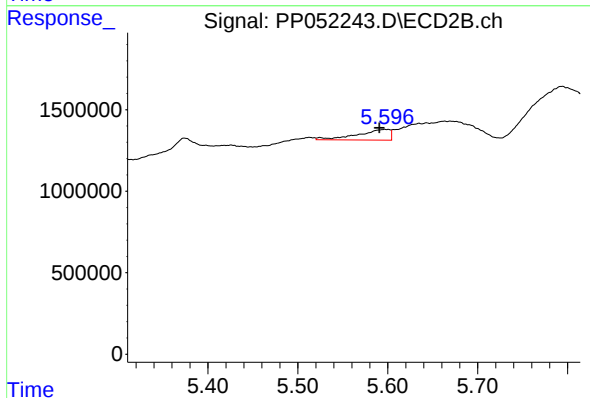


#26 AR-1254-1

R.T.: 5.597 min
Delta R.T.: 0.006 min
Response: 1626068
Conc: 23.24 ng/ml

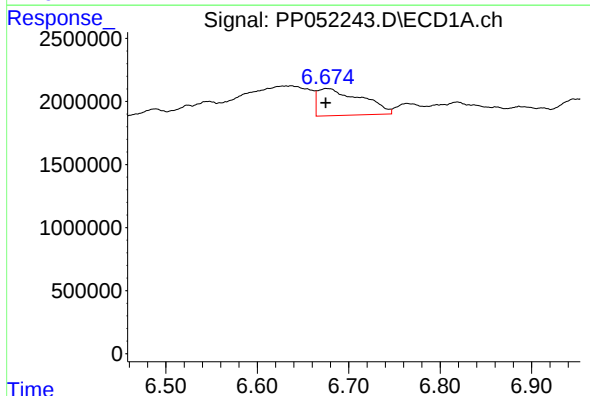


#27 AR-1254-2

R.T.: 6.676 min
Delta R.T.: 0.000 min
Response: 7102940
Conc: 66.60 ng/ml

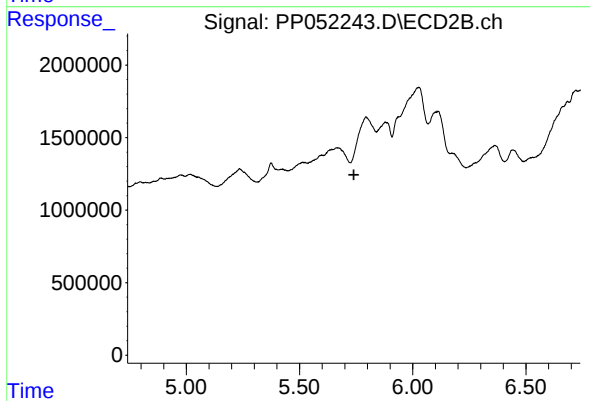

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 5.740 min
Response: 0
Conc: N.D.

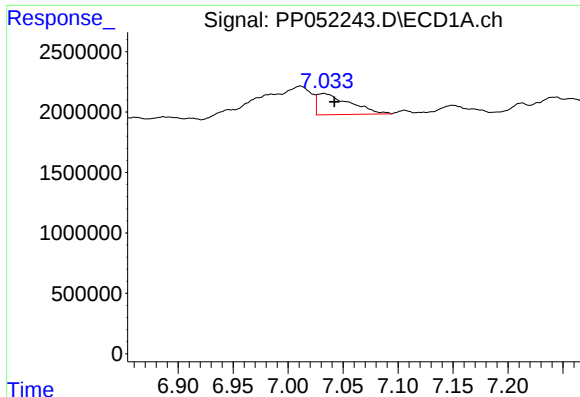

#28 AR-1254-3


R.T.: 7.032 min
Delta R.T.: -0.010 min
Response: 3600673
Conc: 34.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

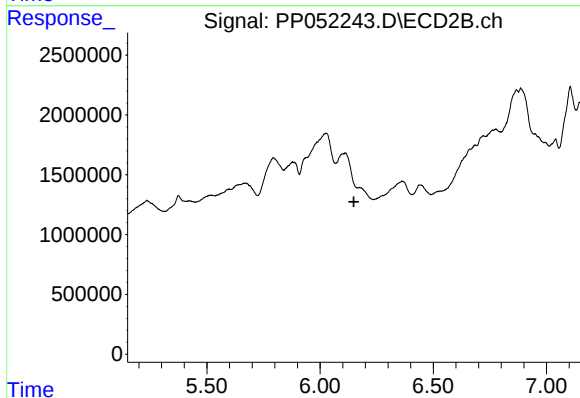


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.150 min
Response: 0
Conc: N.D.

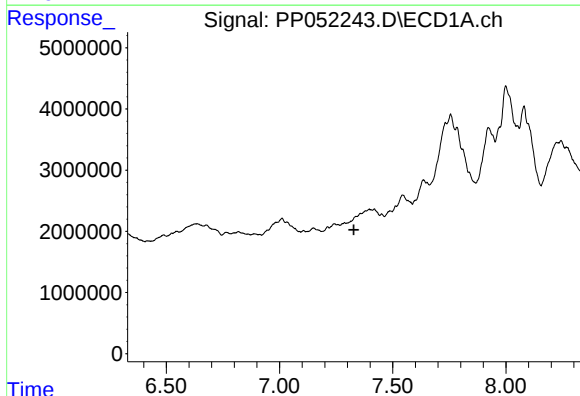


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.328 min
Response: 0
Conc: N.D.

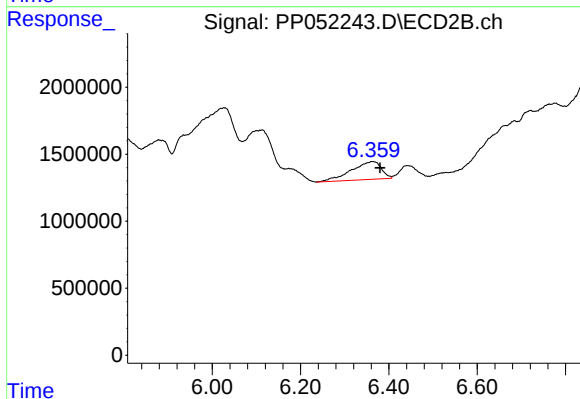

#29 AR-1254-4


R.T.: 6.361 min
Delta R.T.: -0.019 min
Response: 6356276
Conc: 106.33 ng/ml

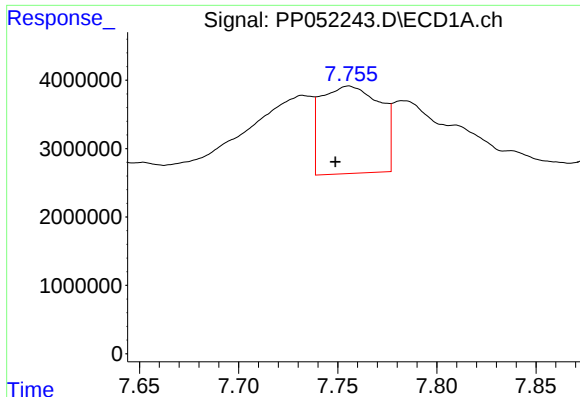

#30 AR-1254-5


R.T.: 7.755 min
Delta R.T.: 0.007 min
Response: 26533649
Conc: 319.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

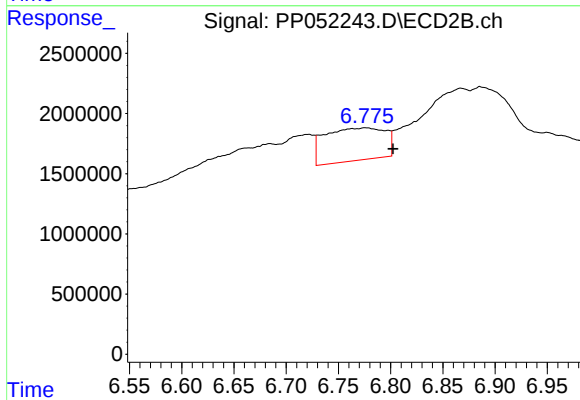


#30 AR-1254-5

R.T.: 6.776 min
Delta R.T.: -0.027 min
Response: 10884778
Conc: 122.78 ng/ml

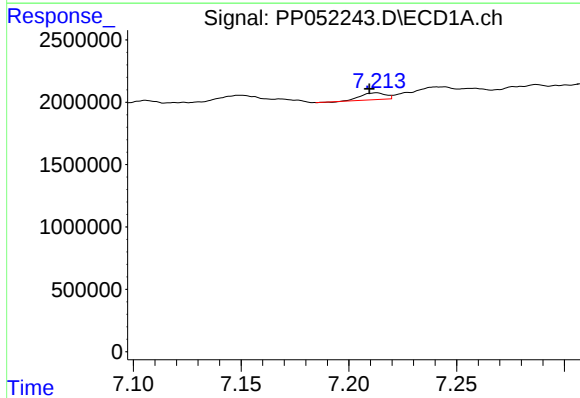


#31 AR-1260-1

R.T.: 7.213 min
Delta R.T.: 0.003 min
Response: 418239
Conc: 5.05 ng/ml

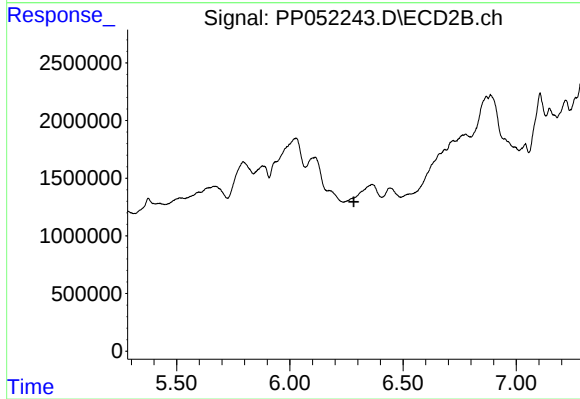

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 6.283 min
Response: 0
Conc: N.D.

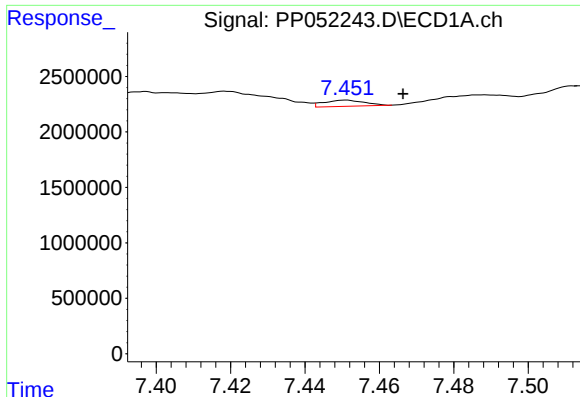

#32 AR-1260-2


R.T.: 7.451 min
Delta R.T.: -0.015 min
Response: 423823
Conc: 4.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

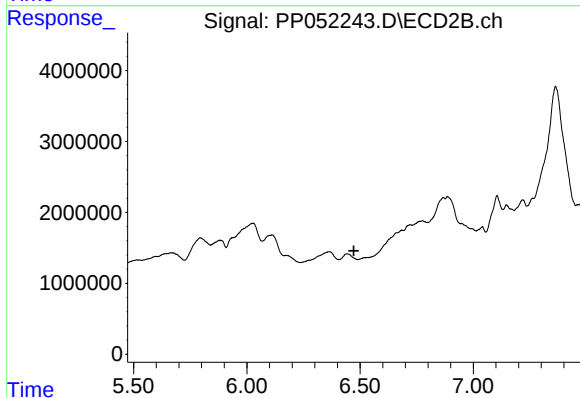


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.472 min
Response: 0
Conc: N.D.

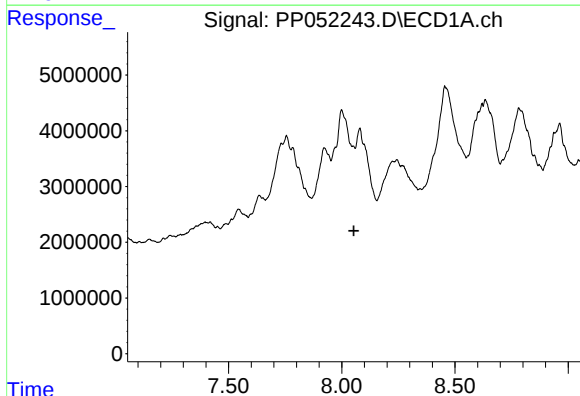


#34 AR-1260-4

R.T.: 8.051 min
Delta R.T.: -0.003 min
Response: -495002
Conc: N.D.

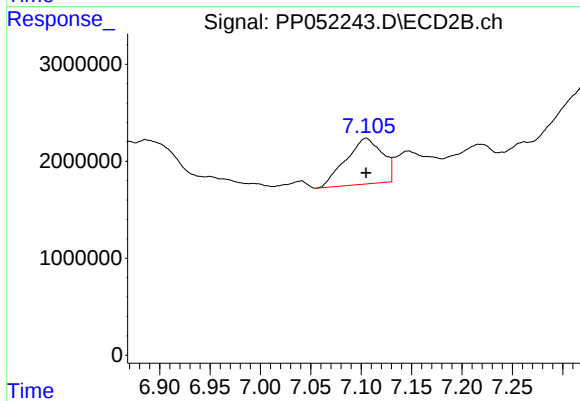

#34 AR-1260-4


R.T.: 7.105 min
Delta R.T.: 0.000 min
Response: 11872706
Conc: 211.20 ng/ml

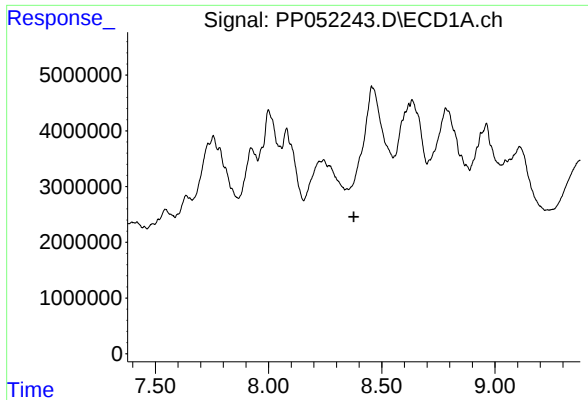

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.377 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

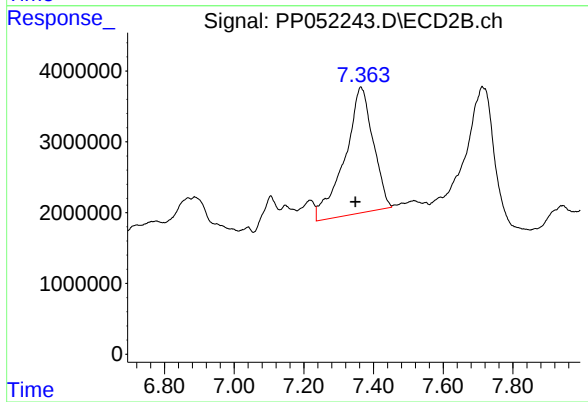


#35 AR-1260-5

R.T.: 7.363 min
Delta R.T.: 0.016 min
Response: 99929838
Conc: 757.75 ng/ml

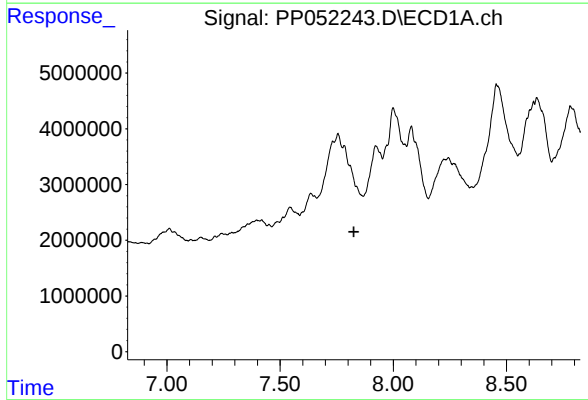


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.826 min
Response: 0
Conc: N.D.

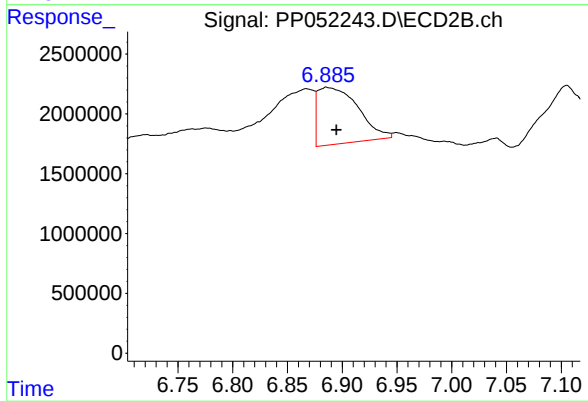

#36 AR-1262-1


R.T.: 6.886 min
Delta R.T.: -0.009 min
Response: 12165852
Conc: 338.21 ng/ml

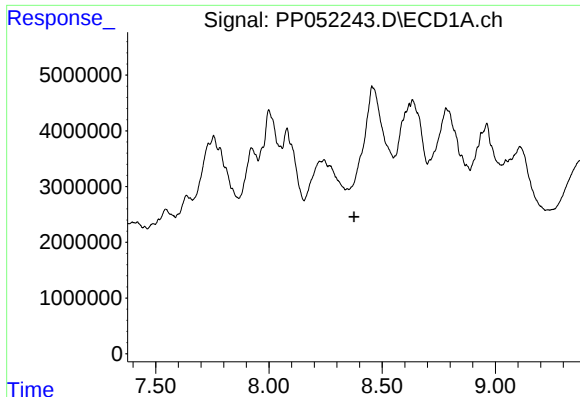

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

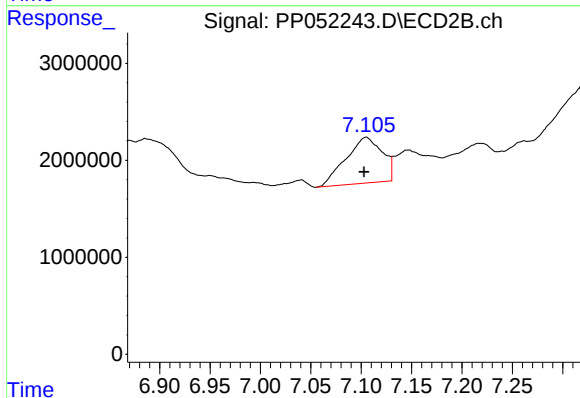


#37 AR-1262-2

R.T.: 7.105 min
Delta R.T.: 0.002 min
Response: 11872706
Conc: 149.94 ng/ml

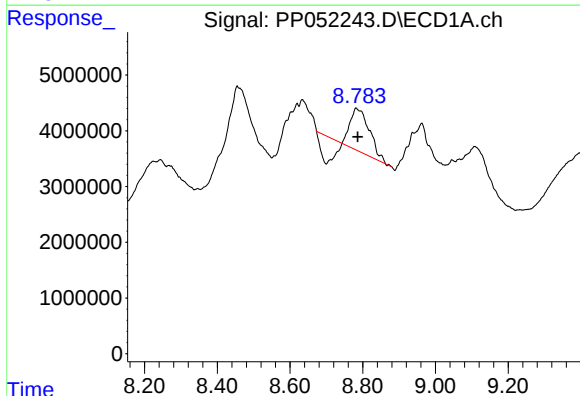


#39 AR-1262-4

R.T.: 8.782 min
Delta R.T.: -0.004 min
Response: 17197937
Conc: 336.43 ng/ml

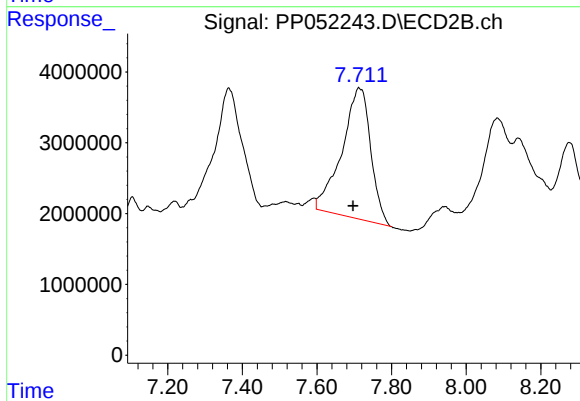

#39 AR-1262-4


R.T.: 7.712 min
Delta R.T.: 0.015 min
Response: 99021652
Conc: 867.37 ng/ml

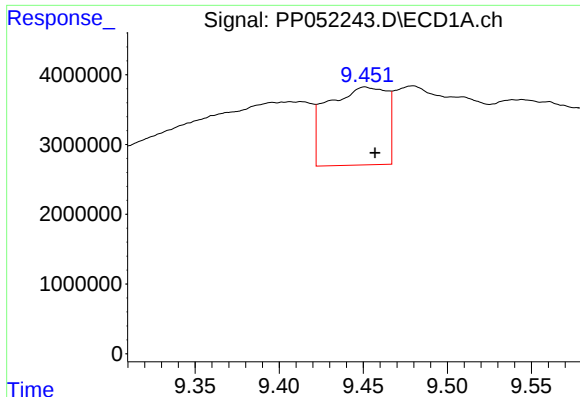

#40 AR-1262-5


R.T.: 9.452 min
Delta R.T.: -0.005 min
Response: 27309670
Conc: 433.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

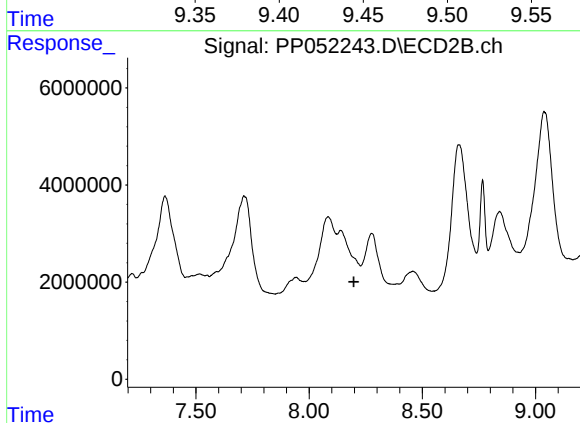


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 8.197 min
Response: 0
Conc: N.D.

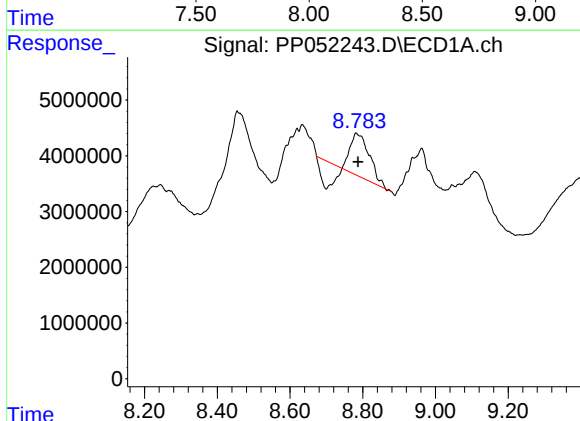


#42 AR-1268-2

R.T.: 8.782 min
Delta R.T.: -0.005 min
Response: 17197937
Conc: 93.66 ng/ml

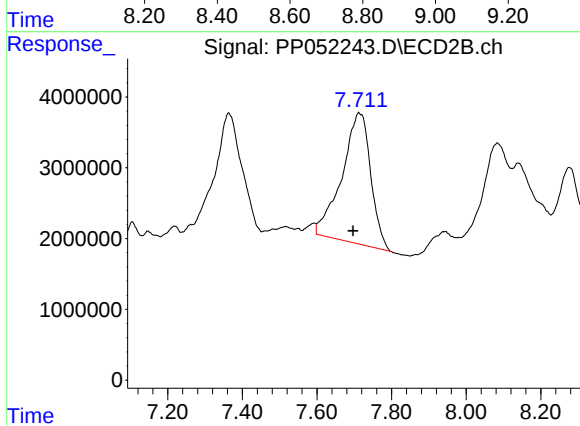

#42 AR-1268-2


R.T.: 7.712 min
Delta R.T.: 0.015 min
Response: 99021652
Conc: 606.06 ng/ml

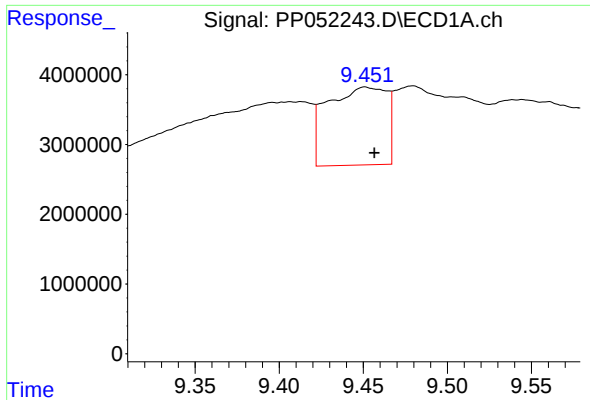

#44 AR-1268-4

R.T.: 9.452 min
Delta R.T.: -0.005 min
Response: 27309670
Conc: 374.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK

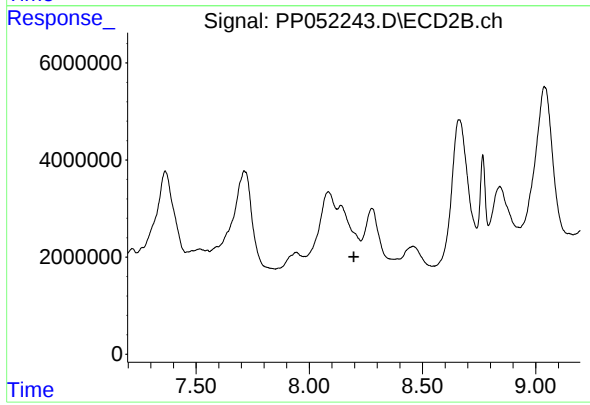

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.197 min
Response: 0
Conc: N.D.