

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
 Data File : PP052243.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 20:08
 Operator : YP\AJ
 Sample : N5059-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RB10622-01-BASEMENT-BATHROOM-SINK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/13/2022
 Supervised By :Ankita Jodhani 10/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 05:42:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 12 05:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.422	3.673	37695331	28563080	23.981	24.932
2) SA Decachlor...	10.239	8.766	30978740	19658351	22.321	17.594m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
Data File : PP052243.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 20:08
Operator : YP\AJ
Sample : N5059-01
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
RB10622-01-BASEMENT-BATHROOM-SINK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/13/2022
Supervised By :Ankita Jodhani 10/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 05:42:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

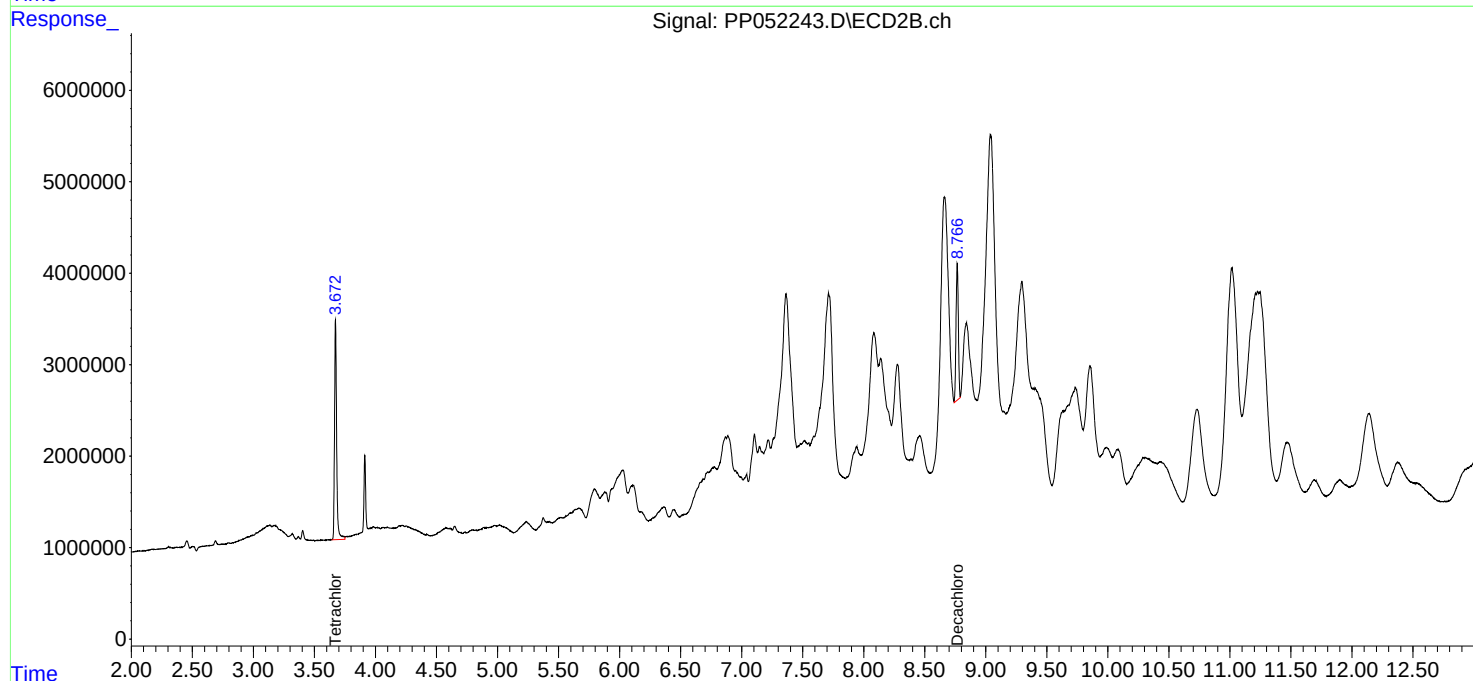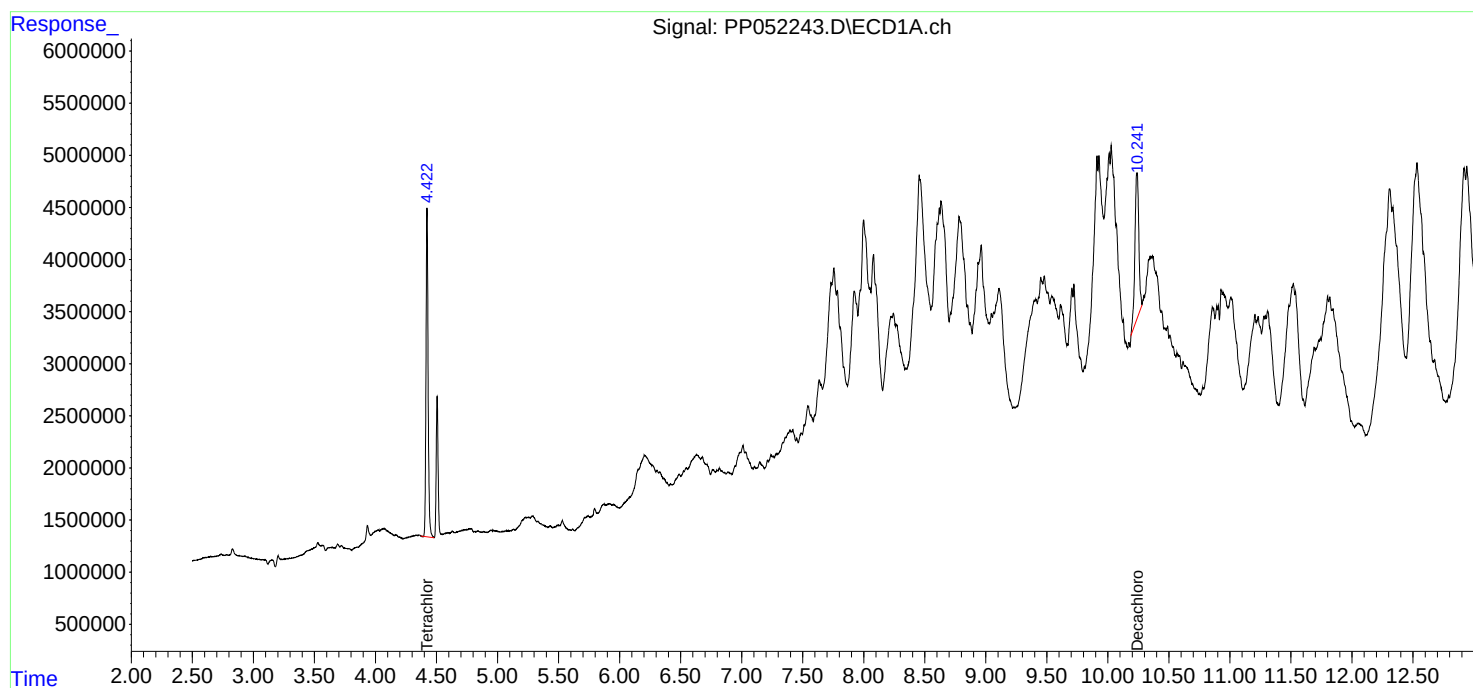

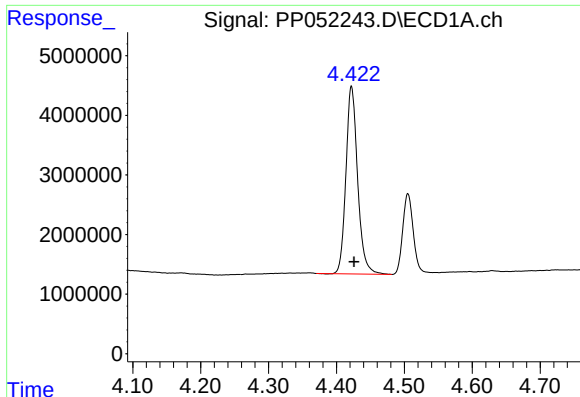

#1 Tetrachloro-m-xylene

R.T.: 4.422 min
Delta R.T.: -0.004 min
Response: 37695331
Conc: 23.98 ng/ml

Instrument :

ECD_P


ClientSampleId :

RB10622-01-BASEMENT-BATHROOM-SINK

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 10/13/2022
Supervised By :Ankita Jodhani 10/13/2022

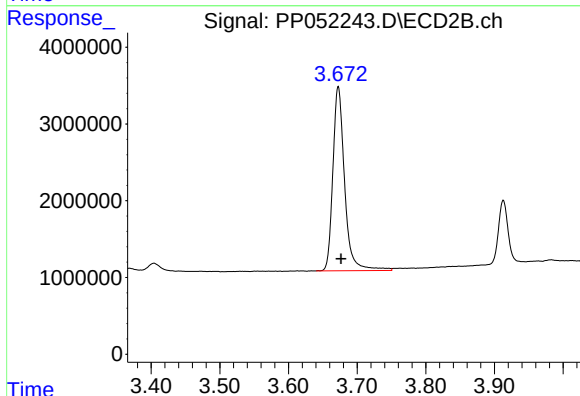


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: -0.004 min
Response: 28563080
Conc: 24.93 ng/ml

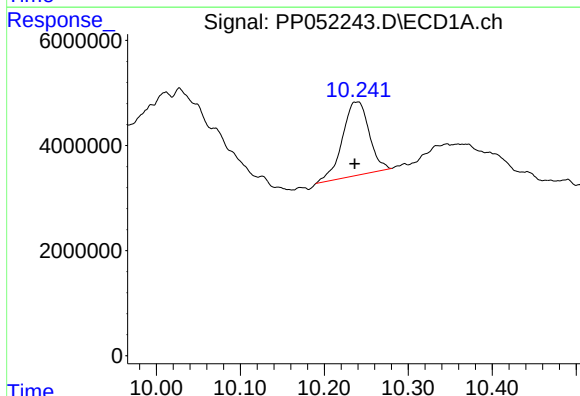

#2 Decachlorobiphenyl

R.T.: 10.239 min
Delta R.T.: 0.002 min
Response: 30978740
Conc: 22.32 ng/ml

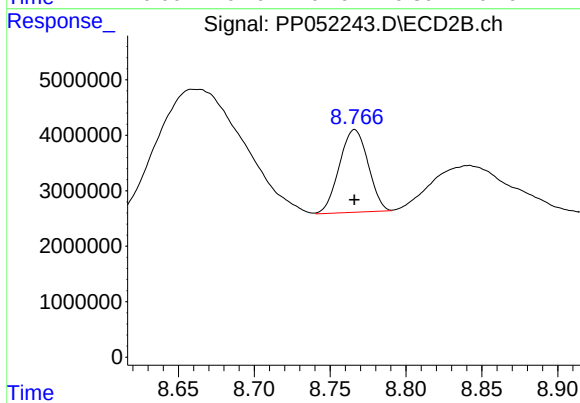

#2 Decachlorobiphenyl

R.T.: 8.766 min
Delta R.T.: 0.000 min
Response: 19658351
Conc: 17.59 ng/ml m