

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
 Data File : PP052254.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2022 00:49
 Operator : YP\AJ
 Sample : N5080-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TR-6-101022

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/13/2022
 Supervised By :Ankita Jodhani 10/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 05:47:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 12 05:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.423	3.673	34575249	25015260	21.996	21.835m
2) SA Decachlor...	10.237	8.764	35926100	20110169	25.886	17.998m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
Data File : PP052254.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2022 00:49
Operator : YP\AJ
Sample : N5080-01
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TR-6-101022


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/13/2022
Supervised By :Ankita Jodhani 10/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 05:47:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

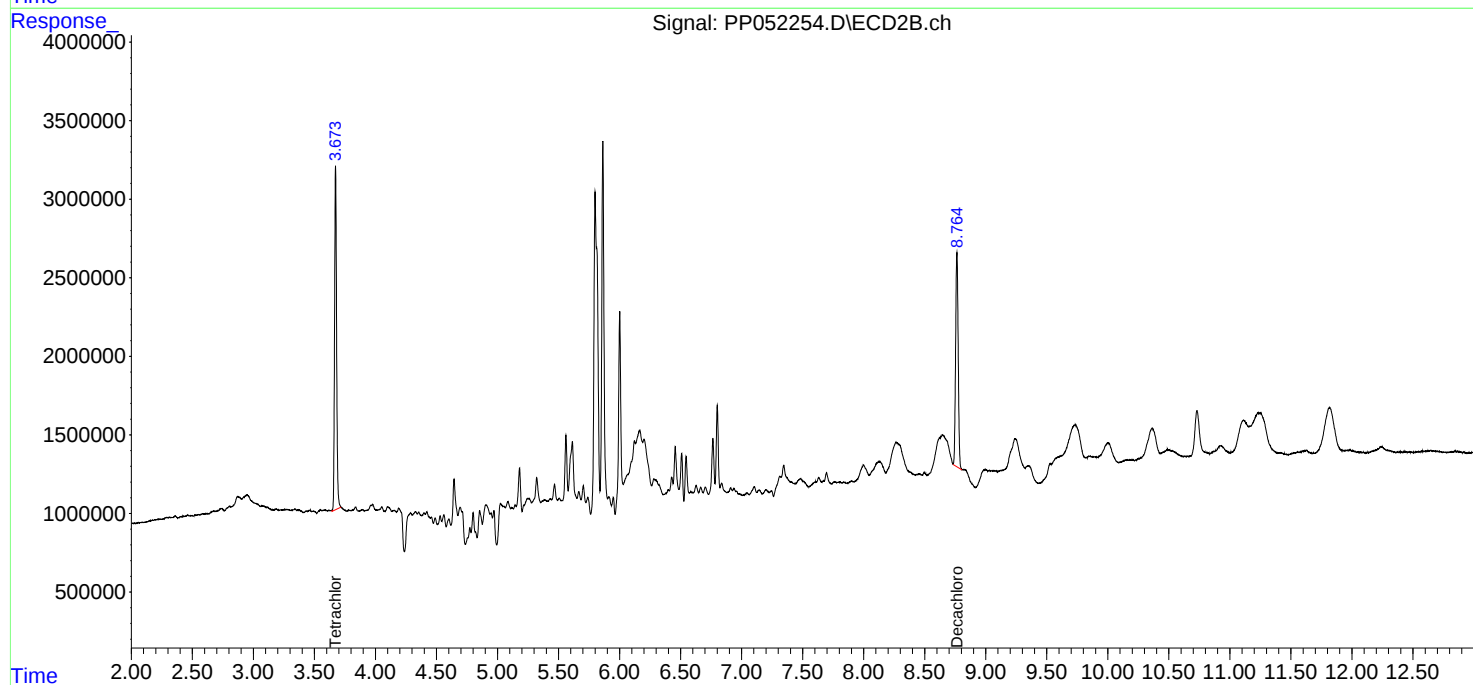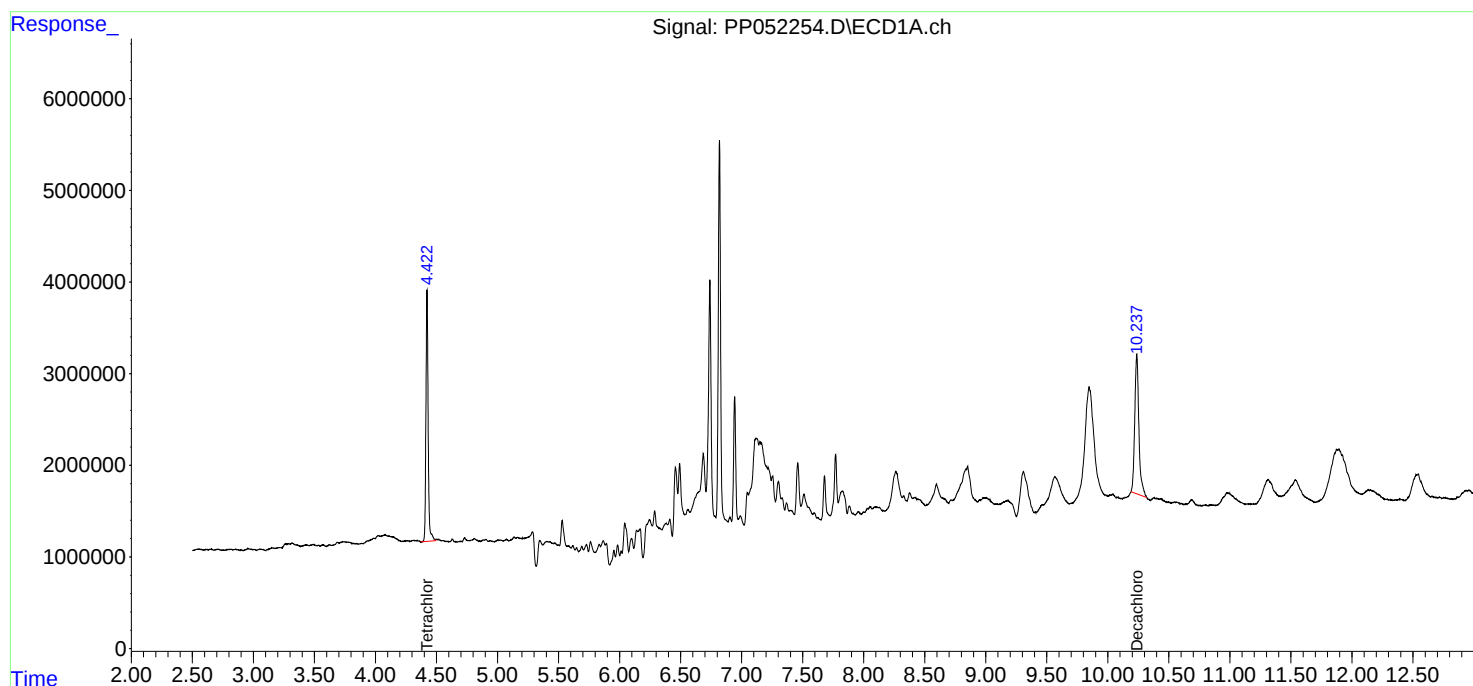

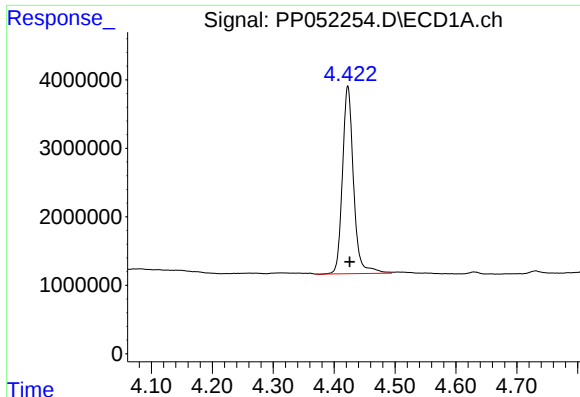


#1 Tetrachloro-m-xylene

R.T.: 4.423 min
Delta R.T.: -0.003 min
Response: 34575249
Conc: 22.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
TR-6-101022


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/13/2022
Supervised By :Ankita Jodhani 10/13/2022

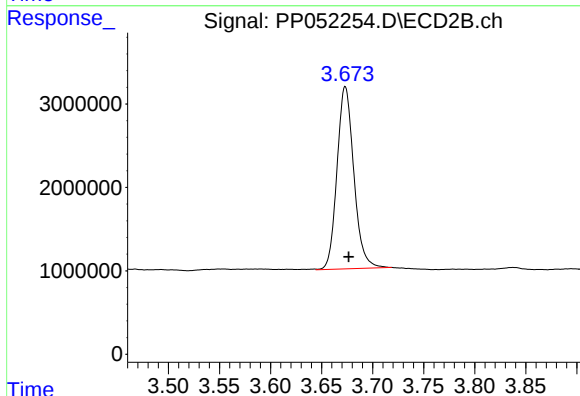


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: -0.004 min
Response: 25015260
Conc: 21.84 ng/ml m

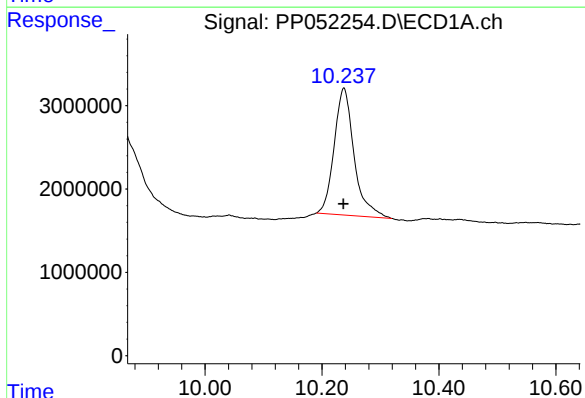

#2 Decachlorobiphenyl

R.T.: 10.237 min
Delta R.T.: 0.001 min
Response: 35926100
Conc: 25.89 ng/ml

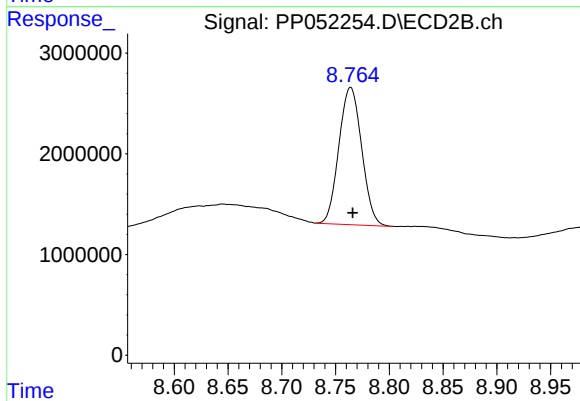

#2 Decachlorobiphenyl

R.T.: 8.764 min
Delta R.T.: -0.002 min
Response: 20110169
Conc: 18.00 ng/ml m