

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101321\
 Data File : PP040014.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Oct 2021 11:10
 Operator : AJ\MA
 Sample : PB139837BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 02:24:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.893	3.981	641764	374892	21.133	22.175
2)	SA Decachlor...	10.913	9.310	542614	517720	21.953	24.394
Target Compounds							
10)	L2 AR-1221-3	0.000	4.420	0	11002	N.D.	20.315 #
11)	L3 AR-1232-1	0.000	4.420	0	11002	N.D.	27.087 #
32)	L7 AR-1260-2	8.171	0.000	17735	0	12.976	N.D. #
33)	L7 AR-1260-3	0.000	7.199	0	11189	N.D.	9.470 #
38)	L8 AR-1262-3	0.000	8.194f	0	54941	N.D.	56.414 #
41)	L9 AR-1268-1	0.000	8.194f	0	54941	N.D.	20.361 #
43)	L9 AR-1268-3	0.000	8.520f	0	47086	N.D.	21.503 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101321\
Data File : PP040014.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Oct 2021 11:10
Operator : AJ\MA
Sample : PB139837BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 02:24:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

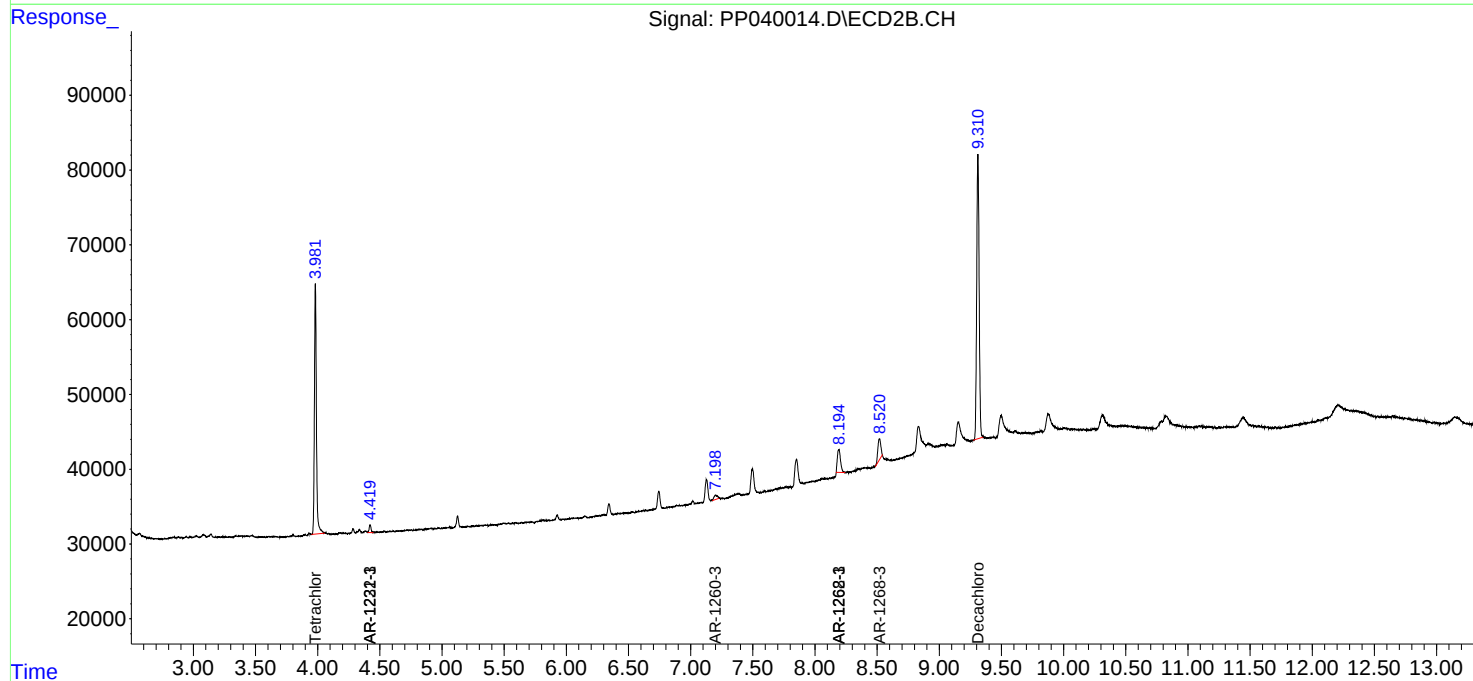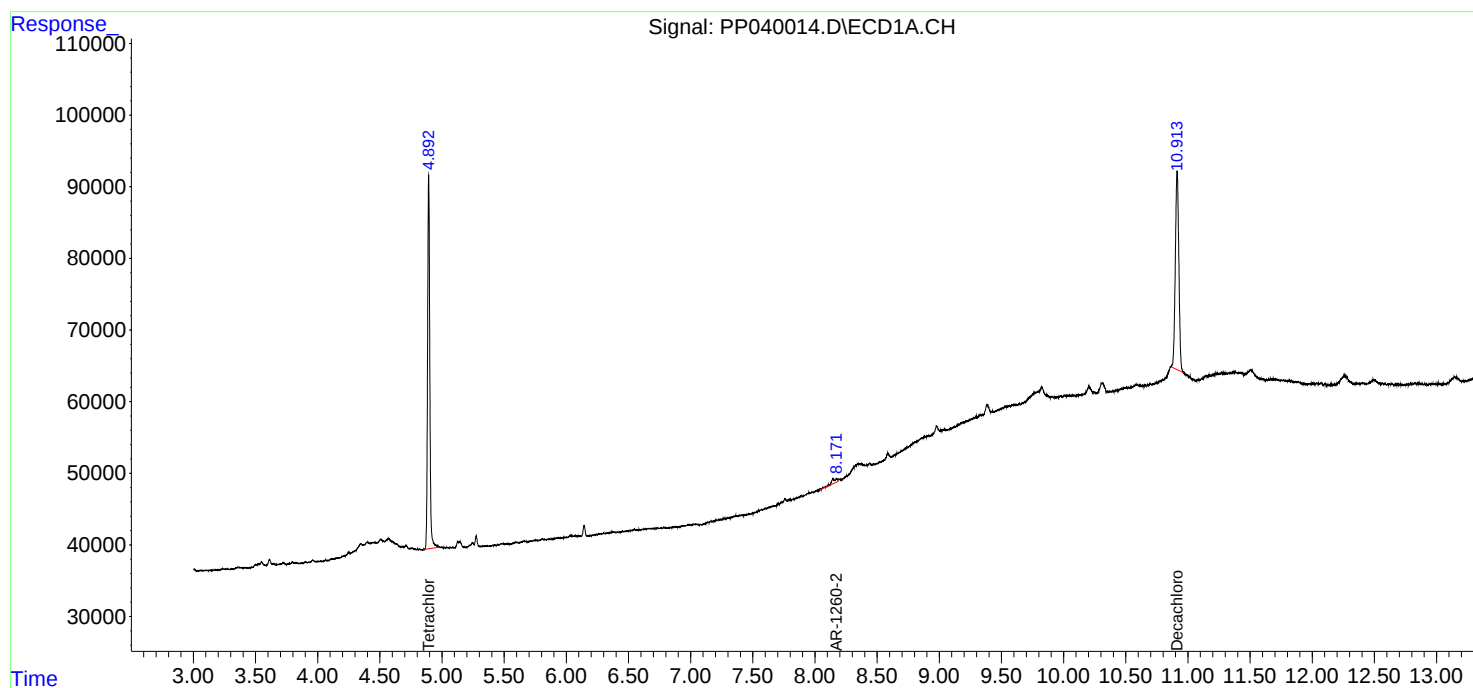


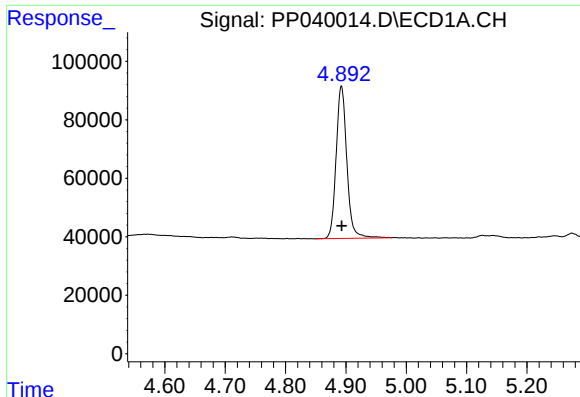

#1 Tetrachloro-m-xylene


R.T.: 4.893 min
Delta R.T.: 0.000 min
Response: 641764
Conc: 21.13 ng/ml

Instrument :
ECD_P
ClientSampleId :

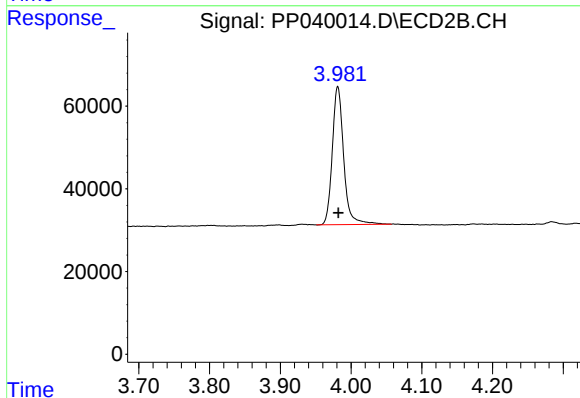


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: -0.001 min
Response: 374892
Conc: 22.18 ng/ml

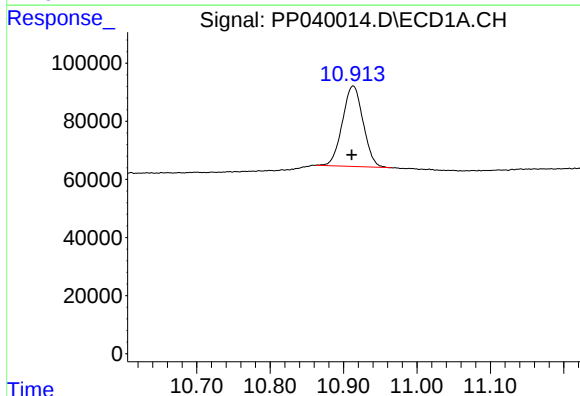


#2 Decachlorobiphenyl

R.T.: 10.913 min
Delta R.T.: 0.002 min
Response: 542614
Conc: 21.95 ng/ml

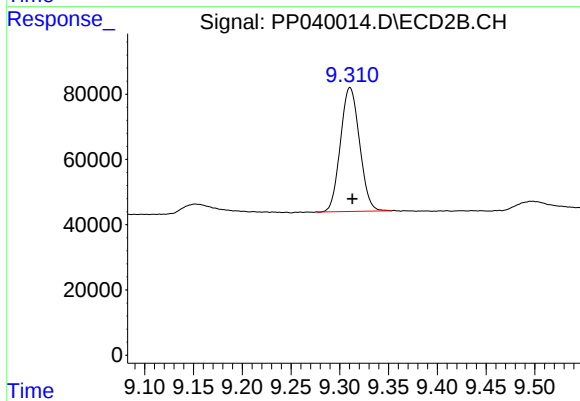

#2 Decachlorobiphenyl


R.T.: 9.310 min
Delta R.T.: -0.002 min
Response: 517720
Conc: 24.39 ng/ml

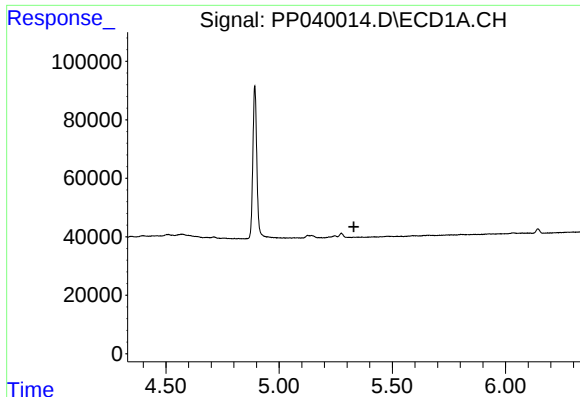

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 5.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

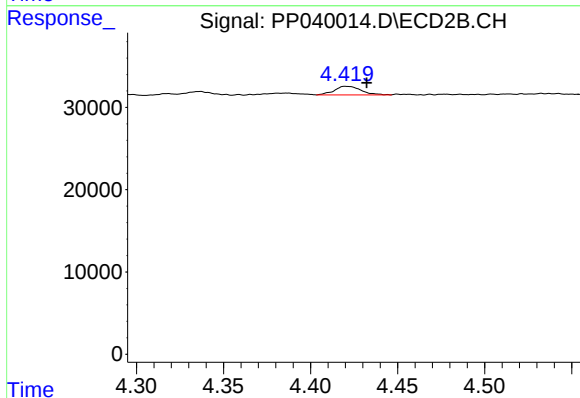


#10 AR-1221-3

R.T.: 4.420 min
Delta R.T.: -0.012 min
Response: 11002
Conc: 20.32 ng/ml

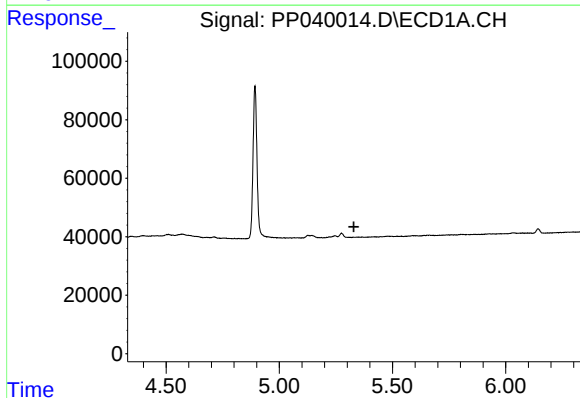


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 5.330 min
Response: 0
Conc: N.D.

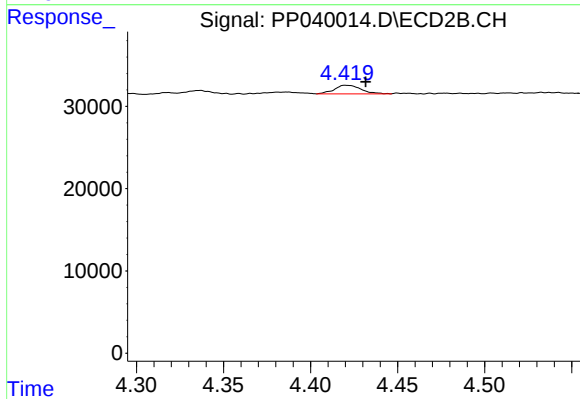

#11 AR-1232-1


R.T.: 4.420 min
Delta R.T.: -0.012 min
Response: 11002
Conc: 27.09 ng/ml

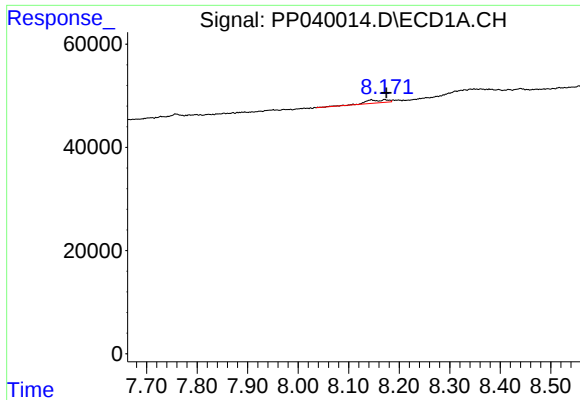

#32 AR-1260-2


R.T.: 8.171 min
Delta R.T.: -0.004 min
Response: 17735
Conc: 12.98 ng/ml

Instrument :
ECD_P
ClientSampleId :

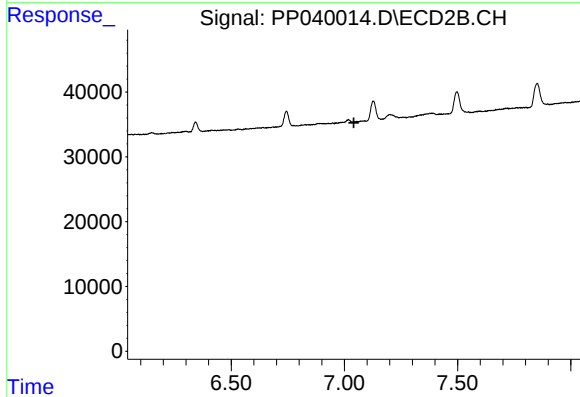


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.042 min
Response: 0
Conc: N.D.

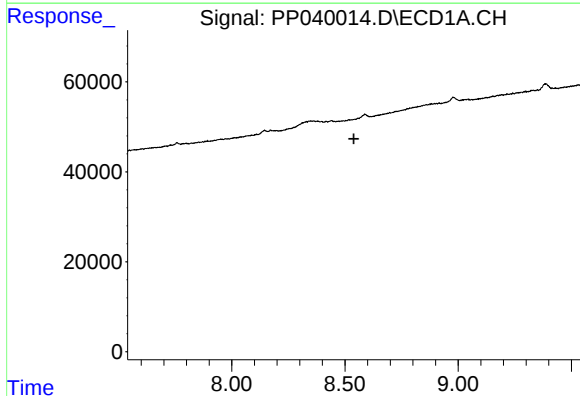


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.540 min
Response: 0
Conc: N.D.

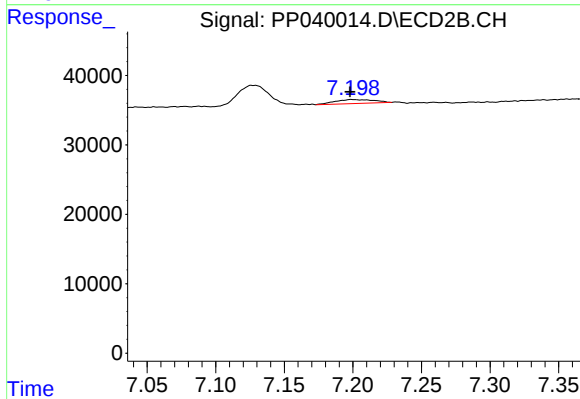

#33 AR-1260-3


R.T.: 7.199 min
Delta R.T.: 0.000 min
Response: 11189
Conc: 9.47 ng/ml

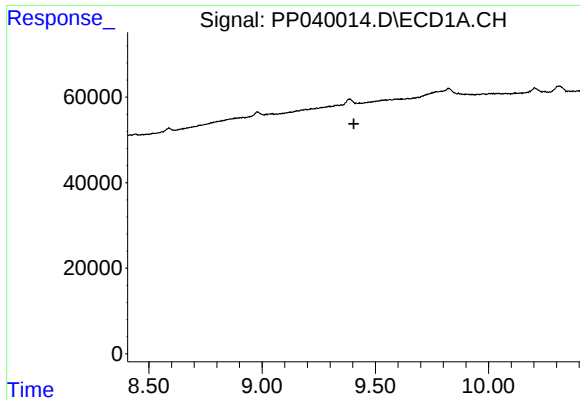

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.405 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

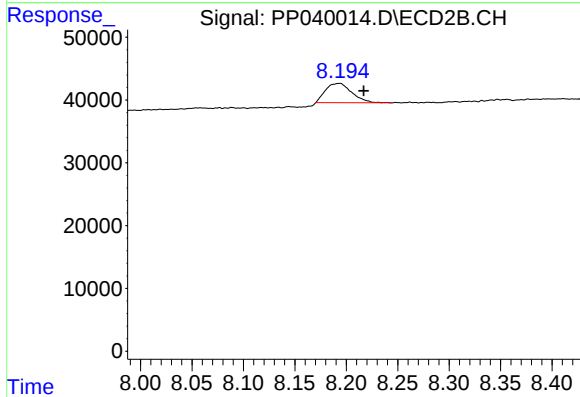


#38 AR-1262-3

R.T.: 8.194 min
Delta R.T.: -0.023 min
Response: 54941
Conc: 56.41 ng/ml

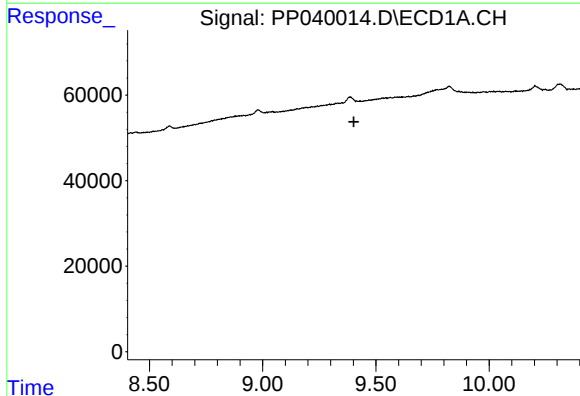


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.403 min
Response: 0
Conc: N.D.

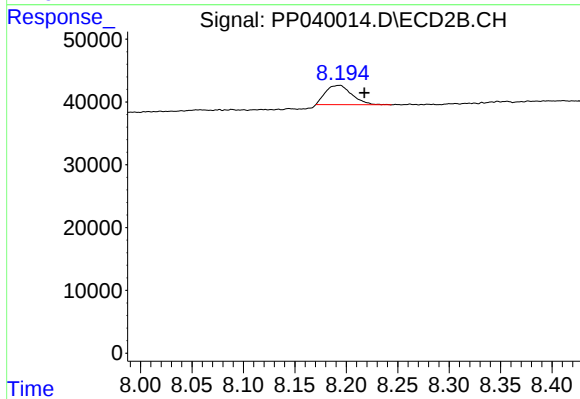

#41 AR-1268-1


R.T.: 8.194 min
Delta R.T.: -0.024 min
Response: 54941
Conc: 20.36 ng/ml

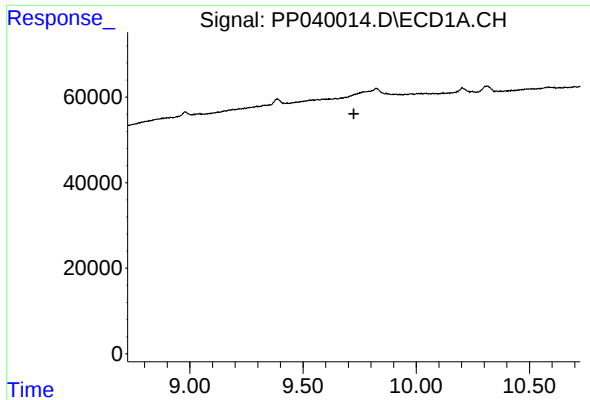

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

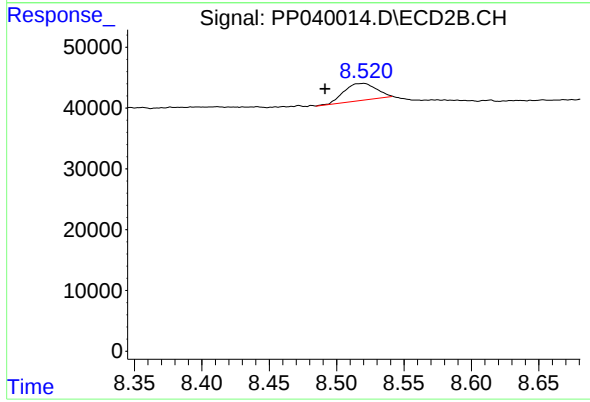

#43 AR-1268-3

R.T.: 8.520 min
Delta R.T.: 0.029 min
Response: 47086
Conc: 21.50 ng/ml