

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101321\
 Data File : PP040023.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Oct 2021 13:40
 Operator : AJ\MA
 Sample : N4171-07 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 02:27:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.895	3.983	40763	28876	1.342	1.708 #
2)	SA Decachlor...	10.915	9.312	35084	34337	1.419	1.618
Target Compounds							
10)	L2 AR-1221-3	0.000	4.422	0	11749	N.D.	21.695 #
11)	L3 AR-1232-1	0.000	4.422	0	11749	N.D.	28.927 #
30)	L6 AR-1254-5	0.000	7.380	0	11907	N.D.	9.225 #
32)	L7 AR-1260-2	0.000	7.019f	0	5430	N.D.	4.586 #
33)	L7 AR-1260-3	0.000	7.196	0	6183	N.D.	5.233 #
36)	L8 AR-1262-1	0.000	7.380	0	11907	N.D.	16.950 #
43)	L9 AR-1268-3	0.000	8.521f	0	7084	N.D.	3.235 #
45)	L9 AR-1268-5	10.596f	0.000	30923	0	3.595	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101321\
Data File : PP040023.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Oct 2021 13:40
Operator : AJ\MA
Sample : N4171-07 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 02:27:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

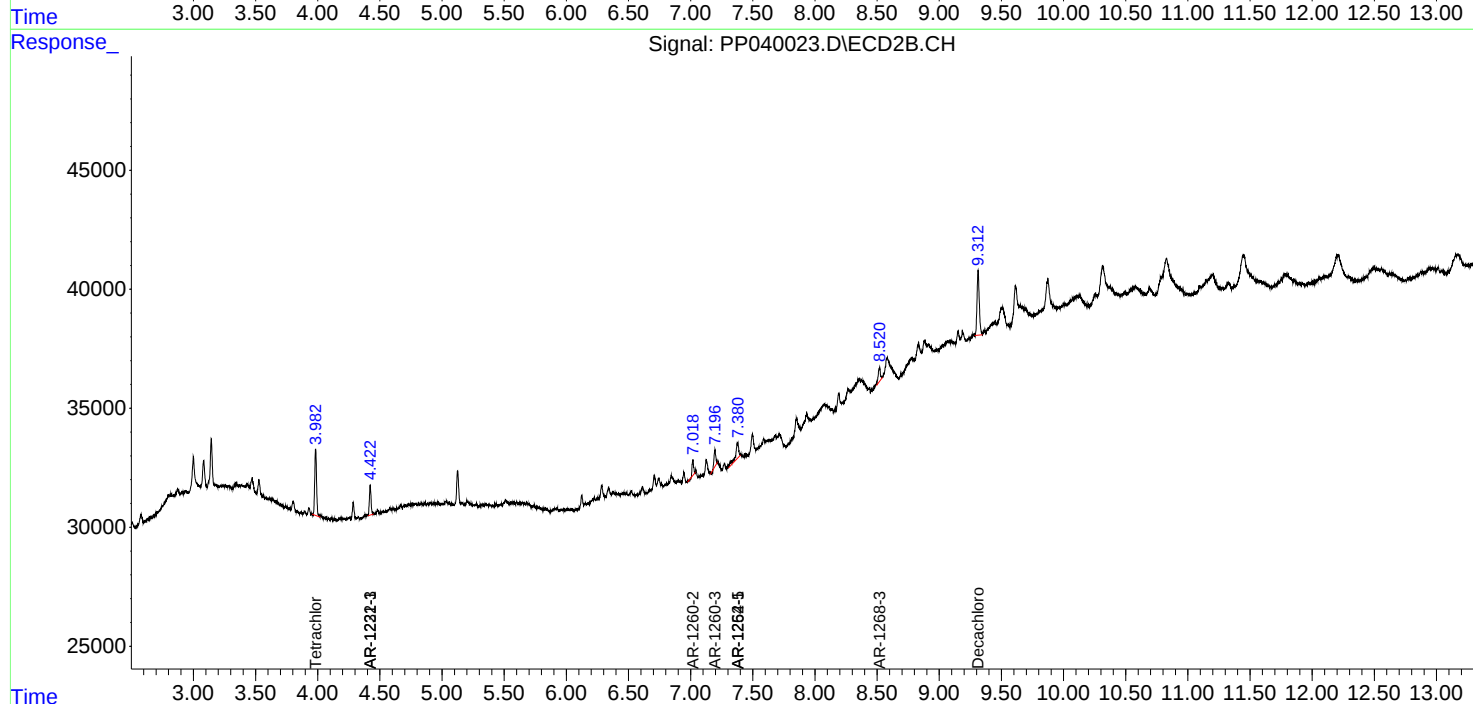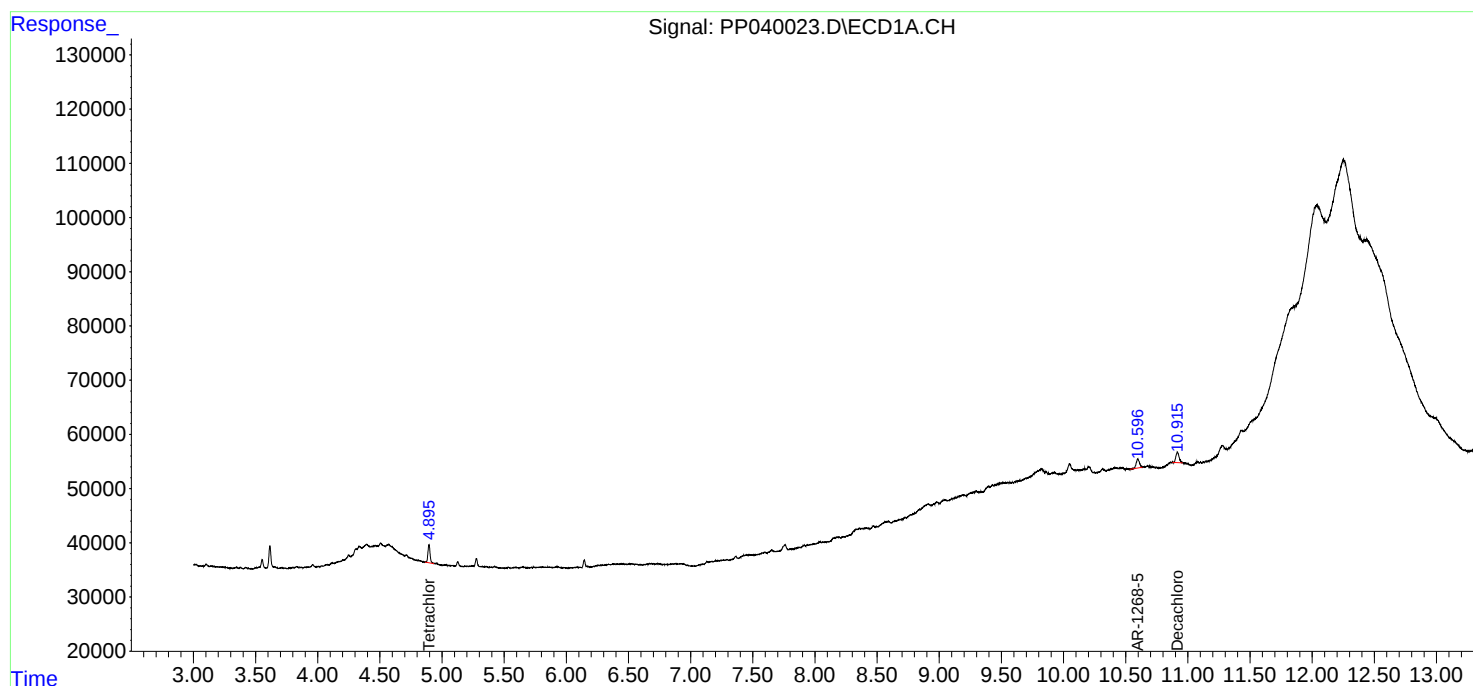


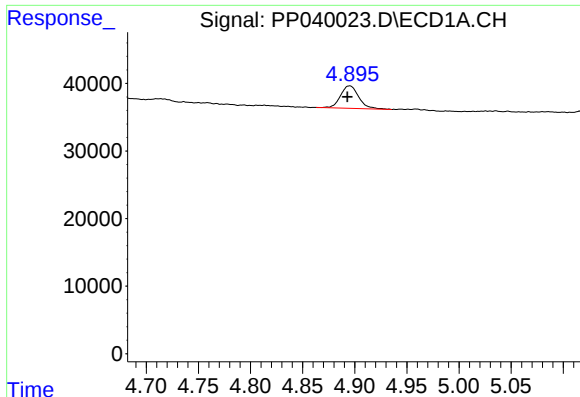

#1 Tetrachloro-m-xylene


R.T.: 4.895 min
Delta R.T.: 0.002 min
Response: 40763
Conc: 1.34 ng/ml

Instrument :
ECD_P
ClientSampleId :

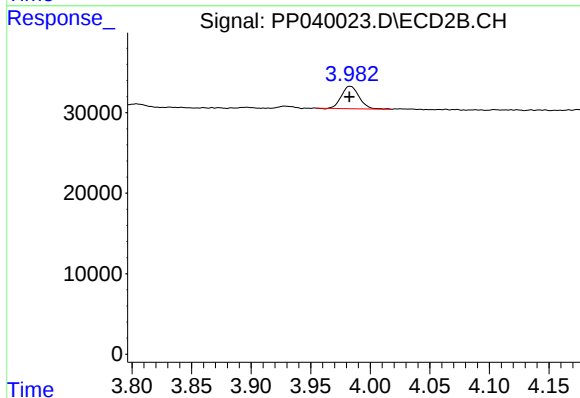


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 28876
Conc: 1.71 ng/ml

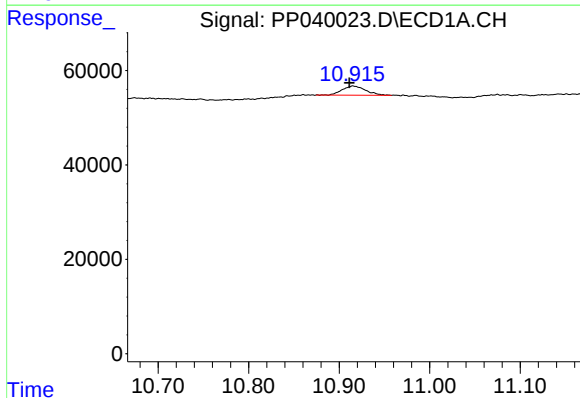


#2 Decachlorobiphenyl

R.T.: 10.915 min
Delta R.T.: 0.004 min
Response: 35084
Conc: 1.42 ng/ml

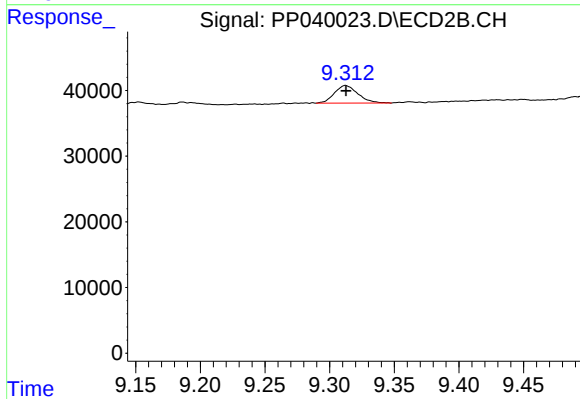

#2 Decachlorobiphenyl


R.T.: 9.312 min
Delta R.T.: 0.000 min
Response: 34337
Conc: 1.62 ng/ml

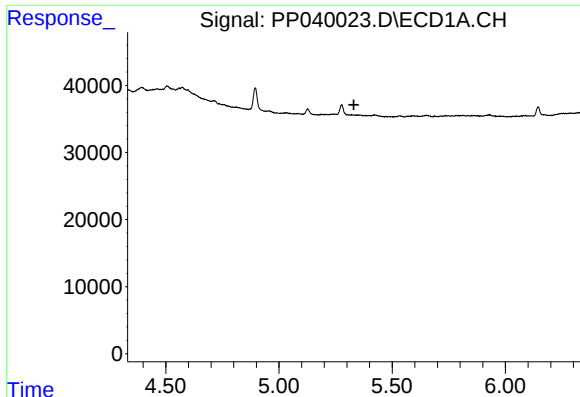

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 5.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

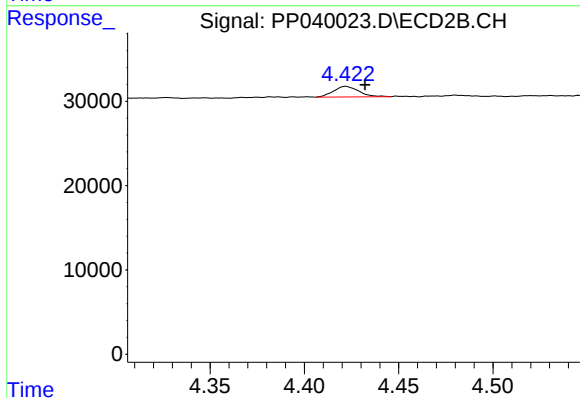


#10 AR-1221-3

R.T.: 4.422 min
Delta R.T.: -0.010 min
Response: 11749
Conc: 21.70 ng/ml

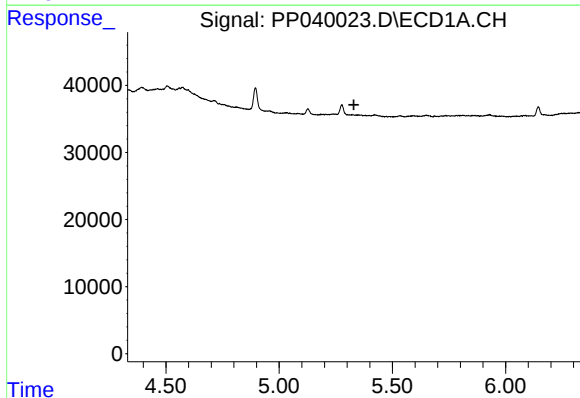


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 5.330 min
Response: 0
Conc: N.D.

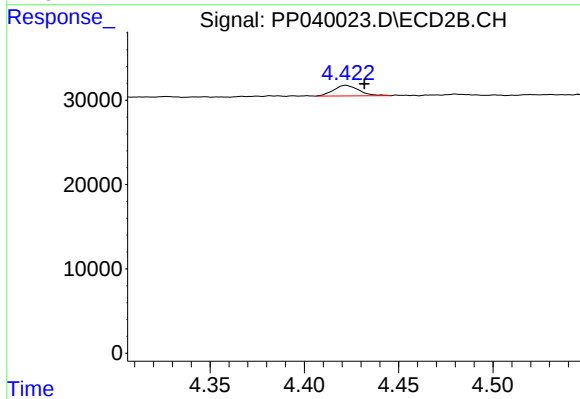

#11 AR-1232-1


R.T.: 4.422 min
Delta R.T.: -0.010 min
Response: 11749
Conc: 28.93 ng/ml

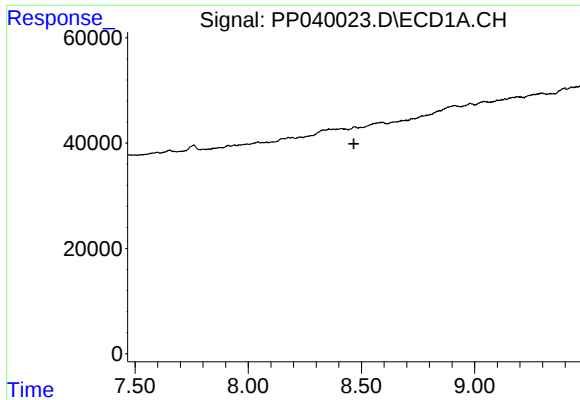

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 8.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

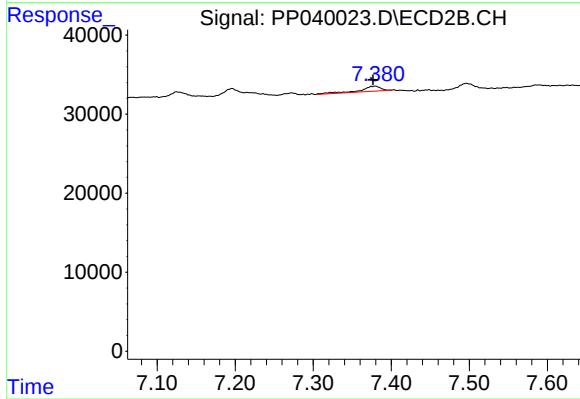


#30 AR-1254-5

R.T.: 7.380 min
Delta R.T.: 0.003 min
Response: 11907
Conc: 9.22 ng/ml

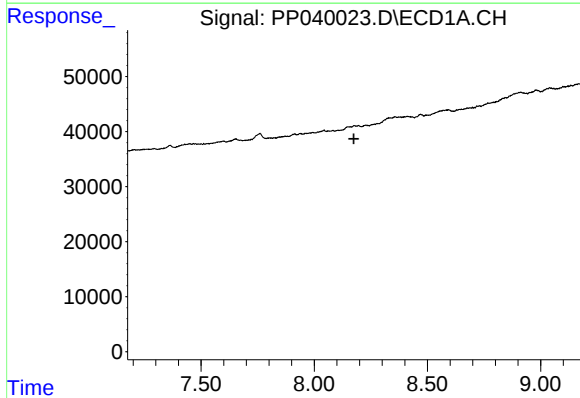


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 8.175 min
Response: 0
Conc: N.D.

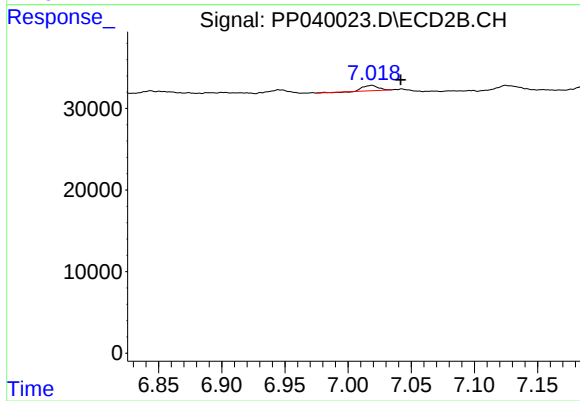

#32 AR-1260-2


R.T.: 7.019 min
Delta R.T.: -0.023 min
Response: 5430
Conc: 4.59 ng/ml

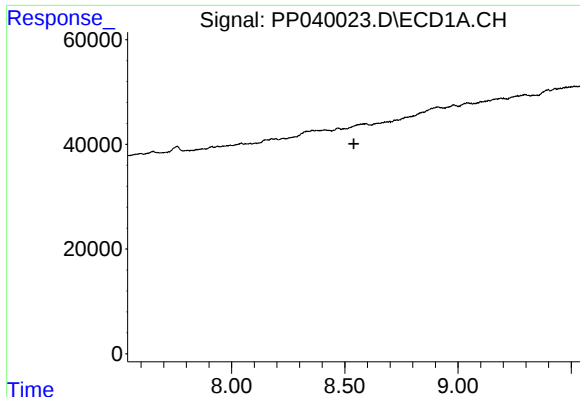

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.540 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

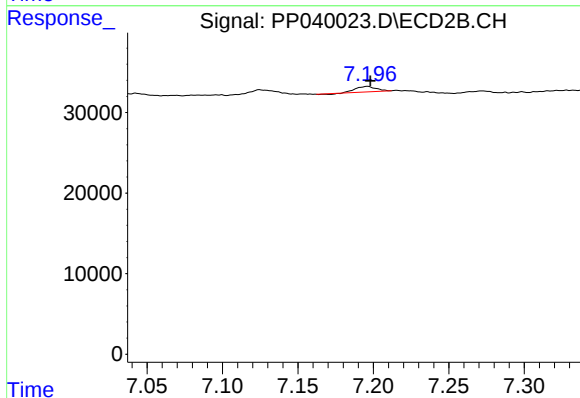


#33 AR-1260-3

R.T.: 7.196 min
Delta R.T.: -0.002 min
Response: 6183
Conc: 5.23 ng/ml

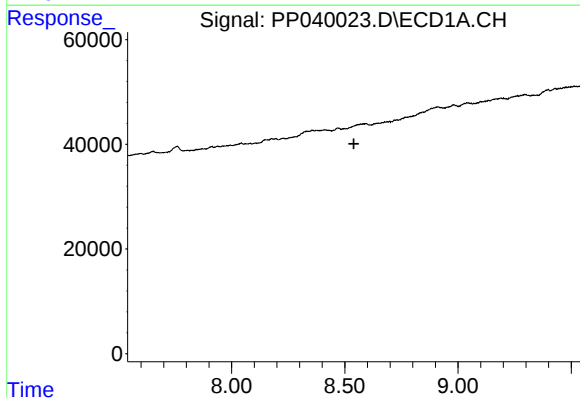


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 8.540 min
Response: 0
Conc: N.D.

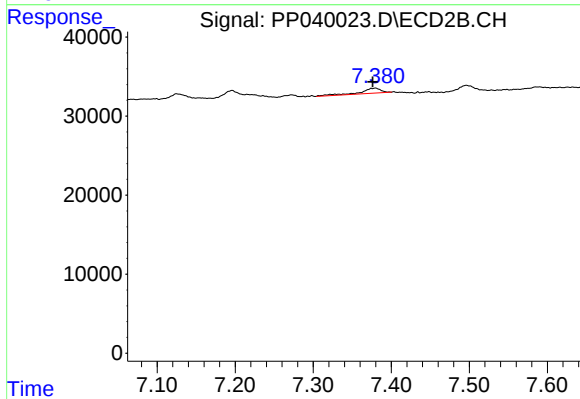

#36 AR-1262-1


R.T.: 7.380 min
Delta R.T.: 0.004 min
Response: 11907
Conc: 16.95 ng/ml

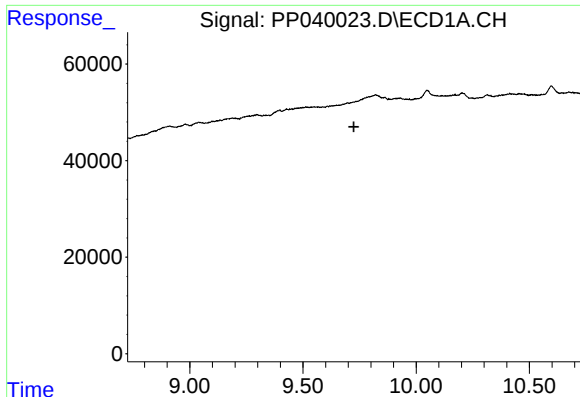

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

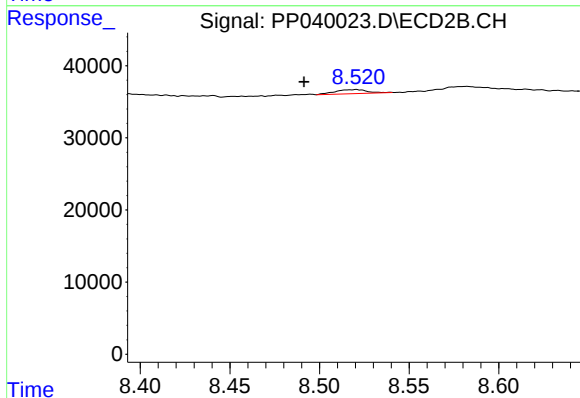


#43 AR-1268-3

R.T.: 8.521 min
Delta R.T.: 0.029 min
Response: 7084
Conc: 3.24 ng/ml

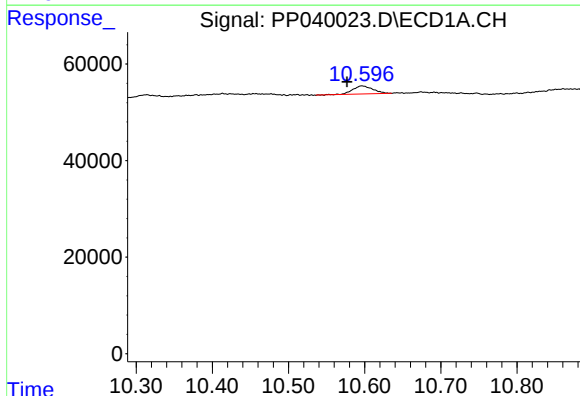

#45 AR-1268-5

R.T.: 10.596 min
Delta R.T.: 0.020 min
Response: 30923
Conc: 3.60 ng/ml

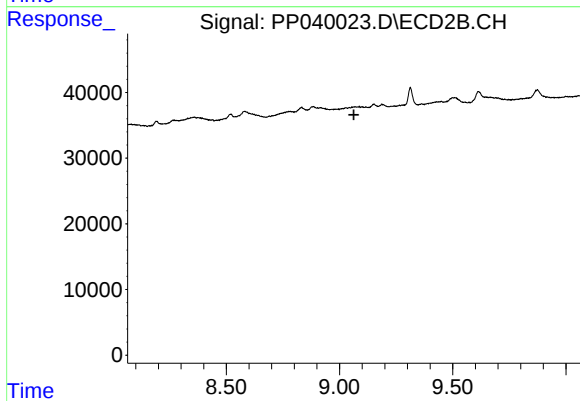

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.064 min
Response: 0
Conc: N.D.