

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101321\
 Data File : PP040029.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Oct 2021 15:20
 Operator : AJ\MA
 Sample : M4171-10 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 02:29:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.894	3.982	42143	27441	1.388	1.623
2)	SA Decachlor...	10.917	9.313	34230	34498	1.385	1.625
Target Compounds							
10)	L2 AR-1221-3	0.000	4.422	0	14338	N.D.	26.476 #
11)	L3 AR-1232-1	0.000	4.422	0	14338	N.D.	35.301 #
32)	L7 AR-1260-2	8.195f	7.018f	36572	33397	26.758	28.204
33)	L7 AR-1260-3	0.000	7.193	0	66125	N.D.	55.966 #
35)	L7 AR-1260-5	0.000	7.934	0	6027	N.D.	2.949 #
37)	L8 AR-1262-2	0.000	7.934	0	6027	N.D.	2.678 #
45)	L9 AR-1268-5	10.597f	0.000	29100	0	3.383	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101321\
Data File : PP040029.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Oct 2021 15:20
Operator : AJ\MA
Sample : M4171-10 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 02:29:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

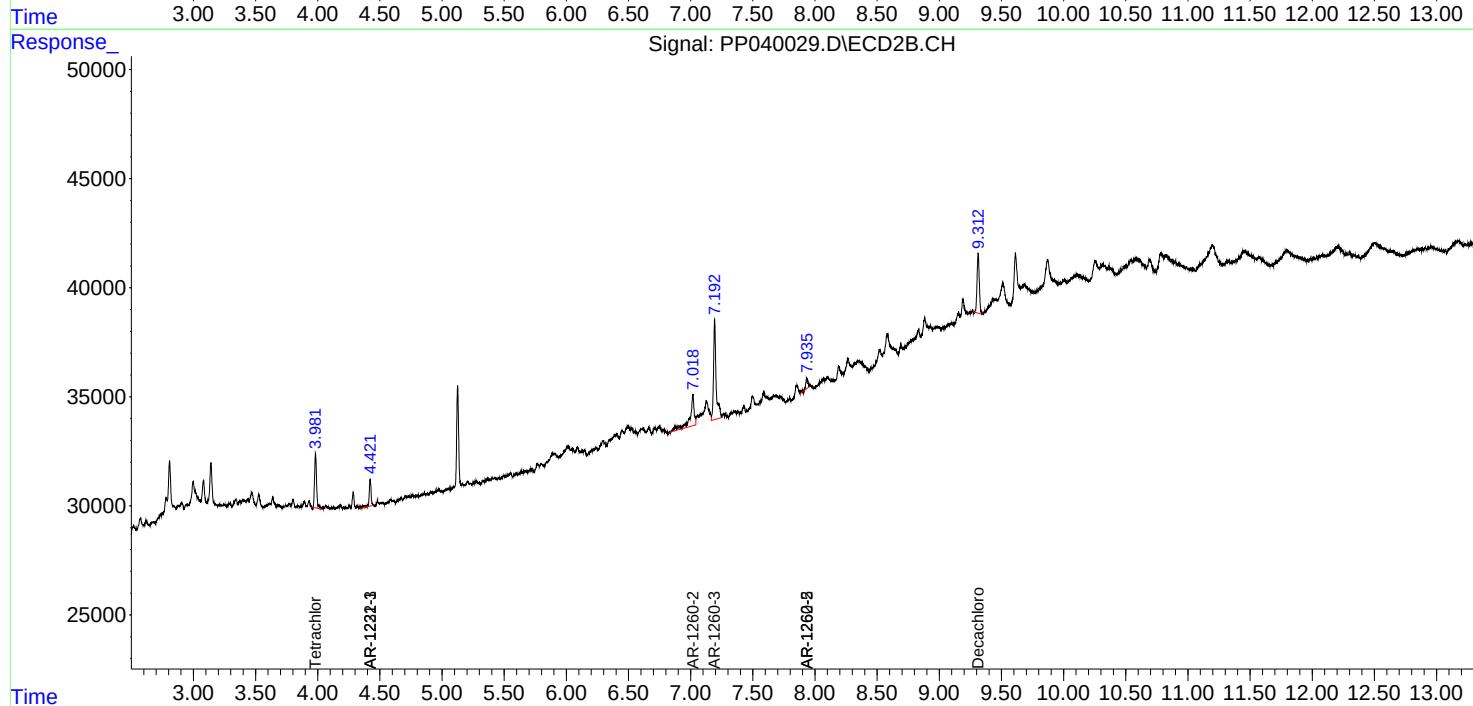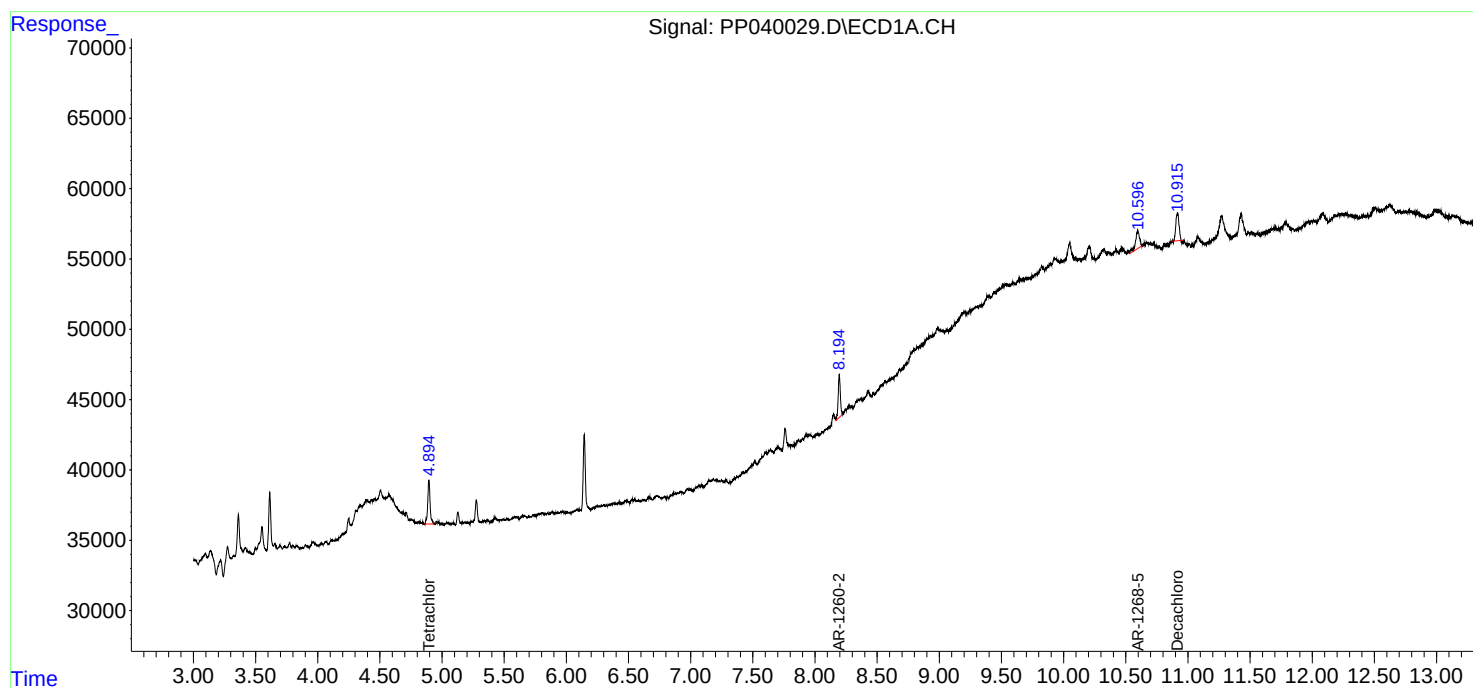


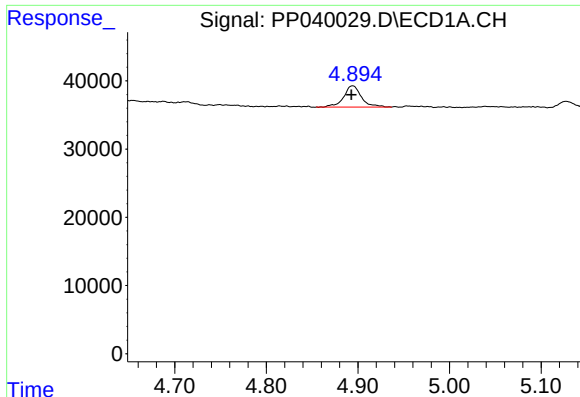

#1 Tetrachloro-m-xylene


R.T.: 4.894 min
Delta R.T.: 0.001 min
Response: 42143
Conc: 1.39 ng/ml

Instrument :
ECD_P
ClientSampleId :

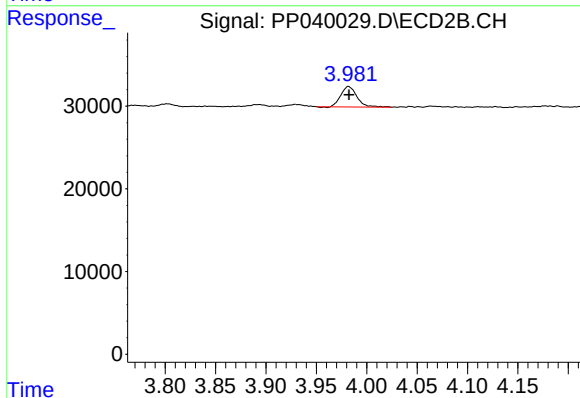


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 27441
Conc: 1.62 ng/ml

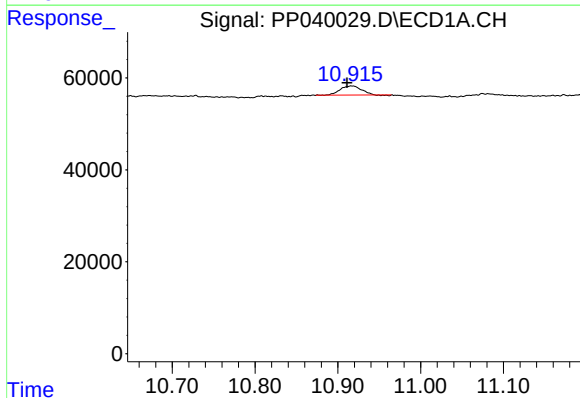


#2 Decachlorobiphenyl

R.T.: 10.917 min
Delta R.T.: 0.005 min
Response: 34230
Conc: 1.38 ng/ml

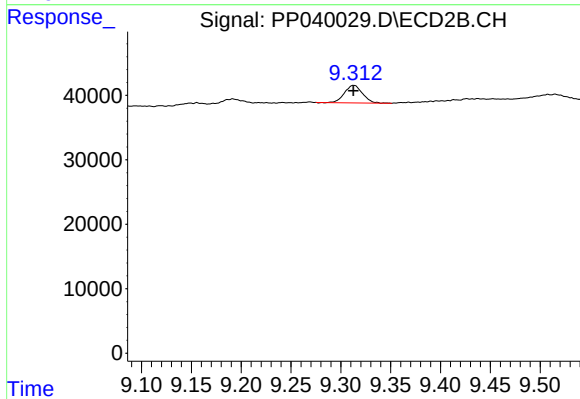

#2 Decachlorobiphenyl


R.T.: 9.313 min
Delta R.T.: 0.000 min
Response: 34498
Conc: 1.63 ng/ml

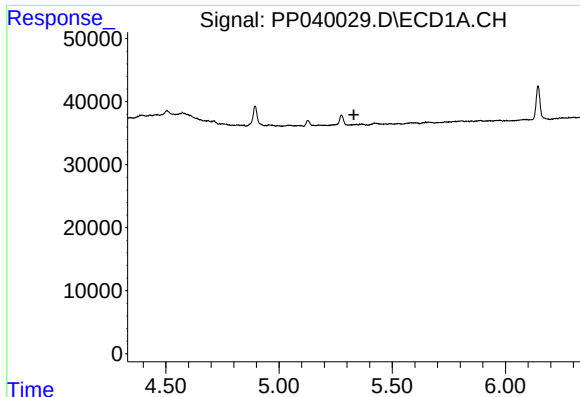

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 5.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

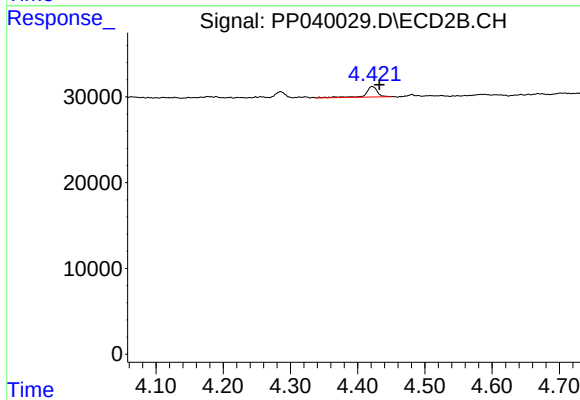


#10 AR-1221-3

R.T.: 4.422 min
Delta R.T.: -0.011 min
Response: 14338
Conc: 26.48 ng/ml

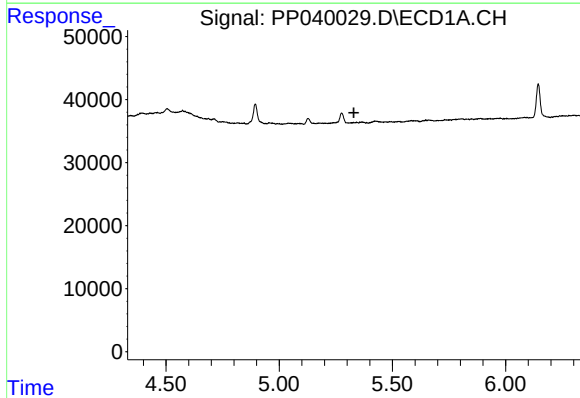


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 5.330 min
Response: 0
Conc: N.D.

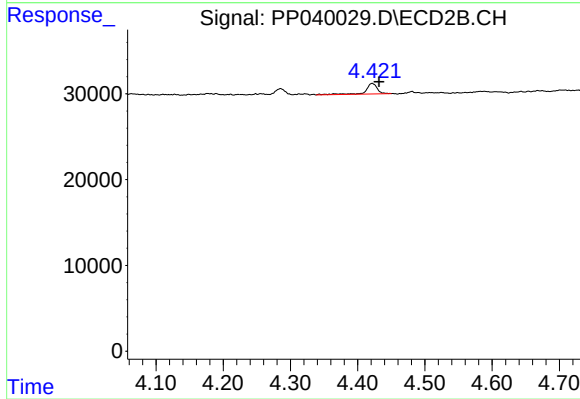

#11 AR-1232-1


R.T.: 4.422 min
Delta R.T.: -0.010 min
Response: 14338
Conc: 35.30 ng/ml

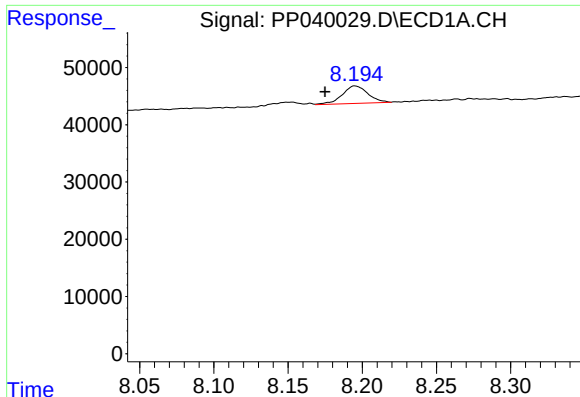

#32 AR-1260-2


R.T.: 8.195 min
Delta R.T.: 0.020 min
Response: 36572
Conc: 26.76 ng/ml

Instrument :
ECD_P
ClientSampleId :

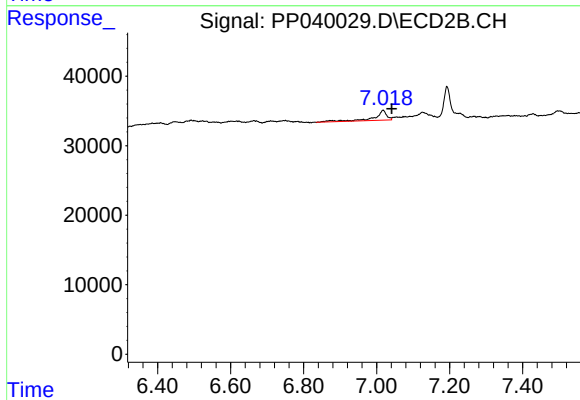


#32 AR-1260-2

R.T.: 7.018 min
Delta R.T.: -0.024 min
Response: 33397
Conc: 28.20 ng/ml

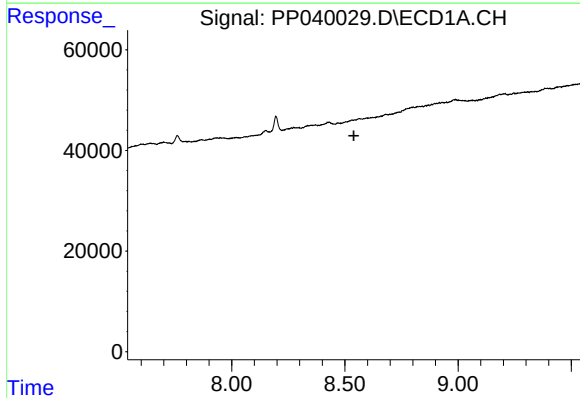


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.540 min
Response: 0
Conc: N.D.

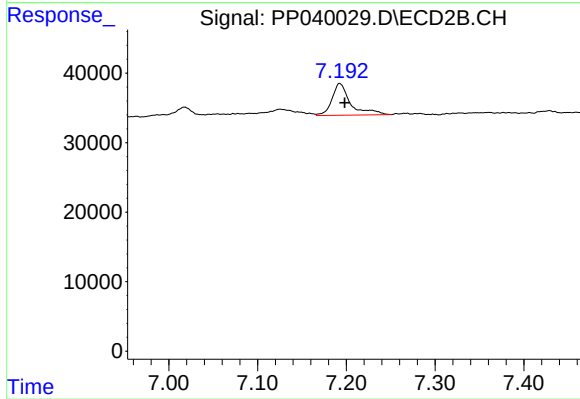

#33 AR-1260-3


R.T.: 7.193 min
Delta R.T.: -0.005 min
Response: 66125
Conc: 55.97 ng/ml

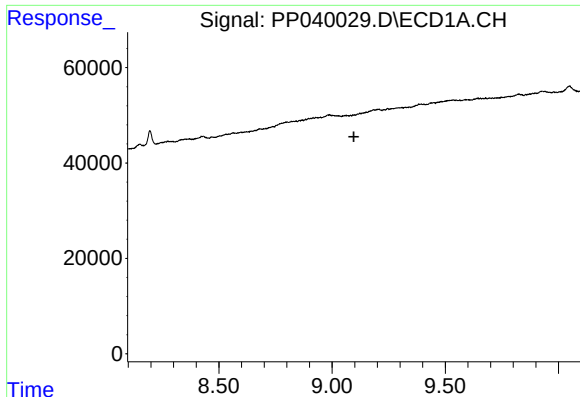

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 9.097 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

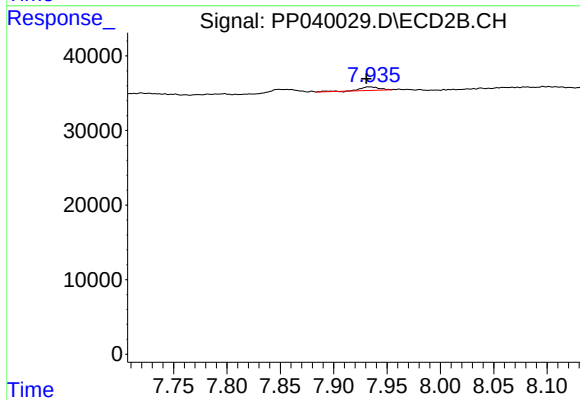


#35 AR-1260-5

R.T.: 7.934 min
Delta R.T.: 0.003 min
Response: 6027
Conc: 2.95 ng/ml

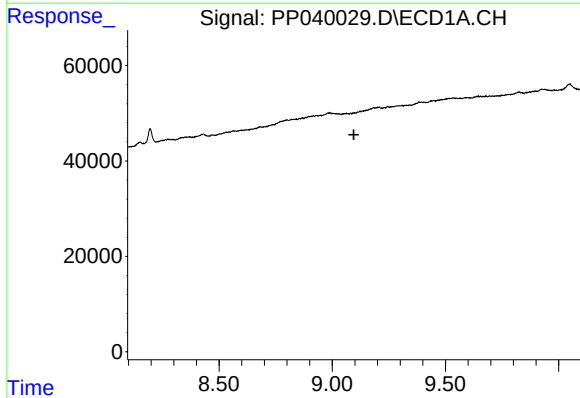


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.

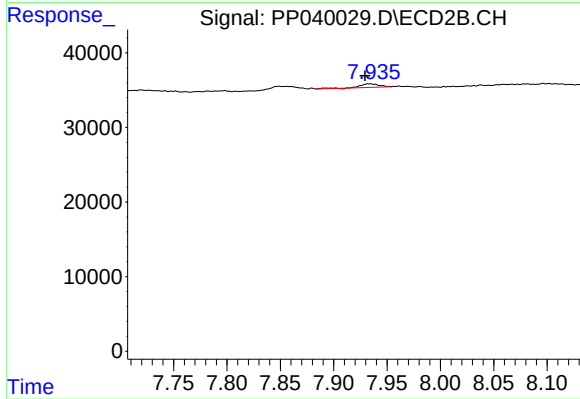

#37 AR-1262-2


R.T.: 7.934 min
Delta R.T.: 0.004 min
Response: 6027
Conc: 2.68 ng/ml

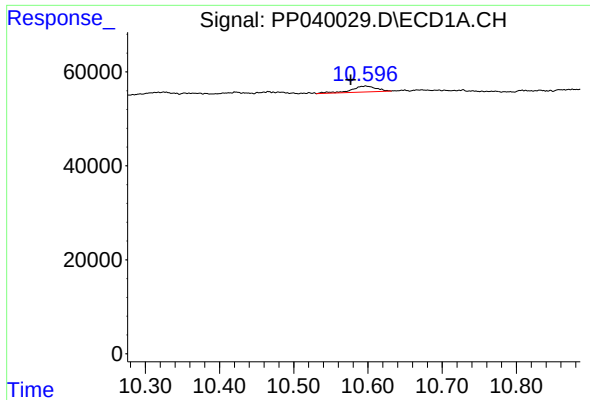

#45 AR-1268-5

R.T.: 10.597 min
Delta R.T.: 0.020 min
Response: 29100
Conc: 3.38 ng/ml

Instrument :
ECD_P
ClientSampleId :

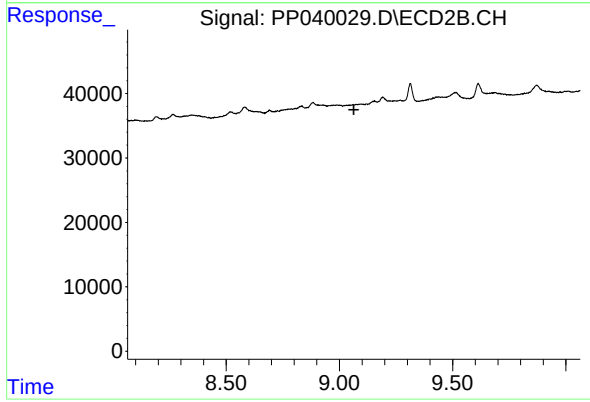

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.064 min
Response: 0
Conc: N.D.