

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101322\
 Data File : PP052336.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2022 03:38
 Operator : YP\AJ
 Sample : N5114-03
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FMC-0080

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/14/2022
 Supervised By :Ankita Jodhani 10/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 06:41:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 12 05:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.424	3.692	29719533	25566431	18.907	22.316
2) SA Decachlor...	10.213	8.827f	17036461	18559356	12.275m	16.610m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101322\
Data File : PP052336.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2022 03:38
Operator : YP\AJ
Sample : N5114-03
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
FMC-0080


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/14/2022
Supervised By :Ankita Jodhani 10/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 06:41:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

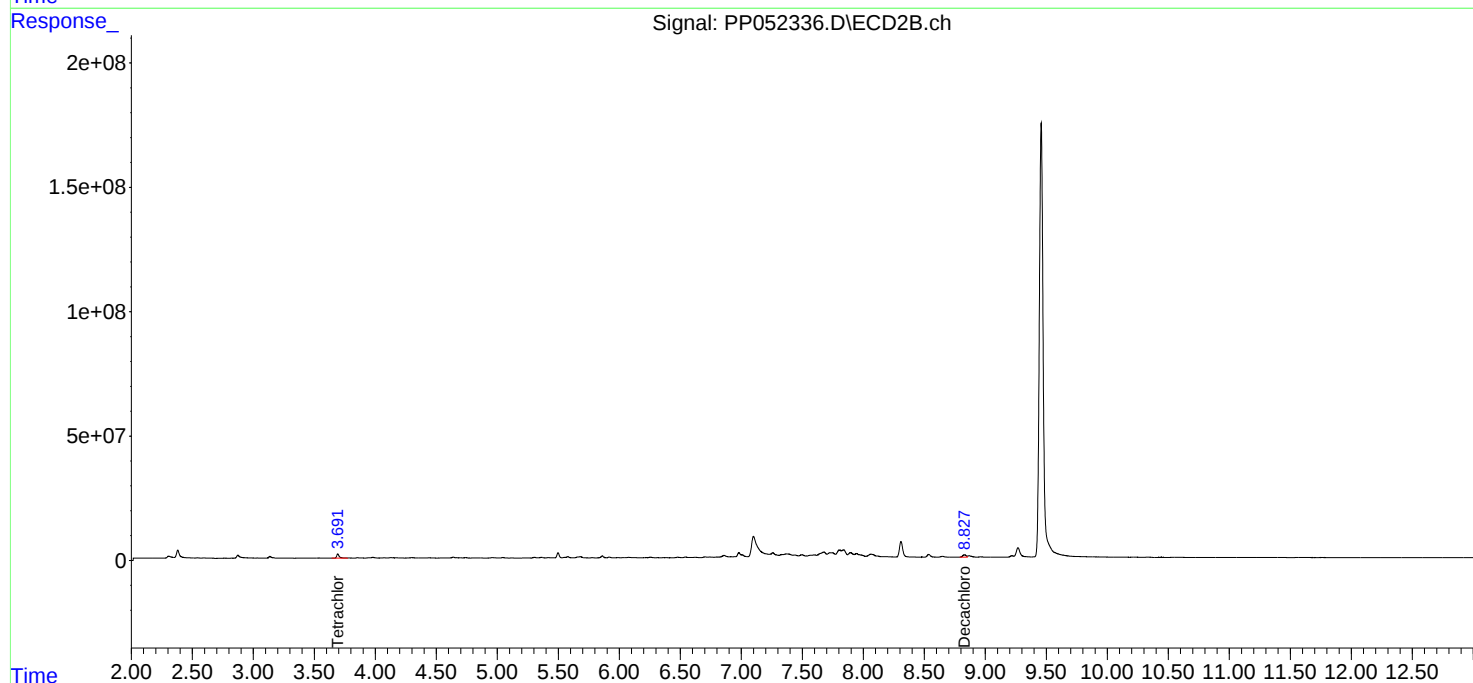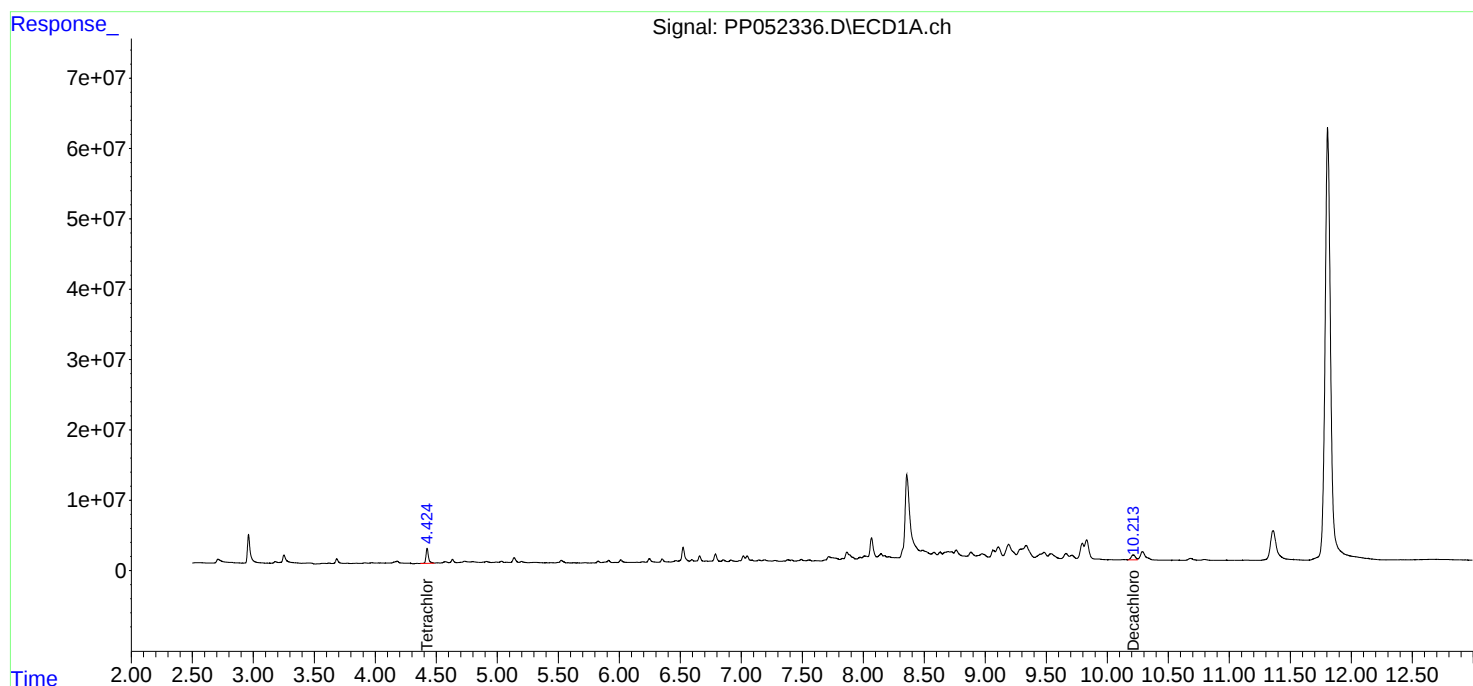

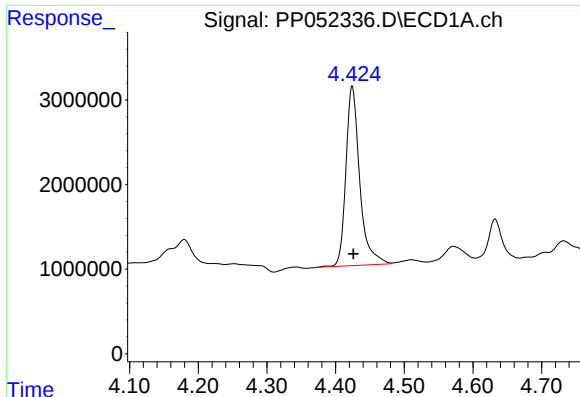


#1 Tetrachloro-m-xylene

R.T.: 4.424 min
Delta R.T.: -0.002 min
Response: 29719533
Conc: 18.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
FMC-0080


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/14/2022
Supervised By :Ankita Jodhani 10/14/2022

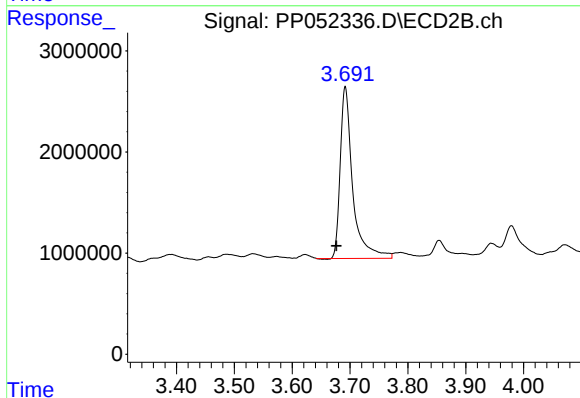


#1 Tetrachloro-m-xylene

R.T.: 3.692 min
Delta R.T.: 0.015 min
Response: 25566431
Conc: 22.32 ng/ml

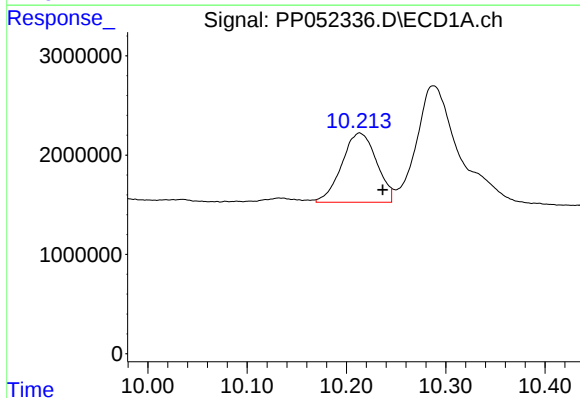

#2 Decachlorobiphenyl

R.T.: 10.213 min
Delta R.T.: -0.024 min
Response: 17036461
Conc: 12.28 ng/ml m

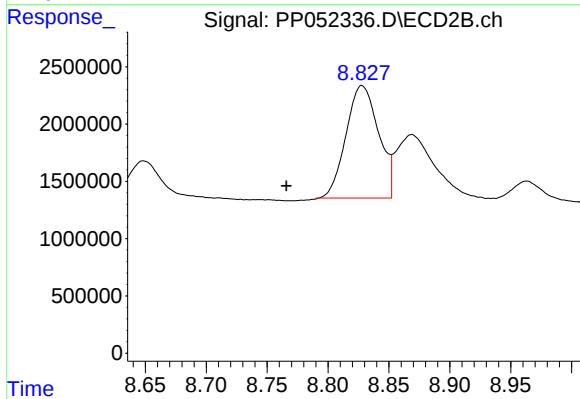

#2 Decachlorobiphenyl

R.T.: 8.827 min
Delta R.T.: 0.061 min
Response: 18559356
Conc: 16.61 ng/ml m