

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101322\
 Data File : PP052337.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2022 03:55
 Operator : YP\AJ
 Sample : N5114-04
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FMC-0095

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/14/2022
 Supervised By :Ankita Jodhani 10/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 06:42:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 12 05:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.413	3.656	139.1E6	28854400	88.470	25.186m#
2) SA Decachlor...	10.257	8.784	29142828	24114912	20.999	21.582

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101322\
Data File : PP052337.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2022 03:55
Operator : YP\AJ
Sample : N5114-04
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
FMC-0095


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/14/2022
Supervised By :Ankita Jodhani 10/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 06:42:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

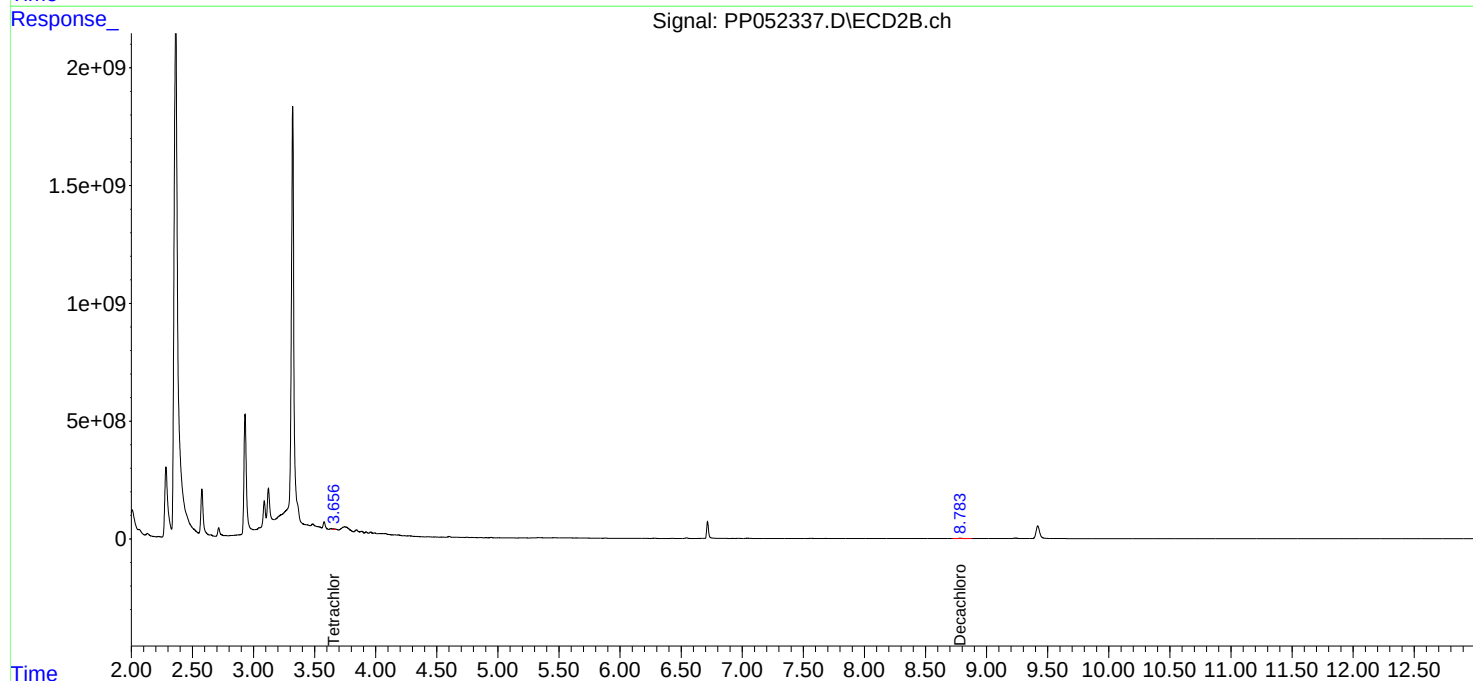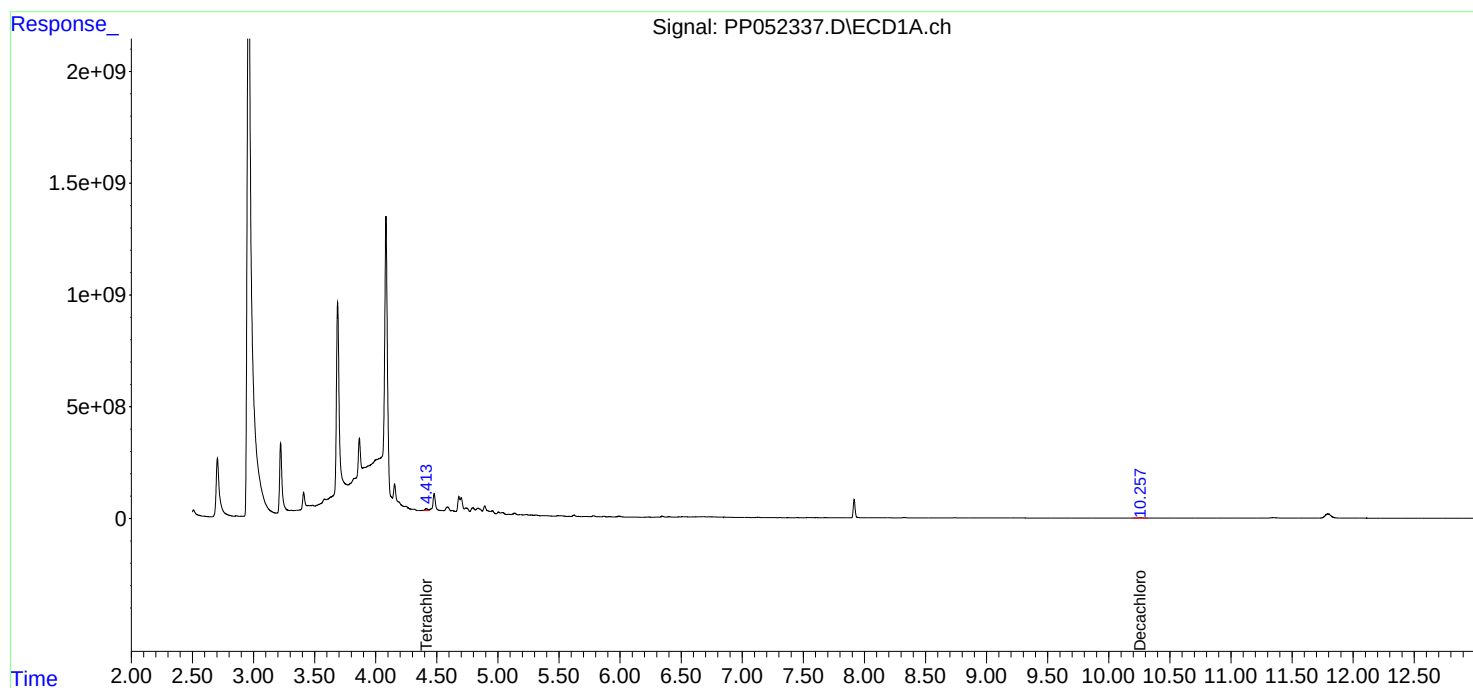

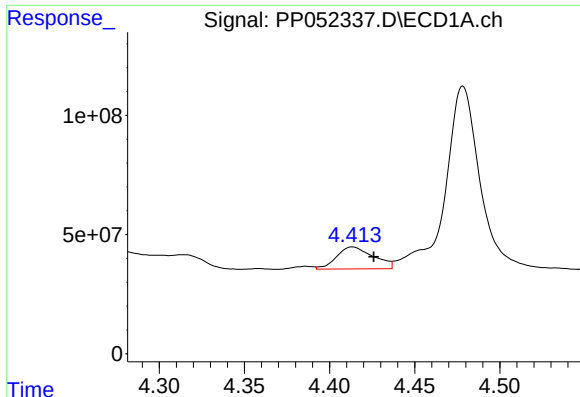


#1 Tetrachloro-m-xylene

R.T.: 4.413 min
Delta R.T.: -0.013 min
Response: 139062839
Conc: 88.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
FMC-0095


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/14/2022
Supervised By :Ankita Jodhani 10/14/2022

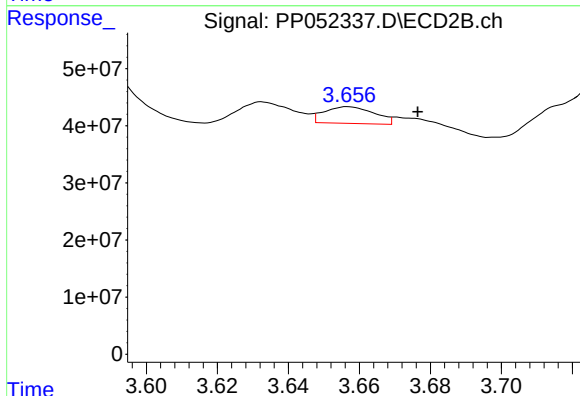


#1 Tetrachloro-m-xylene

R.T.: 3.656 min
Delta R.T.: -0.020 min
Response: 28854400
Conc: 25.19 ng/ml m

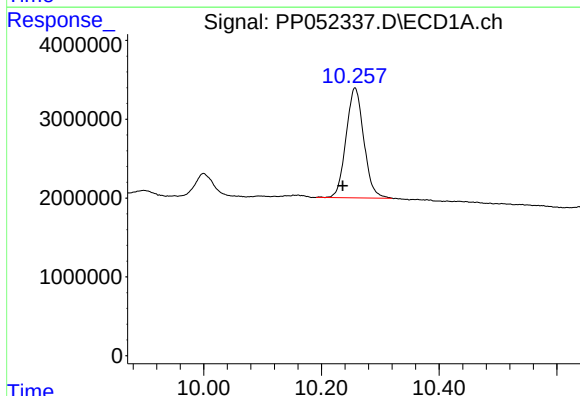

#2 Decachlorobiphenyl

R.T.: 10.257 min
Delta R.T.: 0.021 min
Response: 29142828
Conc: 21.00 ng/ml

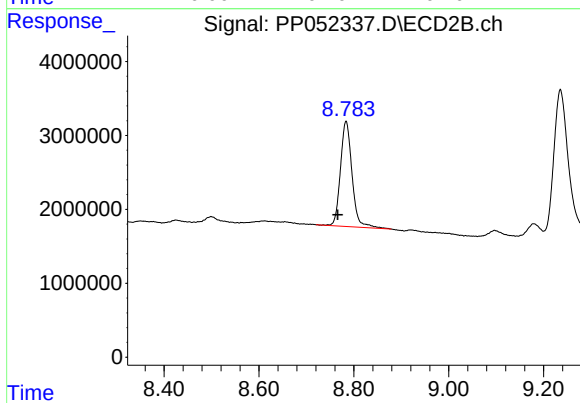

#2 Decachlorobiphenyl

R.T.: 8.784 min
Delta R.T.: 0.018 min
Response: 24114912
Conc: 21.58 ng/ml