

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101322\
 Data File : PP052347.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2022 07:30
 Operator : YP\AJ
 Sample : N5096-04 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 2699

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/14/2022
 Supervised By :Ankita Jodhani 10/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 11:05:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 12 05:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.421	3.671	3057589	2096867	1.945	1.830m
2) SA Decachlor...	10.239	8.766	3921272	2416773	2.825	2.163

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101322\
Data File : PP052347.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2022 07:30
Operator : YP\AJ
Sample : N5096-04 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
2699


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/14/2022
Supervised By :Ankita Jodhani 10/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 11:05:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

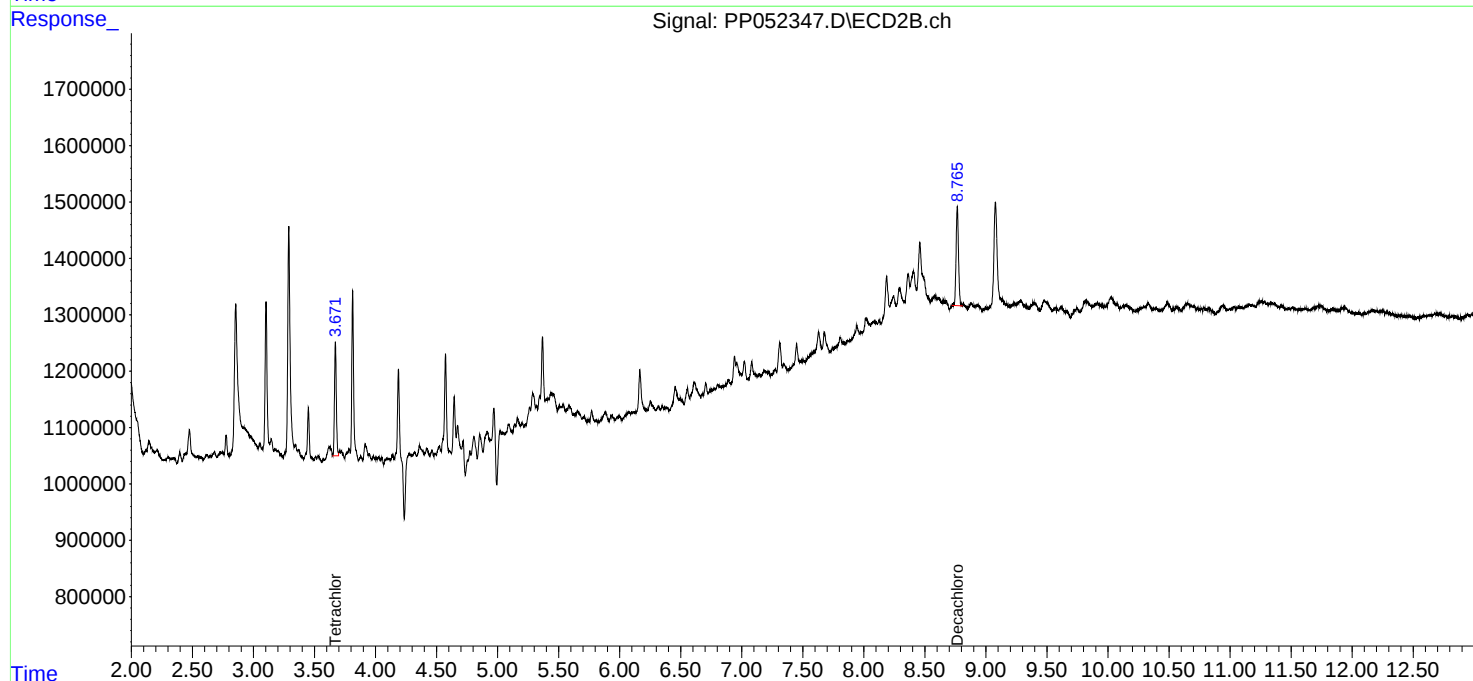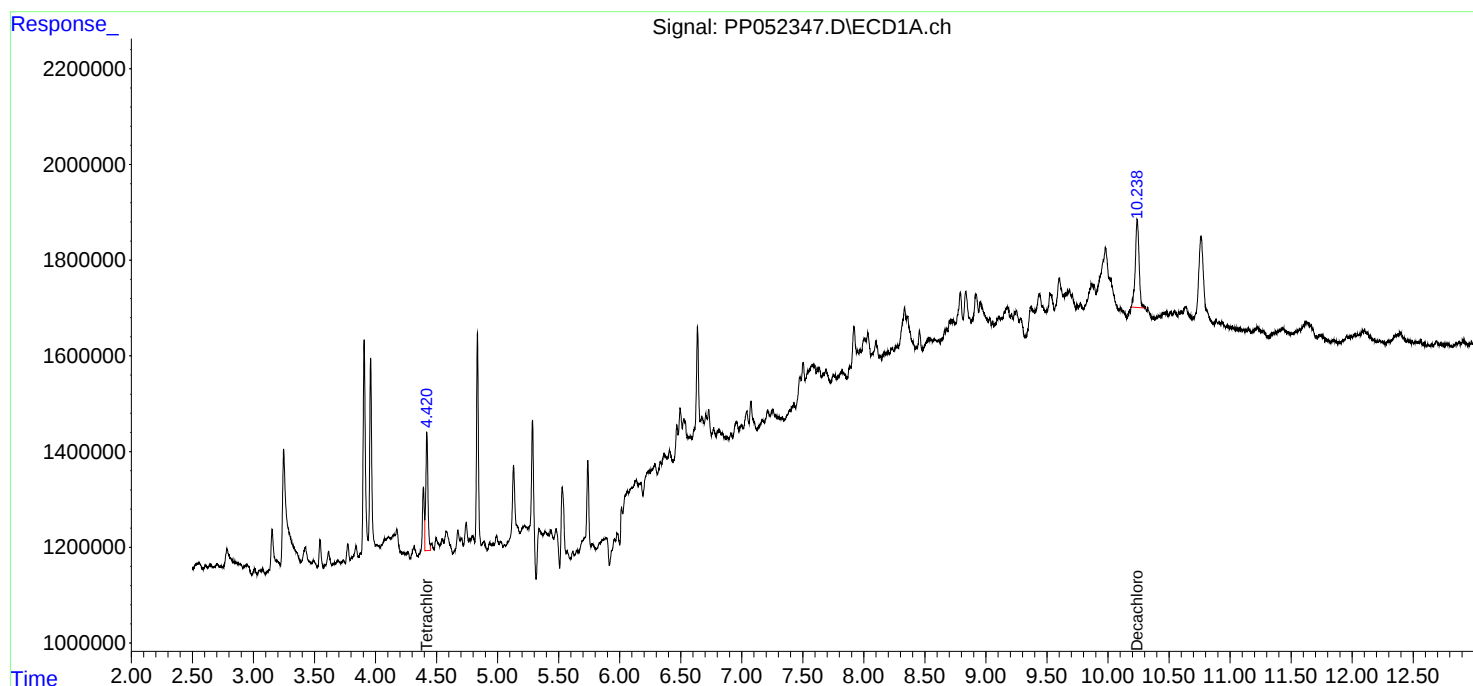

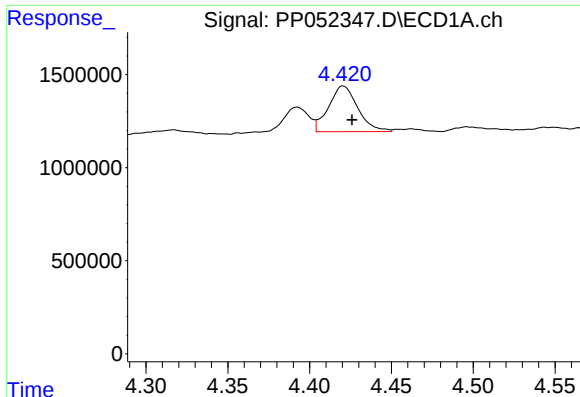


#1 Tetrachloro-m-xylene

R.T.: 4.421 min
Delta R.T.: -0.005 min
Response: 3057589
Conc: 1.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
2699


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/14/2022
Supervised By :Ankita Jodhani 10/14/2022

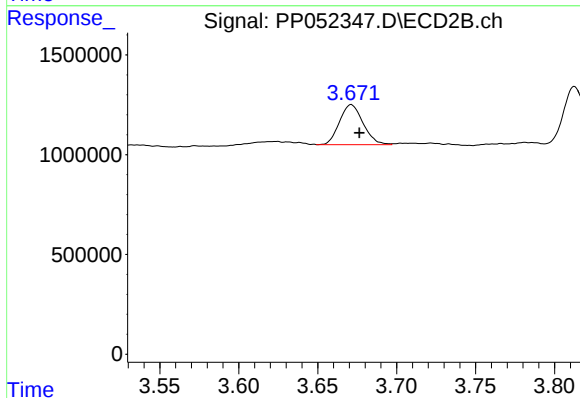


#1 Tetrachloro-m-xylene

R.T.: 3.671 min
Delta R.T.: -0.006 min
Response: 2096867
Conc: 1.83 ng/ml m

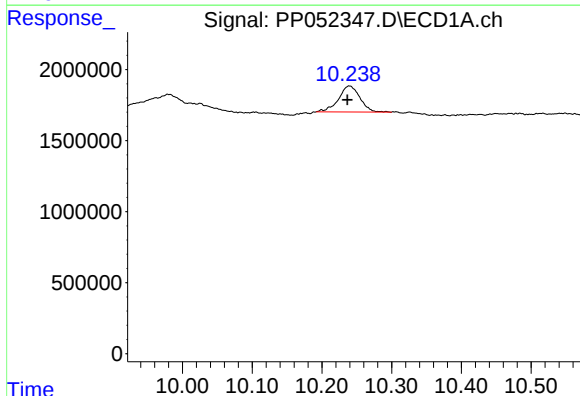

#2 Decachlorobiphenyl

R.T.: 10.239 min
Delta R.T.: 0.003 min
Response: 3921272
Conc: 2.83 ng/ml

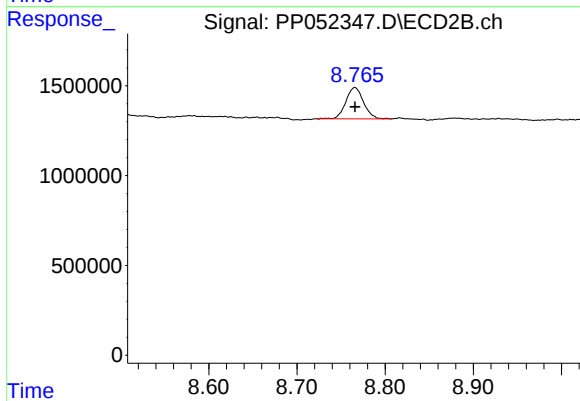

#2 Decachlorobiphenyl

R.T.: 8.766 min
Delta R.T.: 0.000 min
Response: 2416773
Conc: 2.16 ng/ml