

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101323\
 Data File : PP060986.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2023 01:39
 Operator : YP\AJ
 Sample : 04699-07
 Misc : AR1232 LOD 25 PPB
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 13:42:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 14 13:32:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.552	3.688	51241501	30761853	23.309	22.753
2) SA Decachlor...	10.512	8.757	38831810	34236475	24.797	22.771
Target Compounds						
11) L3 AR-1232-1	4.930	4.068	1454067	1078084	28.743	31.218
12) L3 AR-1232-2	5.471	4.807	715421	889952	26.822	26.911
13) L3 AR-1232-3	5.767	4.984	1445401	486114	30.800	26.233
14) L3 AR-1232-4	5.930	5.070	658108	362400	28.129	21.573
15) L3 AR-1232-5	6.022	5.241	618285	495420	31.726	26.374



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101323\
Data File : PP060986.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2023 01:39
Operator : YP\AJ
Sample : 04699-07
Misc : AR1232 LOD 25 PPB
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 13:42:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 14 13:32:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

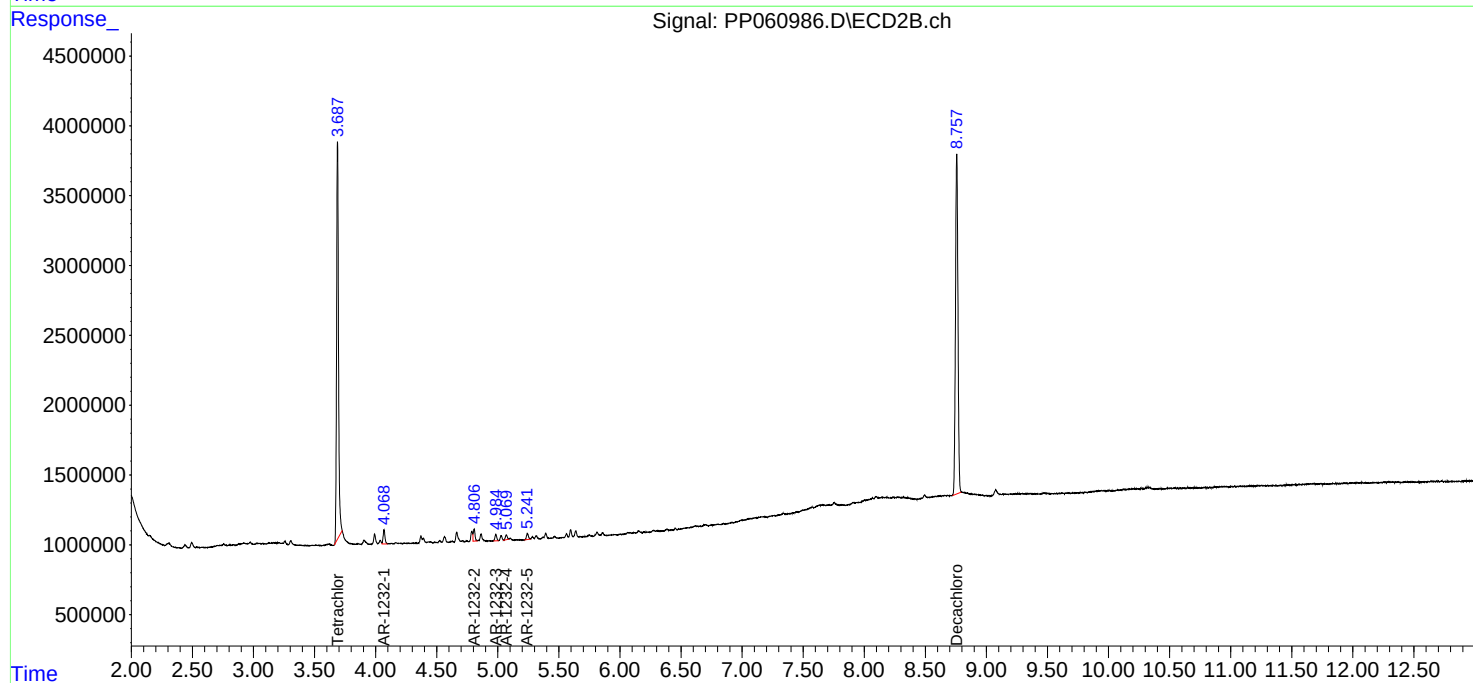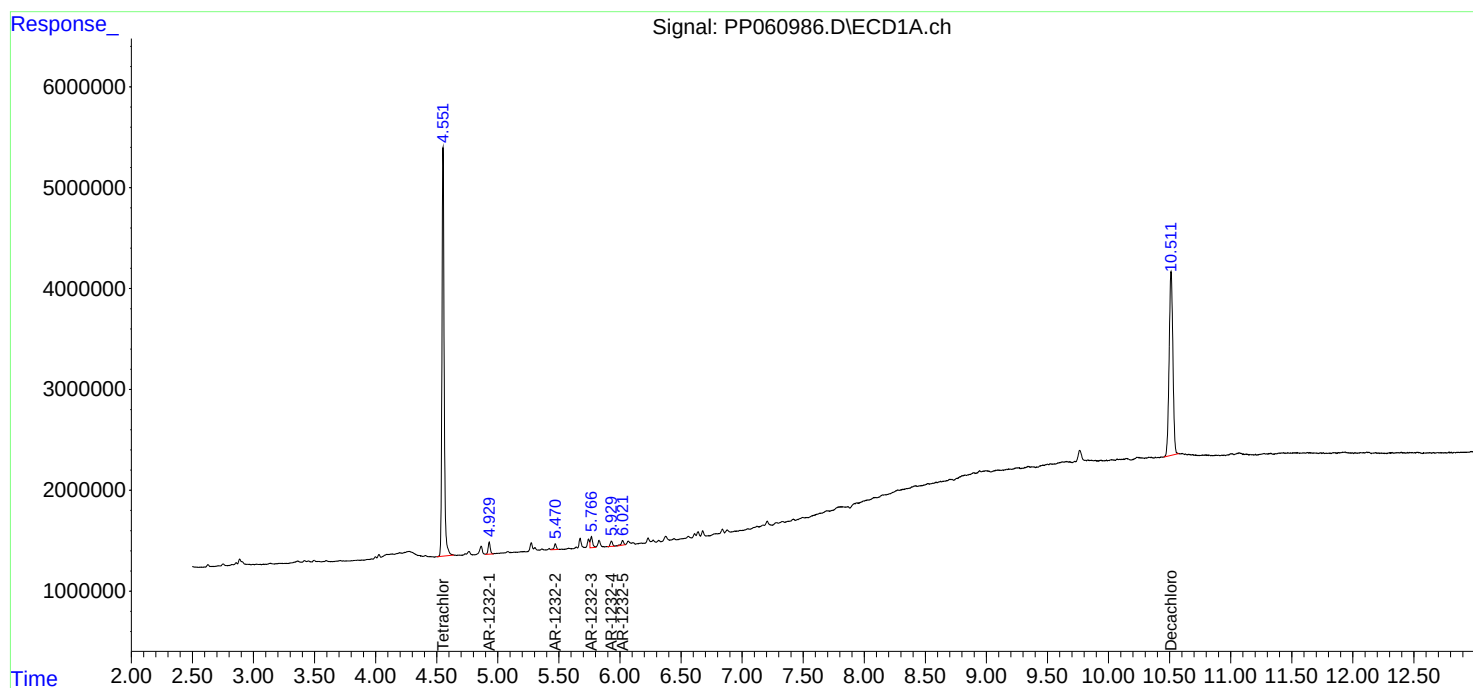


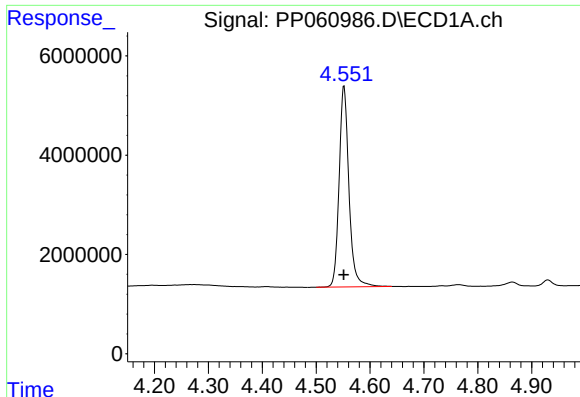

#1 Tetrachloro-m-xylene


R.T.: 4.552 min
Delta R.T.: 0.000 min
Response: 51241501
Conc: 23.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2023

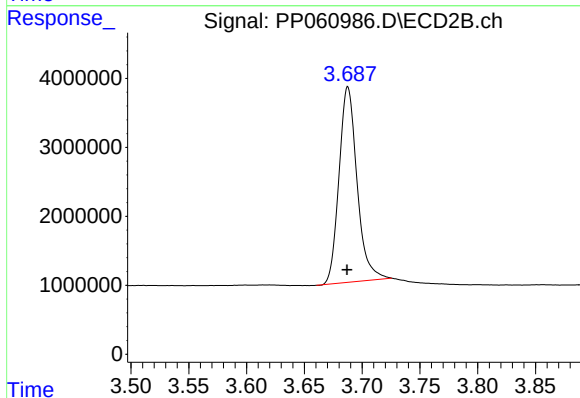


#1 Tetrachloro-m-xylene

R.T.: 3.688 min
Delta R.T.: 0.000 min
Response: 30761853
Conc: 22.75 ng/ml

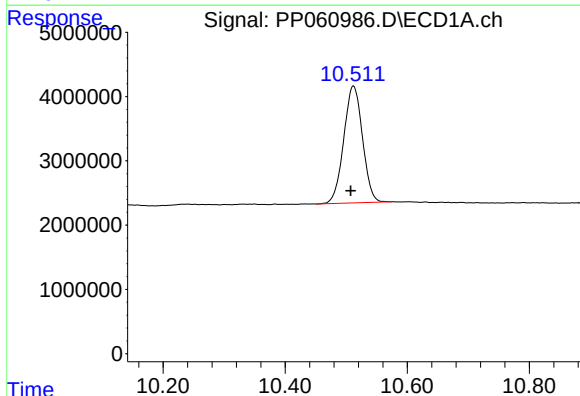


#2 Decachlorobiphenyl

R.T.: 10.512 min
Delta R.T.: 0.005 min
Response: 38831810
Conc: 24.80 ng/ml

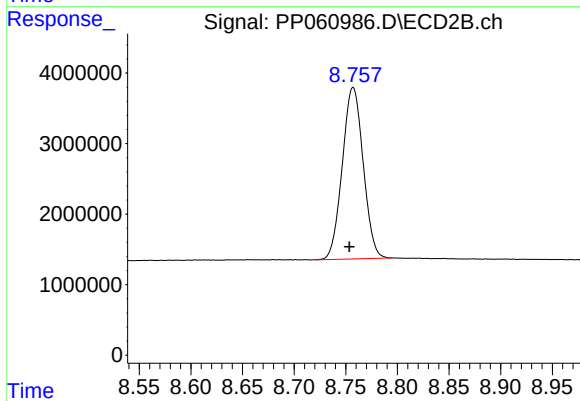

#2 Decachlorobiphenyl


R.T.: 8.757 min
Delta R.T.: 0.003 min
Response: 34236475
Conc: 22.77 ng/ml

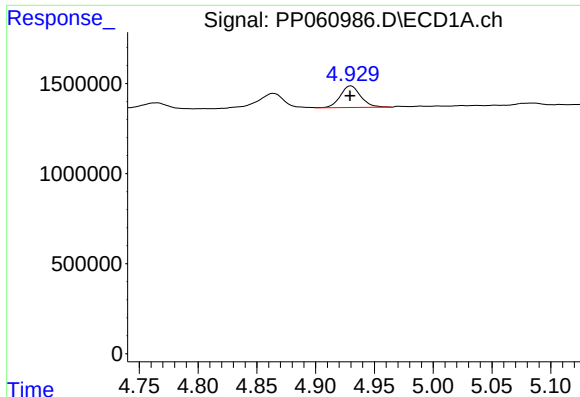

#11 AR-1232-1


R.T.: 4.930 min
Delta R.T.: 0.000 min
Response: 1454067
Conc: 28.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2023

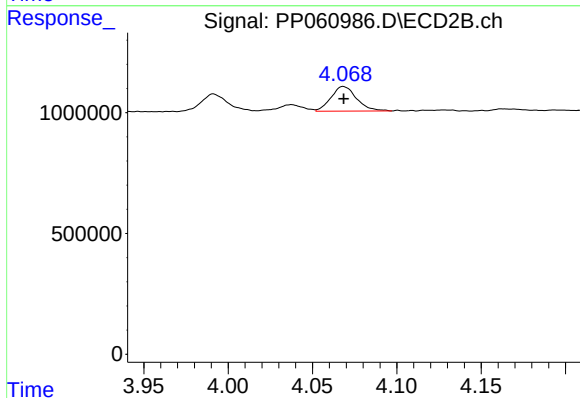


#11 AR-1232-1

R.T.: 4.068 min
Delta R.T.: 0.000 min
Response: 1078084
Conc: 31.22 ng/ml

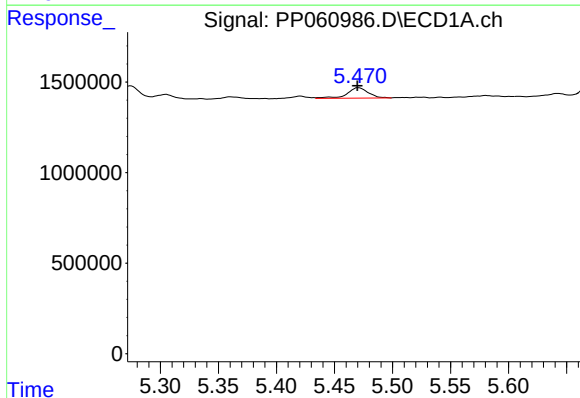


#12 AR-1232-2

R.T.: 5.471 min
Delta R.T.: 0.000 min
Response: 715421
Conc: 26.82 ng/ml

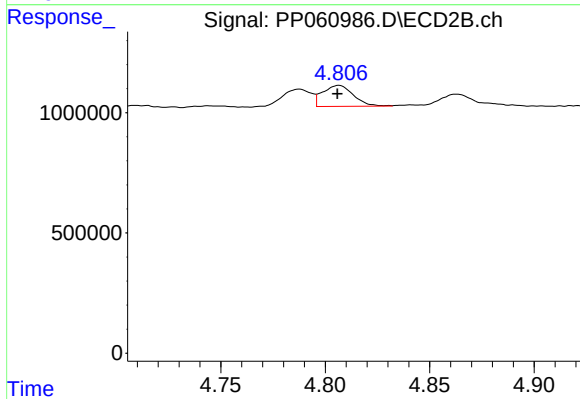

#12 AR-1232-2


R.T.: 4.807 min
Delta R.T.: 0.000 min
Response: 889952
Conc: 26.91 ng/ml

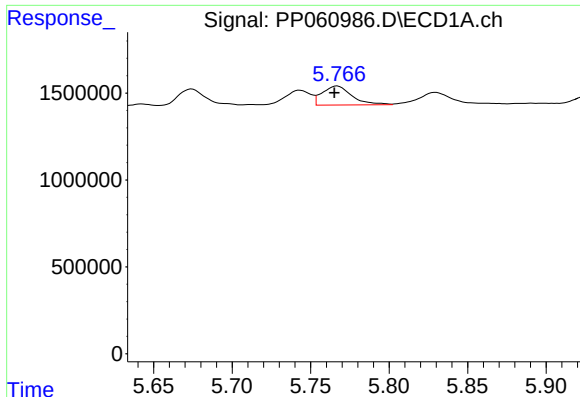

#13 AR-1232-3


R.T.: 5.767 min
Delta R.T.: 0.002 min
Response: 1445401
Conc: 30.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2023

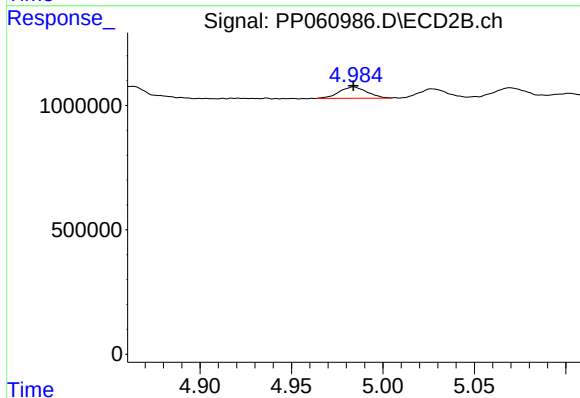


#13 AR-1232-3

R.T.: 4.984 min
Delta R.T.: 0.000 min
Response: 486114
Conc: 26.23 ng/ml

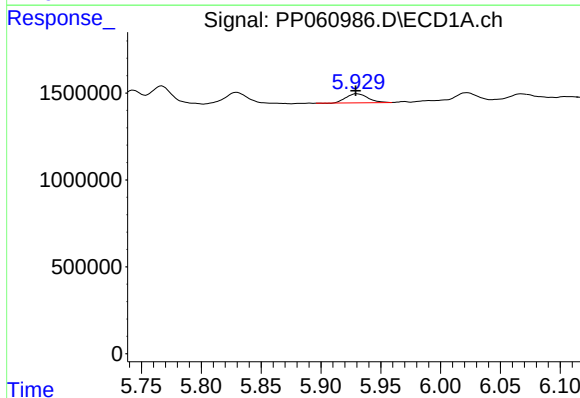


#14 AR-1232-4

R.T.: 5.930 min
Delta R.T.: 0.000 min
Response: 658108
Conc: 28.13 ng/ml

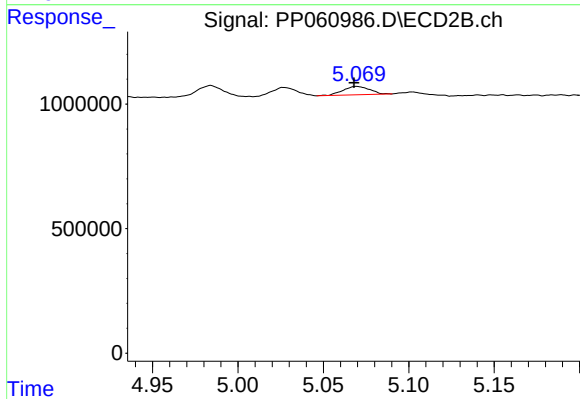

#14 AR-1232-4


R.T.: 5.070 min
Delta R.T.: 0.002 min
Response: 362400
Conc: 21.57 ng/ml

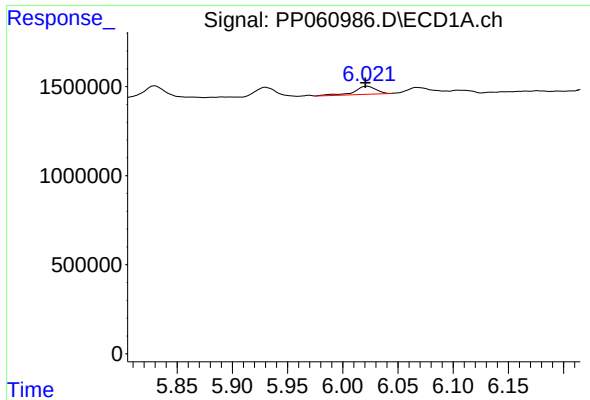

#15 AR-1232-5

R.T.: 6.022 min
Delta R.T.: 0.001 min
Response: 618285
Conc: 31.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2023

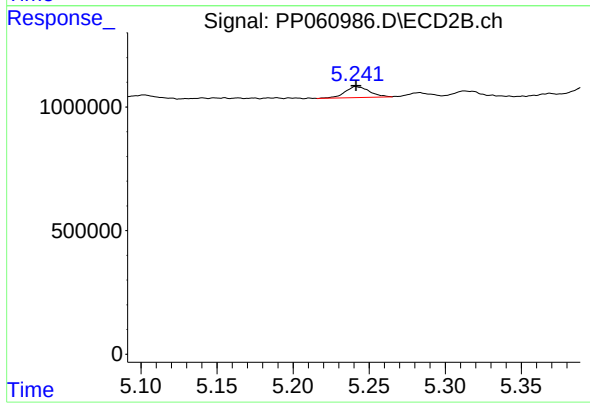

#15 AR-1232-5

R.T.: 5.241 min
Delta R.T.: 0.000 min
Response: 495420
Conc: 26.37 ng/ml