

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101325\
 Data File : PP075766.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2025 23:13
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 03:33:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 24 10:55:35 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.683f	3.794	326768	1564604	0.250	0.256
2)	SA Decachlor...	10.418	8.795	326757	1442290	0.328	0.239 #
Target Compounds							
3)	L1 AR-1016-1	0.000	4.893	0	2323033	N.D.	4.141 #
4)	L1 AR-1016-2	0.000	4.952	0	3202715	N.D.	12.462 #
5)	L1 AR-1016-3	0.000	5.074	0	7301196	N.D.	47.023 #
6)	L1 AR-1016-4	0.000	5.136	0	7280974	N.D.	49.541 #
7)	L1 AR-1016-5	6.297	5.335	1115816	9237264	33.089	56.538 #
8)	L2 AR-1221-1	0.000	4.004	0	1200308	N.D.	15.695 #
9)	L2 AR-1221-2	0.000	4.086	0	1512167	N.D.	28.934 #
10)	L2 AR-1221-3	5.078f	4.167	667930	892125	16.134	4.685 #
11)	L3 AR-1232-1	5.078f	4.167	667930	892125	20.798	6.087 #
12)	L3 AR-1232-2	5.499f	4.893	670317	2323033	39.960	9.211 #
13)	L3 AR-1232-3	0.000	5.074	0	7301196	N.D.	115.865 #
14)	L3 AR-1232-4	0.000	5.156	0	5646306	N.D.	54.732 #
15)	L3 AR-1232-5	6.063	5.335	585835	9237264	48.802	144.227 #
16)	L4 AR-1242-1	0.000	4.893	0	2323033	N.D.	4.973 #
17)	L4 AR-1242-2	0.000	4.952	0	3202715	N.D.	15.327 #
18)	L4 AR-1242-3	0.000	5.074	0	7301196	N.D.	59.864 #
19)	L4 AR-1242-4	6.063f	5.156	585835	5646306	18.637	35.491 #
20)	L4 AR-1242-5	0.000	5.653	0	8474649	N.D.	43.530 #
21)	L5 AR-1248-1	5.737f	4.893	3012180	2323033	95.444	7.731 #
22)	L5 AR-1248-2	6.063	5.136	585835	7280974	13.508	35.959 #
23)	L5 AR-1248-3	6.297	5.156	1115816	5646306	23.364	22.608
24)	L5 AR-1248-4	6.651	5.335	2500861	9237264	42.307	39.689
25)	L5 AR-1248-5	6.651f	5.755f	2500861	48391917	42.316	118.442 #
26)	L6 AR-1254-1	6.651	5.653	2500861	8474649	38.940	16.990 #
27)	L6 AR-1254-2	6.863	5.837	6144670	23459773	71.505	58.769
28)	L6 AR-1254-3	7.230	6.231	6891506	53636014	74.565	80.689
29)	L6 AR-1254-4	7.509	6.416f	1521485	13882698	21.324	28.123 #
30)	L6 AR-1254-5	7.947	6.858	618.0E6	4611.9E6	7553.984	8081.234
31)	L7 AR-1260-1	7.397	6.351	702432	9777254	11.684	24.086 #
32)	L7 AR-1260-2	7.632	6.537	805.4E6	8955954	11063.759	15.553 #
33)	L7 AR-1260-3	7.947f	0.000	618.0E6	0	11413.237	N.D. #
35)	L7 AR-1260-5	0.000	7.407	0	1860786	N.D.	1.769 #
36)	L8 AR-1262-1	8.212	6.858f	-50201	4611.9E6	N.D.	5829.608 #
37)	L8 AR-1262-2	0.000	7.162	0	381869	N.D.	0.691 #
38)	L8 AR-1262-3	8.862	7.688	92564	8918389	0.991	17.838 #
39)	L8 AR-1262-4	8.953	7.753	44051	8206539	0.610	9.037 #
40)	L8 AR-1262-5	9.660	8.240	2199631	7191182	42.191	16.727 #
41)	L9 AR-1268-1	8.862	7.688	92564	8918389	0.572	6.182 #
42)	L9 AR-1268-2	8.953	7.753	44051	8206539	0.297	5.884 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101325\
 Data File : PP075766.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2025 23:13
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 03:33:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 24 10:55:35 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	7.927	0	12076007	N.D.	11.070 #
44) L9	AR-1268-4	9.660	8.240	2199631	7191182	36.890	15.982 #
45) L9	AR-1268-5	10.086	8.541	1495492	3715195	3.852	1.223 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101325\
Data File : PP075766.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2025 23:13
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 03:33:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 24 10:55:35 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

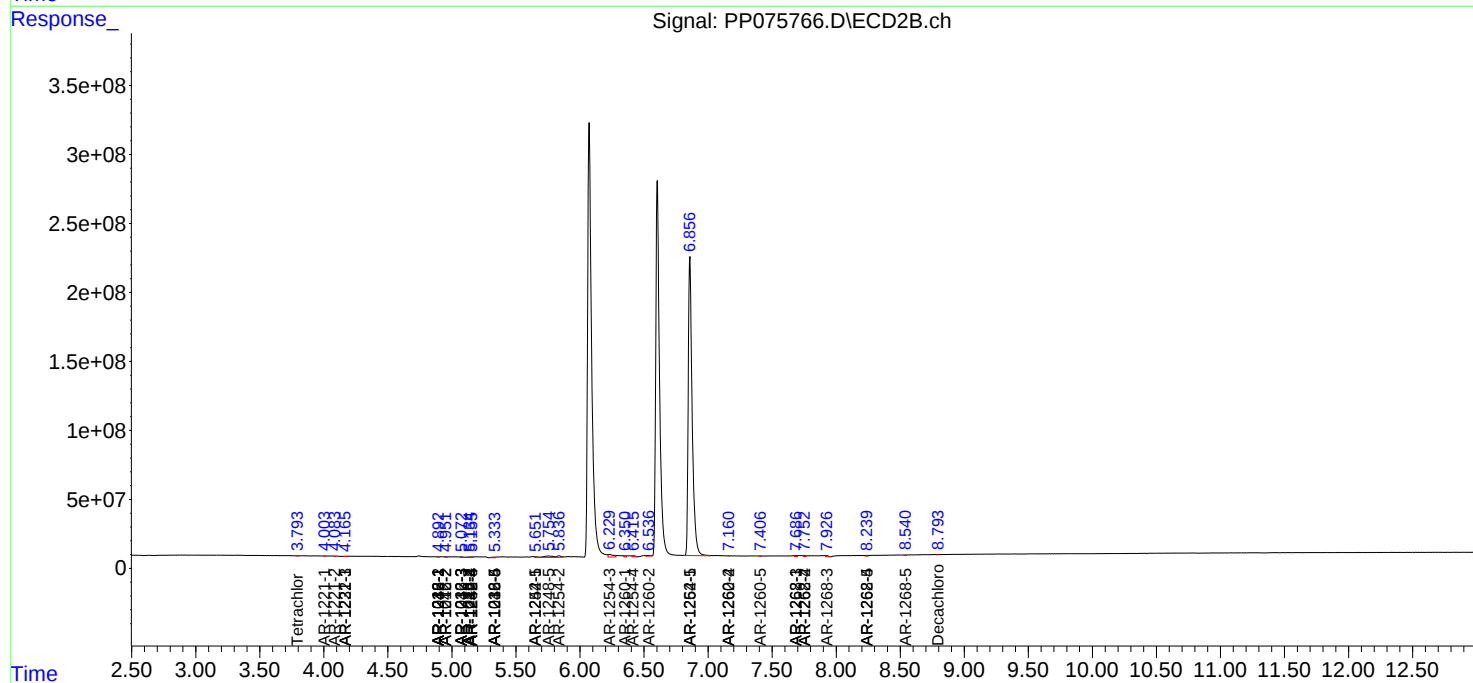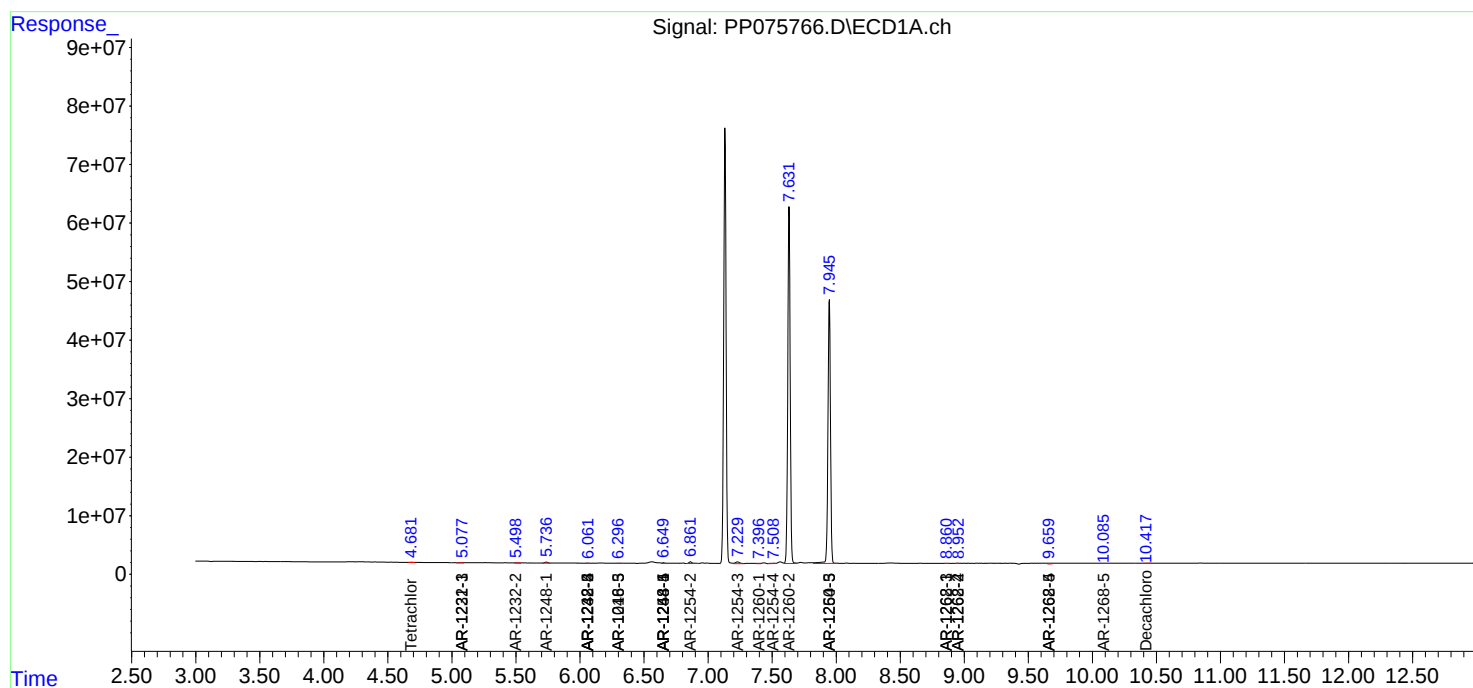


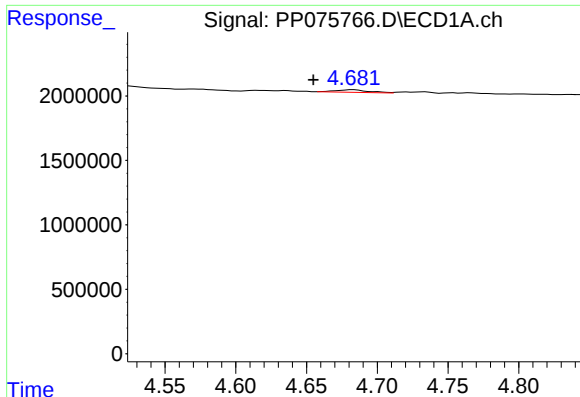

#1 Tetrachloro-m-xylene


R.T.: 4.683 min
Delta R.T.: 0.028 min
Response: 326768
Conc: 0.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

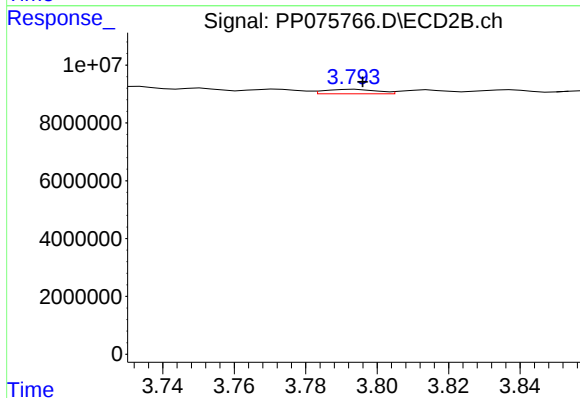


#1 Tetrachloro-m-xylene

R.T.: 3.794 min
Delta R.T.: -0.002 min
Response: 1564604
Conc: 0.26 ng/ml

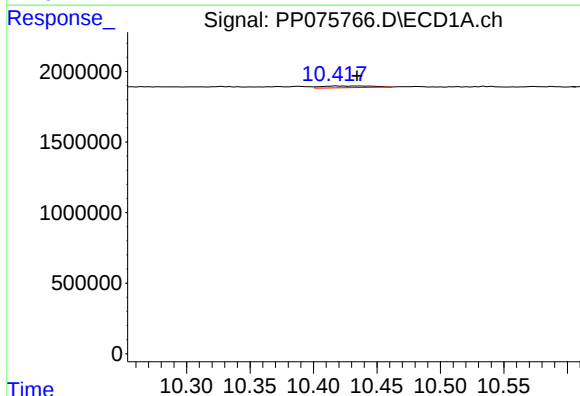


#2 Decachlorobiphenyl

R.T.: 10.418 min
Delta R.T.: -0.017 min
Response: 326757
Conc: 0.33 ng/ml

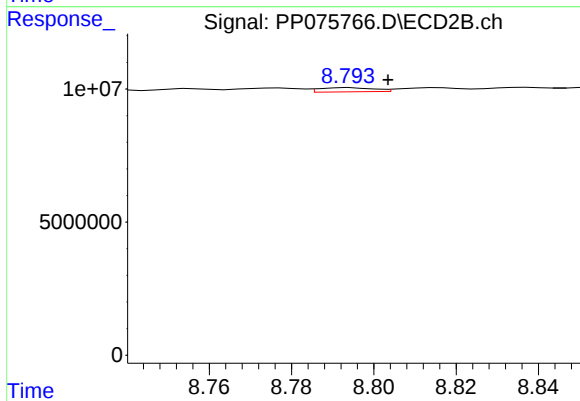

#2 Decachlorobiphenyl


R.T.: 8.795 min
Delta R.T.: -0.009 min
Response: 1442290
Conc: 0.24 ng/ml

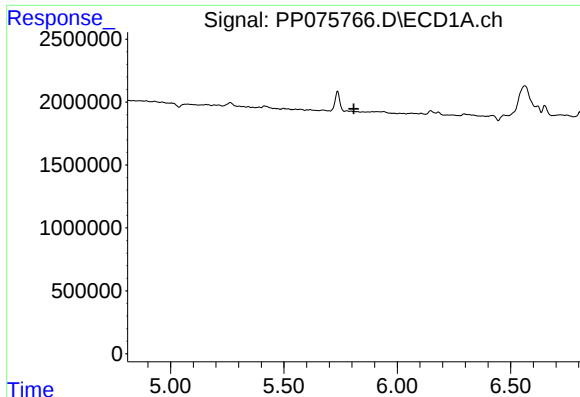

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.808 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

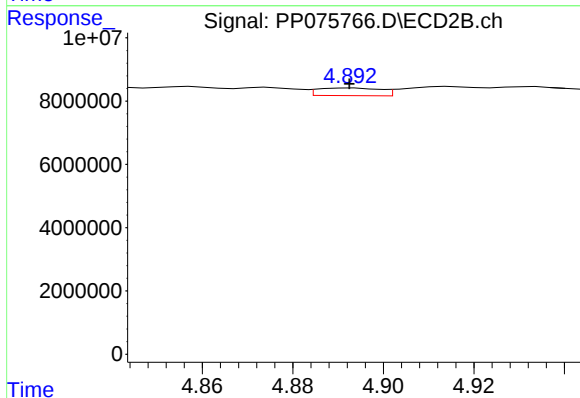


#3 AR-1016-1

R.T.: 4.893 min
Delta R.T.: 0.000 min
Response: 2323033
Conc: 4.14 ng/ml

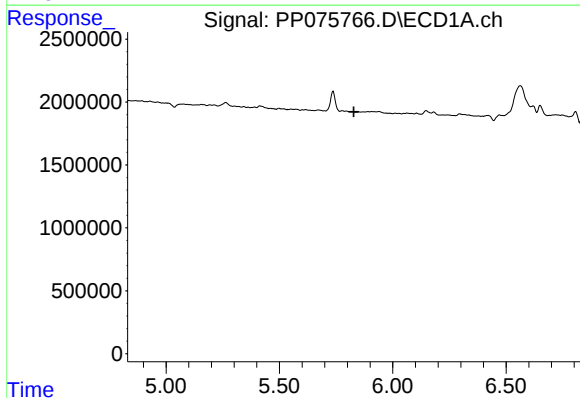


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.829 min
Response: 0
Conc: N.D.

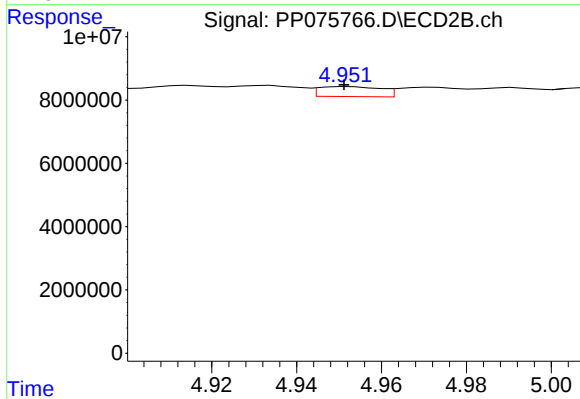

#4 AR-1016-2


R.T.: 4.952 min
Delta R.T.: 0.001 min
Response: 3202715
Conc: 12.46 ng/ml

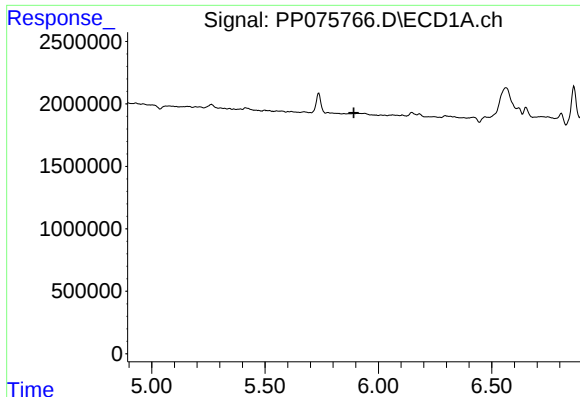

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.892 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

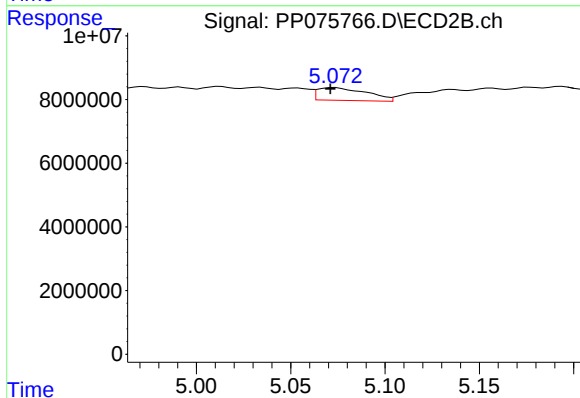


#5 AR-1016-3

R.T.: 5.074 min
Delta R.T.: 0.003 min
Response: 7301196
Conc: 47.02 ng/ml

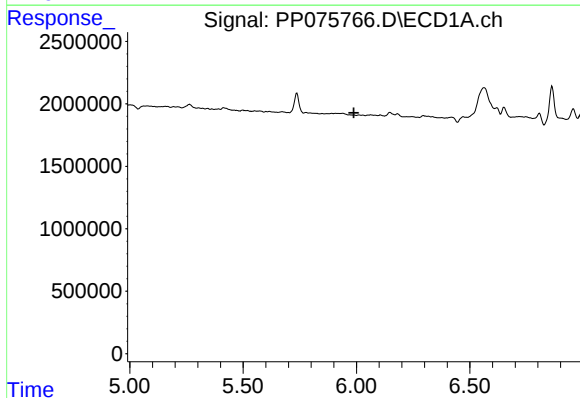


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.989 min
Response: 0
Conc: N.D.

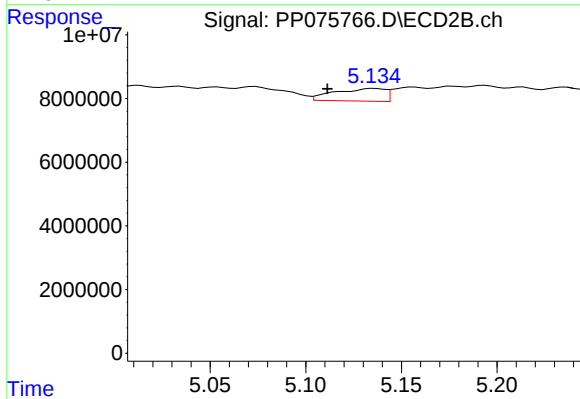

#6 AR-1016-4


R.T.: 5.136 min
Delta R.T.: 0.025 min
Response: 7280974
Conc: 49.54 ng/ml

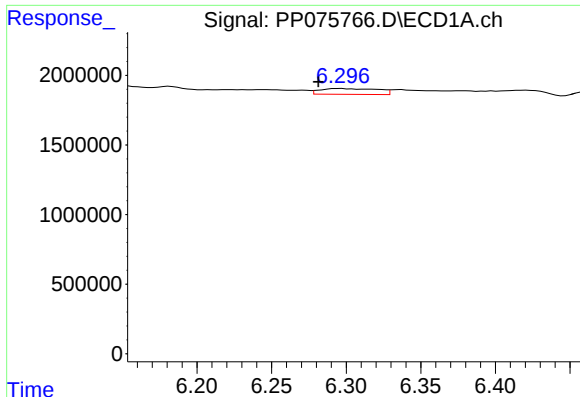

#7 AR-1016-5


R.T.: 6.297 min
Delta R.T.: 0.016 min
Response: 1115816
Conc: 33.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

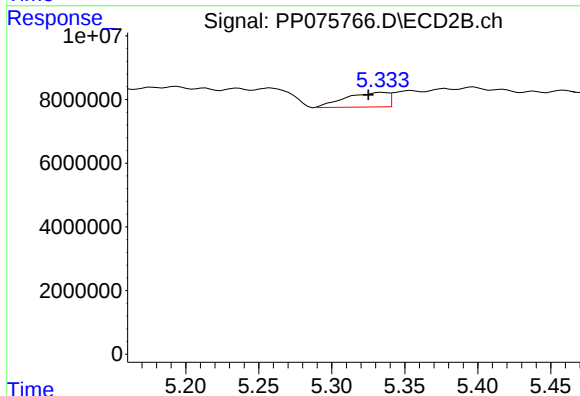


#7 AR-1016-5

R.T.: 5.335 min
Delta R.T.: 0.009 min
Response: 9237264
Conc: 56.54 ng/ml

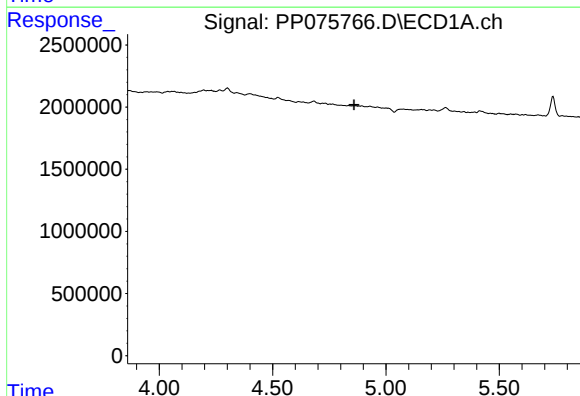


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.860 min
Response: 0
Conc: N.D.

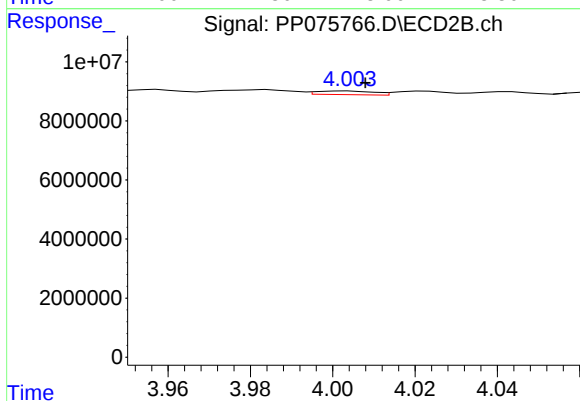

#8 AR-1221-1


R.T.: 4.004 min
Delta R.T.: -0.004 min
Response: 1200308
Conc: 15.69 ng/ml

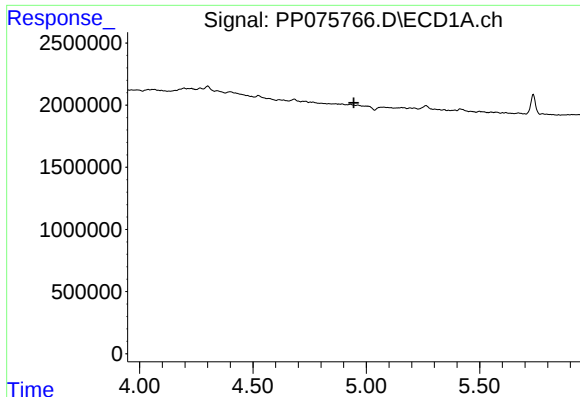

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.946 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

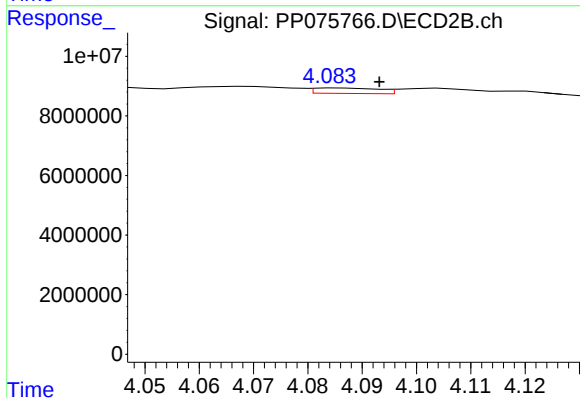


#9 AR-1221-2

R.T.: 4.086 min
Delta R.T.: -0.008 min
Response: 1512167
Conc: 28.93 ng/ml

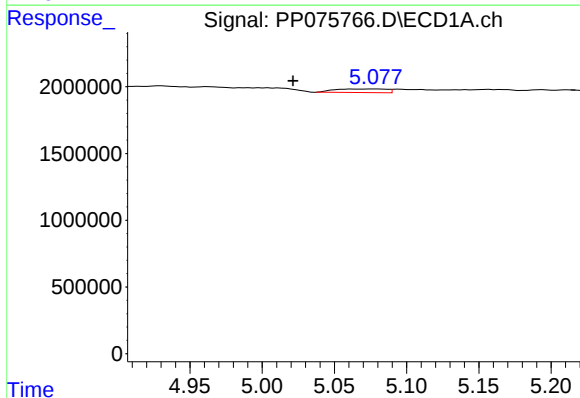


#10 AR-1221-3

R.T.: 5.078 min
Delta R.T.: 0.057 min
Response: 667930
Conc: 16.13 ng/ml

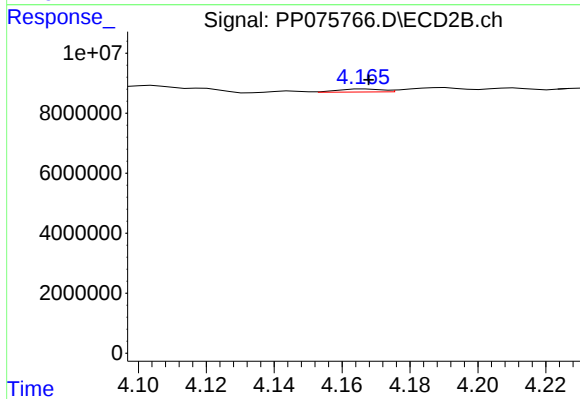

#10 AR-1221-3


R.T.: 4.167 min
Delta R.T.: 0.000 min
Response: 892125
Conc: 4.69 ng/ml

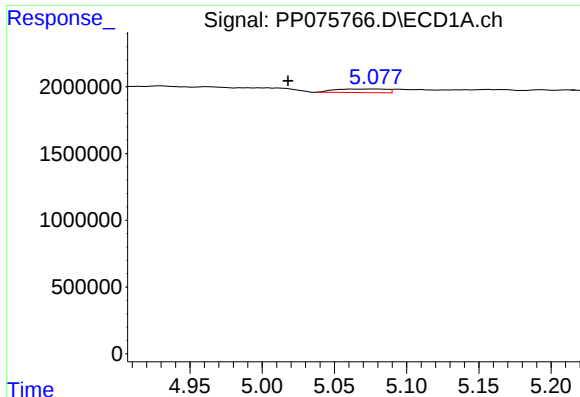

#11 AR-1232-1


R.T.: 5.078 min
Delta R.T.: 0.061 min
Response: 667930
Conc: 20.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

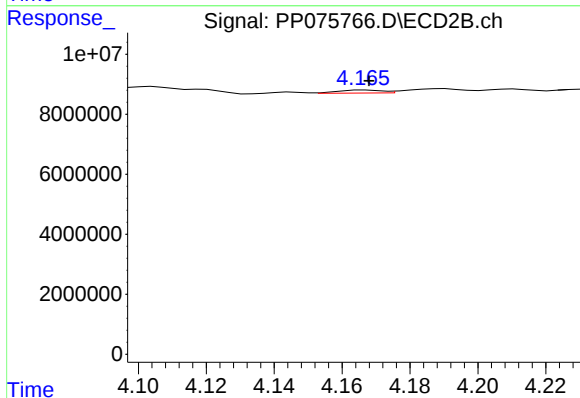


#11 AR-1232-1

R.T.: 4.167 min
Delta R.T.: -0.001 min
Response: 892125
Conc: 6.09 ng/ml

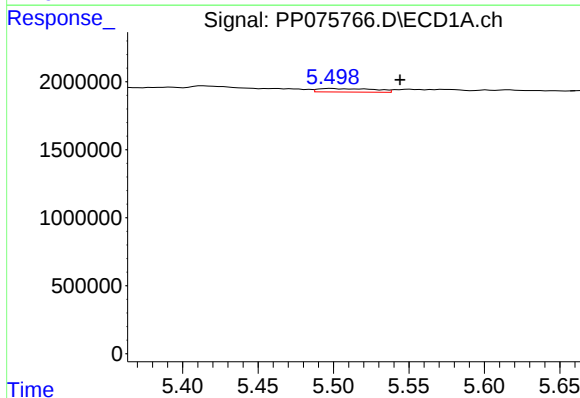


#12 AR-1232-2

R.T.: 5.499 min
Delta R.T.: -0.045 min
Response: 670317
Conc: 39.96 ng/ml

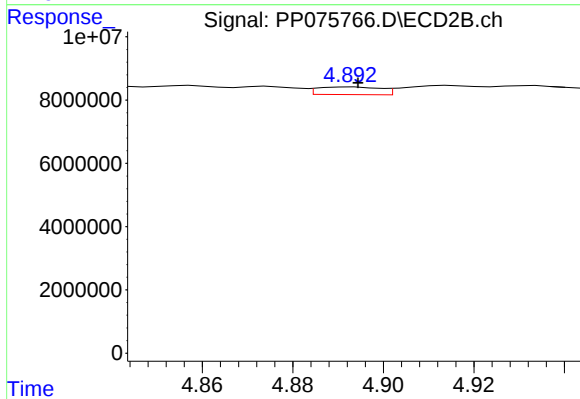

#12 AR-1232-2


R.T.: 4.893 min
Delta R.T.: -0.001 min
Response: 2323033
Conc: 9.21 ng/ml

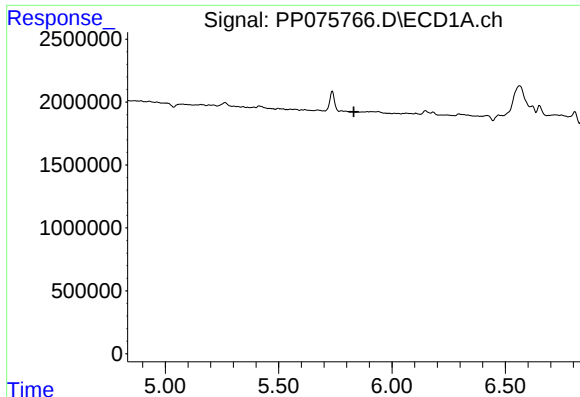

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.831 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

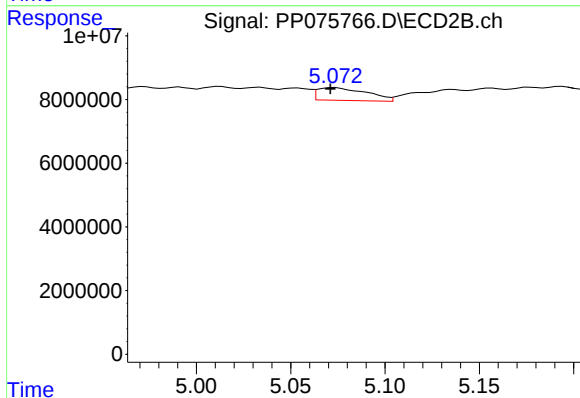


#13 AR-1232-3

R.T.: 5.074 min
Delta R.T.: 0.002 min
Response: 7301196
Conc: 115.86 ng/ml

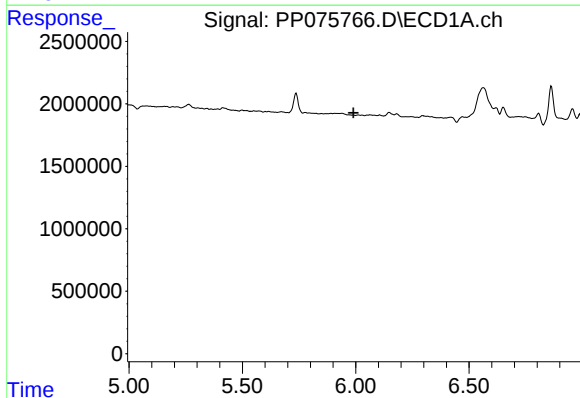


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.990 min
Response: 0
Conc: N.D.

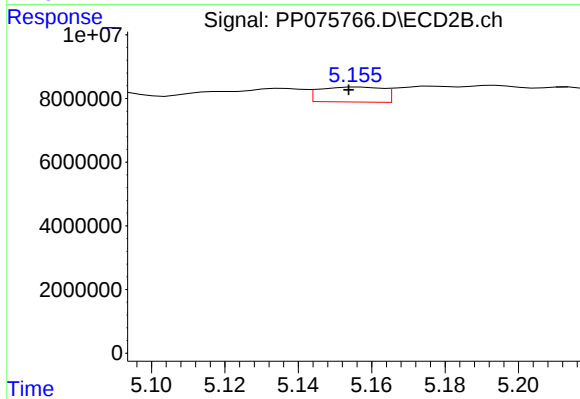

#14 AR-1232-4


R.T.: 5.156 min
Delta R.T.: 0.003 min
Response: 5646306
Conc: 54.73 ng/ml

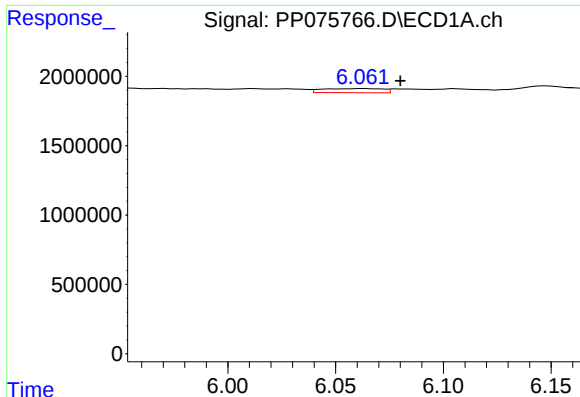

#15 AR-1232-5


R.T.: 6.063 min
Delta R.T.: -0.017 min
Response: 585835
Conc: 48.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

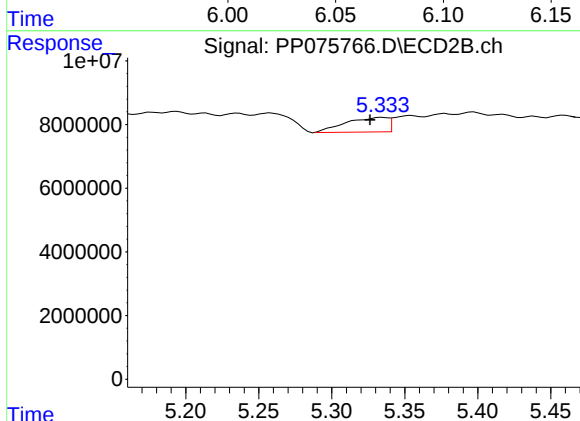


#15 AR-1232-5

R.T.: 5.335 min
Delta R.T.: 0.008 min
Response: 9237264
Conc: 144.23 ng/ml

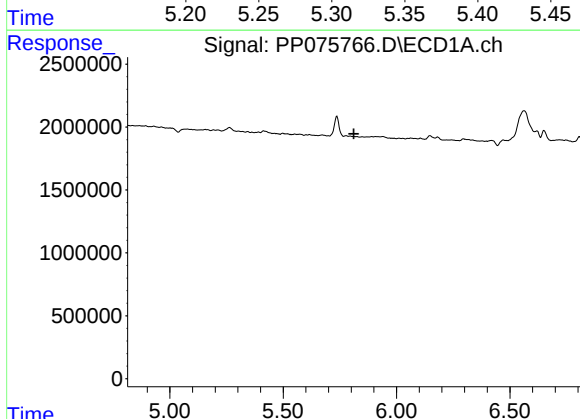


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 5.812 min
Response: 0
Conc: N.D.

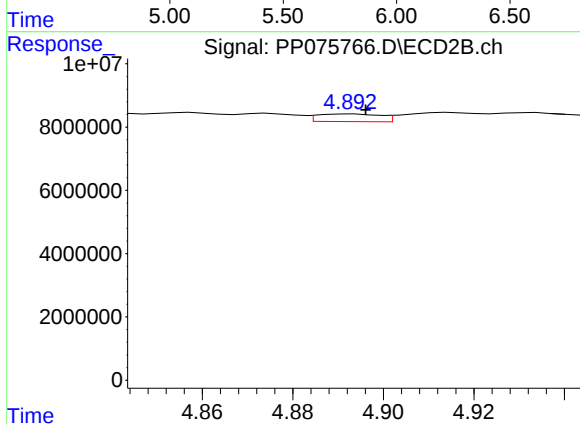

#16 AR-1242-1


R.T.: 4.893 min
Delta R.T.: -0.003 min
Response: 2323033
Conc: 4.97 ng/ml

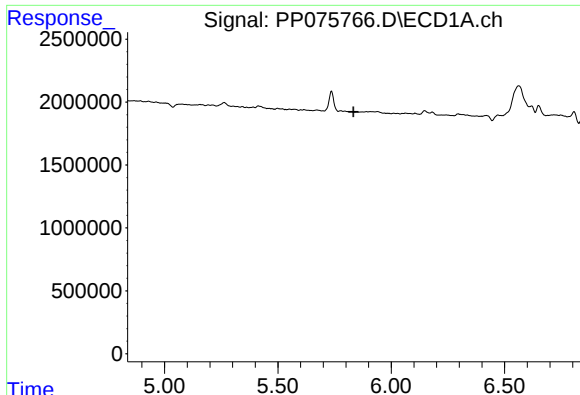

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.834 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

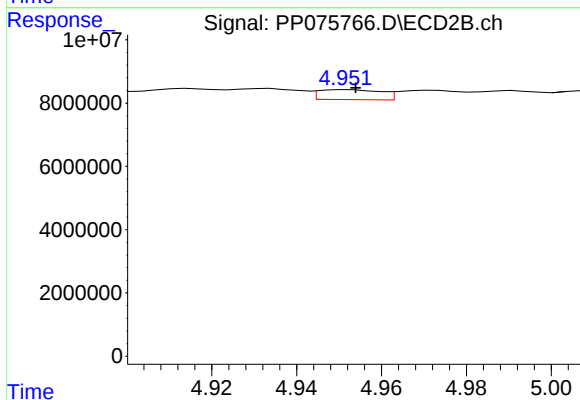


#17 AR-1242-2

R.T.: 4.952 min
Delta R.T.: -0.002 min
Response: 3202715
Conc: 15.33 ng/ml

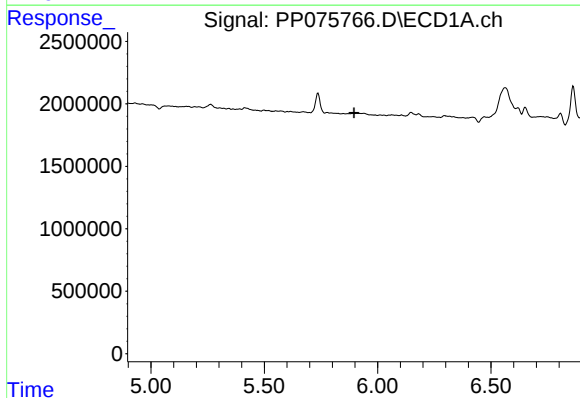


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.896 min
Response: 0
Conc: N.D.

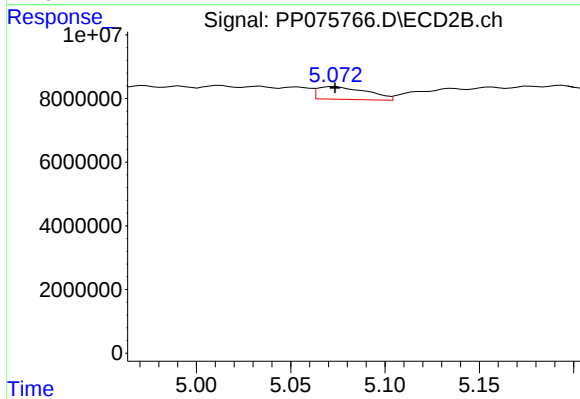

#18 AR-1242-3


R.T.: 5.074 min
Delta R.T.: 0.000 min
Response: 7301196
Conc: 59.86 ng/ml

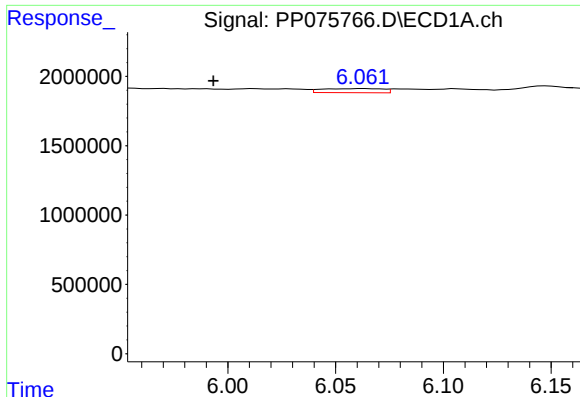

#19 AR-1242-4


R.T.: 6.063 min
Delta R.T.: 0.070 min
Response: 585835
Conc: 18.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

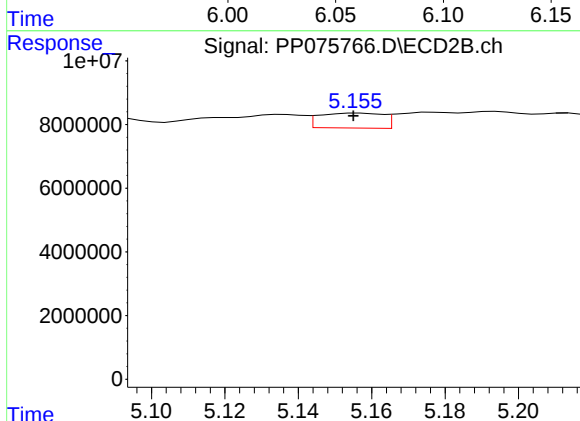


#19 AR-1242-4

R.T.: 5.156 min
Delta R.T.: 0.001 min
Response: 5646306
Conc: 35.49 ng/ml

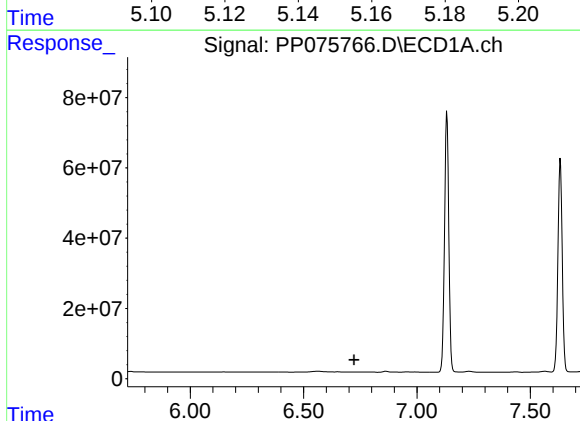


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.723 min
Response: 0
Conc: N.D.

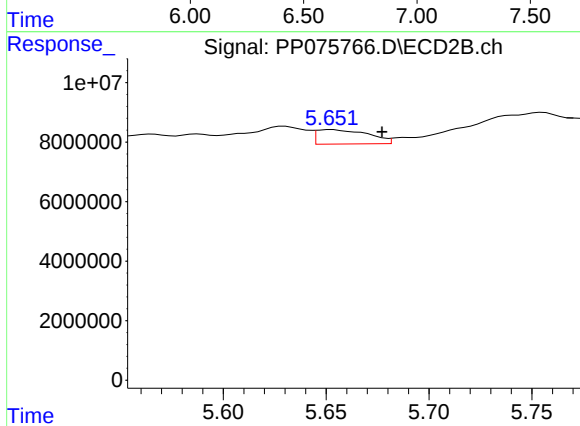

#20 AR-1242-5


R.T.: 5.653 min
Delta R.T.: -0.025 min
Response: 8474649
Conc: 43.53 ng/ml

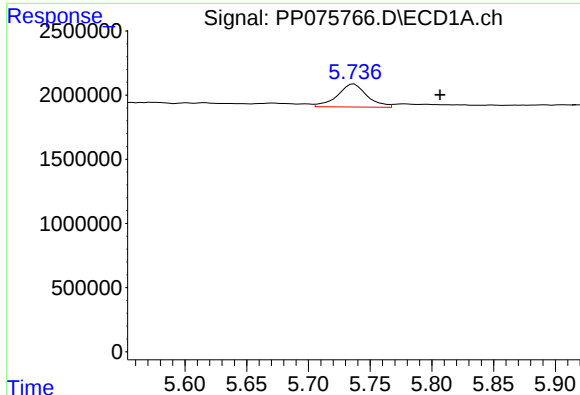

#21 AR-1248-1


R.T.: 5.737 min
Delta R.T.: -0.070 min
Response: 3012180
Conc: 95.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

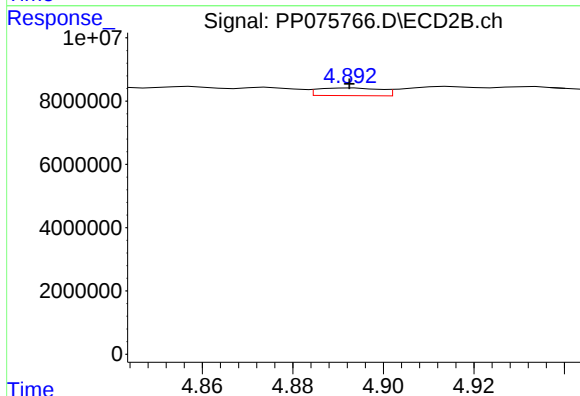


#21 AR-1248-1

R.T.: 4.893 min
Delta R.T.: 0.000 min
Response: 2323033
Conc: 7.73 ng/ml

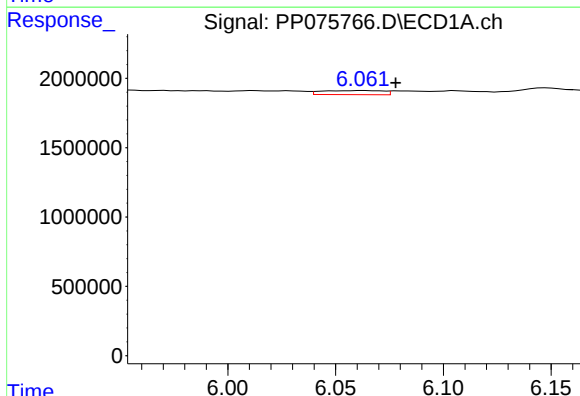


#22 AR-1248-2

R.T.: 6.063 min
Delta R.T.: -0.015 min
Response: 585835
Conc: 13.51 ng/ml

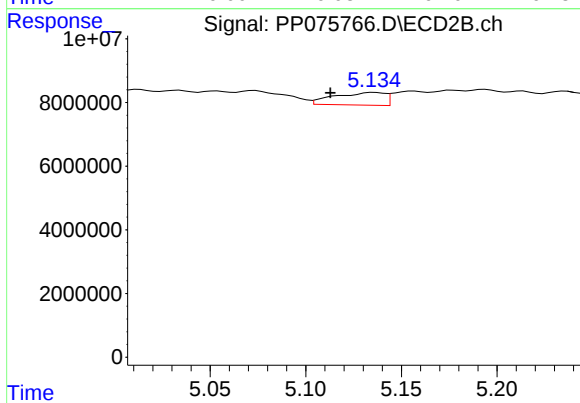

#22 AR-1248-2


R.T.: 5.136 min
Delta R.T.: 0.023 min
Response: 7280974
Conc: 35.96 ng/ml

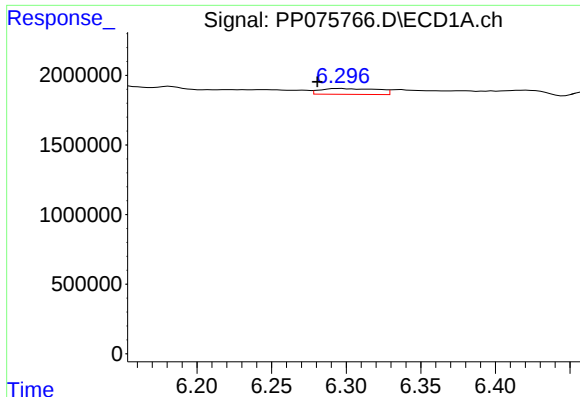

#23 AR-1248-3


R.T.: 6.297 min
Delta R.T.: 0.016 min
Response: 1115816
Conc: 23.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

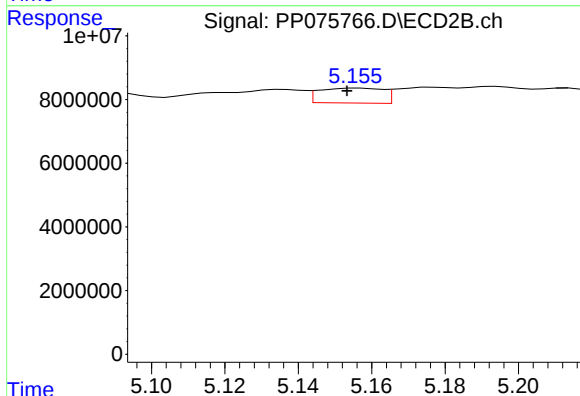


#23 AR-1248-3

R.T.: 5.156 min
Delta R.T.: 0.003 min
Response: 5646306
Conc: 22.61 ng/ml

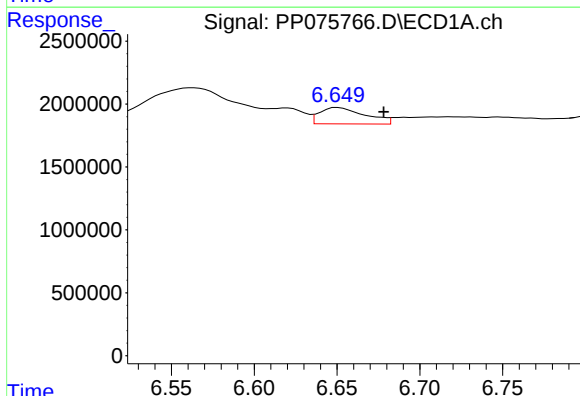


#24 AR-1248-4

R.T.: 6.651 min
Delta R.T.: -0.028 min
Response: 2500861
Conc: 42.31 ng/ml

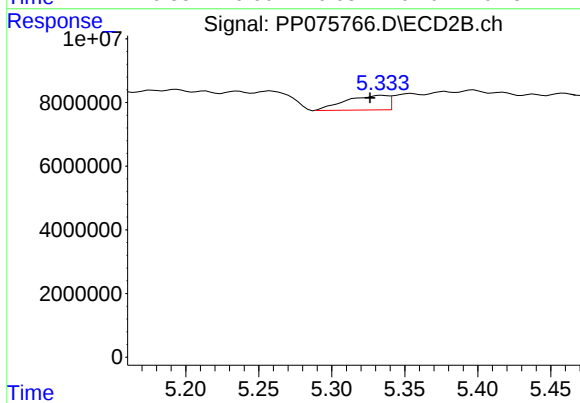

#24 AR-1248-4


R.T.: 5.335 min
Delta R.T.: 0.008 min
Response: 9237264
Conc: 39.69 ng/ml

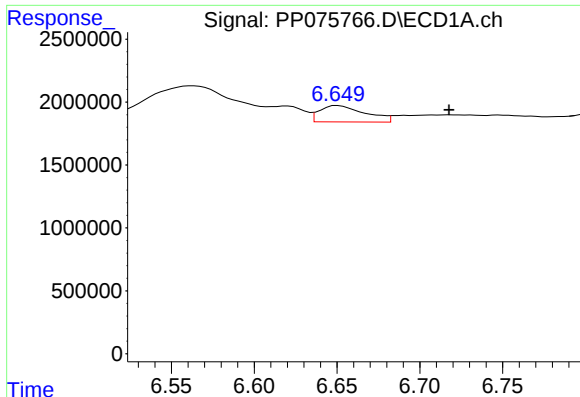

#25 AR-1248-5


R.T.: 6.651 min
Delta R.T.: -0.067 min
Response: 2500861
Conc: 42.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

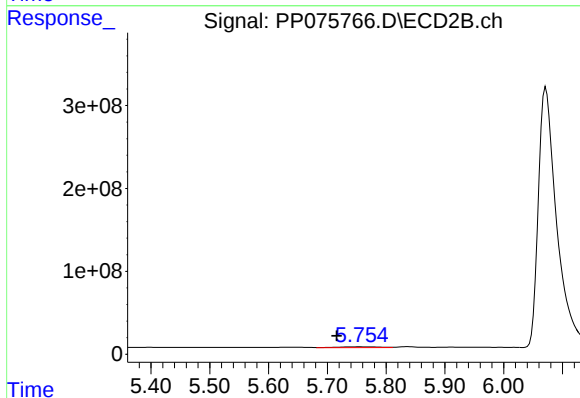


#25 AR-1248-5

R.T.: 5.755 min
Delta R.T.: 0.040 min
Response: 48391917
Conc: 118.44 ng/ml

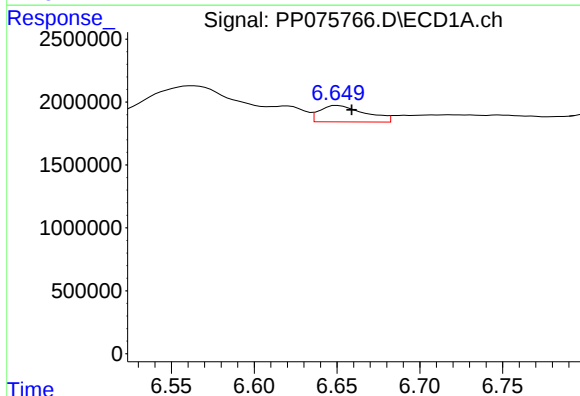


#26 AR-1254-1

R.T.: 6.651 min
Delta R.T.: -0.008 min
Response: 2500861
Conc: 38.94 ng/ml

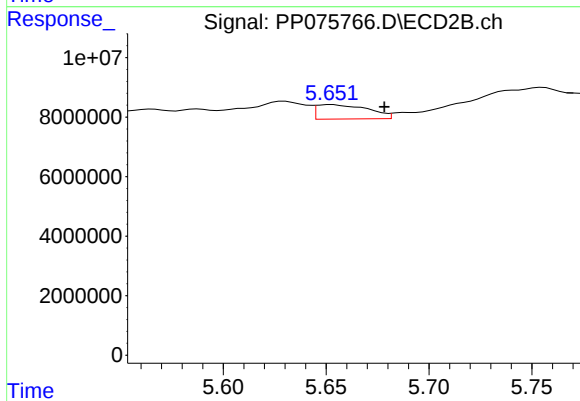

#26 AR-1254-1


R.T.: 5.653 min
Delta R.T.: -0.026 min
Response: 8474649
Conc: 16.99 ng/ml

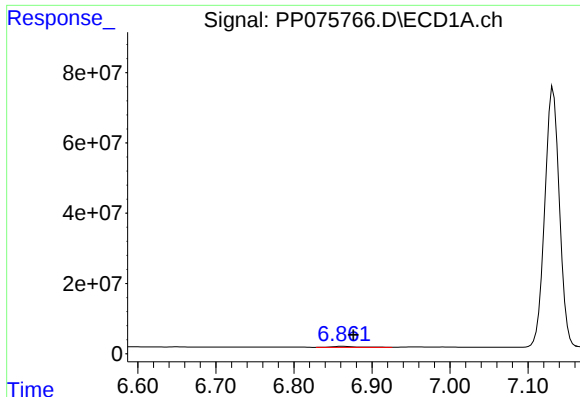

#27 AR-1254-2


R.T.: 6.863 min
Delta R.T.: -0.013 min
Response: 6144670
Conc: 71.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

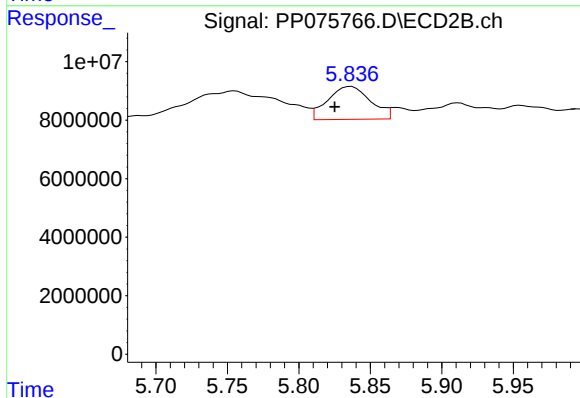


#27 AR-1254-2

R.T.: 5.837 min
Delta R.T.: 0.011 min
Response: 23459773
Conc: 58.77 ng/ml

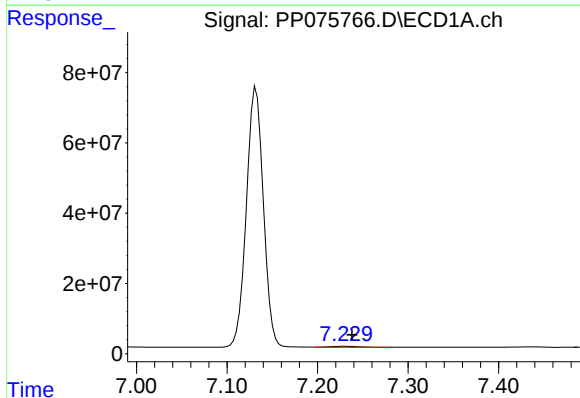


#28 AR-1254-3

R.T.: 7.230 min
Delta R.T.: -0.008 min
Response: 6891506
Conc: 74.57 ng/ml

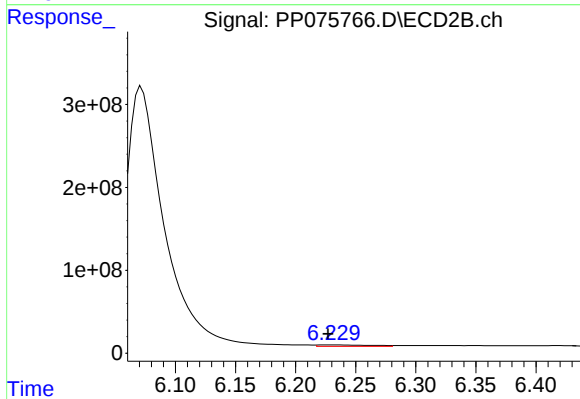

#28 AR-1254-3


R.T.: 6.231 min
Delta R.T.: 0.004 min
Response: 53636014
Conc: 80.69 ng/ml

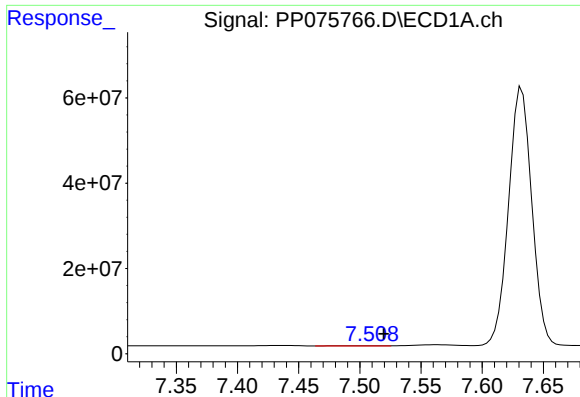

#29 AR-1254-4


R.T.: 7.509 min
Delta R.T.: -0.010 min
Response: 1521485
Conc: 21.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

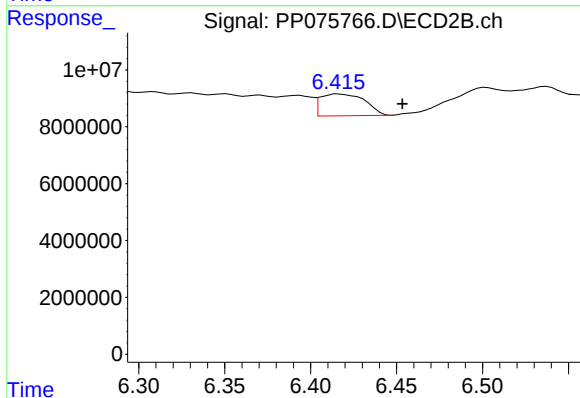


#29 AR-1254-4

R.T.: 6.416 min
Delta R.T.: -0.037 min
Response: 13882698
Conc: 28.12 ng/ml

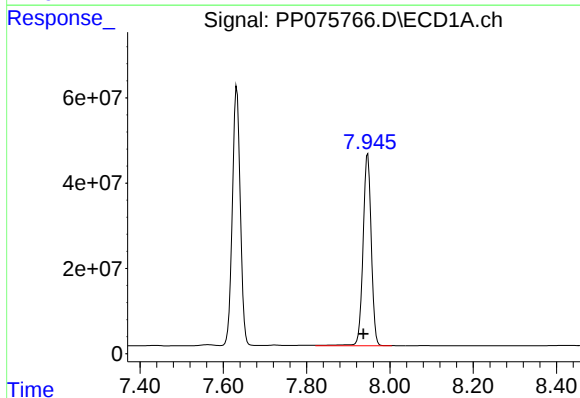


#30 AR-1254-5

R.T.: 7.947 min
Delta R.T.: 0.011 min
Response: 617971282
Conc: 7553.98 ng/ml

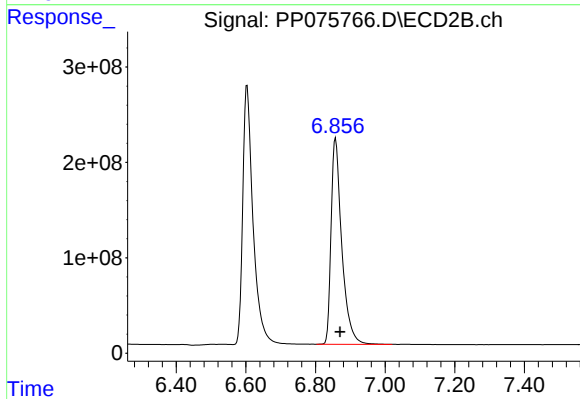

#30 AR-1254-5


R.T.: 6.858 min
Delta R.T.: -0.013 min
Response: 4611901519
Conc: 8081.23 ng/ml

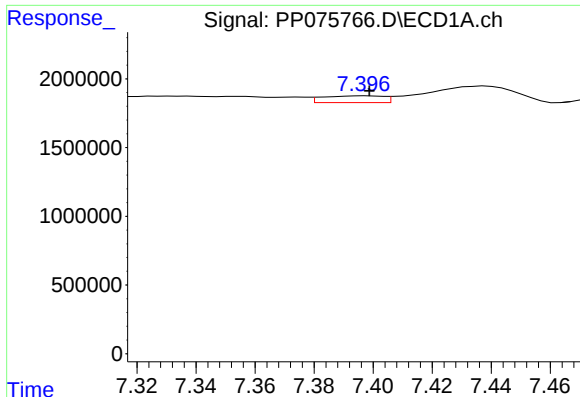

#31 AR-1260-1


R.T.: 7.397 min
Delta R.T.: -0.002 min
Response: 702432
Conc: 11.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

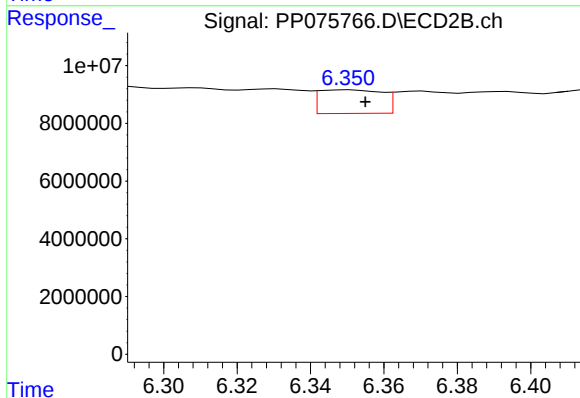


#31 AR-1260-1

R.T.: 6.351 min
Delta R.T.: -0.004 min
Response: 9777254
Conc: 24.09 ng/ml

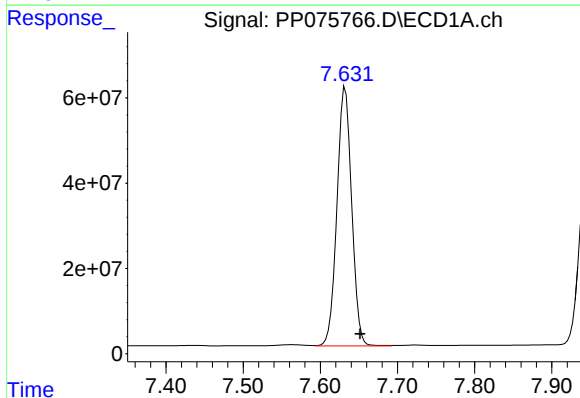


#32 AR-1260-2

R.T.: 7.632 min
Delta R.T.: -0.019 min
Response: 805419575
Conc: 11063.76 ng/ml

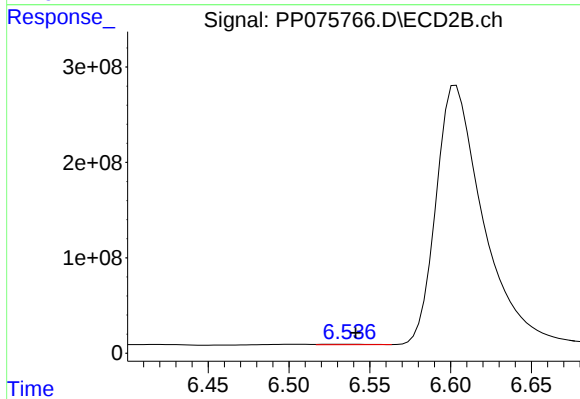

#32 AR-1260-2


R.T.: 6.537 min
Delta R.T.: -0.004 min
Response: 8955954
Conc: 15.55 ng/ml

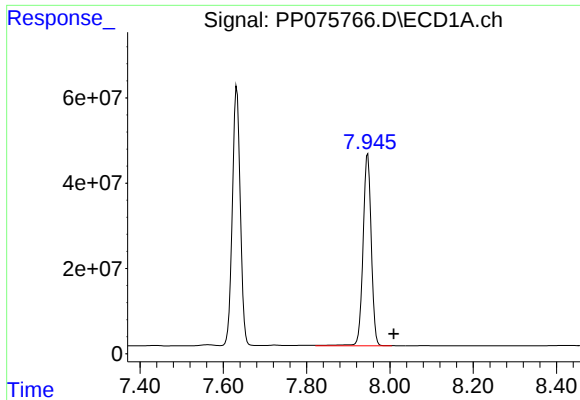

#33 AR-1260-3


R.T.: 7.947 min
Delta R.T.: -0.062 min
Response: 617971282
Conc: 11413.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

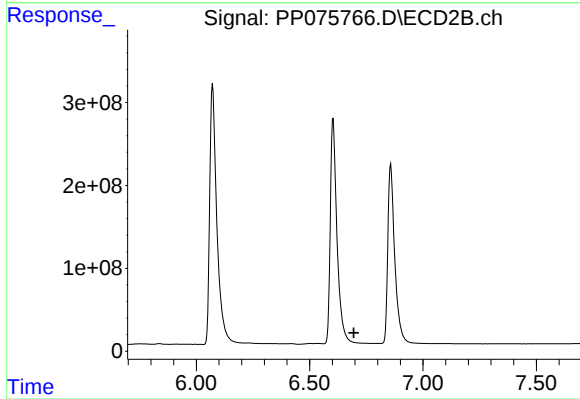


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.695 min
Response: 0
Conc: N.D.

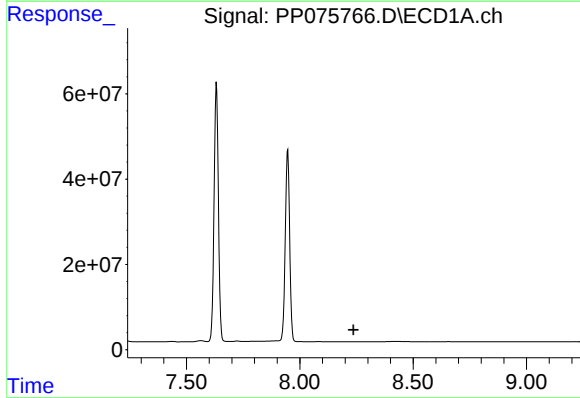


#34 AR-1260-4

R.T.: 8.212 min
Delta R.T.: -0.025 min
Response: -50201
Conc: N.D.

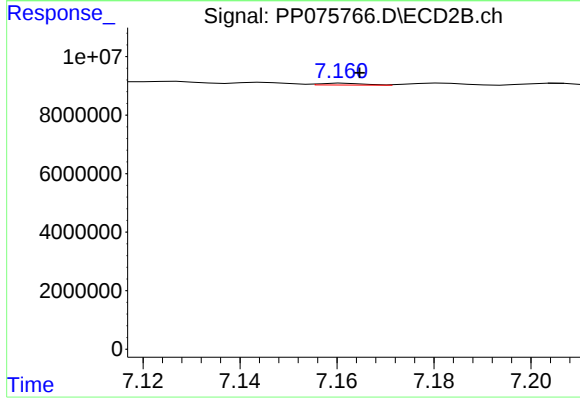

#34 AR-1260-4


R.T.: 7.162 min
Delta R.T.: -0.003 min
Response: 381869
Conc: 0.89 ng/ml

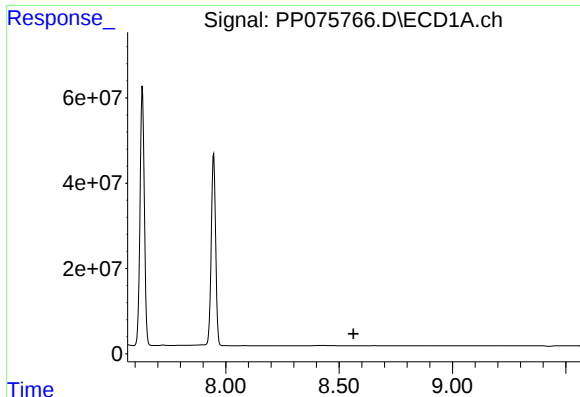

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

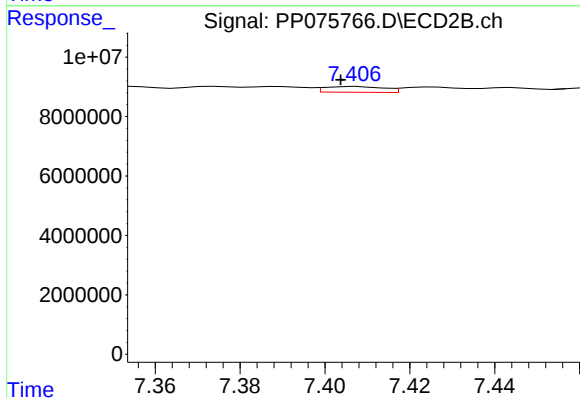


#35 AR-1260-5

R.T.: 7.407 min
Delta R.T.: 0.004 min
Response: 1860786
Conc: 1.77 ng/ml

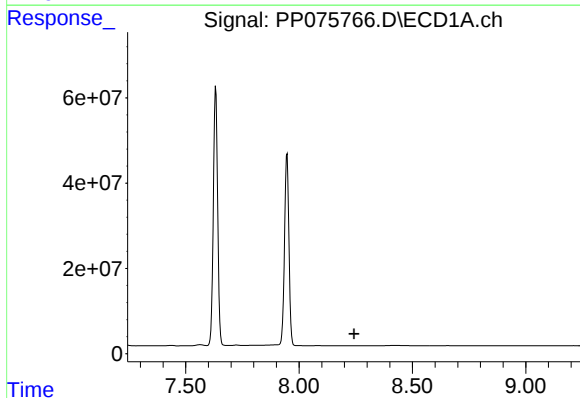


#36 AR-1262-1

R.T.: 8.212 min
Delta R.T.: -0.031 min
Response: -50201
Conc: N.D.

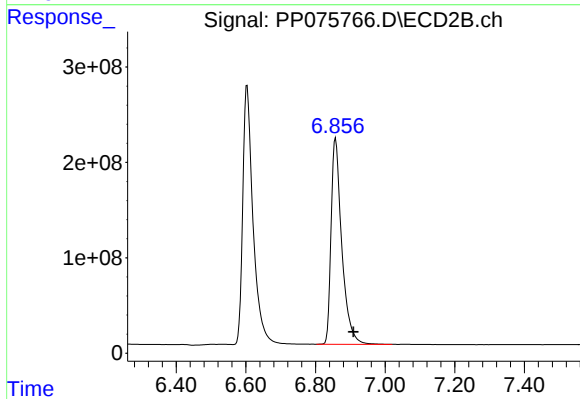

#36 AR-1262-1


R.T.: 6.858 min
Delta R.T.: -0.052 min
Response: 4611901519
Conc: 5829.61 ng/ml

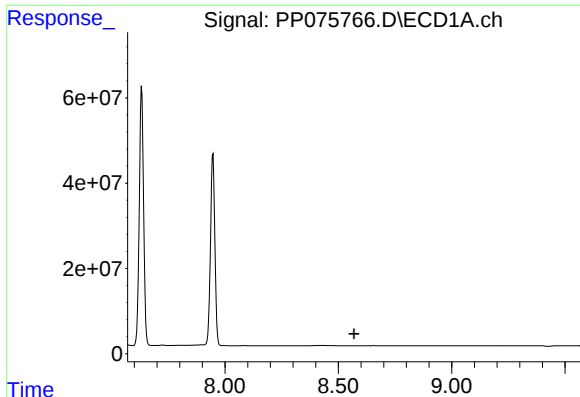

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

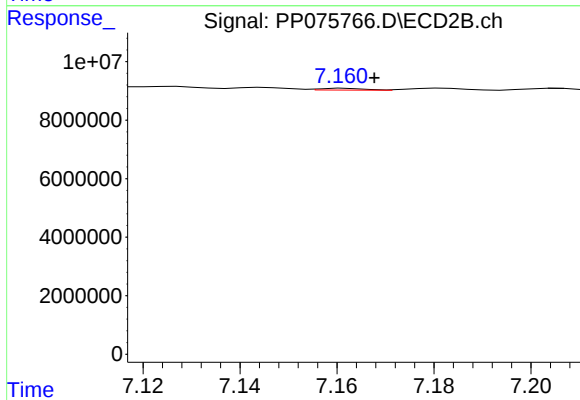


#37 AR-1262-2

R.T.: 7.162 min
Delta R.T.: -0.006 min
Response: 381869
Conc: 0.69 ng/ml

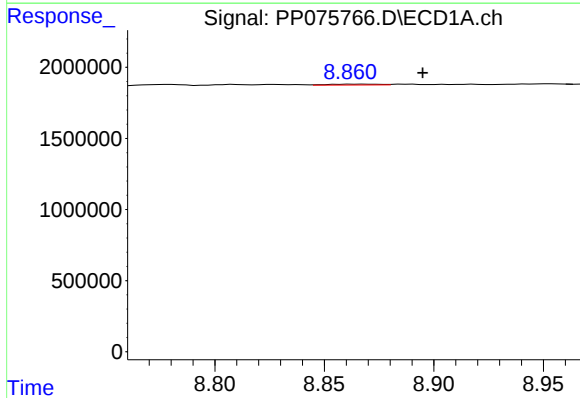


#38 AR-1262-3

R.T.: 8.862 min
Delta R.T.: -0.033 min
Response: 92564
Conc: 0.99 ng/ml

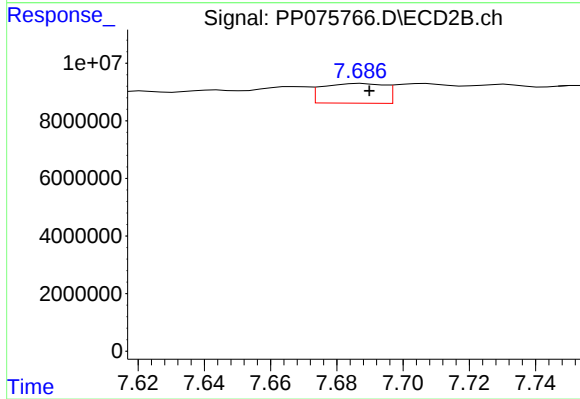

#38 AR-1262-3


R.T.: 7.688 min
Delta R.T.: -0.002 min
Response: 8918389
Conc: 17.84 ng/ml

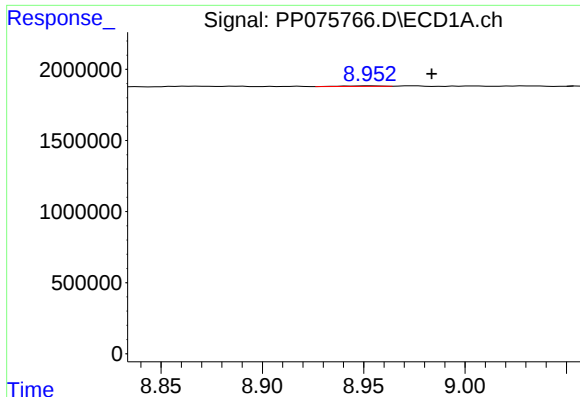

#39 AR-1262-4


R.T.: 8.953 min
Delta R.T.: -0.031 min
Response: 44051
Conc: 0.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

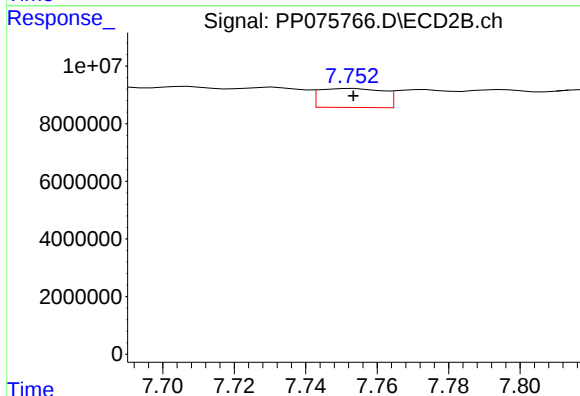


#39 AR-1262-4

R.T.: 7.753 min
Delta R.T.: 0.000 min
Response: 8206539
Conc: 9.04 ng/ml

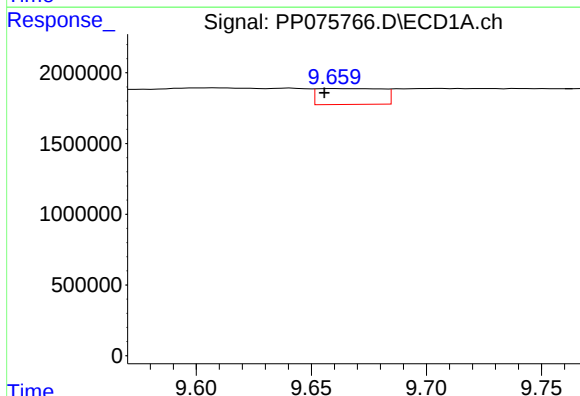


#40 AR-1262-5

R.T.: 9.660 min
Delta R.T.: 0.004 min
Response: 2199631
Conc: 42.19 ng/ml

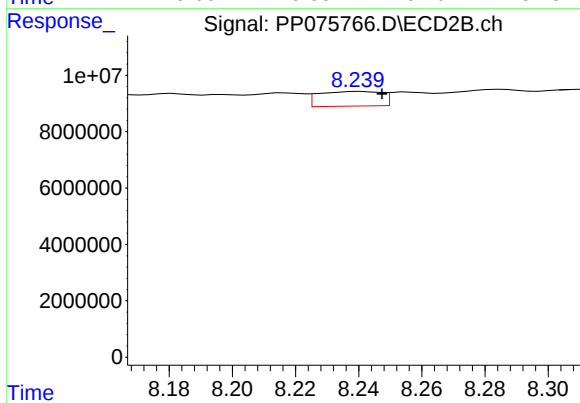

#40 AR-1262-5


R.T.: 8.240 min
Delta R.T.: -0.007 min
Response: 7191182
Conc: 16.73 ng/ml

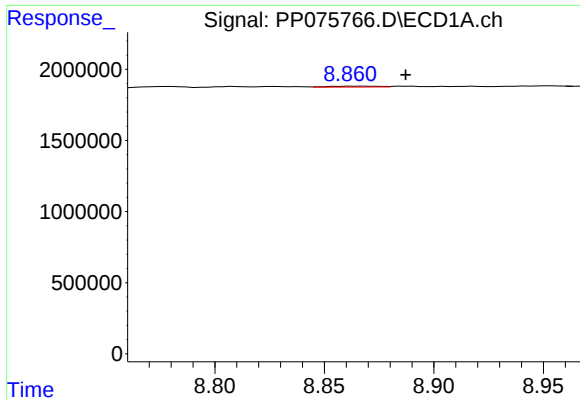

#41 AR-1268-1


R.T.: 8.862 min
Delta R.T.: -0.025 min
Response: 92564
Conc: 0.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

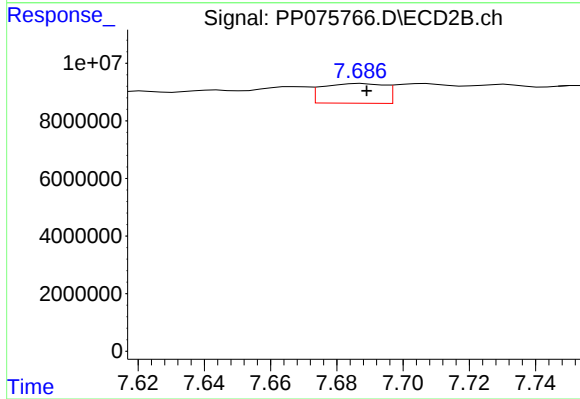


#41 AR-1268-1

R.T.: 7.688 min
Delta R.T.: -0.001 min
Response: 8918389
Conc: 6.18 ng/ml

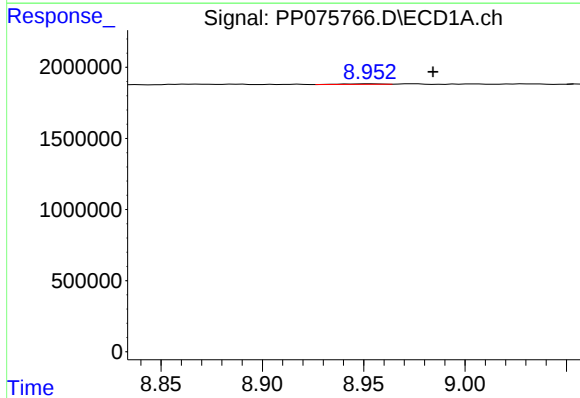


#42 AR-1268-2

R.T.: 8.953 min
Delta R.T.: -0.031 min
Response: 44051
Conc: 0.30 ng/ml

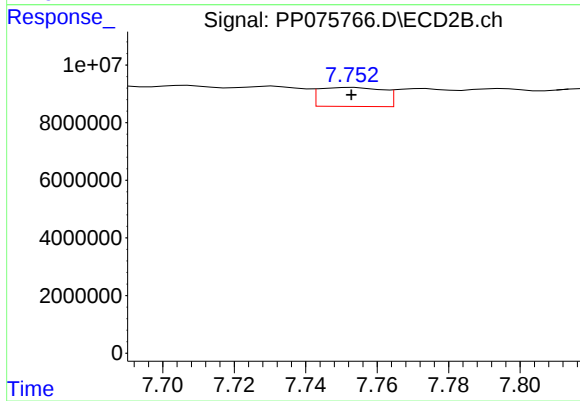

#42 AR-1268-2


R.T.: 7.753 min
Delta R.T.: 0.000 min
Response: 8206539
Conc: 5.88 ng/ml

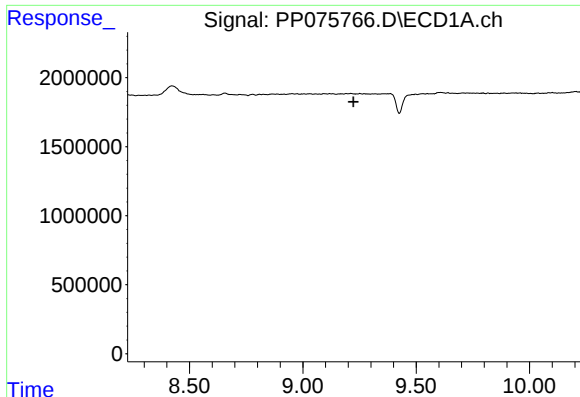

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.224 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

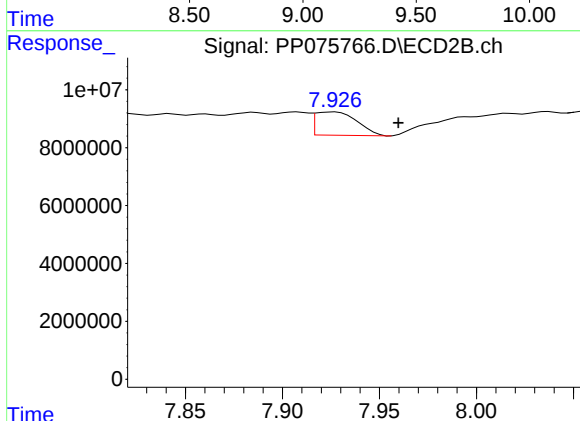


#43 AR-1268-3

R.T.: 7.927 min
Delta R.T.: -0.033 min
Response: 12076007
Conc: 11.07 ng/ml

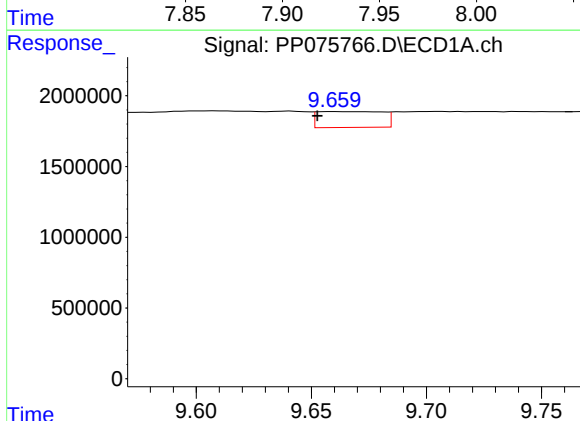


#44 AR-1268-4

R.T.: 9.660 min
Delta R.T.: 0.007 min
Response: 2199631
Conc: 36.89 ng/ml

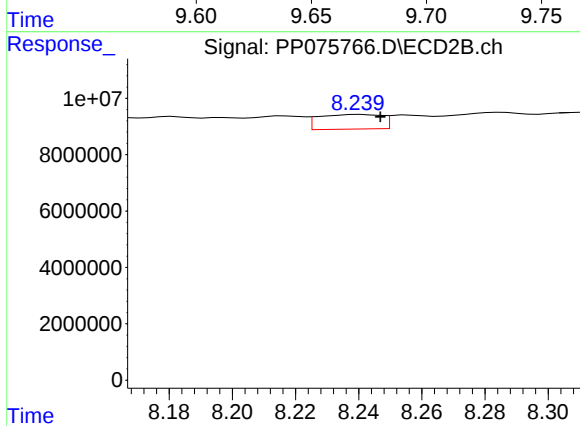

#44 AR-1268-4


R.T.: 8.240 min
Delta R.T.: -0.007 min
Response: 7191182
Conc: 15.98 ng/ml

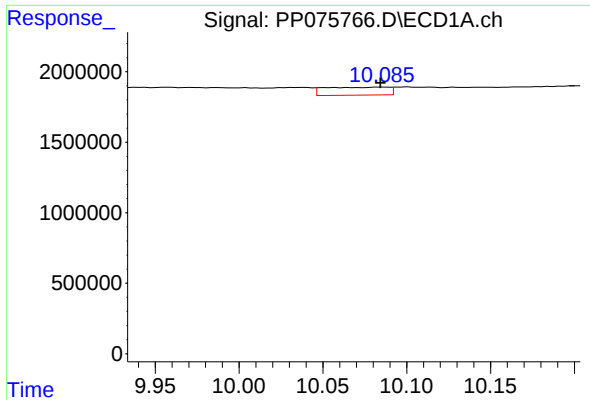

#45 AR-1268-5

R.T.: 10.086 min
Delta R.T.: 0.001 min
Response: 1495492
Conc: 3.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

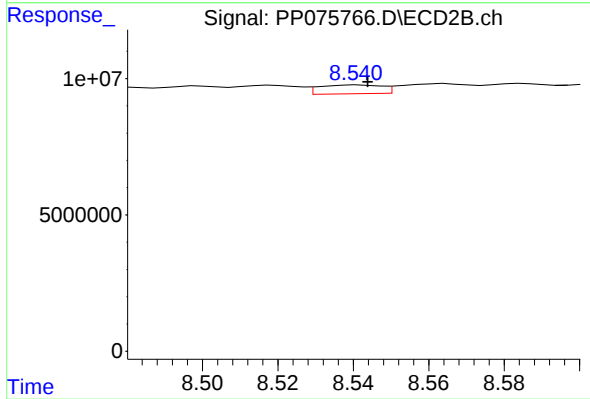

#45 AR-1268-5

R.T.: 8.541 min
Delta R.T.: -0.002 min
Response: 3715195
Conc: 1.22 ng/ml