

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101419\
 Data File : PP030464.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Oct 2019 11:59
 Operator : DD\AJ
 Sample : PB123884TB
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 14:16:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100919.M
 Quant Title : 8080.M
 QLast Update : Thu Oct 10 09:35:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.035	11.189	270.7E6	105.7E6	748.814	481.009 #
Target Compounds							
6) T	MCP	11.680	11.705	49755825	48857111	54.602	114.764 #
8) T	DICHLORPROP	0.000	12.541	0	25410586	N.D.	122.246 #
15) T	Picloram	16.481	0.000	8633532	0	3.773	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101419\
Data File : PP030464.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Oct 2019 11:59
Operator : DD\AJ
Sample : PB123884TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 14:16:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100919.M
Quant Title : 8080.M
QLast Update : Thu Oct 10 09:35:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

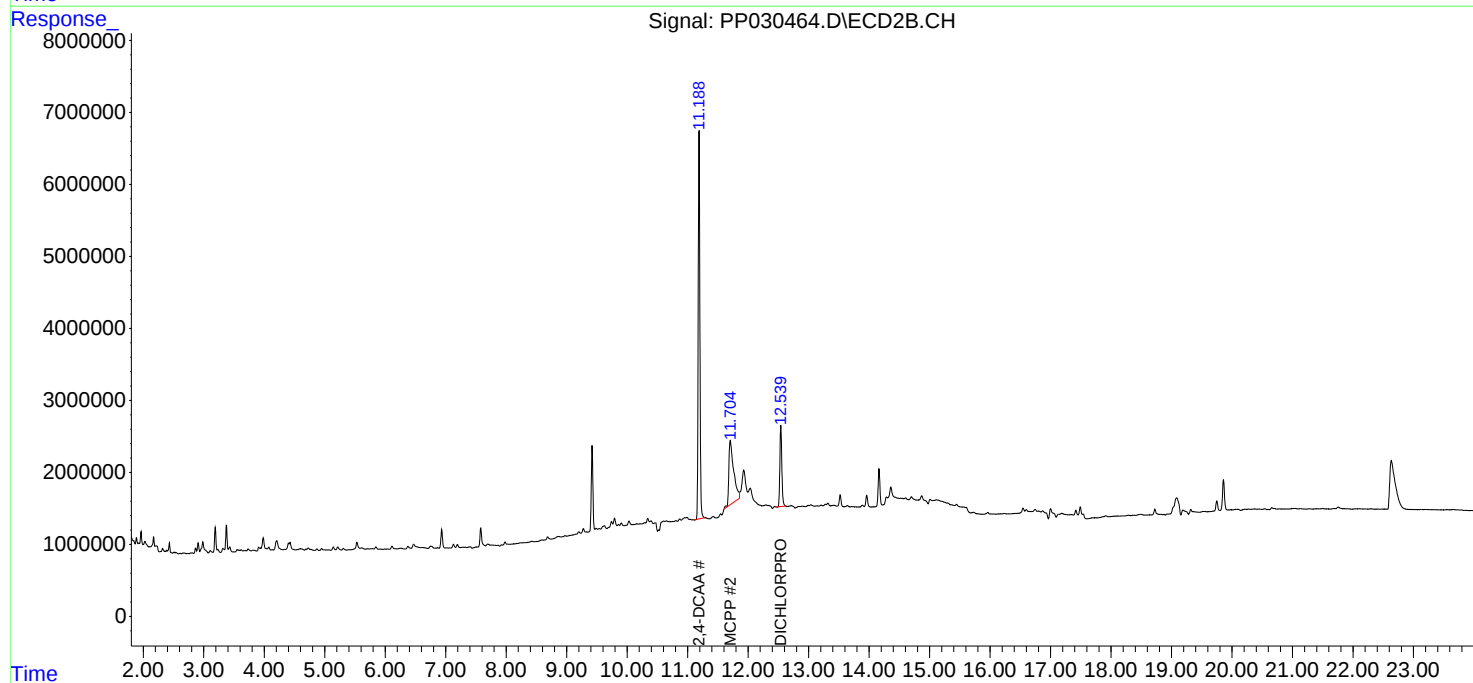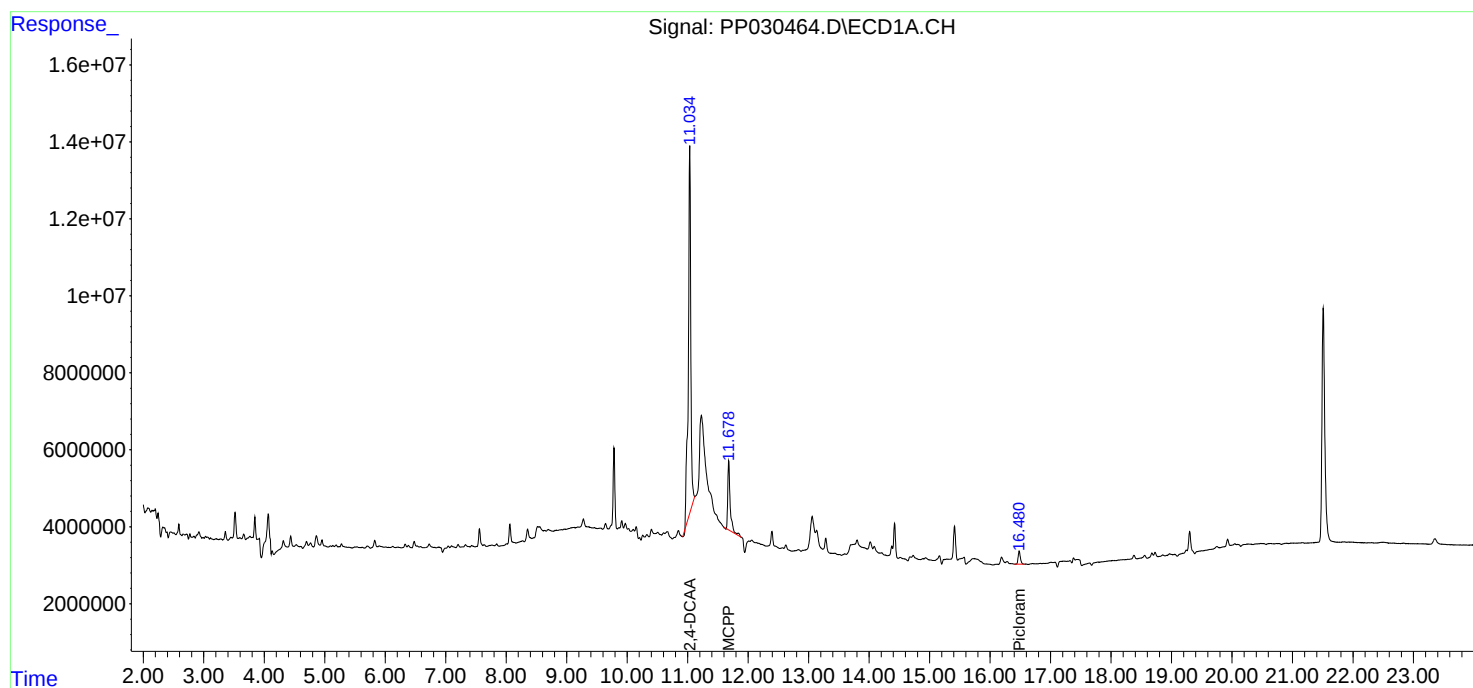


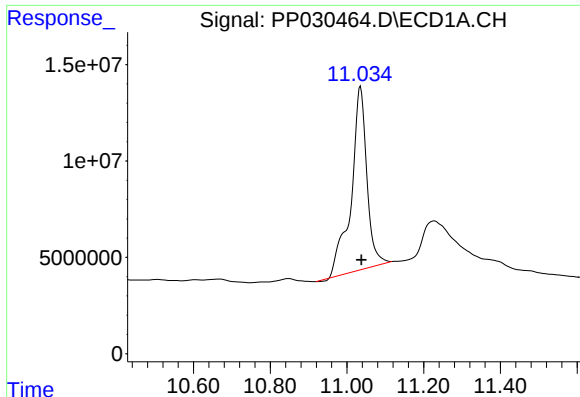

#4 2,4-DCAA


R.T.: 11.035 min
Delta R.T.: -0.002 min
Response: 270746849
Conc: 748.81 ng/ml

Instrument :
ECD_P
ClientSampleId :

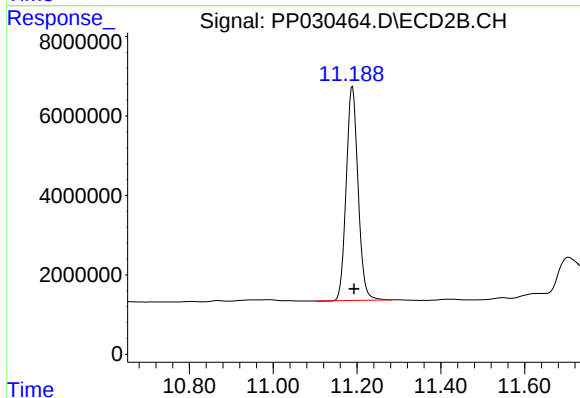


#4 2,4-DCAA

R.T.: 11.189 min
Delta R.T.: -0.004 min
Response: 105705311
Conc: 481.01 ng/ml

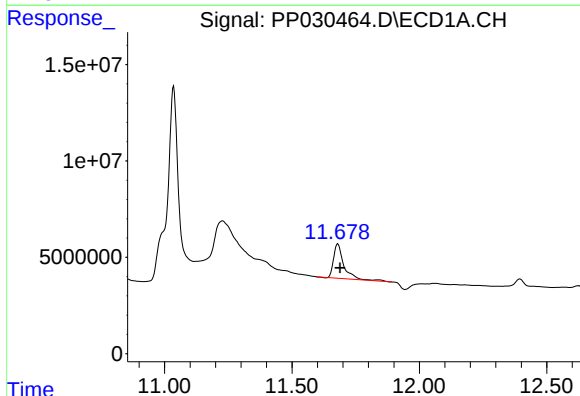


#6 MCP

R.T.: 11.680 min
Delta R.T.: -0.009 min
Response: 49755825
Conc: 54.60 ug/ml

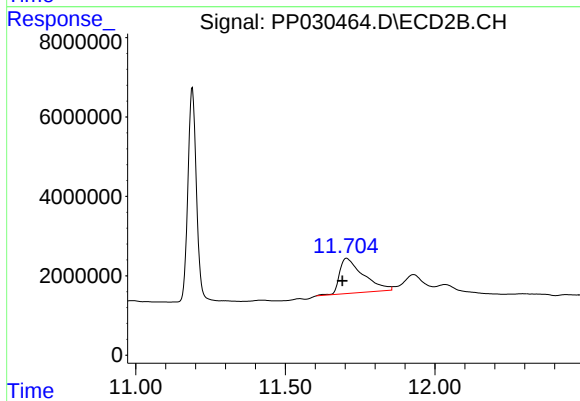

#6 MCP


R.T.: 11.705 min
Delta R.T.: 0.014 min
Response: 48857111
Conc: 114.76 ug/ml

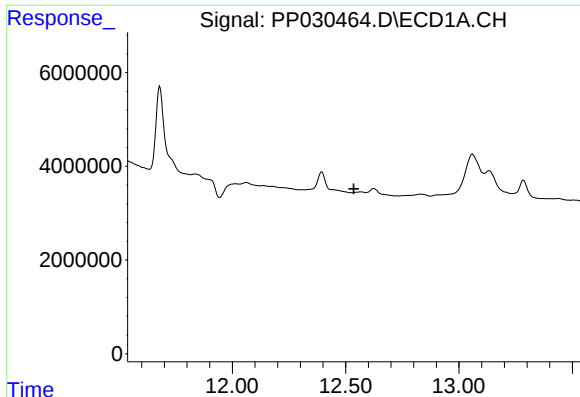

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.536 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

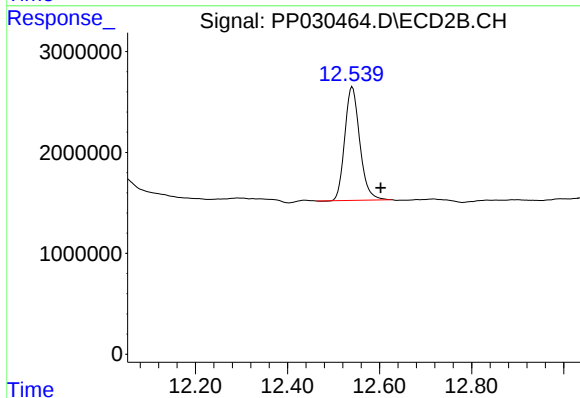


#8 DICHLORPROP

R.T.: 12.541 min
Delta R.T.: -0.062 min
Response: 25410586
Conc: 122.25 ng/ml

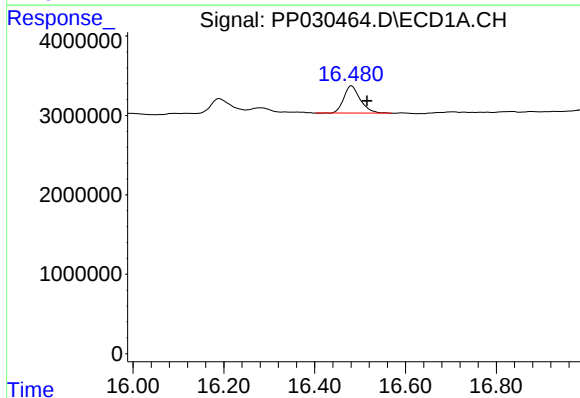

#15 Picloram

R.T.: 16.481 min
Delta R.T.: -0.034 min
Response: 8633532
Conc: 3.77 ng/ml

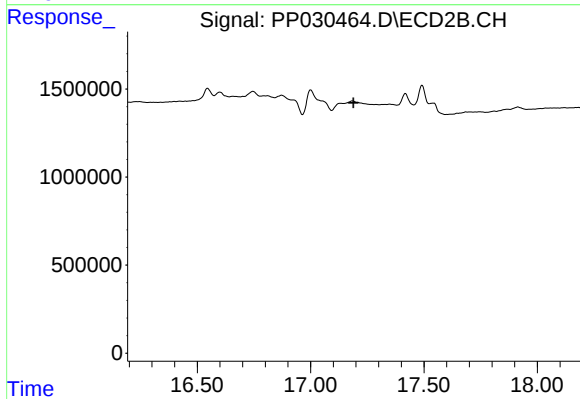

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.190 min
Response: 0
Conc: N.D.