

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101424\
 Data File : PP067784.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2024 13:43
 Operator : YP\AJ
 Sample : P4390-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/15/2024
 Supervised By :Ankita Jodhani 10/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 16:06:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.754	4.052	12498838	12207358	13.503m	12.082
2) SA Decachlor...	10.672	9.219	16930698	14617329	14.706	13.034

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101424\
Data File : PP067784.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2024 13:43
Operator : YP\AJ
Sample : P4390-04
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/15/2024
Supervised By :Ankita Jodhani 10/15/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 16:06:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

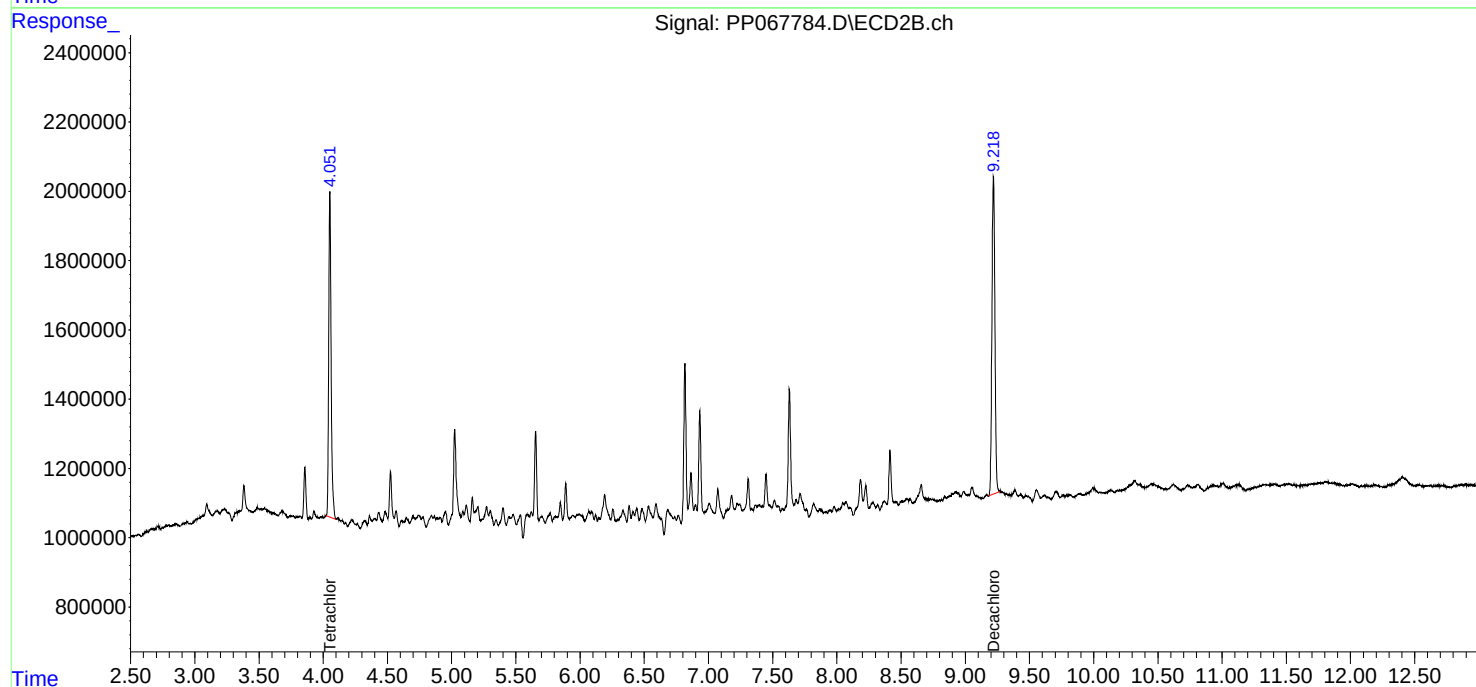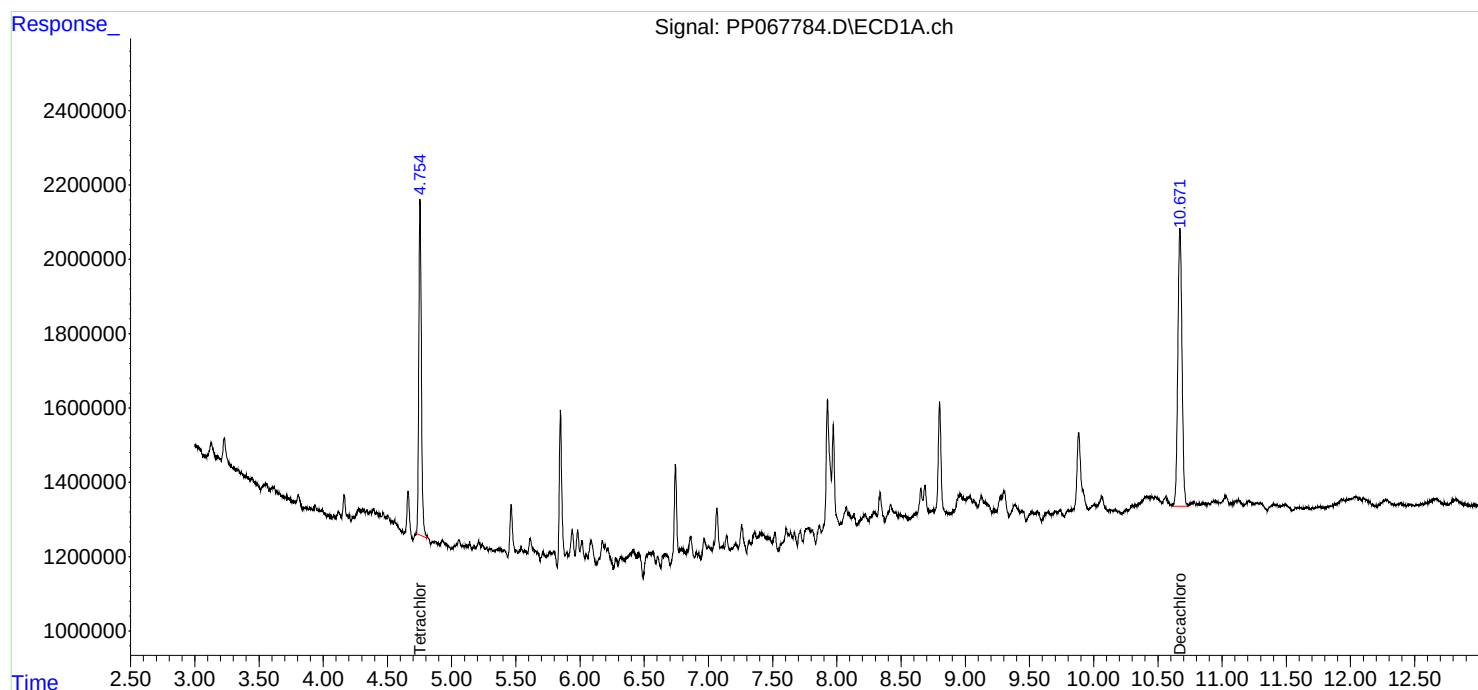

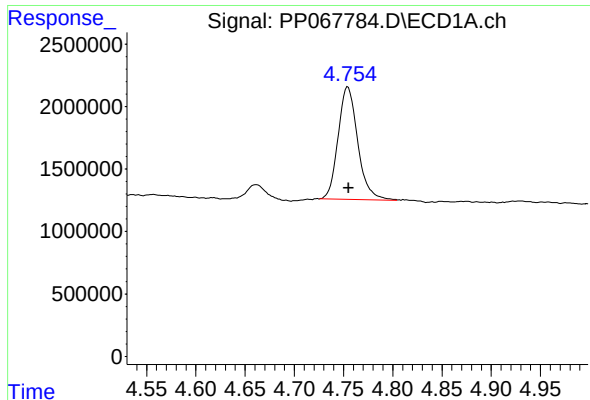


#1 Tetrachloro-m-xylene

R.T.: 4.754 min
Delta R.T.: -0.001 min
Response: 12498838
Conc: 13.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/15/2024
Supervised By :Ankita Jodhani 10/15/2024

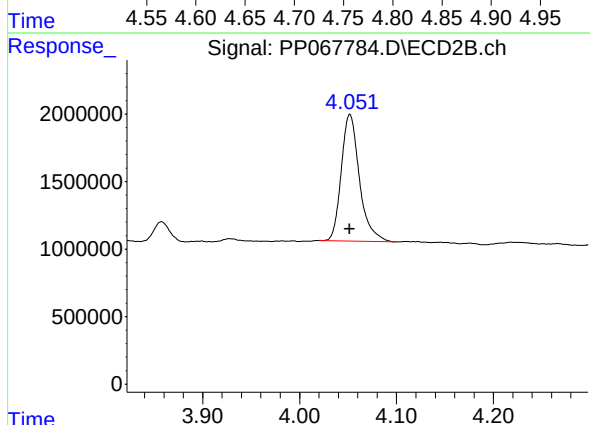


#1 Tetrachloro-m-xylene

R.T.: 4.052 min
Delta R.T.: 0.000 min
Response: 12207358
Conc: 12.08 ng/ml

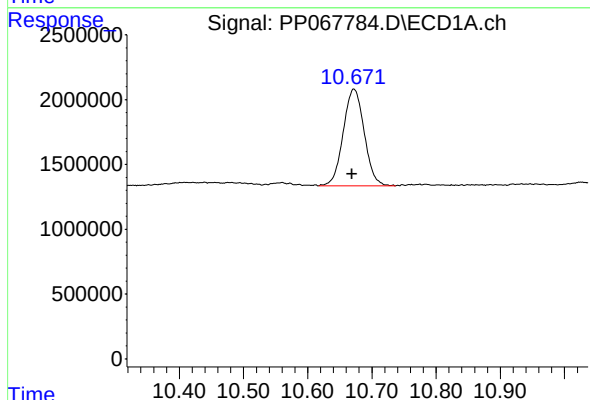

#2 Decachlorobiphenyl

R.T.: 10.672 min
Delta R.T.: 0.003 min
Response: 16930698
Conc: 14.71 ng/ml

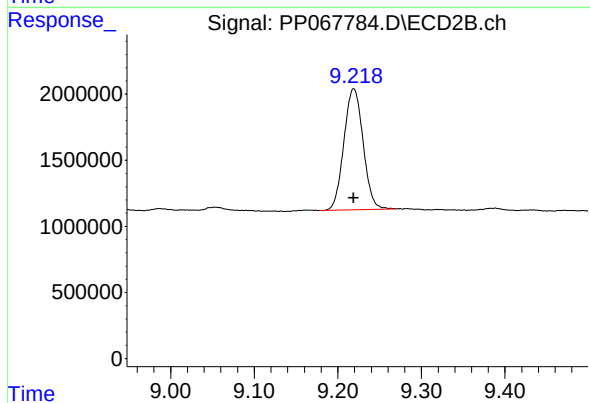

#2 Decachlorobiphenyl

R.T.: 9.219 min
Delta R.T.: 0.000 min
Response: 14617329
Conc: 13.03 ng/ml