

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101425\
 Data File : PP075775.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2025 11:22
 Operator : YP\AJ
 Sample : Q3332-02RE 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 100725-B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/14/2025
 Supervised By :mohammad ahmed 10/16/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 11:53:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 24 10:55:35 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.649	3.790	1167631	4555605	0.892m	0.747m
2) SA Decachlor...	10.420	8.808	195491	1168362	0.196m	0.194

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101425\
Data File : PP075775.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2025 11:22
Operator : YP\AJ
Sample : Q3332-02RE 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
100725-B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/14/2025
Supervised By :mohammad ahmed 10/16/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 11:53:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 24 10:55:35 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

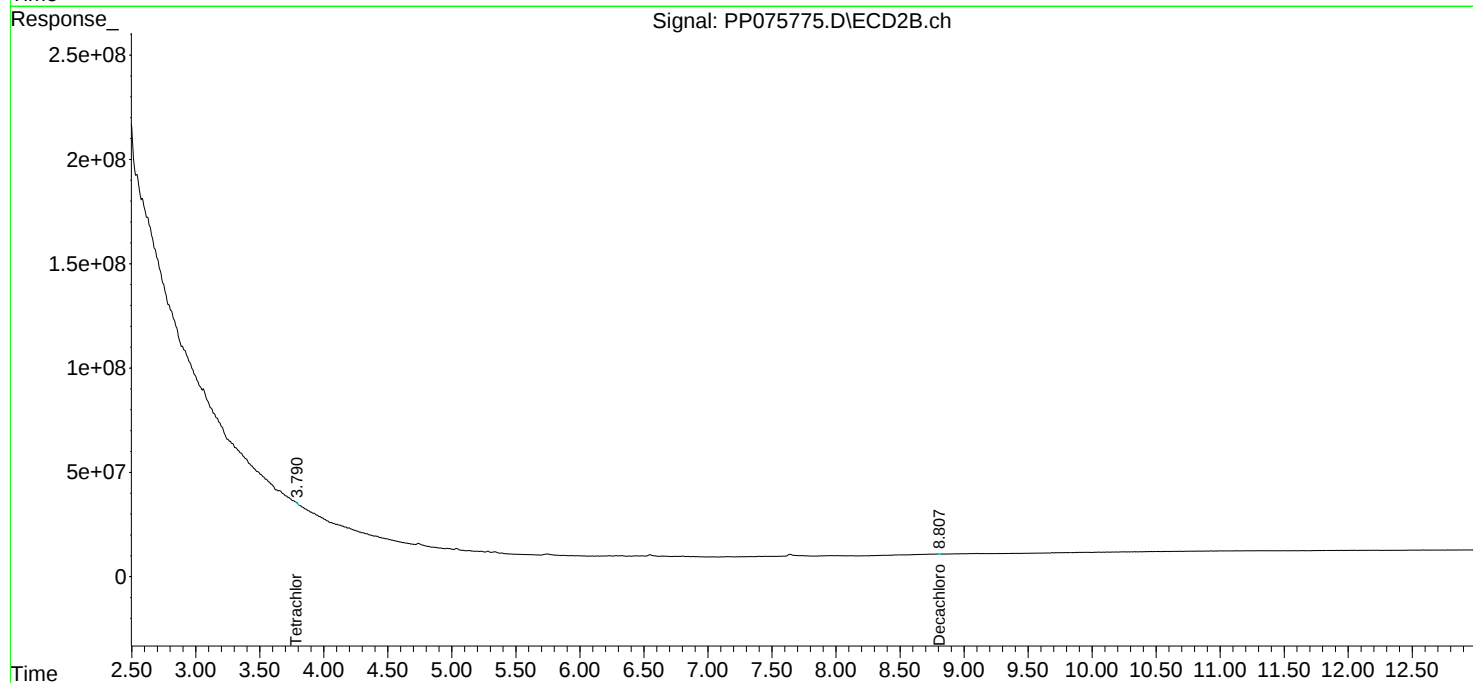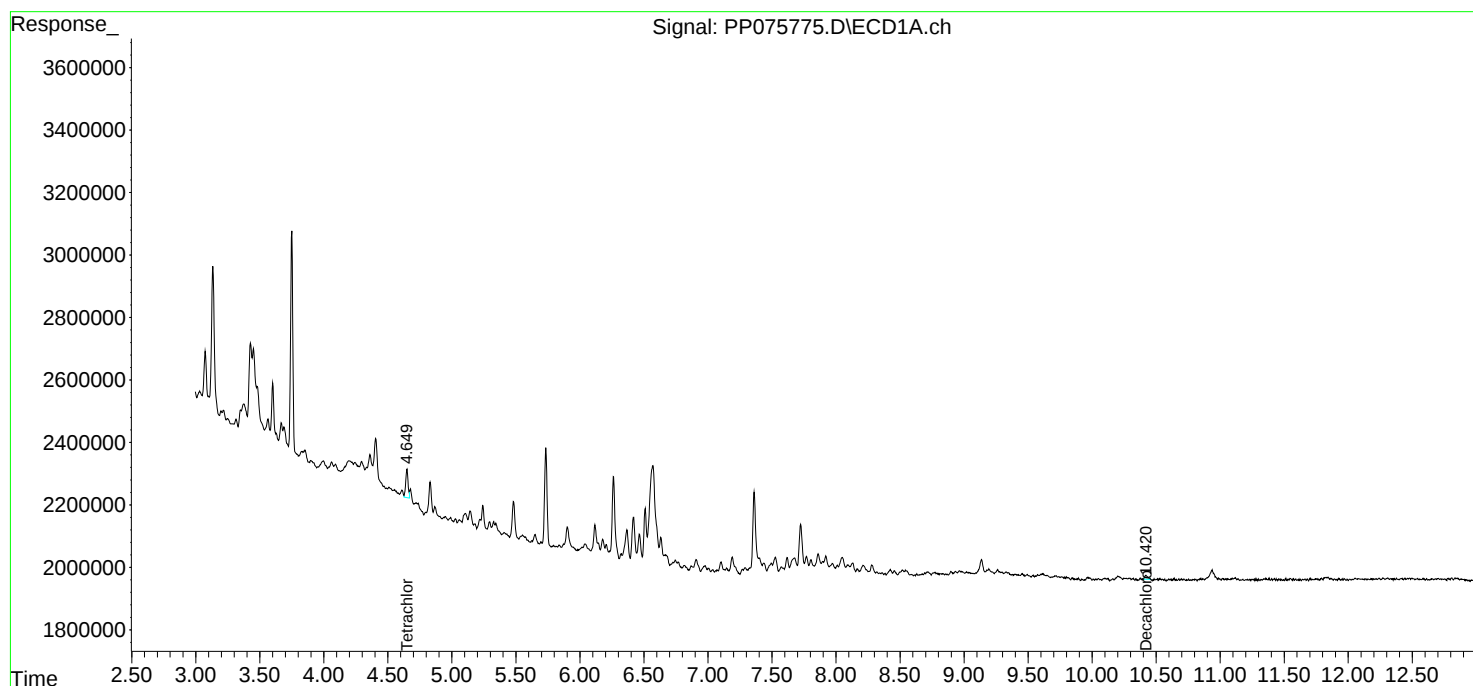

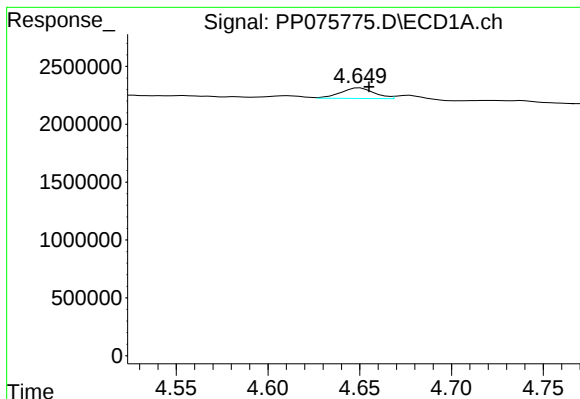


#1 Tetrachloro-m-xylene

R.T.: 4.649 min
Delta R.T.: -0.006 min
Response: 1167631
Conc: 0.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
100725-B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/14/2025
Supervised By :mohammad ahmed 10/16/2025

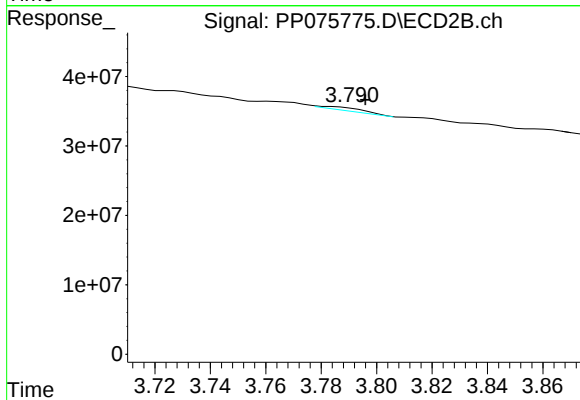


#1 Tetrachloro-m-xylene

R.T.: 3.790 min
Delta R.T.: -0.006 min
Response: 4555605
Conc: 0.75 ng/ml m

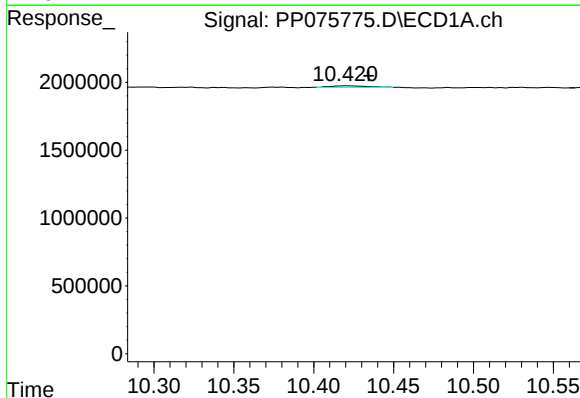

#2 Decachlorobiphenyl

R.T.: 10.420 min
Delta R.T.: -0.015 min
Response: 195491
Conc: 0.20 ng/ml m

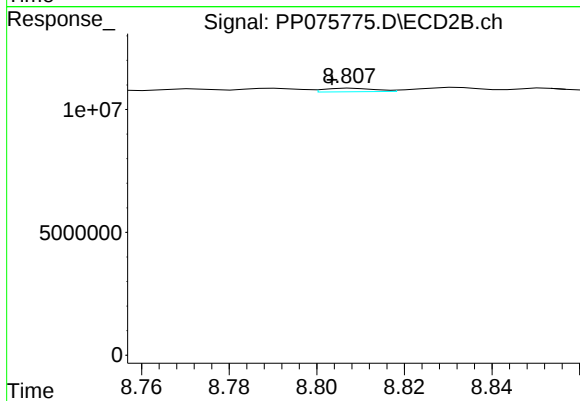

#2 Decachlorobiphenyl

R.T.: 8.808 min
Delta R.T.: 0.005 min
Response: 1168362
Conc: 0.19 ng/ml