

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101521\
 Data File : PP040087.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2021 13:46
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:45:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.893	3.982	653770	357834	21.528	21.166
2)	SA Decachlor...	10.914	9.310	549080	514341	22.215	24.235
Target Compounds							
10)	L2 AR-1221-3	0.000	4.422	0	9635	N.D.	17.792 #
11)	L3 AR-1232-1	0.000	4.422	0	9635	N.D.	23.723 #
32)	L7 AR-1260-2	8.195f	7.017f	15325	14627	11.213	12.353
33)	L7 AR-1260-3	0.000	7.192	0	10367	N.D.	8.774 #
35)	L7 AR-1260-5	0.000	7.930	0	6924	N.D.	3.388 #
37)	L8 AR-1262-2	0.000	7.930	0	6924	N.D.	3.077 #
45)	L9 AR-1268-5	10.596f	0.000	41806	0	4.861	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101521\
Data File : PP040087.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2021 13:46
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:45:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

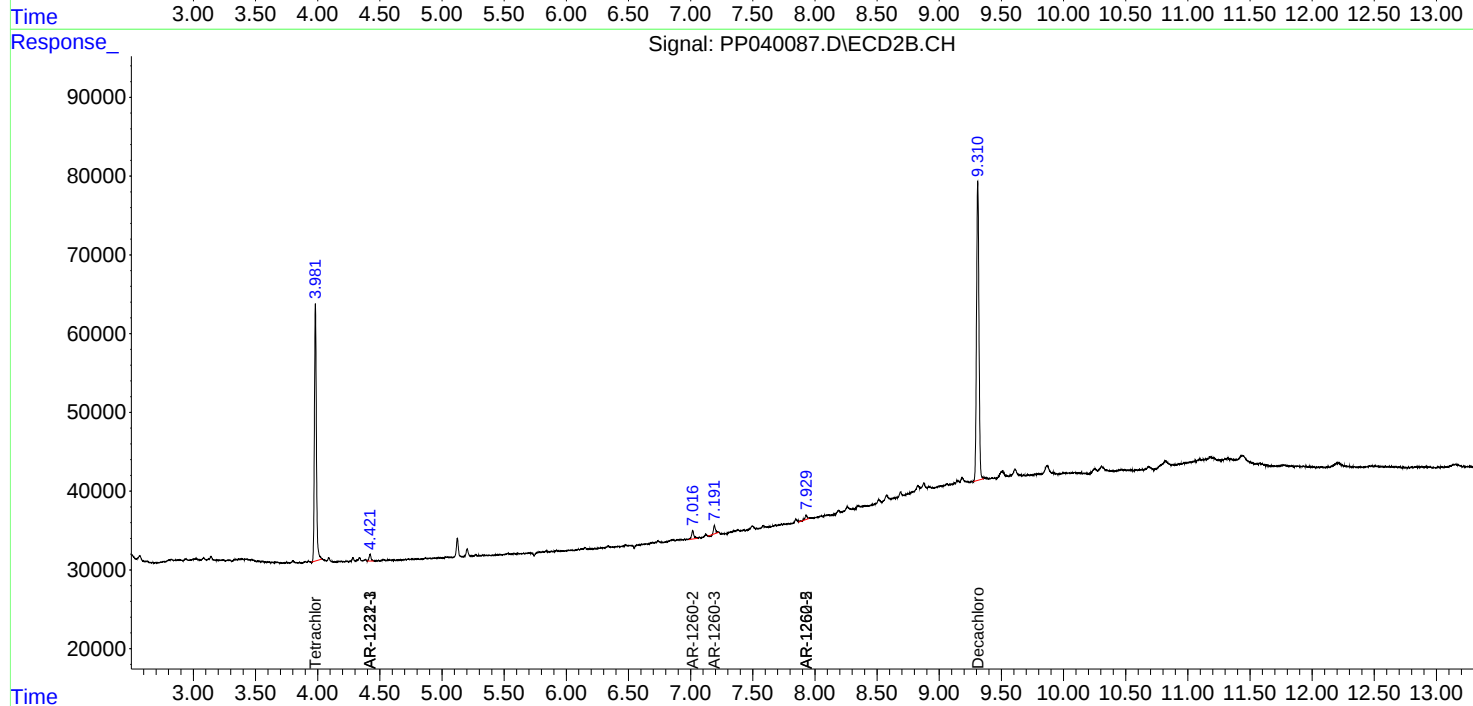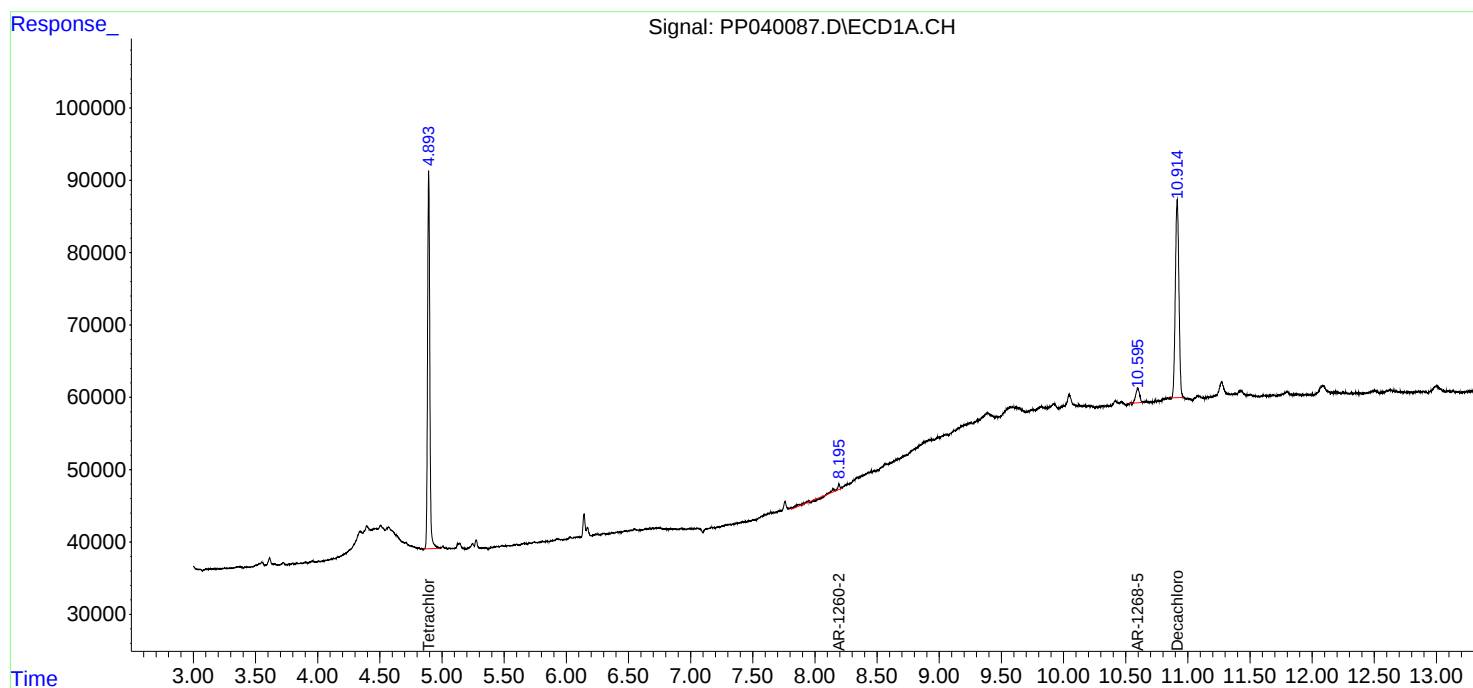


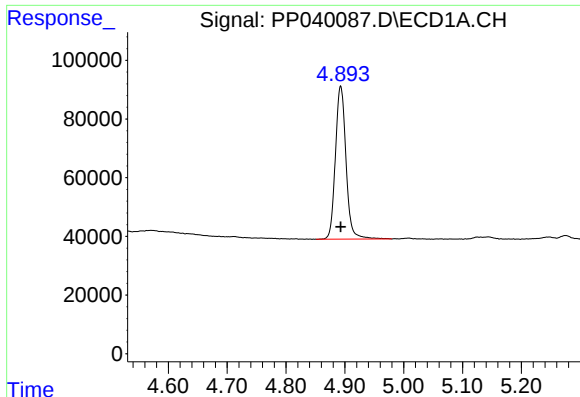

#1 Tetrachloro-m-xylene


R.T.: 4.893 min
Delta R.T.: 0.000 min
Response: 653770
Conc: 21.53 ng/ml

Instrument :
ECD_P
ClientSampleId :

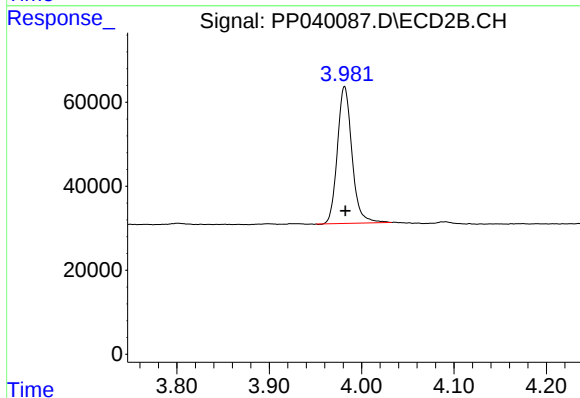


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 357834
Conc: 21.17 ng/ml

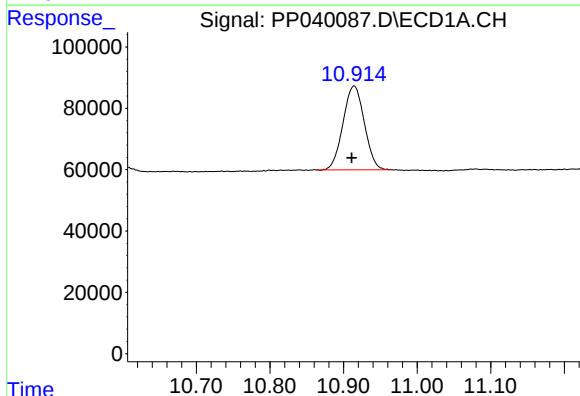


#2 Decachlorobiphenyl

R.T.: 10.914 min
Delta R.T.: 0.003 min
Response: 549080
Conc: 22.21 ng/ml

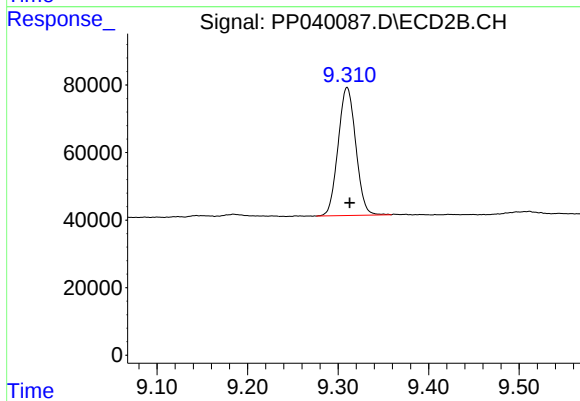

#2 Decachlorobiphenyl


R.T.: 9.310 min
Delta R.T.: -0.003 min
Response: 514341
Conc: 24.24 ng/ml

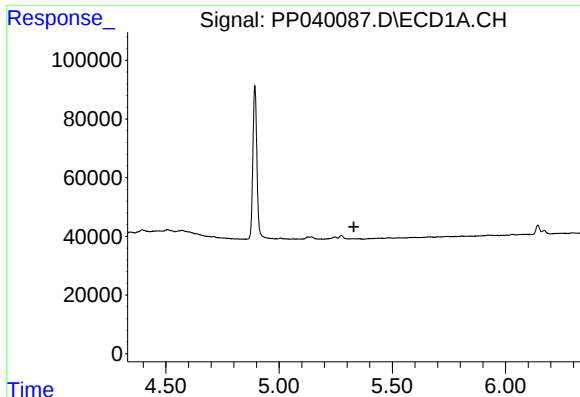

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 5.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

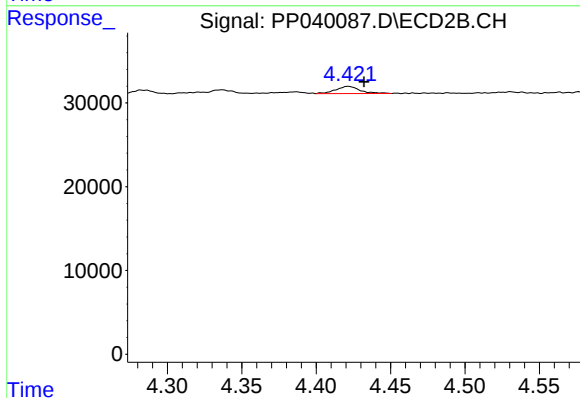


#10 AR-1221-3

R.T.: 4.422 min
Delta R.T.: -0.011 min
Response: 9635
Conc: 17.79 ng/ml

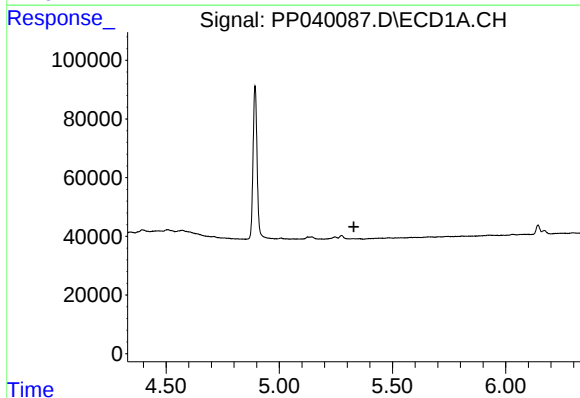


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 5.330 min
Response: 0
Conc: N.D.

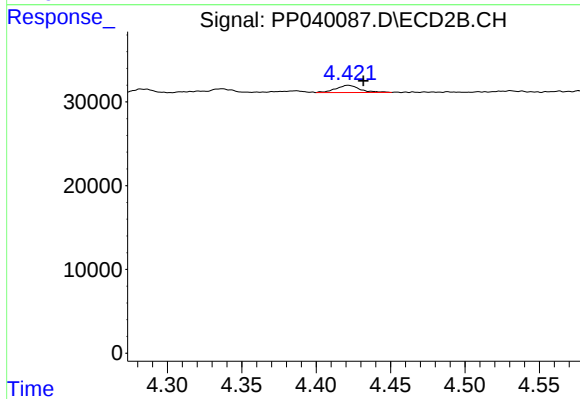

#11 AR-1232-1


R.T.: 4.422 min
Delta R.T.: -0.010 min
Response: 9635
Conc: 23.72 ng/ml

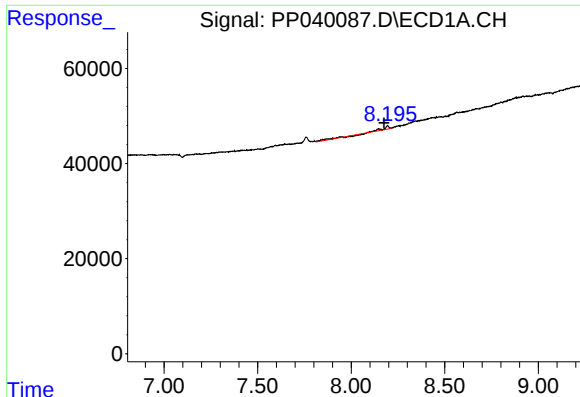

#32 AR-1260-2


R.T.: 8.195 min
Delta R.T.: 0.020 min
Response: 15325
Conc: 11.21 ng/ml

Instrument :
ECD_P
ClientSampleId :

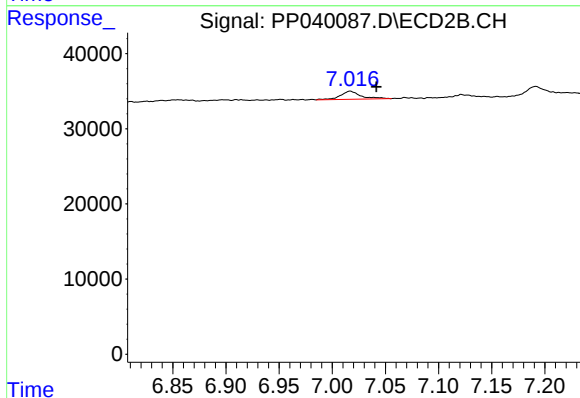


#32 AR-1260-2

R.T.: 7.017 min
Delta R.T.: -0.025 min
Response: 14627
Conc: 12.35 ng/ml

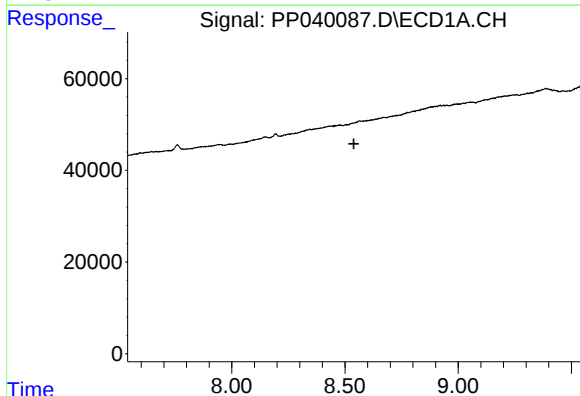


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.540 min
Response: 0
Conc: N.D.

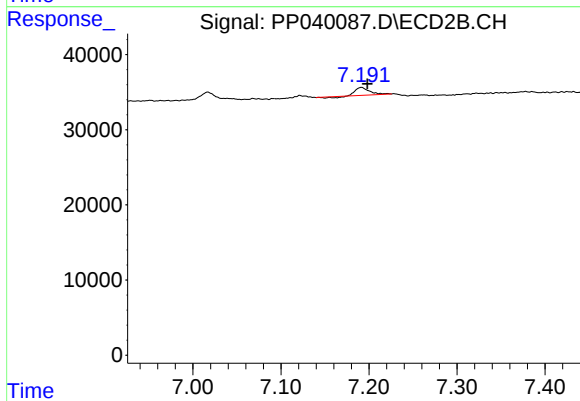

#33 AR-1260-3


R.T.: 7.192 min
Delta R.T.: -0.007 min
Response: 10367
Conc: 8.77 ng/ml

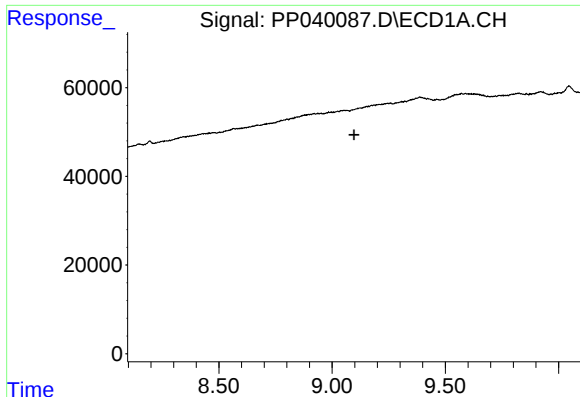

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 9.097 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

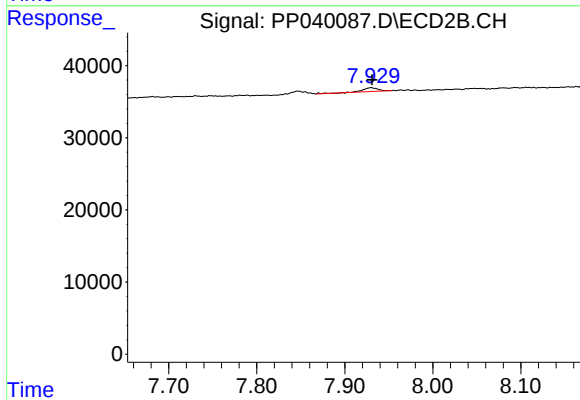


#35 AR-1260-5

R.T.: 7.930 min
Delta R.T.: 0.000 min
Response: 6924
Conc: 3.39 ng/ml

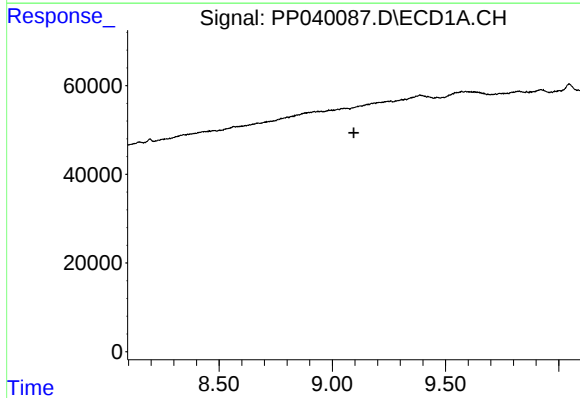


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.

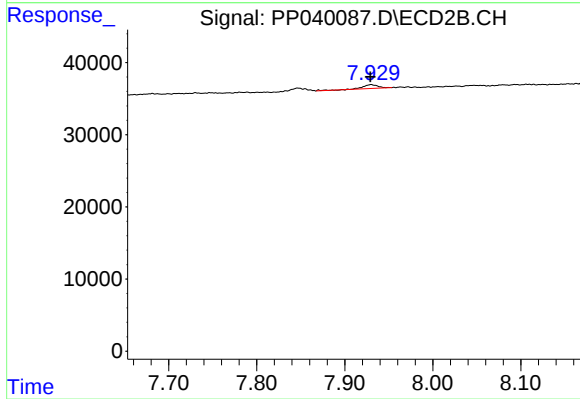

#37 AR-1262-2


R.T.: 7.930 min
Delta R.T.: 0.000 min
Response: 6924
Conc: 3.08 ng/ml

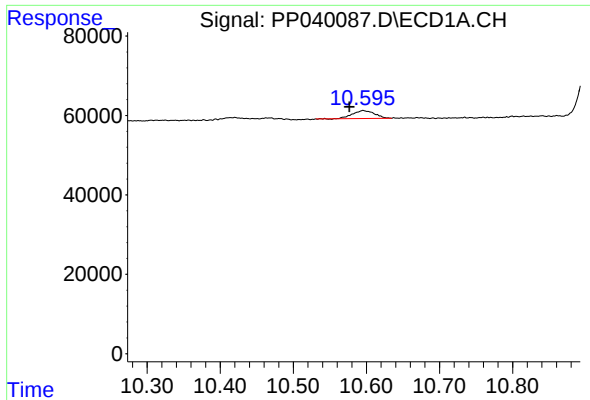

#45 AR-1268-5

R.T.: 10.596 min
Delta R.T.: 0.019 min
Response: 41806
Conc: 4.86 ng/ml

Instrument :
ECD_P
ClientSampleId :

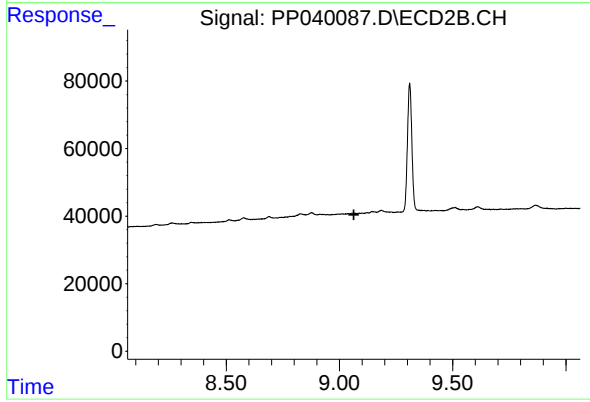

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.064 min
Response: 0
Conc: N.D.