

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101521\
 Data File : PP040092.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2021 15:10
 Operator : AJ\MA
 Sample : M4160-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:46:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.894	3.982	671498	385788	22.112	22.820
2)	SA Decachlor...	10.915	9.310	594301	520118	24.045	24.507
Target Compounds							
9)	L2 AR-1221-2	5.240	0.000	30823	0	138.350	N.D. #
32)	L7 AR-1260-2	0.000	7.048	0	8589	N.D.	7.254 #
33)	L7 AR-1260-3	0.000	7.219f	0	15589	N.D.	13.194 #
34)	L7 AR-1260-4	0.000	7.681	0	12714	N.D.	14.465 #
35)	L7 AR-1260-5	0.000	7.930	0	5239	N.D.	2.563 #
37)	L8 AR-1262-2	0.000	7.930	0	5239	N.D.	2.328 #
43)	L9 AR-1268-3	0.000	8.513f	0	6537	N.D.	2.985 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101521\
Data File : PP040092.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2021 15:10
Operator : AJ\MA
Sample : M4160-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:46:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

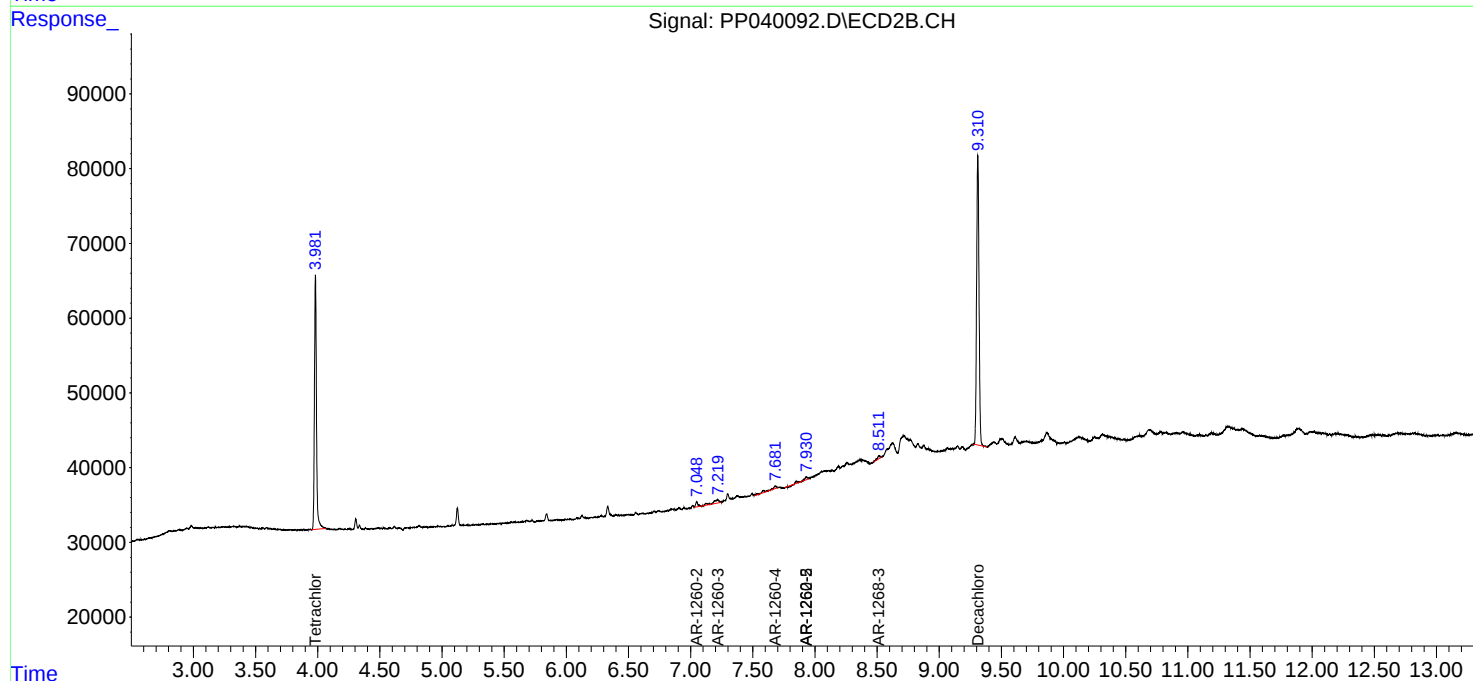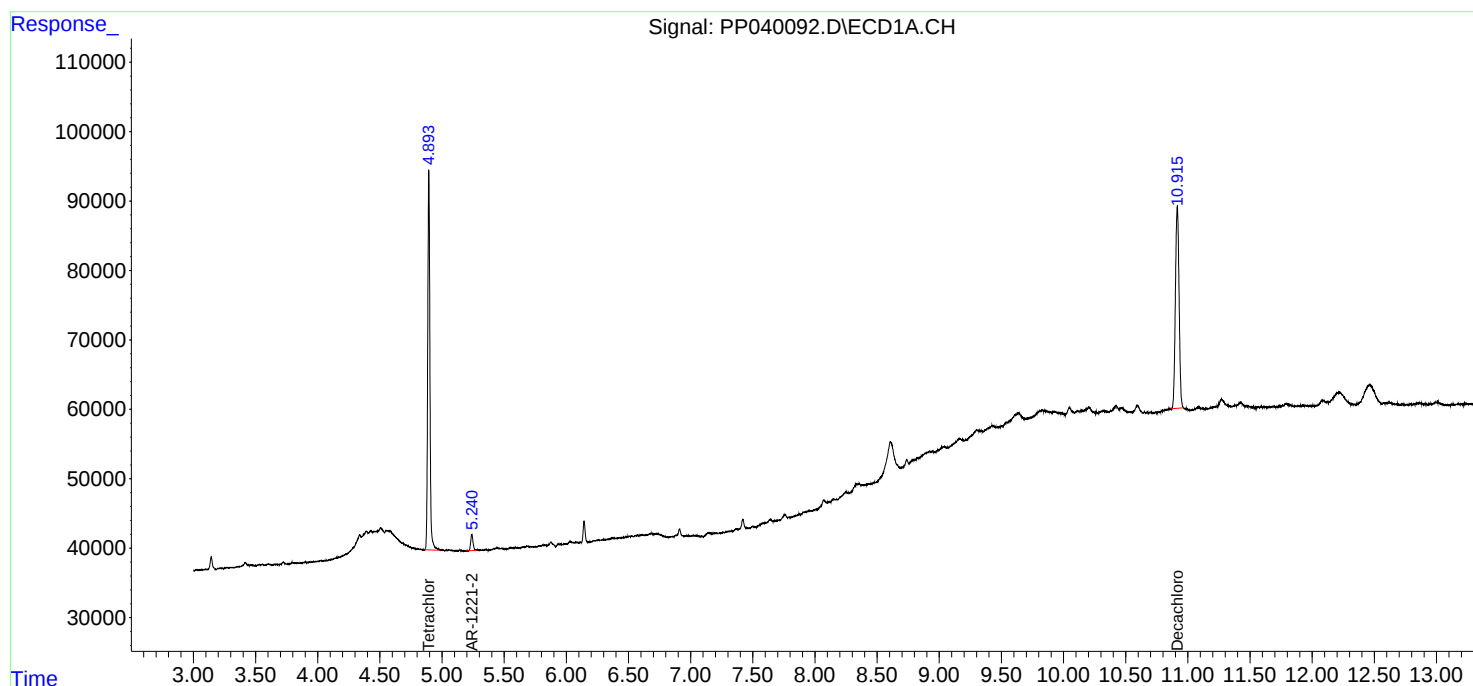


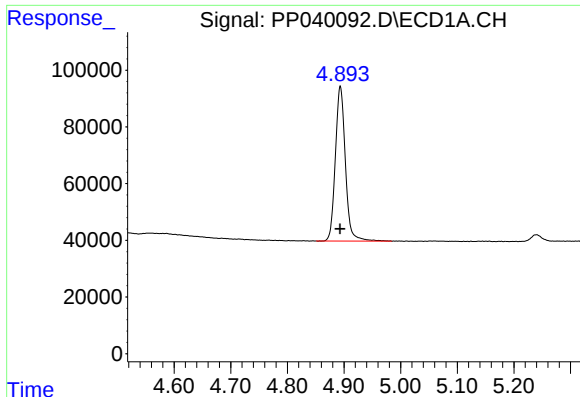

#1 Tetrachloro-m-xylene


R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 671498
Conc: 22.11 ng/ml

Instrument :
ECD_P
ClientSampleId :

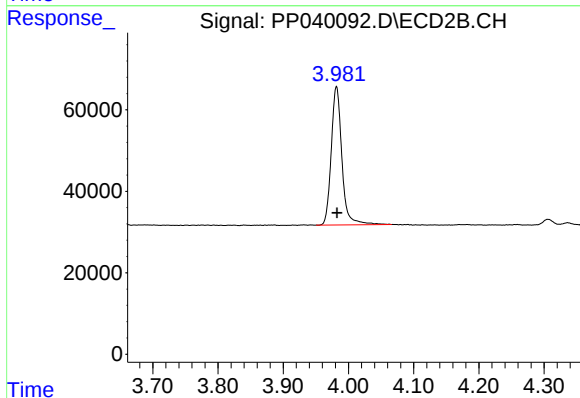


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 385788
Conc: 22.82 ng/ml

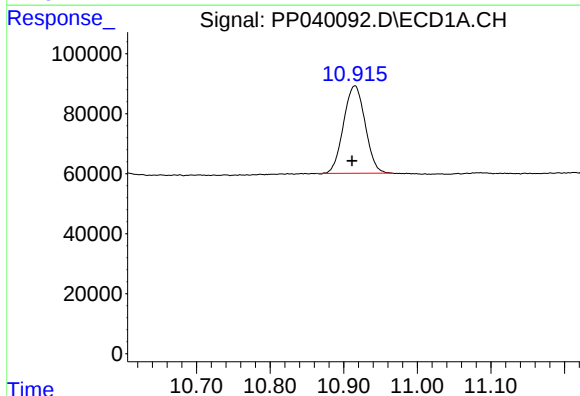


#2 Decachlorobiphenyl

R.T.: 10.915 min
Delta R.T.: 0.004 min
Response: 594301
Conc: 24.04 ng/ml

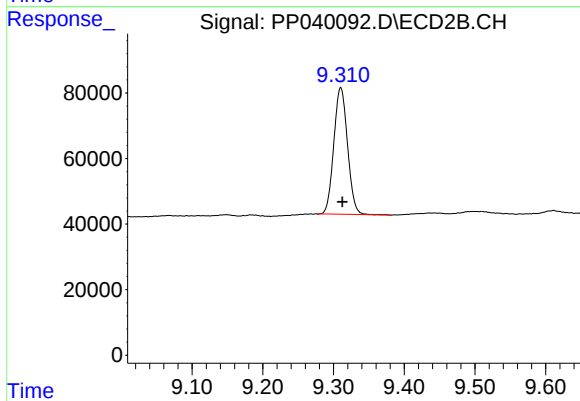

#2 Decachlorobiphenyl


R.T.: 9.310 min
Delta R.T.: -0.003 min
Response: 520118
Conc: 24.51 ng/ml

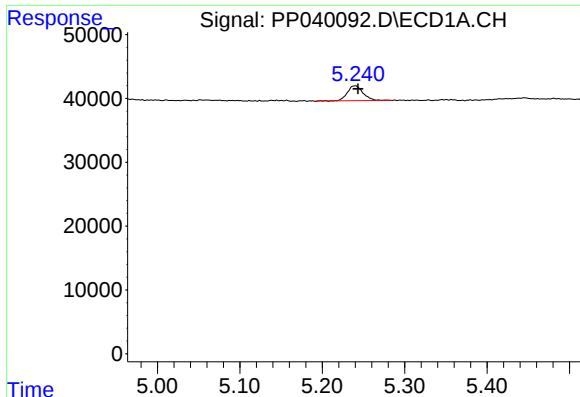

#9 AR-1221-2


R.T.: 5.240 min
Delta R.T.: -0.004 min
Response: 30823
Conc: 138.35 ng/ml

Instrument :
ECD_P
ClientSampleId :

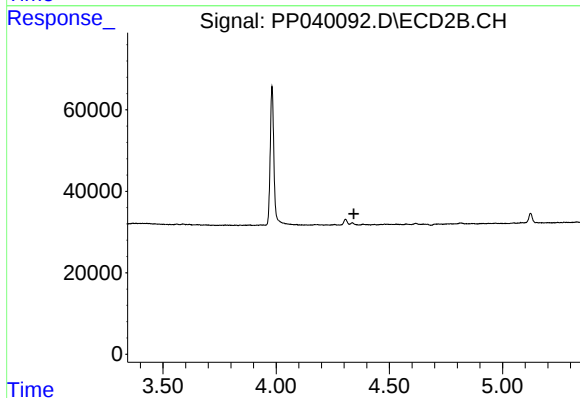


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.343 min
Response: 0
Conc: N.D.

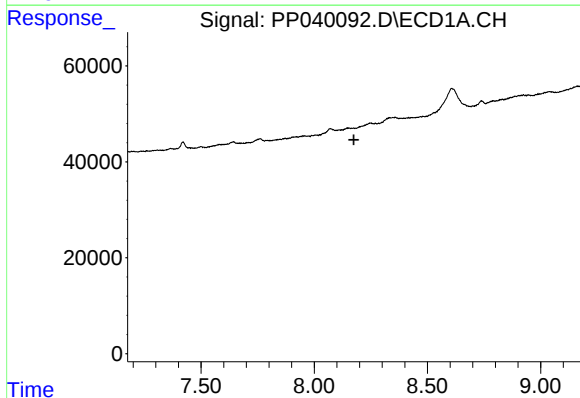


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.175 min
Response: 0
Conc: N.D.

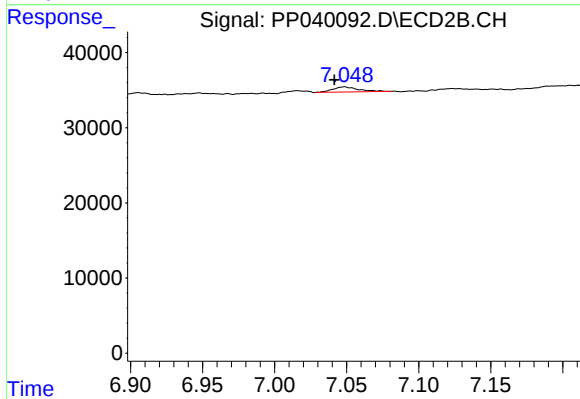

#32 AR-1260-2


R.T.: 7.048 min
Delta R.T.: 0.007 min
Response: 8589
Conc: 7.25 ng/ml

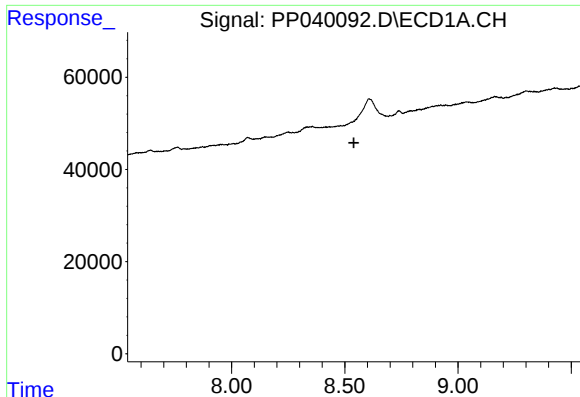

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.540 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

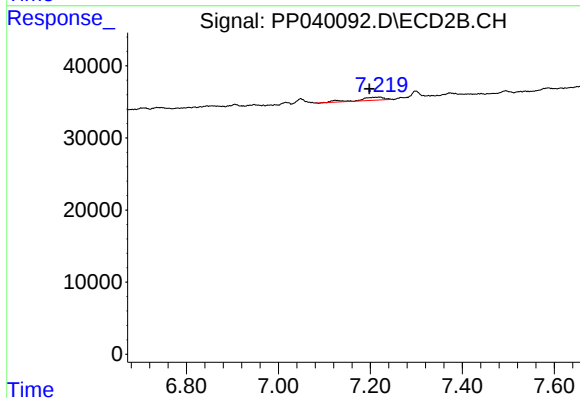


#33 AR-1260-3

R.T.: 7.219 min
Delta R.T.: 0.021 min
Response: 15589
Conc: 13.19 ng/ml

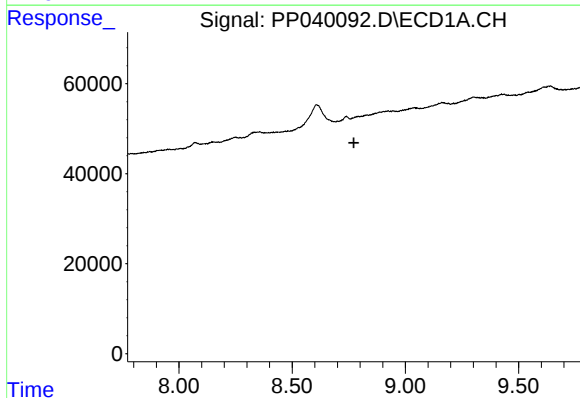


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 8.772 min
Response: 0
Conc: N.D.

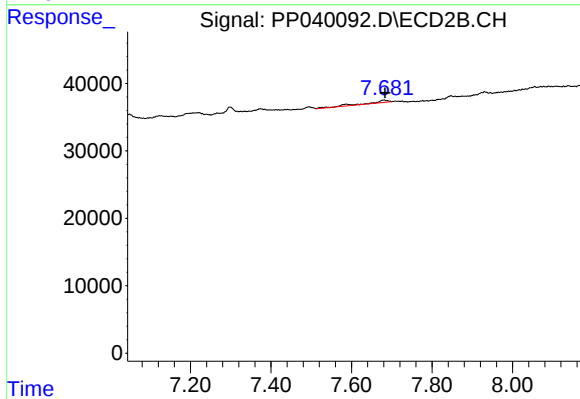

#34 AR-1260-4


R.T.: 7.681 min
Delta R.T.: -0.003 min
Response: 12714
Conc: 14.47 ng/ml

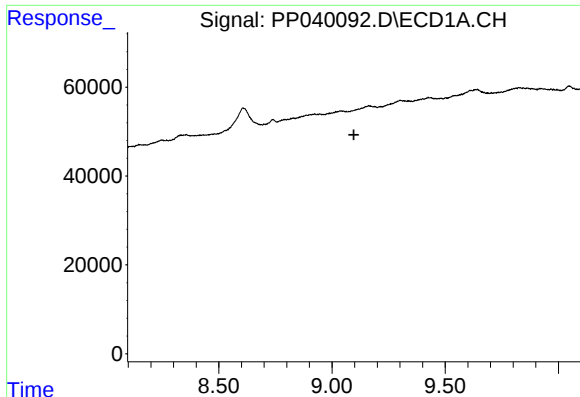

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 9.097 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

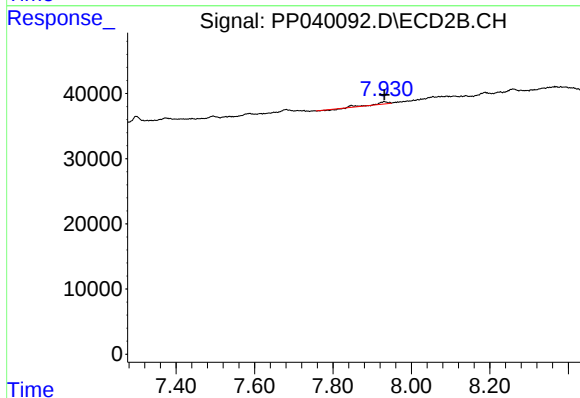


#35 AR-1260-5

R.T.: 7.930 min
Delta R.T.: 0.000 min
Response: 5239
Conc: 2.56 ng/ml

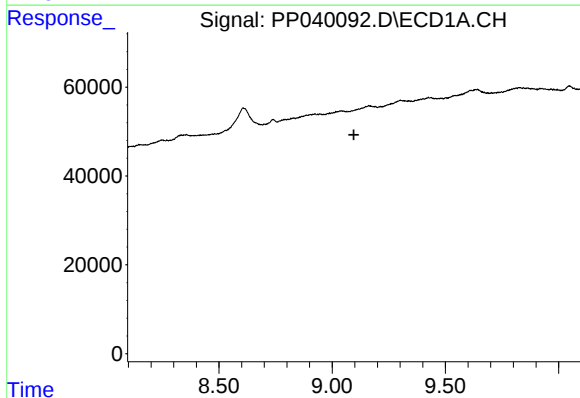


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.

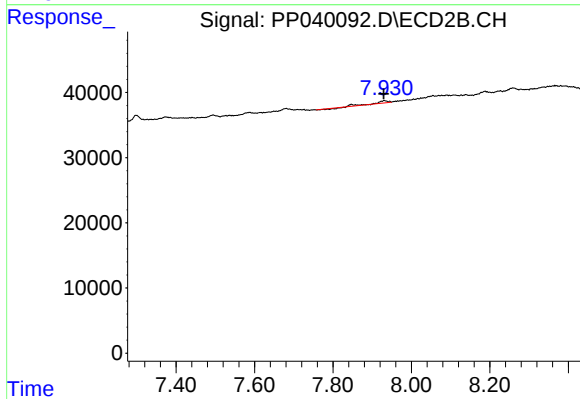

#37 AR-1262-2


R.T.: 7.930 min
Delta R.T.: 0.001 min
Response: 5239
Conc: 2.33 ng/ml

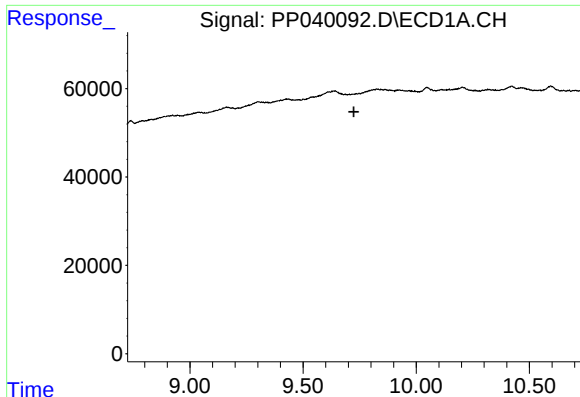

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

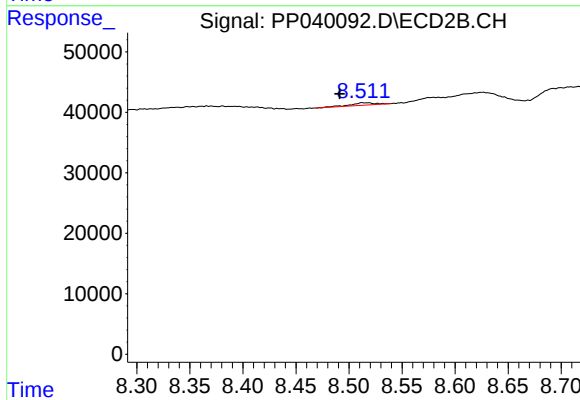

#43 AR-1268-3

R.T.: 8.513 min
Delta R.T.: 0.021 min
Response: 6537
Conc: 2.99 ng/ml