

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101521\
 Data File : PP040105.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2021 19:16
 Operator : AJ\MA
 Sample : M4227-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:50:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.894	3.982	756816	425412	24.921	25.163
2)	SA Decachlor...	10.913	9.310	639956	572154	25.892	26.959
Target Compounds							
8)	L2 AR-1221-1	5.145	4.262f	23459	55468	67.361	271.042 #
9)	L2 AR-1221-2	0.000	4.341	0	49024	N.D.	291.450 #
10)	L2 AR-1221-3	5.357f	0.000	76880	0	95.362	N.D. #
11)	L3 AR-1232-1	5.357f	0.000	76880	0	123.551	N.D. #
28)	L6 AR-1254-3	7.758f	0.000	16409	0	11.518	N.D. #
32)	L7 AR-1260-2	8.172	0.000	29443	0	21.542	N.D. #
35)	L7 AR-1260-5	0.000	7.929	0	8732	N.D.	4.272 #
37)	L8 AR-1262-2	0.000	7.929	0	8732	N.D.	3.880 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101521\
Data File : PP040105.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2021 19:16
Operator : AJ\MA
Sample : M4227-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:50:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

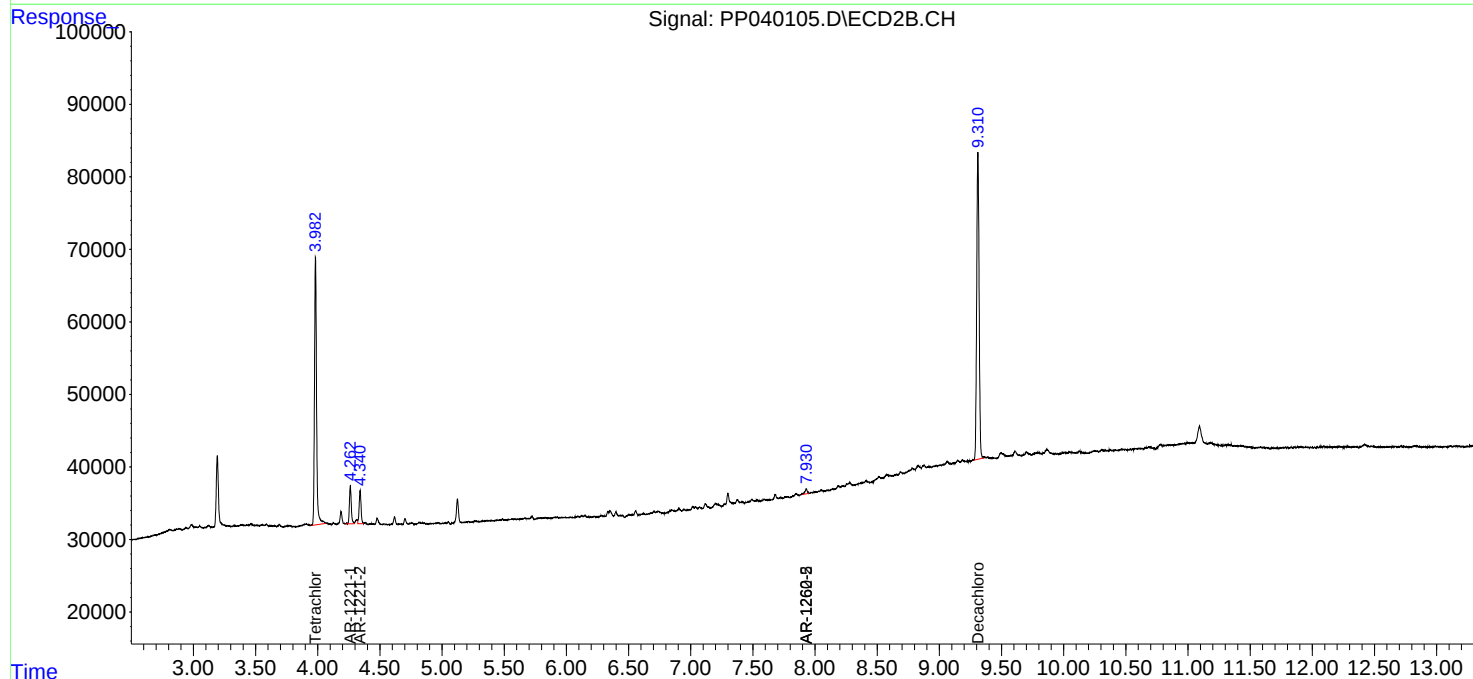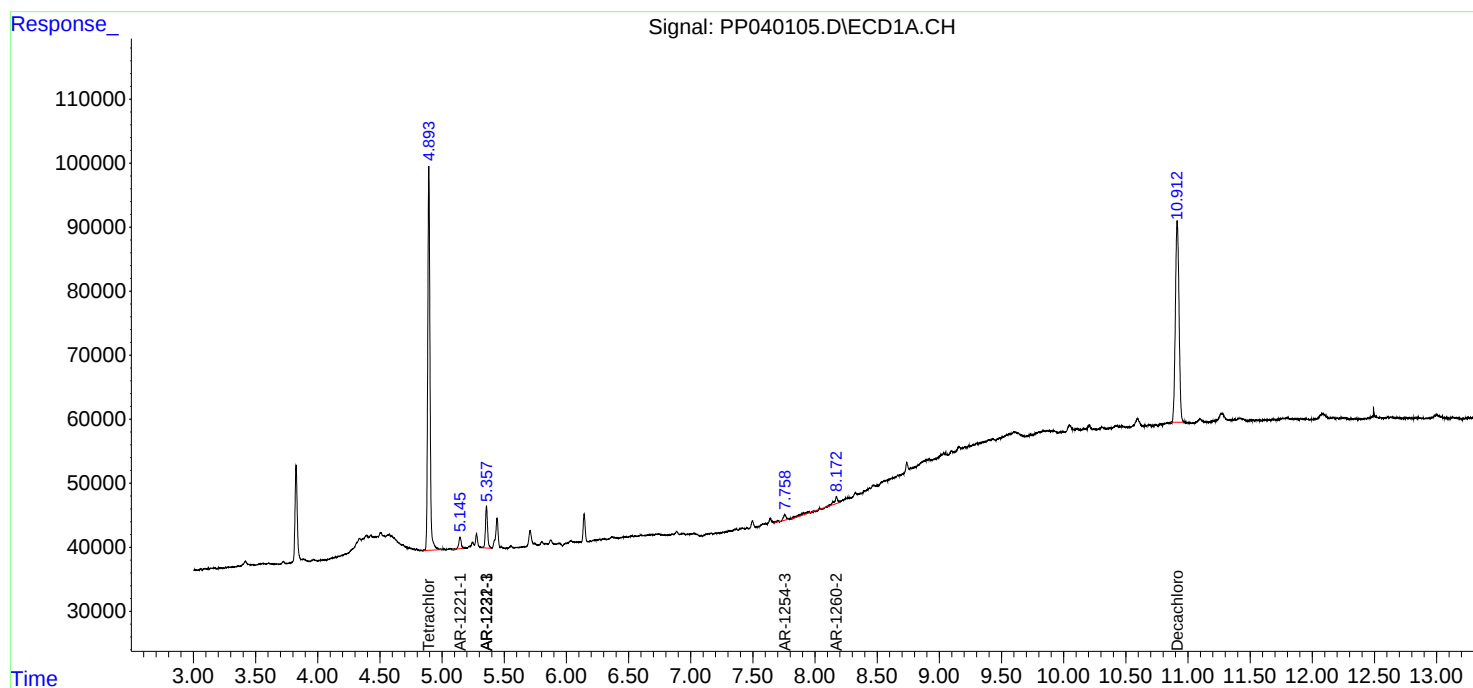


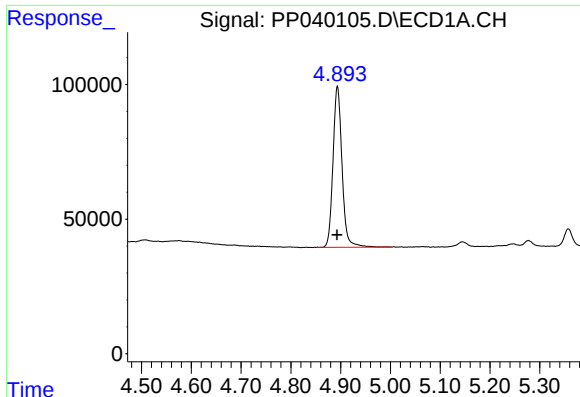

#1 Tetrachloro-m-xylene


R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 756816
Conc: 24.92 ng/ml

Instrument :
ECD_P
ClientSampleId :

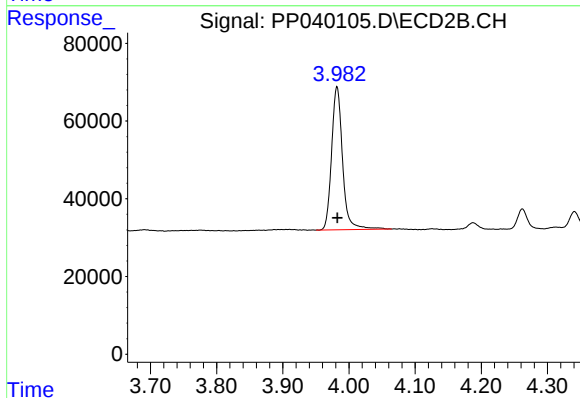


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 425412
Conc: 25.16 ng/ml

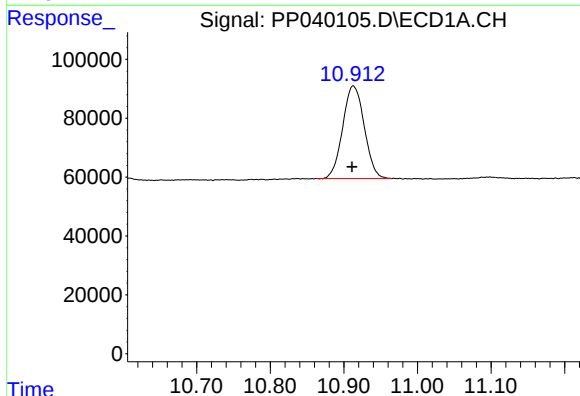


#2 Decachlorobiphenyl

R.T.: 10.913 min
Delta R.T.: 0.002 min
Response: 639956
Conc: 25.89 ng/ml

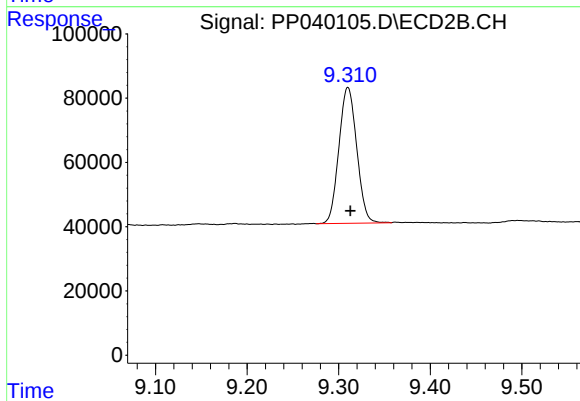

#2 Decachlorobiphenyl


R.T.: 9.310 min
Delta R.T.: -0.003 min
Response: 572154
Conc: 26.96 ng/ml

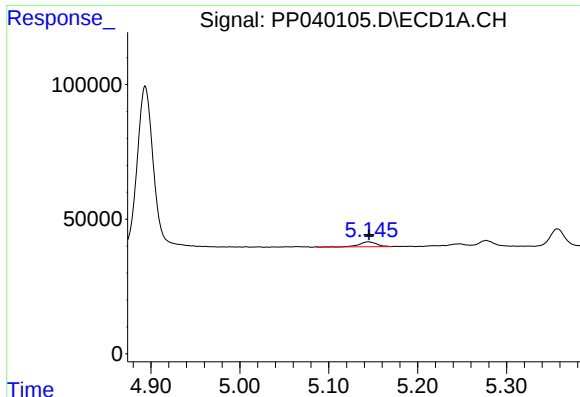

#8 AR-1221-1


R.T.: 5.145 min
Delta R.T.: 0.000 min
Response: 23459
Conc: 67.36 ng/ml

Instrument :
ECD_P
ClientSampleId :

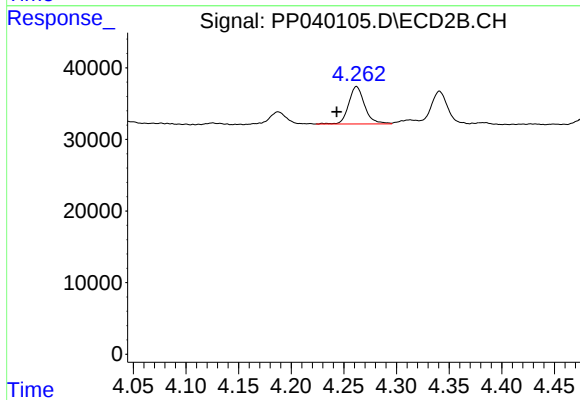


#8 AR-1221-1

R.T.: 4.262 min
Delta R.T.: 0.019 min
Response: 55468
Conc: 271.04 ng/ml

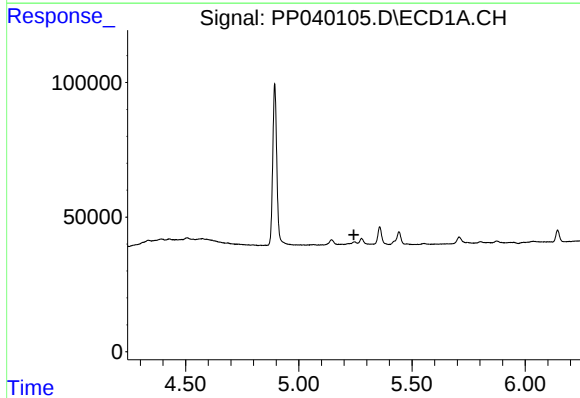


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.243 min
Response: 0
Conc: N.D.

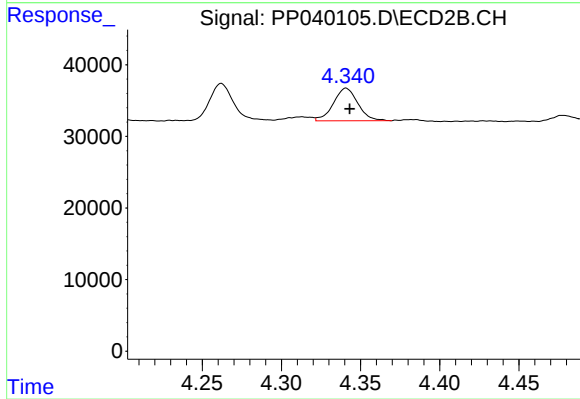

#9 AR-1221-2


R.T.: 4.341 min
Delta R.T.: -0.002 min
Response: 49024
Conc: 291.45 ng/ml

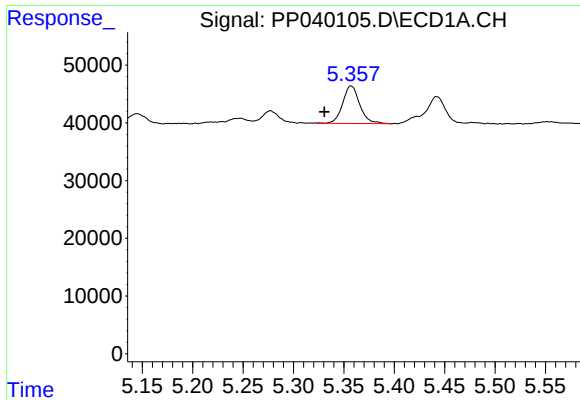

#10 AR-1221-3


R.T.: 5.357 min
Delta R.T.: 0.027 min
Response: 76880
Conc: 95.36 ng/ml

Instrument :
ECD_P
ClientSampleId :

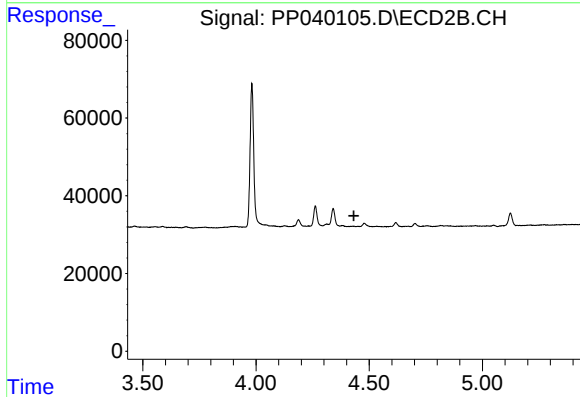


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.432 min
Response: 0
Conc: N.D.

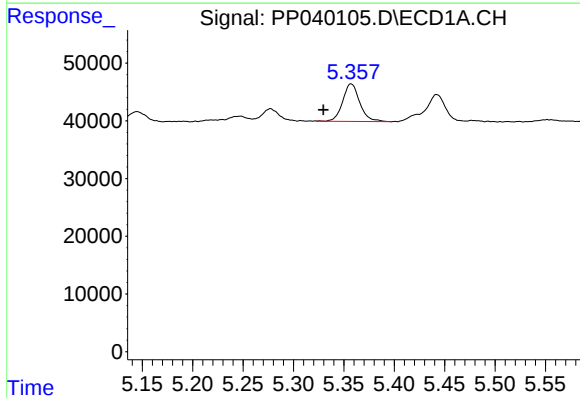


#11 AR-1232-1

R.T.: 5.357 min
Delta R.T.: 0.028 min
Response: 76880
Conc: 123.55 ng/ml

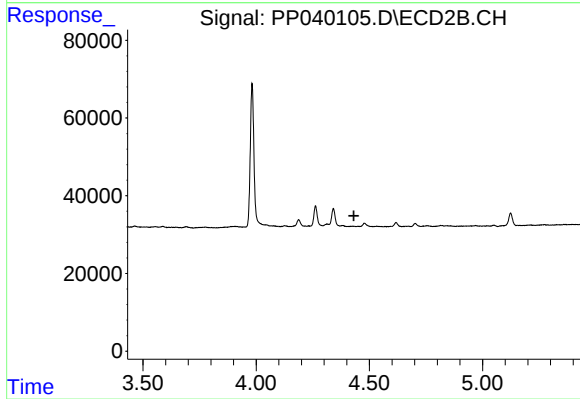

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.432 min
Response: 0
Conc: N.D.

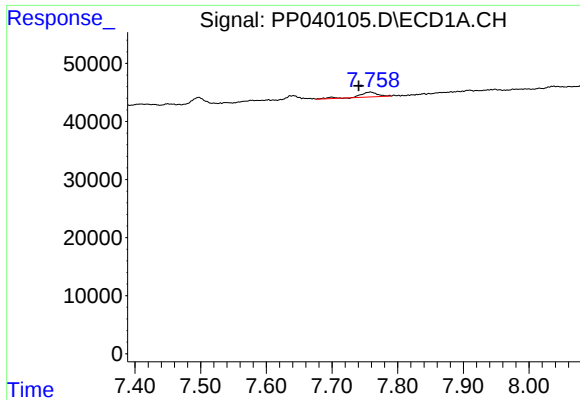

#28 AR-1254-3


R.T.: 7.758 min
Delta R.T.: 0.017 min
Response: 16409
Conc: 11.52 ng/ml

Instrument :
ECD_P
ClientSampleId :

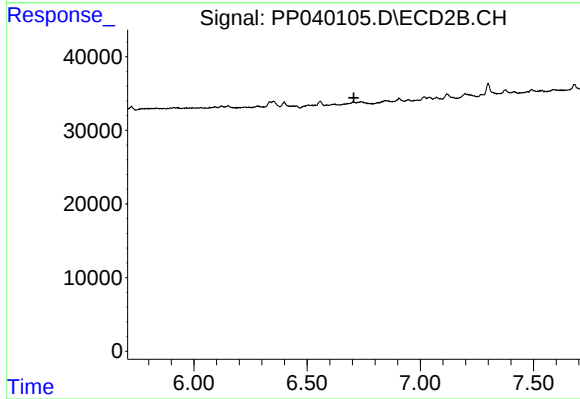


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.706 min
Response: 0
Conc: N.D.

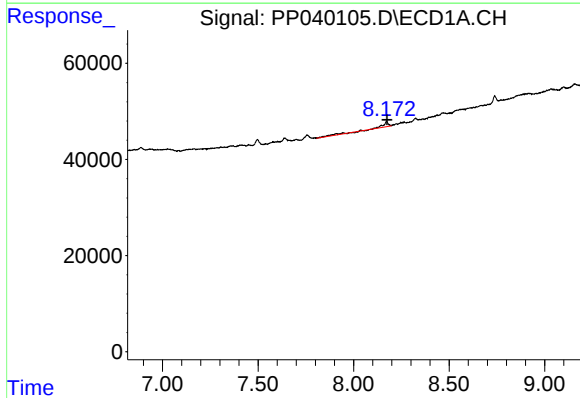


#32 AR-1260-2

R.T.: 8.172 min
Delta R.T.: -0.002 min
Response: 29443
Conc: 21.54 ng/ml

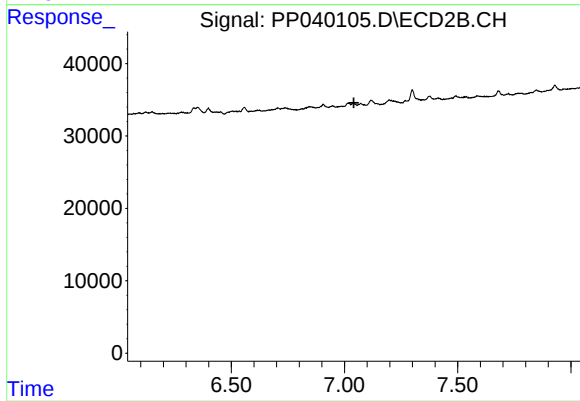

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.042 min
Response: 0
Conc: N.D.

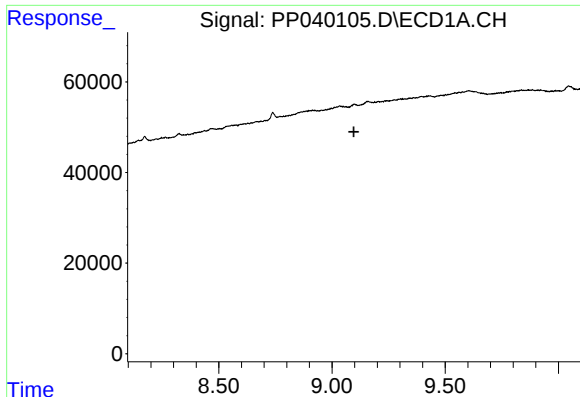

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 9.097 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

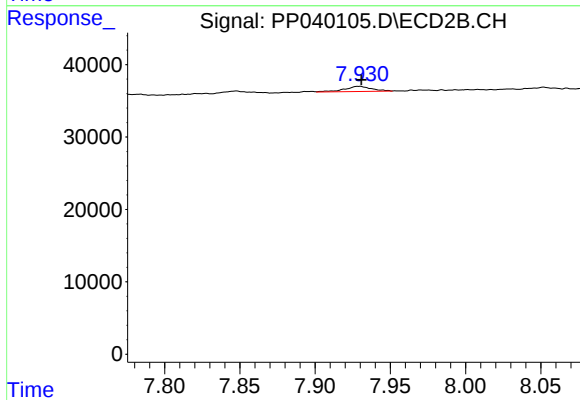


#35 AR-1260-5

R.T.: 7.929 min
Delta R.T.: -0.002 min
Response: 8732
Conc: 4.27 ng/ml

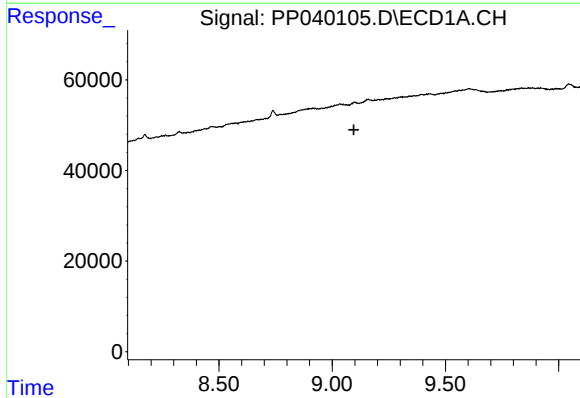

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 9.096 min
Response: 0
Conc: N.D.

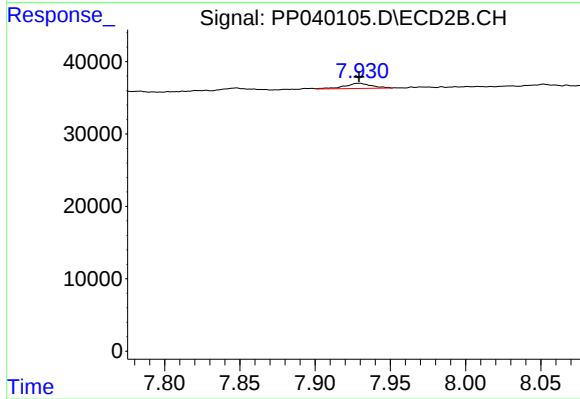

#37 AR-1262-2

R.T.: 7.929 min
Delta R.T.: 0.000 min
Response: 8732
Conc: 3.88 ng/ml