

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101521\
 Data File : PP040107.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2021 19:50
 Operator : AJ\MA
 Sample : M4242-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:51:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.894	3.982	672099	371744	22.132	21.989
2)	SA Decachlor...	10.916	9.311	559803	461317	22.649	21.737
Target Compounds							
8)	L2 AR-1221-1	0.000	4.261f	0	17858	N.D.	87.264 #
9)	L2 AR-1221-2	0.000	4.339	0	12999	N.D.	77.277 #
32)	L7 AR-1260-2	8.174	0.000	14616	0	10.694	N.D. #
35)	L7 AR-1260-5	0.000	7.945	0	35486	N.D.	17.364 #
37)	L8 AR-1262-2	0.000	7.945f	0	35486	N.D.	15.769 #
39)	L8 AR-1262-4	0.000	8.280	0	17013	N.D.	9.597 #
42)	L9 AR-1268-2	0.000	8.280	0	17013	N.D.	6.795 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101521\
Data File : PP040107.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2021 19:50
Operator : AJ\MA
Sample : M4242-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:51:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

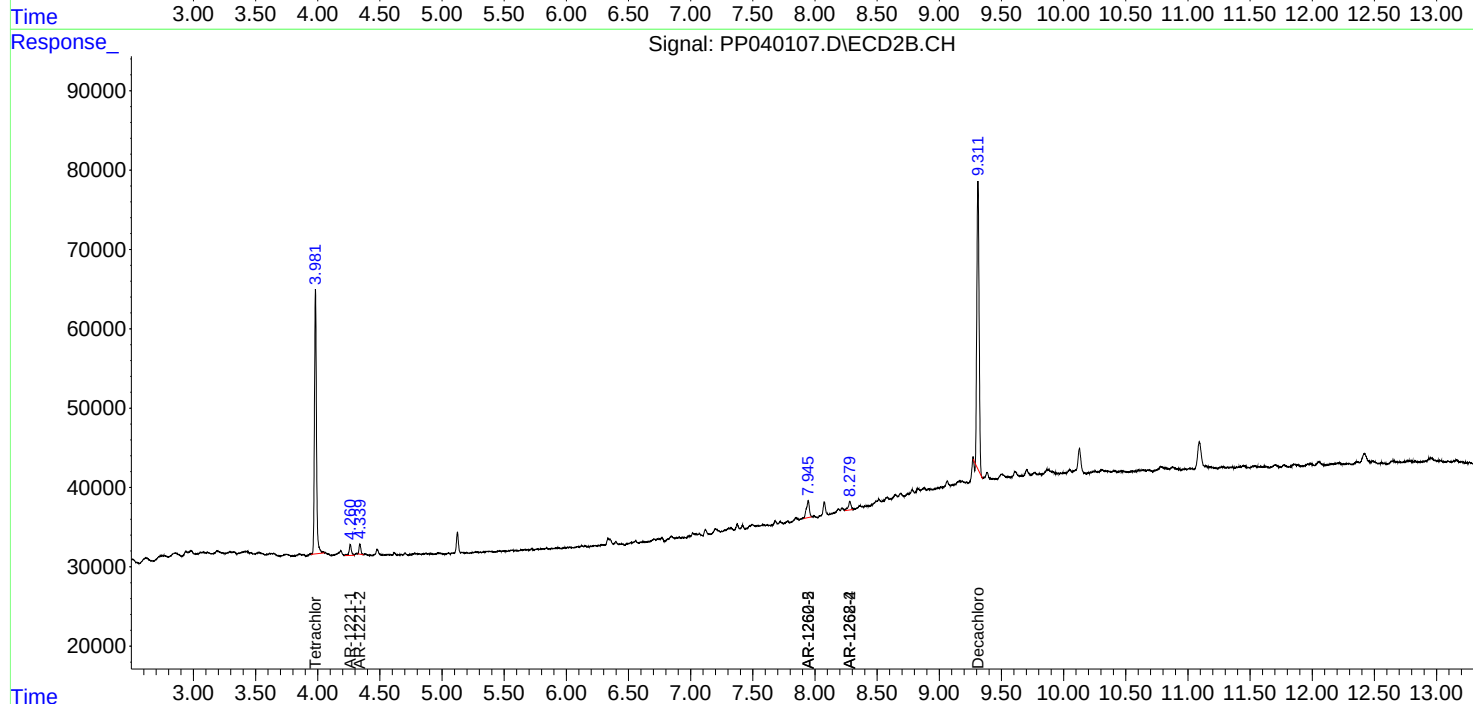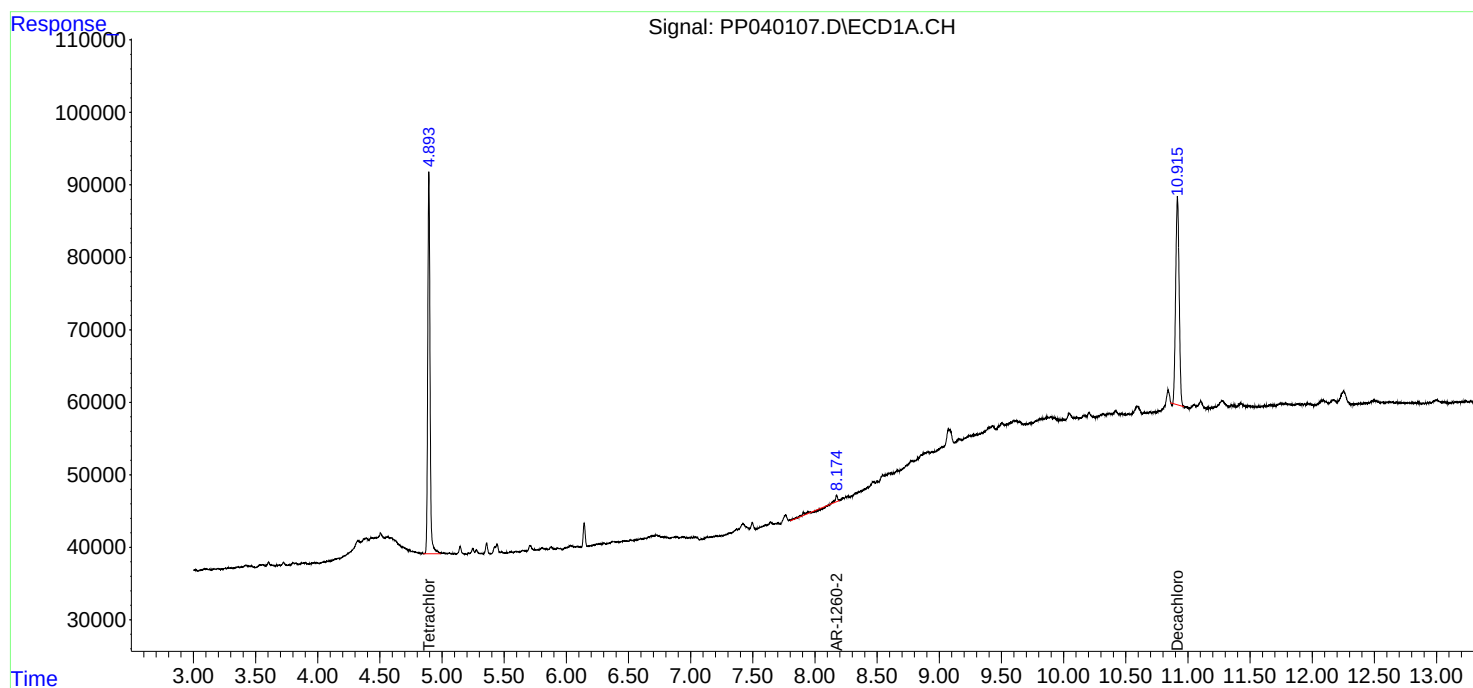


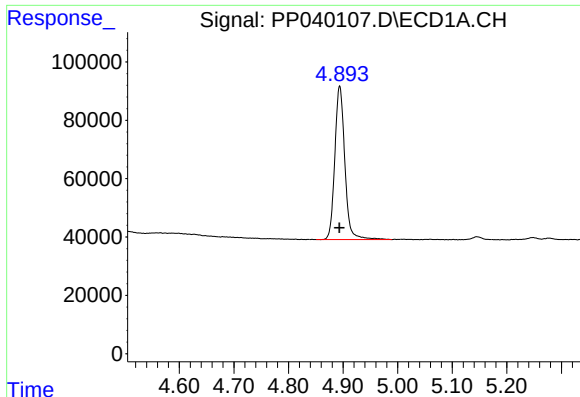

#1 Tetrachloro-m-xylene


R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 672099
Conc: 22.13 ng/ml

Instrument :
ECD_P
ClientSampleId :

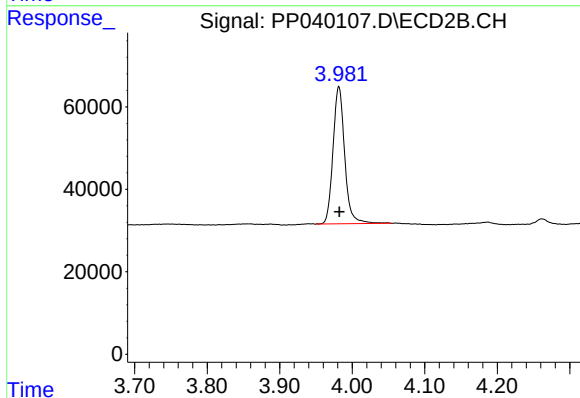


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 371744
Conc: 21.99 ng/ml

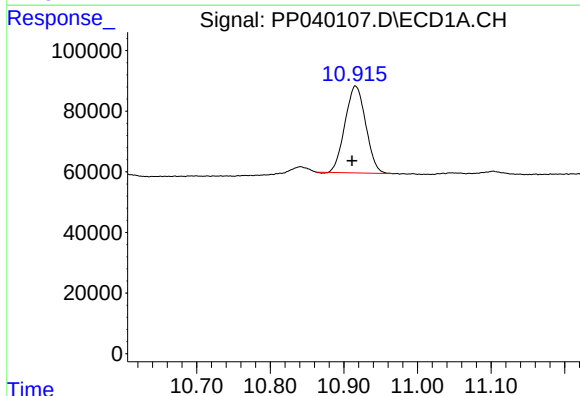


#2 Decachlorobiphenyl

R.T.: 10.916 min
Delta R.T.: 0.005 min
Response: 559803
Conc: 22.65 ng/ml

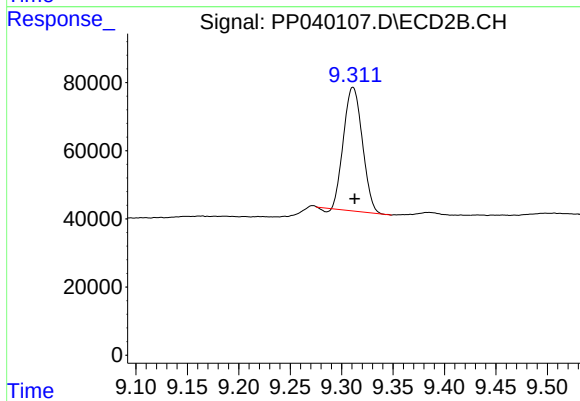

#2 Decachlorobiphenyl


R.T.: 9.311 min
Delta R.T.: -0.002 min
Response: 461317
Conc: 21.74 ng/ml

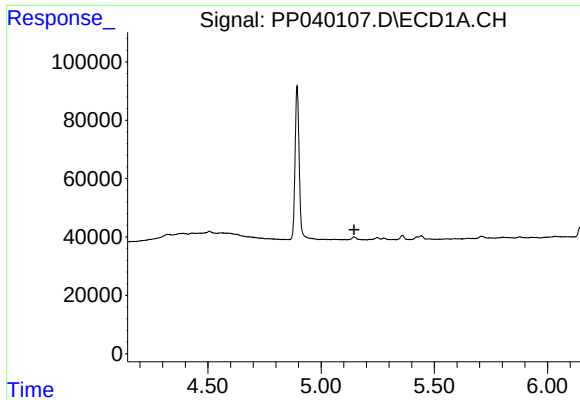

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 5.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

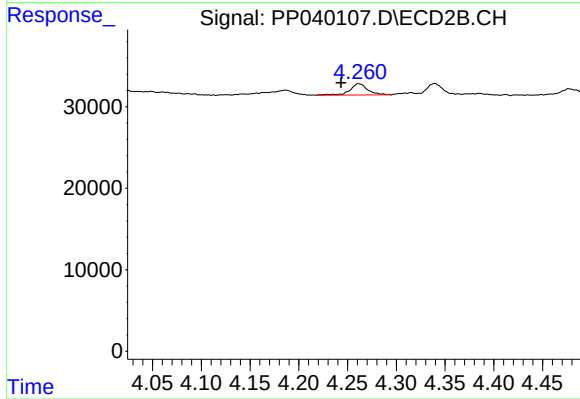


#8 AR-1221-1

R.T.: 4.261 min
Delta R.T.: 0.018 min
Response: 17858
Conc: 87.26 ng/ml

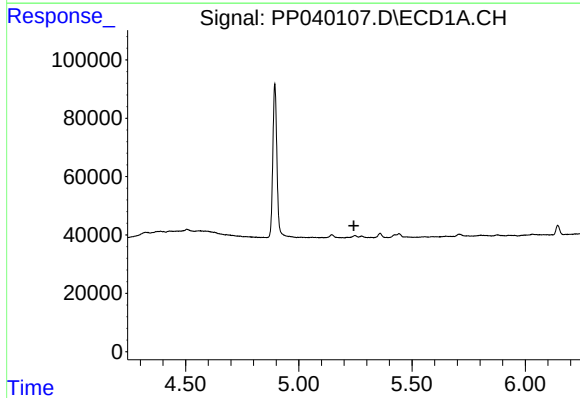


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.243 min
Response: 0
Conc: N.D.

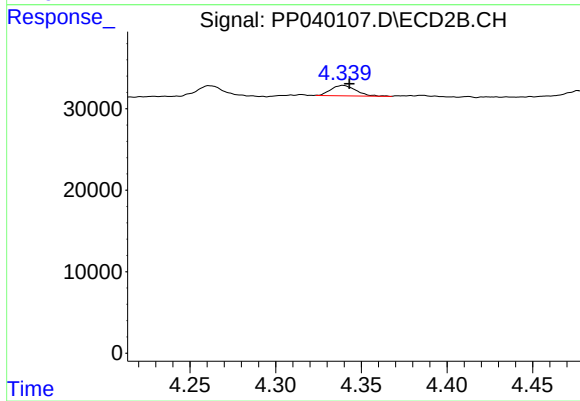

#9 AR-1221-2


R.T.: 4.339 min
Delta R.T.: -0.004 min
Response: 12999
Conc: 77.28 ng/ml

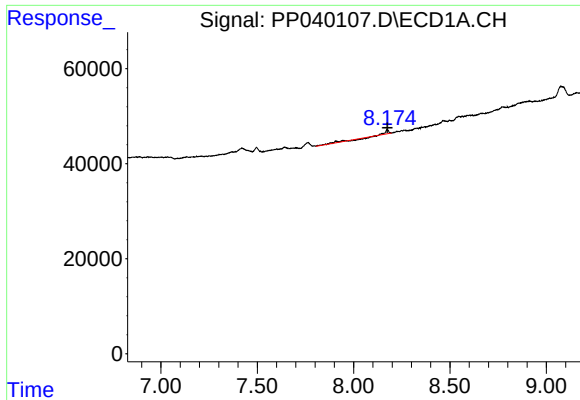

#32 AR-1260-2


R.T.: 8.174 min
Delta R.T.: 0.000 min
Response: 14616
Conc: 10.69 ng/ml

Instrument :
ECD_P
ClientSampleId :

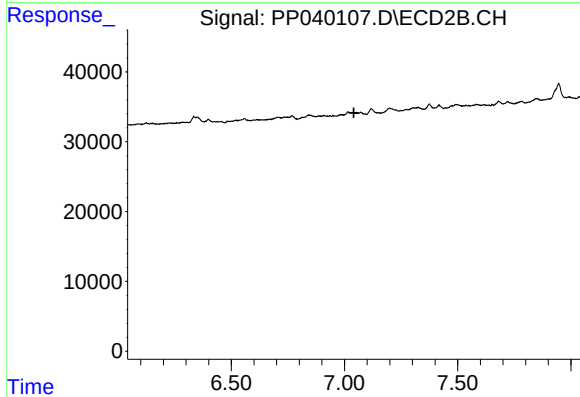


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.042 min
Response: 0
Conc: N.D.

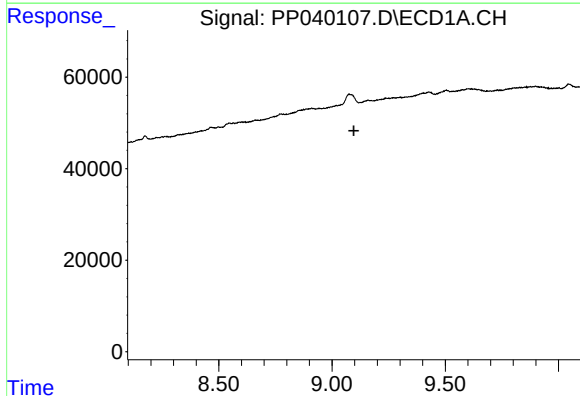


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 9.097 min
Response: 0
Conc: N.D.

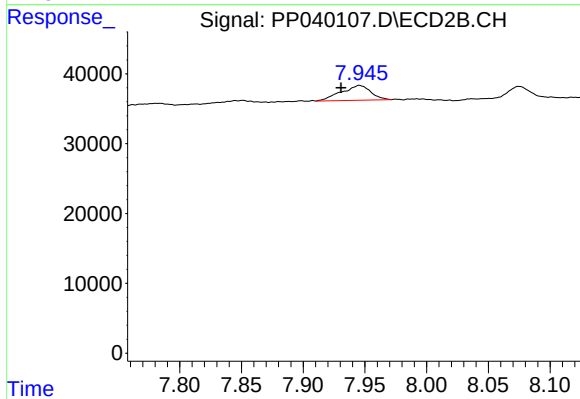

#35 AR-1260-5


R.T.: 7.945 min
Delta R.T.: 0.015 min
Response: 35486
Conc: 17.36 ng/ml

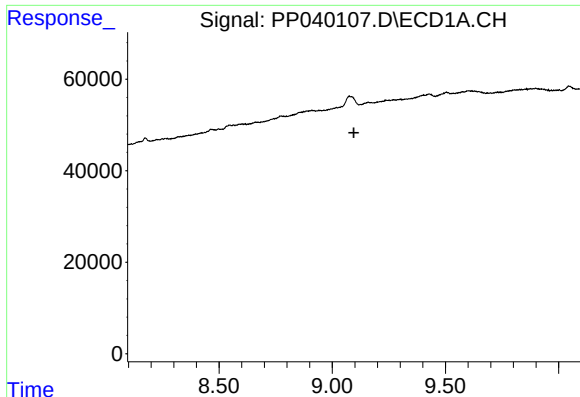

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 9.096 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

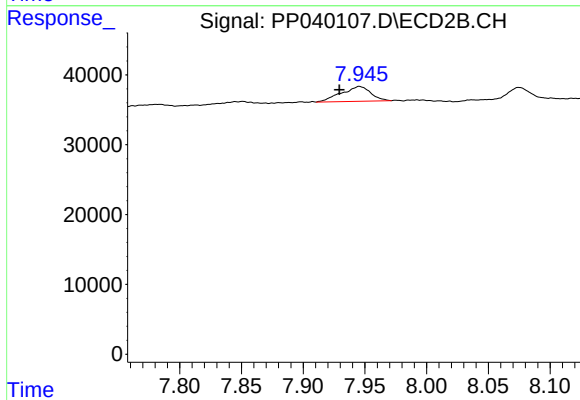


#37 AR-1262-2

R.T.: 7.945 min
Delta R.T.: 0.016 min
Response: 35486
Conc: 15.77 ng/ml

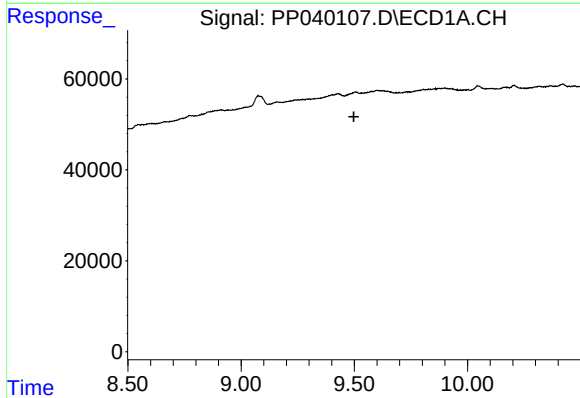


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 9.498 min
Response: 0
Conc: N.D.

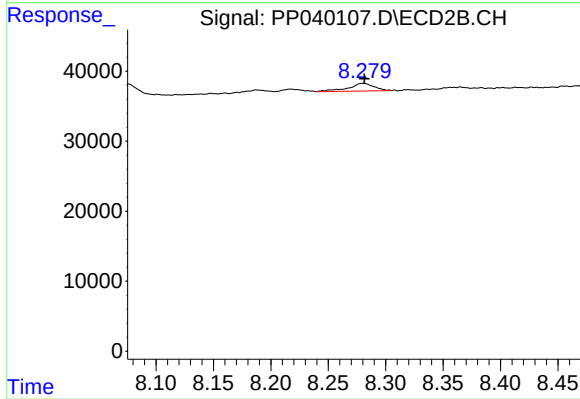

#39 AR-1262-4


R.T.: 8.280 min
Delta R.T.: -0.002 min
Response: 17013
Conc: 9.60 ng/ml

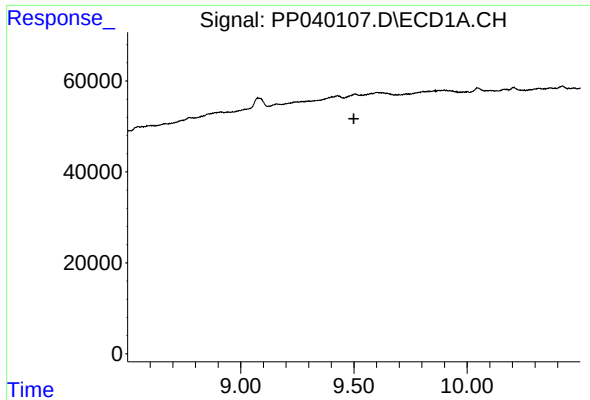

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 9.500 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

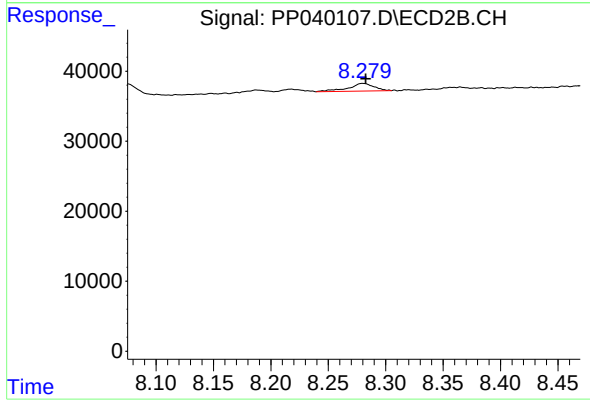

#42 AR-1268-2

R.T.: 8.280 min
Delta R.T.: -0.003 min
Response: 17013
Conc: 6.80 ng/ml