

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101521\
 Data File : PP040132.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Oct 2021 4:38
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:41:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.893	3.981	717488	389581	23.626	23.044
2)	SA Decachlor...	10.913	9.307	624966	555646	25.285	26.182
Target Compounds							
10)	L2 AR-1221-3	0.000	4.420	0	8840	N.D.	16.323 #
11)	L3 AR-1232-1	0.000	4.420	0	8840	N.D.	21.764 #
20)	L4 AR-1242-5	0.000	6.147f	0	16103	N.D.	33.762 #
25)	L5 AR-1248-5	0.000	6.147f	0	16103	N.D.	25.813 #
26)	L6 AR-1254-1	0.000	6.147f	0	16103	N.D.	16.809 #
28)	L6 AR-1254-3	7.758f	0.000	32322	0	22.688	N.D. #
32)	L7 AR-1260-2	8.194f	7.014f	76602	11605	56.046	9.801 #
33)	L7 AR-1260-3	0.000	7.189	0	18450	N.D.	15.616 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101521\
Data File : PP040132.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Oct 2021 4:38
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:41:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

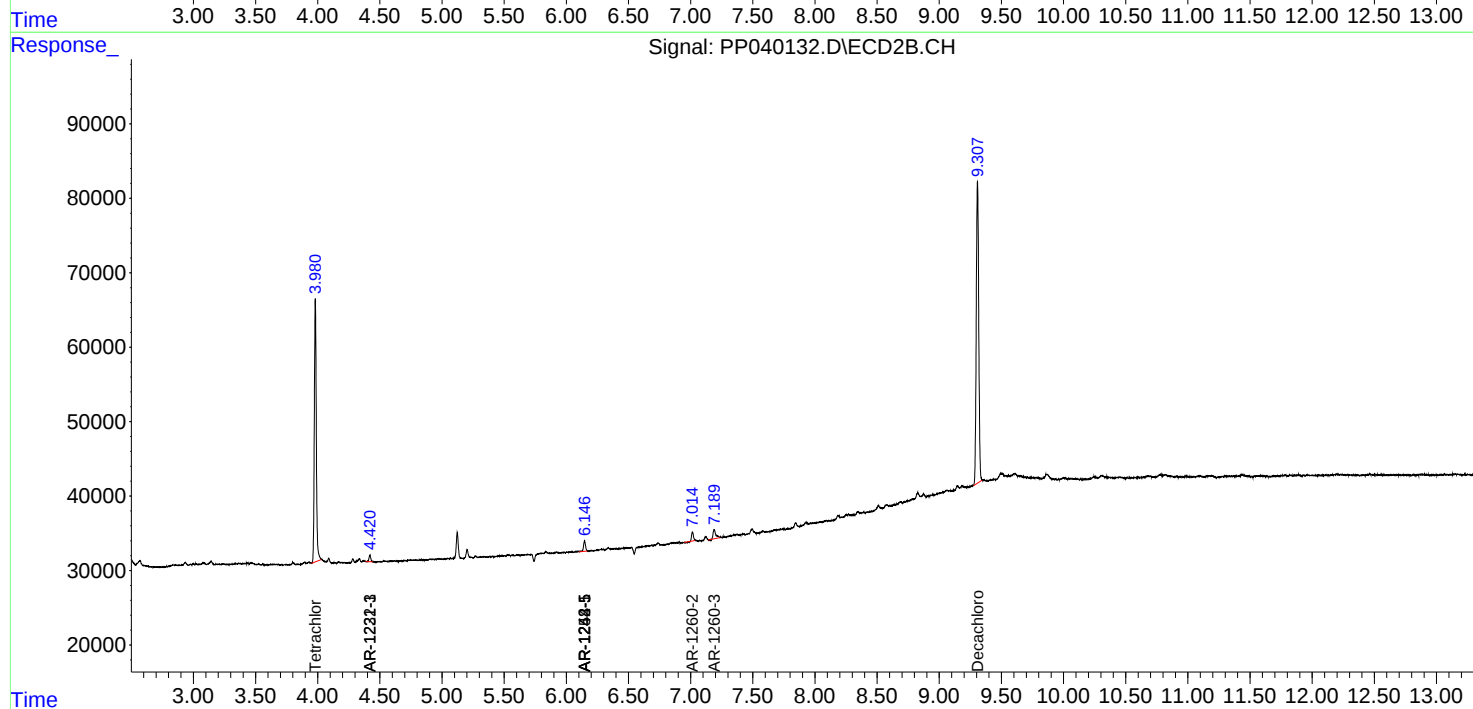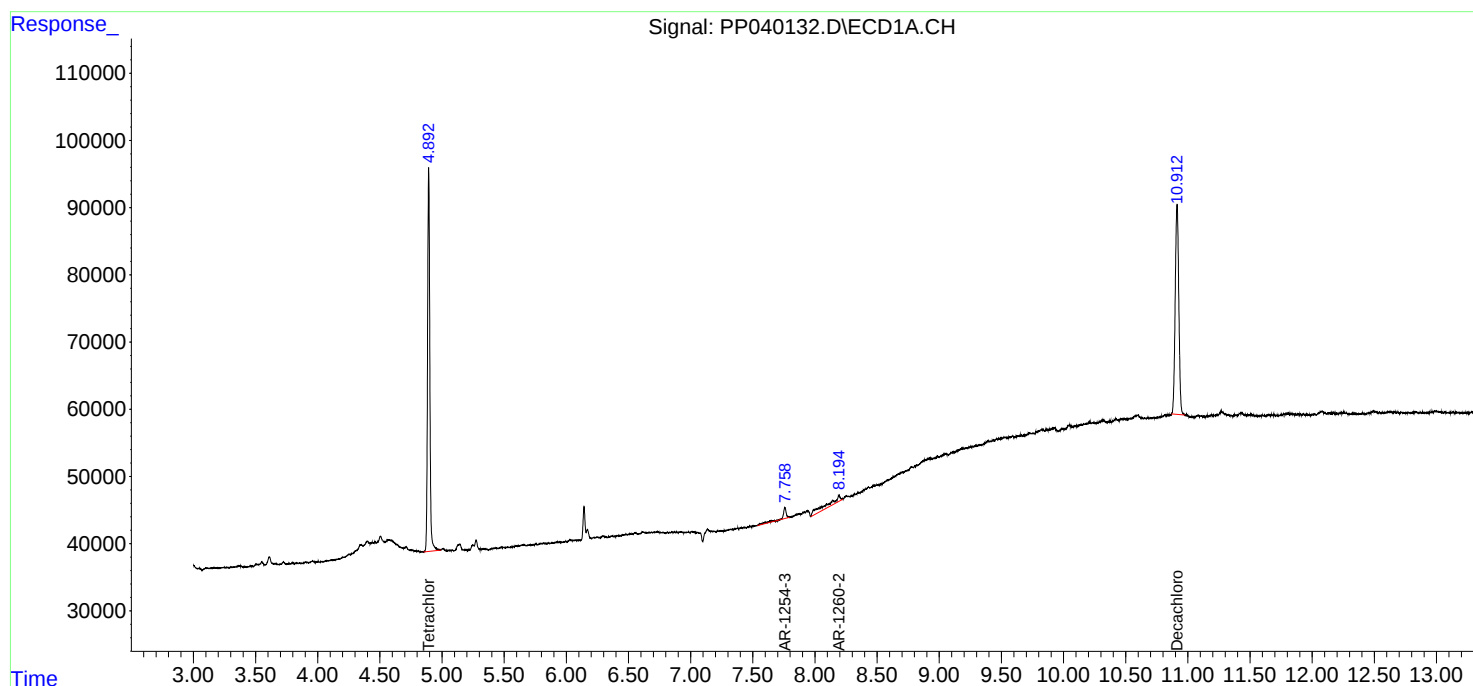


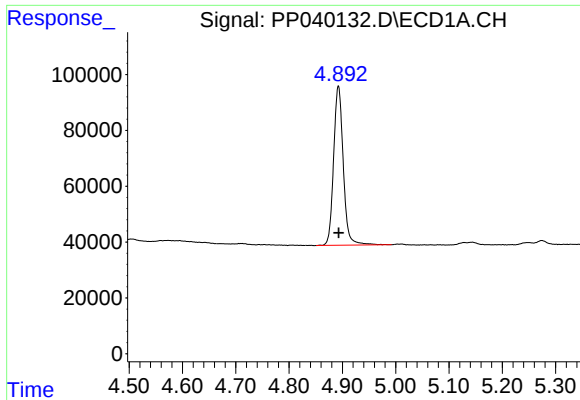

#1 Tetrachloro-m-xylene


R.T.: 4.893 min
Delta R.T.: 0.000 min
Response: 717488
Conc: 23.63 ng/ml

Instrument :
ECD_P
ClientSampleId :

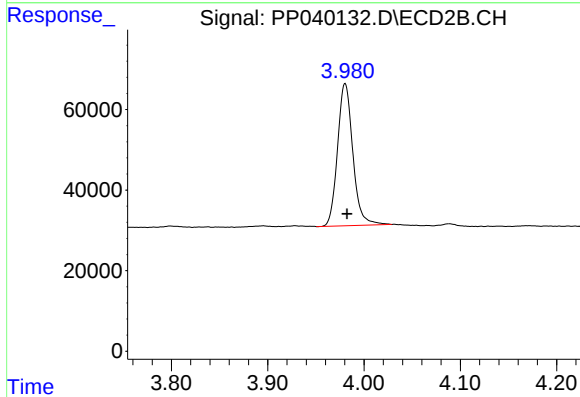


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: -0.002 min
Response: 389581
Conc: 23.04 ng/ml

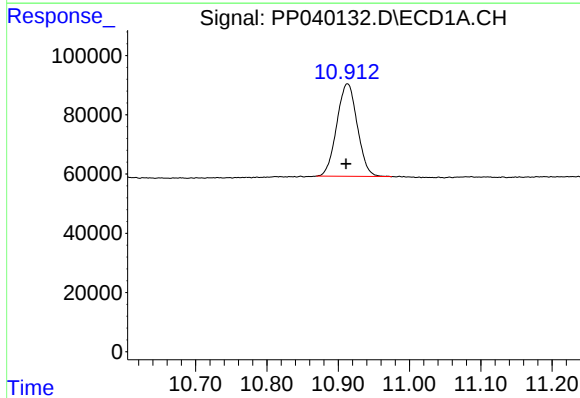


#2 Decachlorobiphenyl

R.T.: 10.913 min
Delta R.T.: 0.002 min
Response: 624966
Conc: 25.29 ng/ml

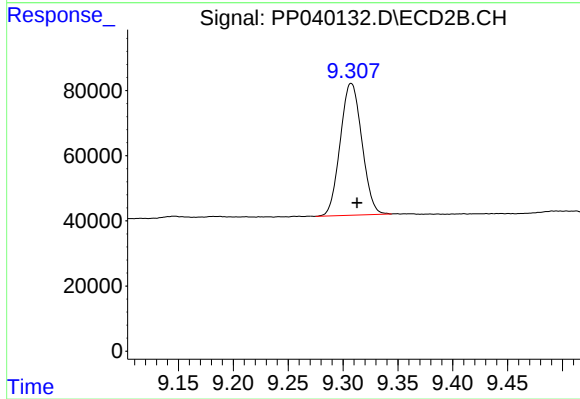

#2 Decachlorobiphenyl


R.T.: 9.307 min
Delta R.T.: -0.005 min
Response: 555646
Conc: 26.18 ng/ml

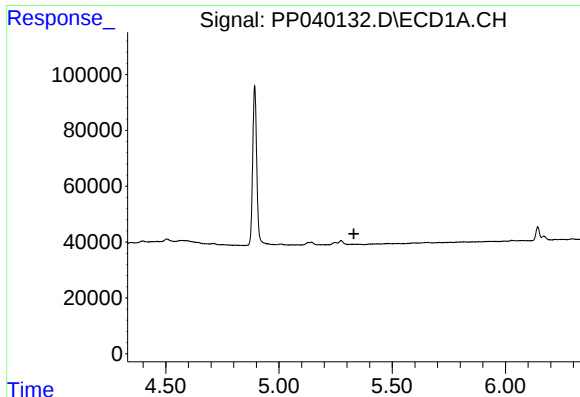

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 5.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

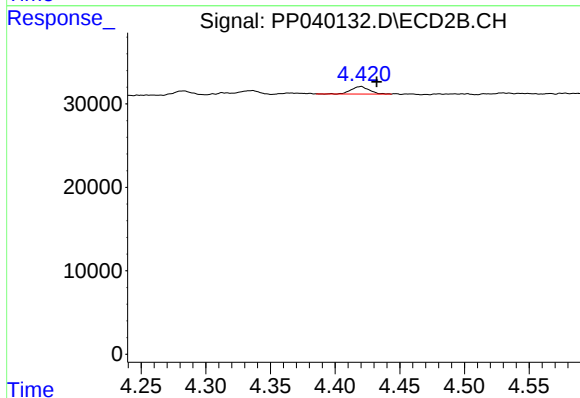


#10 AR-1221-3

R.T.: 4.420 min
Delta R.T.: -0.012 min
Response: 8840
Conc: 16.32 ng/ml

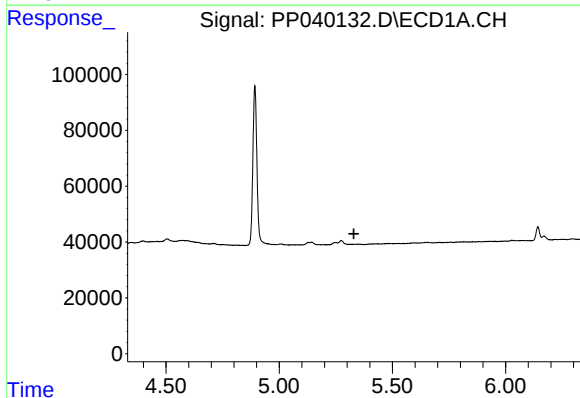


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 5.330 min
Response: 0
Conc: N.D.

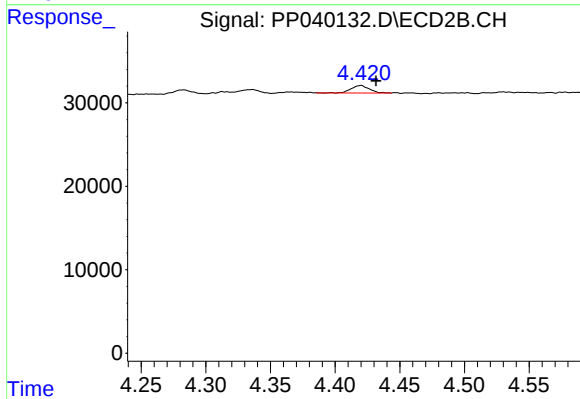

#11 AR-1232-1


R.T.: 4.420 min
Delta R.T.: -0.011 min
Response: 8840
Conc: 21.76 ng/ml

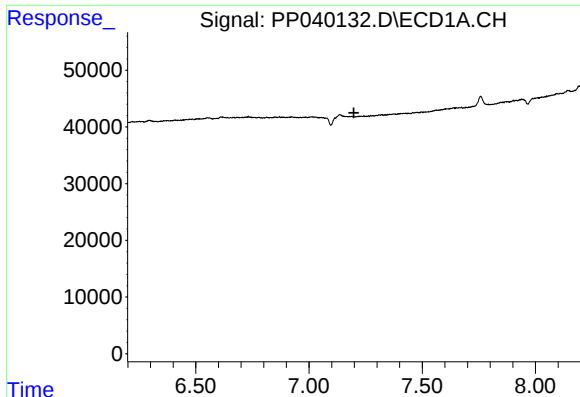

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.198 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

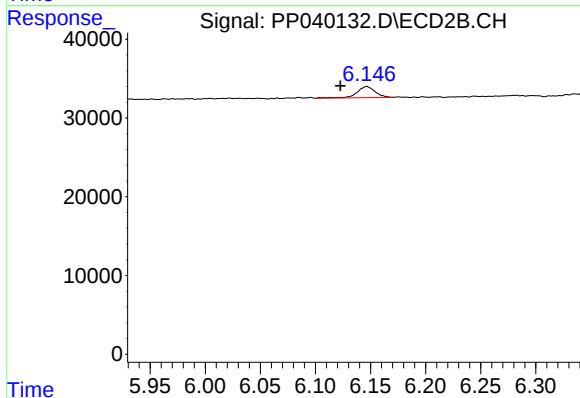


#20 AR-1242-5

R.T.: 6.147 min
Delta R.T.: 0.024 min
Response: 16103
Conc: 33.76 ng/ml

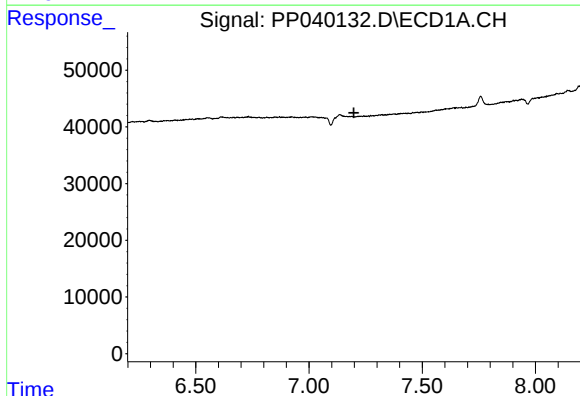


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 7.198 min
Response: 0
Conc: N.D.

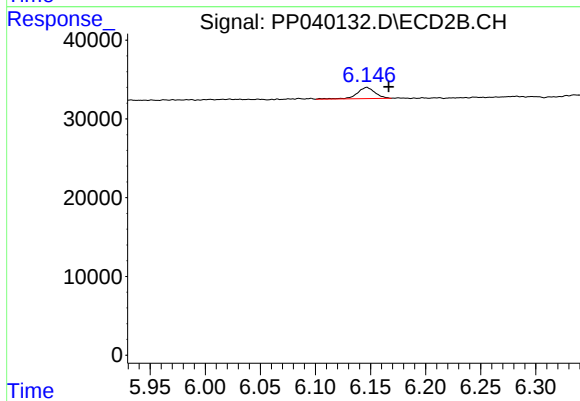

#25 AR-1248-5


R.T.: 6.147 min
Delta R.T.: -0.020 min
Response: 16103
Conc: 25.81 ng/ml

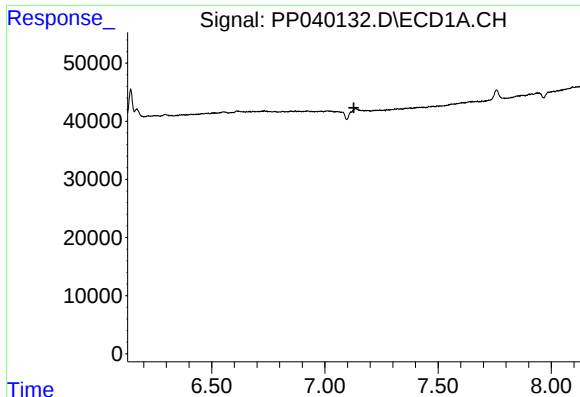

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 7.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

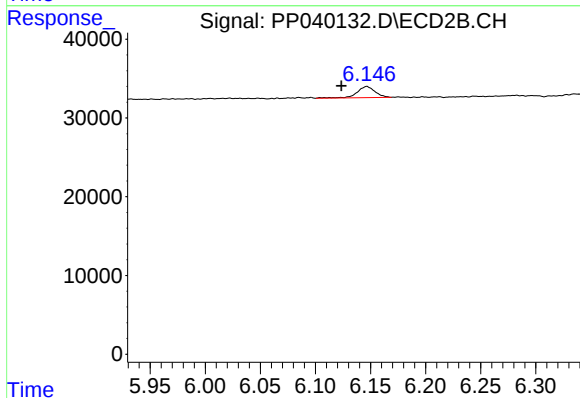


#26 AR-1254-1

R.T.: 6.147 min
Delta R.T.: 0.023 min
Response: 16103
Conc: 16.81 ng/ml

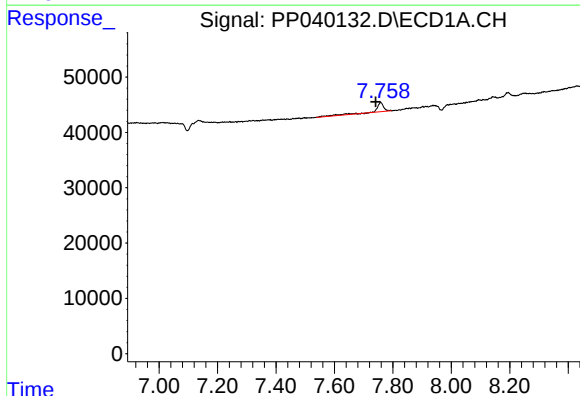


#28 AR-1254-3

R.T.: 7.758 min
Delta R.T.: 0.017 min
Response: 32322
Conc: 22.69 ng/ml

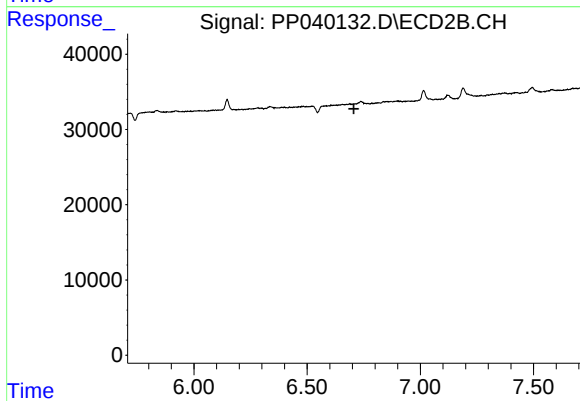

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.706 min
Response: 0
Conc: N.D.

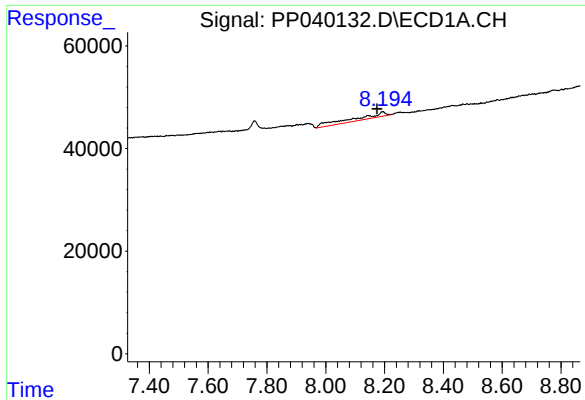

#32 AR-1260-2


R.T.: 8.194 min
Delta R.T.: 0.019 min
Response: 76602
Conc: 56.05 ng/ml

Instrument :
ECD_P
ClientSampleId :

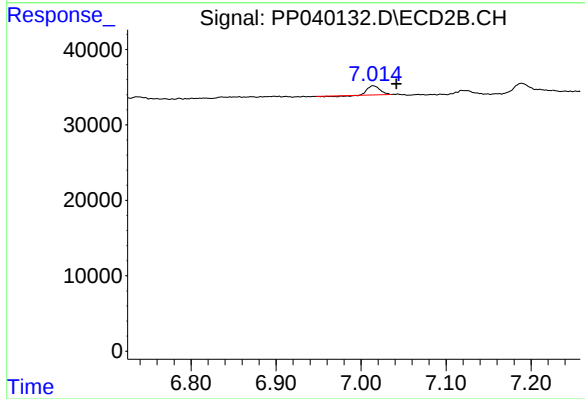


#32 AR-1260-2

R.T.: 7.014 min
Delta R.T.: -0.028 min
Response: 11605
Conc: 9.80 ng/ml

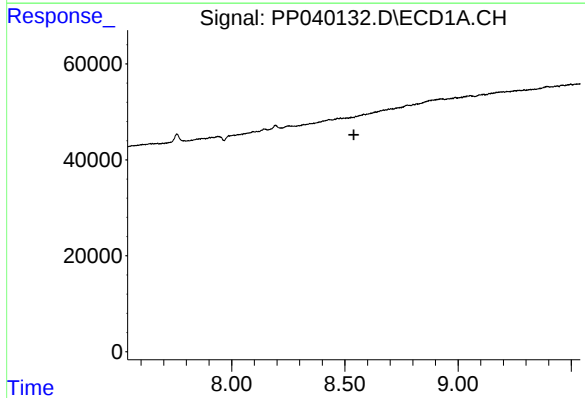

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.540 min
Response: 0
Conc: N.D.

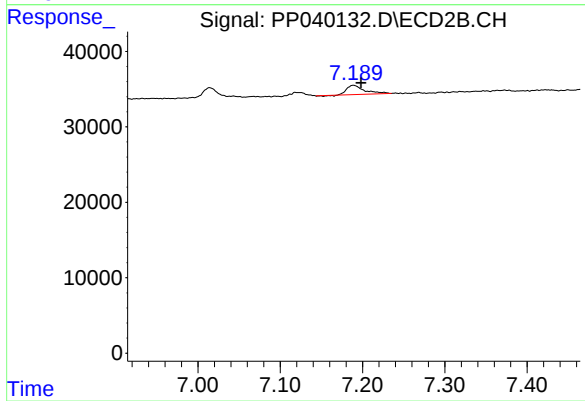

#33 AR-1260-3

R.T.: 7.189 min
Delta R.T.: -0.009 min
Response: 18450
Conc: 15.62 ng/ml