

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101521\
 Data File : PP040082.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2021 10:57
 Operator : AJ\MA
 Sample : M4165-02RE 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 732910-10-06-21-02RE

Manual Integrations
 APPROVED

mohammad
 10/18/2021 2:40:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:43:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.893	3.981	15757	33777	0.519m	1.998 #
2) SA Decachlor...	10.916	9.306	19156	87389	0.775m	4.118 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101521\
Data File : PP040082.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2021 10:57
Operator : AJ\MA
Sample : M4165-02RE 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
732910-10-06-21-02RE


Manual Integrations
APPROVED

mohammad
10/18/2021 2:40:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:43:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

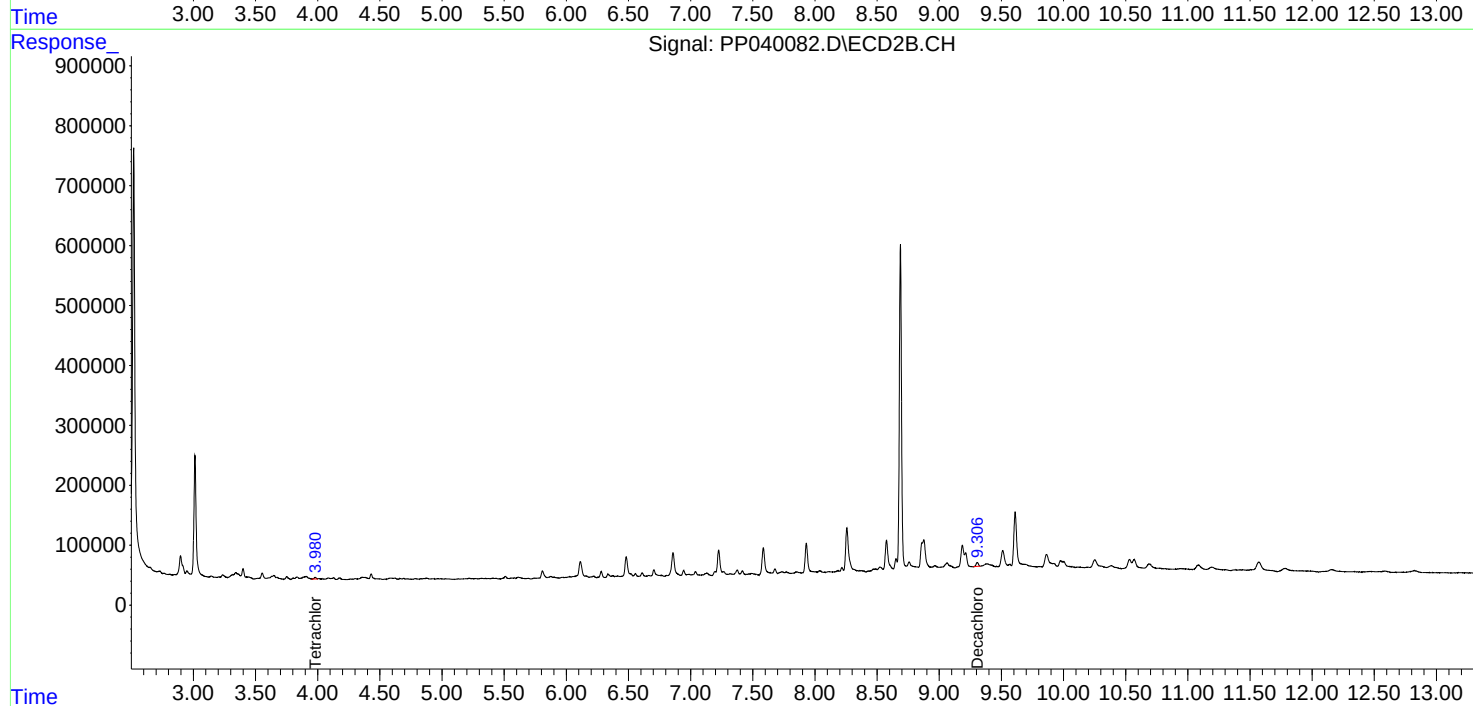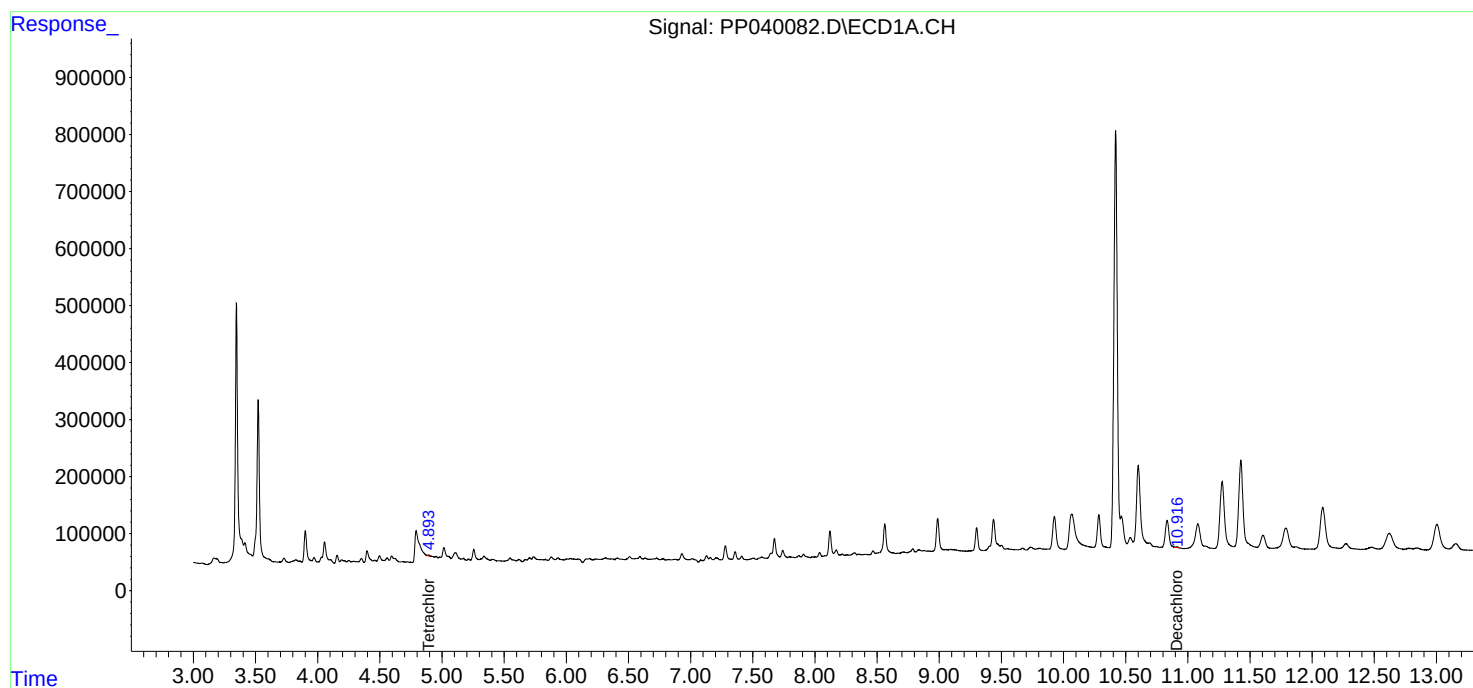

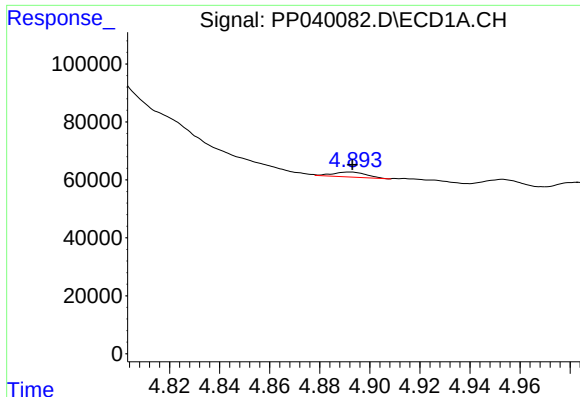


#1 Tetrachloro-m-xylene

R.T.: 4.893 min
Delta R.T.: 0.000 min
Response: 15757
Conc: 0.52 ng/ml m

Instrument :
ECD_P
ClientSampleId :
732910-10-06-21-02RE


Manual Integrations
APPROVED

mohammad
10/18/2021 2:40:59 PM

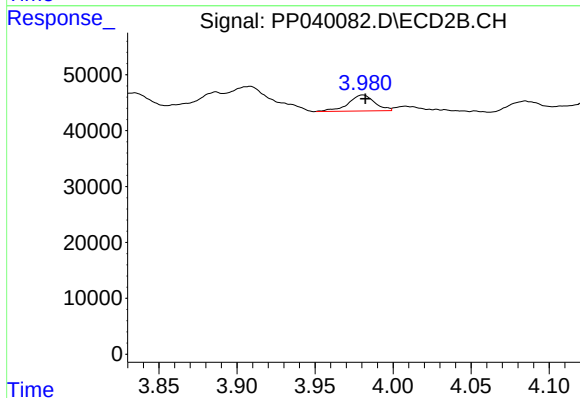


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: -0.002 min
Response: 33777
Conc: 2.00 ng/ml

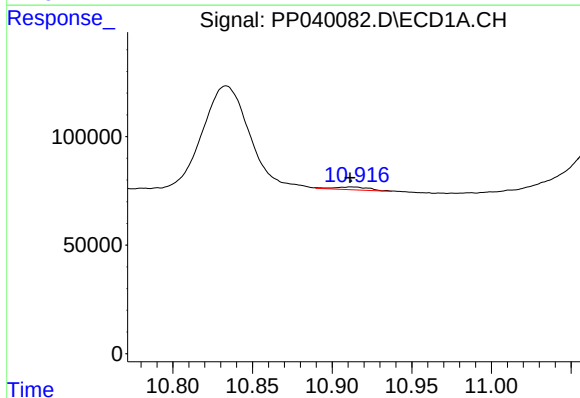

#2 Decachlorobiphenyl

R.T.: 10.916 min
Delta R.T.: 0.004 min
Response: 19156
Conc: 0.78 ng/ml m

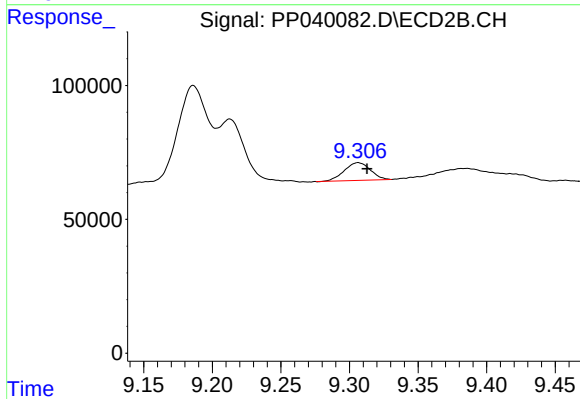

#2 Decachlorobiphenyl

R.T.: 9.306 min
Delta R.T.: -0.006 min
Response: 87389
Conc: 4.12 ng/ml