

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101521\
 Data File : PP040126.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Oct 2021 2:17
 Operator : AJ\MA
 Sample : M4250-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PIPESEG-A

Manual Integrations
 APPROVED

mohammad
 10/18/2021 2:41:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:39:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.893	3.981	600262	419990	19.766	24.843m#
2) SA Decachlor...	10.912	9.309	515989	439458	20.876	20.707

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101521\
Data File : PP040126.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Oct 2021 2:17
Operator : AJ\MA
Sample : M4250-01
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PIPESEG-A


Manual Integrations
APPROVED

mohammad
10/18/2021 2:41:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:39:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

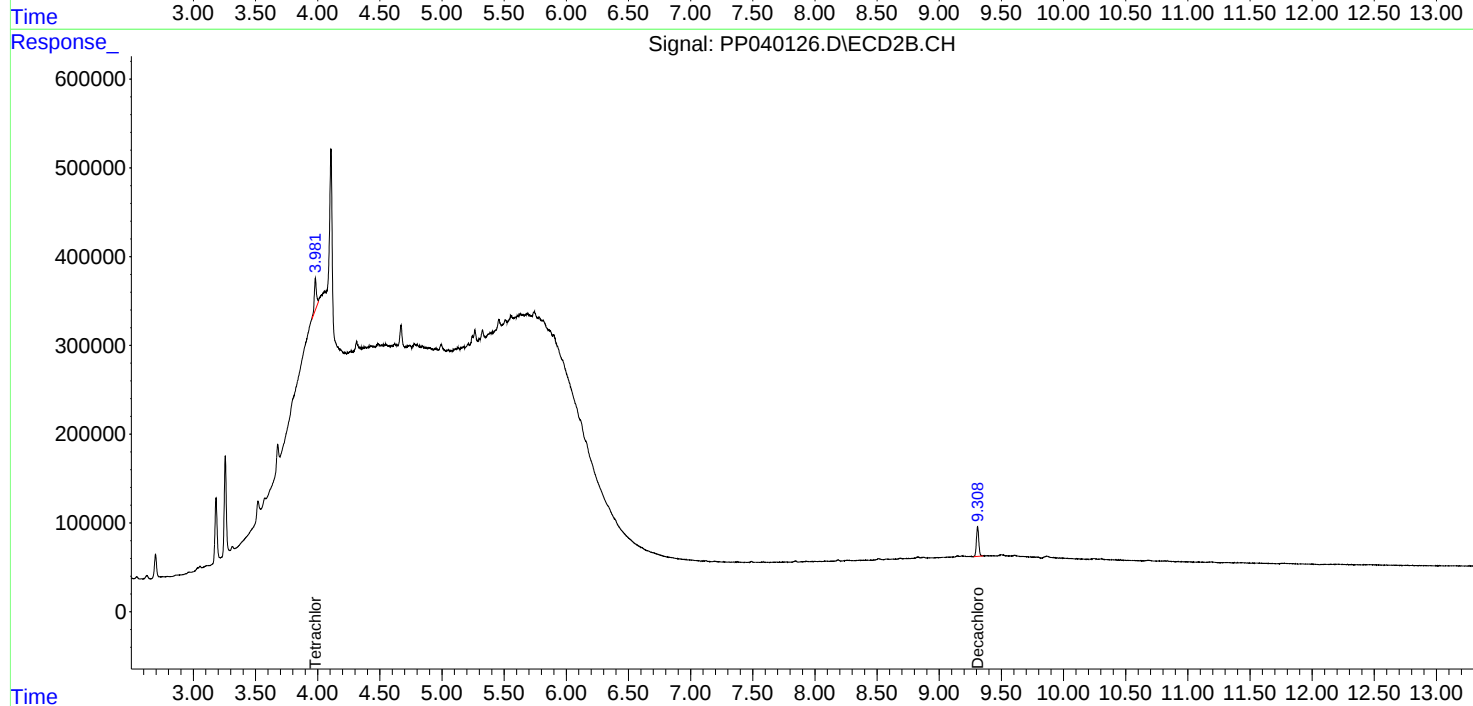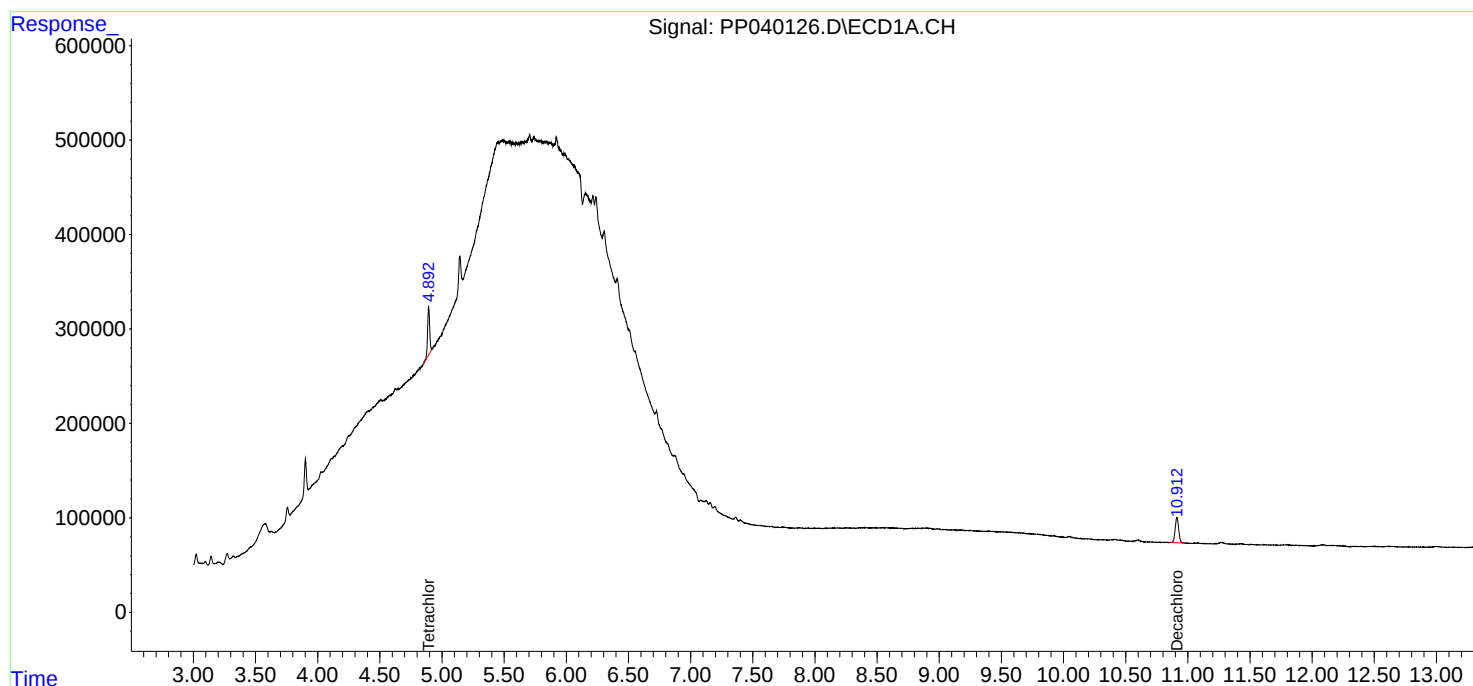

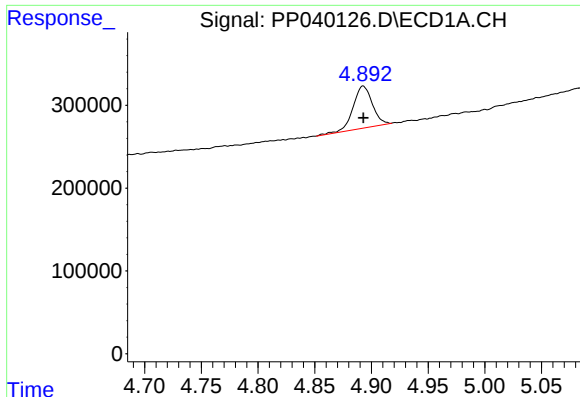


#1 Tetrachloro-m-xylene

R.T.: 4.893 min
Delta R.T.: 0.000 min
Response: 600262
Conc: 19.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
PIPESEG-A


Manual Integrations
APPROVED

mohammad
10/18/2021 2:41:35 PM

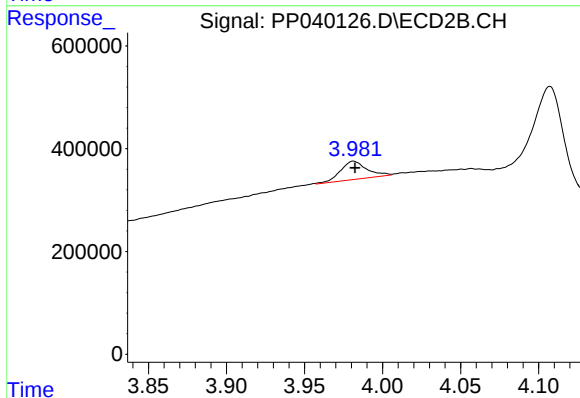


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: -0.002 min
Response: 419990
Conc: 24.84 ng/ml m

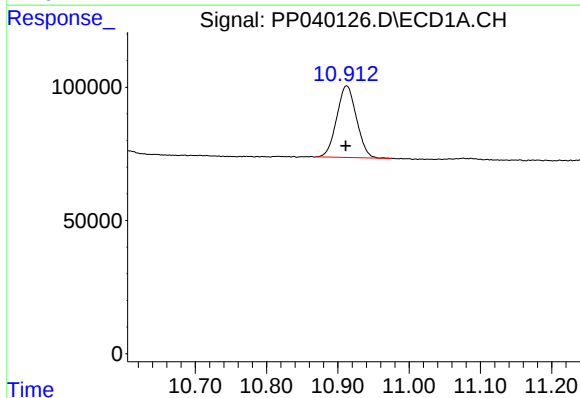

#2 Decachlorobiphenyl

R.T.: 10.912 min
Delta R.T.: 0.001 min
Response: 515989
Conc: 20.88 ng/ml

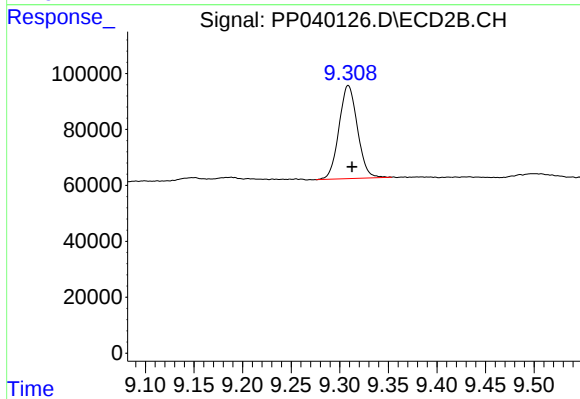

#2 Decachlorobiphenyl

R.T.: 9.309 min
Delta R.T.: -0.004 min
Response: 439458
Conc: 20.71 ng/ml