

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101524\
 Data File : PP067836.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 12:40
 Operator : YP\AJ
 Sample : P4396-01
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WASTE-WATER-FRAC-TANK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 13:12:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.755	4.051	20642702	21190192	22.301	20.972
2) SA Decachlor...	10.668	9.215	19347005	18457923	16.804	16.459
Target Compounds						
26) L6 AR-1254-1	6.775	5.974	7070530	10616464	157.886	179.685
27) L6 AR-1254-2	6.992	6.121	13297386	7551507	201.178	143.936 #
28) L6 AR-1254-3	7.356	6.531	9996390	11270577	143.931	135.451
29) L6 AR-1254-4	7.638	6.759	5955150	5824309	119.331	120.650
30) L6 AR-1254-5	8.057	7.180	5525157	6278771	93.184	85.366



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101524\
Data File : PP067836.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 12:40
Operator : YP\AJ
Sample : P4396-01
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
WASTE-WATER-FRAC-TANK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 13:12:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

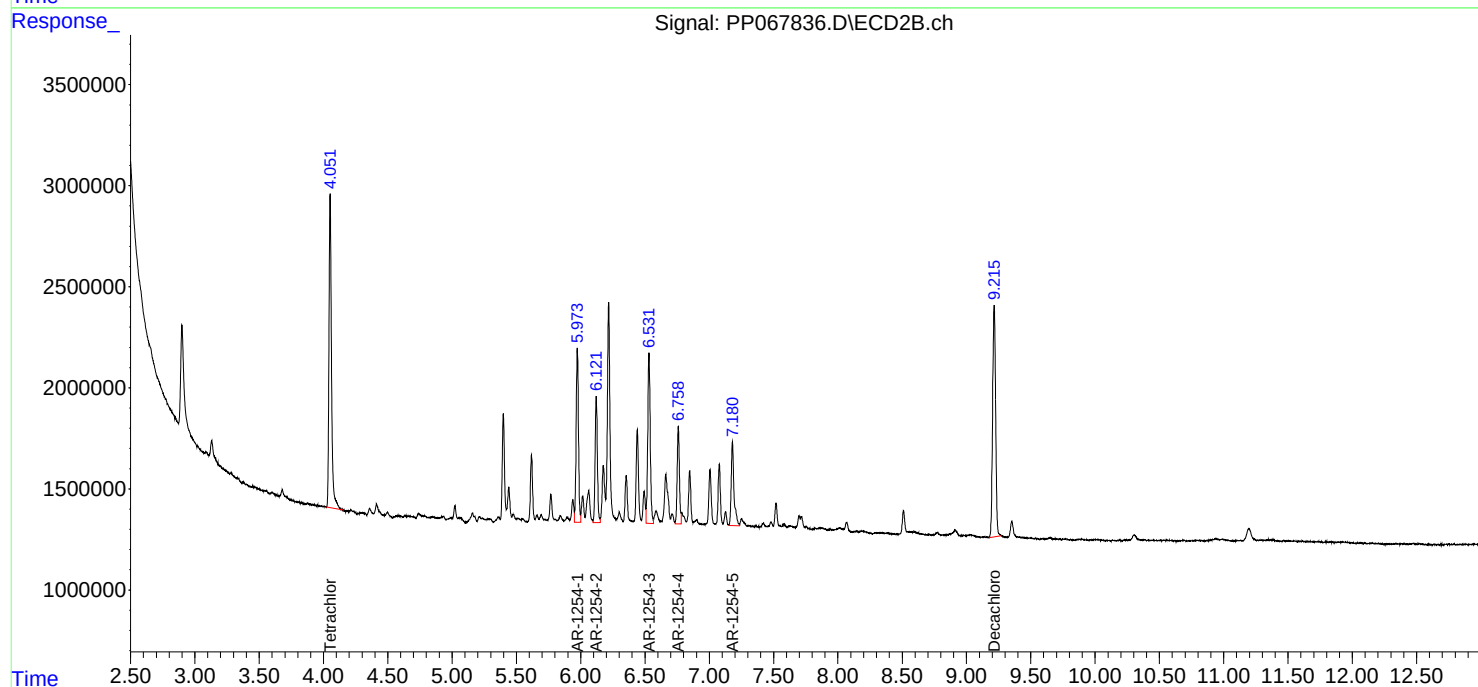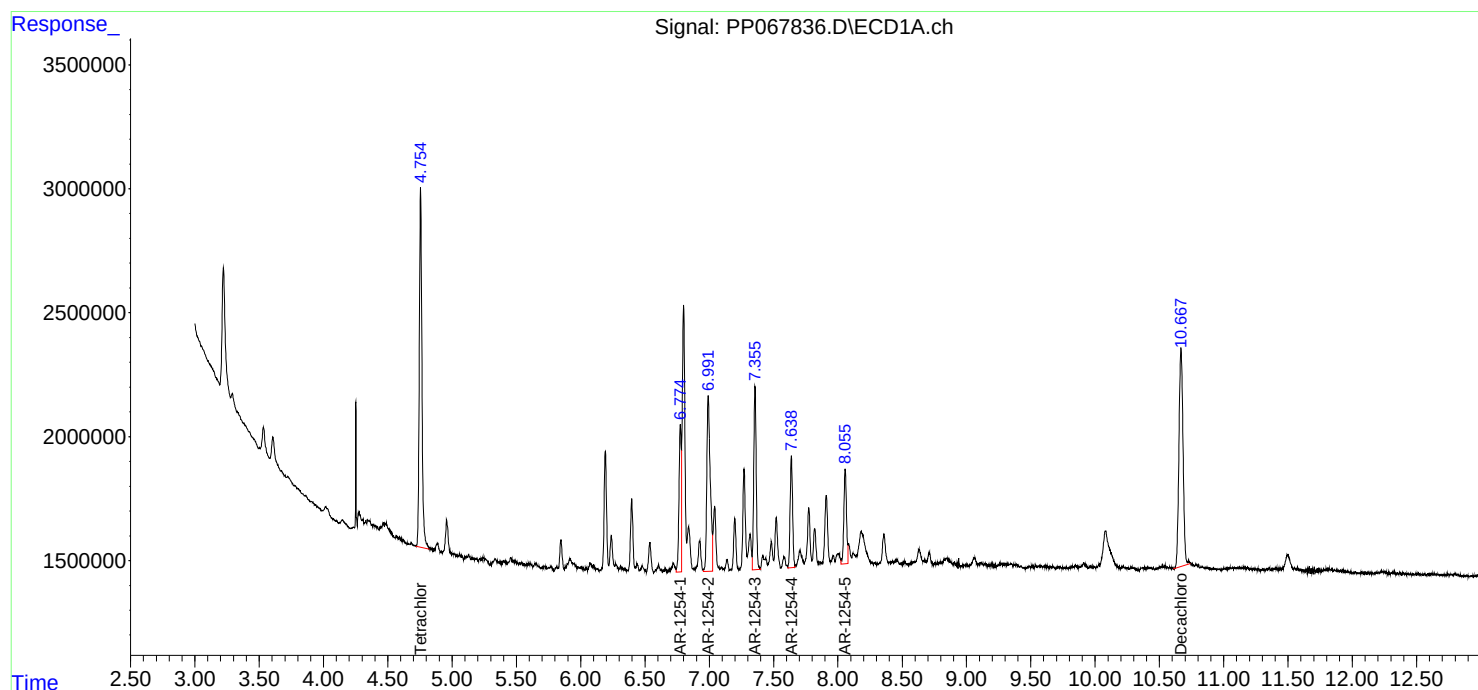


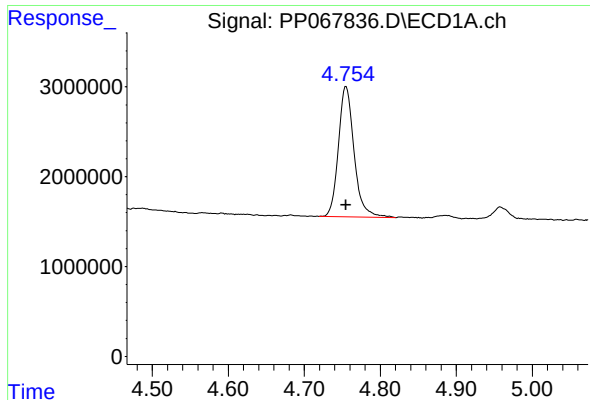

#1 Tetrachloro-m-xylene


R.T.: 4.755 min
Delta R.T.: 0.000 min
Response: 20642702
Conc: 22.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
WASTE-WATER-FRAC-TANK

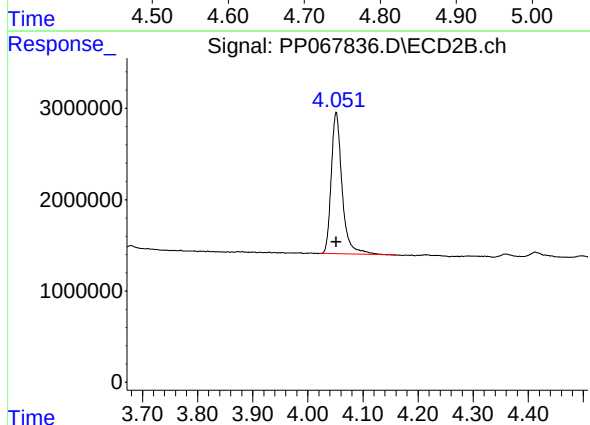


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 21190192
Conc: 20.97 ng/ml

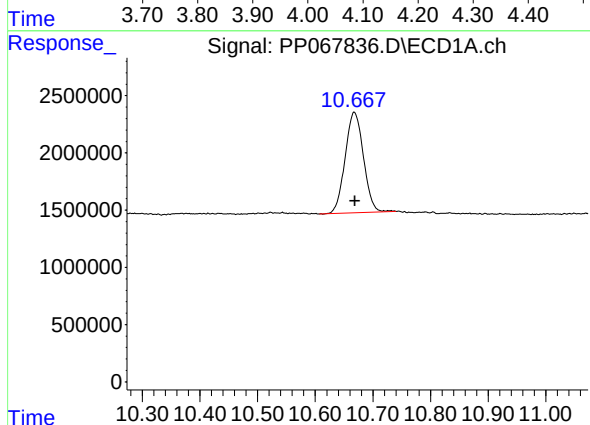


#2 Decachlorobiphenyl

R.T.: 10.668 min
Delta R.T.: -0.001 min
Response: 19347005
Conc: 16.80 ng/ml

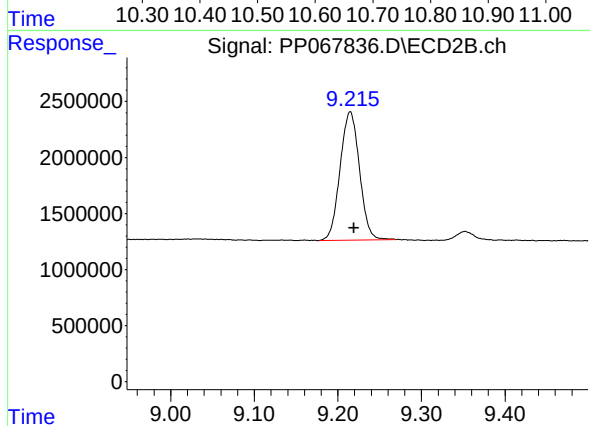

#2 Decachlorobiphenyl


R.T.: 9.215 min
Delta R.T.: -0.004 min
Response: 18457923
Conc: 16.46 ng/ml

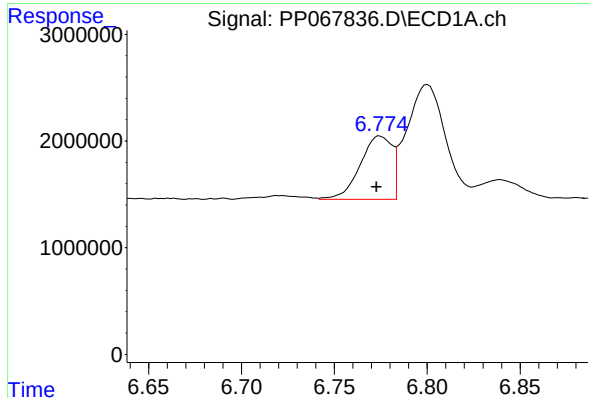

#26 AR-1254-1


R.T.: 6.775 min
Delta R.T.: 0.002 min
Response: 7070530
Conc: 157.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
WASTE-WATER-FRAC-TANK

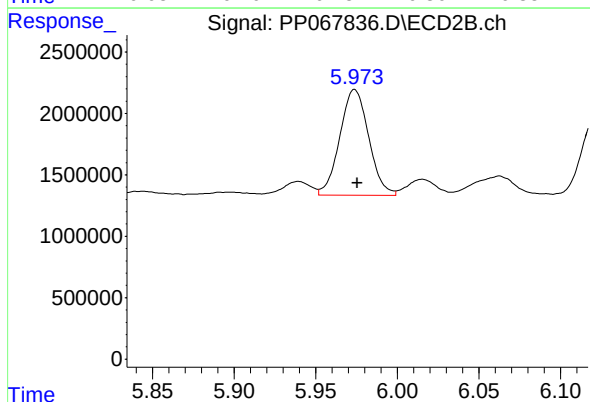


#26 AR-1254-1

R.T.: 5.974 min
Delta R.T.: -0.002 min
Response: 10616464
Conc: 179.68 ng/ml

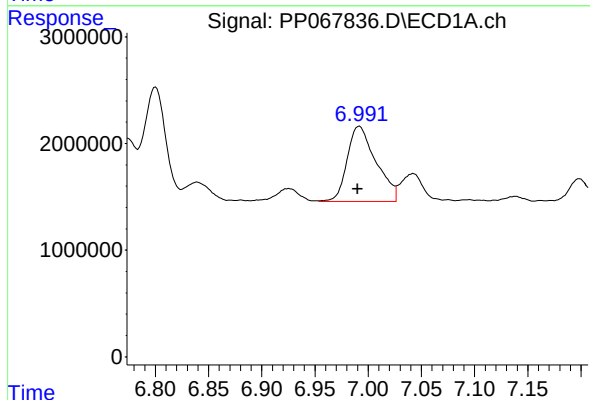


#27 AR-1254-2

R.T.: 6.992 min
Delta R.T.: 0.002 min
Response: 13297386
Conc: 201.18 ng/ml

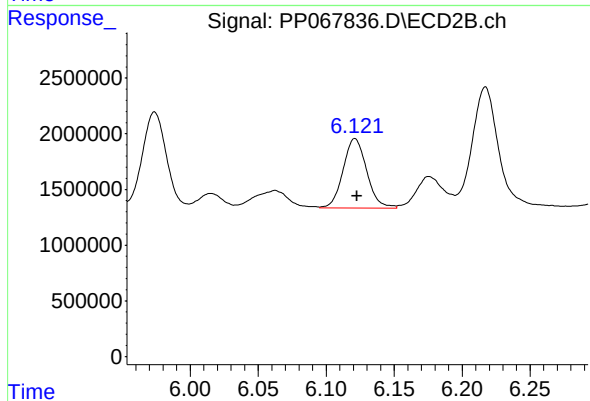

#27 AR-1254-2


R.T.: 6.121 min
Delta R.T.: -0.001 min
Response: 7551507
Conc: 143.94 ng/ml

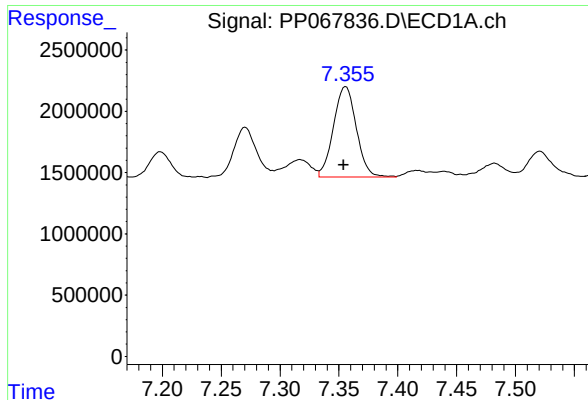

#28 AR-1254-3


R.T.: 7.356 min
Delta R.T.: 0.002 min
Response: 9996390
Conc: 143.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
WASTE-WATER-FRAC-TANK

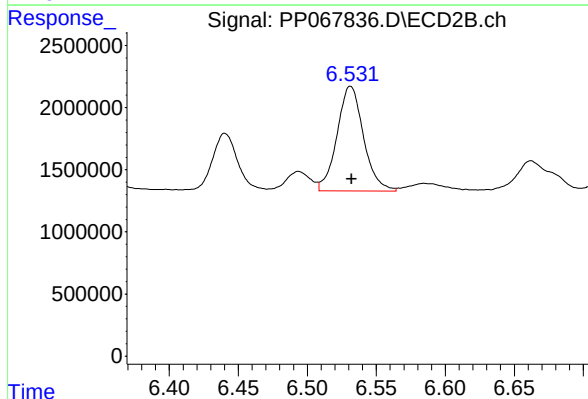


#28 AR-1254-3

R.T.: 6.531 min
Delta R.T.: 0.000 min
Response: 11270577
Conc: 135.45 ng/ml

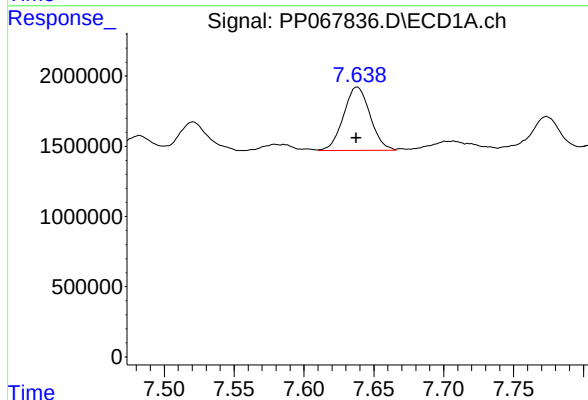


#29 AR-1254-4

R.T.: 7.638 min
Delta R.T.: 0.000 min
Response: 5955150
Conc: 119.33 ng/ml

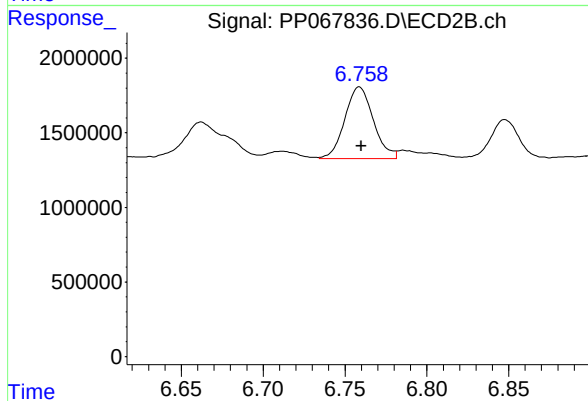

#29 AR-1254-4


R.T.: 6.759 min
Delta R.T.: -0.001 min
Response: 5824309
Conc: 120.65 ng/ml

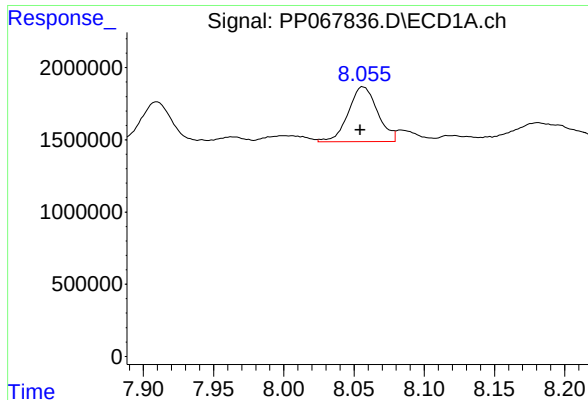

#30 AR-1254-5

R.T.: 8.057 min
Delta R.T.: 0.002 min
Response: 5525157
Conc: 93.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
WASTE-WATER-FRAC-TANK

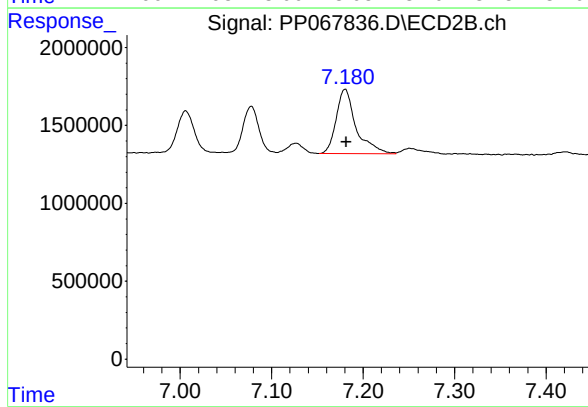

#30 AR-1254-5

R.T.: 7.180 min
Delta R.T.: -0.001 min
Response: 6278771
Conc: 85.37 ng/ml