

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101524\
 Data File : PP067837.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 13:00
 Operator : YP\AJ
 Sample : P4402-02RE
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 2 - DrumRE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/16/2024
 Supervised By :Ankita Jodhani 10/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 13:14:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.761	4.052	7539437	9924448	8.145	9.822m
2) SA Decachlor...	10.675	9.218	5800486	5634417	5.038m	5.024

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101524\
Data File : PP067837.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 13:00
Operator : YP\AJ
Sample : P4402-02RE
Misc :
ALS Vial : 55 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
2 - DrumRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/16/2024
Supervised By :Ankita Jodhani 10/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 13:14:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

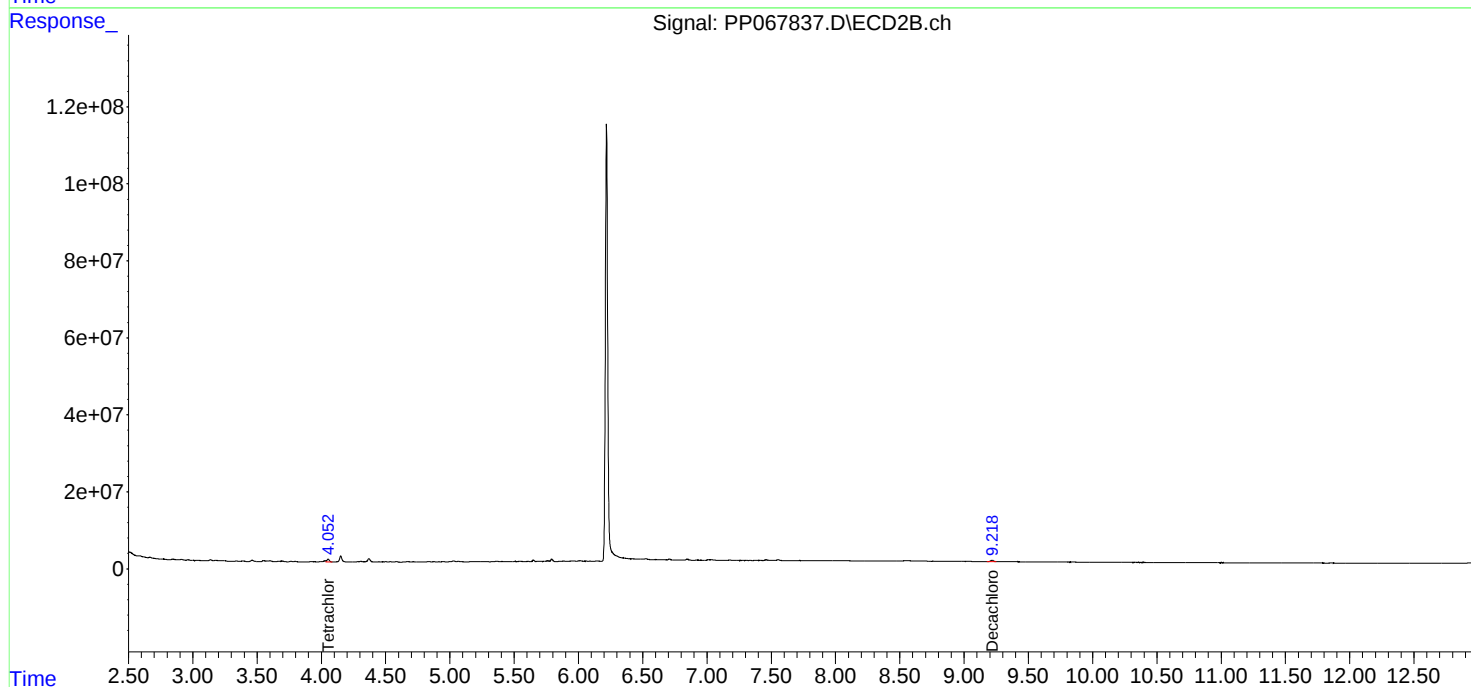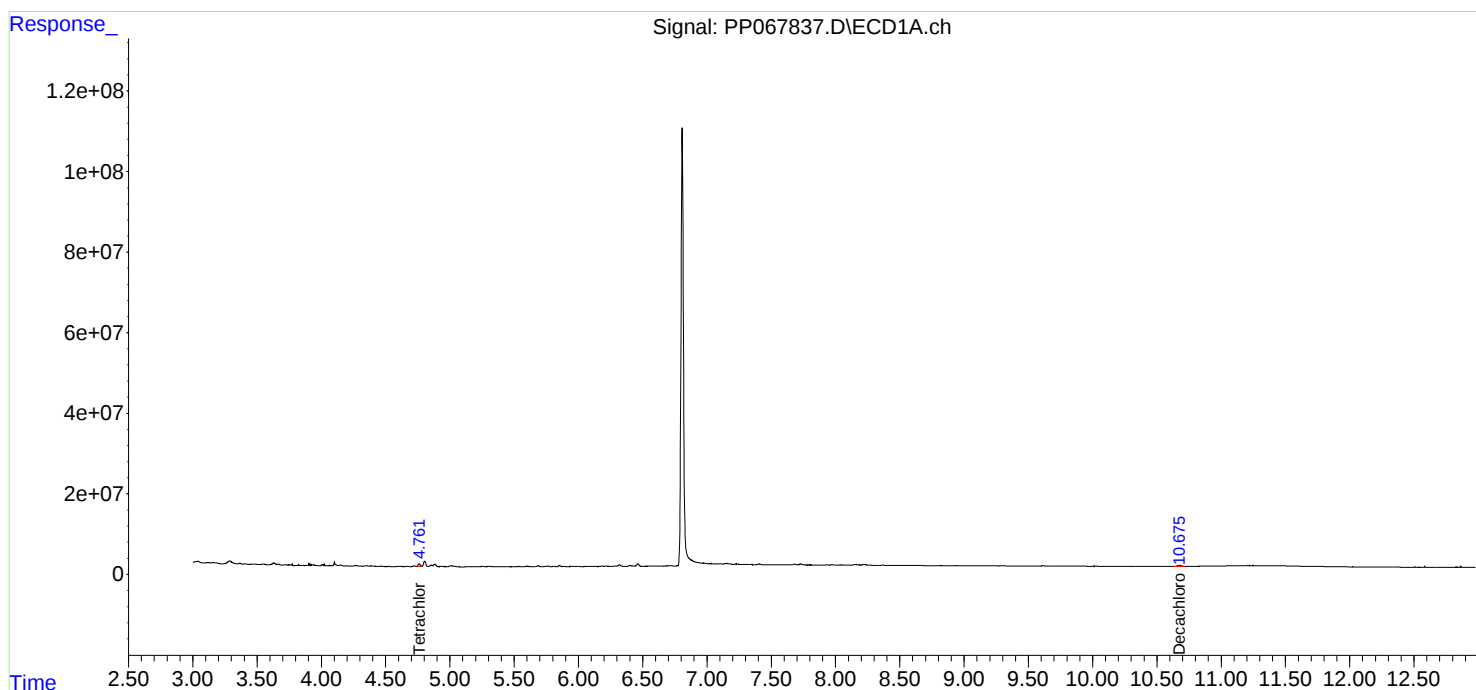

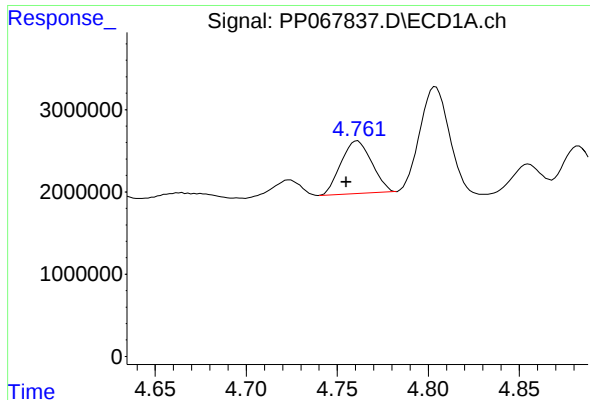


#1 Tetrachloro-m-xylene

R.T.: 4.761 min
Delta R.T.: 0.006 min
Response: 7539437
Conc: 8.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
2 - DrumRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/16/2024
Supervised By :Ankita Jodhani 10/16/2024

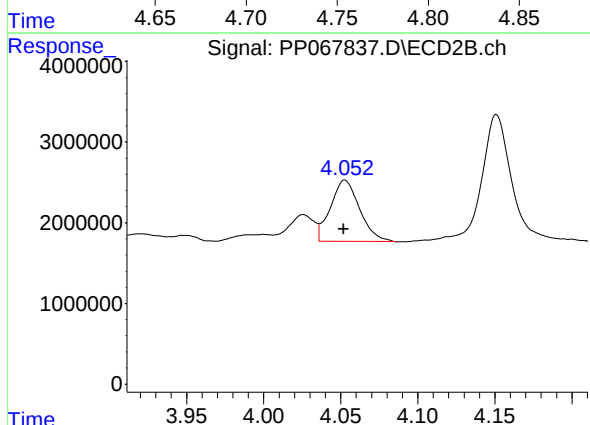


#1 Tetrachloro-m-xylene

R.T.: 4.052 min
Delta R.T.: 0.000 min
Response: 9924448
Conc: 9.82 ng/ml m

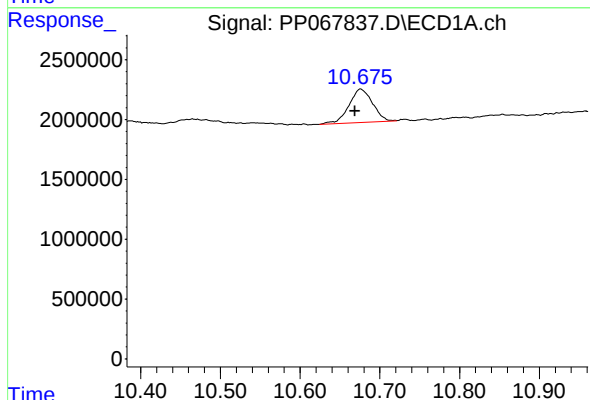

#2 Decachlorobiphenyl

R.T.: 10.675 min
Delta R.T.: 0.006 min
Response: 5800486
Conc: 5.04 ng/ml m

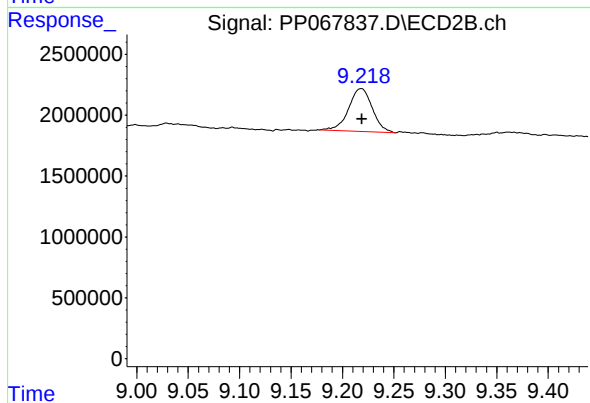

#2 Decachlorobiphenyl

R.T.: 9.218 min
Delta R.T.: 0.000 min
Response: 5634417
Conc: 5.02 ng/ml