

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101524\
 Data File : PP067839.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 13:32
 Operator : YP\AJ
 Sample : P4402-01RE 10X
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 1 - Drum

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/16/2024
 Supervised By :Ankita Jodhani 10/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 13:46:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.756	4.051	1442907	1907982	1.559m	1.888m
2) SA Decachlor...	10.674	9.216	802851	414897	0.697m	0.370m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101524\
Data File : PP067839.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 13:32
Operator : YP\AJ
Sample : P4402-01RE 10X
Misc :
ALS Vial : 54 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
1 - Drum


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/16/2024
Supervised By :Ankita Jodhani 10/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 13:46:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

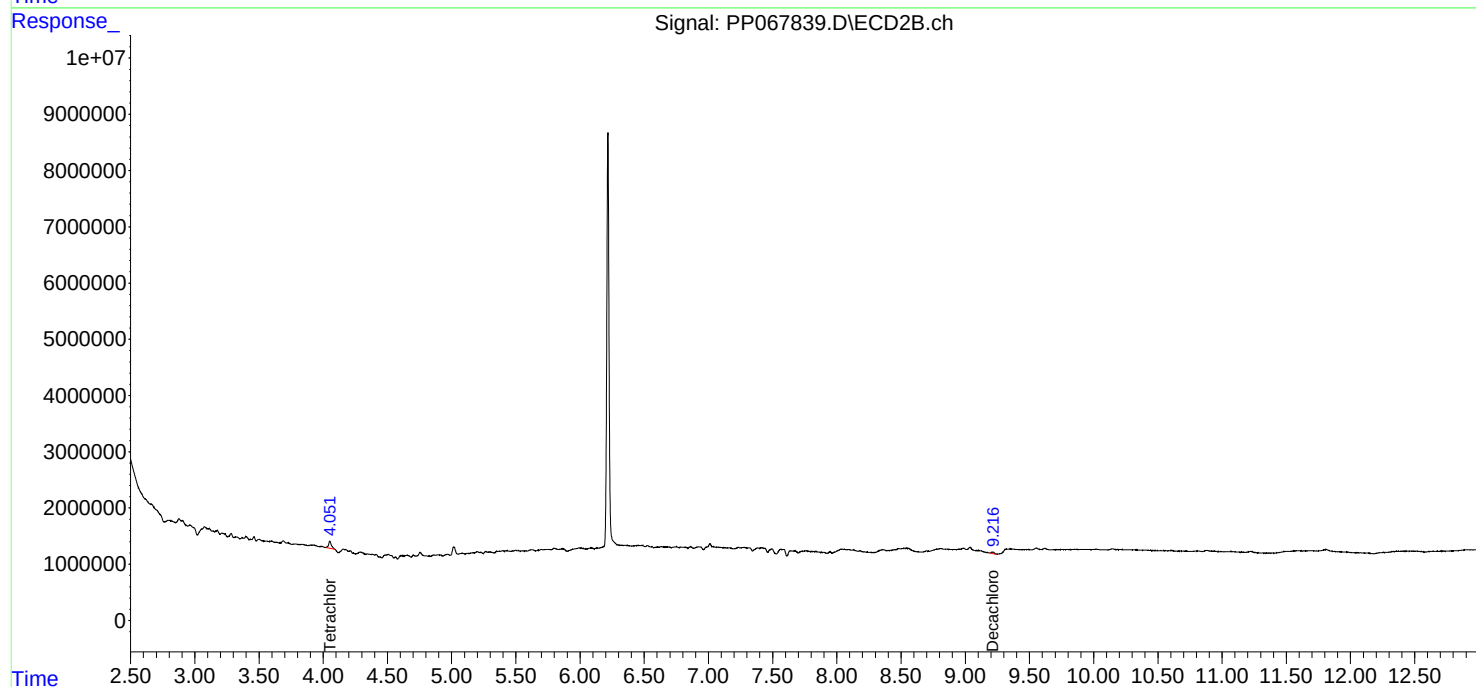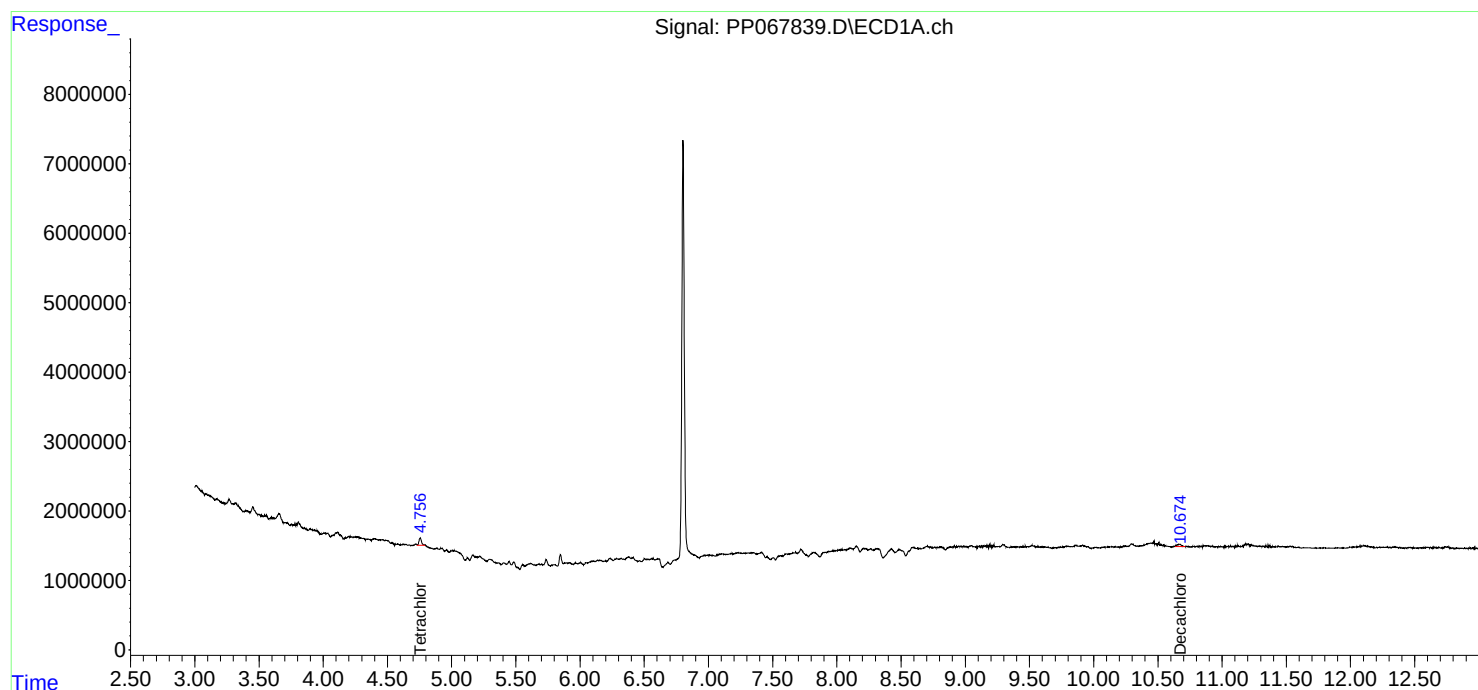

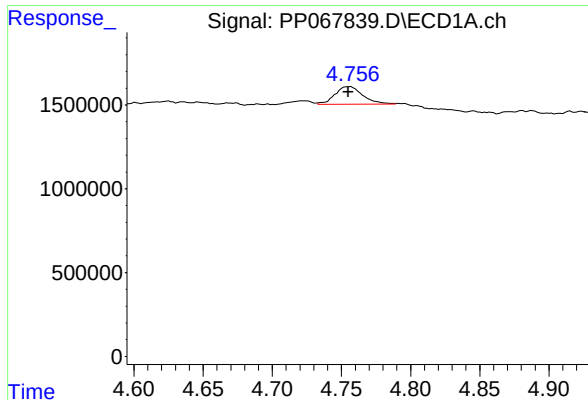


#1 Tetrachloro-m-xylene

R.T.: 4.756 min
Delta R.T.: 0.001 min
Response: 1442907
Conc: 1.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
1 - Drum


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/16/2024
Supervised By :Ankita Jodhani 10/16/2024

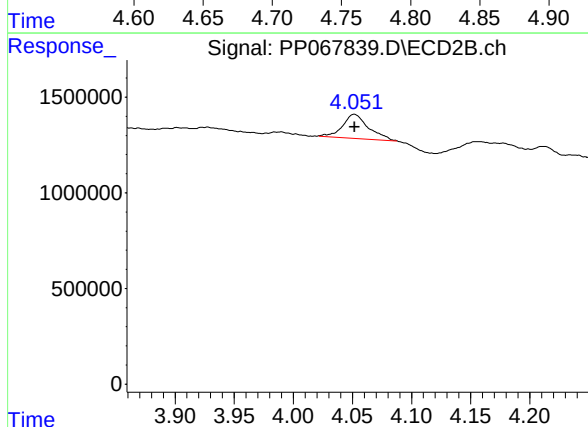


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 1907982
Conc: 1.89 ng/ml

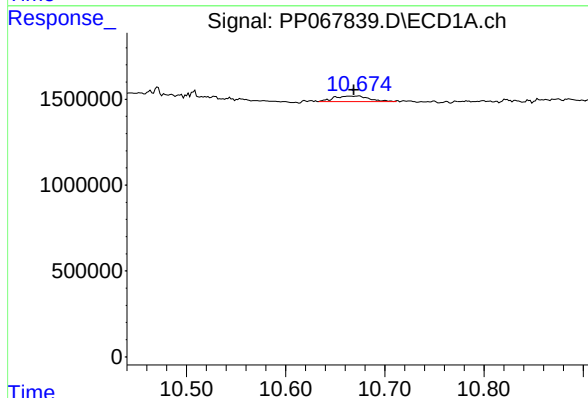

#2 Decachlorobiphenyl

R.T.: 10.674 min
Delta R.T.: 0.005 min
Response: 802851
Conc: 0.70 ng/ml

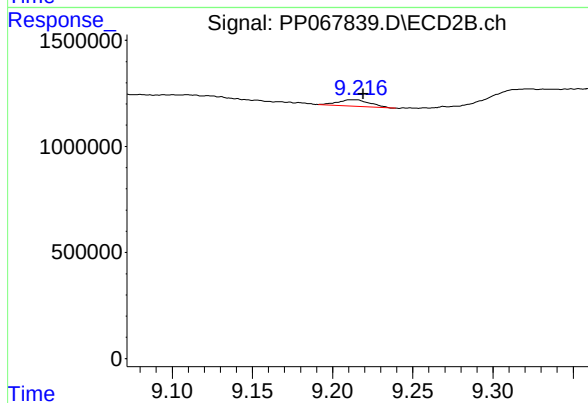

#2 Decachlorobiphenyl

R.T.: 9.216 min
Delta R.T.: -0.003 min
Response: 414897
Conc: 0.37 ng/ml