

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
 Data File : PP067897.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 11:21
 Operator : YP\AJ
 Sample : P4368-07
 Misc : AR1254 LOD 25 PPB
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 07:05:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.754	4.051	15654930	16536983	16.913	16.367
2)	SA Decachlor...	10.667	9.213	21164701	19358280	18.383	17.262
Target Compounds							
3)	L1 AR-1016-1	0.000	5.210f	0	177361	N.D.	5.069 #
4)	L1 AR-1016-2	0.000	5.210	0	177361	N.D.	3.682 #
5)	L1 AR-1016-3	0.000	5.398f	0	675864	N.D.	25.090 #
6)	L1 AR-1016-4	0.000	5.398	0	675864	N.D.	28.061 #
7)	L1 AR-1016-5	6.397	5.618	411416	404867	15.200	13.314
9)	L2 AR-1221-2	5.058	4.359	209583	381203	22.153	38.269 #
10)	L2 AR-1221-3	5.058f	0.000	209583	0	7.250	N.D. #
11)	L3 AR-1232-1	5.058f	0.000	209583	0	9.168	N.D. #
12)	L3 AR-1232-2	0.000	5.210	0	177361	N.D.	7.930 #
13)	L3 AR-1232-3	0.000	5.398f	0	675864	N.D.	56.587 #
14)	L3 AR-1232-4	0.000	5.441	0	186391	N.D.	16.164 #
15)	L3 AR-1232-5	6.190	5.618	520668	404867	57.090	30.101 #
16)	L4 AR-1242-1	5.847f	5.210f	119866	177361	4.291	6.100 #
17)	L4 AR-1242-2	0.000	5.210	0	177361	N.D.	4.418 #
18)	L4 AR-1242-3	0.000	5.398f	0	675864	N.D.	30.045 #
19)	L4 AR-1242-4	0.000	5.441	0	186391	N.D.	7.852 #
20)	L4 AR-1242-5	6.837	5.973	396862	1529801	16.450	53.397 #
21)	L5 AR-1248-1	0.000	5.210f	0	177361	N.D.	7.826 #
22)	L5 AR-1248-2	6.190	5.398	520668	675864	15.488	20.421 #
23)	L5 AR-1248-3	6.397	5.441	411416	186391	11.233	5.407 #
24)	L5 AR-1248-4	6.795	5.618	500108	404867	12.363	9.885
25)	L5 AR-1248-5	6.837	6.017	396862	170771	10.006	4.561 #
26)	L6 AR-1254-1	6.775	5.973	1130613	1529801	25.247	25.892
27)	L6 AR-1254-2	6.991	6.120	1871861	1393094	28.320	26.553
28)	L6 AR-1254-3	7.355	6.530	1801686	2099298	25.941	25.230
29)	L6 AR-1254-4	7.638	6.758	1195314	1167024	23.952	24.175
30)	L6 AR-1254-5	8.055	7.180	1217185	1730948	20.528	23.534
31)	L7 AR-1260-1	7.518	6.662	708665	1031601	13.118	18.110 #
32)	L7 AR-1260-2	7.772	6.848	799432	953991	12.635	14.302
33)	L7 AR-1260-3	8.121	7.005	36683	950076	0.708	14.915 #
34)	L7 AR-1260-4	8.359	7.483	595361	101088	9.891	1.828 #
35)	L7 AR-1260-5	8.709	7.715	313301	276404	2.909	2.260
36)	L8 AR-1262-1	8.359	7.252	595361	196069	8.295	2.492 #
37)	L8 AR-1262-2	8.709	7.483	313301	101088	2.577	1.425 #
38)	L8 AR-1262-3	0.000	8.070f	0	180042	N.D.	3.153 #
39)	L8 AR-1262-4	0.000	8.070	0	180042	N.D.	1.793 #
41)	L9 AR-1268-1	0.000	8.070f	0	180042	N.D.	1.131 #
42)	L9 AR-1268-2	0.000	8.070	0	180042	N.D.	1.257 #
43)	L9 AR-1268-3	0.000	8.290	0	66841	N.D.	0.524 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
 Data File : PP067897.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 11:21
 Operator : YP\AJ
 Sample : P4368-07
 Misc : AR1254 LOD 25 PPB
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 07:05:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
45) L9	AR-1268-5	10.289	8.918	67379	143912	0.180	0.381 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
Data File : PP067897.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 11:21
Operator : YP\AJ
Sample : P4368-07
Misc : AR1254 LOD 25 PPB
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:05:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

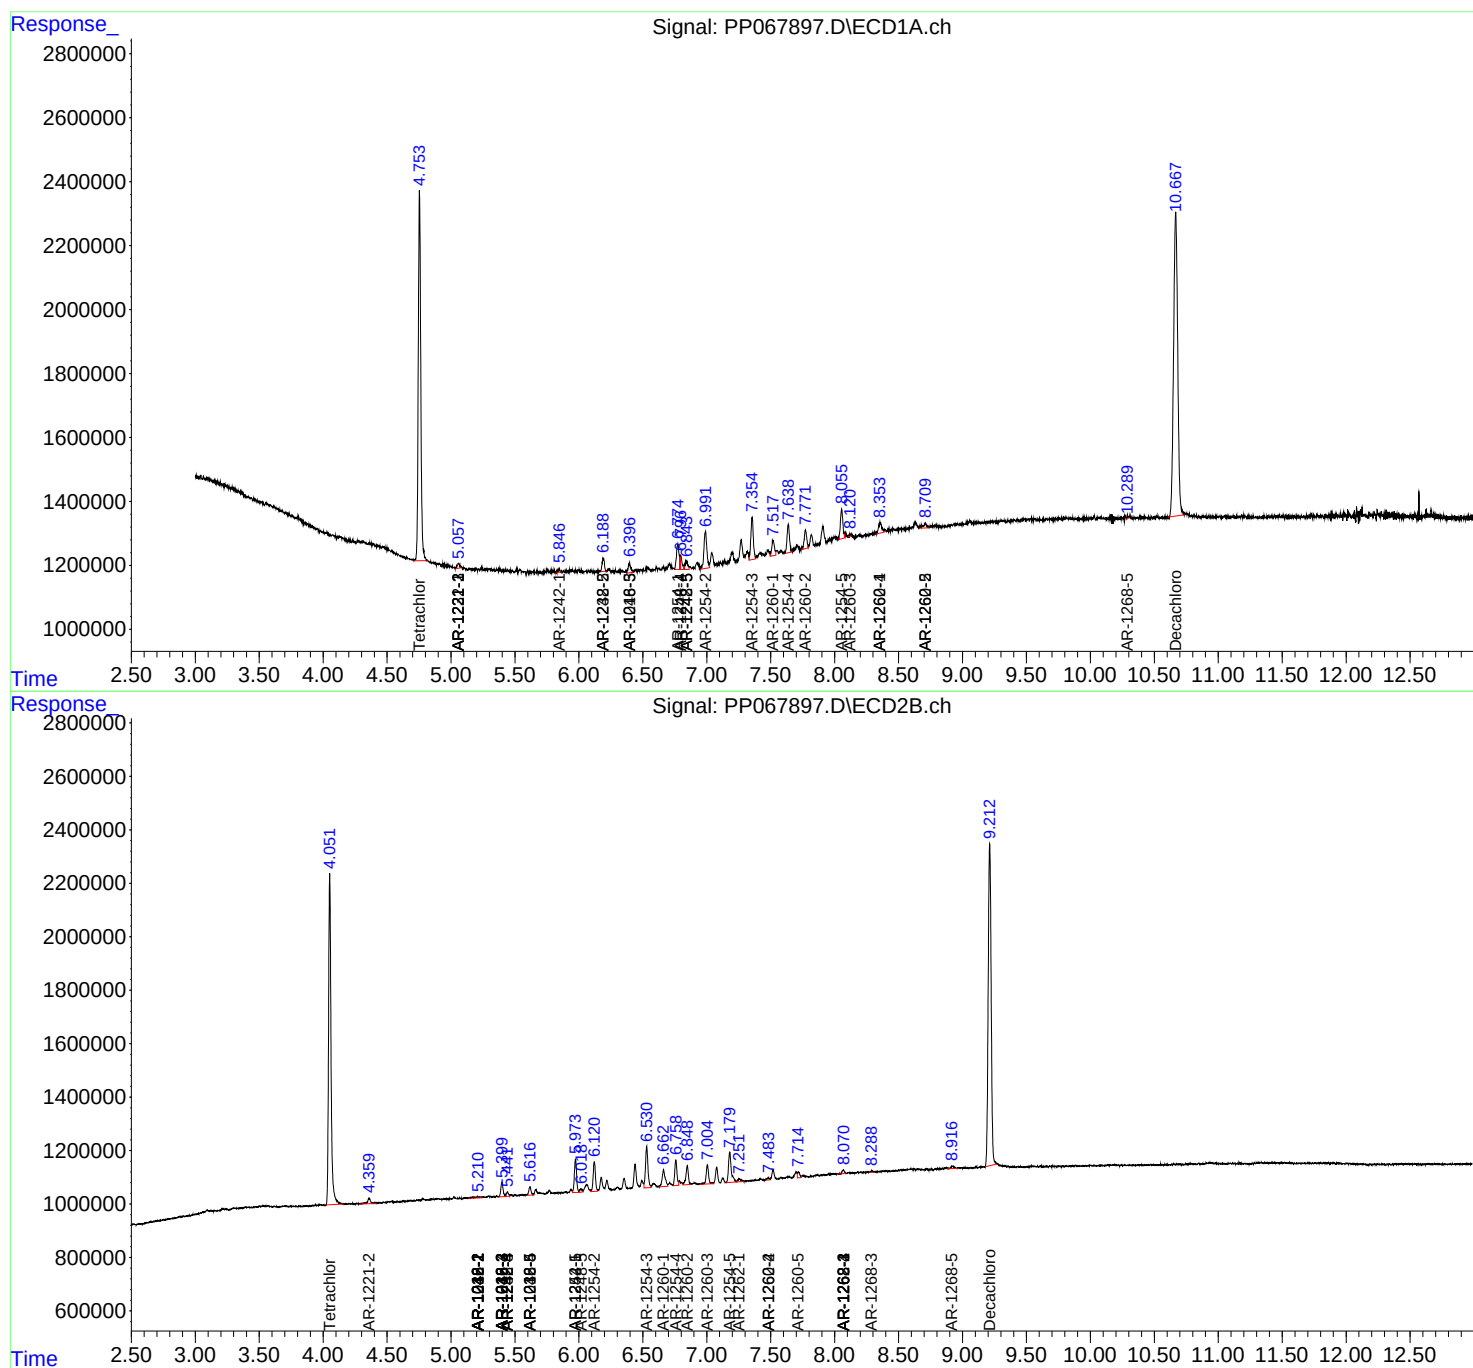


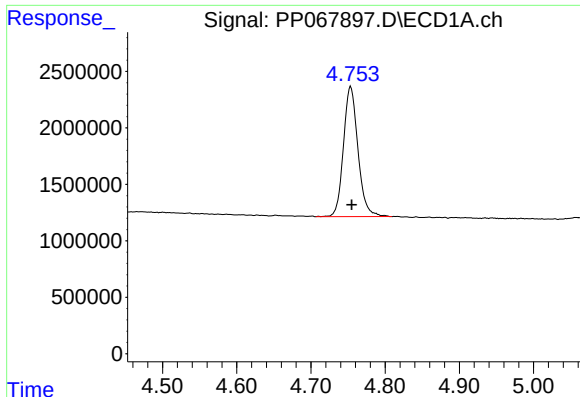

#1 Tetrachloro-m-xylene


R.T.: 4.754 min
Delta R.T.: -0.001 min
Response: 15654930
Conc: 16.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

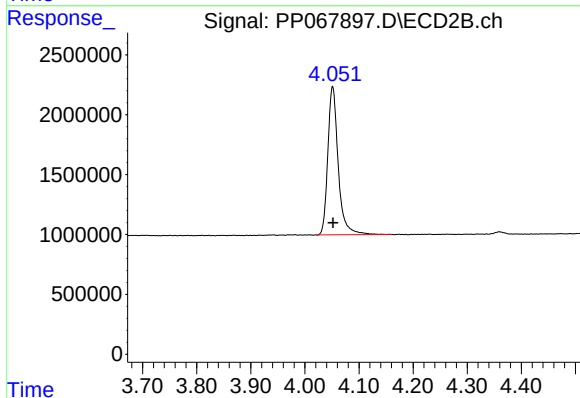


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 16536983
Conc: 16.37 ng/ml

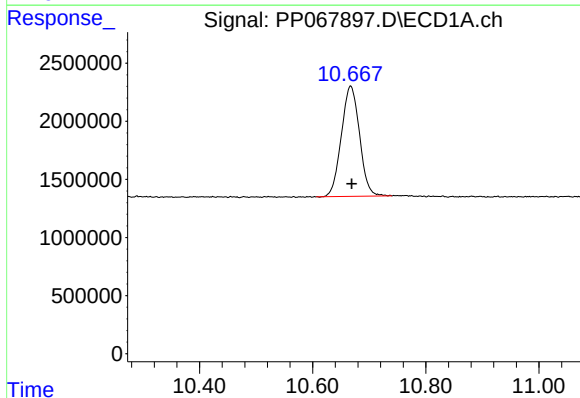


#2 Decachlorobiphenyl

R.T.: 10.667 min
Delta R.T.: -0.001 min
Response: 21164701
Conc: 18.38 ng/ml

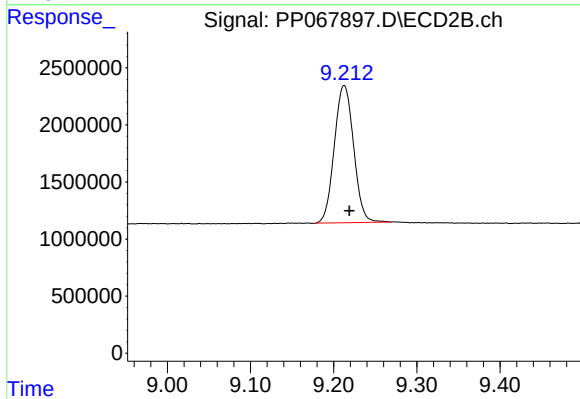

#2 Decachlorobiphenyl


R.T.: 9.213 min
Delta R.T.: -0.006 min
Response: 19358280
Conc: 17.26 ng/ml

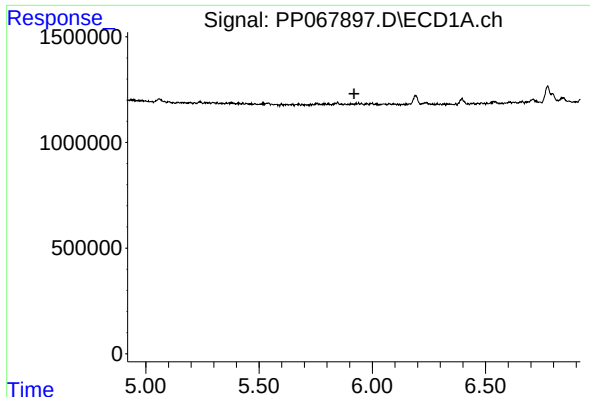

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.919 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

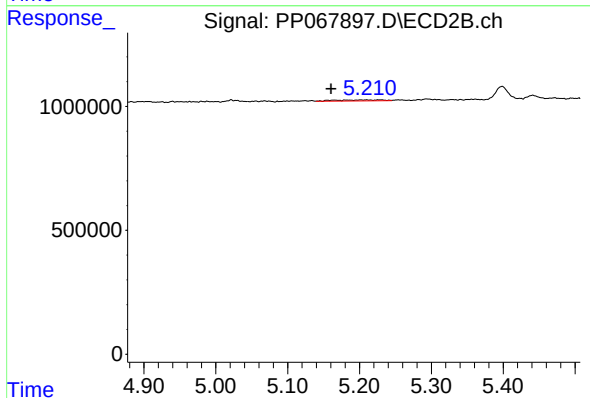


#3 AR-1016-1

R.T.: 5.210 min
Delta R.T.: 0.050 min
Response: 177361
Conc: 5.07 ng/ml

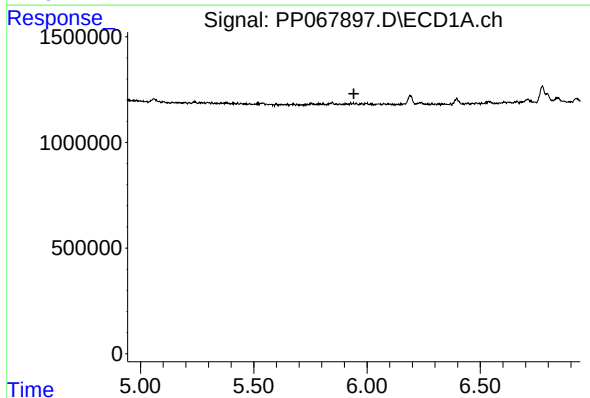


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.942 min
Response: 0
Conc: N.D.

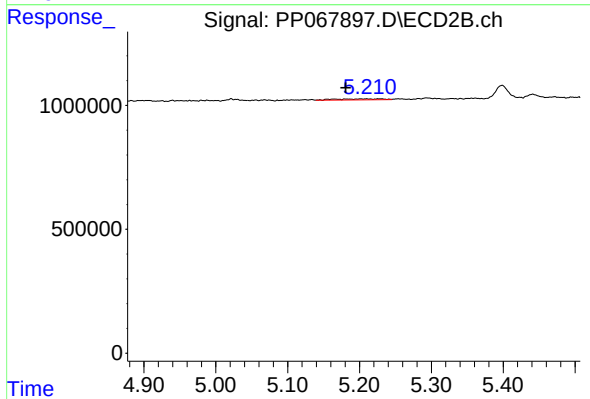

#4 AR-1016-2


R.T.: 5.210 min
Delta R.T.: 0.029 min
Response: 177361
Conc: 3.68 ng/ml

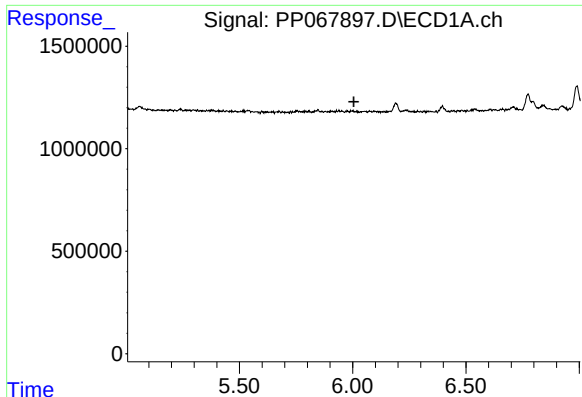

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 6.005 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

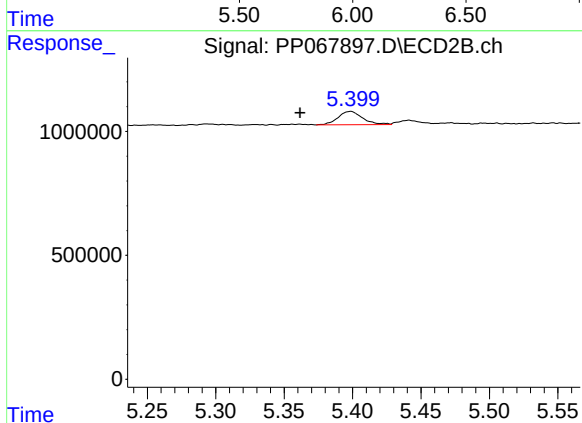


#5 AR-1016-3

R.T.: 5.398 min
Delta R.T.: 0.037 min
Response: 675864
Conc: 25.09 ng/ml

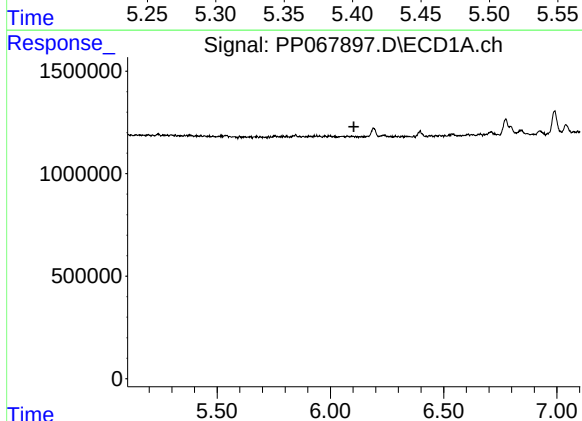


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 6.103 min
Response: 0
Conc: N.D.

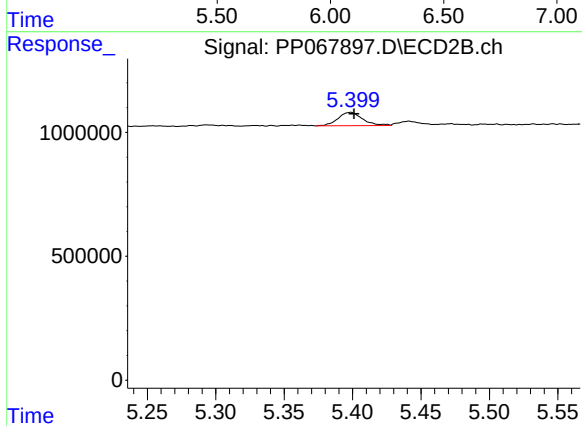

#6 AR-1016-4


R.T.: 5.398 min
Delta R.T.: -0.003 min
Response: 675864
Conc: 28.06 ng/ml

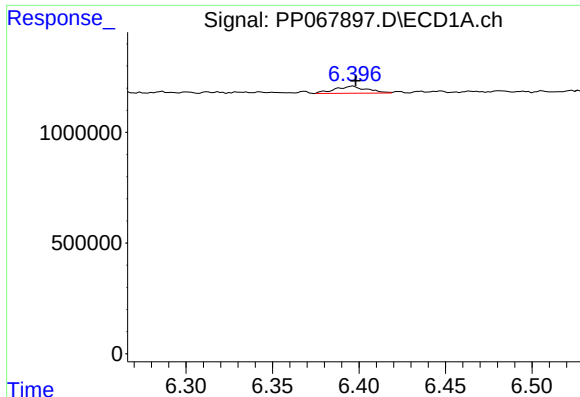

#7 AR-1016-5


R.T.: 6.397 min
Delta R.T.: -0.002 min
Response: 411416
Conc: 15.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

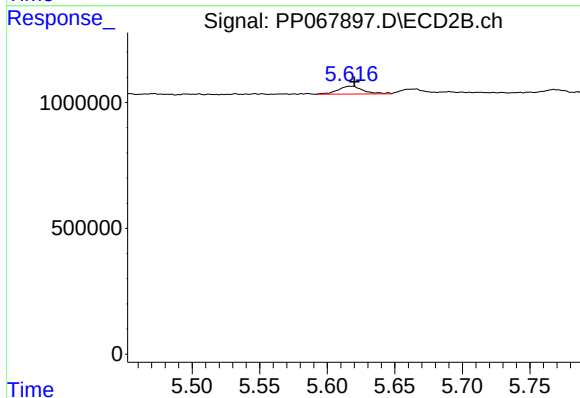


#7 AR-1016-5

R.T.: 5.618 min
Delta R.T.: -0.003 min
Response: 404867
Conc: 13.31 ng/ml

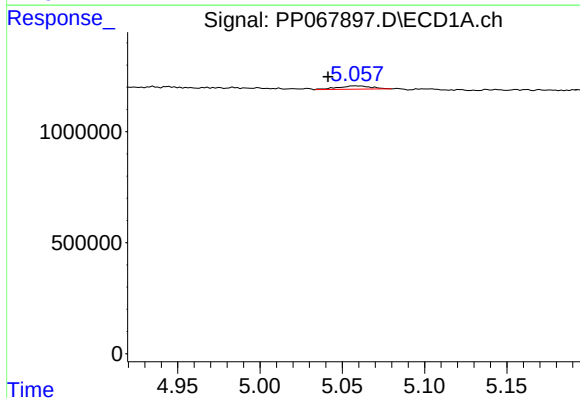


#9 AR-1221-2

R.T.: 5.058 min
Delta R.T.: 0.016 min
Response: 209583
Conc: 22.15 ng/ml

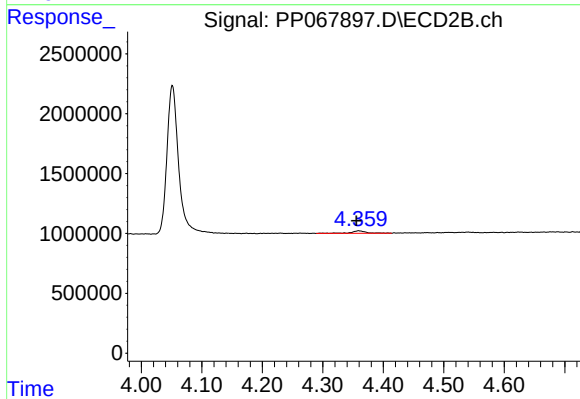

#9 AR-1221-2


R.T.: 4.359 min
Delta R.T.: 0.004 min
Response: 381203
Conc: 38.27 ng/ml

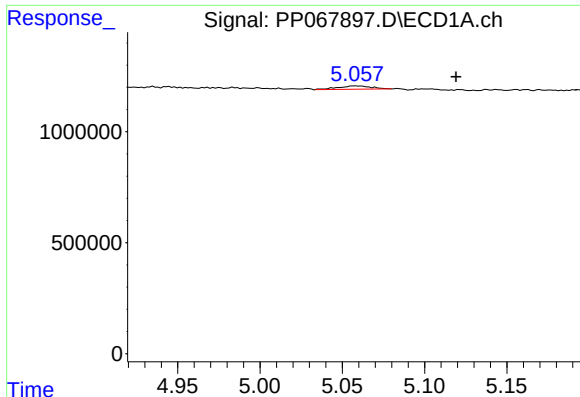

#10 AR-1221-3


R.T.: 5.058 min
Delta R.T.: -0.061 min
Response: 209583
Conc: 7.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

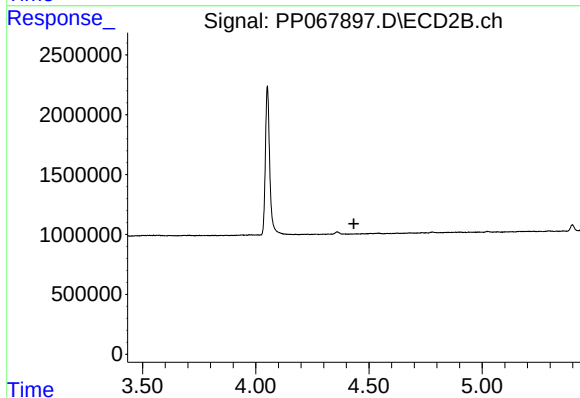


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.434 min
Response: 0
Conc: N.D.

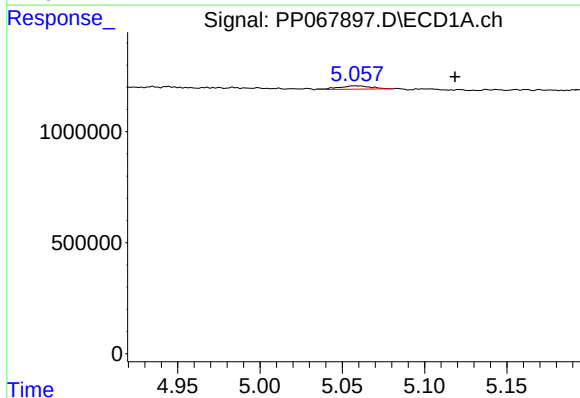


#11 AR-1232-1

R.T.: 5.058 min
Delta R.T.: -0.061 min
Response: 209583
Conc: 9.17 ng/ml

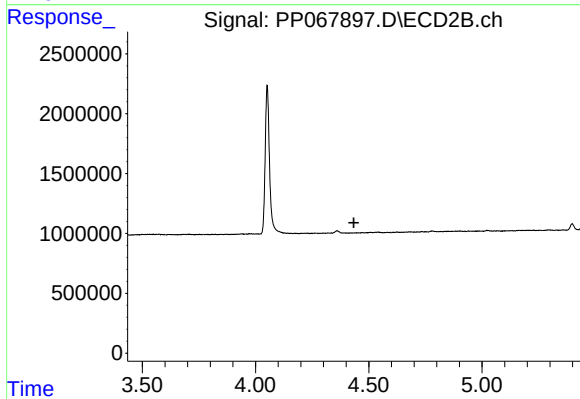

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.434 min
Response: 0
Conc: N.D.

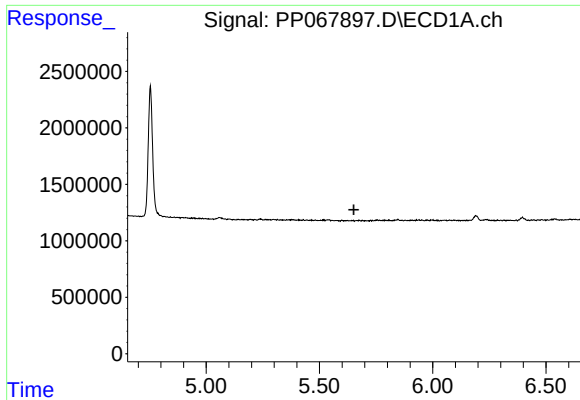

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 5.651 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

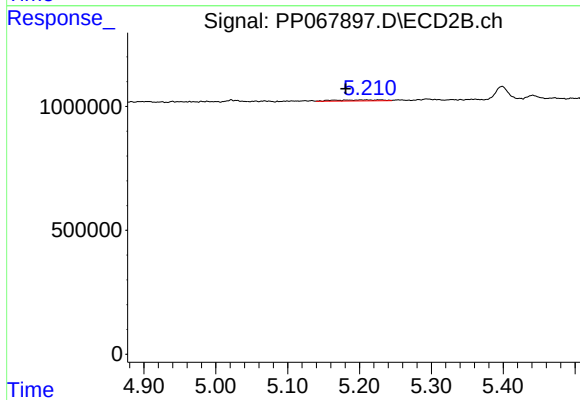


#12 AR-1232-2

R.T.: 5.210 min
Delta R.T.: 0.029 min
Response: 177361
Conc: 7.93 ng/ml

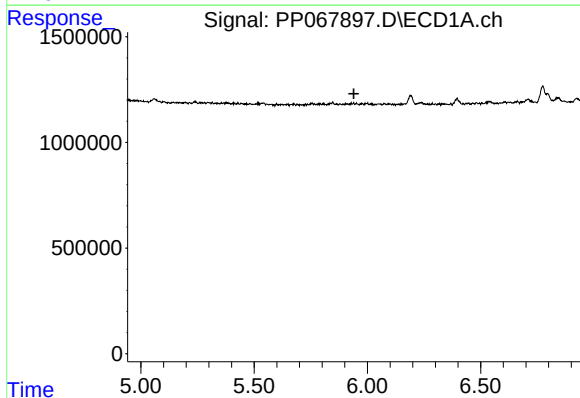


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T.: 5.940 min
Response: 0
Conc: N.D.

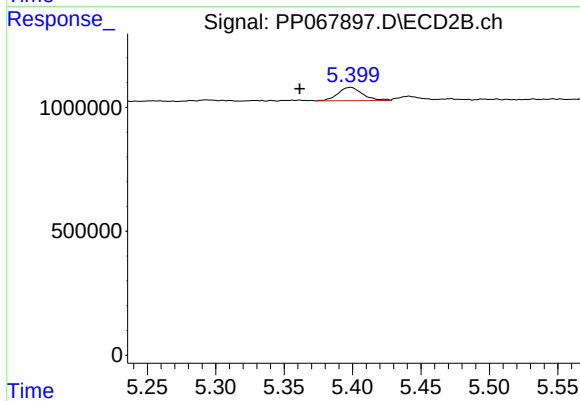

#13 AR-1232-3


R.T.: 5.398 min
Delta R.T.: 0.037 min
Response: 675864
Conc: 56.59 ng/ml

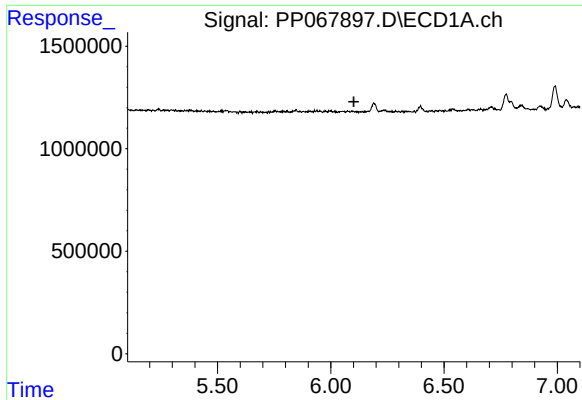

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T.: 6.101 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

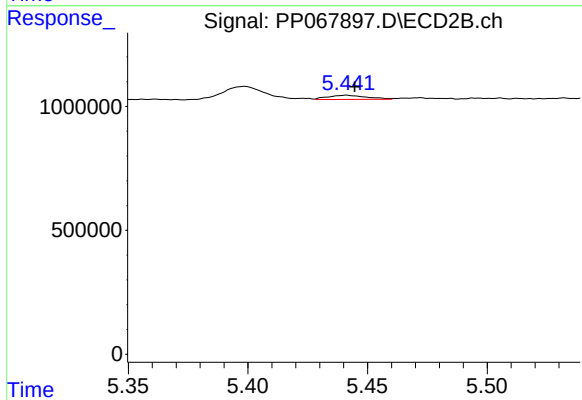


#14 AR-1232-4

R.T.: 5.441 min
Delta R.T.: -0.003 min
Response: 186391
Conc: 16.16 ng/ml

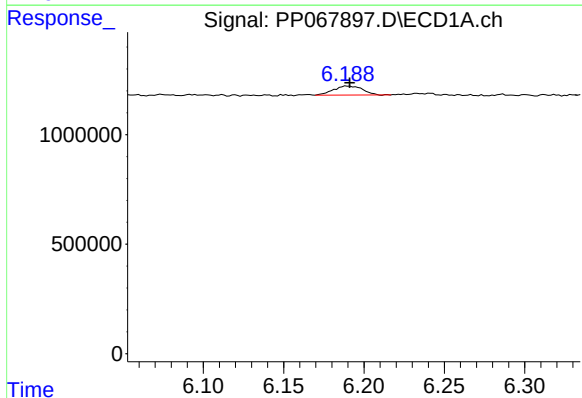


#15 AR-1232-5

R.T.: 6.190 min
Delta R.T.: -0.001 min
Response: 520668
Conc: 57.09 ng/ml

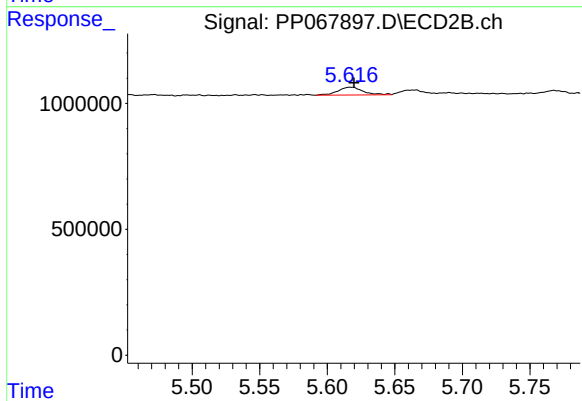

#15 AR-1232-5


R.T.: 5.618 min
Delta R.T.: -0.002 min
Response: 404867
Conc: 30.10 ng/ml

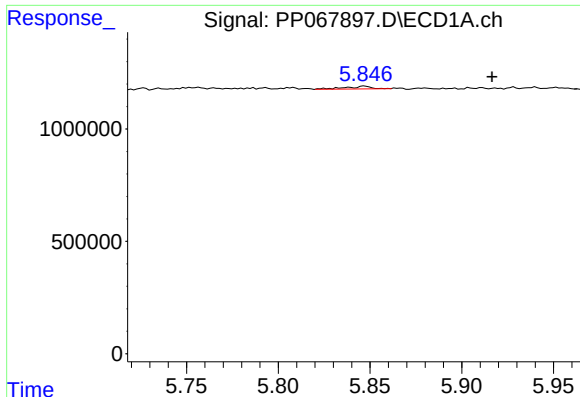

#16 AR-1242-1


R.T.: 5.847 min
Delta R.T.: -0.069 min
Response: 119866
Conc: 4.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

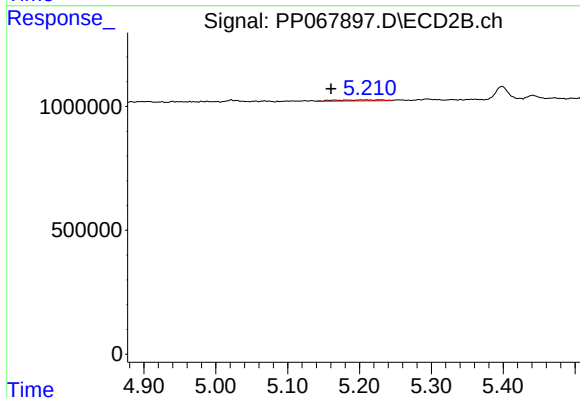


#16 AR-1242-1

R.T.: 5.210 min
Delta R.T.: 0.050 min
Response: 177361
Conc: 6.10 ng/ml

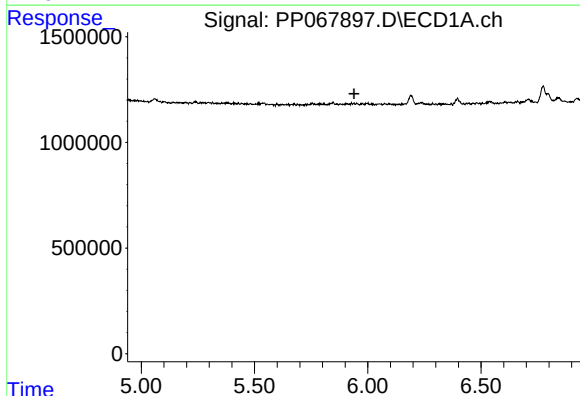


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 5.939 min
Response: 0
Conc: N.D.

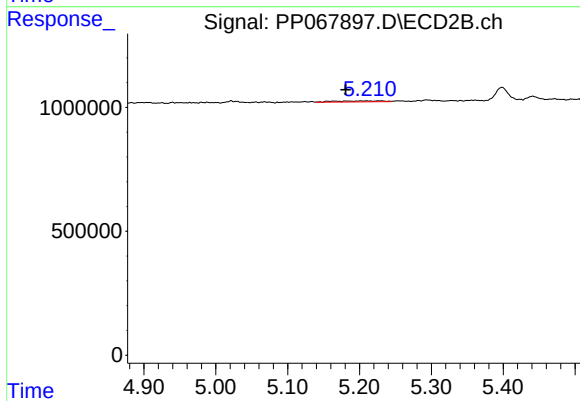

#17 AR-1242-2


R.T.: 5.210 min
Delta R.T.: 0.029 min
Response: 177361
Conc: 4.42 ng/ml

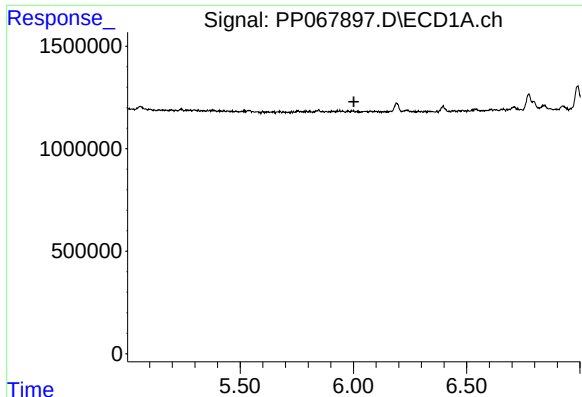

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 6.002 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

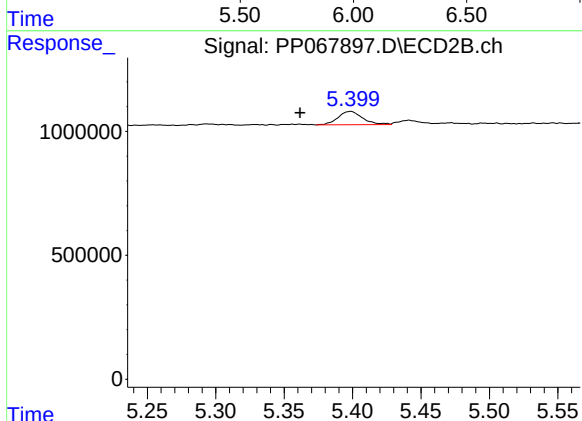


#18 AR-1242-3

R.T.: 5.398 min
Delta R.T.: 0.037 min
Response: 675864
Conc: 30.05 ng/ml

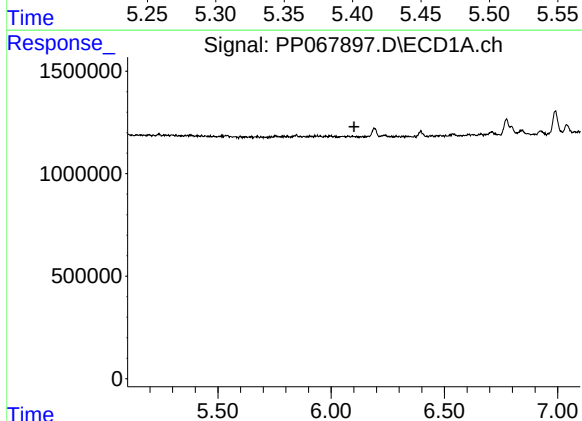


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T.: 6.101 min
Response: 0
Conc: N.D.

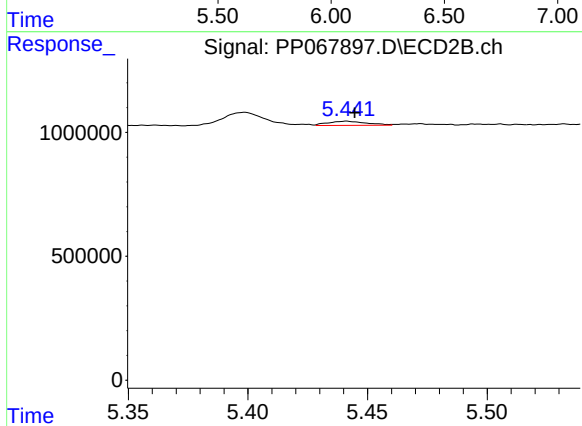

#19 AR-1242-4


R.T.: 5.441 min
Delta R.T.: -0.003 min
Response: 186391
Conc: 7.85 ng/ml

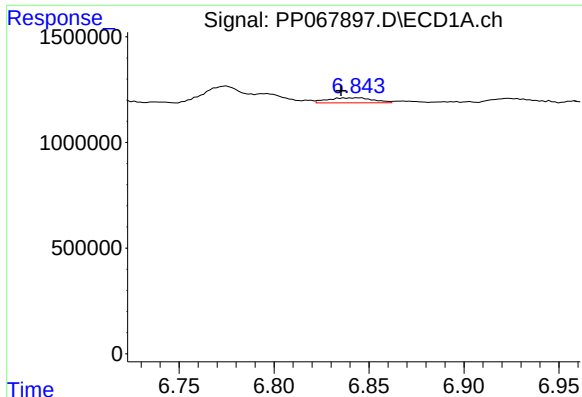

#20 AR-1242-5


R.T.: 6.837 min
Delta R.T.: 0.002 min
Response: 396862
Conc: 16.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

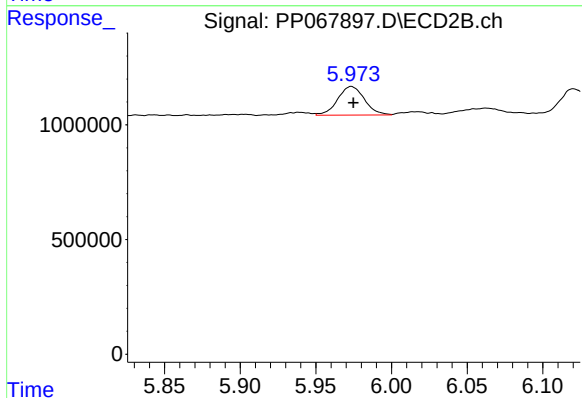


#20 AR-1242-5

R.T.: 5.973 min
Delta R.T.: -0.001 min
Response: 1529801
Conc: 53.40 ng/ml

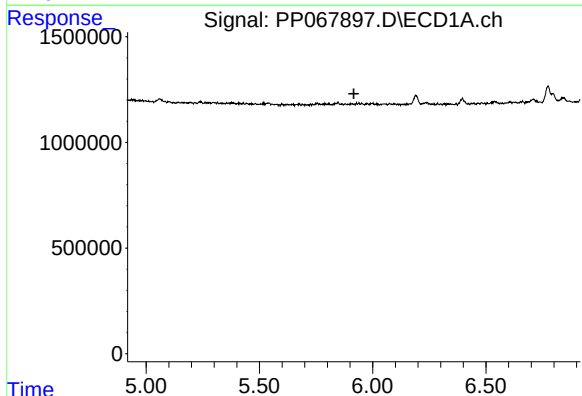


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 5.917 min
Response: 0
Conc: N.D.

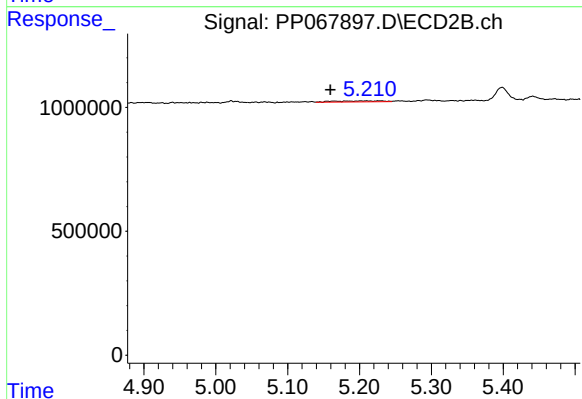

#21 AR-1248-1


R.T.: 5.210 min
Delta R.T.: 0.051 min
Response: 177361
Conc: 7.83 ng/ml

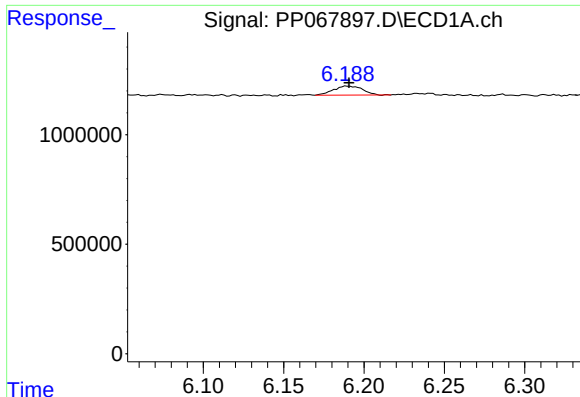

#22 AR-1248-2


R.T.: 6.190 min
Delta R.T.: 0.000 min
Response: 520668
Conc: 15.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

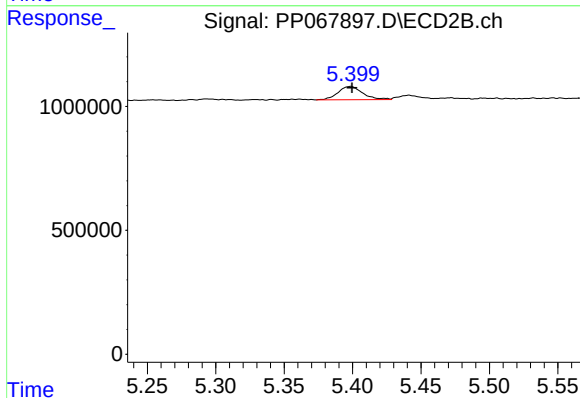


#22 AR-1248-2

R.T.: 5.398 min
Delta R.T.: -0.001 min
Response: 675864
Conc: 20.42 ng/ml

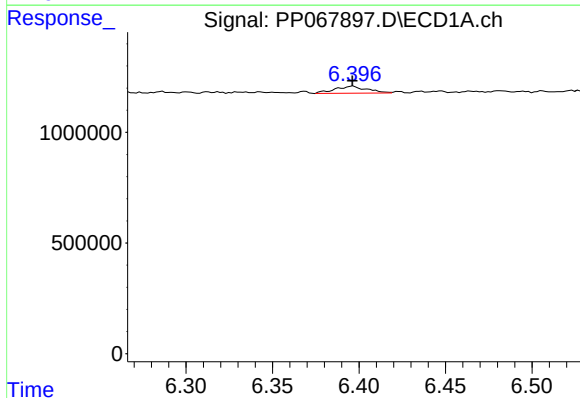


#23 AR-1248-3

R.T.: 6.397 min
Delta R.T.: 0.000 min
Response: 411416
Conc: 11.23 ng/ml

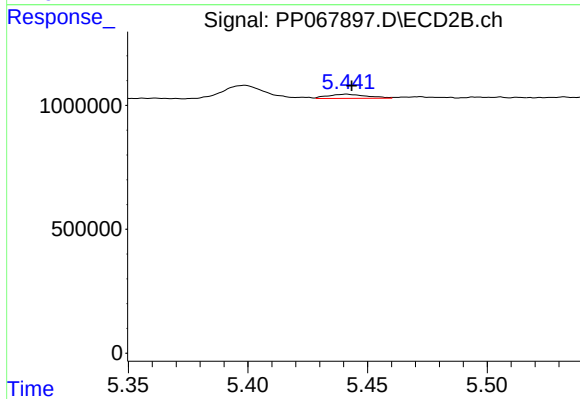

#23 AR-1248-3


R.T.: 5.441 min
Delta R.T.: -0.002 min
Response: 186391
Conc: 5.41 ng/ml

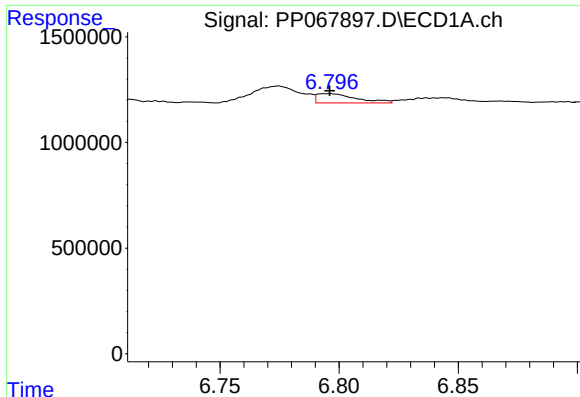

#24 AR-1248-4


R.T.: 6.795 min
Delta R.T.: 0.000 min
Response: 500108
Conc: 12.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

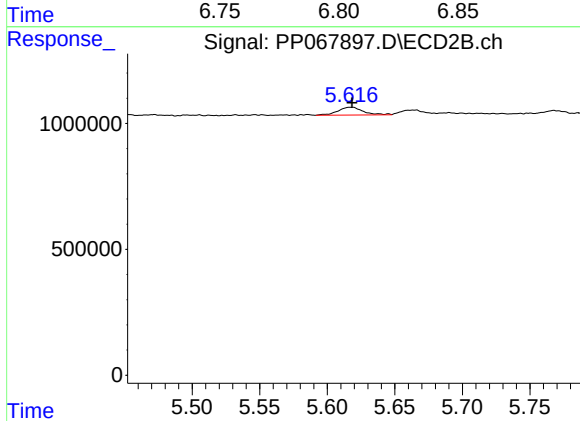


#24 AR-1248-4

R.T.: 5.618 min
Delta R.T.: 0.000 min
Response: 404867
Conc: 9.89 ng/ml

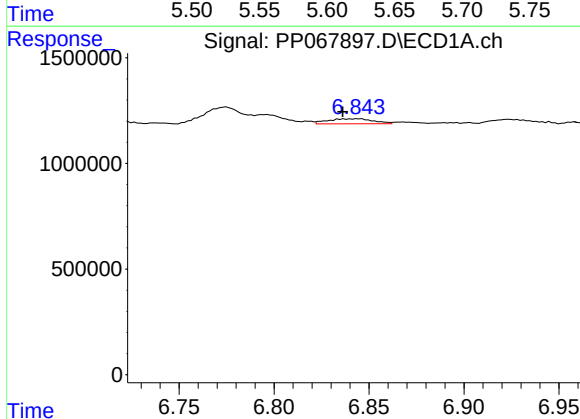


#25 AR-1248-5

R.T.: 6.837 min
Delta R.T.: 0.001 min
Response: 396862
Conc: 10.01 ng/ml

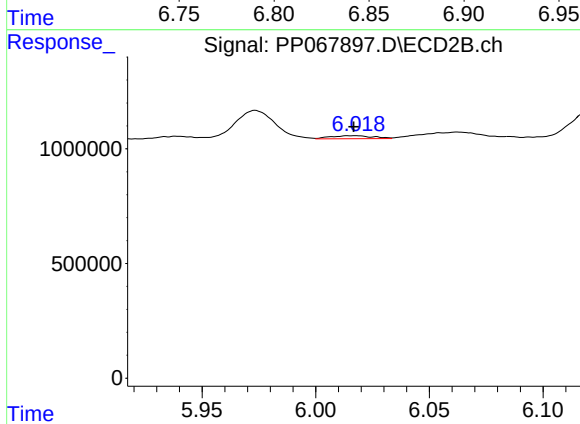

#25 AR-1248-5


R.T.: 6.017 min
Delta R.T.: 0.000 min
Response: 170771
Conc: 4.56 ng/ml

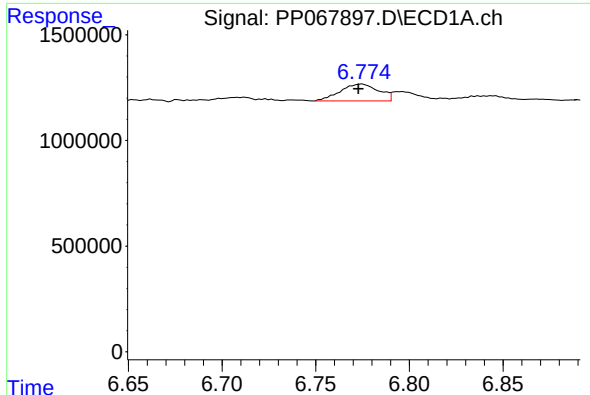

#26 AR-1254-1


R.T.: 6.775 min
Delta R.T.: 0.002 min
Response: 1130613
Conc: 25.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

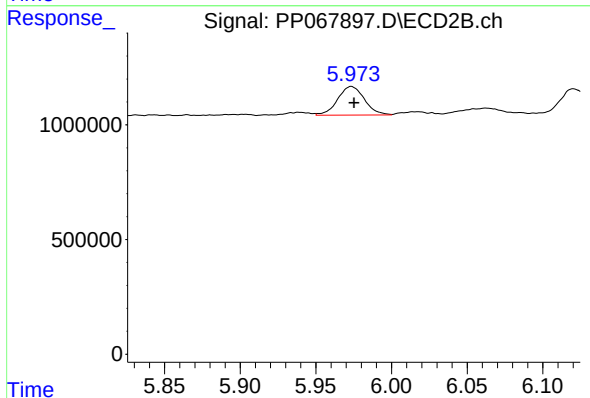


#26 AR-1254-1

R.T.: 5.973 min
Delta R.T.: -0.002 min
Response: 1529801
Conc: 25.89 ng/ml

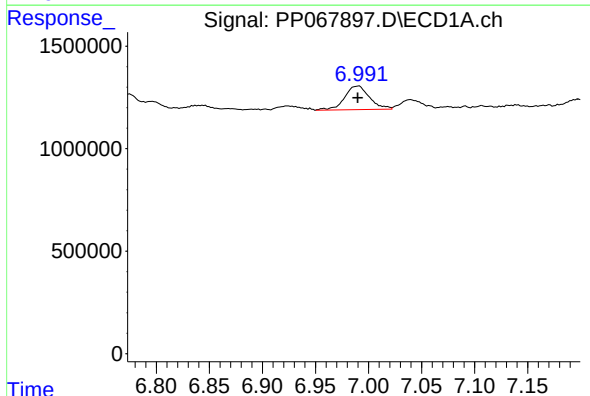


#27 AR-1254-2

R.T.: 6.991 min
Delta R.T.: 0.000 min
Response: 1871861
Conc: 28.32 ng/ml

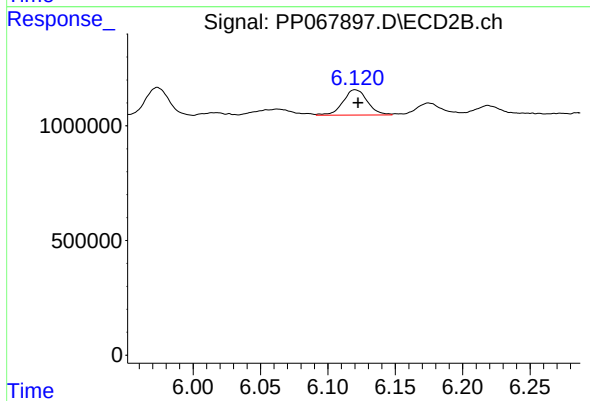

#27 AR-1254-2


R.T.: 6.120 min
Delta R.T.: -0.002 min
Response: 1393094
Conc: 26.55 ng/ml

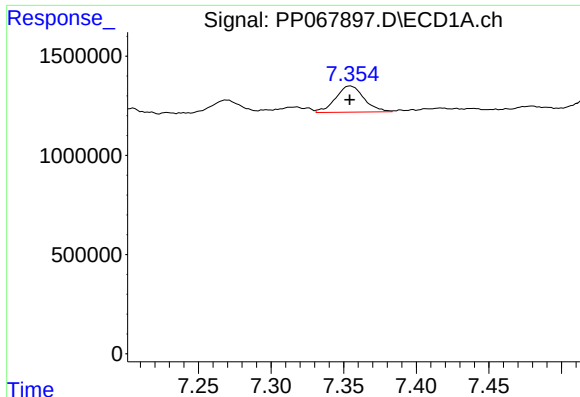

#28 AR-1254-3


R.T.: 7.355 min
Delta R.T.: 0.000 min
Response: 1801686
Conc: 25.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

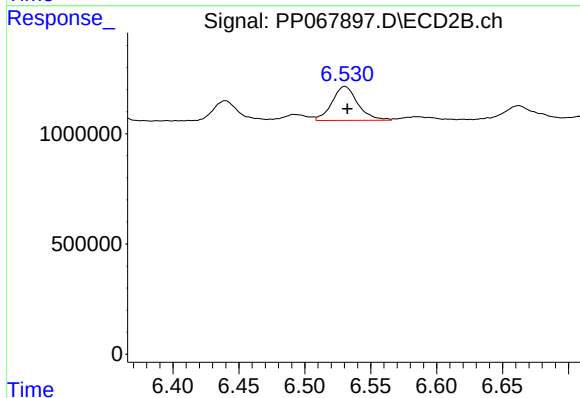


#28 AR-1254-3

R.T.: 6.530 min
Delta R.T.: -0.002 min
Response: 2099298
Conc: 25.23 ng/ml

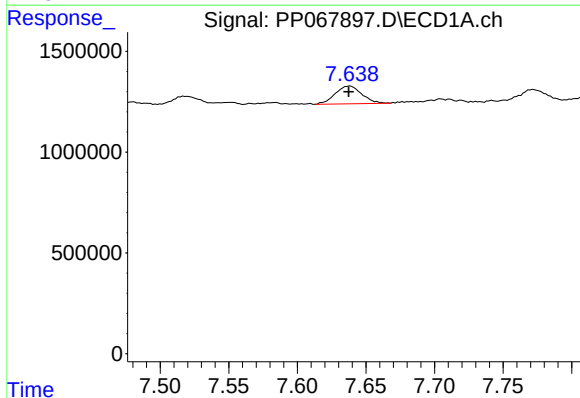


#29 AR-1254-4

R.T.: 7.638 min
Delta R.T.: 0.000 min
Response: 1195314
Conc: 23.95 ng/ml

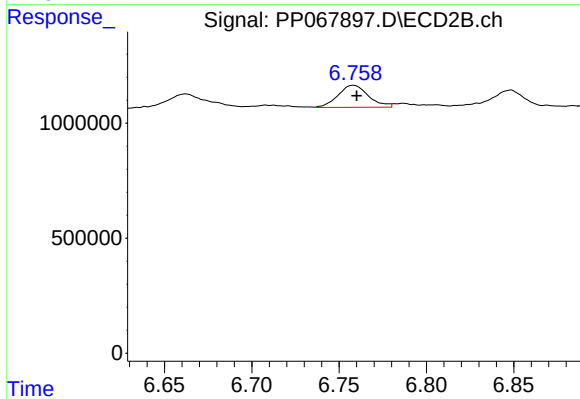

#29 AR-1254-4


R.T.: 6.758 min
Delta R.T.: -0.002 min
Response: 1167024
Conc: 24.17 ng/ml

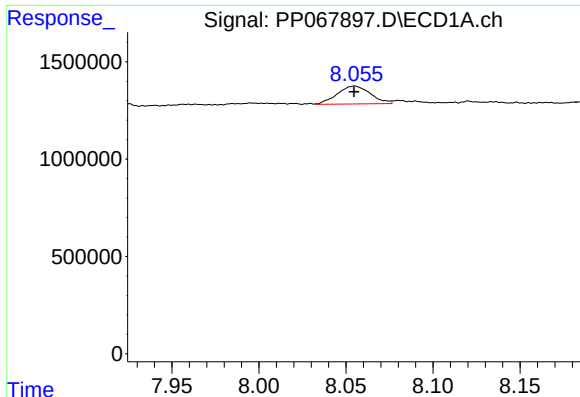

#30 AR-1254-5


R.T.: 8.055 min
Delta R.T.: 0.000 min
Response: 1217185
Conc: 20.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

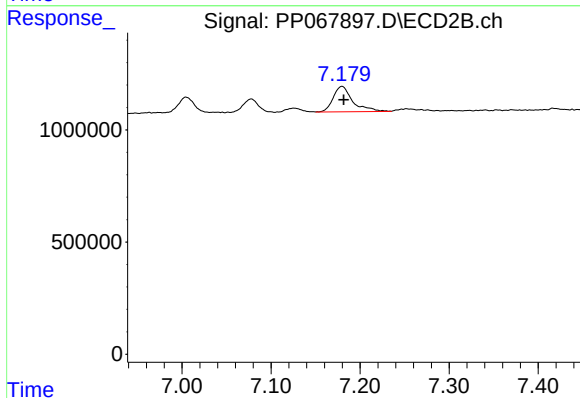


#30 AR-1254-5

R.T.: 7.180 min
Delta R.T.: -0.002 min
Response: 1730948
Conc: 23.53 ng/ml

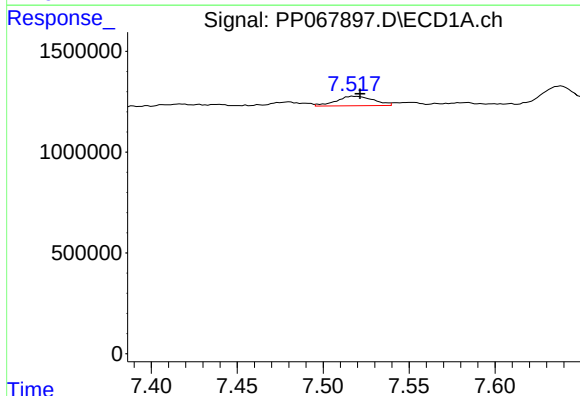


#31 AR-1260-1

R.T.: 7.518 min
Delta R.T.: -0.004 min
Response: 708665
Conc: 13.12 ng/ml

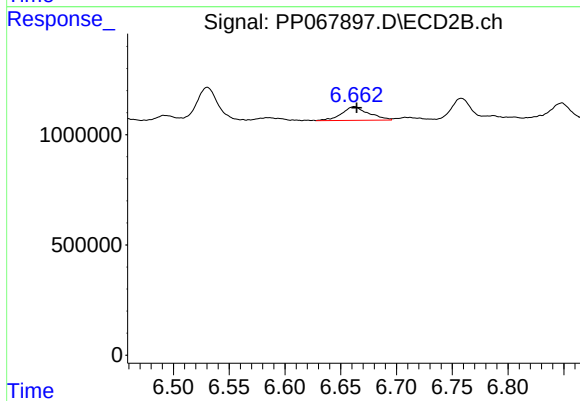

#31 AR-1260-1


R.T.: 6.662 min
Delta R.T.: -0.002 min
Response: 1031601
Conc: 18.11 ng/ml

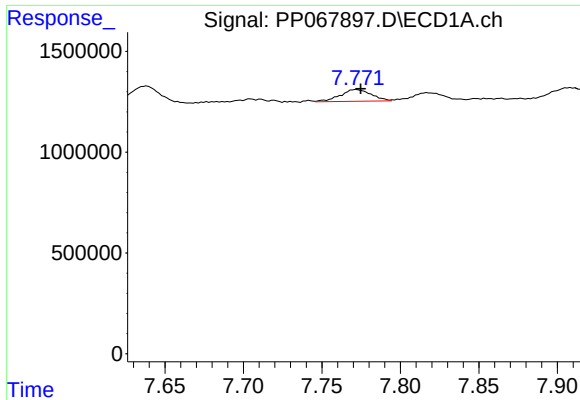

#32 AR-1260-2


R.T.: 7.772 min
Delta R.T.: -0.003 min
Response: 799432
Conc: 12.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

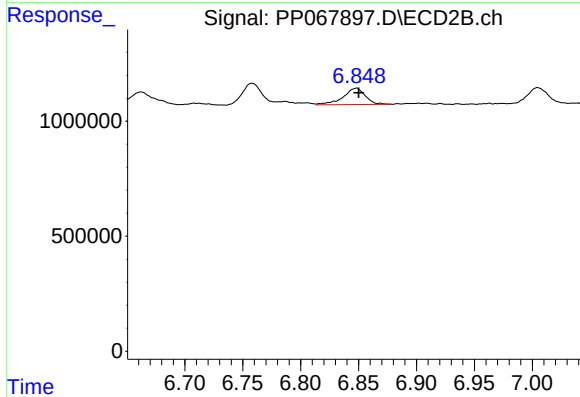


#32 AR-1260-2

R.T.: 6.848 min
Delta R.T.: -0.002 min
Response: 953991
Conc: 14.30 ng/ml

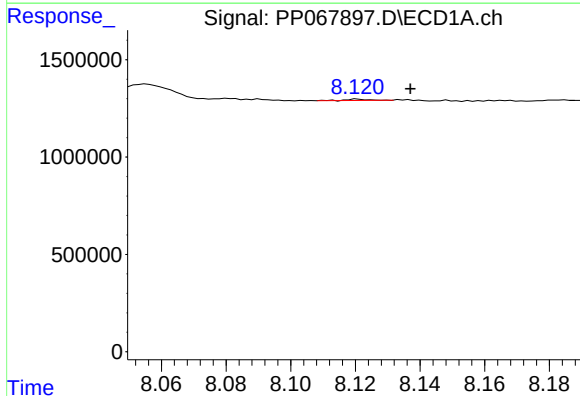


#33 AR-1260-3

R.T.: 8.121 min
Delta R.T.: -0.016 min
Response: 36683
Conc: 0.71 ng/ml

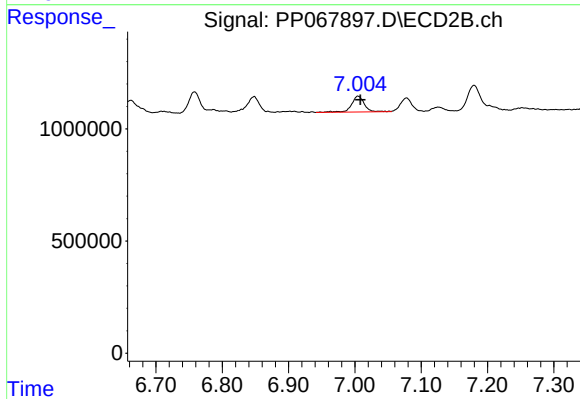

#33 AR-1260-3


R.T.: 7.005 min
Delta R.T.: -0.004 min
Response: 950076
Conc: 14.91 ng/ml

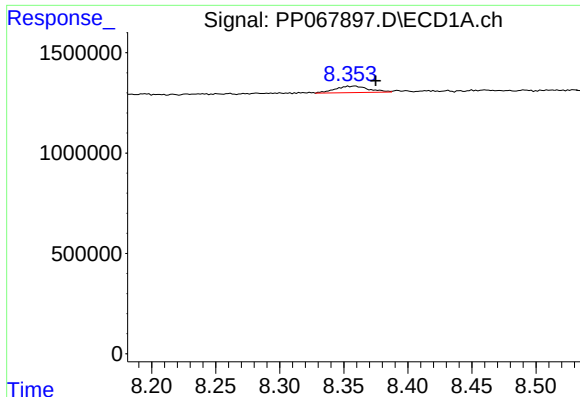

#34 AR-1260-4


R.T.: 8.359 min
Delta R.T.: -0.016 min
Response: 595361
Conc: 9.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

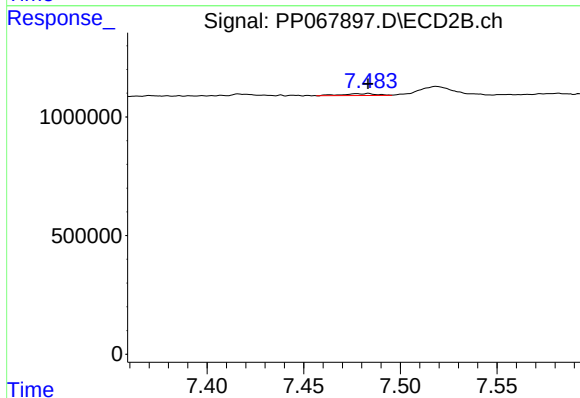


#34 AR-1260-4

R.T.: 7.483 min
Delta R.T.: 0.000 min
Response: 101088
Conc: 1.83 ng/ml

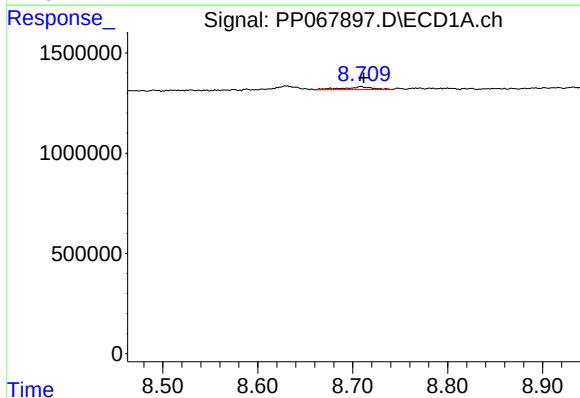


#35 AR-1260-5

R.T.: 8.709 min
Delta R.T.: -0.003 min
Response: 313301
Conc: 2.91 ng/ml

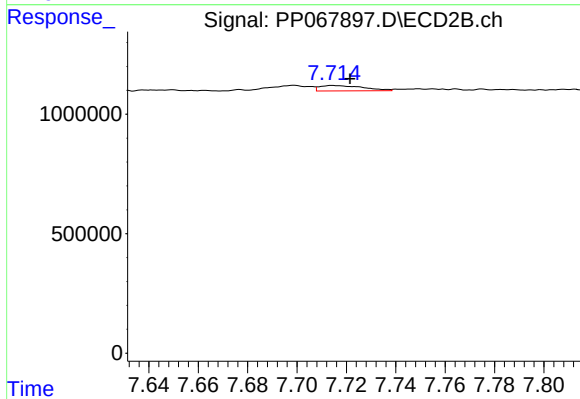

#35 AR-1260-5


R.T.: 7.715 min
Delta R.T.: -0.007 min
Response: 276404
Conc: 2.26 ng/ml

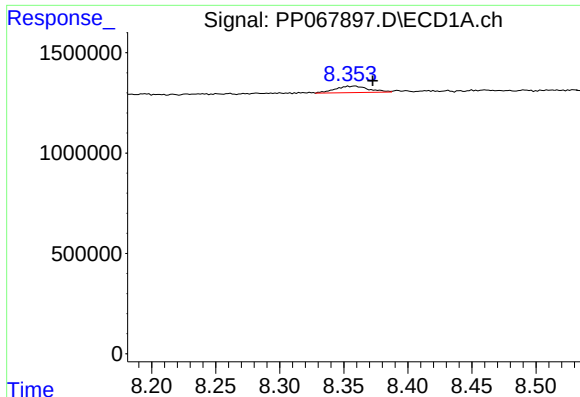

#36 AR-1262-1


R.T.: 8.359 min
Delta R.T.: -0.014 min
Response: 595361
Conc: 8.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

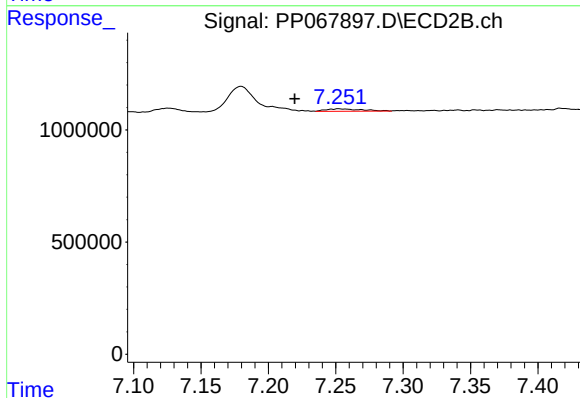


#36 AR-1262-1

R.T.: 7.252 min
Delta R.T.: 0.033 min
Response: 196069
Conc: 2.49 ng/ml

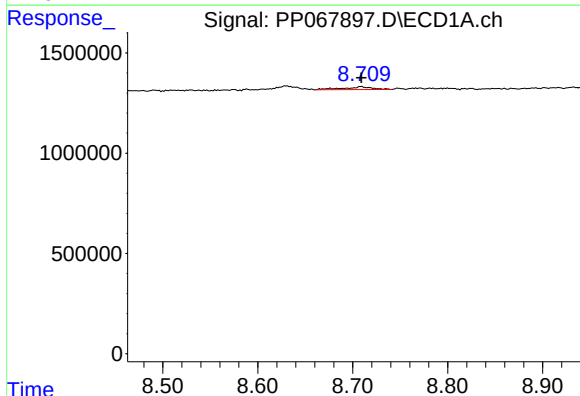


#37 AR-1262-2

R.T.: 8.709 min
Delta R.T.: 0.000 min
Response: 313301
Conc: 2.58 ng/ml

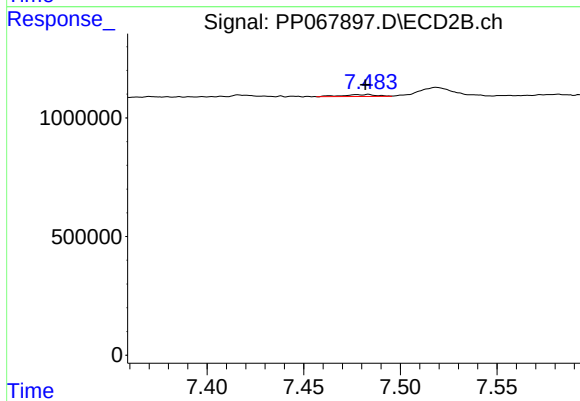

#37 AR-1262-2


R.T.: 7.483 min
Delta R.T.: 0.001 min
Response: 101088
Conc: 1.42 ng/ml

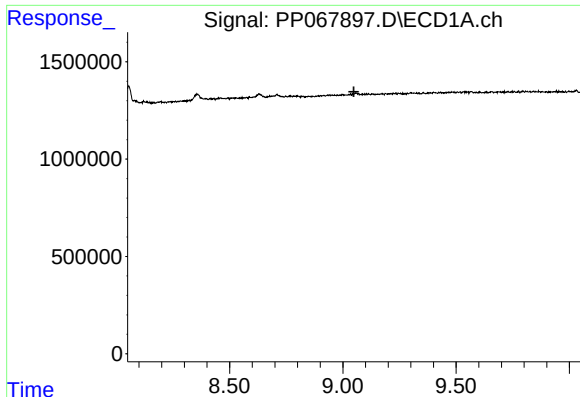

#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 9.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

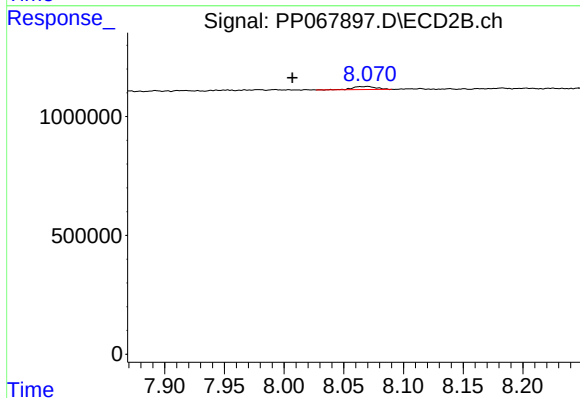


#38 AR-1262-3

R.T.: 8.070 min
Delta R.T.: 0.063 min
Response: 180042
Conc: 3.15 ng/ml


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 9.140 min
Response: 0
Conc: N.D.

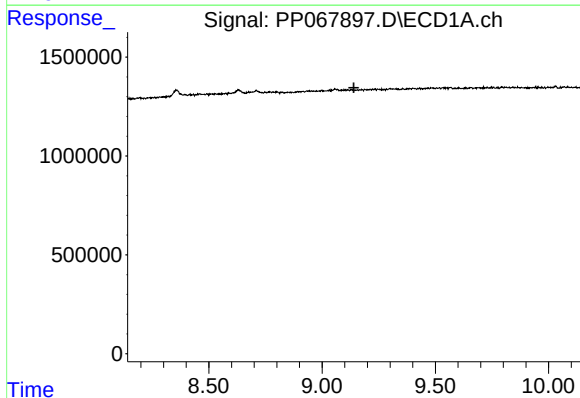

#39 AR-1262-4


R.T.: 8.070 min
Delta R.T.: 0.000 min
Response: 180042
Conc: 1.79 ng/ml

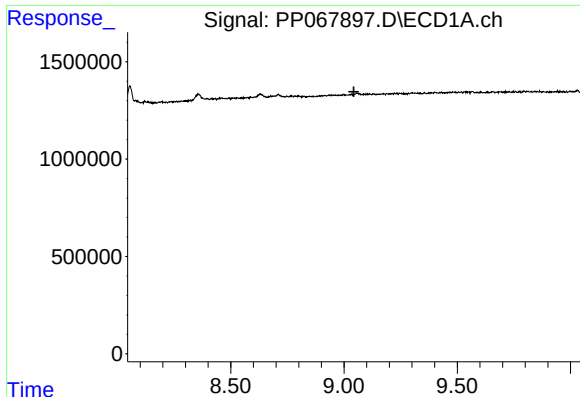

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 9.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

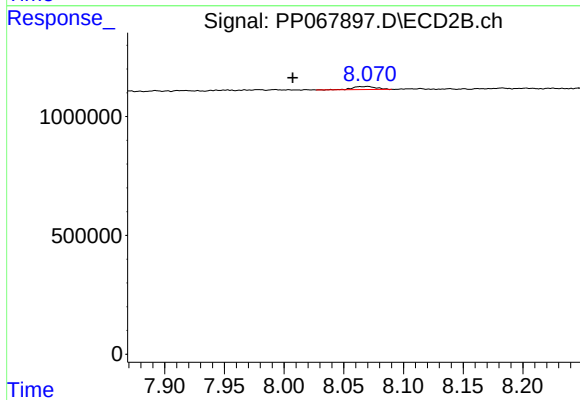


#41 AR-1268-1

R.T.: 8.070 min
Delta R.T.: 0.063 min
Response: 180042
Conc: 1.13 ng/ml

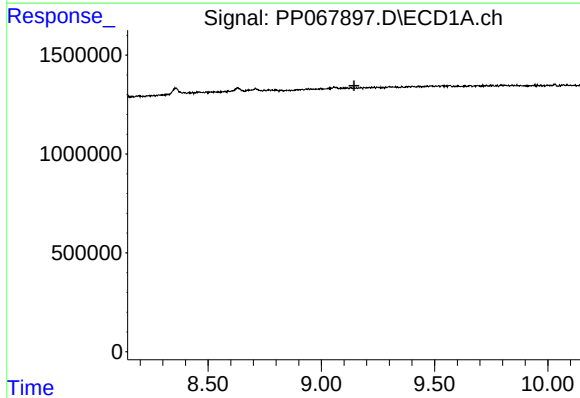


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 9.144 min
Response: 0
Conc: N.D.

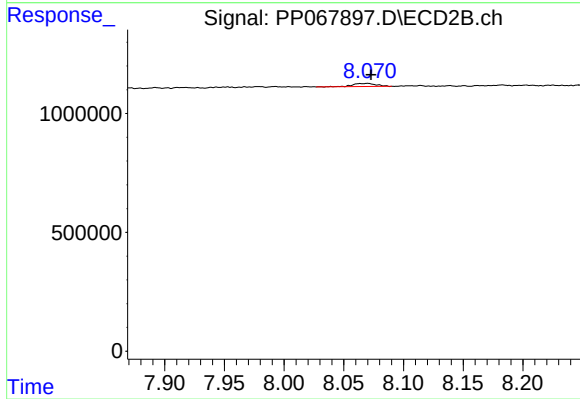

#42 AR-1268-2


R.T.: 8.070 min
Delta R.T.: -0.003 min
Response: 180042
Conc: 1.26 ng/ml

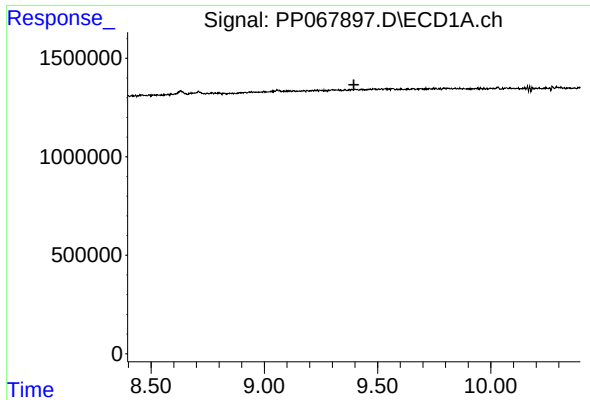

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

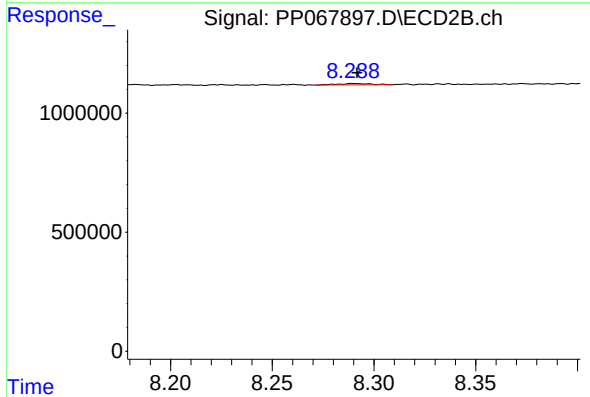


#43 AR-1268-3

R.T.: 8.290 min
Delta R.T.: -0.002 min
Response: 66841
Conc: 0.52 ng/ml

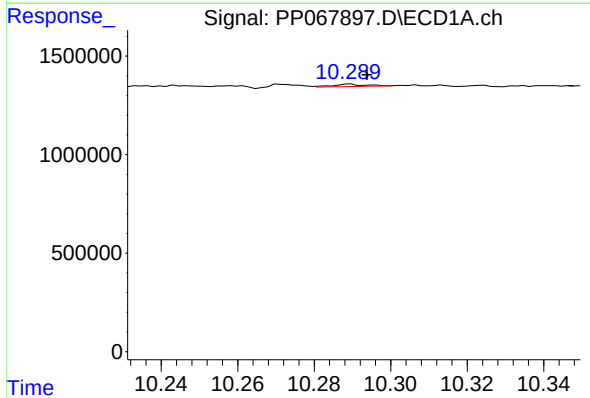

#45 AR-1268-5

R.T.: 10.289 min
Delta R.T.: -0.004 min
Response: 67379
Conc: 0.18 ng/ml

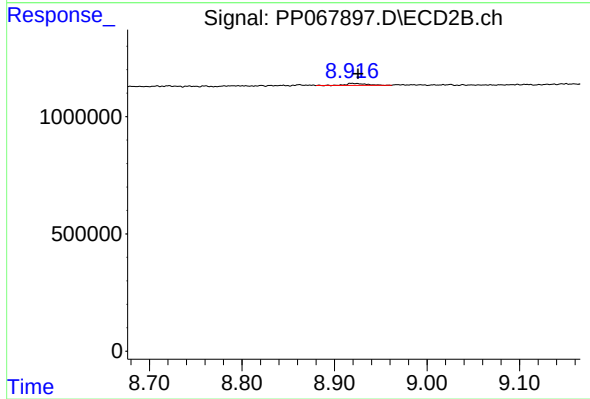

#45 AR-1268-5

R.T.: 8.918 min
Delta R.T.: -0.007 min
Response: 143912
Conc: 0.38 ng/ml