

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
 Data File : PP067898.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 11:38
 Operator : YP\AJ
 Sample : P4368-07
 Misc : AR1262 LOD 25 PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 07:05:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.755	4.050	15862614	16931584	17.137	16.757
2)	SA Decachlor...	10.665	9.213	21892293	19778118	19.015	17.636
Target Compounds							
3)	L1 AR-1016-1	0.000	5.166	0	42748	N.D.	1.222 #
4)	L1 AR-1016-2	0.000	5.166	0	42748	N.D.	0.887 #
5)	L1 AR-1016-3	0.000	5.396	0	32114	N.D.	1.192 #
6)	L1 AR-1016-4	0.000	5.396	0	32114	N.D.	1.333 #
7)	L1 AR-1016-5	0.000	5.662f	0	281725	N.D.	9.264 #
9)	L2 AR-1221-2	5.063	4.363	135366	309652	14.308	31.086 #
10)	L2 AR-1221-3	5.063f	0.000	135366	0	4.683	N.D. #
11)	L3 AR-1232-1	5.063f	0.000	135366	0	5.922	N.D. #
12)	L3 AR-1232-2	0.000	5.166	0	42748	N.D.	1.911 #
13)	L3 AR-1232-3	0.000	5.396f	0	32114	N.D.	2.689 #
14)	L3 AR-1232-4	0.000	5.396f	0	32114	N.D.	2.785 #
15)	L3 AR-1232-5	0.000	5.662f	0	281725	N.D.	20.946 #
16)	L4 AR-1242-1	0.000	5.166	0	42748	N.D.	1.470 #
17)	L4 AR-1242-2	0.000	5.166	0	42748	N.D.	1.065 #
18)	L4 AR-1242-3	0.000	5.396	0	32114	N.D.	1.428 #
19)	L4 AR-1242-4	0.000	5.396f	0	32114	N.D.	1.353 #
20)	L4 AR-1242-5	6.777f	5.972	199617	242876	8.274	8.477
21)	L5 AR-1248-1	0.000	5.166	0	42748	N.D.	1.886 #
22)	L5 AR-1248-2	0.000	5.396	0	32114	N.D.	0.970 #
23)	L5 AR-1248-3	0.000	5.396f	0	32114	N.D.	0.932 #
24)	L5 AR-1248-4	6.777	5.662f	199617	281725	4.935	6.879 #
25)	L5 AR-1248-5	6.777f	5.972f	199617	242876	5.033	6.487 #
26)	L6 AR-1254-1	6.777	5.972	199617	242876	4.457	4.111
27)	L6 AR-1254-2	6.993	6.118	124019	247073	1.876	4.709 #
28)	L6 AR-1254-3	7.352	6.545	288907	1036322	4.160	12.455 #
29)	L6 AR-1254-4	7.695f	6.759	99936	30590	2.003	0.634 #
30)	L6 AR-1254-5	8.055	7.178	1215406	896898	20.498	12.194 #
31)	L7 AR-1260-1	7.519	6.660	1163112	1178212	21.530	20.684
32)	L7 AR-1260-2	7.774	6.846	1460624	1500199	23.085	22.490
33)	L7 AR-1260-3	8.135	7.009	1759148	1378542	33.928	21.641 #
34)	L7 AR-1260-4	8.374	7.479	1597710	1691889	26.542	30.599
35)	L7 AR-1260-5	8.709	7.717	2957998	3193118	27.462	26.109
36)	L8 AR-1262-1	8.374	7.217	1597710	1921638	22.261	24.425
37)	L8 AR-1262-2	8.709	7.479	2957998	1691889	24.330	23.842
38)	L8 AR-1262-3	9.050	8.004	2183639	1480903	24.670	25.936
39)	L8 AR-1262-4	9.140	8.069	1517367	2341879	21.694	23.317
40)	L8 AR-1262-5	9.840	8.596	985360	1119171	21.059	22.375
41)	L9 AR-1268-1	9.050	8.004	2183639	1480903	14.305	9.306 #
42)	L9 AR-1268-2	9.140	8.069	1517367	2341879	11.108	16.355 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
Data File : PP067898.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 11:38
Operator : YP\AJ
Sample : P4368-07
Misc : AR1262 LOD 25 PPB
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:05:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	8.286	0	161714	N.D.	1.268 #
44) L9	AR-1268-4	9.840	8.596	985360	1119171	19.389	19.817
45) L9	AR-1268-5	10.294	8.922	332221	500397	0.890	1.324 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
Data File : PP067898.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 11:38
Operator : YP\AJ
Sample : P4368-07
Misc : AR1262 LOD 25 PPB
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:05:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

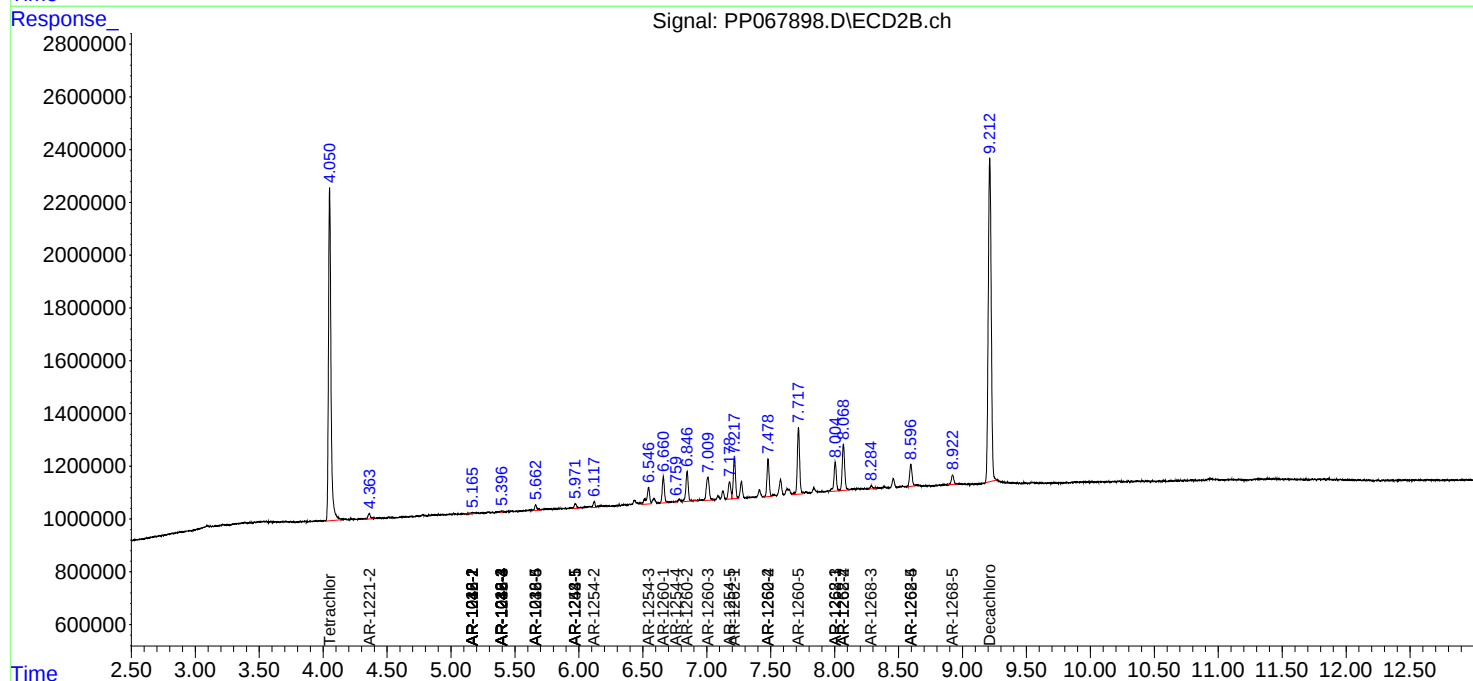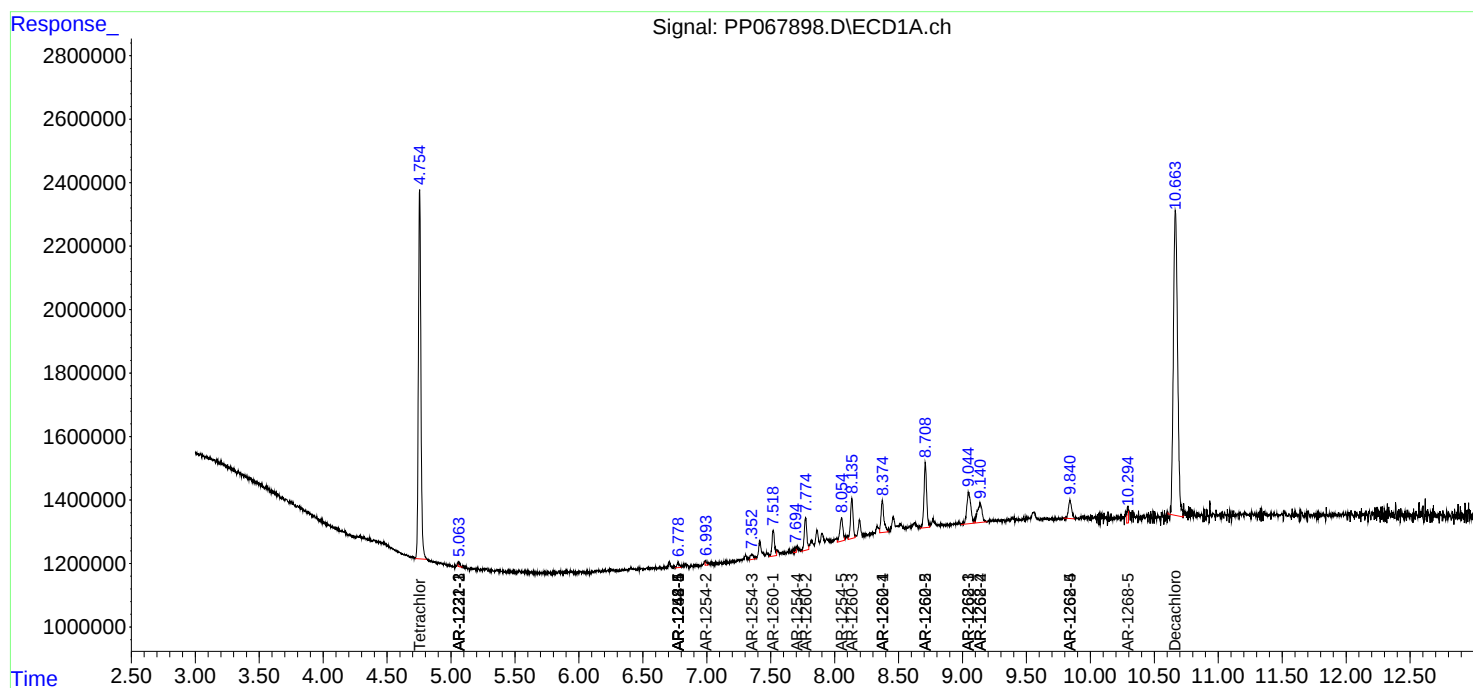


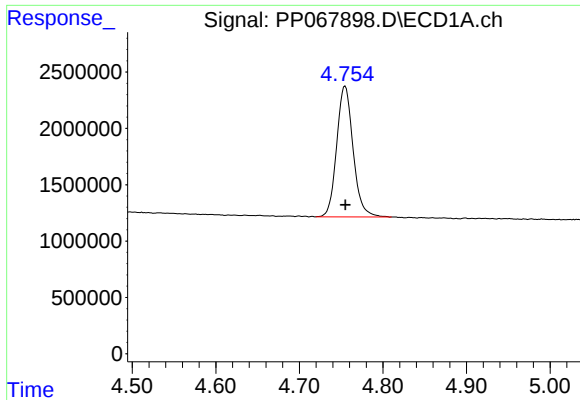

#1 Tetrachloro-m-xylene


R.T.: 4.755 min
Delta R.T.: 0.000 min
Response: 15862614
Conc: 17.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

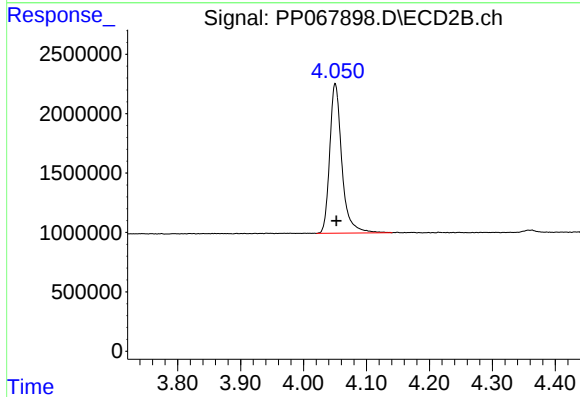


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 16931584
Conc: 16.76 ng/ml

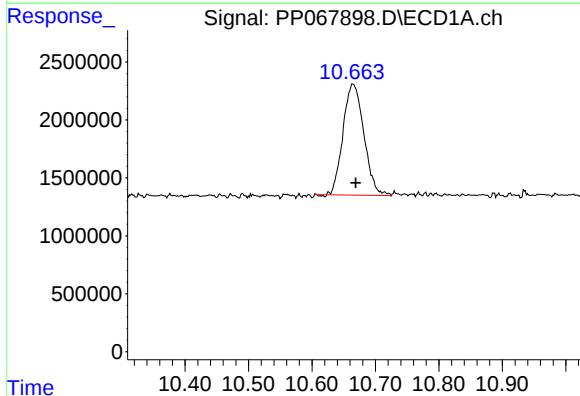


#2 Decachlorobiphenyl

R.T.: 10.665 min
Delta R.T.: -0.004 min
Response: 21892293
Conc: 19.02 ng/ml

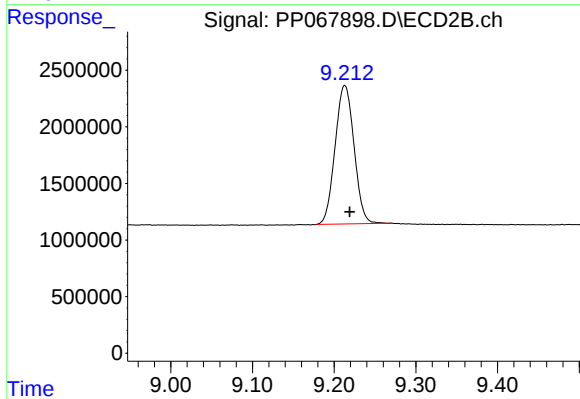

#2 Decachlorobiphenyl


R.T.: 9.213 min
Delta R.T.: -0.006 min
Response: 19778118
Conc: 17.64 ng/ml

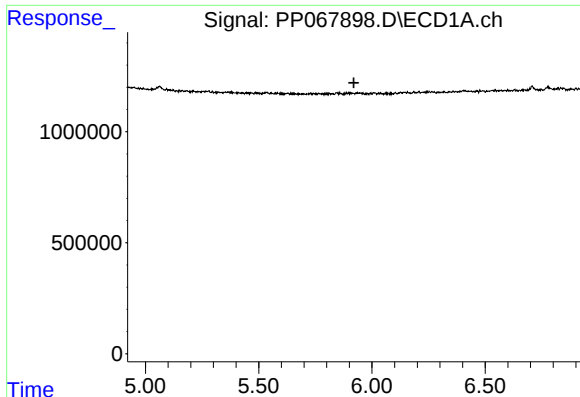

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.919 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

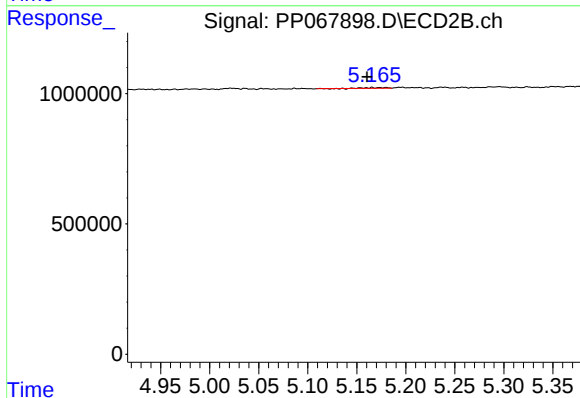


#3 AR-1016-1

R.T.: 5.166 min
Delta R.T.: 0.005 min
Response: 42748
Conc: 1.22 ng/ml

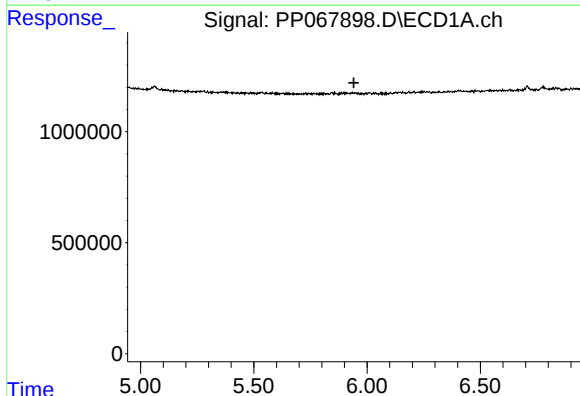


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.942 min
Response: 0
Conc: N.D.

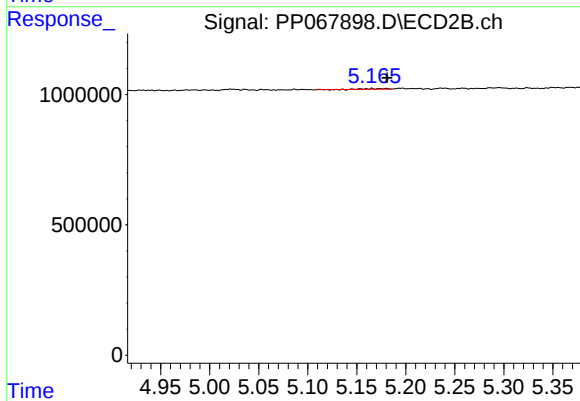

#4 AR-1016-2


R.T.: 5.166 min
Delta R.T.: -0.015 min
Response: 42748
Conc: 0.89 ng/ml

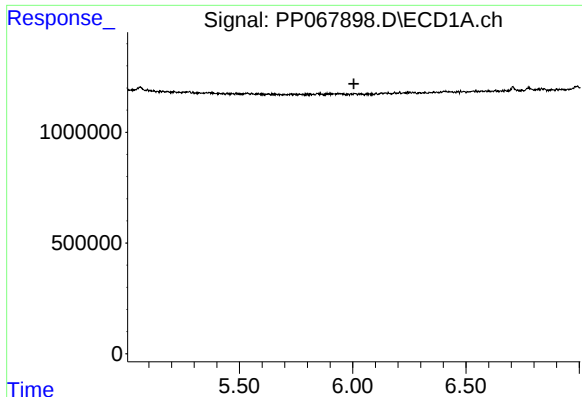

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 6.005 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

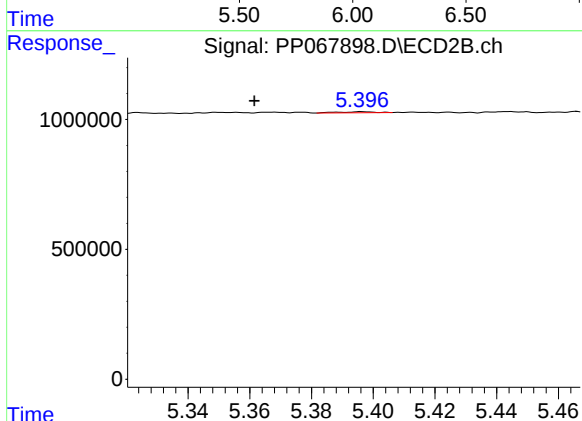


#5 AR-1016-3

R.T.: 5.396 min
Delta R.T.: 0.035 min
Response: 32114
Conc: 1.19 ng/ml

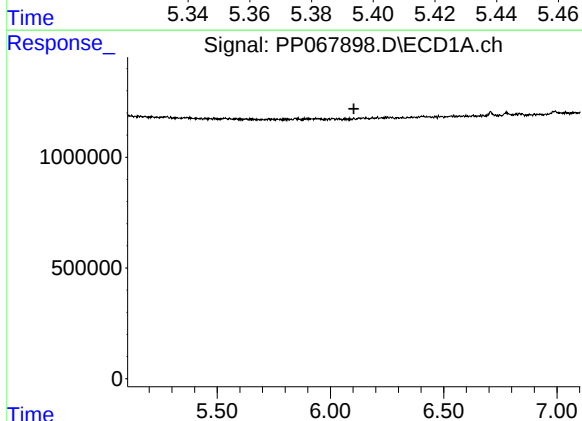


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 6.103 min
Response: 0
Conc: N.D.

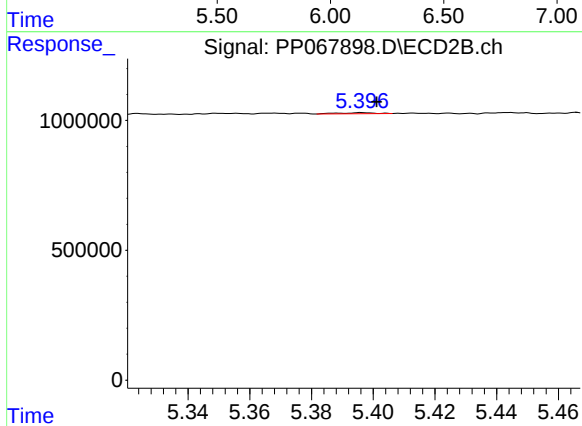

#6 AR-1016-4


R.T.: 5.396 min
Delta R.T.: -0.005 min
Response: 32114
Conc: 1.33 ng/ml

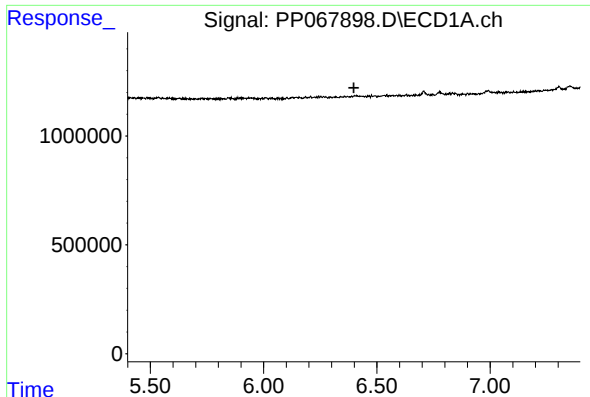

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

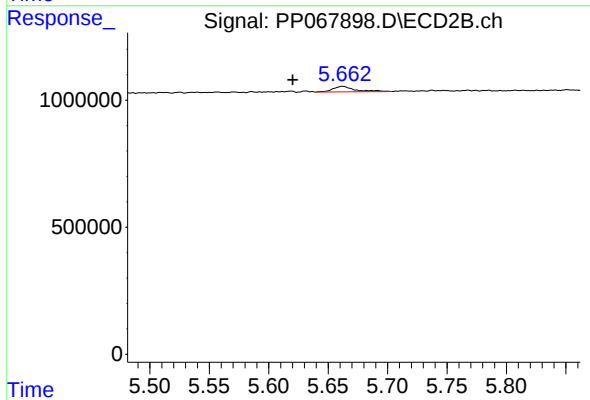


#7 AR-1016-5

R.T.: 5.662 min
Delta R.T.: 0.042 min
Response: 281725
Conc: 9.26 ng/ml

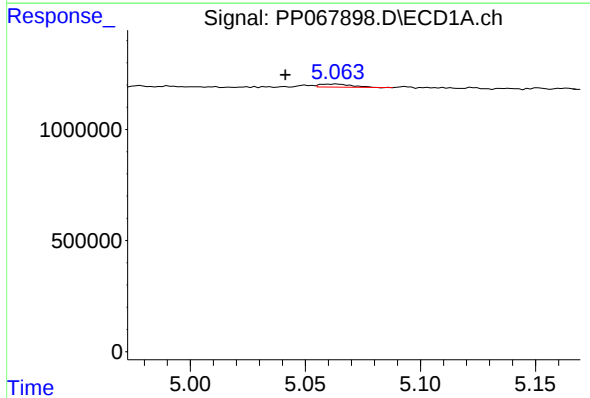


#9 AR-1221-2

R.T.: 5.063 min
Delta R.T.: 0.022 min
Response: 135366
Conc: 14.31 ng/ml

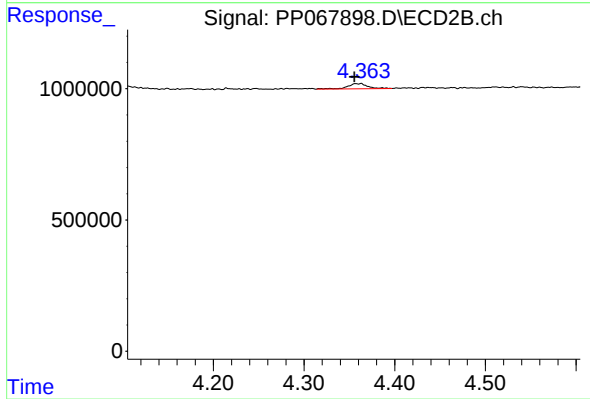

#9 AR-1221-2


R.T.: 4.363 min
Delta R.T.: 0.007 min
Response: 309652
Conc: 31.09 ng/ml

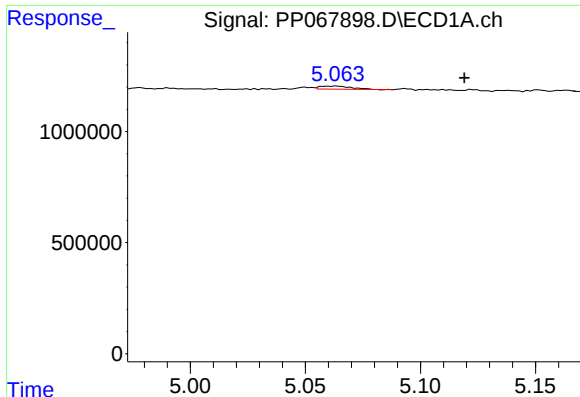

#10 AR-1221-3


R.T.: 5.063 min
Delta R.T.: -0.056 min
Response: 135366
Conc: 4.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

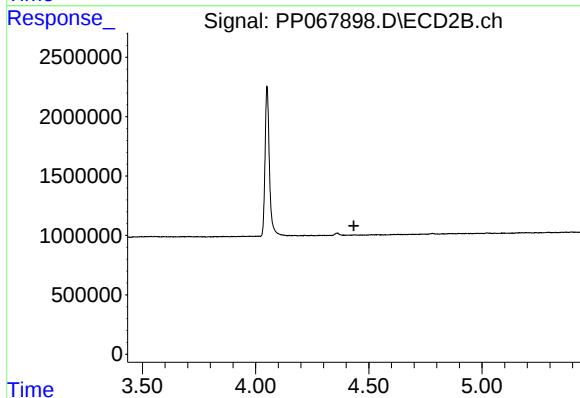


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.434 min
Response: 0
Conc: N.D.

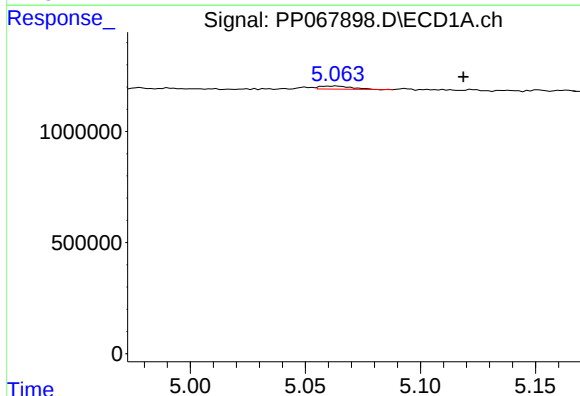


#11 AR-1232-1

R.T.: 5.063 min
Delta R.T.: -0.055 min
Response: 135366
Conc: 5.92 ng/ml

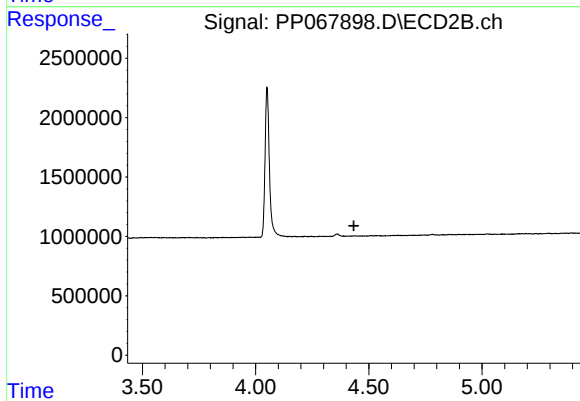

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.434 min
Response: 0
Conc: N.D.

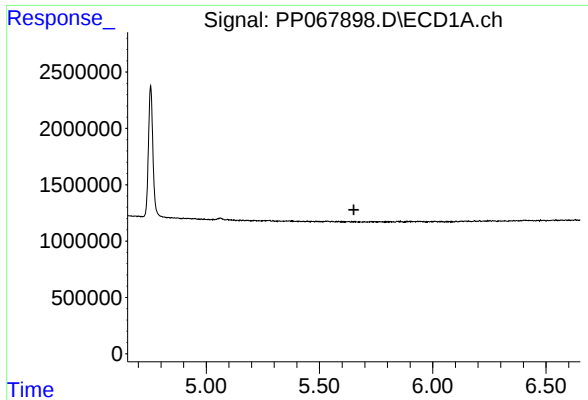

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 5.651 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

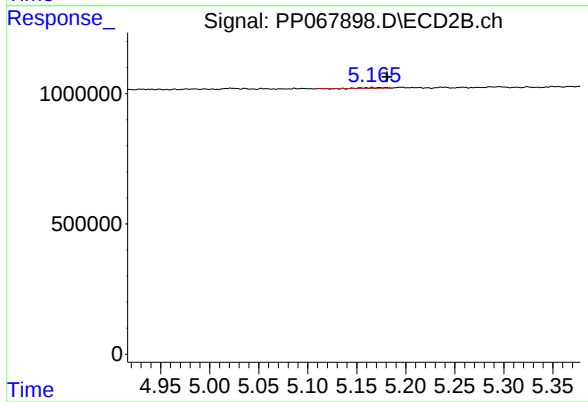


#12 AR-1232-2

R.T.: 5.166 min
Delta R.T.: -0.015 min
Response: 42748
Conc: 1.91 ng/ml

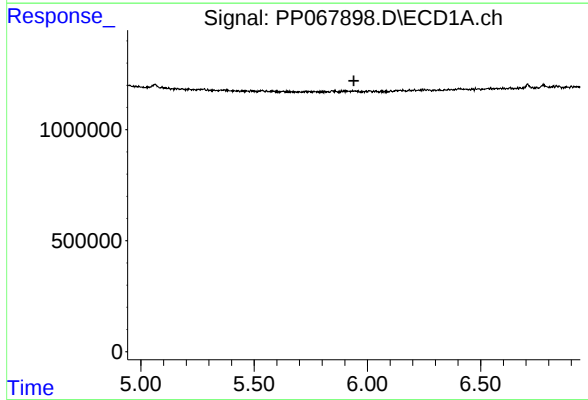


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 5.940 min
Response: 0
Conc: N.D.

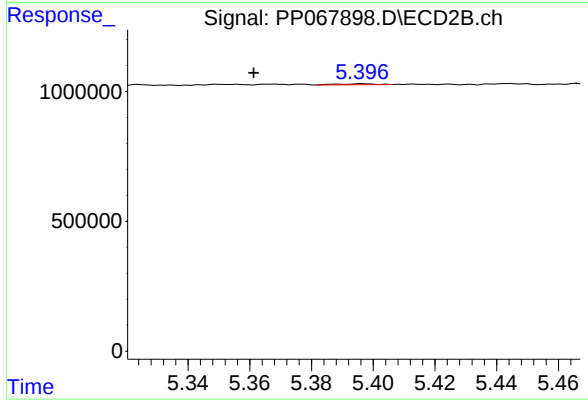

#13 AR-1232-3


R.T.: 5.396 min
Delta R.T.: 0.035 min
Response: 32114
Conc: 2.69 ng/ml

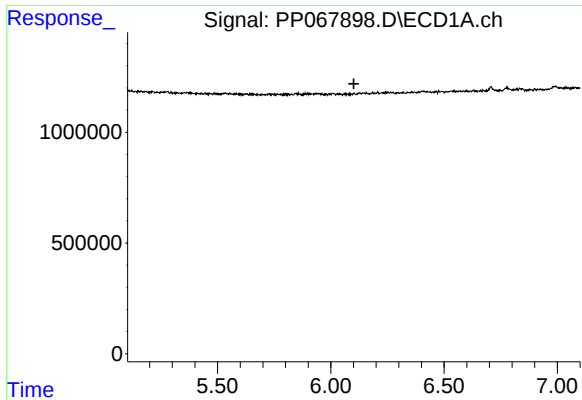

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T.: 6.101 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

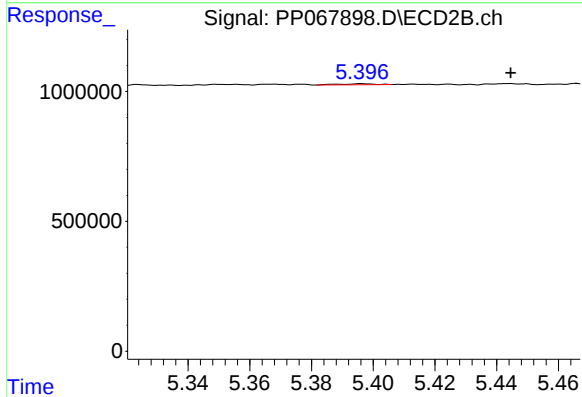


#14 AR-1232-4

R.T.: 5.396 min
Delta R.T.: -0.048 min
Response: 32114
Conc: 2.78 ng/ml

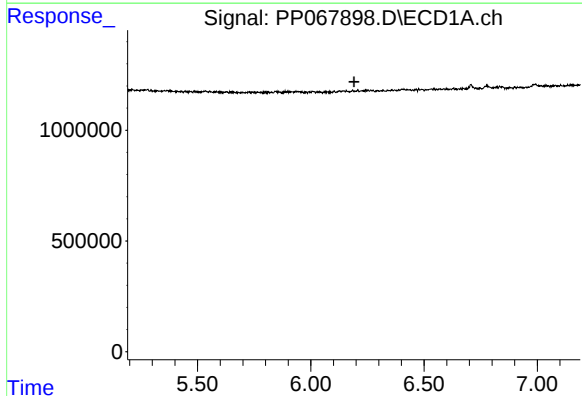


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

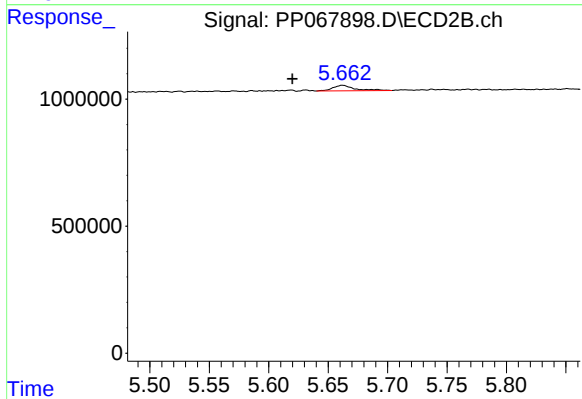

#15 AR-1232-5


R.T.: 5.662 min
Delta R.T.: 0.042 min
Response: 281725
Conc: 20.95 ng/ml

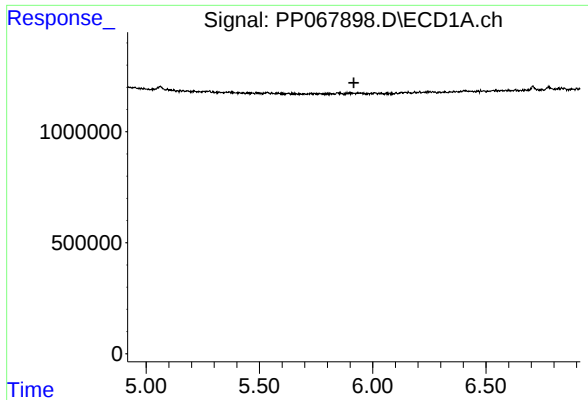

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T.: 5.916 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

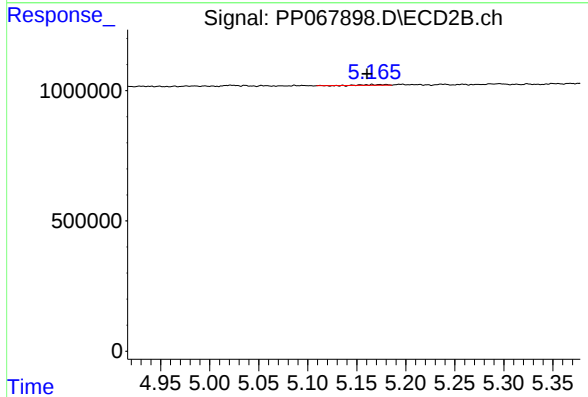


#16 AR-1242-1

R.T.: 5.166 min
Delta R.T.: 0.005 min
Response: 42748
Conc: 1.47 ng/ml

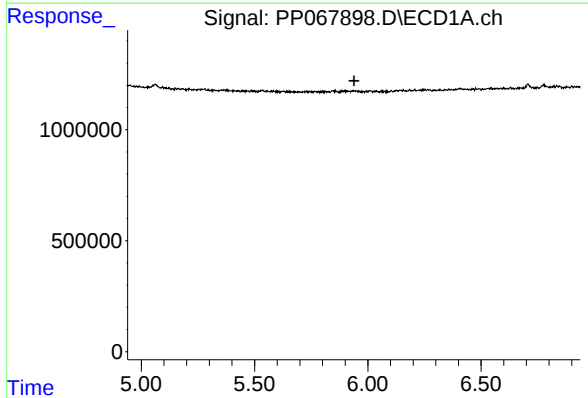


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T.: 5.939 min
Response: 0
Conc: N.D.

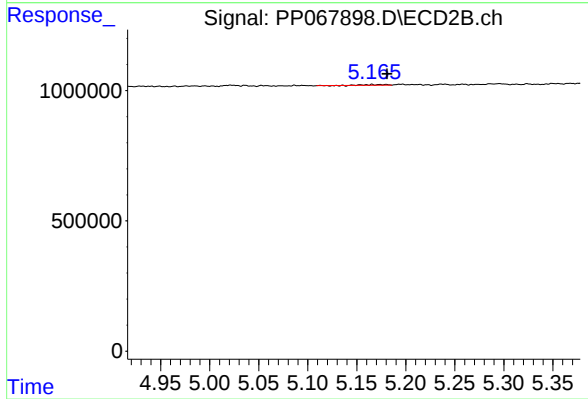

#17 AR-1242-2


R.T.: 5.166 min
Delta R.T.: -0.015 min
Response: 42748
Conc: 1.06 ng/ml

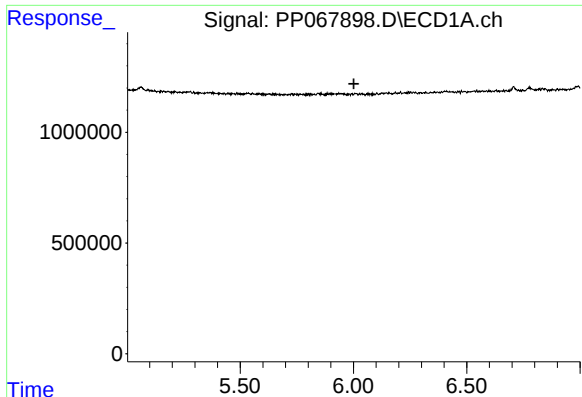

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 6.002 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

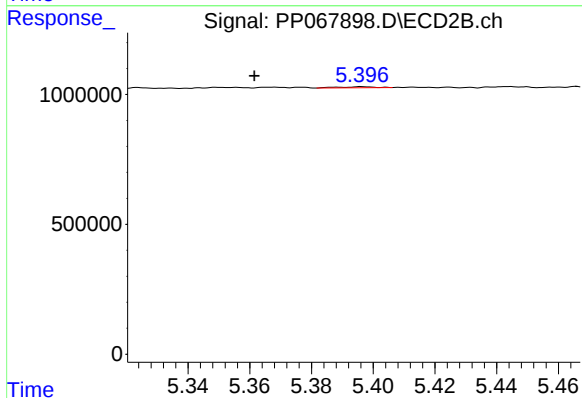


#18 AR-1242-3

R.T.: 5.396 min
Delta R.T.: 0.035 min
Response: 32114
Conc: 1.43 ng/ml

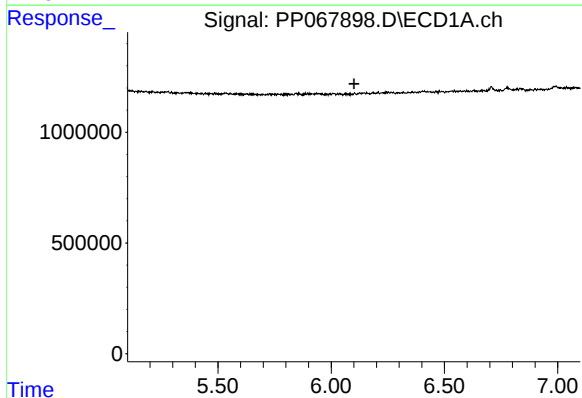


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T.: 6.101 min
Response: 0
Conc: N.D.

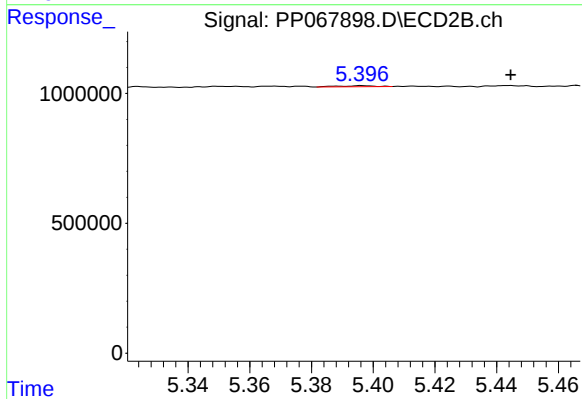

#19 AR-1242-4


R.T.: 5.396 min
Delta R.T.: -0.048 min
Response: 32114
Conc: 1.35 ng/ml

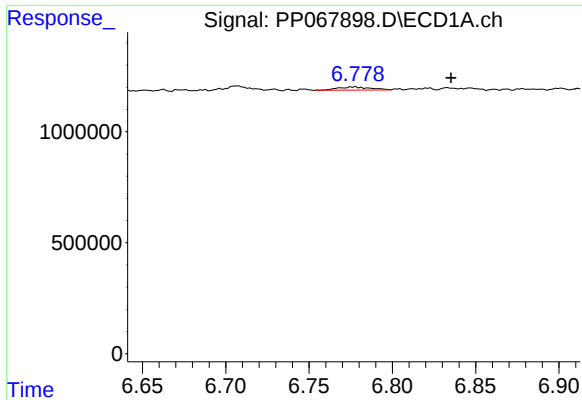

#20 AR-1242-5


R.T.: 6.777 min
Delta R.T.: -0.058 min
Response: 199617
Conc: 8.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

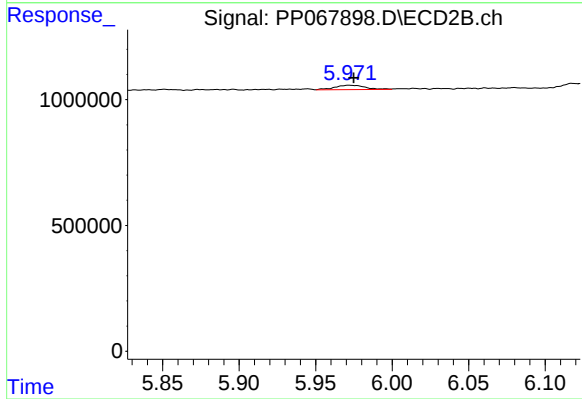


#20 AR-1242-5

R.T.: 5.972 min
Delta R.T.: -0.003 min
Response: 242876
Conc: 8.48 ng/ml

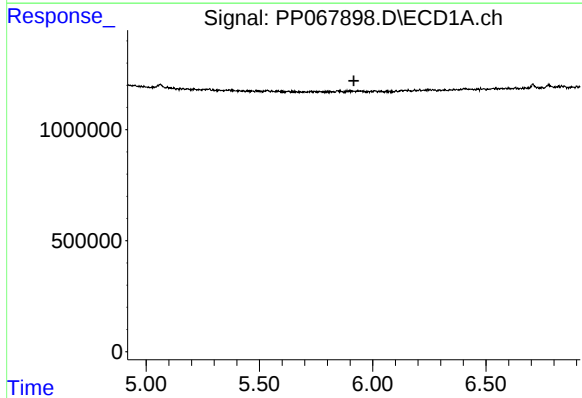


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 5.917 min
Response: 0
Conc: N.D.

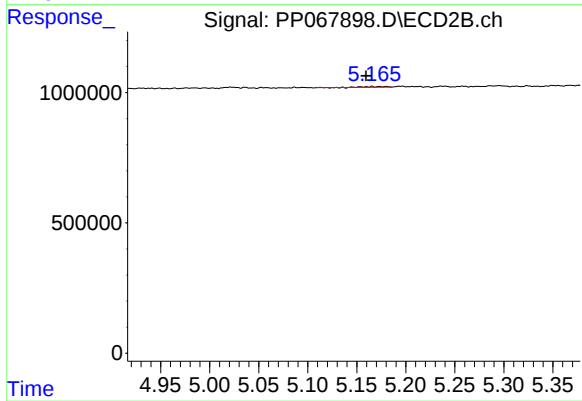

#21 AR-1248-1


R.T.: 5.166 min
Delta R.T.: 0.006 min
Response: 42748
Conc: 1.89 ng/ml

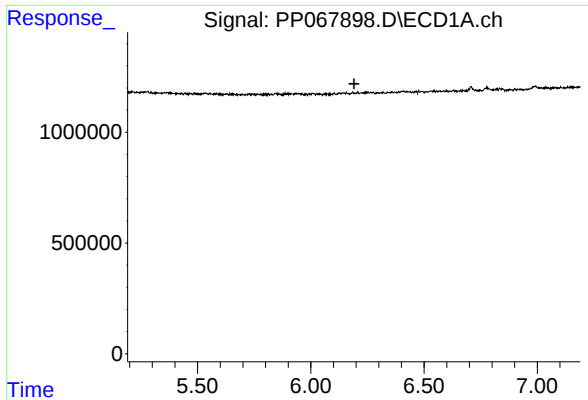

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

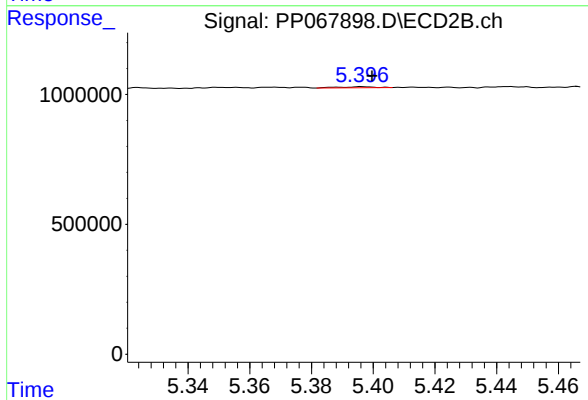


#22 AR-1248-2

R.T.: 5.396 min
Delta R.T.: -0.003 min
Response: 32114
Conc: 0.97 ng/ml

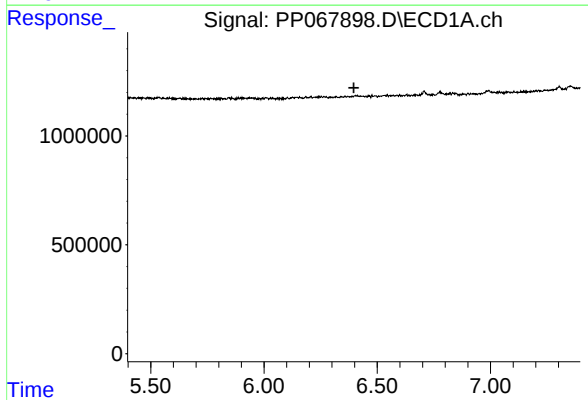


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

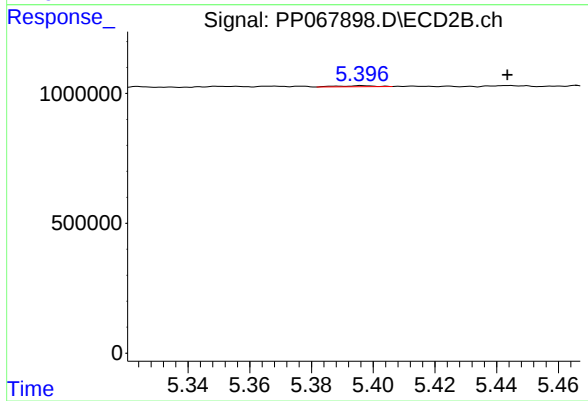

#23 AR-1248-3


R.T.: 5.396 min
Delta R.T.: -0.047 min
Response: 32114
Conc: 0.93 ng/ml

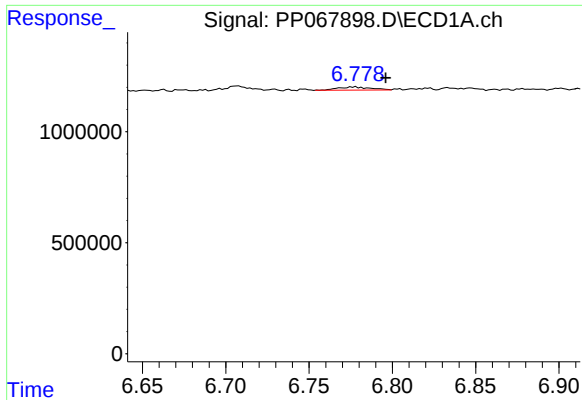

#24 AR-1248-4


R.T.: 6.777 min
Delta R.T.: -0.019 min
Response: 199617
Conc: 4.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

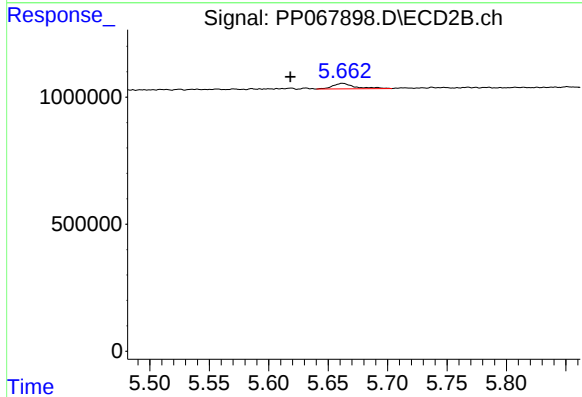


#24 AR-1248-4

R.T.: 5.662 min
Delta R.T.: 0.044 min
Response: 281725
Conc: 6.88 ng/ml

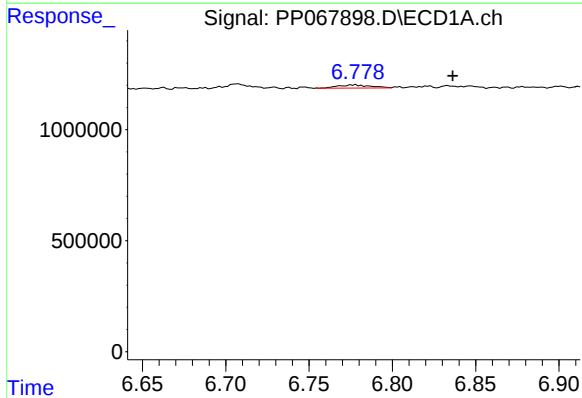


#25 AR-1248-5

R.T.: 6.777 min
Delta R.T.: -0.059 min
Response: 199617
Conc: 5.03 ng/ml

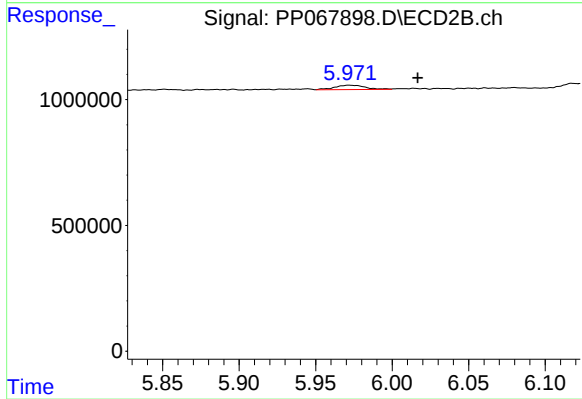

#25 AR-1248-5


R.T.: 5.972 min
Delta R.T.: -0.045 min
Response: 242876
Conc: 6.49 ng/ml

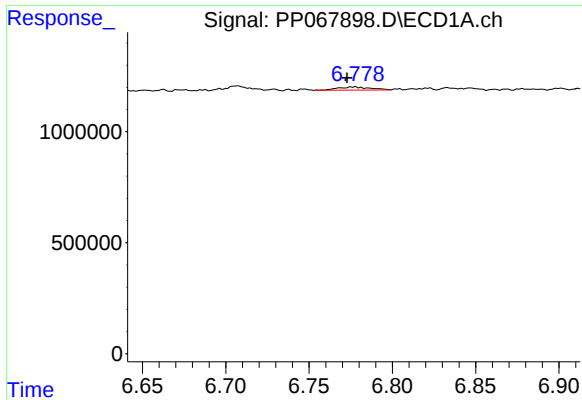

#26 AR-1254-1


R.T.: 6.777 min
Delta R.T.: 0.005 min
Response: 199617
Conc: 4.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

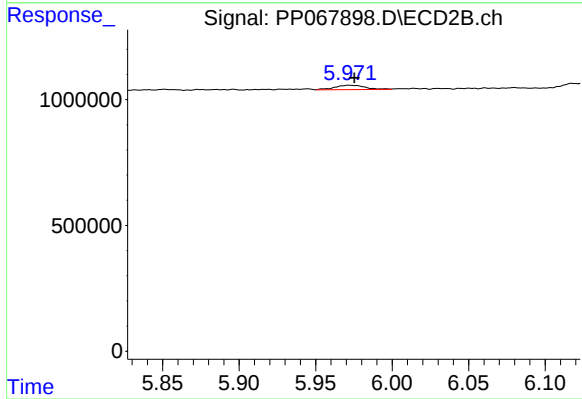


#26 AR-1254-1

R.T.: 5.972 min
Delta R.T.: -0.003 min
Response: 242876
Conc: 4.11 ng/ml

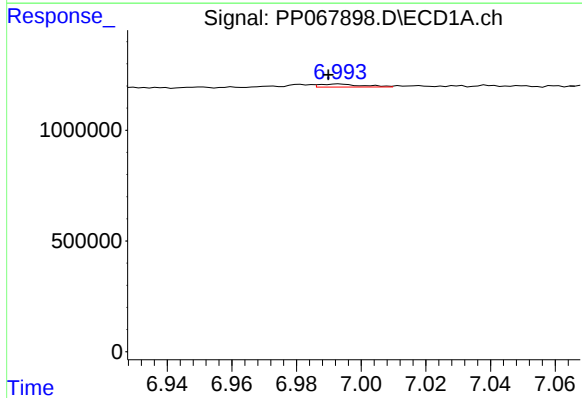


#27 AR-1254-2

R.T.: 6.993 min
Delta R.T.: 0.003 min
Response: 124019
Conc: 1.88 ng/ml

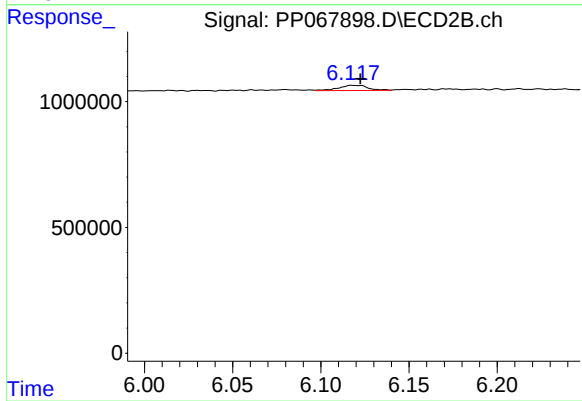

#27 AR-1254-2


R.T.: 6.118 min
Delta R.T.: -0.004 min
Response: 247073
Conc: 4.71 ng/ml

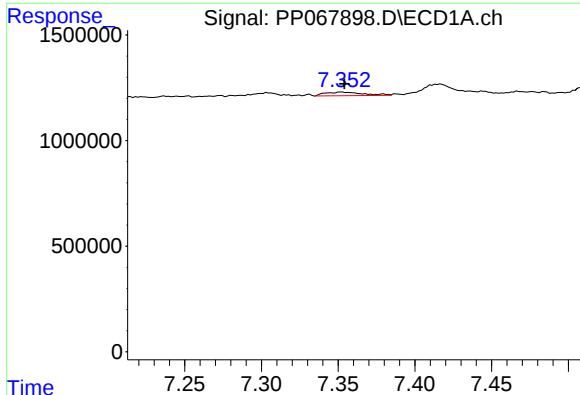

#28 AR-1254-3


R.T.: 7.352 min
Delta R.T.: -0.002 min
Response: 288907
Conc: 4.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

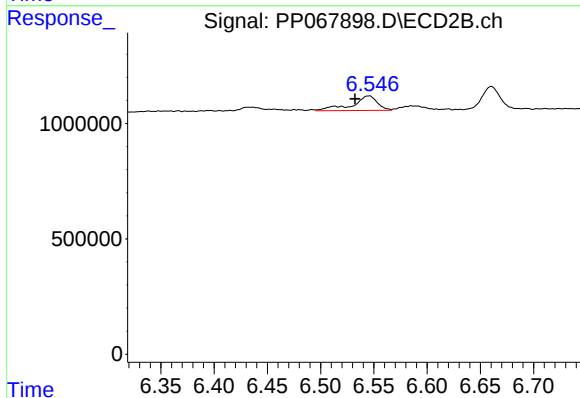


#28 AR-1254-3

R.T.: 6.545 min
Delta R.T.: 0.013 min
Response: 1036322
Conc: 12.45 ng/ml

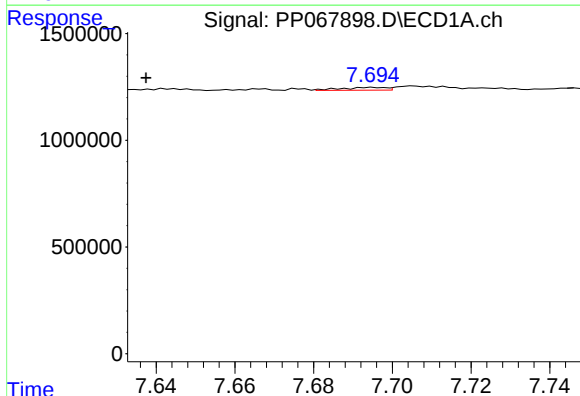


#29 AR-1254-4

R.T.: 7.695 min
Delta R.T.: 0.057 min
Response: 99936
Conc: 2.00 ng/ml

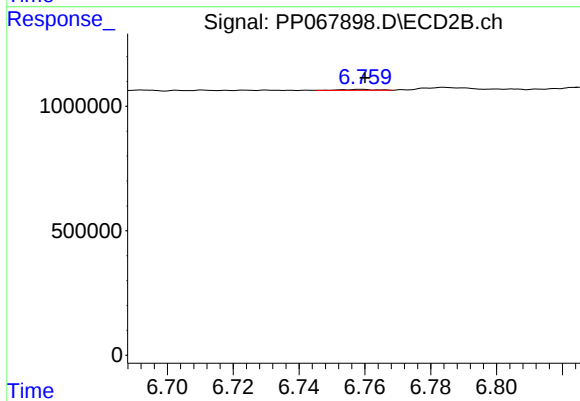

#29 AR-1254-4


R.T.: 6.759 min
Delta R.T.: -0.001 min
Response: 30590
Conc: 0.63 ng/ml

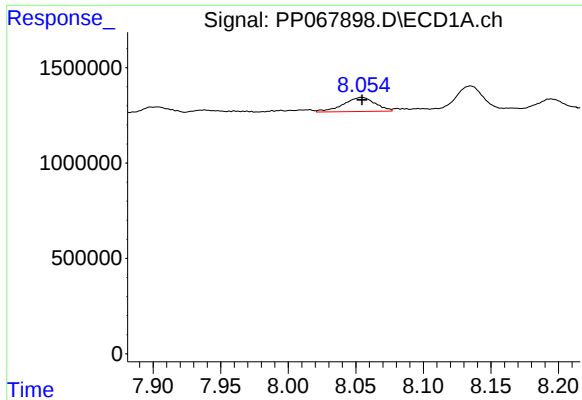

#30 AR-1254-5


R.T.: 8.055 min
Delta R.T.: 0.000 min
Response: 1215406
Conc: 20.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

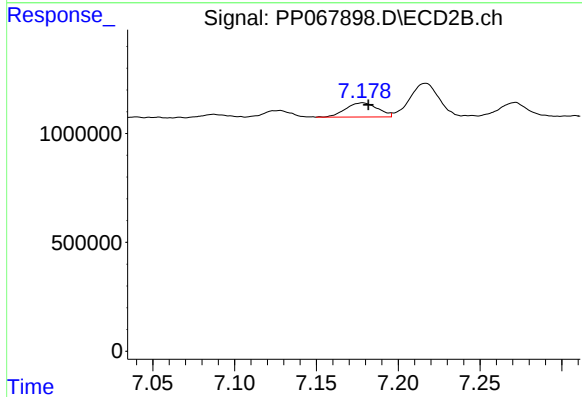


#30 AR-1254-5

R.T.: 7.178 min
Delta R.T.: -0.004 min
Response: 896898
Conc: 12.19 ng/ml

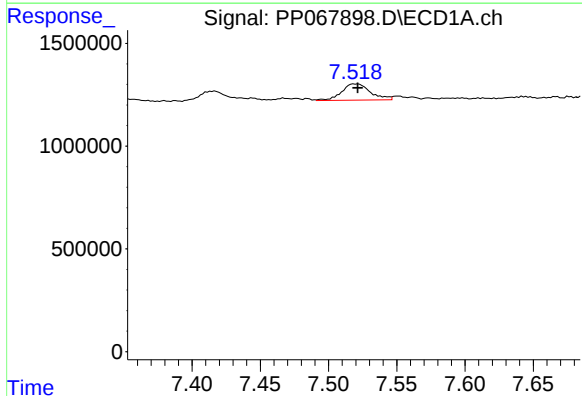


#31 AR-1260-1

R.T.: 7.519 min
Delta R.T.: -0.002 min
Response: 1163112
Conc: 21.53 ng/ml

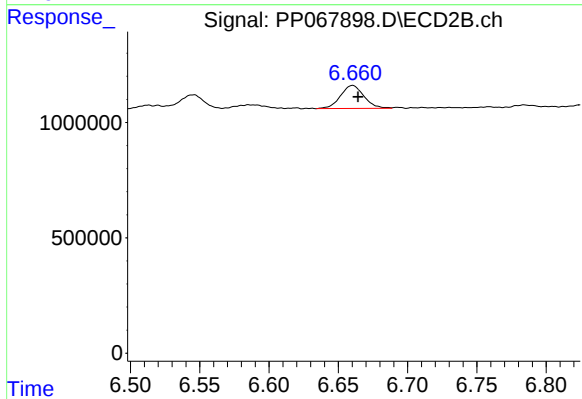

#31 AR-1260-1


R.T.: 6.660 min
Delta R.T.: -0.004 min
Response: 1178212
Conc: 20.68 ng/ml

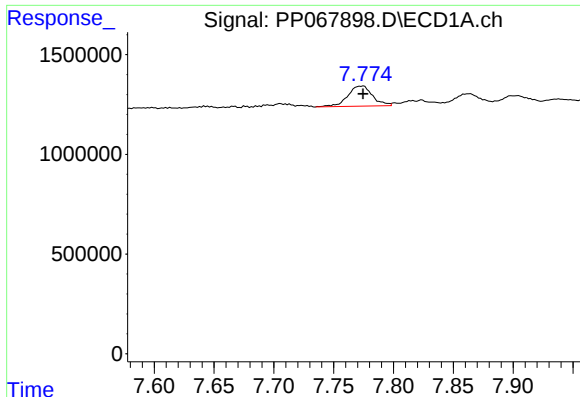

#32 AR-1260-2


R.T.: 7.774 min
Delta R.T.: 0.000 min
Response: 1460624
Conc: 23.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

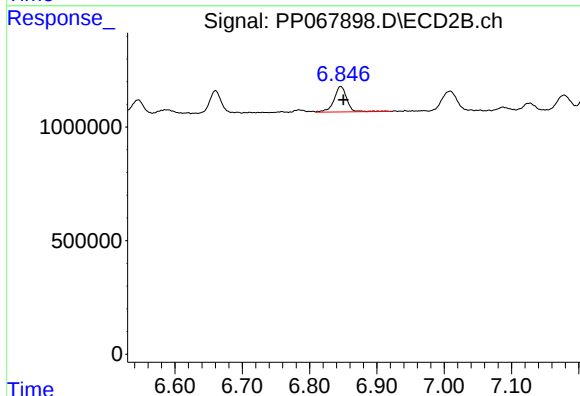


#32 AR-1260-2

R.T.: 6.846 min
Delta R.T.: -0.004 min
Response: 1500199
Conc: 22.49 ng/ml

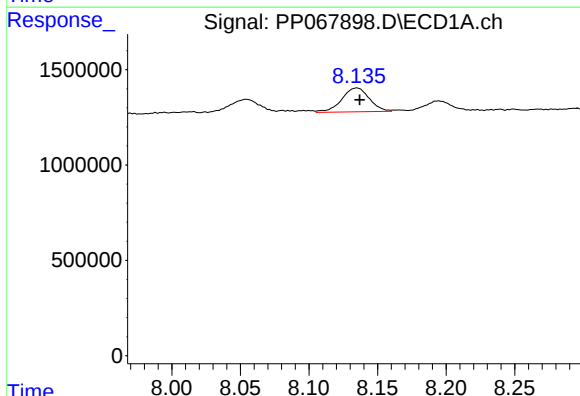


#33 AR-1260-3

R.T.: 8.135 min
Delta R.T.: -0.002 min
Response: 1759148
Conc: 33.93 ng/ml

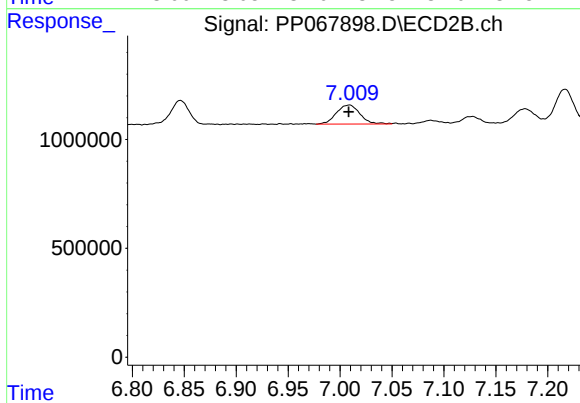

#33 AR-1260-3


R.T.: 7.009 min
Delta R.T.: 0.000 min
Response: 1378542
Conc: 21.64 ng/ml

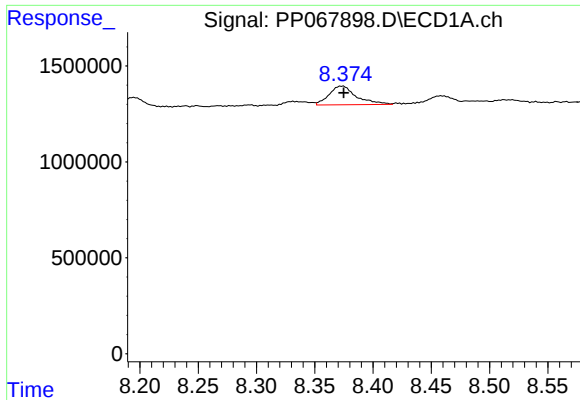

#34 AR-1260-4


R.T.: 8.374 min
Delta R.T.: -0.001 min
Response: 1597710
Conc: 26.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

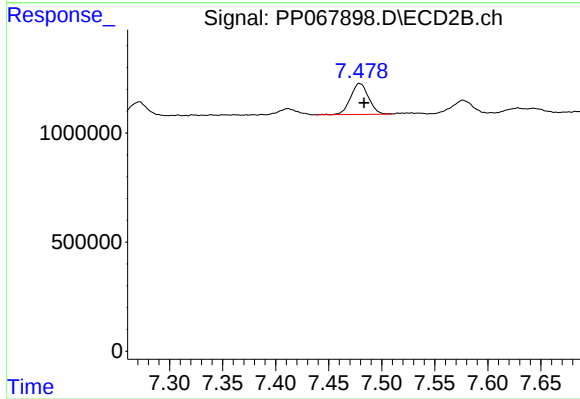


#34 AR-1260-4

R.T.: 7.479 min
Delta R.T.: -0.004 min
Response: 1691889
Conc: 30.60 ng/ml

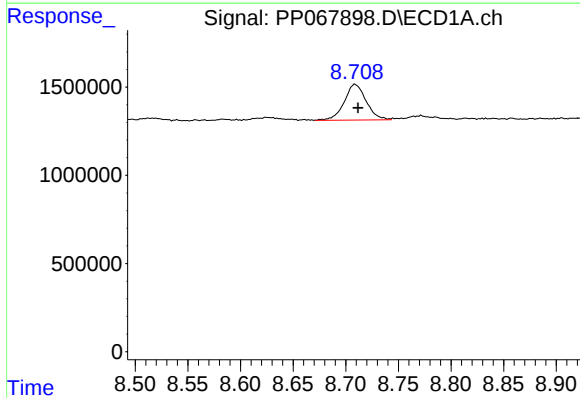


#35 AR-1260-5

R.T.: 8.709 min
Delta R.T.: -0.003 min
Response: 2957998
Conc: 27.46 ng/ml

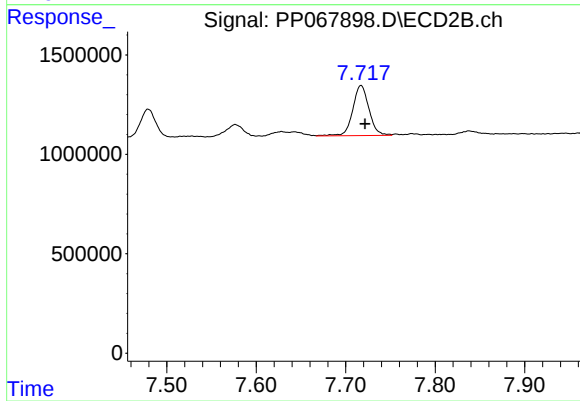

#35 AR-1260-5


R.T.: 7.717 min
Delta R.T.: -0.004 min
Response: 3193118
Conc: 26.11 ng/ml

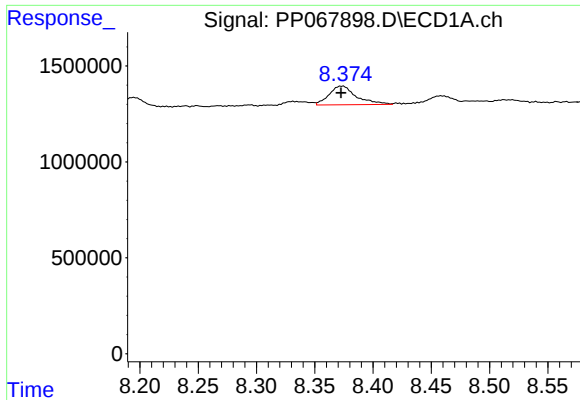

#36 AR-1262-1


R.T.: 8.374 min
Delta R.T.: 0.000 min
Response: 1597710
Conc: 22.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

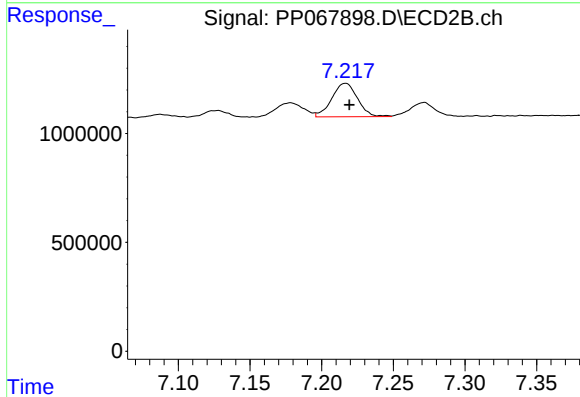


#36 AR-1262-1

R.T.: 7.217 min
Delta R.T.: -0.003 min
Response: 1921638
Conc: 24.43 ng/ml

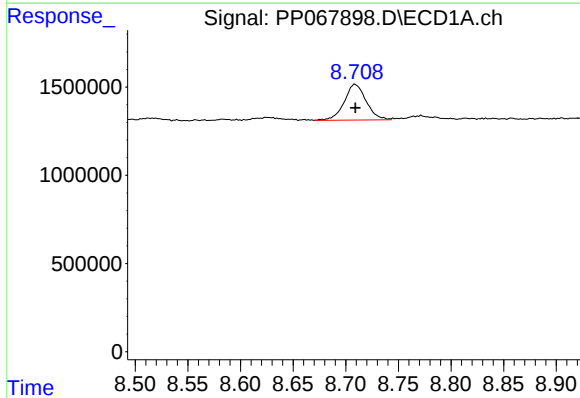


#37 AR-1262-2

R.T.: 8.709 min
Delta R.T.: 0.000 min
Response: 2957998
Conc: 24.33 ng/ml

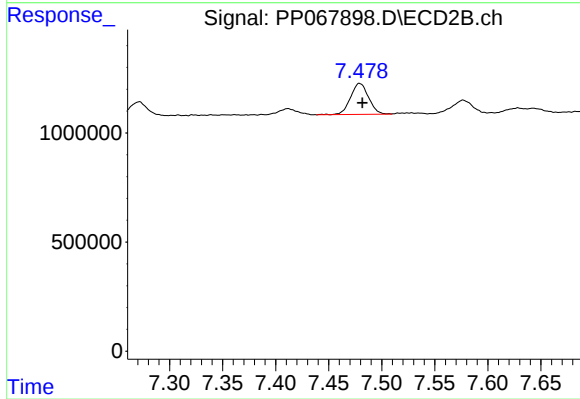

#37 AR-1262-2


R.T.: 7.479 min
Delta R.T.: -0.003 min
Response: 1691889
Conc: 23.84 ng/ml

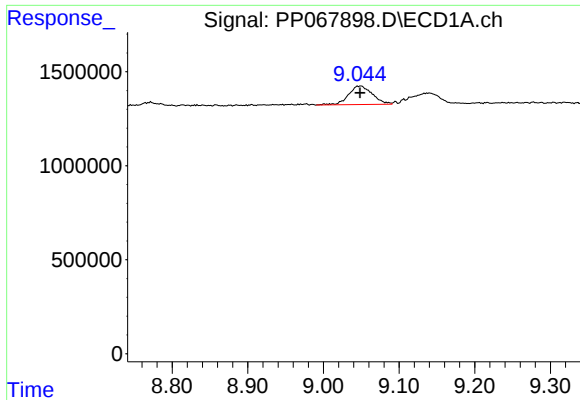

#38 AR-1262-3


R.T.: 9.050 min
Delta R.T.: 0.002 min
Response: 2183639
Conc: 24.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

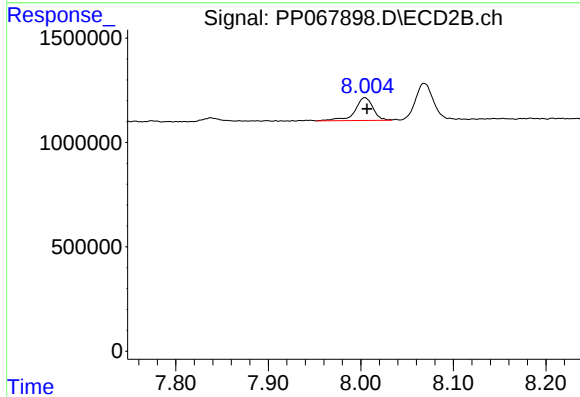


#38 AR-1262-3

R.T.: 8.004 min
Delta R.T.: -0.002 min
Response: 1480903
Conc: 25.94 ng/ml

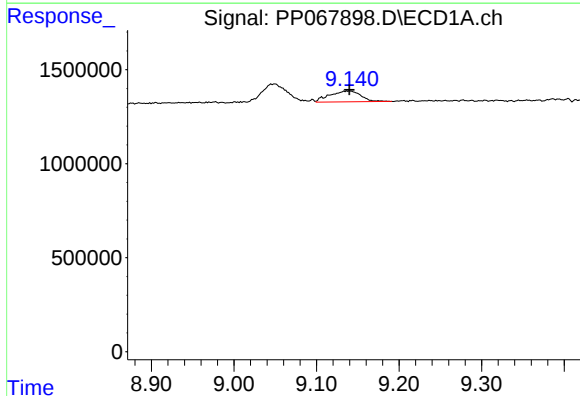


#39 AR-1262-4

R.T.: 9.140 min
Delta R.T.: 0.000 min
Response: 1517367
Conc: 21.69 ng/ml

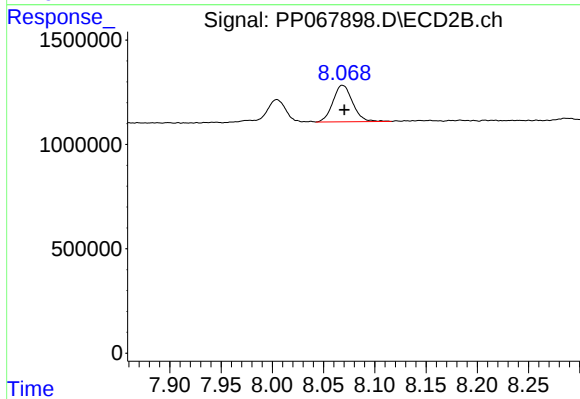

#39 AR-1262-4


R.T.: 8.069 min
Delta R.T.: -0.002 min
Response: 2341879
Conc: 23.32 ng/ml

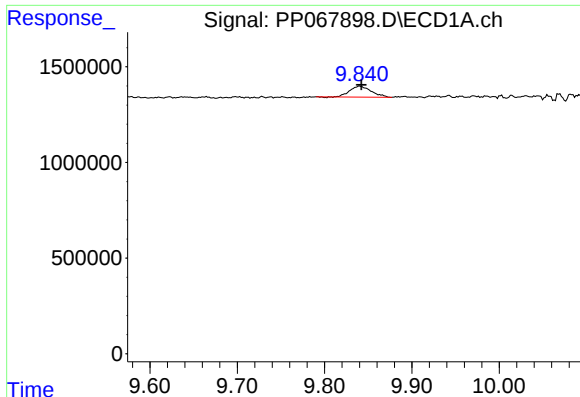

#40 AR-1262-5


R.T.: 9.840 min
Delta R.T.: -0.002 min
Response: 985360
Conc: 21.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

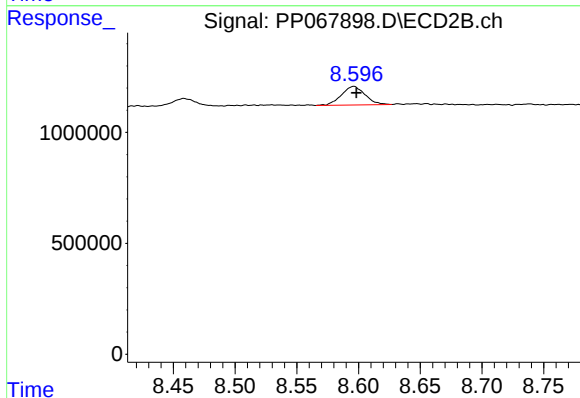


#40 AR-1262-5

R.T.: 8.596 min
Delta R.T.: -0.002 min
Response: 1119171
Conc: 22.38 ng/ml

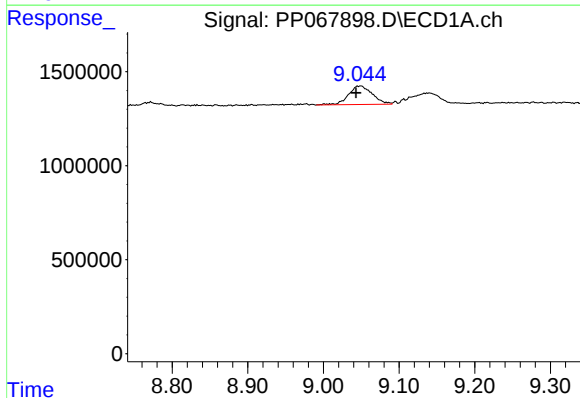


#41 AR-1268-1

R.T.: 9.050 min
Delta R.T.: 0.007 min
Response: 2183639
Conc: 14.31 ng/ml

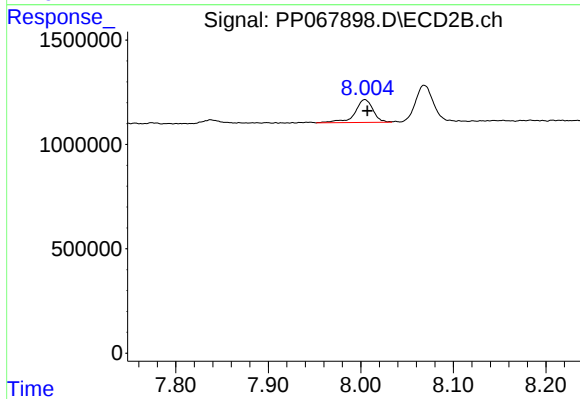

#41 AR-1268-1


R.T.: 8.004 min
Delta R.T.: -0.003 min
Response: 1480903
Conc: 9.31 ng/ml

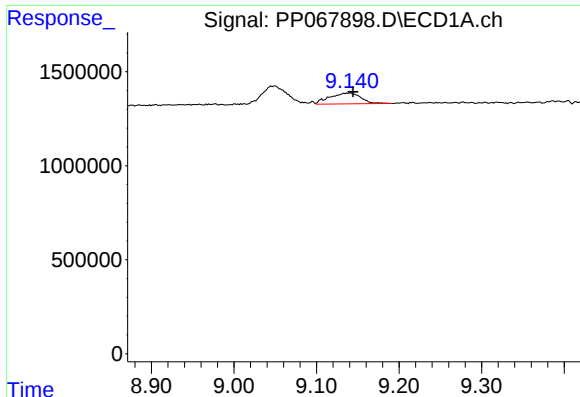

#42 AR-1268-2


R.T.: 9.140 min
Delta R.T.: -0.004 min
Response: 1517367
Conc: 11.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

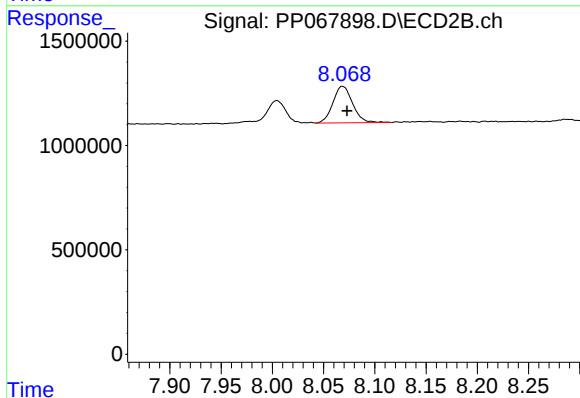


#42 AR-1268-2

R.T.: 8.069 min
Delta R.T.: -0.004 min
Response: 2341879
Conc: 16.36 ng/ml

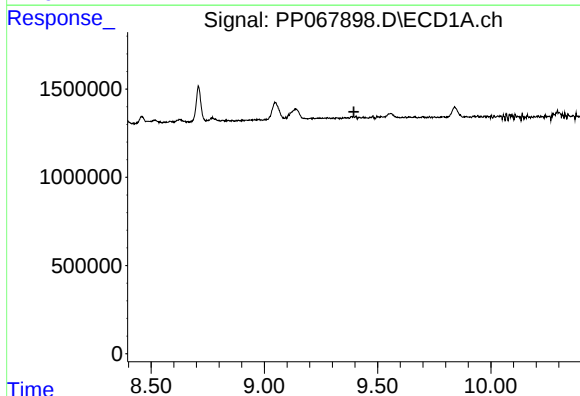


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 9.395 min
Response: 0
Conc: N.D.

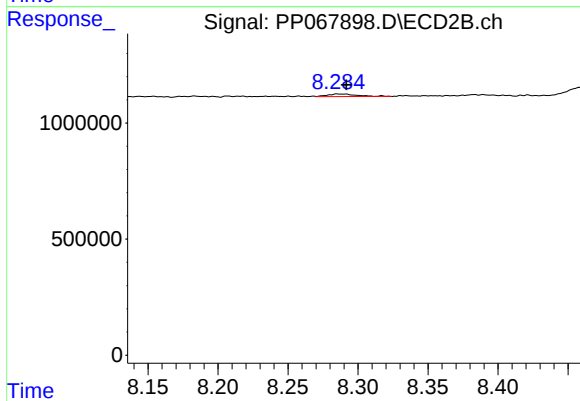

#43 AR-1268-3


R.T.: 8.286 min
Delta R.T.: -0.006 min
Response: 161714
Conc: 1.27 ng/ml

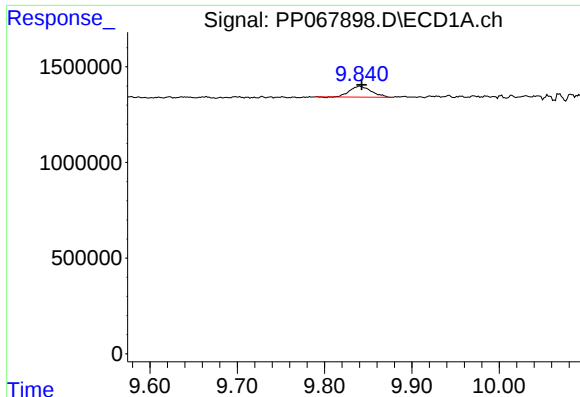

#44 AR-1268-4


R.T.: 9.840 min
Delta R.T.: -0.002 min
Response: 985360
Conc: 19.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

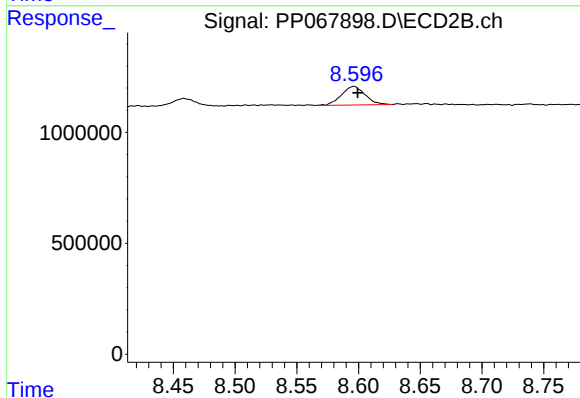


#44 AR-1268-4

R.T.: 8.596 min
Delta R.T.: -0.003 min
Response: 1119171
Conc: 19.82 ng/ml

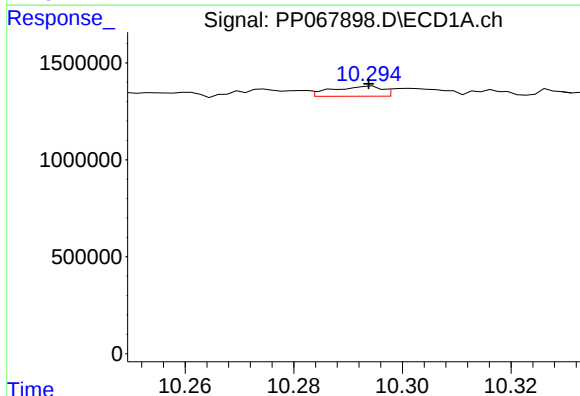

#45 AR-1268-5

R.T.: 10.294 min
Delta R.T.: 0.000 min
Response: 332221
Conc: 0.89 ng/ml

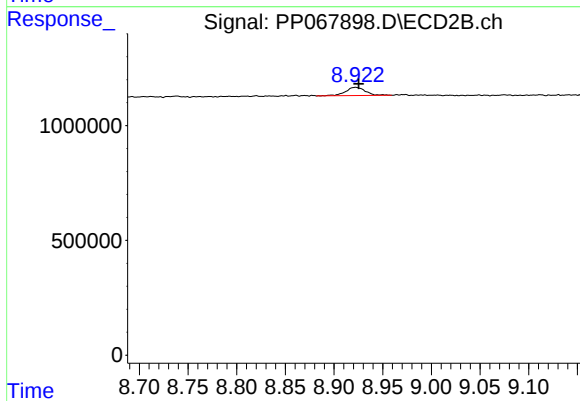

#45 AR-1268-5

R.T.: 8.922 min
Delta R.T.: -0.003 min
Response: 500397
Conc: 1.32 ng/ml