

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
 Data File : PP067947.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2024 00:46
 Operator : YP\AJ
 Sample : P4368-07
 Misc : AR1232 LOD 40 PPB
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 07:29:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.753	4.050	15369738	16383981	16.604	16.215
2)	SA Decachlor...	10.662	9.210	21351655	19618379	18.546	17.494
Target Compounds							
3)	L1 AR-1016-1	5.917	5.158	530734	611814	16.050	17.487
4)	L1 AR-1016-2	5.938	5.177	785503	804446	16.106	16.701
5)	L1 AR-1016-3	6.003	5.357	434377	400913	13.785	14.883
6)	L1 AR-1016-4	6.100	5.396	409522	340046	15.908	14.119
7)	L1 AR-1016-5	6.397	5.615	394726	440168	14.583	14.474
8)	L2 AR-1221-1	4.956	4.263	224676	271044	17.539	20.580
9)	L2 AR-1221-2	5.040	4.357	166180	494632	17.566	49.656 #
10)	L2 AR-1221-3	5.119	4.431	726877	950212	25.145	30.523
11)	L3 AR-1232-1	5.119	4.431	726877	950212	31.797	39.050
12)	L3 AR-1232-2	5.652	5.177	458639	804446	38.924	35.969
13)	L3 AR-1232-3	5.938	5.357	785503	400913	35.264	33.567
14)	L3 AR-1232-4	6.100	5.440	409522	383058	36.281	33.219
15)	L3 AR-1232-5	6.186	5.615	310047	440168	33.996	32.725
16)	L4 AR-1242-1	5.917	5.158	530734	611814	18.997	21.042
17)	L4 AR-1242-2	5.938	5.177	785503	804446	19.331	20.037
18)	L4 AR-1242-3	6.003	5.357	434377	400913	16.109	17.822
19)	L4 AR-1242-4	6.100	5.440	409522	383058	19.092	16.137
20)	L4 AR-1242-5	6.837	5.970	330217	551943	13.687	19.265 #
21)	L5 AR-1248-1	5.917	5.158	530734	611814	24.774	26.995
22)	L5 AR-1248-2	6.186	5.396	310047	340046	9.223	10.275
23)	L5 AR-1248-3	6.397	5.440	394726	383058	10.777	11.111
24)	L5 AR-1248-4	6.794	5.615	362323	440168	8.957	10.747
25)	L5 AR-1248-5	6.837	6.013	330217	430325	8.326	11.493 #
26)	L6 AR-1254-1	6.771	5.970	371933	551943	8.305	9.342
27)	L6 AR-1254-2	6.992	6.117	402963	188069	6.096	3.585 #
28)	L6 AR-1254-3	7.350	6.527	188719	433654	2.717	5.212 #
29)	L6 AR-1254-4	7.637	6.760	241440	179989	4.838	3.728
30)	L6 AR-1254-5	8.054	7.180	235114	234330	3.965	3.186
31)	L7 AR-1260-1	7.556	6.678	185290	227235	3.430	3.989
32)	L7 AR-1260-2	7.772	6.845	113275	79119	1.790	1.186 #
33)	L7 AR-1260-3	8.130	7.009	289770	213281	5.589	3.348 #
34)	L7 AR-1260-4	0.000	7.478	0	63887	N.D.	1.155 #
35)	L7 AR-1260-5	8.726	7.710	277069	223450	2.572	1.827 #
36)	L8 AR-1262-1	0.000	7.220	0	25024	N.D.	0.318 #
37)	L8 AR-1262-2	8.726	7.478	277069	63887	2.279	0.900 #
38)	L8 AR-1262-3	0.000	8.060f	0	112603	N.D.	1.972 #
39)	L8 AR-1262-4	0.000	8.060	0	112603	N.D.	1.121 #
40)	L8 AR-1262-5	0.000	8.599	0	39209	N.D.	0.784 #
41)	L9 AR-1268-1	0.000	8.060f	0	112603	N.D.	0.708 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
Data File : PP067947.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 00:46
Operator : YP\AJ
Sample : P4368-07
Misc : AR1232 LOD 40 PPB
ALS Vial : 53 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:29:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	8.060	0	112603	N.D.	0.786 #
43) L9	AR-1268-3	0.000	8.284	0	90315	N.D.	0.708 #
44) L9	AR-1268-4	0.000	8.599	0	39209	N.D.	0.694 #
45) L9	AR-1268-5	0.000	8.921	0	61770	N.D.	0.163 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

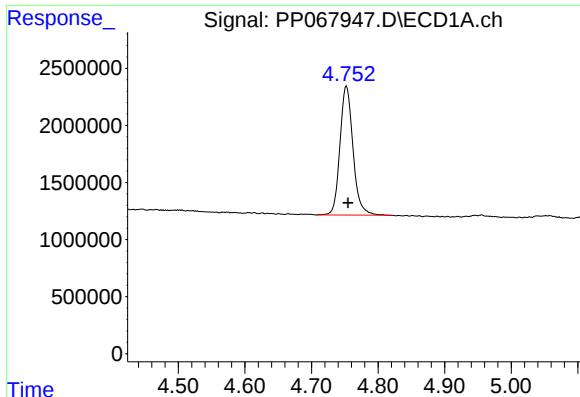

#1 Tetrachloro-m-xylene


R.T.: 4.753 min
Delta R.T.: -0.002 min
Response: 15369738
Conc: 16.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

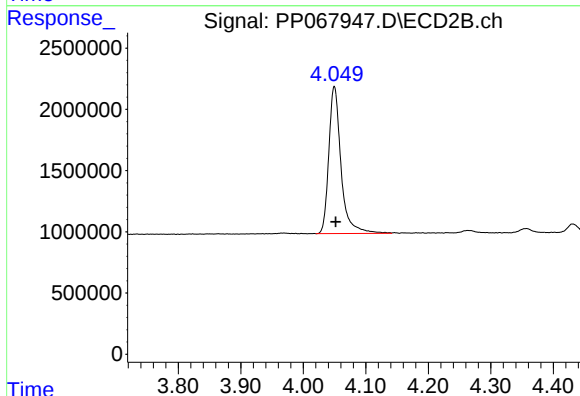


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 16383981
Conc: 16.22 ng/ml

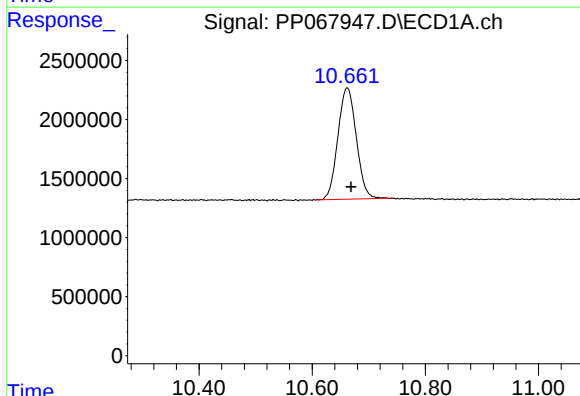


#2 Decachlorobiphenyl

R.T.: 10.662 min
Delta R.T.: -0.007 min
Response: 21351655
Conc: 18.55 ng/ml

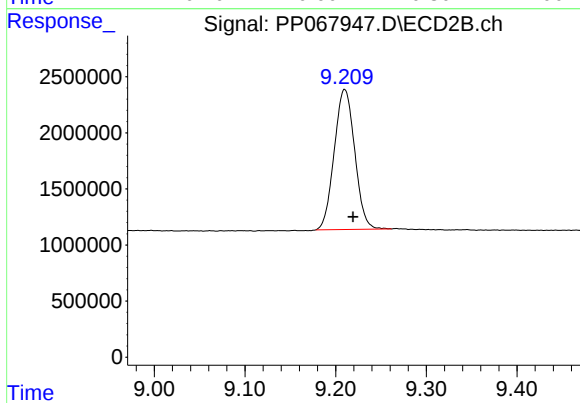

#2 Decachlorobiphenyl


R.T.: 9.210 min
Delta R.T.: -0.009 min
Response: 19618379
Conc: 17.49 ng/ml

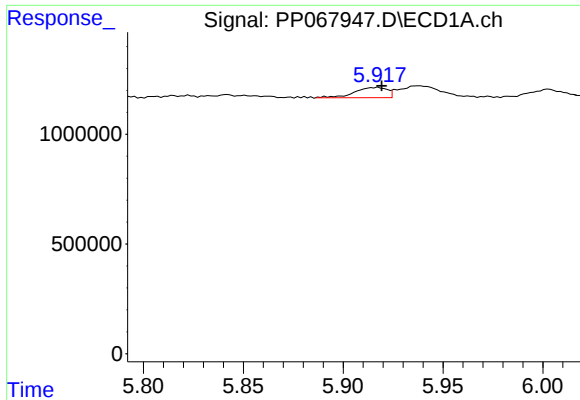

#3 AR-1016-1


R.T.: 5.917 min
Delta R.T.: -0.002 min
Response: 530734
Conc: 16.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

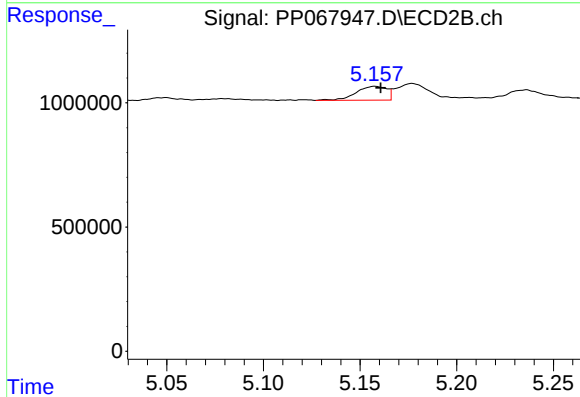


#3 AR-1016-1

R.T.: 5.158 min
Delta R.T.: -0.003 min
Response: 611814
Conc: 17.49 ng/ml

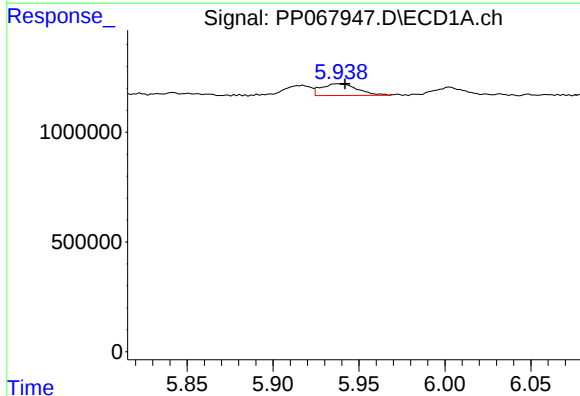


#4 AR-1016-2

R.T.: 5.938 min
Delta R.T.: -0.004 min
Response: 785503
Conc: 16.11 ng/ml

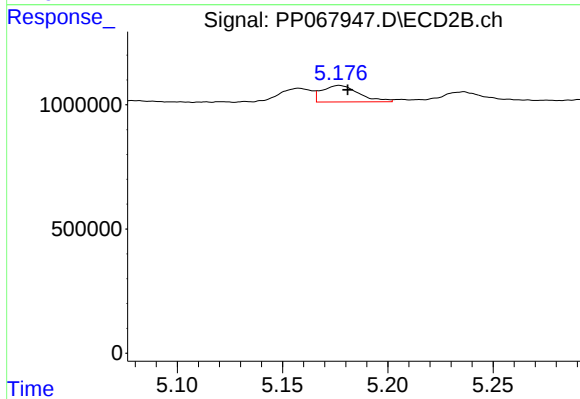

#4 AR-1016-2


R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 804446
Conc: 16.70 ng/ml

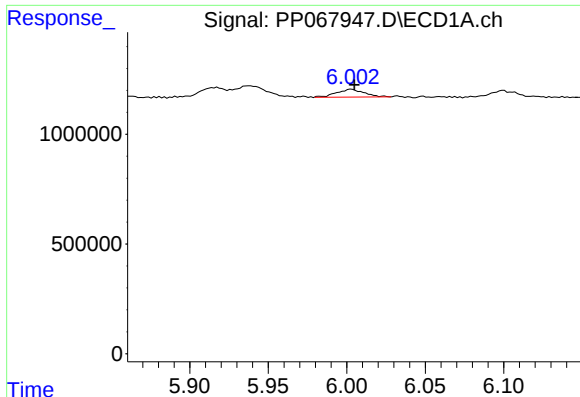

#5 AR-1016-3


R.T.: 6.003 min
Delta R.T.: -0.002 min
Response: 434377
Conc: 13.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

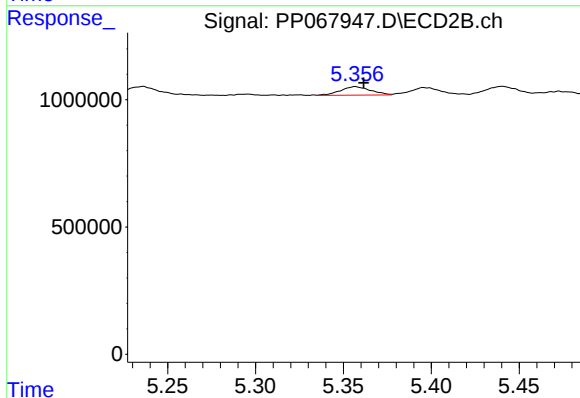


#5 AR-1016-3

R.T.: 5.357 min
Delta R.T.: -0.005 min
Response: 400913
Conc: 14.88 ng/ml

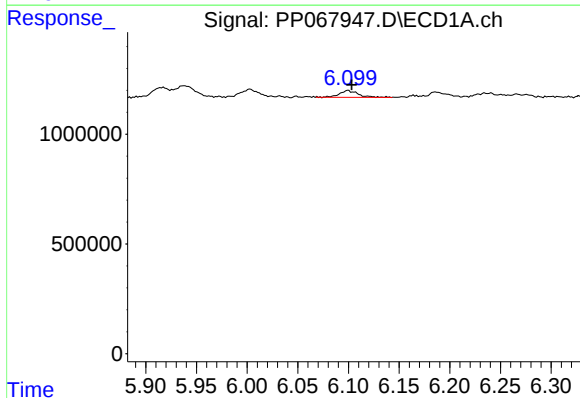


#6 AR-1016-4

R.T.: 6.100 min
Delta R.T.: -0.004 min
Response: 409522
Conc: 15.91 ng/ml

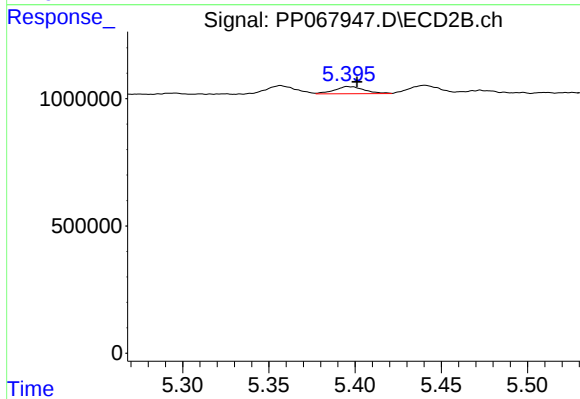

#6 AR-1016-4


R.T.: 5.396 min
Delta R.T.: -0.005 min
Response: 340046
Conc: 14.12 ng/ml

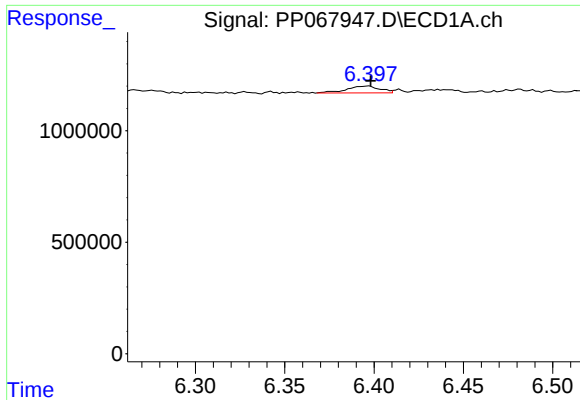

#7 AR-1016-5


R.T.: 6.397 min
Delta R.T.: -0.001 min
Response: 394726
Conc: 14.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

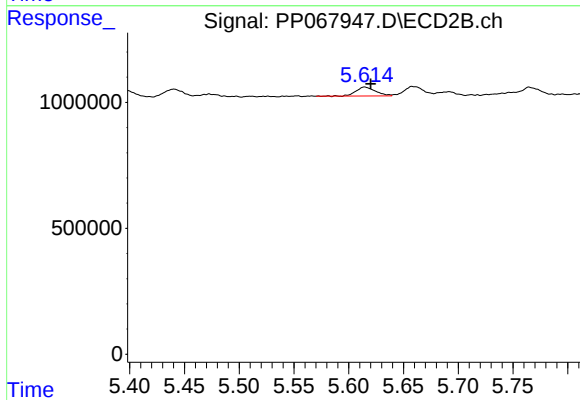


#7 AR-1016-5

R.T.: 5.615 min
Delta R.T.: -0.005 min
Response: 440168
Conc: 14.47 ng/ml

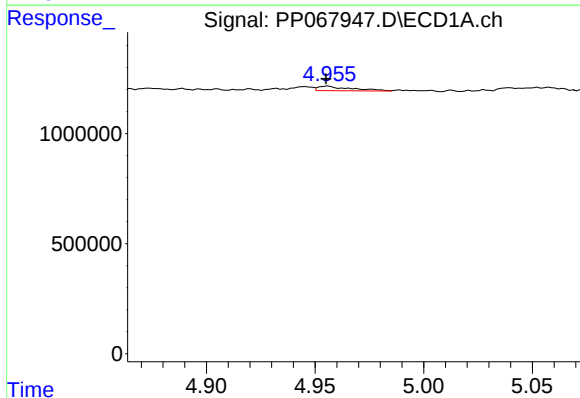


#8 AR-1221-1

R.T.: 4.956 min
Delta R.T.: 0.000 min
Response: 224676
Conc: 17.54 ng/ml

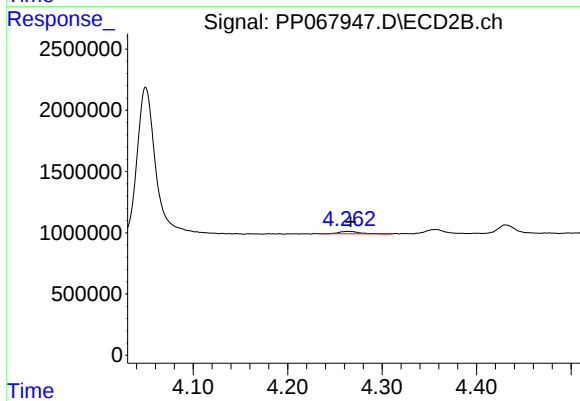

#8 AR-1221-1


R.T.: 4.263 min
Delta R.T.: -0.003 min
Response: 271044
Conc: 20.58 ng/ml

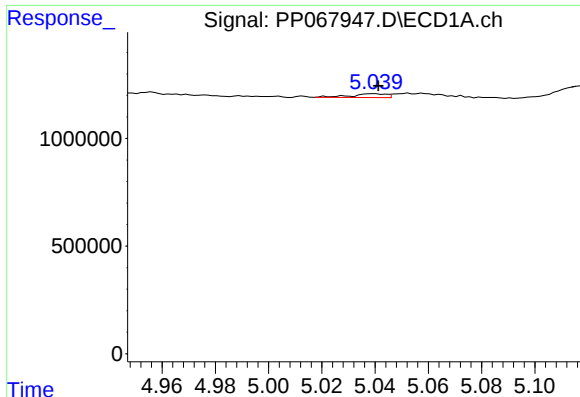

#9 AR-1221-2


R.T.: 5.040 min
Delta R.T.: -0.002 min
Response: 166180
Conc: 17.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

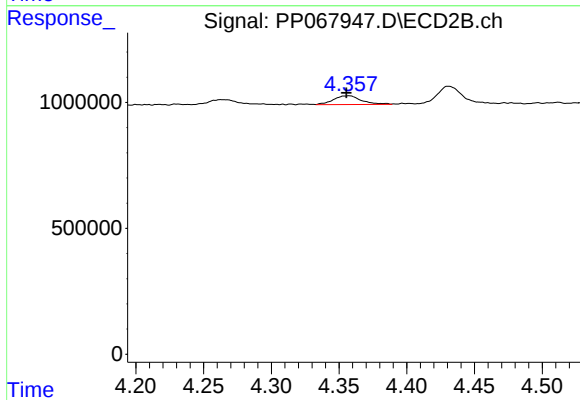


#9 AR-1221-2

R.T.: 4.357 min
Delta R.T.: 0.002 min
Response: 494632
Conc: 49.66 ng/ml

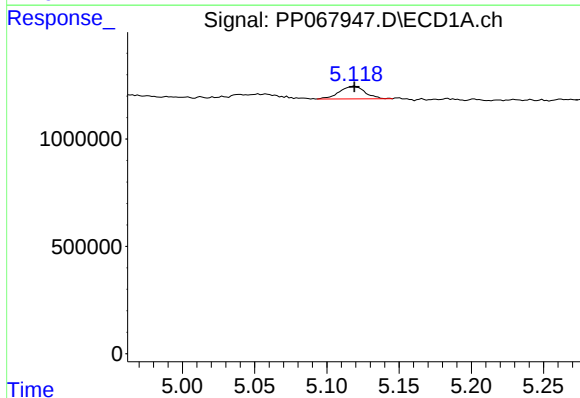


#10 AR-1221-3

R.T.: 5.119 min
Delta R.T.: 0.000 min
Response: 726877
Conc: 25.14 ng/ml

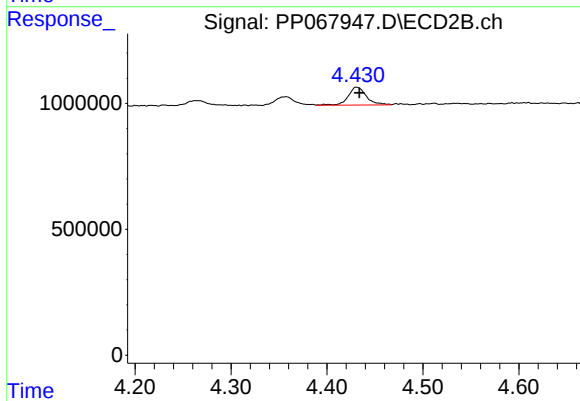

#10 AR-1221-3


R.T.: 4.431 min
Delta R.T.: -0.003 min
Response: 950212
Conc: 30.52 ng/ml

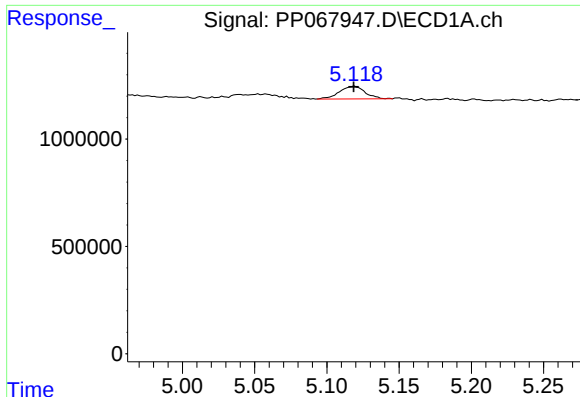

#11 AR-1232-1


R.T.: 5.119 min
Delta R.T.: 0.000 min
Response: 726877
Conc: 31.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

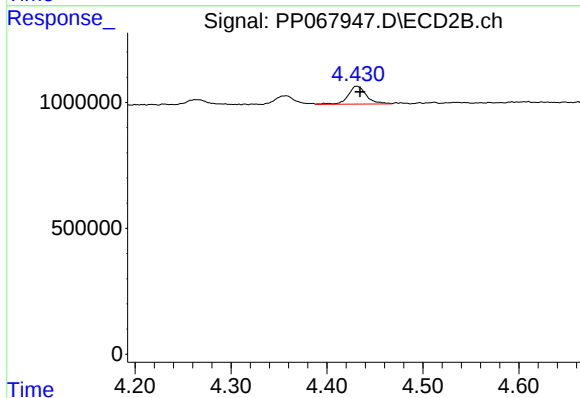


#11 AR-1232-1

R.T.: 4.431 min
Delta R.T.: -0.003 min
Response: 950212
Conc: 39.05 ng/ml

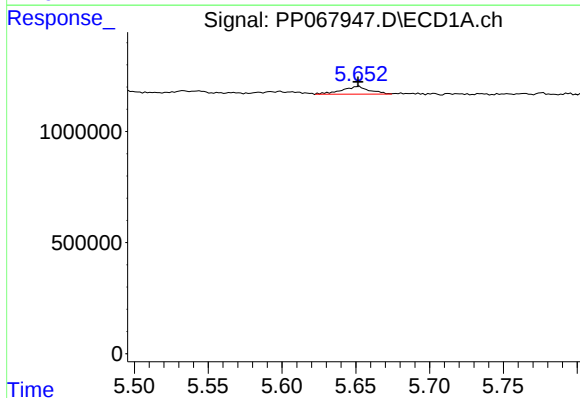


#12 AR-1232-2

R.T.: 5.652 min
Delta R.T.: 0.000 min
Response: 458639
Conc: 38.92 ng/ml

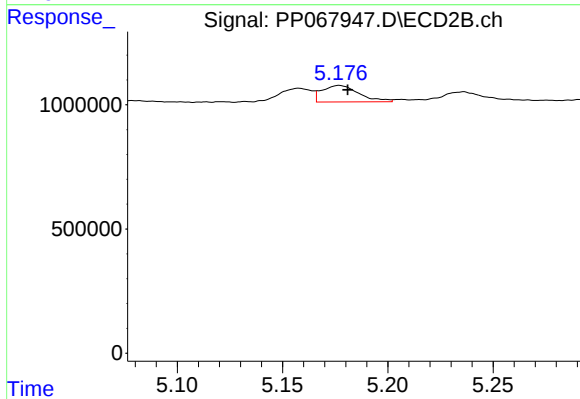

#12 AR-1232-2


R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 804446
Conc: 35.97 ng/ml

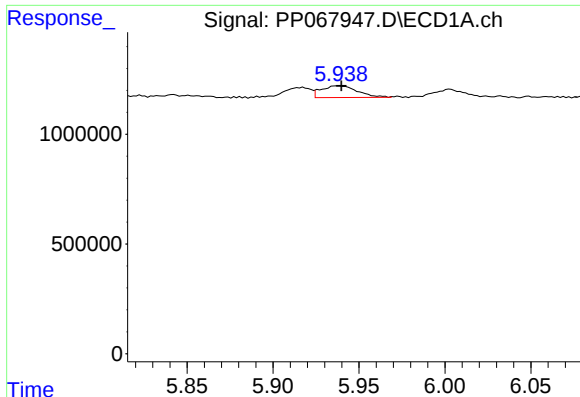

#13 AR-1232-3


R.T.: 5.938 min
Delta R.T.: -0.002 min
Response: 785503
Conc: 35.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

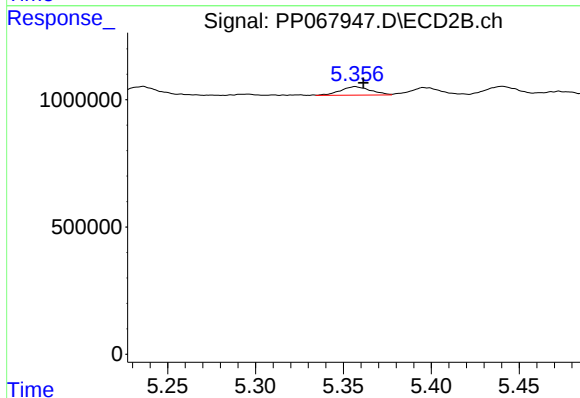


#13 AR-1232-3

R.T.: 5.357 min
Delta R.T.: -0.005 min
Response: 400913
Conc: 33.57 ng/ml

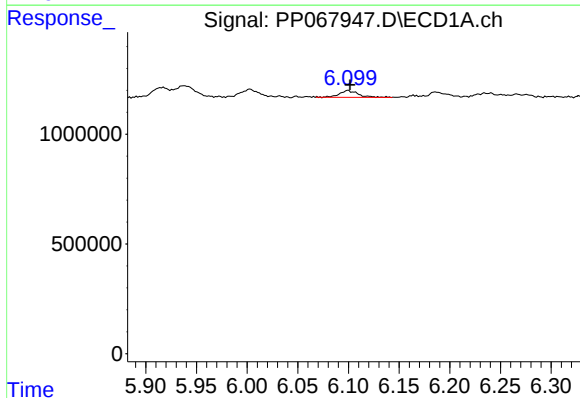


#14 AR-1232-4

R.T.: 6.100 min
Delta R.T.: -0.002 min
Response: 409522
Conc: 36.28 ng/ml

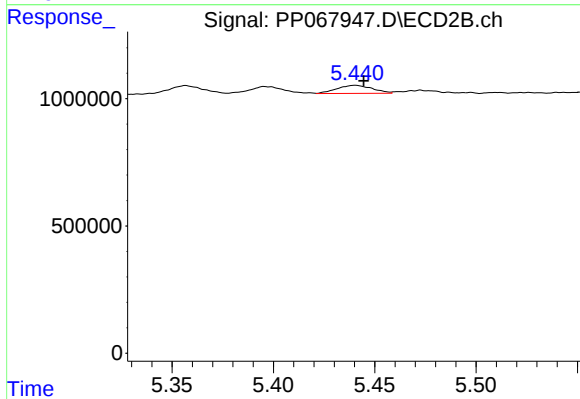

#14 AR-1232-4


R.T.: 5.440 min
Delta R.T.: -0.004 min
Response: 383058
Conc: 33.22 ng/ml

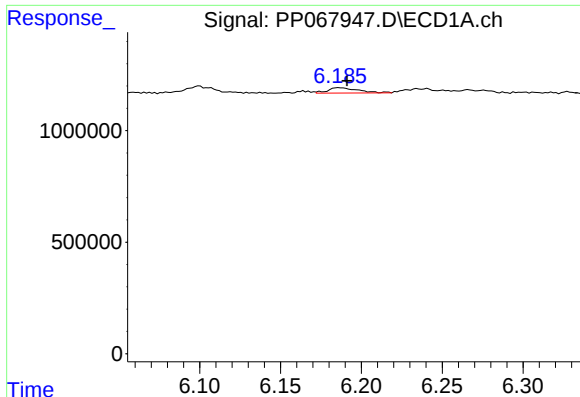

#15 AR-1232-5


R.T.: 6.186 min
Delta R.T.: -0.005 min
Response: 310047
Conc: 34.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

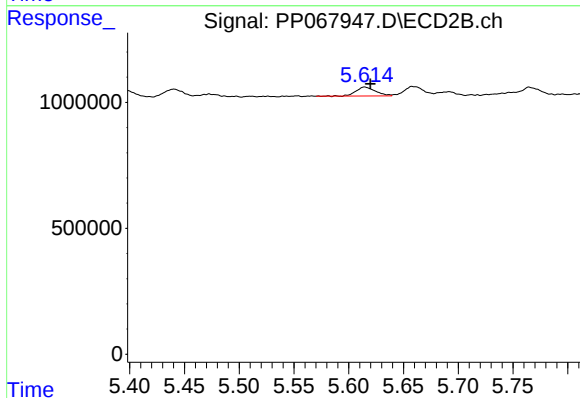


#15 AR-1232-5

R.T.: 5.615 min
Delta R.T.: -0.005 min
Response: 440168
Conc: 32.73 ng/ml

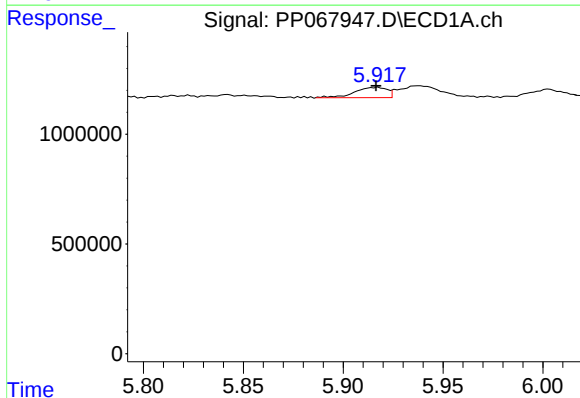


#16 AR-1242-1

R.T.: 5.917 min
Delta R.T.: 0.000 min
Response: 530734
Conc: 19.00 ng/ml

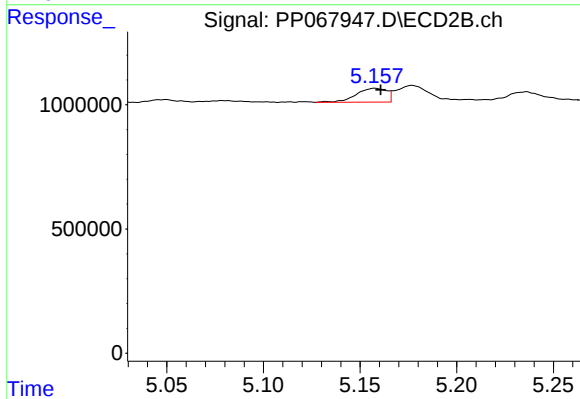

#16 AR-1242-1


R.T.: 5.158 min
Delta R.T.: -0.003 min
Response: 611814
Conc: 21.04 ng/ml

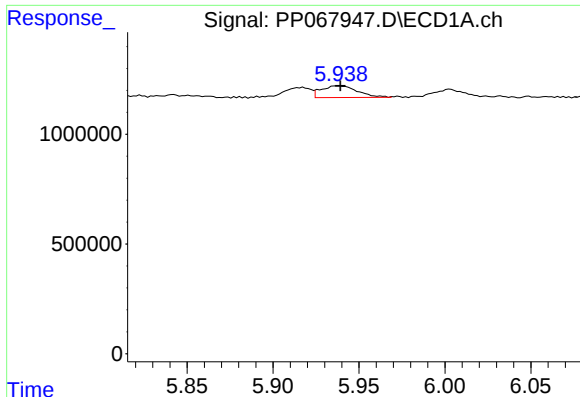

#17 AR-1242-2


R.T.: 5.938 min
Delta R.T.: -0.001 min
Response: 785503
Conc: 19.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

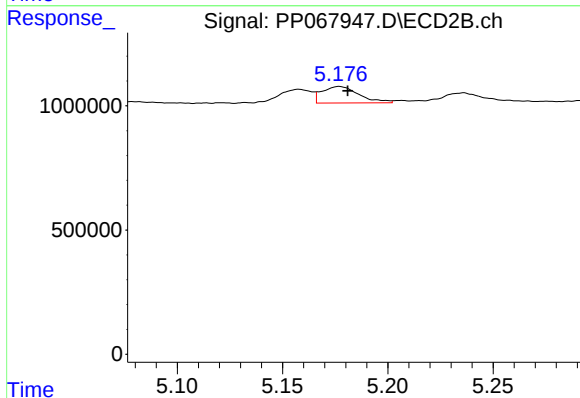


#17 AR-1242-2

R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 804446
Conc: 20.04 ng/ml

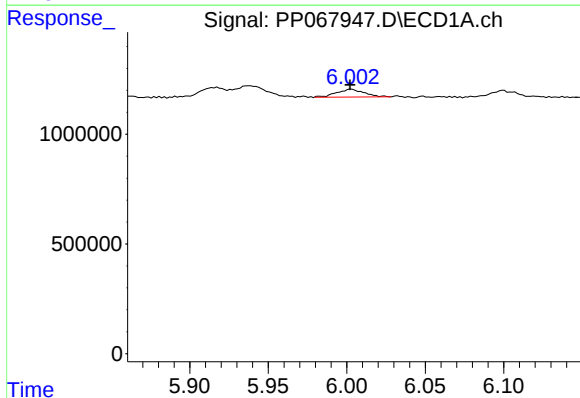


#18 AR-1242-3

R.T.: 6.003 min
Delta R.T.: 0.000 min
Response: 434377
Conc: 16.11 ng/ml

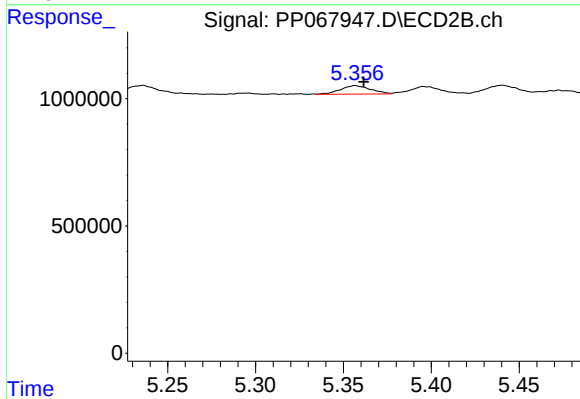

#18 AR-1242-3


R.T.: 5.357 min
Delta R.T.: -0.005 min
Response: 400913
Conc: 17.82 ng/ml

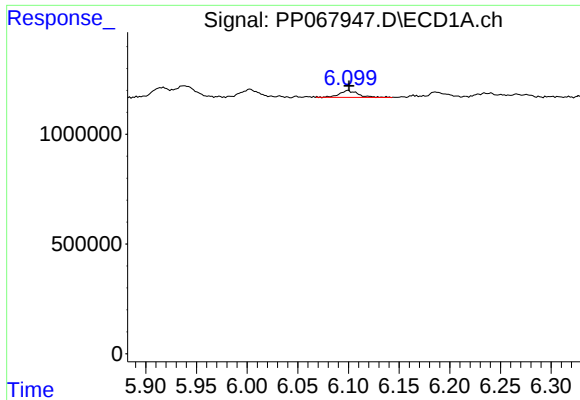

#19 AR-1242-4


R.T.: 6.100 min
Delta R.T.: -0.001 min
Response: 409522
Conc: 19.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

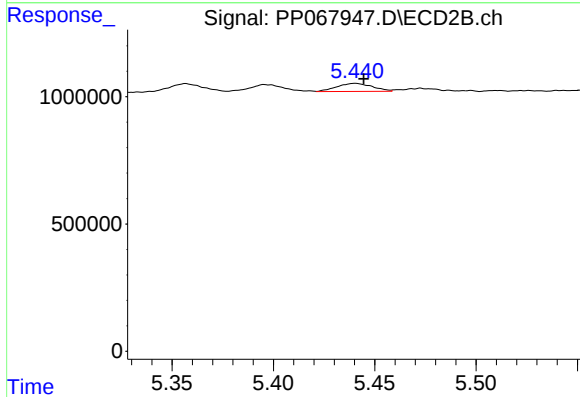


#19 AR-1242-4

R.T.: 5.440 min
Delta R.T.: -0.004 min
Response: 383058
Conc: 16.14 ng/ml

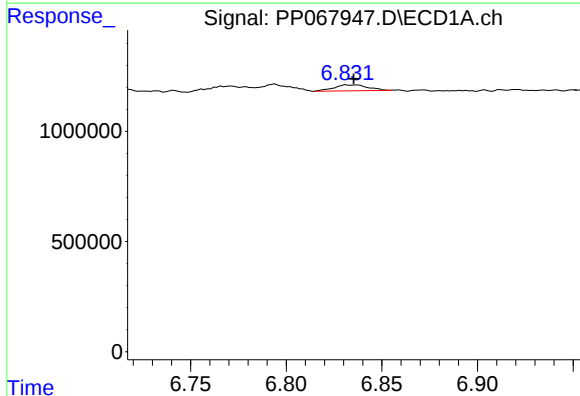


#20 AR-1242-5

R.T.: 6.837 min
Delta R.T.: 0.002 min
Response: 330217
Conc: 13.69 ng/ml

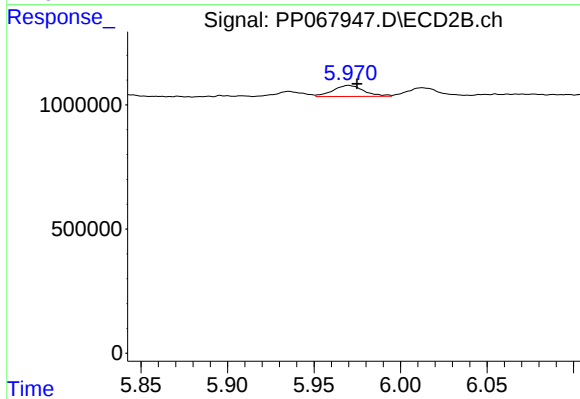

#20 AR-1242-5


R.T.: 5.970 min
Delta R.T.: -0.005 min
Response: 551943
Conc: 19.27 ng/ml

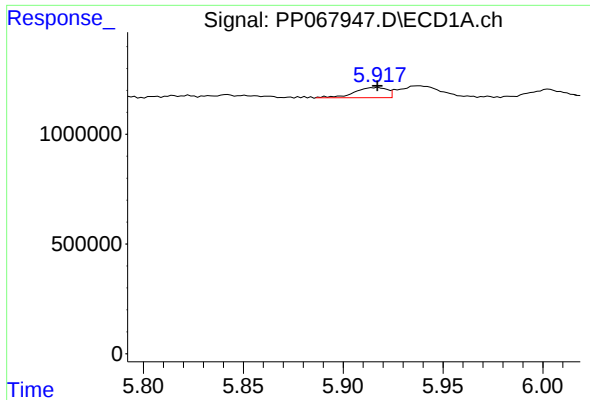

#21 AR-1248-1


R.T.: 5.917 min
Delta R.T.: 0.000 min
Response: 530734
Conc: 24.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

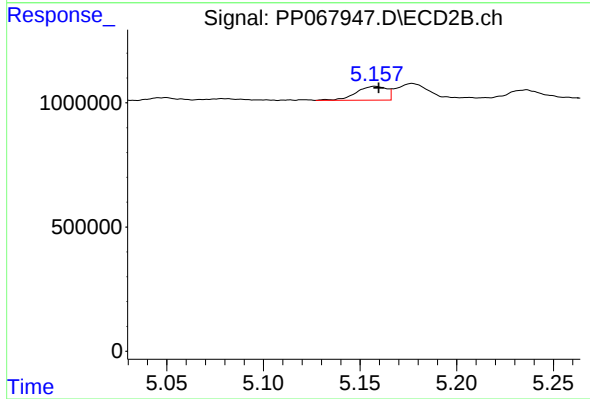


#21 AR-1248-1

R.T.: 5.158 min
Delta R.T.: -0.002 min
Response: 611814
Conc: 27.00 ng/ml

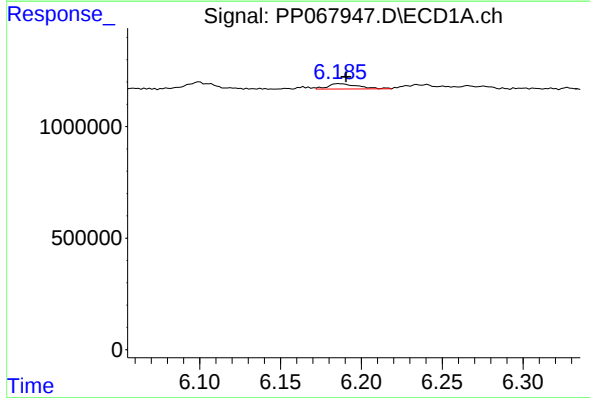


#22 AR-1248-2

R.T.: 6.186 min
Delta R.T.: -0.004 min
Response: 310047
Conc: 9.22 ng/ml

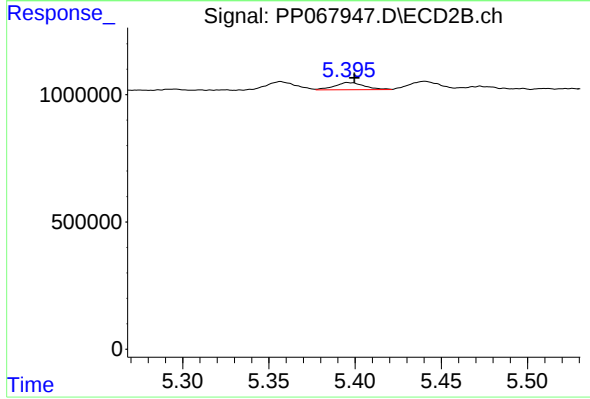

#22 AR-1248-2


R.T.: 5.396 min
Delta R.T.: -0.003 min
Response: 340046
Conc: 10.27 ng/ml

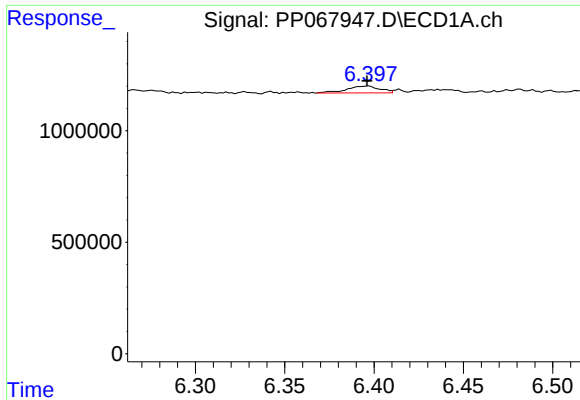

#23 AR-1248-3


R.T.: 6.397 min
Delta R.T.: 0.000 min
Response: 394726
Conc: 10.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

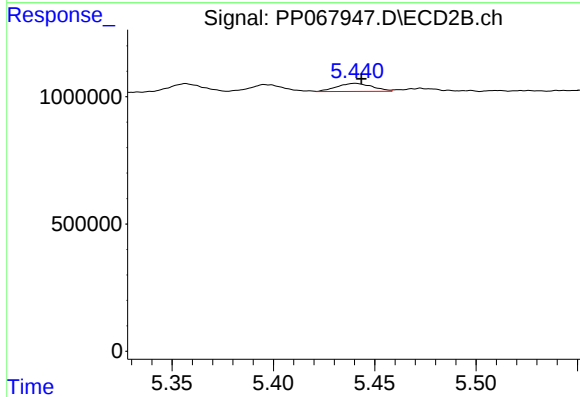


#23 AR-1248-3

R.T.: 5.440 min
Delta R.T.: -0.003 min
Response: 383058
Conc: 11.11 ng/ml

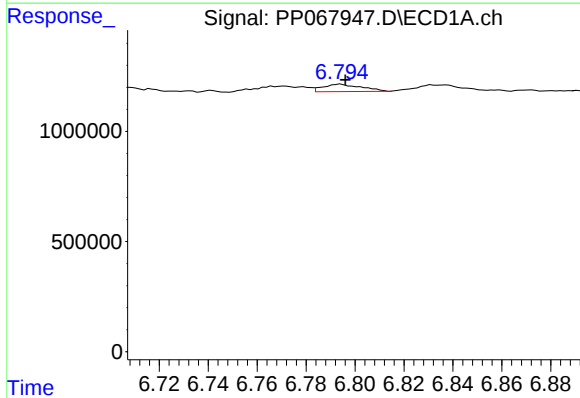


#24 AR-1248-4

R.T.: 6.794 min
Delta R.T.: -0.002 min
Response: 362323
Conc: 8.96 ng/ml

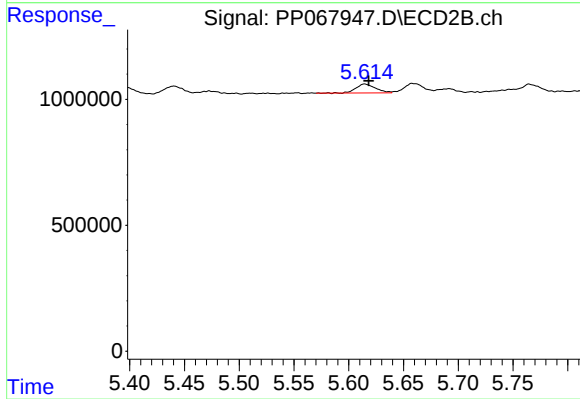

#24 AR-1248-4


R.T.: 5.615 min
Delta R.T.: -0.004 min
Response: 440168
Conc: 10.75 ng/ml

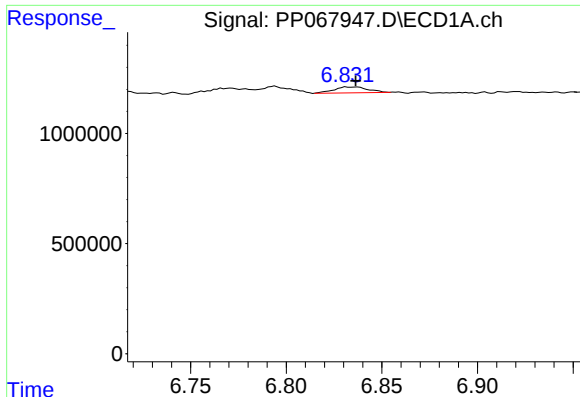

#25 AR-1248-5


R.T.: 6.837 min
Delta R.T.: 0.000 min
Response: 330217
Conc: 8.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

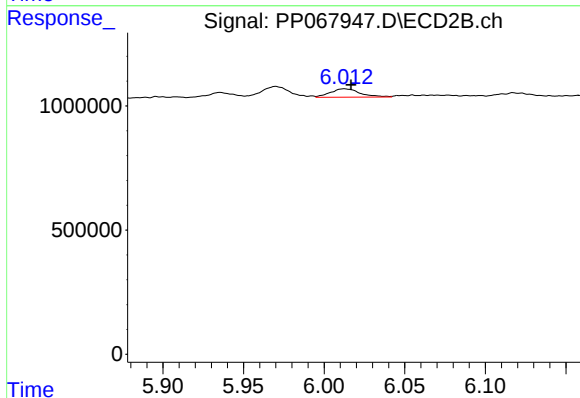


#25 AR-1248-5

R.T.: 6.013 min
Delta R.T.: -0.004 min
Response: 430325
Conc: 11.49 ng/ml

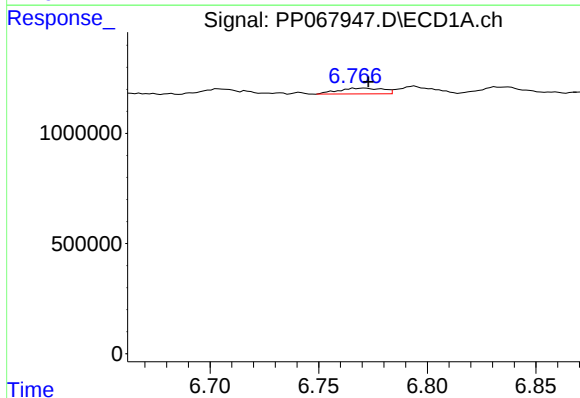


#26 AR-1254-1

R.T.: 6.771 min
Delta R.T.: -0.002 min
Response: 371933
Conc: 8.31 ng/ml

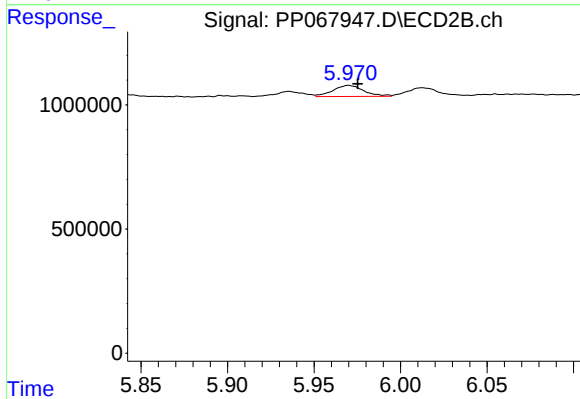

#26 AR-1254-1


R.T.: 5.970 min
Delta R.T.: -0.005 min
Response: 551943
Conc: 9.34 ng/ml

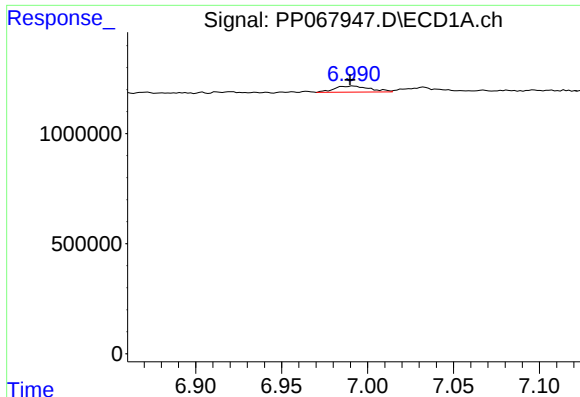

#27 AR-1254-2


R.T.: 6.992 min
Delta R.T.: 0.002 min
Response: 402963
Conc: 6.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

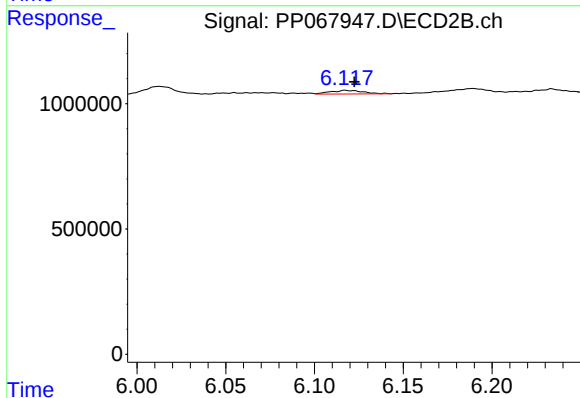


#27 AR-1254-2

R.T.: 6.117 min
Delta R.T.: -0.005 min
Response: 188069
Conc: 3.58 ng/ml

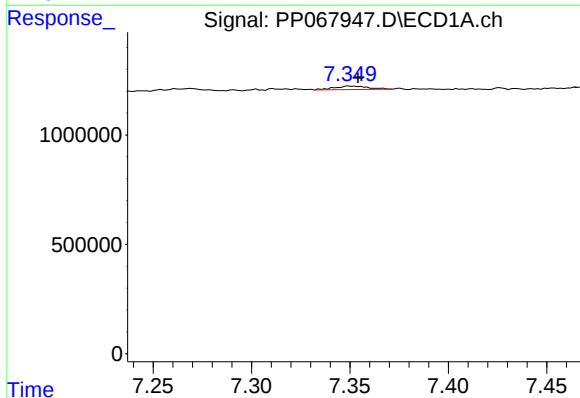


#28 AR-1254-3

R.T.: 7.350 min
Delta R.T.: -0.004 min
Response: 188719
Conc: 2.72 ng/ml

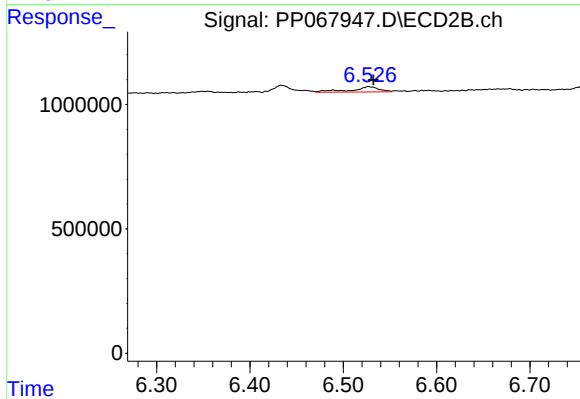

#28 AR-1254-3


R.T.: 6.527 min
Delta R.T.: -0.005 min
Response: 433654
Conc: 5.21 ng/ml

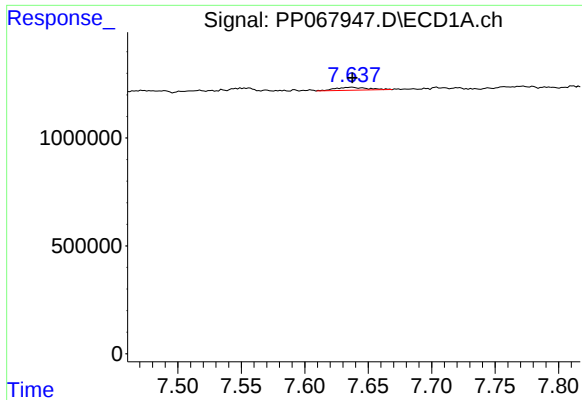

#29 AR-1254-4


R.T.: 7.637 min
Delta R.T.: 0.000 min
Response: 241440
Conc: 4.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

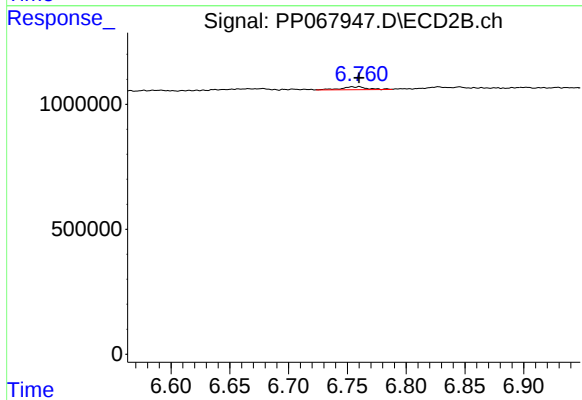


#29 AR-1254-4

R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 179989
Conc: 3.73 ng/ml

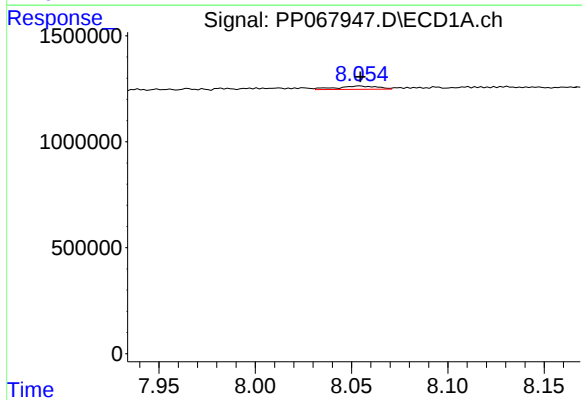


#30 AR-1254-5

R.T.: 8.054 min
Delta R.T.: 0.000 min
Response: 235114
Conc: 3.97 ng/ml

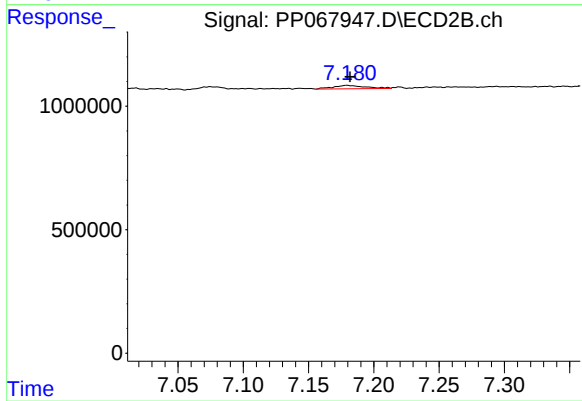

#30 AR-1254-5


R.T.: 7.180 min
Delta R.T.: -0.002 min
Response: 234330
Conc: 3.19 ng/ml

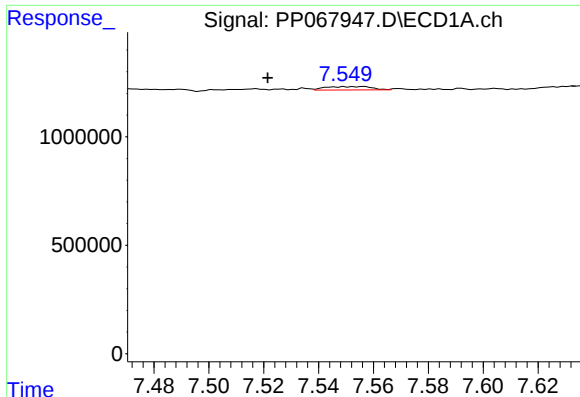

#31 AR-1260-1


R.T.: 7.556 min
Delta R.T.: 0.035 min
Response: 185290
Conc: 3.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

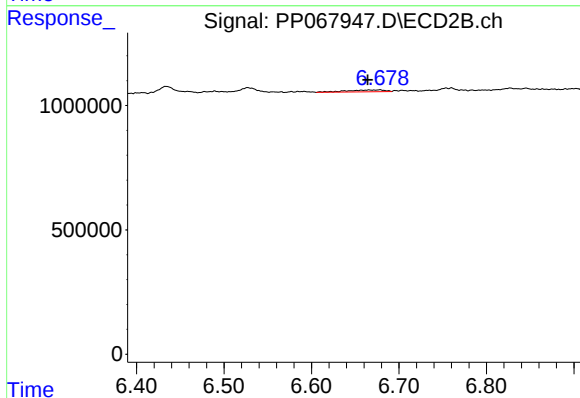


#31 AR-1260-1

R.T.: 6.678 min
Delta R.T.: 0.014 min
Response: 227235
Conc: 3.99 ng/ml

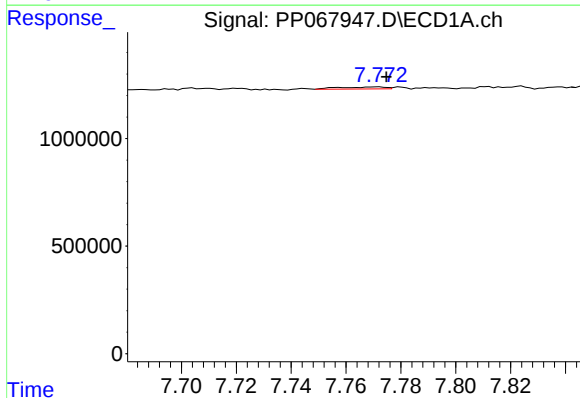


#32 AR-1260-2

R.T.: 7.772 min
Delta R.T.: -0.003 min
Response: 113275
Conc: 1.79 ng/ml

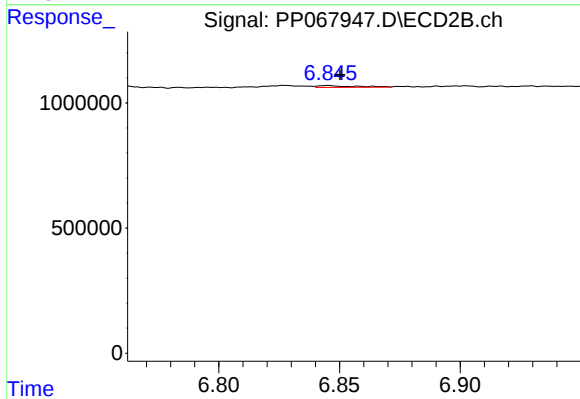

#32 AR-1260-2


R.T.: 6.845 min
Delta R.T.: -0.005 min
Response: 79119
Conc: 1.19 ng/ml

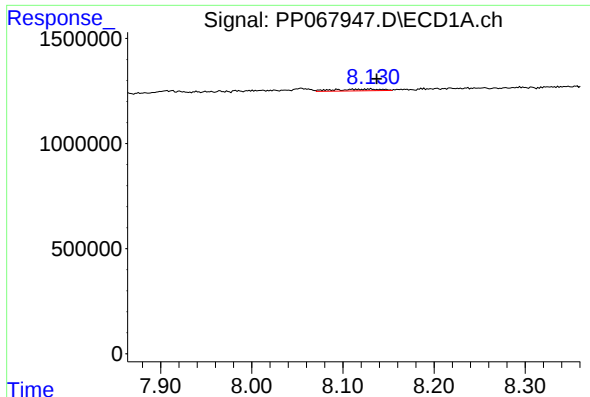

#33 AR-1260-3


R.T.: 8.130 min
Delta R.T.: -0.007 min
Response: 289770
Conc: 5.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

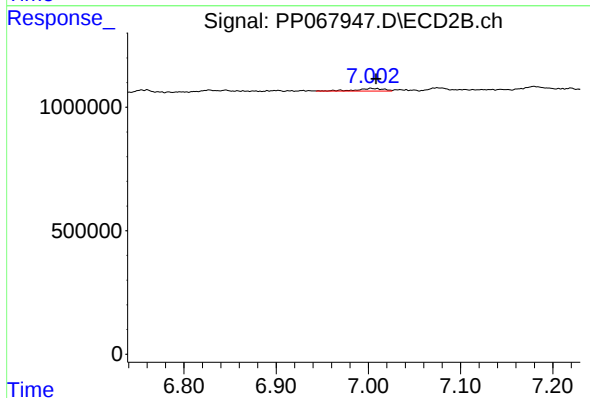


#33 AR-1260-3

R.T.: 7.009 min
Delta R.T.: 0.001 min
Response: 213281
Conc: 3.35 ng/ml

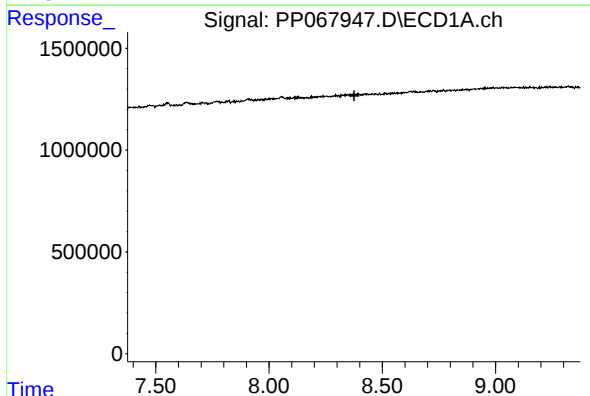


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

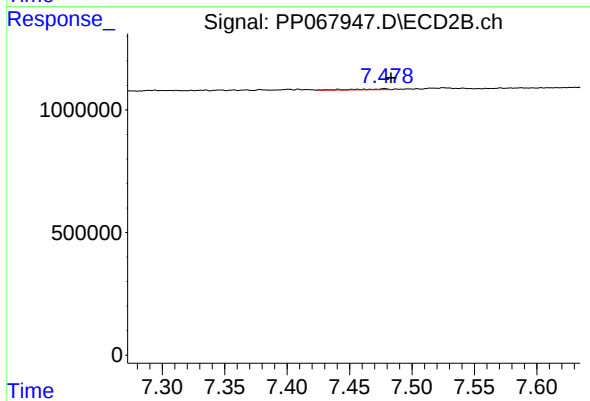

#34 AR-1260-4


R.T.: 7.478 min
Delta R.T.: -0.005 min
Response: 63887
Conc: 1.16 ng/ml

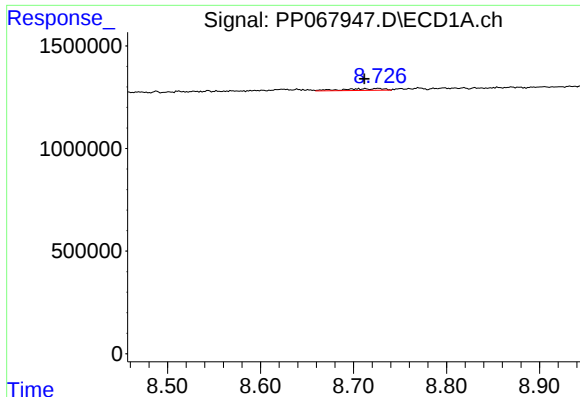

#35 AR-1260-5


R.T.: 8.726 min
Delta R.T.: 0.014 min
Response: 277069
Conc: 2.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

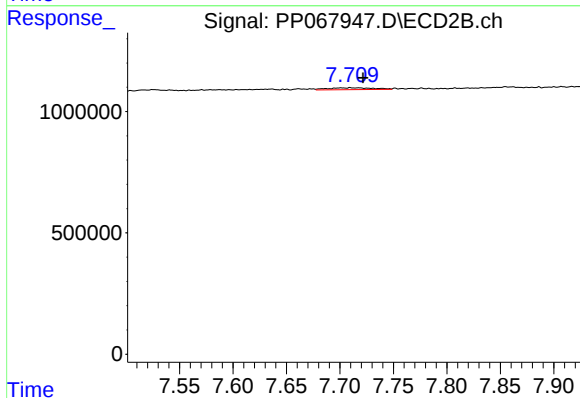


#35 AR-1260-5

R.T.: 7.710 min
Delta R.T.: -0.012 min
Response: 223450
Conc: 1.83 ng/ml

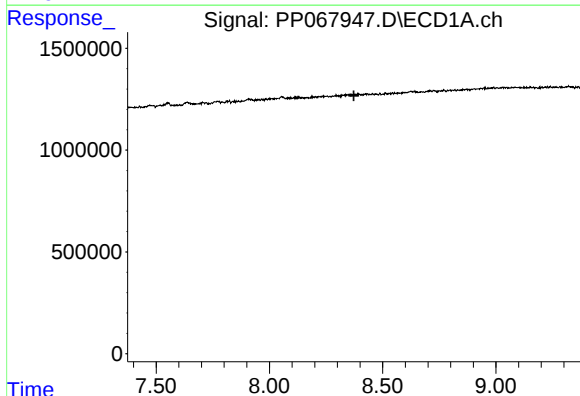


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 8.373 min
Response: 0
Conc: N.D.

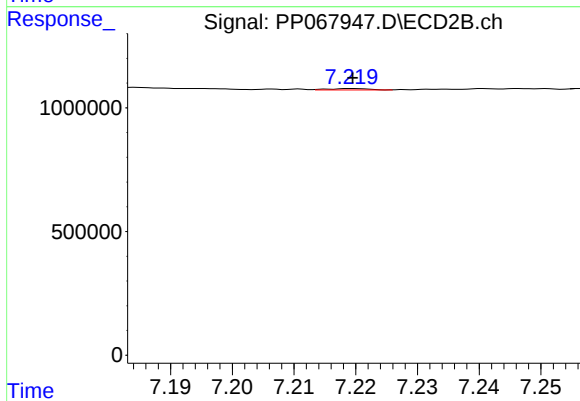

#36 AR-1262-1


R.T.: 7.220 min
Delta R.T.: 0.000 min
Response: 25024
Conc: 0.32 ng/ml

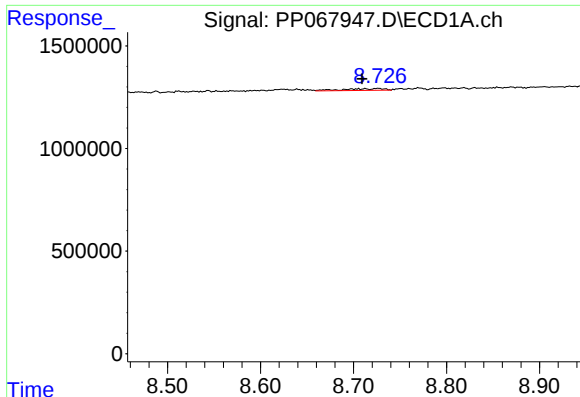

#37 AR-1262-2


R.T.: 8.726 min
Delta R.T.: 0.017 min
Response: 277069
Conc: 2.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

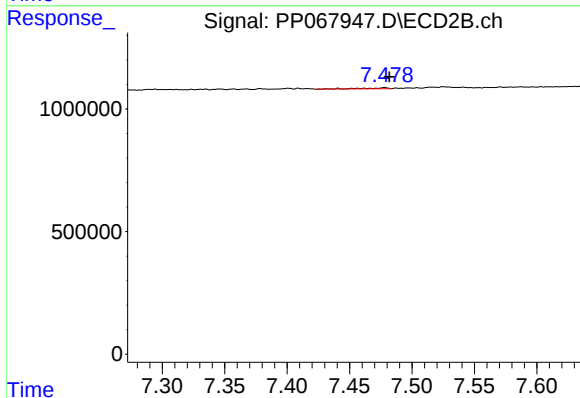


#37 AR-1262-2

R.T.: 7.478 min
Delta R.T.: -0.004 min
Response: 63887
Conc: 0.90 ng/ml

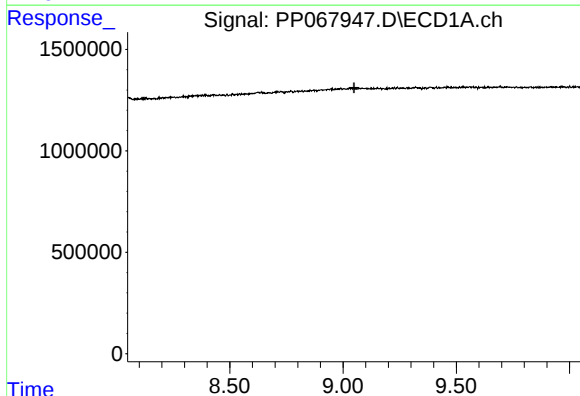


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.048 min
Response: 0
Conc: N.D.

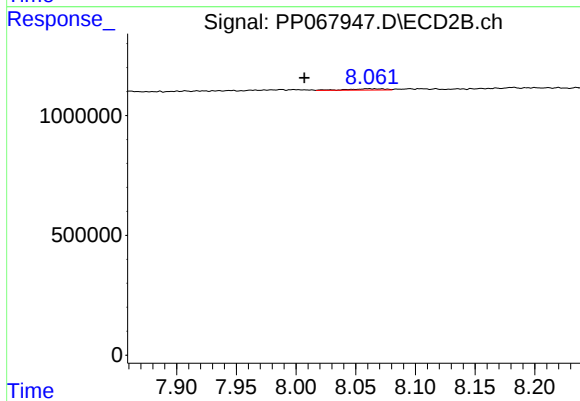

#38 AR-1262-3


R.T.: 8.060 min
Delta R.T.: 0.053 min
Response: 112603
Conc: 1.97 ng/ml

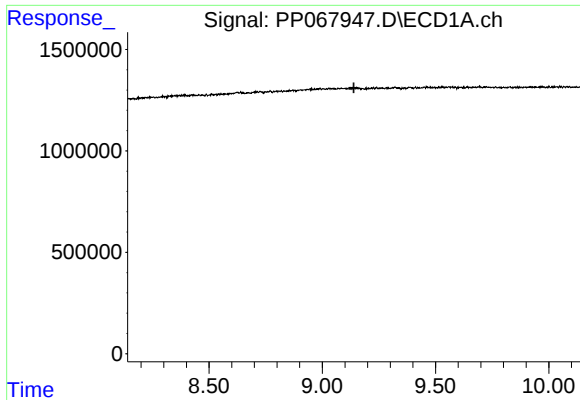

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 9.140 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

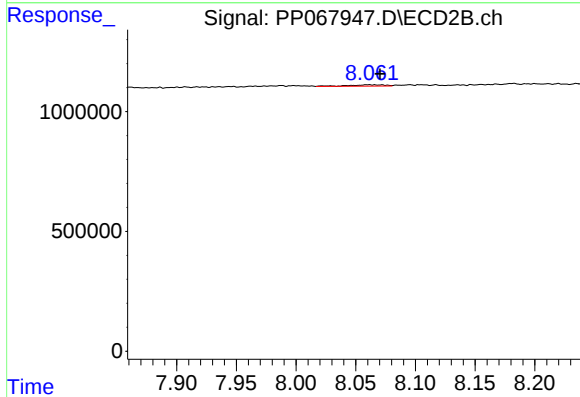


#39 AR-1262-4

R.T.: 8.060 min
Delta R.T.: -0.010 min
Response: 112603
Conc: 1.12 ng/ml

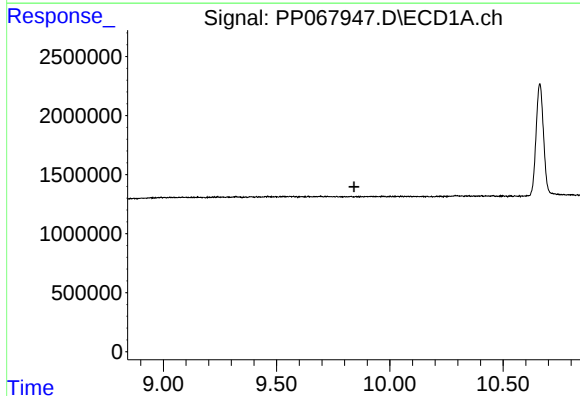


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.842 min
Response: 0
Conc: N.D.

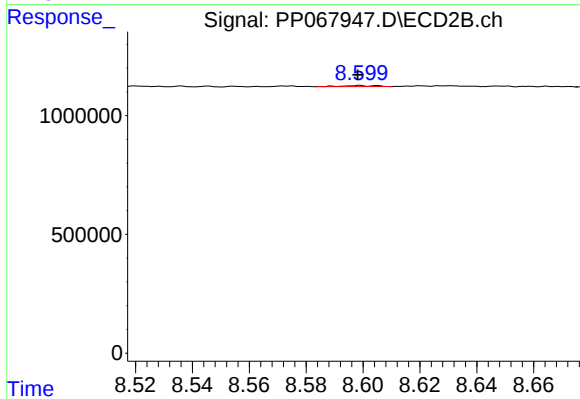

#40 AR-1262-5


R.T.: 8.599 min
Delta R.T.: 0.000 min
Response: 39209
Conc: 0.78 ng/ml

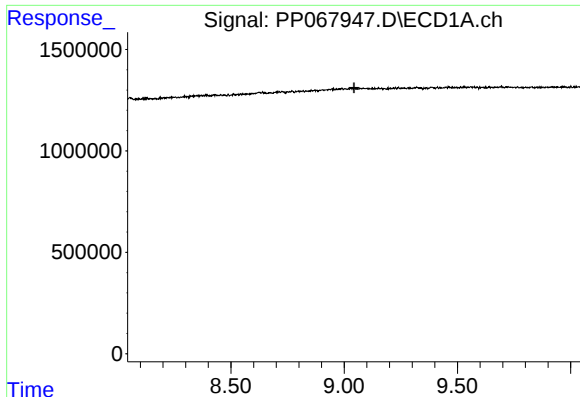

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 9.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

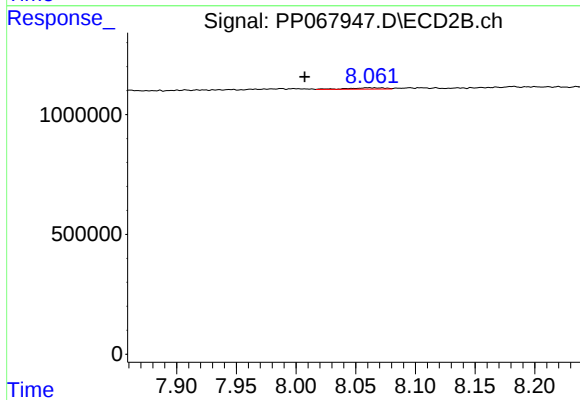


#41 AR-1268-1

R.T.: 8.060 min
Delta R.T.: 0.053 min
Response: 112603
Conc: 0.71 ng/ml

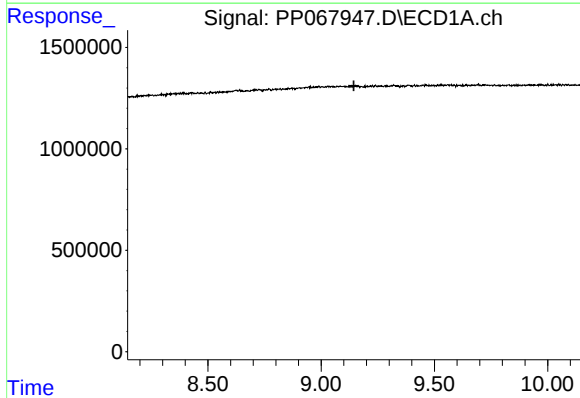


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 9.144 min
Response: 0
Conc: N.D.

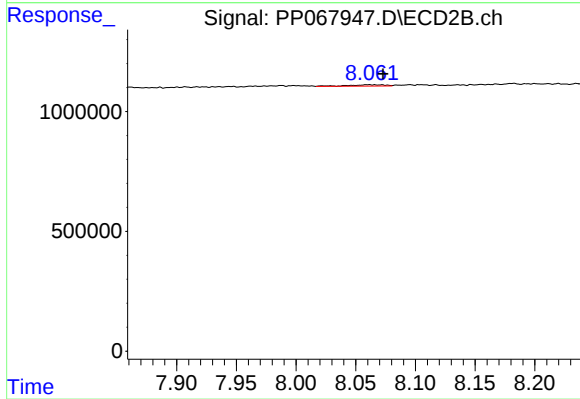

#42 AR-1268-2


R.T.: 8.060 min
Delta R.T.: -0.012 min
Response: 112603
Conc: 0.79 ng/ml

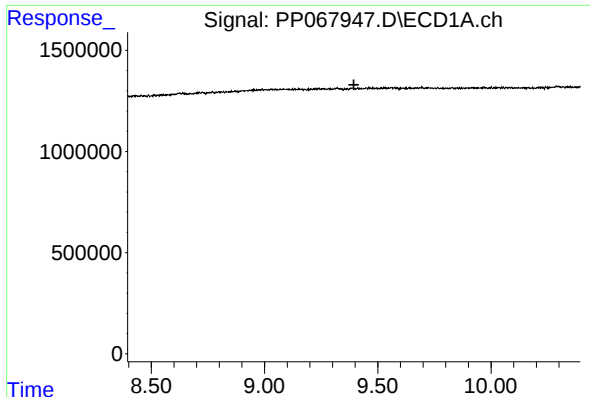

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

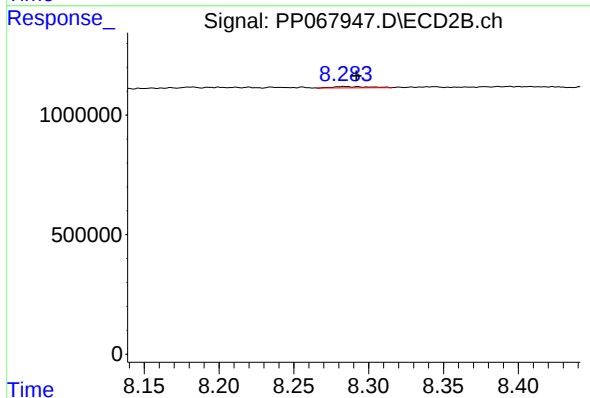


#43 AR-1268-3

R.T.: 8.284 min
Delta R.T.: -0.008 min
Response: 90315
Conc: 0.71 ng/ml

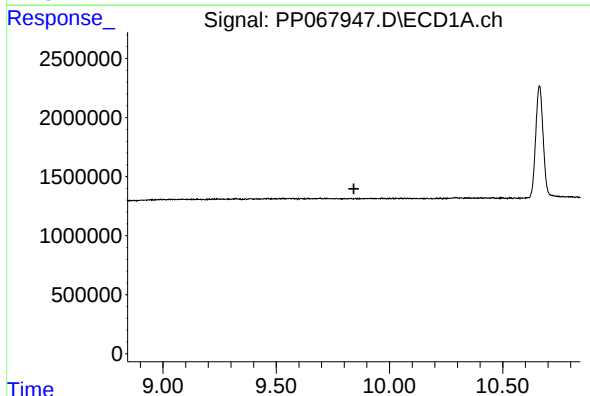


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.843 min
Response: 0
Conc: N.D.

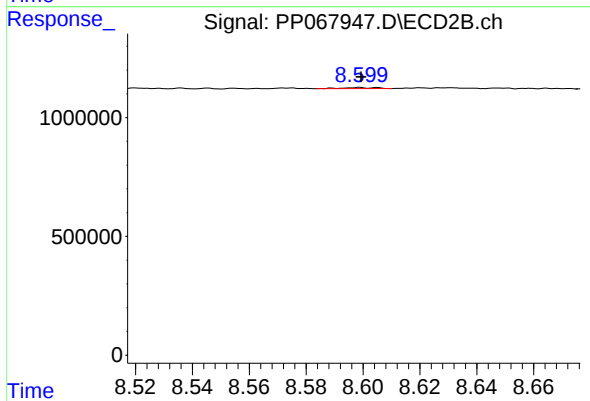

#44 AR-1268-4


R.T.: 8.599 min
Delta R.T.: 0.000 min
Response: 39209
Conc: 0.69 ng/ml

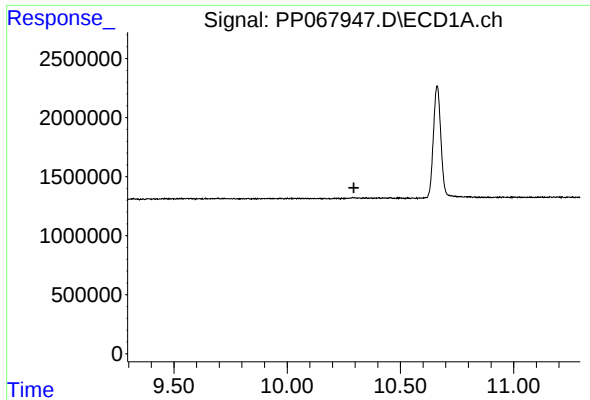

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.294 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

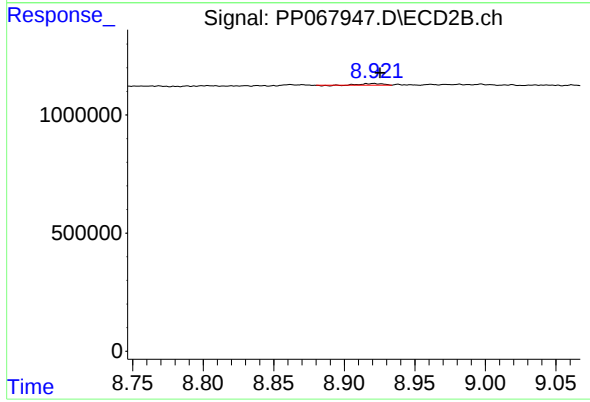

#45 AR-1268-5

R.T.: 8.921 min
Delta R.T.: -0.004 min
Response: 61770
Conc: 0.16 ng/ml