

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
 Data File : PP067948.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2024 01:02
 Operator : YP\AJ
 Sample : P4368-07
 Misc : AR1242 LOD 40 PPB
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 07:29:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.752	4.050	16357778	17404648	17.672	17.225
2)	SA Decachlor...	10.662	9.211	23279937	21208731	20.220	18.912
Target Compounds							
3)	L1 AR-1016-1	5.916	5.157	1093826	985653	33.079	28.172
4)	L1 AR-1016-2	5.938	5.177	1491487	1252294	30.582	25.998
5)	L1 AR-1016-3	6.001	5.357	951205	822719	30.186	30.542
6)	L1 AR-1016-4	6.100	5.398	803761	745791	31.222	30.965
7)	L1 AR-1016-5	6.394	5.616	932897	913633	34.466	30.044
8)	L2 AR-1221-1	0.000	4.263	0	128128	N.D.	9.729 #
9)	L2 AR-1221-2	5.055	4.357	449652	448580	47.529	45.033
10)	L2 AR-1221-3	5.118	4.431	733092	705887	25.360	22.675
11)	L3 AR-1232-1	5.118	4.431	733092	705887	32.069	29.009
12)	L3 AR-1232-2	5.651	5.177	884617	1252294	75.075	55.993 #
13)	L3 AR-1232-3	5.938	5.357	1491487	822719	66.958	68.882
14)	L3 AR-1232-4	6.100	5.441	803761	917565	71.209	79.571
15)	L3 AR-1232-5	6.191	5.616	718911	913633	78.826	67.927
16)	L4 AR-1242-1	5.916	5.157	1093826	985653	39.153	33.899
17)	L4 AR-1242-2	5.938	5.177	1491487	1252294	36.705	31.192
18)	L4 AR-1242-3	6.001	5.357	951205	822719	35.276	36.573
19)	L4 AR-1242-4	6.100	5.441	803761	917565	37.471	38.654
20)	L4 AR-1242-5	6.834	5.970	957085	1082330	39.670	37.778
21)	L5 AR-1248-1	5.916	5.157	1093826	985653	51.059	43.490
22)	L5 AR-1248-2	6.191	5.398	718911	745791	21.386	22.534
23)	L5 AR-1248-3	6.394	5.441	932897	917565	25.471	26.616
24)	L5 AR-1248-4	6.792	5.616	904771	913633	22.367	22.308
25)	L5 AR-1248-5	6.834	6.013	957085	874108	24.132	23.345
26)	L6 AR-1254-1	6.769	5.970	692831	1082330	15.471	18.319
27)	L6 AR-1254-2	6.992	6.120	974639	331847	14.745	6.325 #
28)	L6 AR-1254-3	7.352	6.528	494561	441388	7.121	5.305 #
29)	L6 AR-1254-4	7.640	6.757	377755	305371	7.570	6.326
30)	L6 AR-1254-5	8.054	7.179	570188	235927	9.616	3.208 #
31)	L7 AR-1260-1	7.550	6.676	317251	344622	5.872	6.050
32)	L7 AR-1260-2	7.767	6.847	205933	40290	3.255	0.604 #
33)	L7 AR-1260-3	8.113	7.002	220951	66566	4.261	1.045 #
34)	L7 AR-1260-4	0.000	7.520f	0	133465	N.D.	2.414 #
35)	L7 AR-1260-5	8.707	7.720	131201	45439	1.218	0.372 #
36)	L8 AR-1262-1	0.000	7.225	0	29775	N.D.	0.378 #
37)	L8 AR-1262-2	8.707	7.520f	131201	133465	1.079	1.881 #
38)	L8 AR-1262-3	0.000	8.044f	0	43143	N.D.	0.756 #
39)	L8 AR-1262-4	0.000	8.068	0	58186	N.D.	0.579 #
41)	L9 AR-1268-1	0.000	8.044f	0	43143	N.D.	0.271 #
42)	L9 AR-1268-2	0.000	8.068	0	58186	N.D.	0.406 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
Data File : PP067948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 01:02
Operator : YP\AJ
Sample : P4368-07
Misc : AR1242 LOD 40 PPB
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:29:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	8.291	0	118800	N.D.	0.932 #
45) L9	AR-1268-5	0.000	8.921	0	95529	N.D.	0.253 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
Data File : PP067948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 01:02
Operator : YP\AJ
Sample : P4368-07
Misc : AR1242 LOD 40 PPB
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:29:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

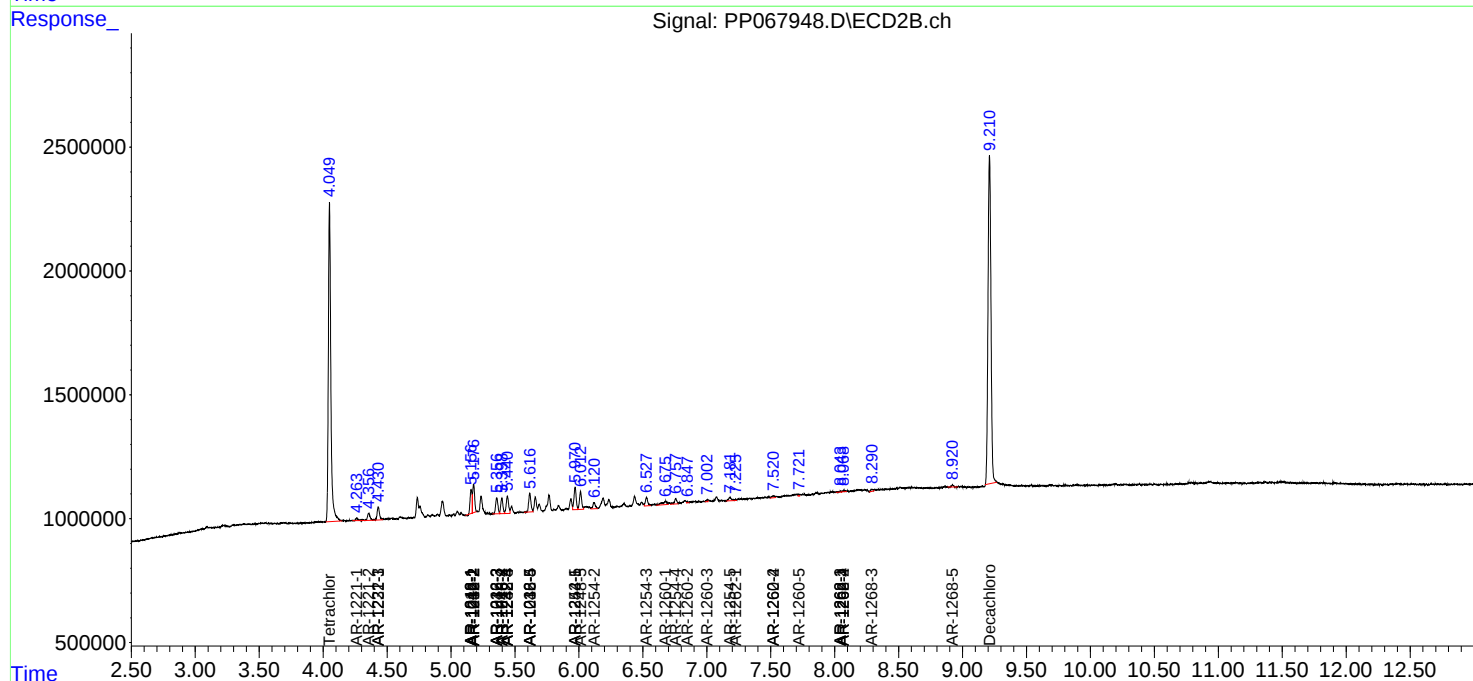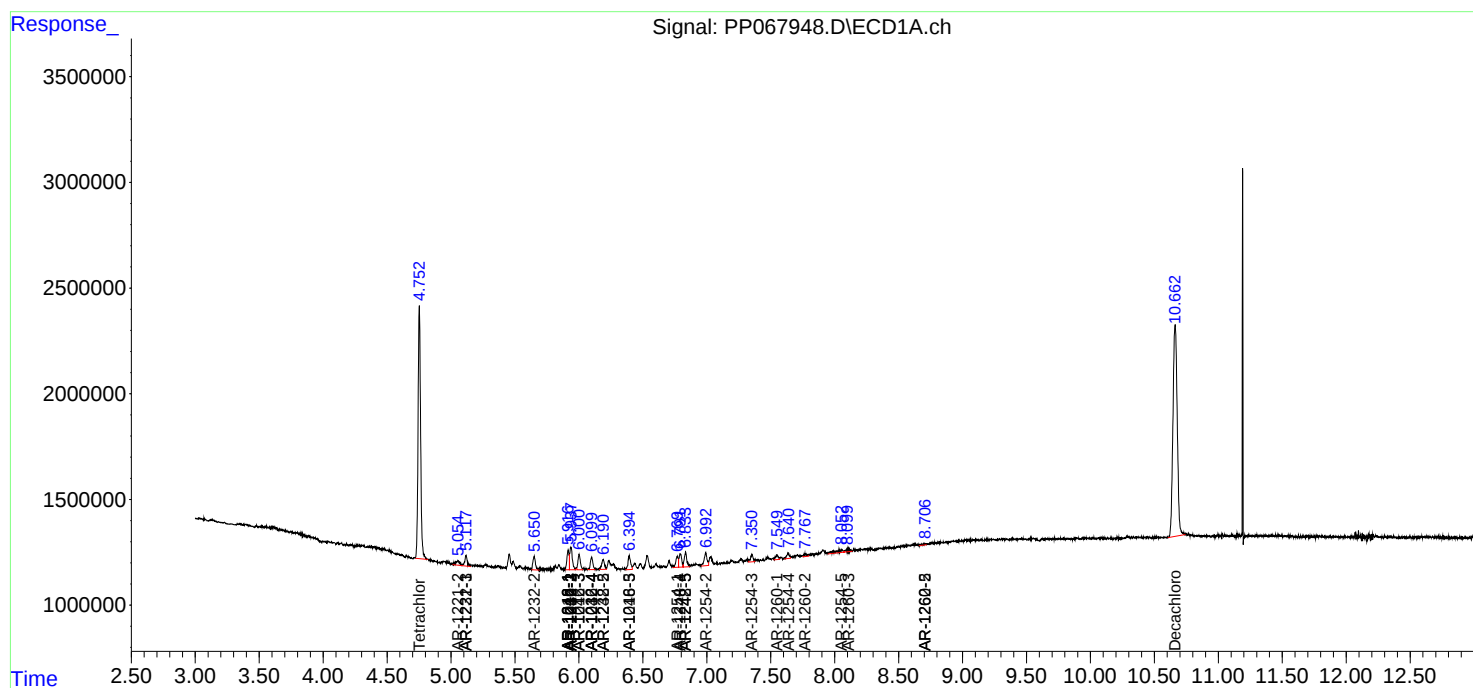


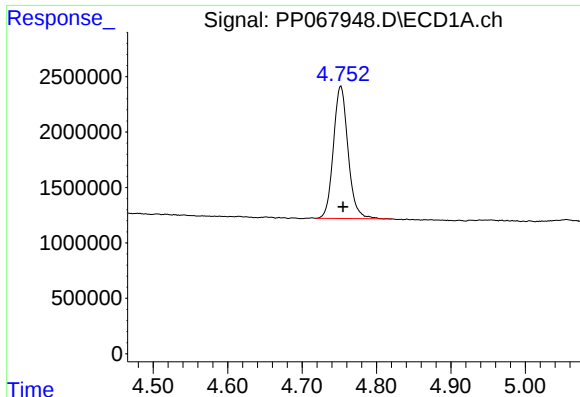

#1 Tetrachloro-m-xylene


R.T.: 4.752 min
Delta R.T.: -0.003 min
Response: 16357778
Conc: 17.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

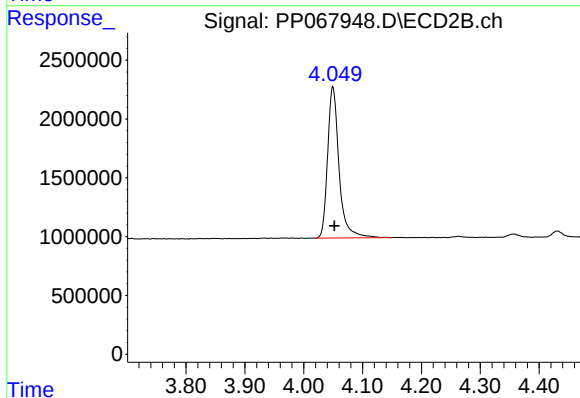


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 17404648
Conc: 17.23 ng/ml

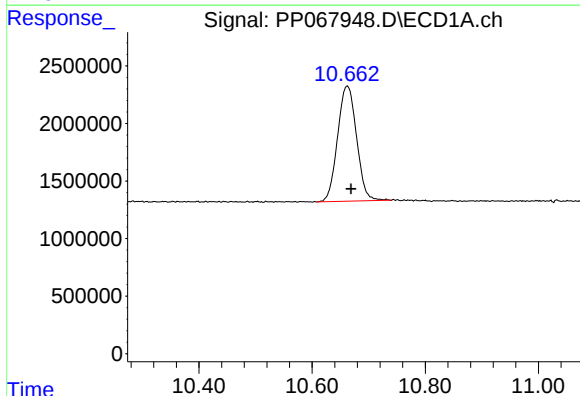


#2 Decachlorobiphenyl

R.T.: 10.662 min
Delta R.T.: -0.007 min
Response: 23279937
Conc: 20.22 ng/ml

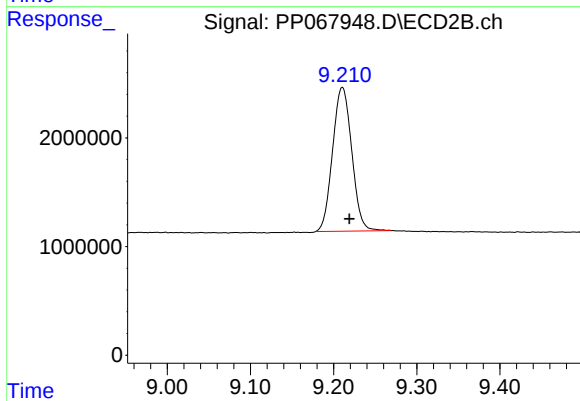

#2 Decachlorobiphenyl


R.T.: 9.211 min
Delta R.T.: -0.008 min
Response: 21208731
Conc: 18.91 ng/ml

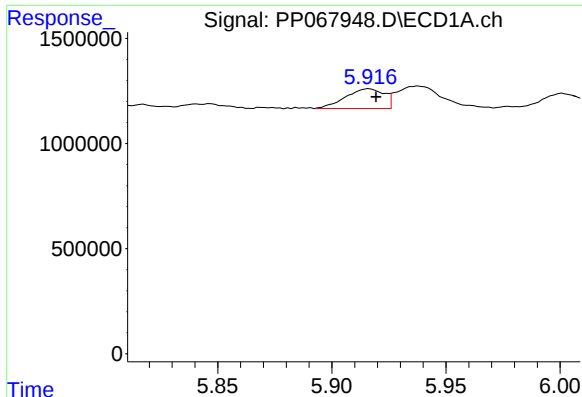

#3 AR-1016-1


R.T.: 5.916 min
Delta R.T.: -0.003 min
Response: 1093826
Conc: 33.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

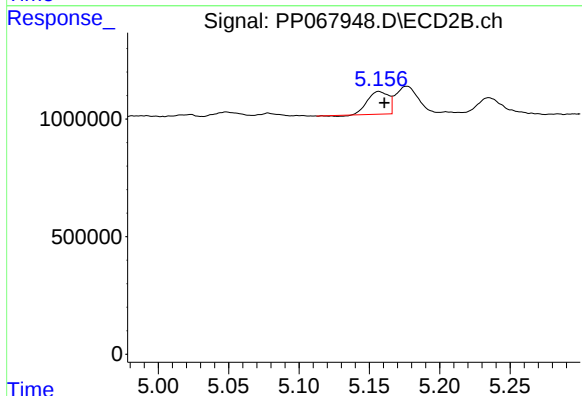


#3 AR-1016-1

R.T.: 5.157 min
Delta R.T.: -0.004 min
Response: 985653
Conc: 28.17 ng/ml

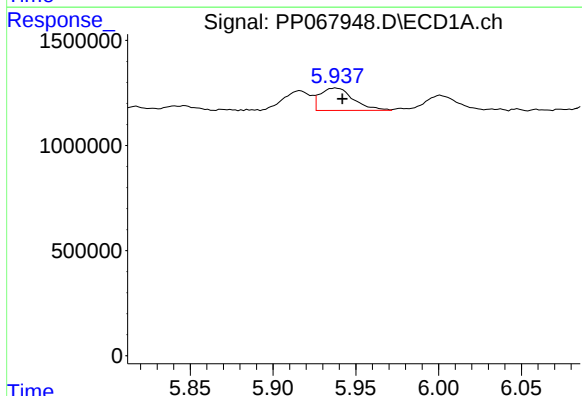


#4 AR-1016-2

R.T.: 5.938 min
Delta R.T.: -0.004 min
Response: 1491487
Conc: 30.58 ng/ml

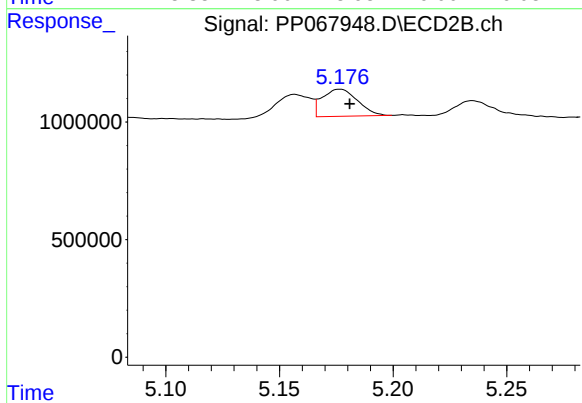

#4 AR-1016-2


R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 1252294
Conc: 26.00 ng/ml

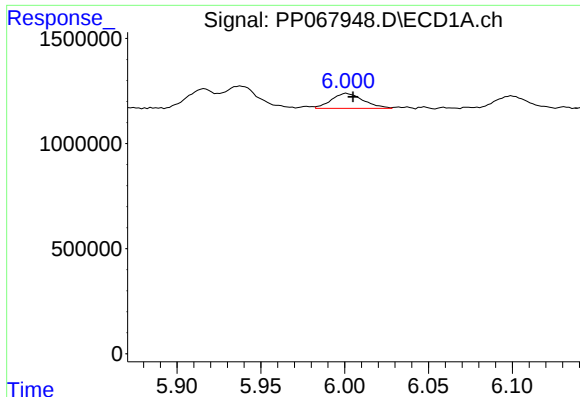

#5 AR-1016-3


R.T.: 6.001 min
Delta R.T.: -0.004 min
Response: 951205
Conc: 30.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

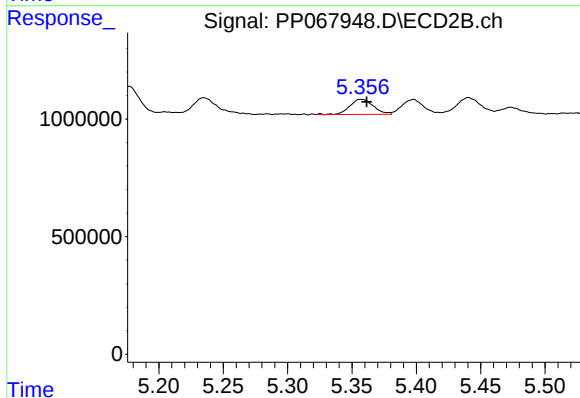


#5 AR-1016-3

R.T.: 5.357 min
Delta R.T.: -0.005 min
Response: 822719
Conc: 30.54 ng/ml

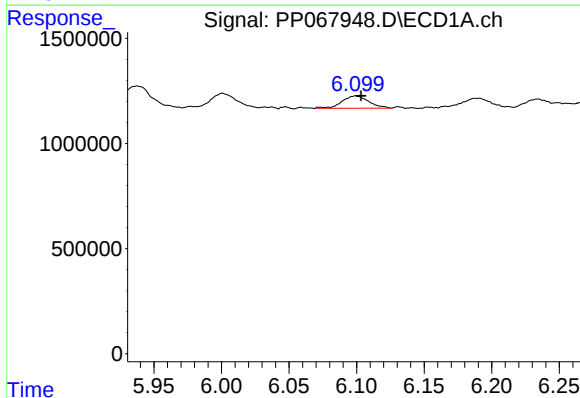


#6 AR-1016-4

R.T.: 6.100 min
Delta R.T.: -0.004 min
Response: 803761
Conc: 31.22 ng/ml

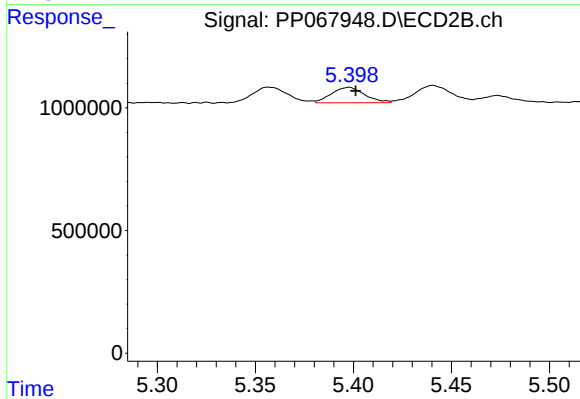

#6 AR-1016-4


R.T.: 5.398 min
Delta R.T.: -0.003 min
Response: 745791
Conc: 30.96 ng/ml

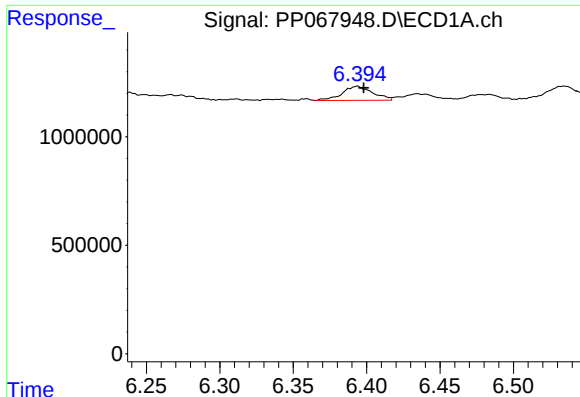

#7 AR-1016-5


R.T.: 6.394 min
Delta R.T.: -0.004 min
Response: 932897
Conc: 34.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

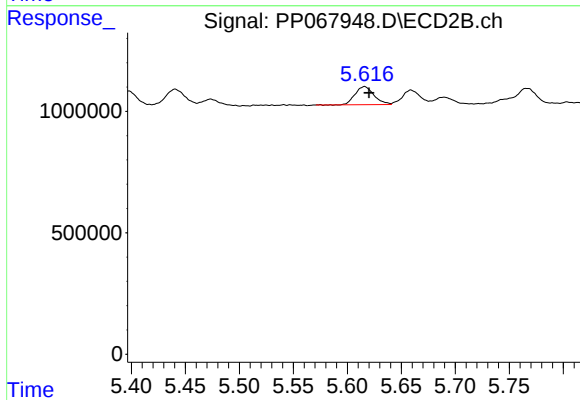


#7 AR-1016-5

R.T.: 5.616 min
Delta R.T.: -0.004 min
Response: 913633
Conc: 30.04 ng/ml

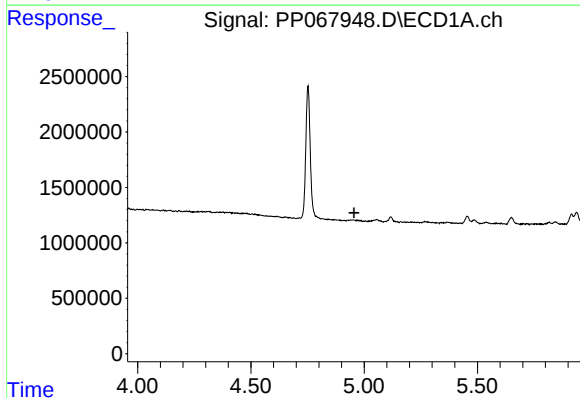


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.955 min
Response: 0
Conc: N.D.

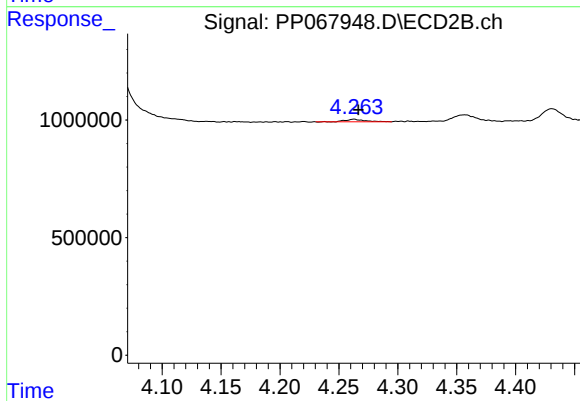

#8 AR-1221-1


R.T.: 4.263 min
Delta R.T.: -0.004 min
Response: 128128
Conc: 9.73 ng/ml

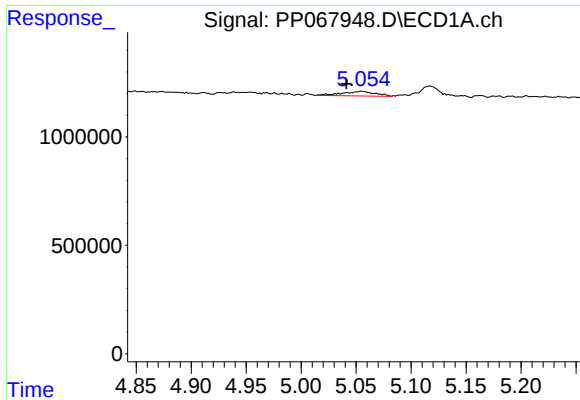

#9 AR-1221-2


R.T.: 5.055 min
Delta R.T.: 0.014 min
Response: 449652
Conc: 47.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

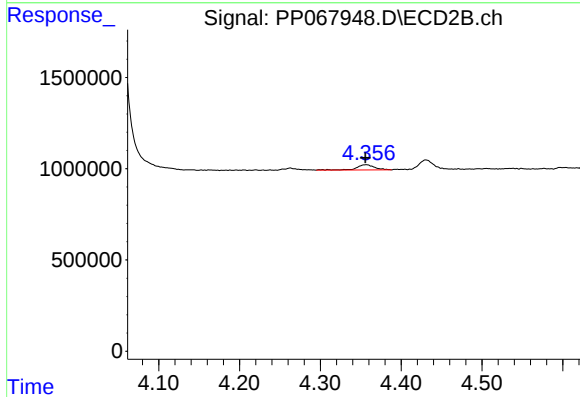


#9 AR-1221-2

R.T.: 4.357 min
Delta R.T.: 0.001 min
Response: 448580
Conc: 45.03 ng/ml

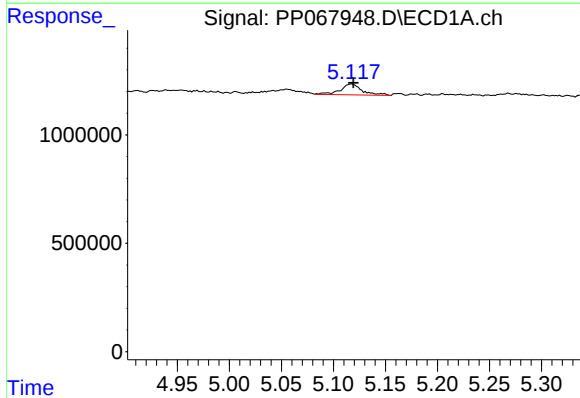


#10 AR-1221-3

R.T.: 5.118 min
Delta R.T.: -0.002 min
Response: 733092
Conc: 25.36 ng/ml

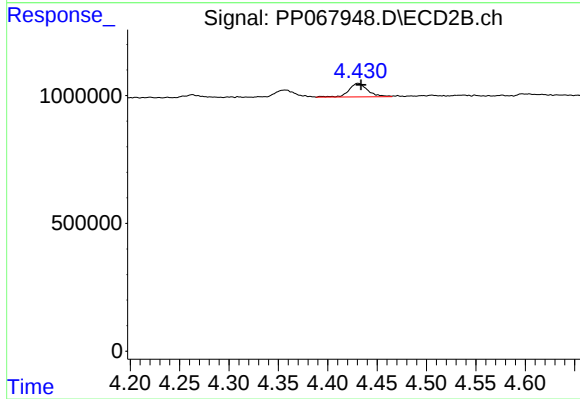

#10 AR-1221-3


R.T.: 4.431 min
Delta R.T.: -0.003 min
Response: 705887
Conc: 22.67 ng/ml

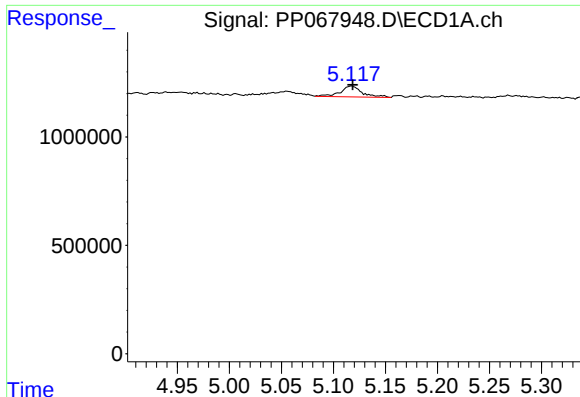

#11 AR-1232-1


R.T.: 5.118 min
Delta R.T.: -0.001 min
Response: 733092
Conc: 32.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

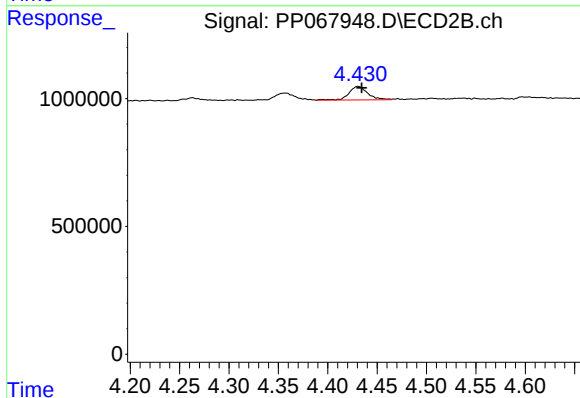


#11 AR-1232-1

R.T.: 4.431 min
Delta R.T.: -0.004 min
Response: 705887
Conc: 29.01 ng/ml

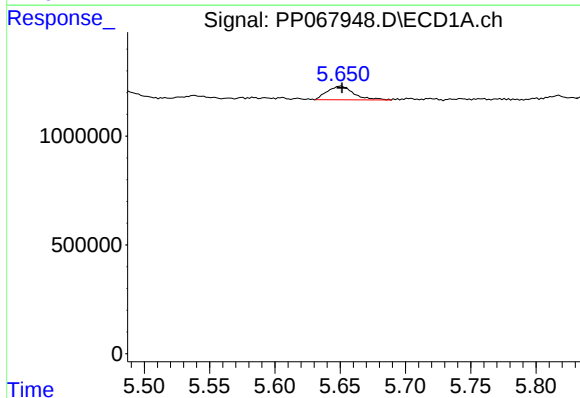


#12 AR-1232-2

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 884617
Conc: 75.08 ng/ml

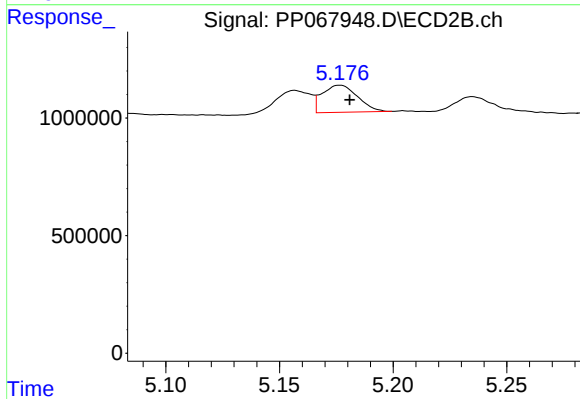

#12 AR-1232-2


R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 1252294
Conc: 55.99 ng/ml

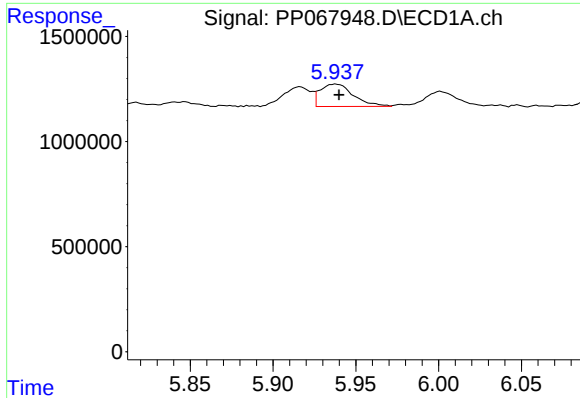

#13 AR-1232-3


R.T.: 5.938 min
Delta R.T.: -0.002 min
Response: 1491487
Conc: 66.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

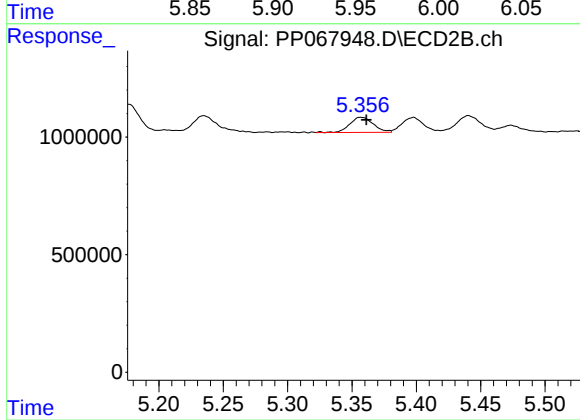


#13 AR-1232-3

R.T.: 5.357 min
Delta R.T.: -0.004 min
Response: 822719
Conc: 68.88 ng/ml

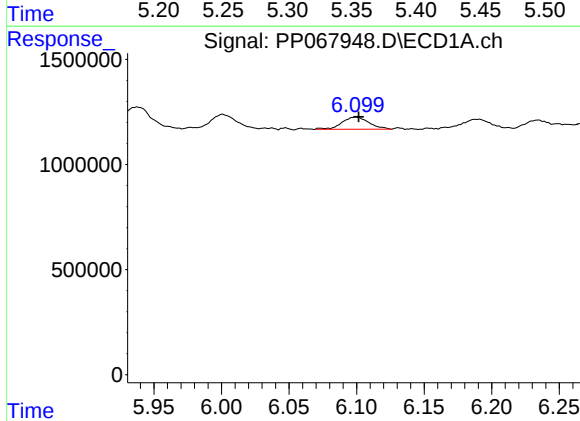


#14 AR-1232-4

R.T.: 6.100 min
Delta R.T.: -0.002 min
Response: 803761
Conc: 71.21 ng/ml

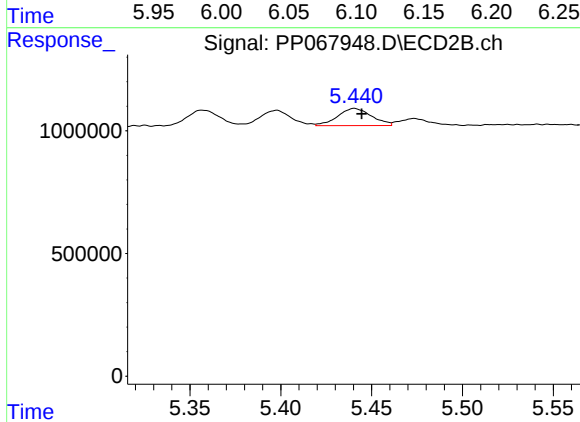

#14 AR-1232-4


R.T.: 5.441 min
Delta R.T.: -0.004 min
Response: 917565
Conc: 79.57 ng/ml

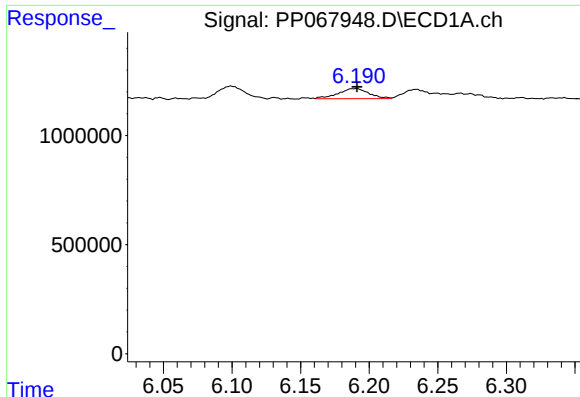

#15 AR-1232-5


R.T.: 6.191 min
Delta R.T.: 0.000 min
Response: 718911
Conc: 78.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

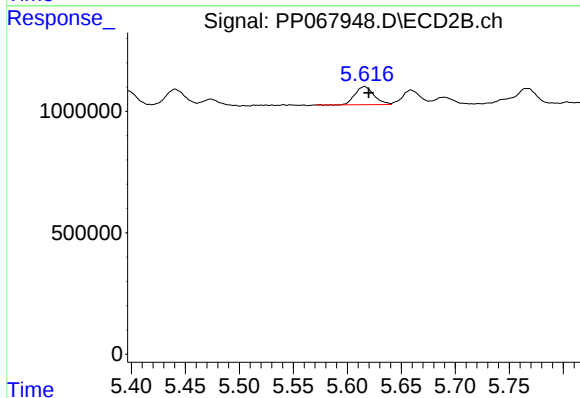


#15 AR-1232-5

R.T.: 5.616 min
Delta R.T.: -0.004 min
Response: 913633
Conc: 67.93 ng/ml

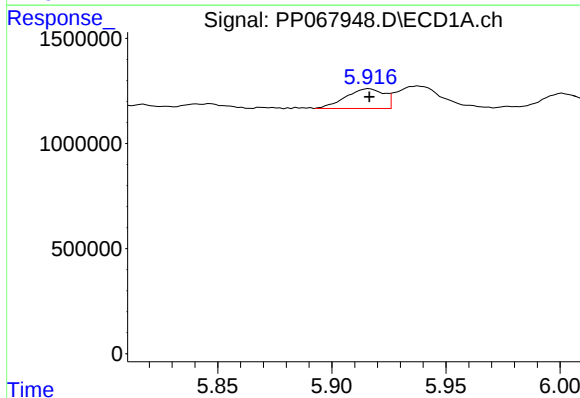


#16 AR-1242-1

R.T.: 5.916 min
Delta R.T.: 0.000 min
Response: 1093826
Conc: 39.15 ng/ml

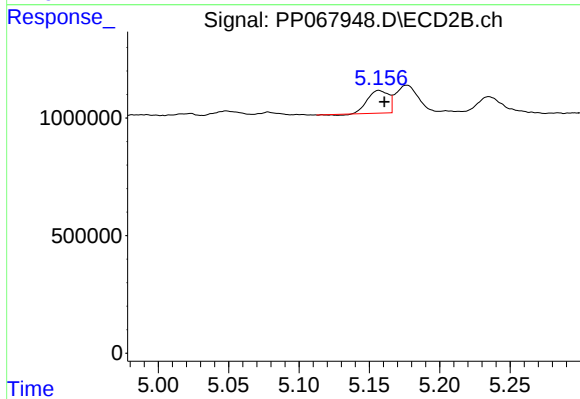

#16 AR-1242-1


R.T.: 5.157 min
Delta R.T.: -0.004 min
Response: 985653
Conc: 33.90 ng/ml

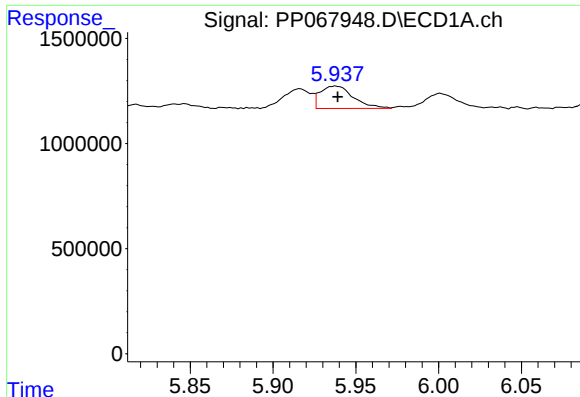

#17 AR-1242-2


R.T.: 5.938 min
Delta R.T.: -0.001 min
Response: 1491487
Conc: 36.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

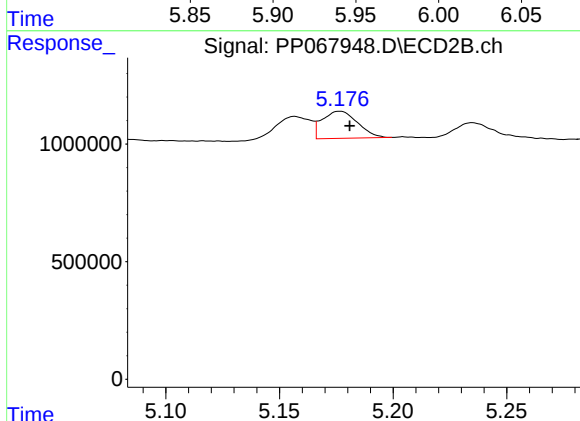


#17 AR-1242-2

R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 1252294
Conc: 31.19 ng/ml

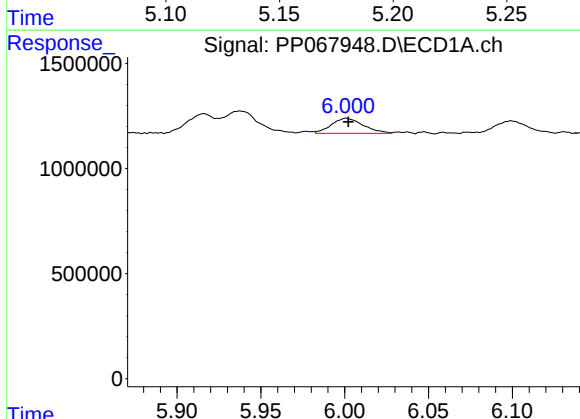


#18 AR-1242-3

R.T.: 6.001 min
Delta R.T.: -0.001 min
Response: 951205
Conc: 35.28 ng/ml

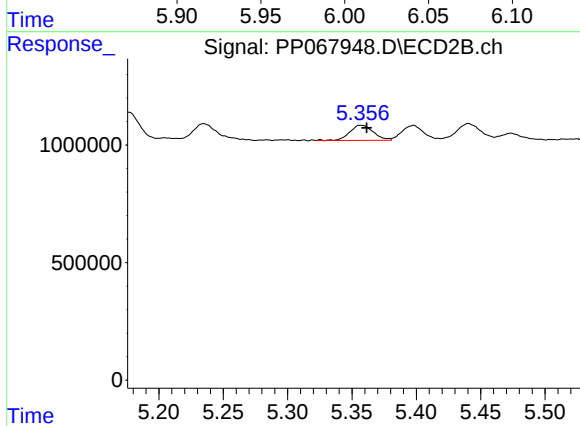

#18 AR-1242-3


R.T.: 5.357 min
Delta R.T.: -0.005 min
Response: 822719
Conc: 36.57 ng/ml

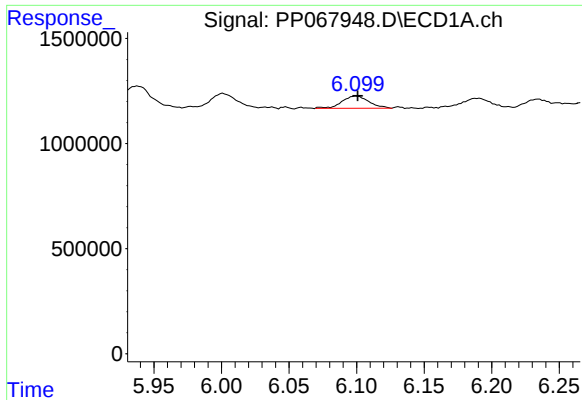

#19 AR-1242-4


R.T.: 6.100 min
Delta R.T.: -0.001 min
Response: 803761
Conc: 37.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

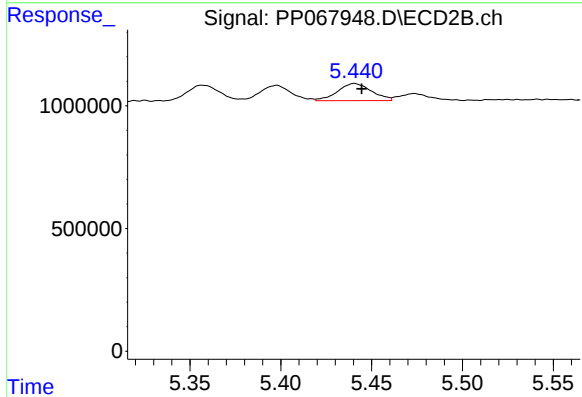


#19 AR-1242-4

R.T.: 5.441 min
Delta R.T.: -0.004 min
Response: 917565
Conc: 38.65 ng/ml

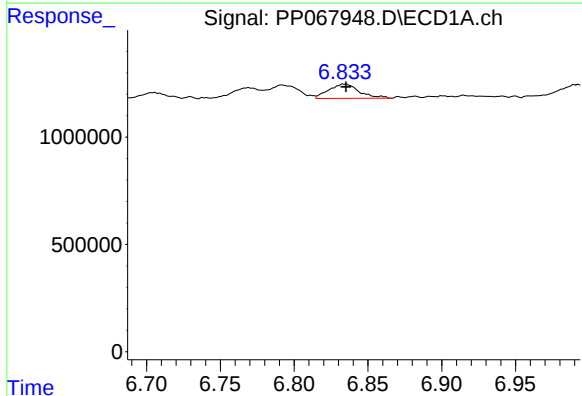


#20 AR-1242-5

R.T.: 6.834 min
Delta R.T.: 0.000 min
Response: 957085
Conc: 39.67 ng/ml

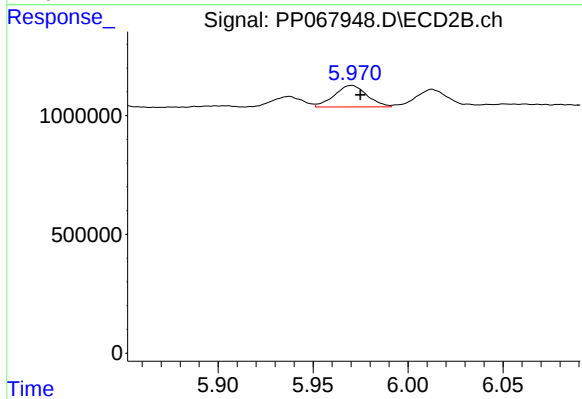

#20 AR-1242-5


R.T.: 5.970 min
Delta R.T.: -0.005 min
Response: 1082330
Conc: 37.78 ng/ml

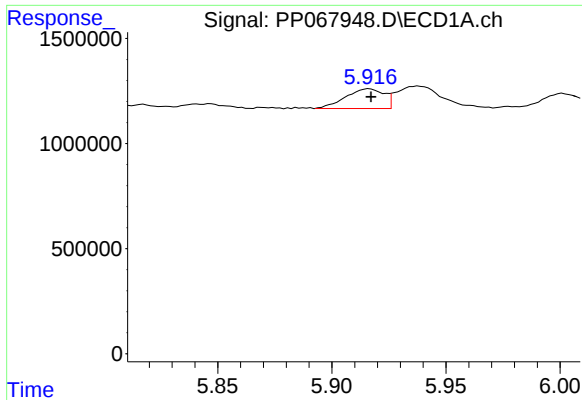

#21 AR-1248-1


R.T.: 5.916 min
Delta R.T.: 0.000 min
Response: 1093826
Conc: 51.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

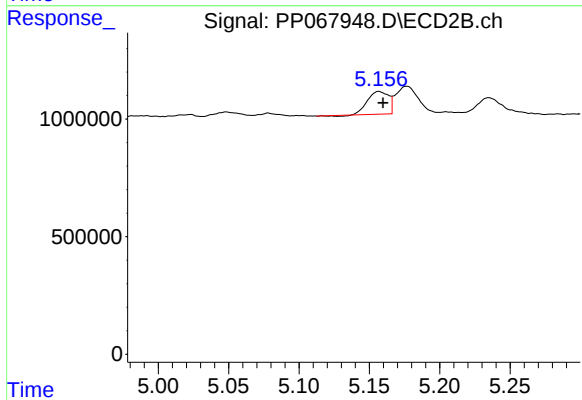


#21 AR-1248-1

R.T.: 5.157 min
Delta R.T.: -0.003 min
Response: 985653
Conc: 43.49 ng/ml

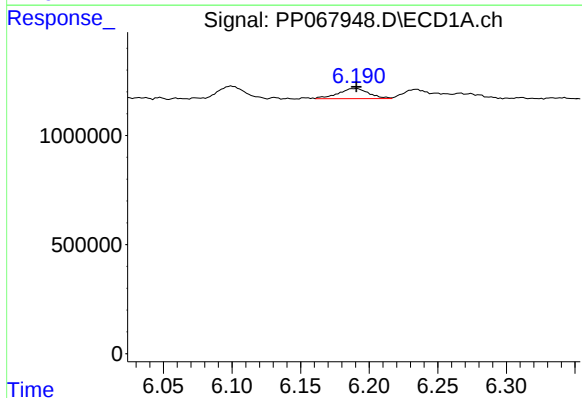


#22 AR-1248-2

R.T.: 6.191 min
Delta R.T.: 0.000 min
Response: 718911
Conc: 21.39 ng/ml

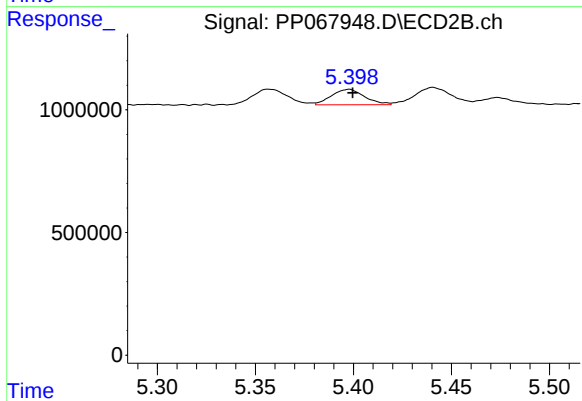

#22 AR-1248-2


R.T.: 5.398 min
Delta R.T.: -0.002 min
Response: 745791
Conc: 22.53 ng/ml

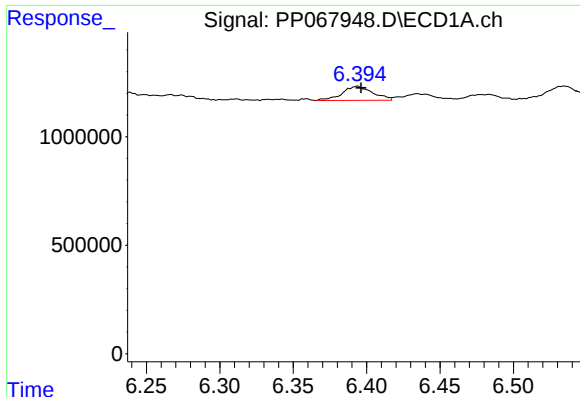

#23 AR-1248-3


R.T.: 6.394 min
Delta R.T.: -0.002 min
Response: 932897
Conc: 25.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

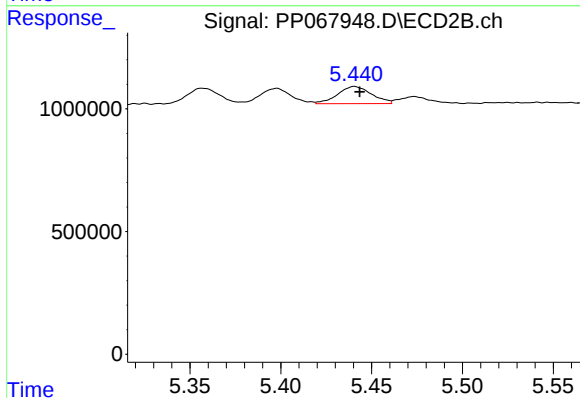


#23 AR-1248-3

R.T.: 5.441 min
Delta R.T.: -0.003 min
Response: 917565
Conc: 26.62 ng/ml

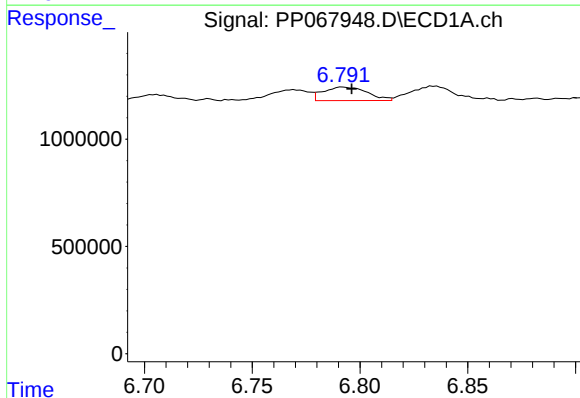


#24 AR-1248-4

R.T.: 6.792 min
Delta R.T.: -0.004 min
Response: 904771
Conc: 22.37 ng/ml

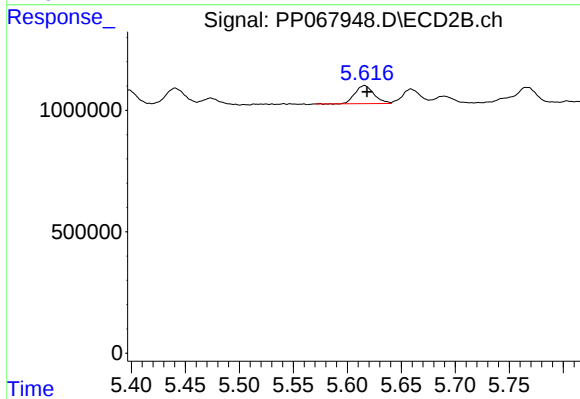

#24 AR-1248-4


R.T.: 5.616 min
Delta R.T.: -0.002 min
Response: 913633
Conc: 22.31 ng/ml

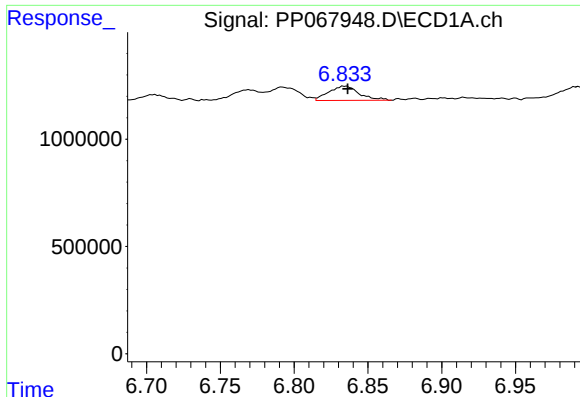

#25 AR-1248-5


R.T.: 6.834 min
Delta R.T.: -0.002 min
Response: 957085
Conc: 24.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

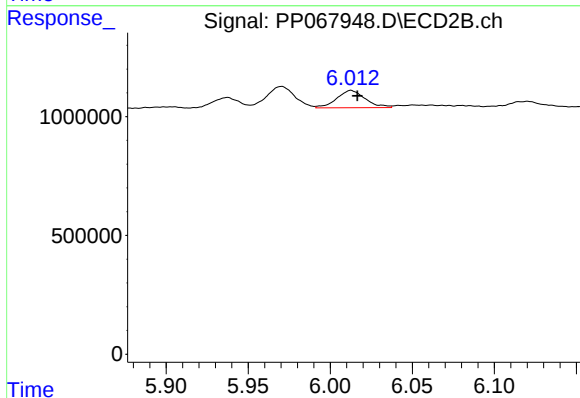


#25 AR-1248-5

R.T.: 6.013 min
Delta R.T.: -0.004 min
Response: 874108
Conc: 23.34 ng/ml

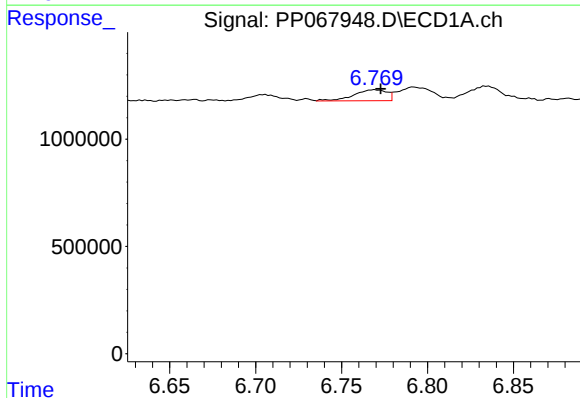


#26 AR-1254-1

R.T.: 6.769 min
Delta R.T.: -0.003 min
Response: 692831
Conc: 15.47 ng/ml

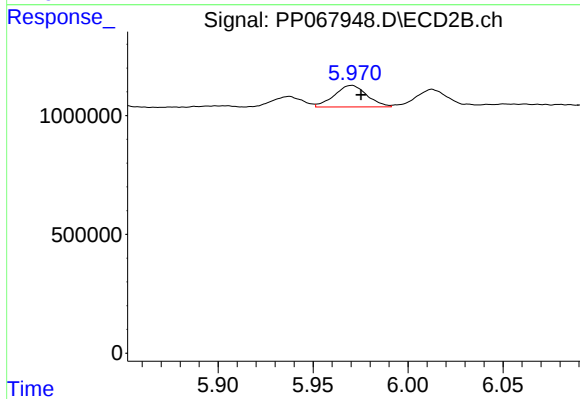

#26 AR-1254-1


R.T.: 5.970 min
Delta R.T.: -0.005 min
Response: 1082330
Conc: 18.32 ng/ml

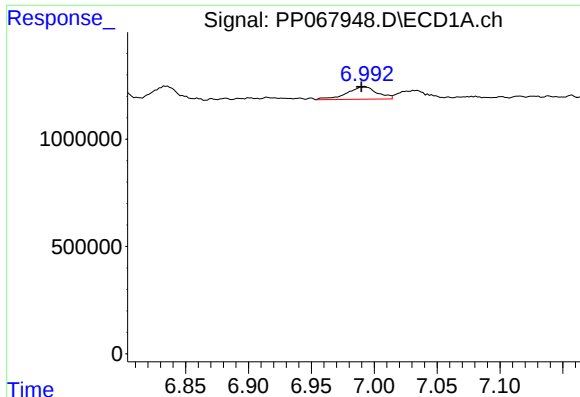

#27 AR-1254-2


R.T.: 6.992 min
Delta R.T.: 0.002 min
Response: 974639
Conc: 14.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

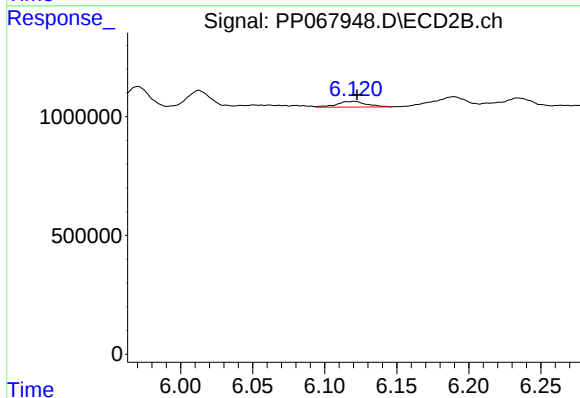


#27 AR-1254-2

R.T.: 6.120 min
Delta R.T.: -0.002 min
Response: 331847
Conc: 6.33 ng/ml

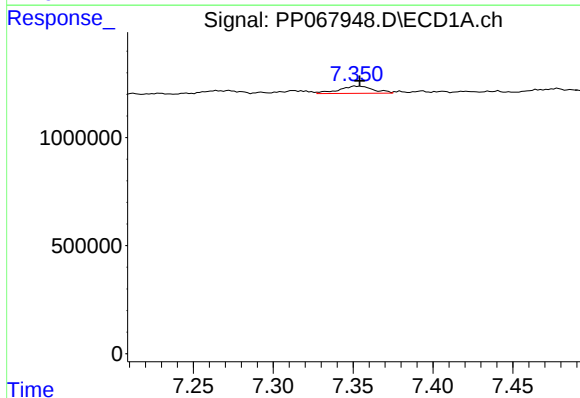


#28 AR-1254-3

R.T.: 7.352 min
Delta R.T.: -0.002 min
Response: 494561
Conc: 7.12 ng/ml

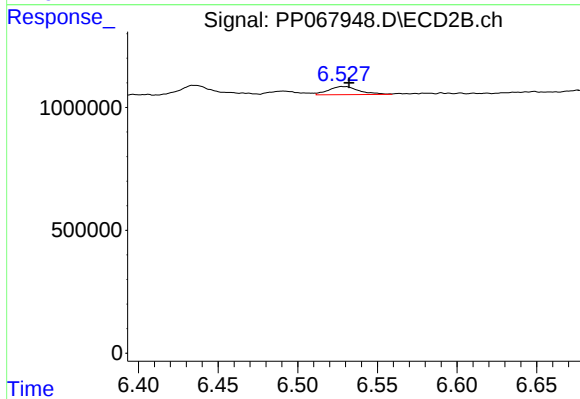

#28 AR-1254-3


R.T.: 6.528 min
Delta R.T.: -0.004 min
Response: 441388
Conc: 5.30 ng/ml

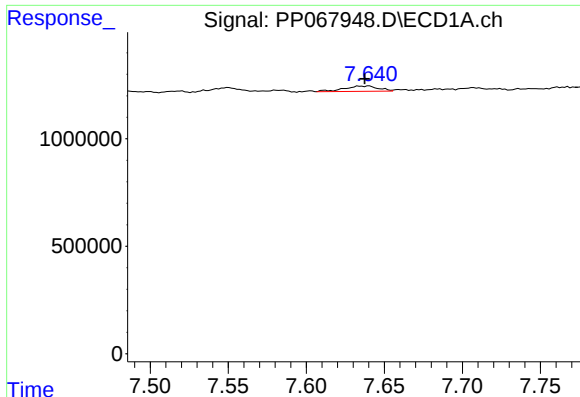

#29 AR-1254-4


R.T.: 7.640 min
Delta R.T.: 0.003 min
Response: 377755
Conc: 7.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

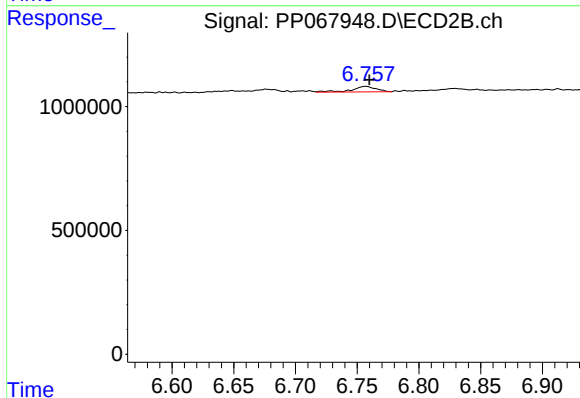


#29 AR-1254-4

R.T.: 6.757 min
Delta R.T.: -0.003 min
Response: 305371
Conc: 6.33 ng/ml

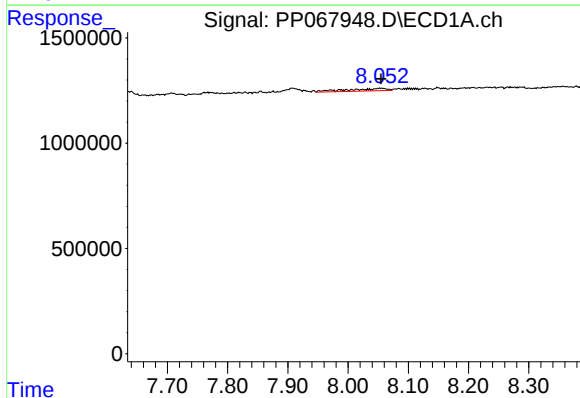


#30 AR-1254-5

R.T.: 8.054 min
Delta R.T.: 0.000 min
Response: 570188
Conc: 9.62 ng/ml

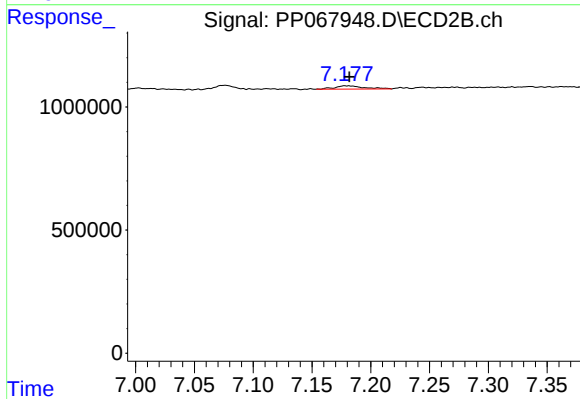

#30 AR-1254-5


R.T.: 7.179 min
Delta R.T.: -0.003 min
Response: 235927
Conc: 3.21 ng/ml

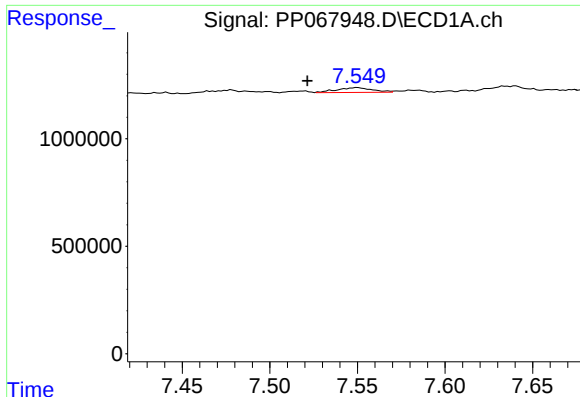

#31 AR-1260-1


R.T.: 7.550 min
Delta R.T.: 0.029 min
Response: 317251
Conc: 5.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

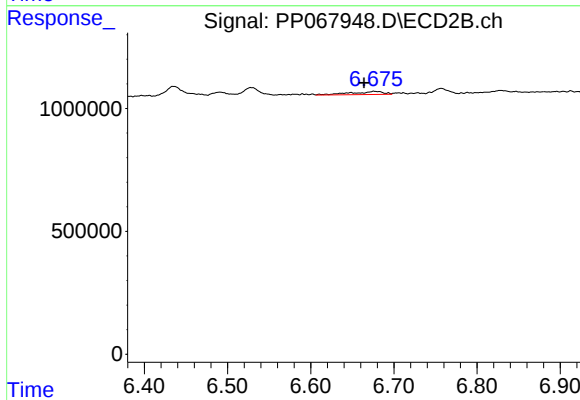


#31 AR-1260-1

R.T.: 6.676 min
Delta R.T.: 0.012 min
Response: 344622
Conc: 6.05 ng/ml

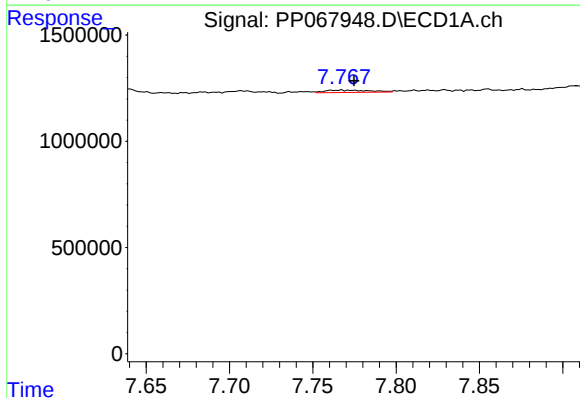


#32 AR-1260-2

R.T.: 7.767 min
Delta R.T.: -0.007 min
Response: 205933
Conc: 3.25 ng/ml

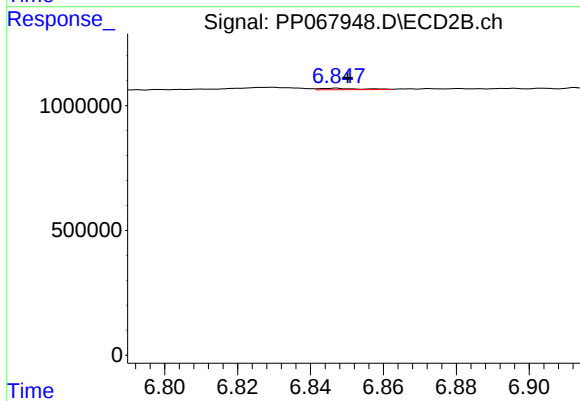

#32 AR-1260-2


R.T.: 6.847 min
Delta R.T.: -0.004 min
Response: 40290
Conc: 0.60 ng/ml

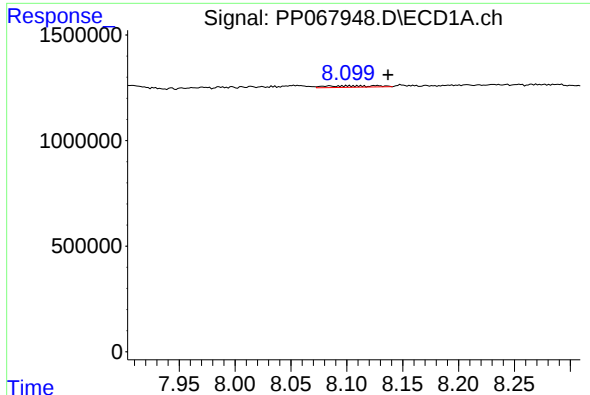

#33 AR-1260-3


R.T.: 8.113 min
Delta R.T.: -0.024 min
Response: 220951
Conc: 4.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

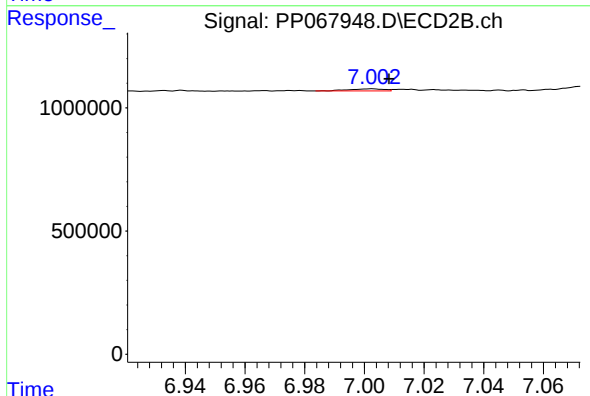


#33 AR-1260-3

R.T.: 7.002 min
Delta R.T.: -0.006 min
Response: 66566
Conc: 1.04 ng/ml

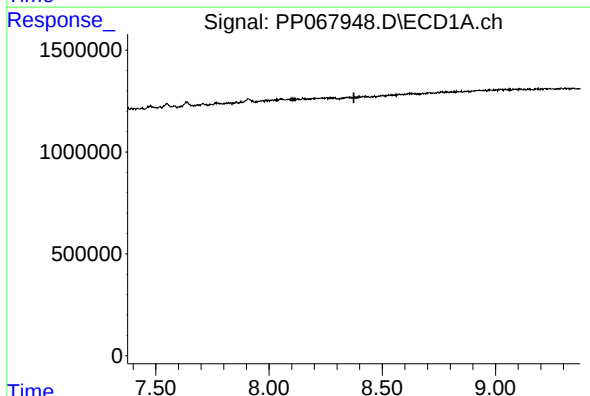


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

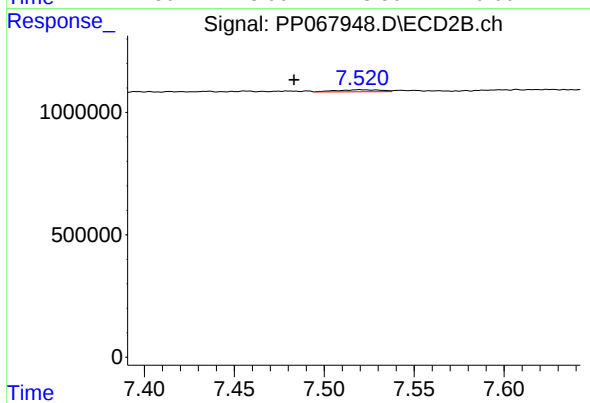

#34 AR-1260-4


R.T.: 7.520 min
Delta R.T.: 0.037 min
Response: 133465
Conc: 2.41 ng/ml

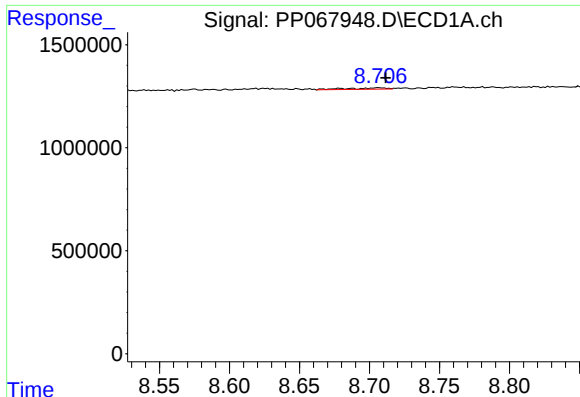

#35 AR-1260-5


R.T.: 8.707 min
Delta R.T.: -0.005 min
Response: 131201
Conc: 1.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

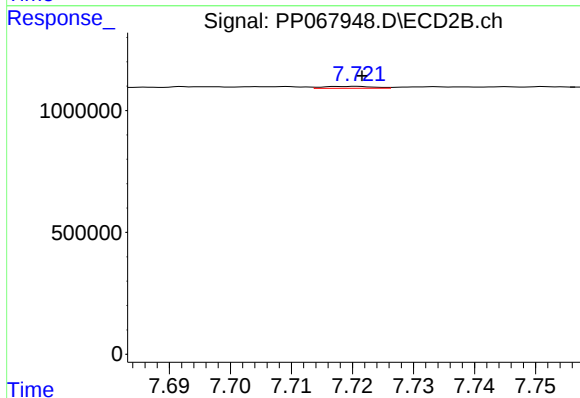


#35 AR-1260-5

R.T.: 7.720 min
Delta R.T.: -0.002 min
Response: 45439
Conc: 0.37 ng/ml

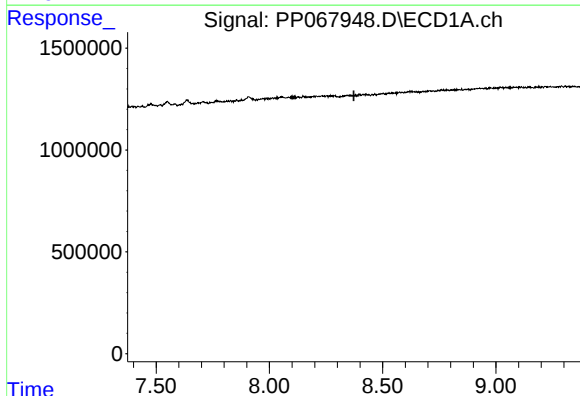


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 8.373 min
Response: 0
Conc: N.D.

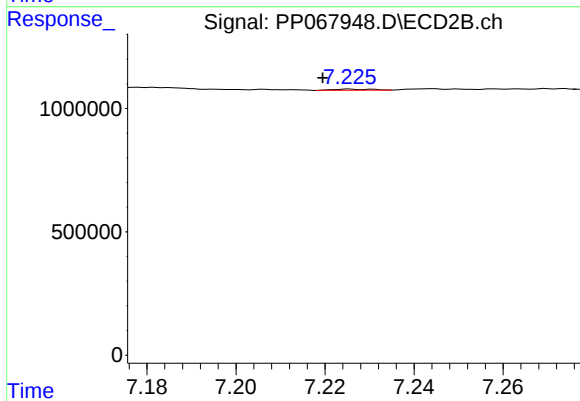

#36 AR-1262-1


R.T.: 7.225 min
Delta R.T.: 0.006 min
Response: 29775
Conc: 0.38 ng/ml

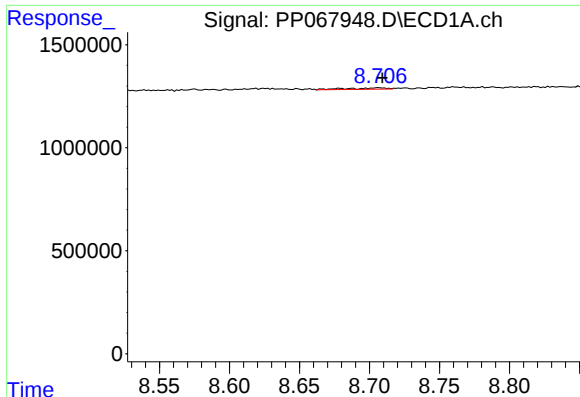

#37 AR-1262-2


R.T.: 8.707 min
Delta R.T.: -0.002 min
Response: 131201
Conc: 1.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

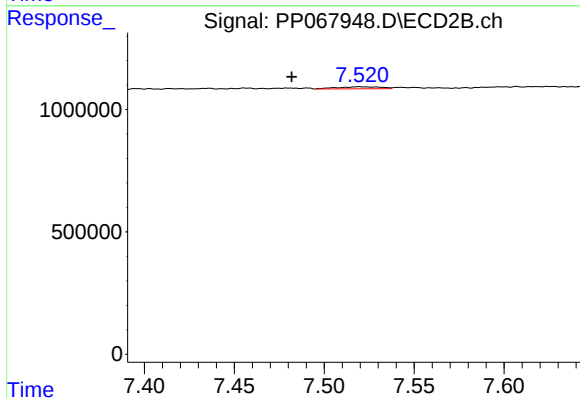


#37 AR-1262-2

R.T.: 7.520 min
Delta R.T.: 0.038 min
Response: 133465
Conc: 1.88 ng/ml

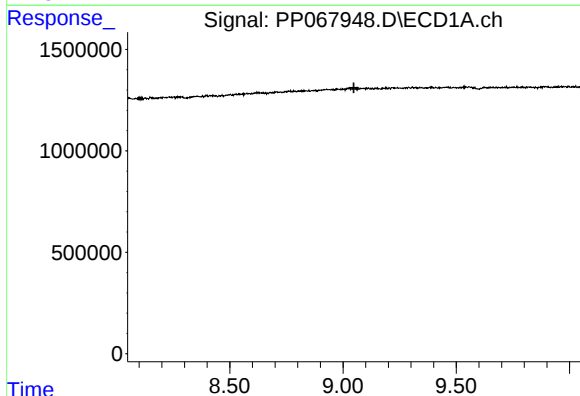


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.048 min
Response: 0
Conc: N.D.

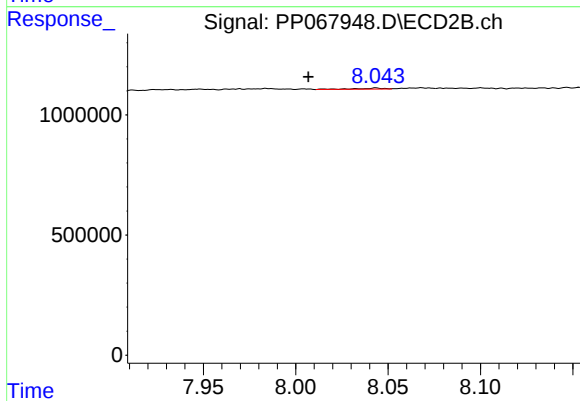

#38 AR-1262-3


R.T.: 8.044 min
Delta R.T.: 0.037 min
Response: 43143
Conc: 0.76 ng/ml

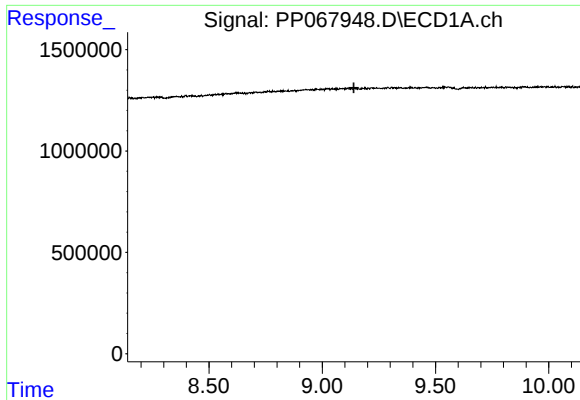

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 9.140 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

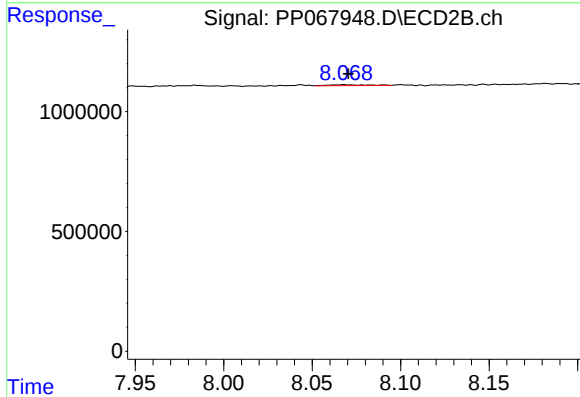


#39 AR-1262-4

R.T.: 8.068 min
Delta R.T.: -0.002 min
Response: 58186
Conc: 0.58 ng/ml

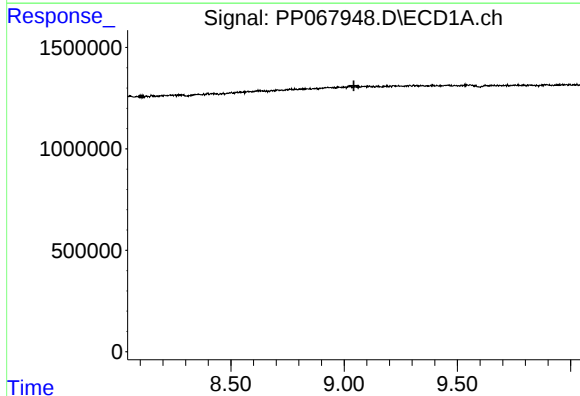


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.043 min
Response: 0
Conc: N.D.

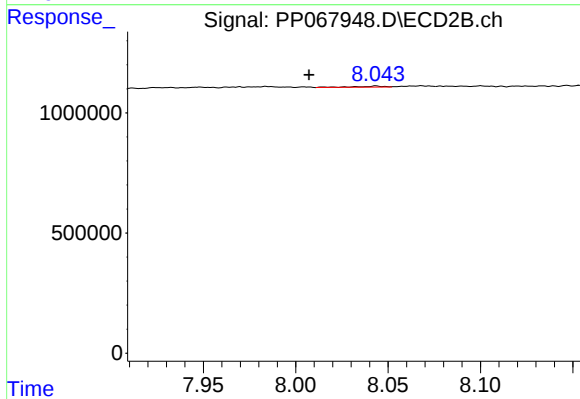

#41 AR-1268-1


R.T.: 8.044 min
Delta R.T.: 0.036 min
Response: 43143
Conc: 0.27 ng/ml

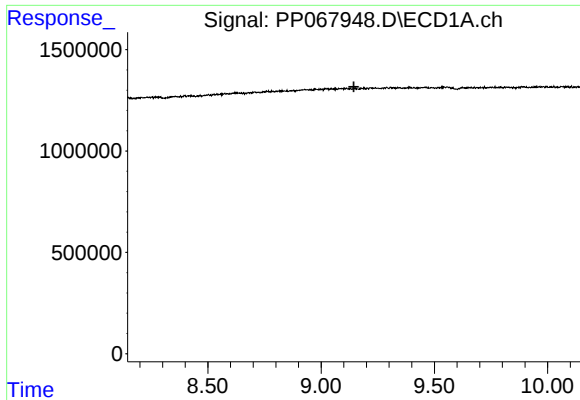

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 9.144 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

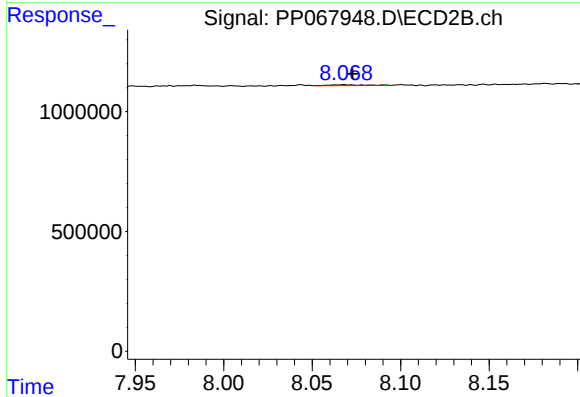


#42 AR-1268-2

R.T.: 8.068 min
Delta R.T.: -0.005 min
Response: 58186
Conc: 0.41 ng/ml

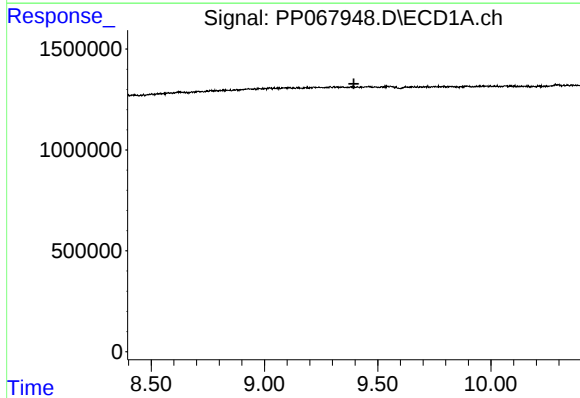


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.395 min
Response: 0
Conc: N.D.

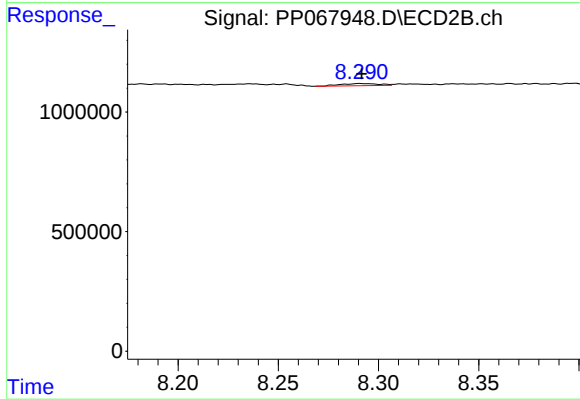

#43 AR-1268-3


R.T.: 8.291 min
Delta R.T.: 0.000 min
Response: 118800
Conc: 0.93 ng/ml

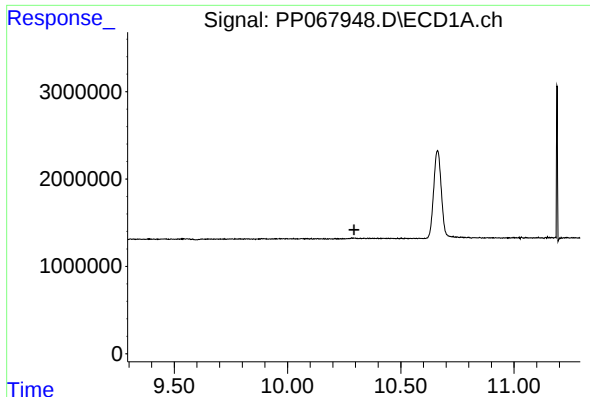

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.294 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

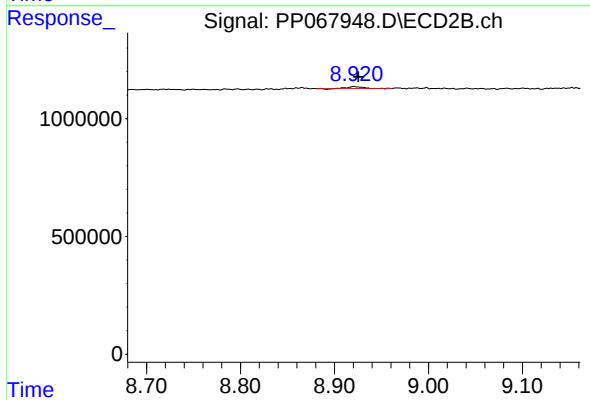

#45 AR-1268-5

R.T.: 8.921 min
Delta R.T.: -0.005 min
Response: 95529
Conc: 0.25 ng/ml