

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
 Data File : PP067949.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2024 01:18
 Operator : YP\AJ
 Sample : P4368-07
 Misc : AR1248 LOD 40 PPB
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 07:30:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.754	4.050	14684770	15335507	15.864	15.178
2)	SA Decachlor...	10.662	9.210	20876426	19308854	18.133	17.218
Target Compounds							
3)	L1 AR-1016-1	5.918	5.157	876198	769817	26.498	22.003
4)	L1 AR-1016-2	5.939	5.177	963471	746070	19.755	15.489
5)	L1 AR-1016-3	6.001	5.359	543779	530502	17.256	19.694
6)	L1 AR-1016-4	6.101	5.397	549628	1231940	21.350	51.149 #
7)	L1 AR-1016-5	6.397	5.616	1407996	1438668	52.019	47.309
9)	L2 AR-1221-2	5.055	4.357	202836	268180	21.440	26.922 #
10)	L2 AR-1221-3	5.055f	4.435	202836	76114	7.017	2.445 #
11)	L3 AR-1232-1	5.055f	4.435	202836	76114	8.873	3.128 #
12)	L3 AR-1232-2	5.647	5.177	401277	746070	34.055	33.359
13)	L3 AR-1232-3	5.939	5.359	963471	530502	43.253	44.416
14)	L3 AR-1232-4	6.101	5.441	549628	1270630	48.694	110.189 #
15)	L3 AR-1232-5	6.190	5.616	1297264	1438668	142.241	106.962
16)	L4 AR-1242-1	5.918	5.157	876198	769817	31.363	26.476
17)	L4 AR-1242-2	5.939	5.177	963471	746070	23.711	18.583
18)	L4 AR-1242-3	6.001	5.359	543779	530502	20.166	23.583
19)	L4 AR-1242-4	6.101	5.441	549628	1270630	25.623	53.528 #
20)	L4 AR-1242-5	6.835	5.971	1475252	2006156	61.148	70.024
21)	L5 AR-1248-1	5.918	5.157	876198	769817	40.900	33.967
22)	L5 AR-1248-2	6.190	5.397	1297264	1231940	38.590	37.223
23)	L5 AR-1248-3	6.397	5.441	1407996	1270630	38.443	36.857
24)	L5 AR-1248-4	6.796	5.616	1450509	1438668	35.859	35.127
25)	L5 AR-1248-5	6.835	6.013	1475252	1316991	37.197	35.173
26)	L6 AR-1254-1	6.771	5.971	1226826	2006156	27.395	33.954
27)	L6 AR-1254-2	6.992	6.119	1579084	676923	23.890	12.903 #
28)	L6 AR-1254-3	7.354	6.529	976905	1034449	14.066	12.432
29)	L6 AR-1254-4	7.638	6.756	651877	635743	13.062	13.169
30)	L6 AR-1254-5	8.055	7.180	159442	386732	2.689	5.258 #
31)	L7 AR-1260-1	7.523	6.676	93043	392587	1.722	6.892 #
32)	L7 AR-1260-2	7.774	6.849	133878	112600	2.116	1.688
33)	L7 AR-1260-3	0.000	7.003	0	263938	N.D.	4.143 #
34)	L7 AR-1260-4	0.000	7.521f	0	188636	N.D.	3.412 #
35)	L7 AR-1260-5	8.643f	0.000	48428	0	0.450	N.D. #
36)	L8 AR-1262-1	0.000	7.249	0	93031	N.D.	1.182 #
37)	L8 AR-1262-2	8.643f	7.521f	48428	188636	0.398	2.658 #
38)	L8 AR-1262-3	0.000	8.066f	0	73191	N.D.	1.282 #
39)	L8 AR-1262-4	0.000	8.066	0	73191	N.D.	0.729 #
41)	L9 AR-1268-1	0.000	8.066f	0	73191	N.D.	0.460 #
42)	L9 AR-1268-2	0.000	8.066	0	73191	N.D.	0.511 #
43)	L9 AR-1268-3	0.000	8.298	0	153825	N.D.	1.206 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
Data File : PP067949.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 01:18
Operator : YP\AJ
Sample : P4368-07
Misc : AR1248 LOD 40 PPB
ALS Vial : 55 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:30:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
45) L9	AR-1268-5	10.290	8.920	72457	91819	0.194	0.243 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
Data File : PP067949.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 01:18
Operator : YP\AJ
Sample : P4368-07
Misc : AR1248 LOD 40 PPB
ALS Vial : 55 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:30:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

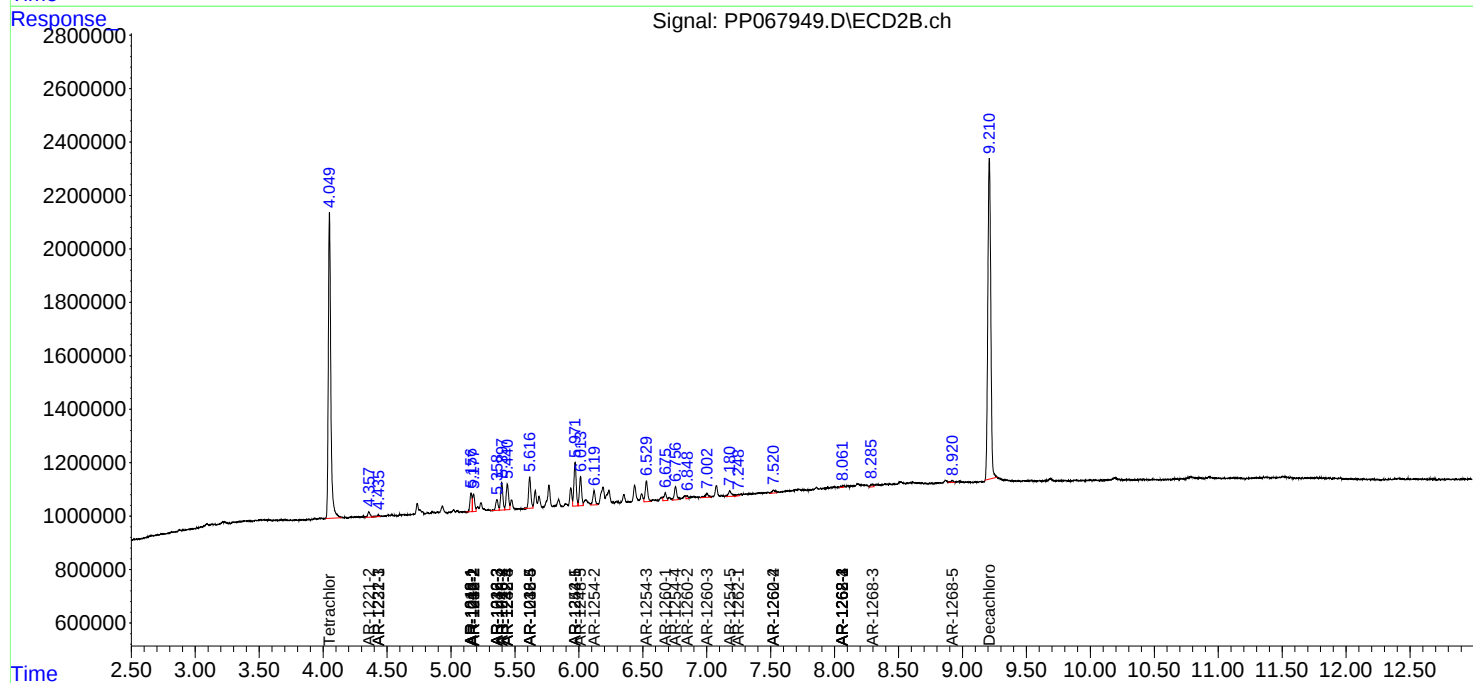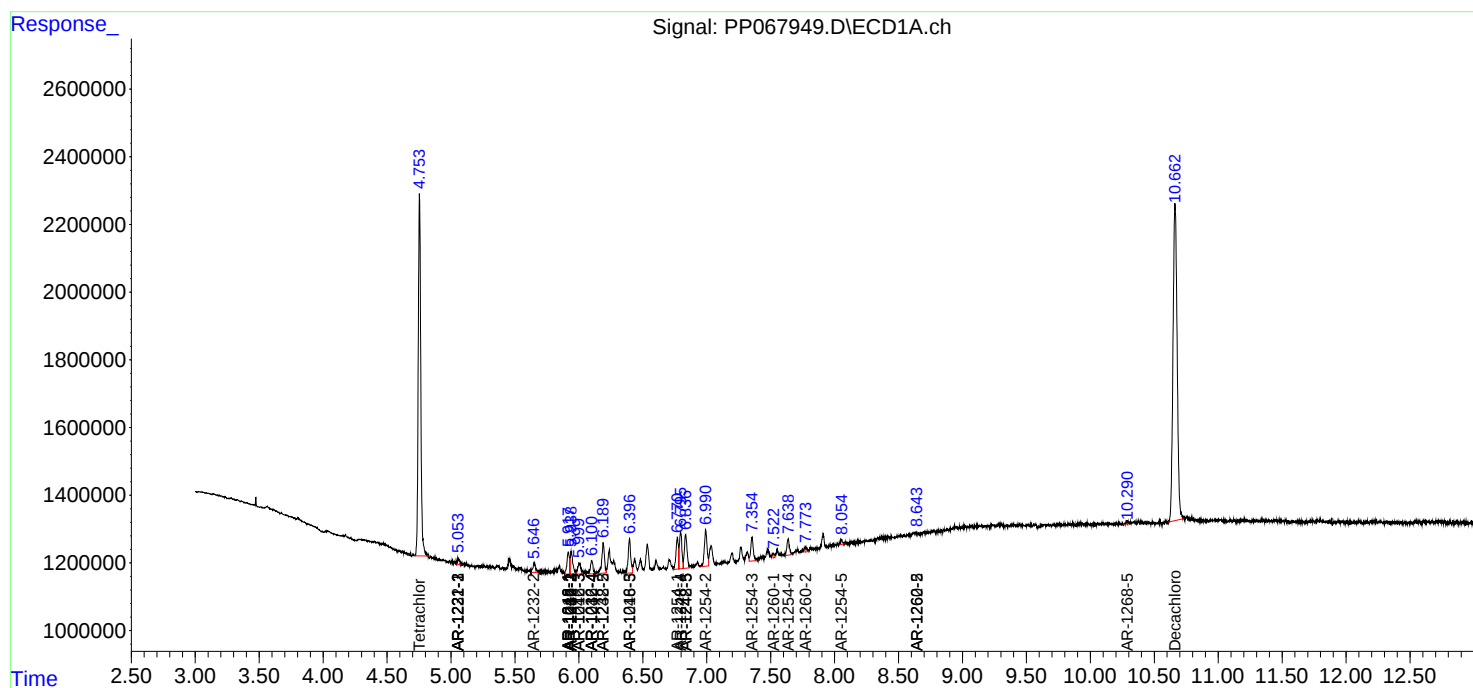


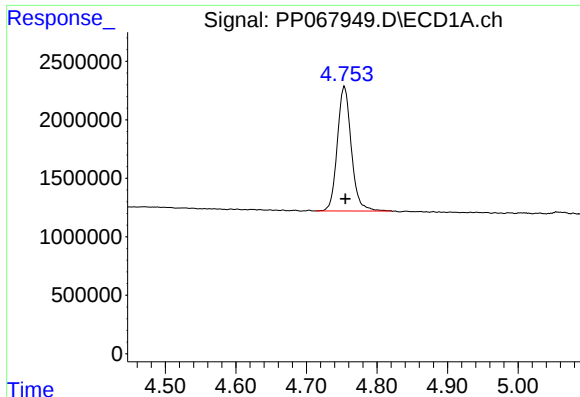

#1 Tetrachloro-m-xylene


R.T.: 4.754 min
Delta R.T.: -0.001 min
Response: 14684770
Conc: 15.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

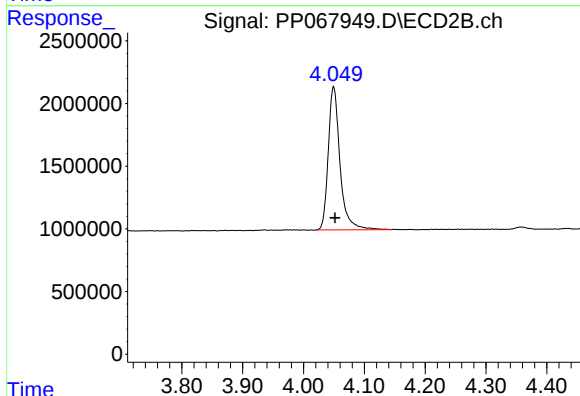


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 15335507
Conc: 15.18 ng/ml

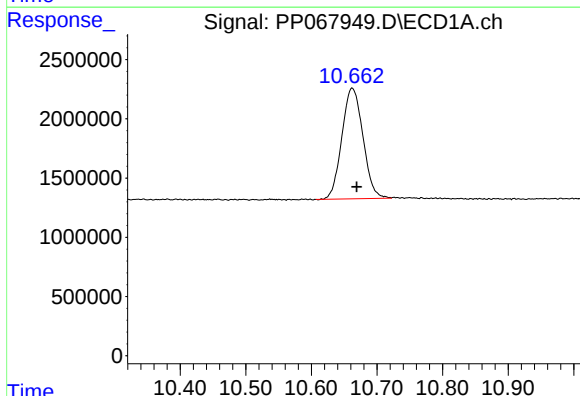


#2 Decachlorobiphenyl

R.T.: 10.662 min
Delta R.T.: -0.007 min
Response: 20876426
Conc: 18.13 ng/ml

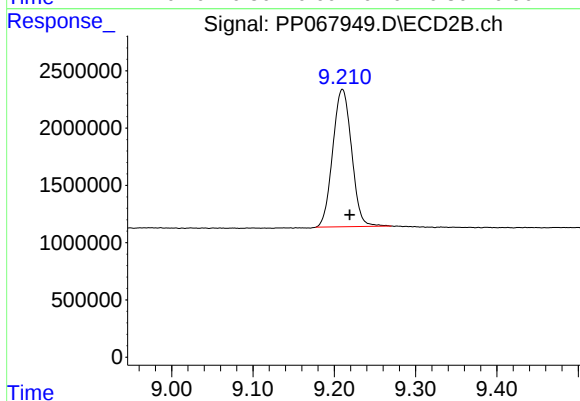

#2 Decachlorobiphenyl


R.T.: 9.210 min
Delta R.T.: -0.009 min
Response: 19308854
Conc: 17.22 ng/ml

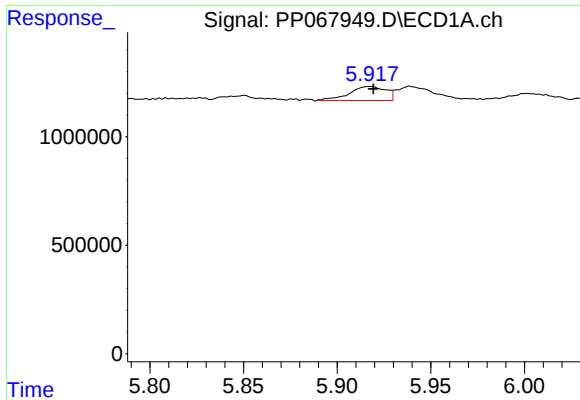

#3 AR-1016-1


R.T.: 5.918 min
Delta R.T.: -0.002 min
Response: 876198
Conc: 26.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

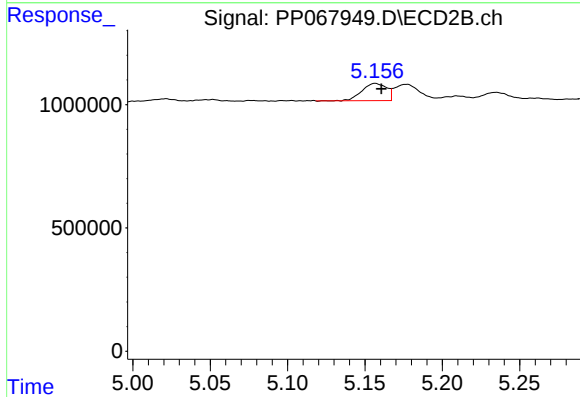


#3 AR-1016-1

R.T.: 5.157 min
Delta R.T.: -0.004 min
Response: 769817
Conc: 22.00 ng/ml

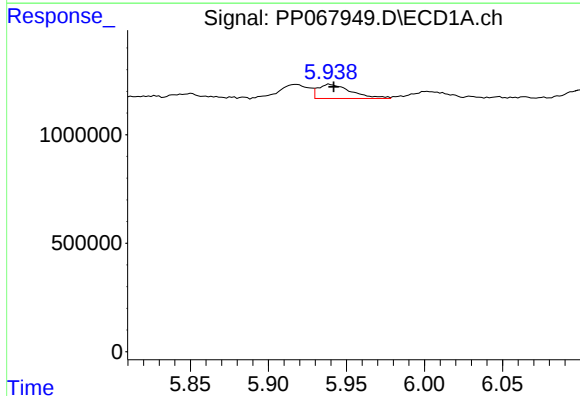


#4 AR-1016-2

R.T.: 5.939 min
Delta R.T.: -0.003 min
Response: 963471
Conc: 19.76 ng/ml

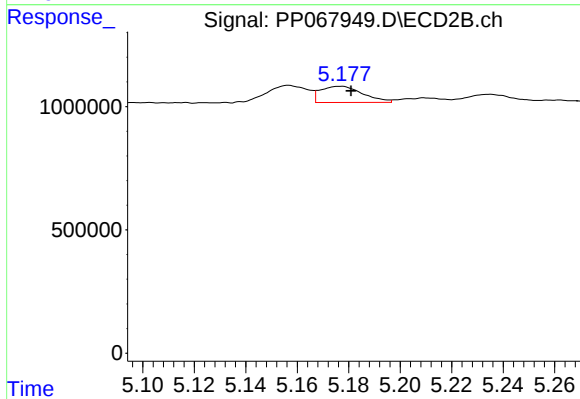

#4 AR-1016-2


R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 746070
Conc: 15.49 ng/ml

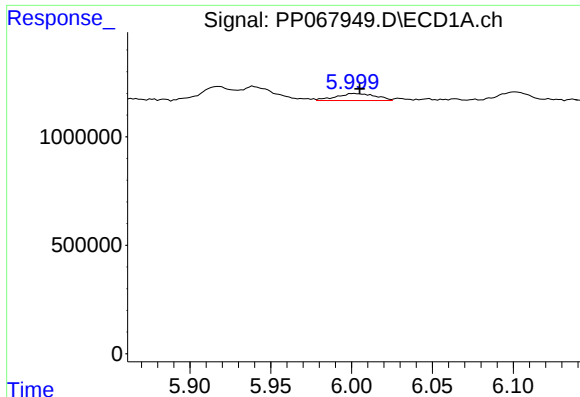

#5 AR-1016-3


R.T.: 6.001 min
Delta R.T.: -0.004 min
Response: 543779
Conc: 17.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

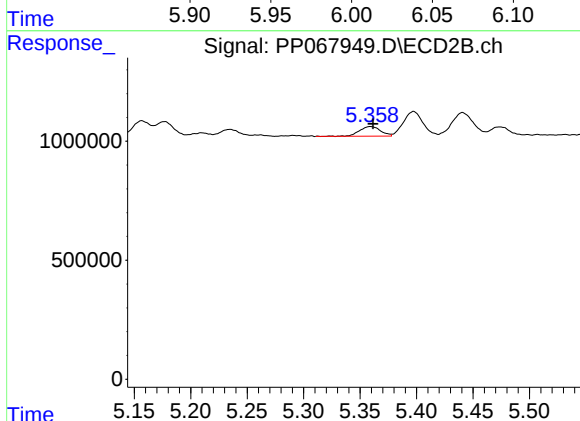


#5 AR-1016-3

R.T.: 5.359 min
Delta R.T.: -0.002 min
Response: 530502
Conc: 19.69 ng/ml

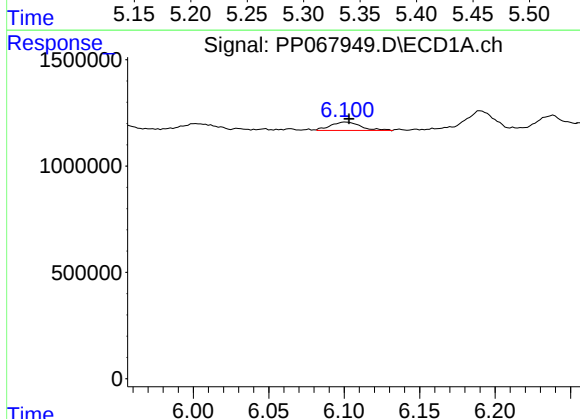


#6 AR-1016-4

R.T.: 6.101 min
Delta R.T.: -0.002 min
Response: 549628
Conc: 21.35 ng/ml

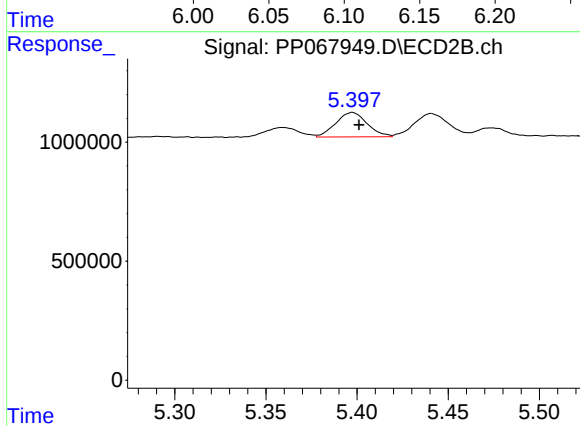

#6 AR-1016-4


R.T.: 5.397 min
Delta R.T.: -0.004 min
Response: 1231940
Conc: 51.15 ng/ml

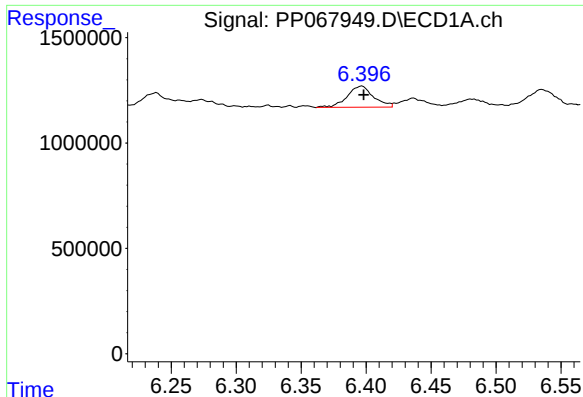

#7 AR-1016-5


R.T.: 6.397 min
Delta R.T.: -0.001 min
Response: 1407996
Conc: 52.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

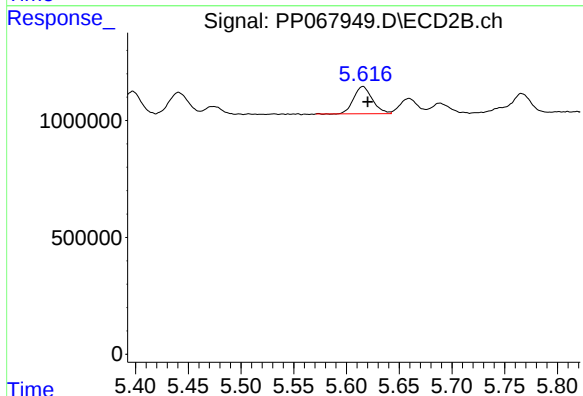


#7 AR-1016-5

R.T.: 5.616 min
Delta R.T.: -0.005 min
Response: 1438668
Conc: 47.31 ng/ml

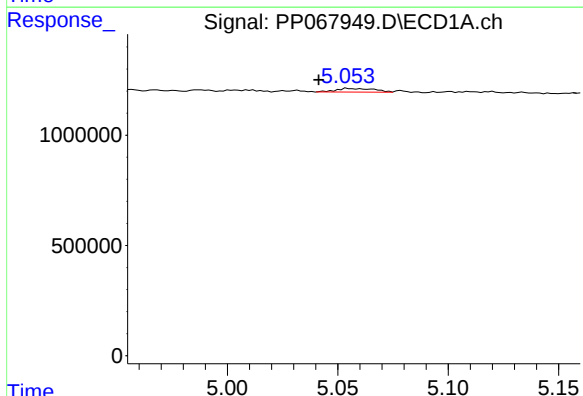


#9 AR-1221-2

R.T.: 5.055 min
Delta R.T.: 0.013 min
Response: 202836
Conc: 21.44 ng/ml

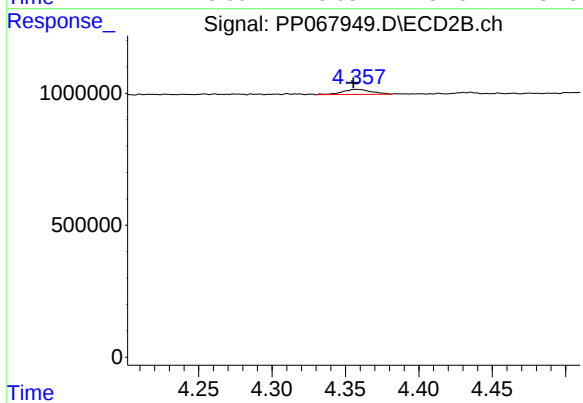

#9 AR-1221-2


R.T.: 4.357 min
Delta R.T.: 0.002 min
Response: 268180
Conc: 26.92 ng/ml

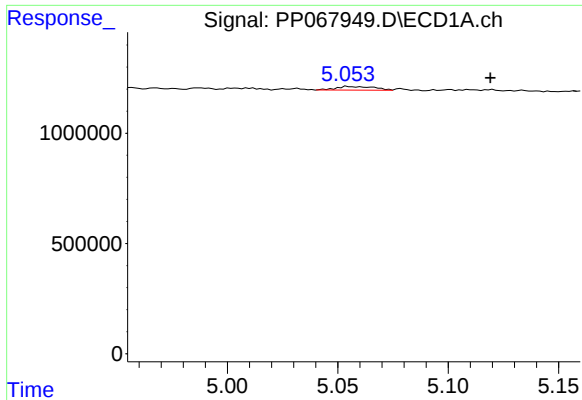

#10 AR-1221-3


R.T.: 5.055 min
Delta R.T.: -0.065 min
Response: 202836
Conc: 7.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

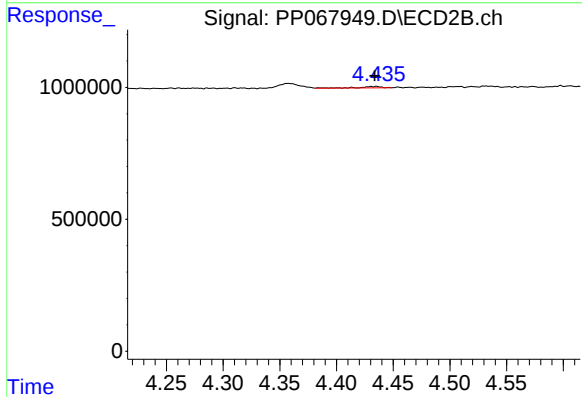


#10 AR-1221-3

R.T.: 4.435 min
Delta R.T.: 0.001 min
Response: 76114
Conc: 2.44 ng/ml

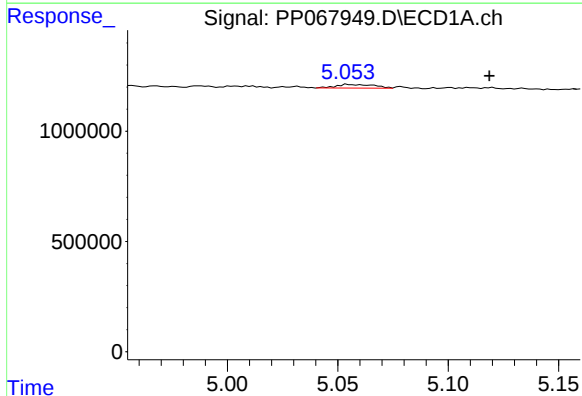


#11 AR-1232-1

R.T.: 5.055 min
Delta R.T.: -0.064 min
Response: 202836
Conc: 8.87 ng/ml

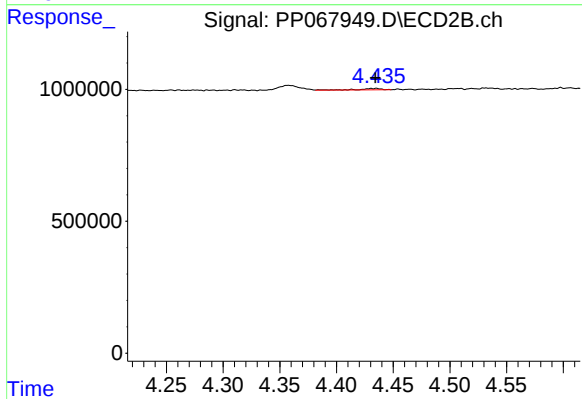

#11 AR-1232-1


R.T.: 4.435 min
Delta R.T.: 0.000 min
Response: 76114
Conc: 3.13 ng/ml

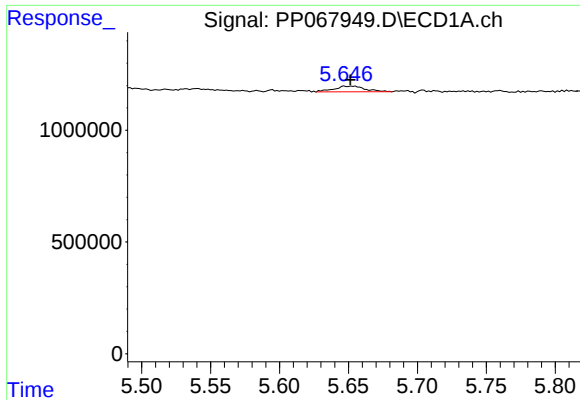

#12 AR-1232-2


R.T.: 5.647 min
Delta R.T.: -0.004 min
Response: 401277
Conc: 34.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

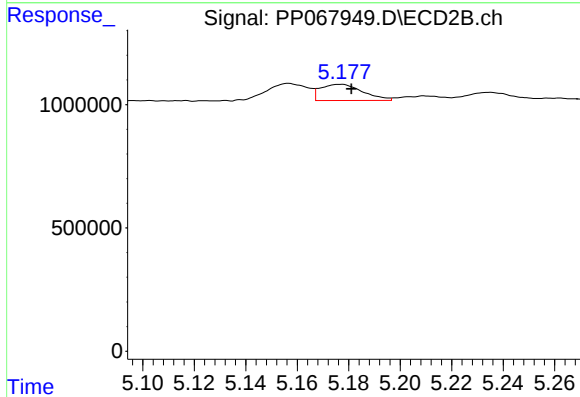


#12 AR-1232-2

R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 746070
Conc: 33.36 ng/ml

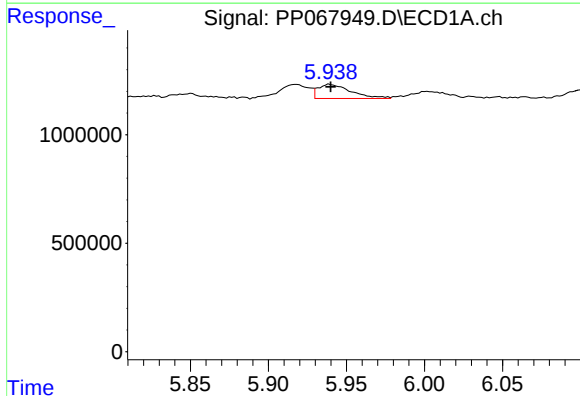


#13 AR-1232-3

R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 963471
Conc: 43.25 ng/ml

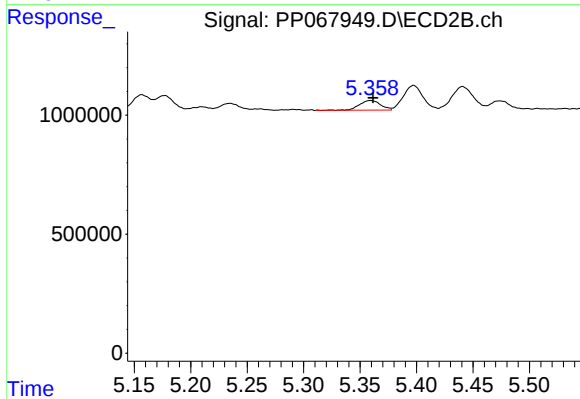

#13 AR-1232-3


R.T.: 5.359 min
Delta R.T.: -0.002 min
Response: 530502
Conc: 44.42 ng/ml

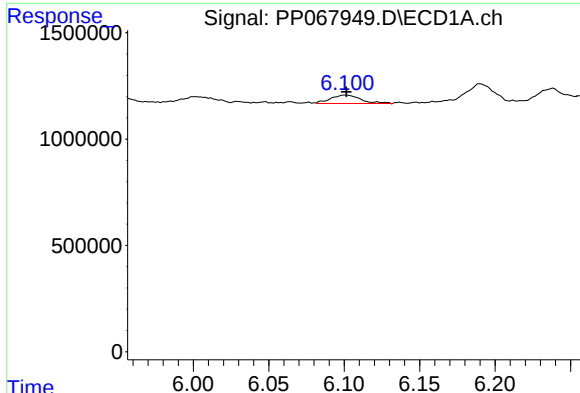

#14 AR-1232-4


R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 549628
Conc: 48.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

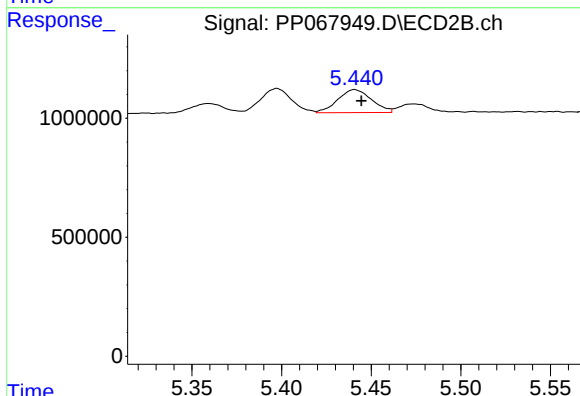


#14 AR-1232-4

R.T.: 5.441 min
Delta R.T.: -0.004 min
Response: 1270630
Conc: 110.19 ng/ml

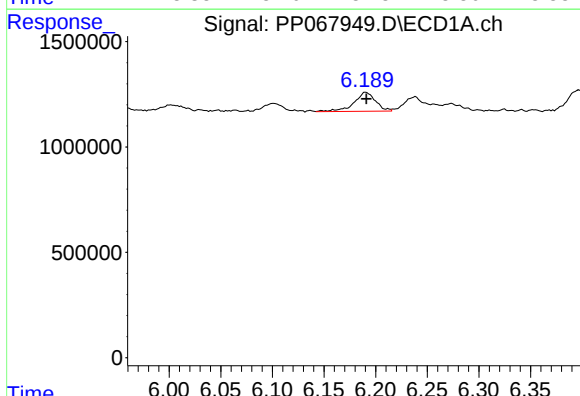


#15 AR-1232-5

R.T.: 6.190 min
Delta R.T.: 0.000 min
Response: 1297264
Conc: 142.24 ng/ml

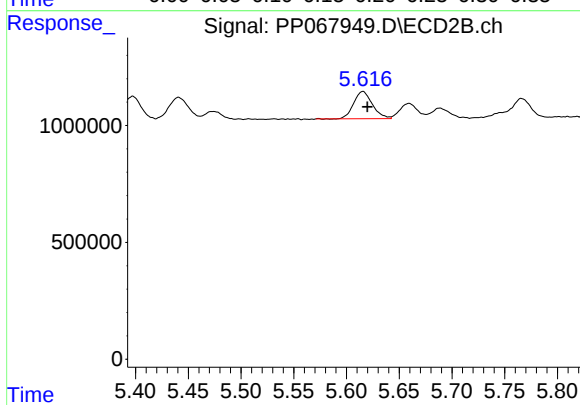

#15 AR-1232-5


R.T.: 5.616 min
Delta R.T.: -0.004 min
Response: 1438668
Conc: 106.96 ng/ml

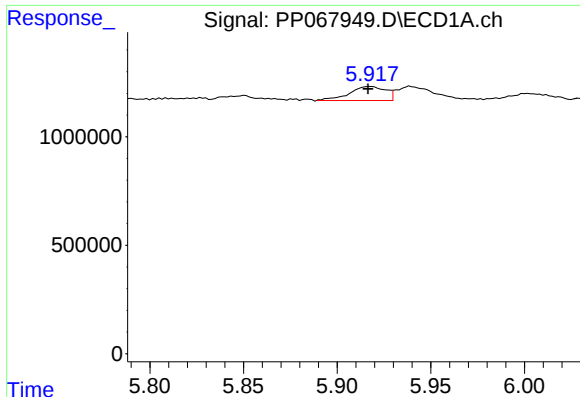

#16 AR-1242-1


R.T.: 5.918 min
Delta R.T.: 0.001 min
Response: 876198
Conc: 31.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

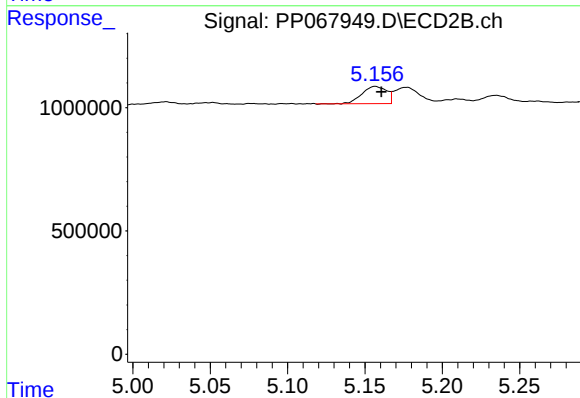


#16 AR-1242-1

R.T.: 5.157 min
Delta R.T.: -0.004 min
Response: 769817
Conc: 26.48 ng/ml

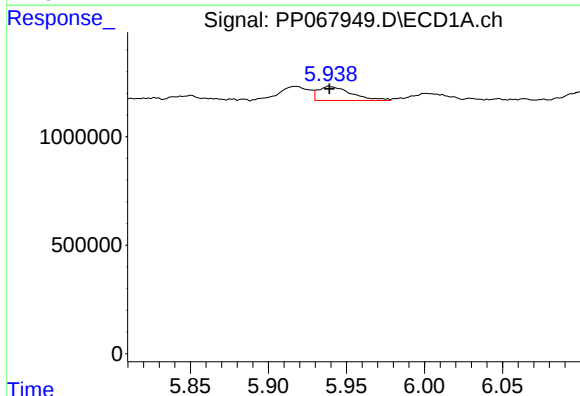


#17 AR-1242-2

R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 963471
Conc: 23.71 ng/ml

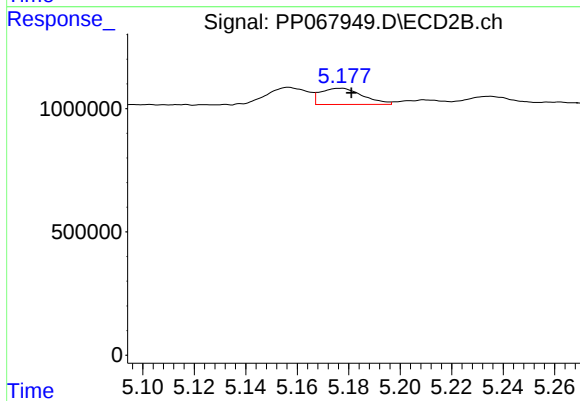

#17 AR-1242-2


R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 746070
Conc: 18.58 ng/ml

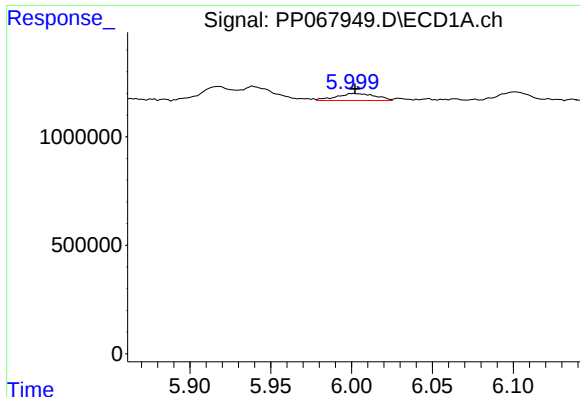

#18 AR-1242-3


R.T.: 6.001 min
Delta R.T.: 0.000 min
Response: 543779
Conc: 20.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

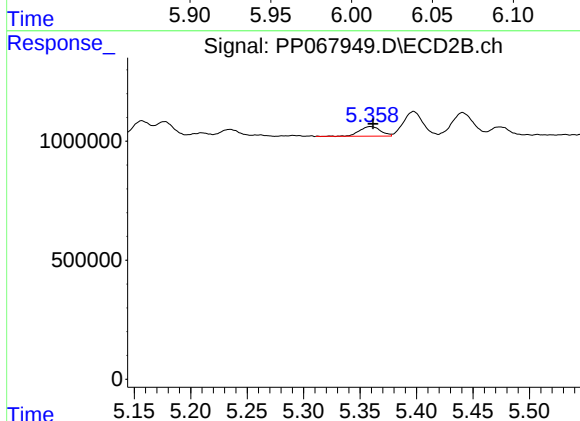


#18 AR-1242-3

R.T.: 5.359 min
Delta R.T.: -0.002 min
Response: 530502
Conc: 23.58 ng/ml

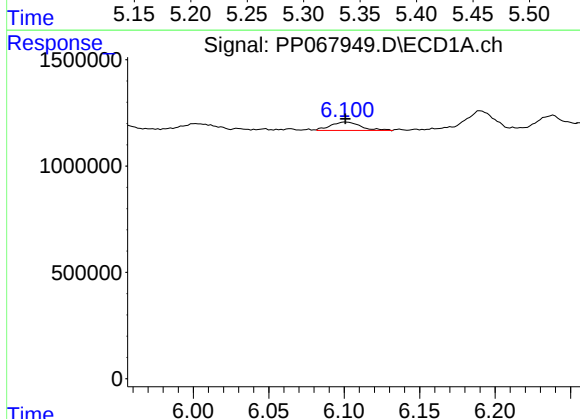


#19 AR-1242-4

R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 549628
Conc: 25.62 ng/ml

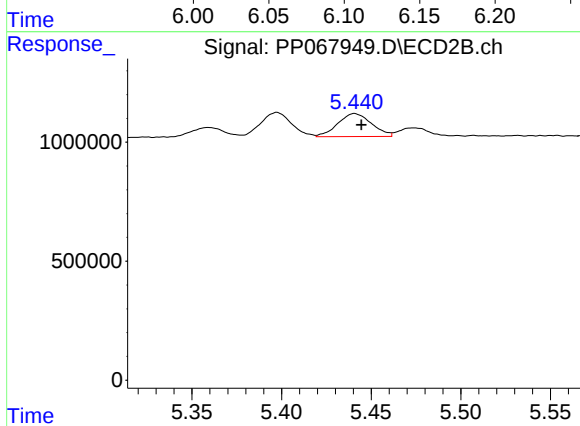

#19 AR-1242-4


R.T.: 5.441 min
Delta R.T.: -0.004 min
Response: 1270630
Conc: 53.53 ng/ml

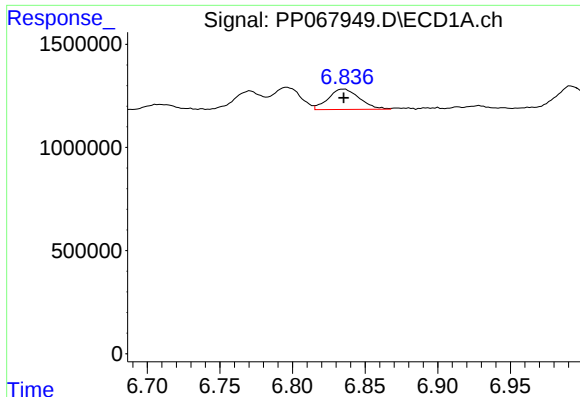

#20 AR-1242-5


R.T.: 6.835 min
Delta R.T.: 0.000 min
Response: 1475252
Conc: 61.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

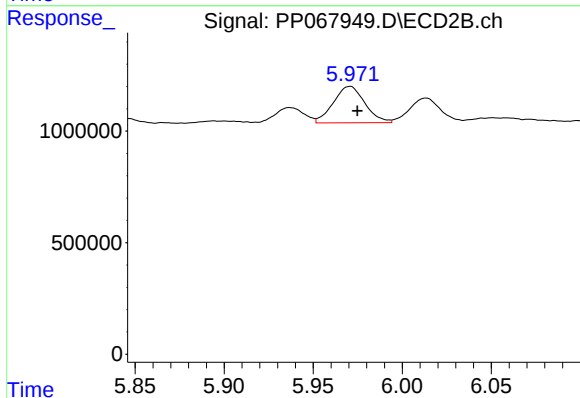


#20 AR-1242-5

R.T.: 5.971 min
Delta R.T.: -0.004 min
Response: 2006156
Conc: 70.02 ng/ml

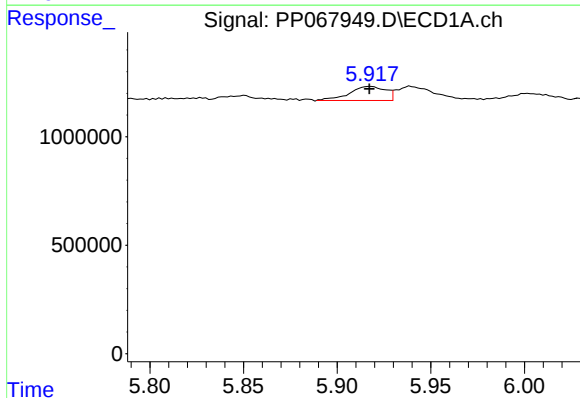


#21 AR-1248-1

R.T.: 5.918 min
Delta R.T.: 0.000 min
Response: 876198
Conc: 40.90 ng/ml

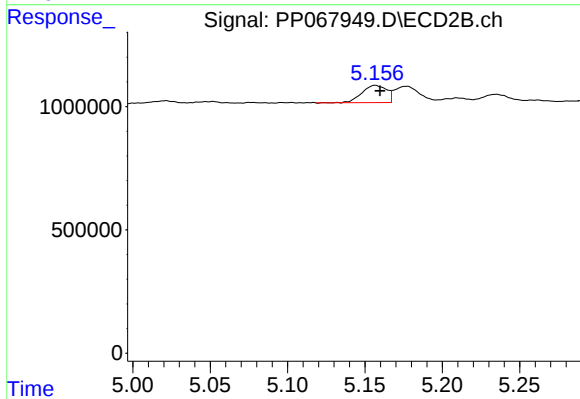

#21 AR-1248-1


R.T.: 5.157 min
Delta R.T.: -0.003 min
Response: 769817
Conc: 33.97 ng/ml

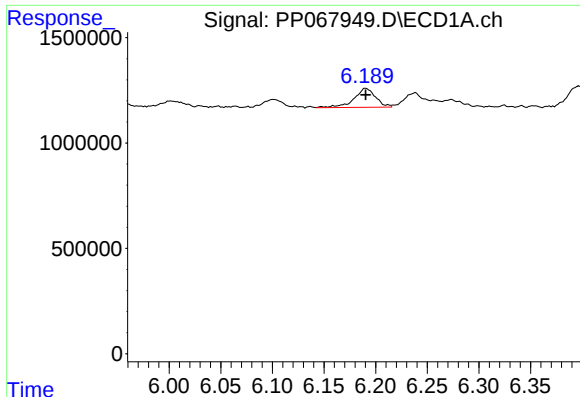

#22 AR-1248-2


R.T.: 6.190 min
Delta R.T.: 0.000 min
Response: 1297264
Conc: 38.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

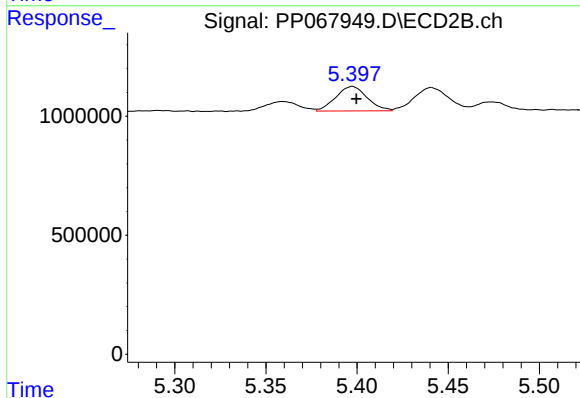


#22 AR-1248-2

R.T.: 5.397 min
Delta R.T.: -0.002 min
Response: 1231940
Conc: 37.22 ng/ml

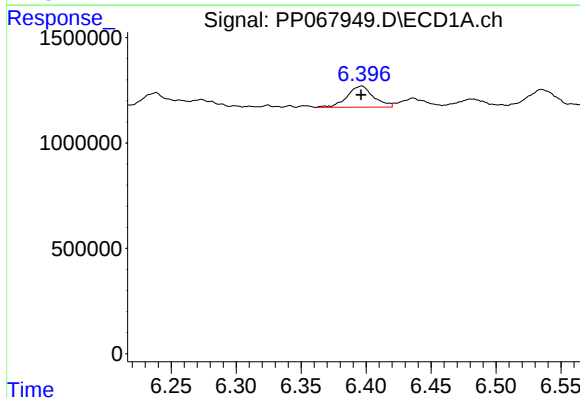


#23 AR-1248-3

R.T.: 6.397 min
Delta R.T.: 0.000 min
Response: 1407996
Conc: 38.44 ng/ml

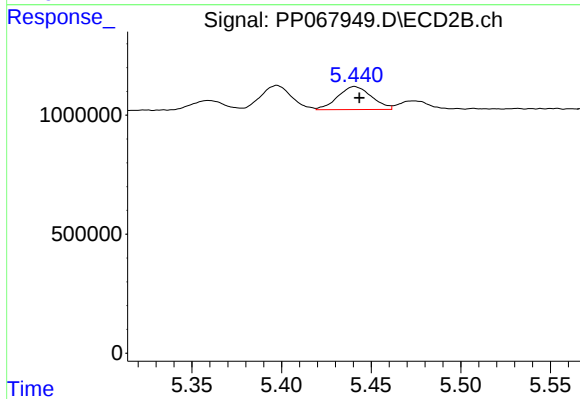

#23 AR-1248-3


R.T.: 5.441 min
Delta R.T.: -0.003 min
Response: 1270630
Conc: 36.86 ng/ml

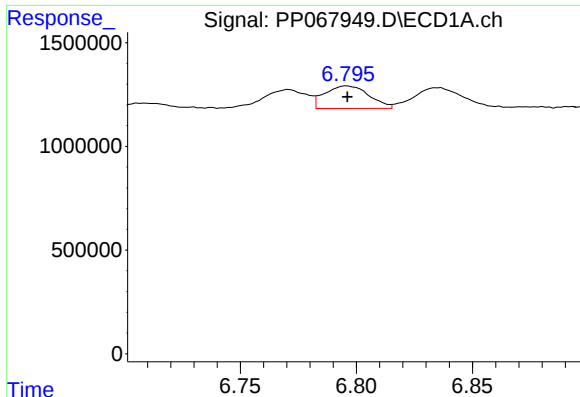

#24 AR-1248-4


R.T.: 6.796 min
Delta R.T.: 0.000 min
Response: 1450509
Conc: 35.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

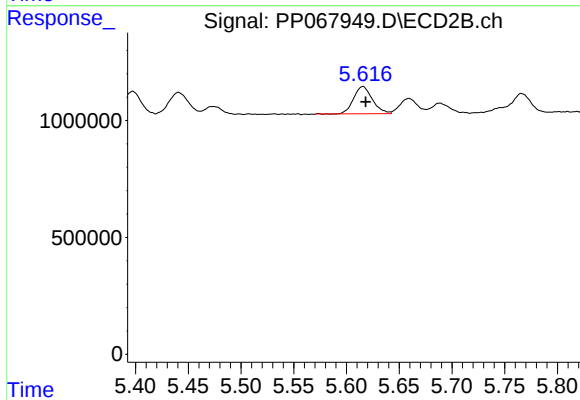


#24 AR-1248-4

R.T.: 5.616 min
Delta R.T.: -0.003 min
Response: 1438668
Conc: 35.13 ng/ml

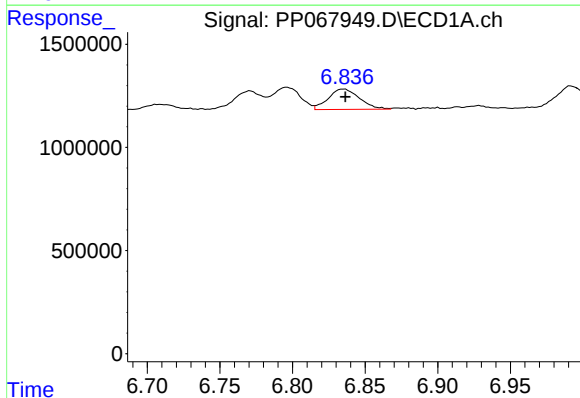


#25 AR-1248-5

R.T.: 6.835 min
Delta R.T.: 0.000 min
Response: 1475252
Conc: 37.20 ng/ml

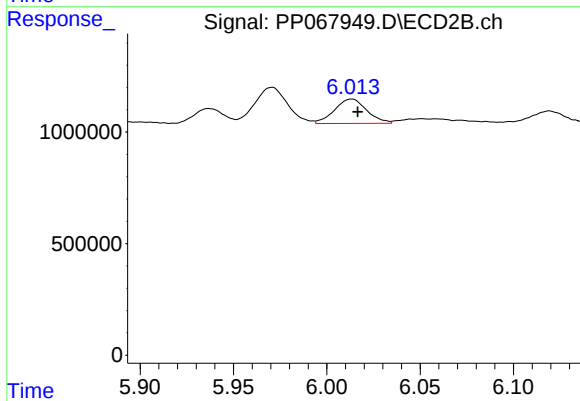

#25 AR-1248-5


R.T.: 6.013 min
Delta R.T.: -0.003 min
Response: 1316991
Conc: 35.17 ng/ml

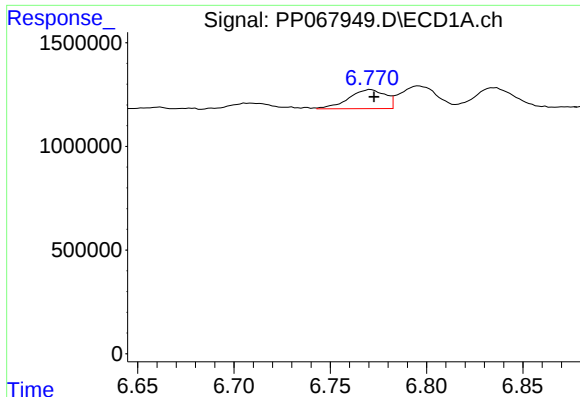

#26 AR-1254-1


R.T.: 6.771 min
Delta R.T.: -0.002 min
Response: 1226826
Conc: 27.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

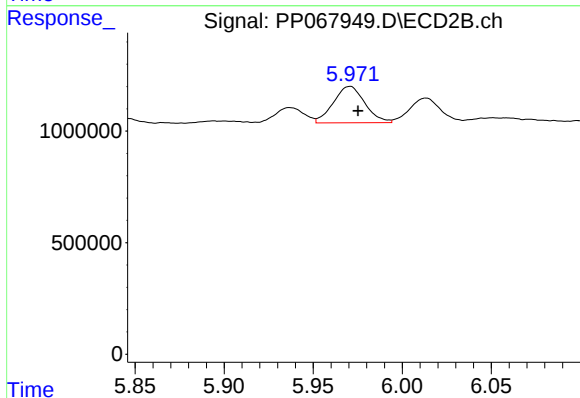


#26 AR-1254-1

R.T.: 5.971 min
Delta R.T.: -0.005 min
Response: 2006156
Conc: 33.95 ng/ml

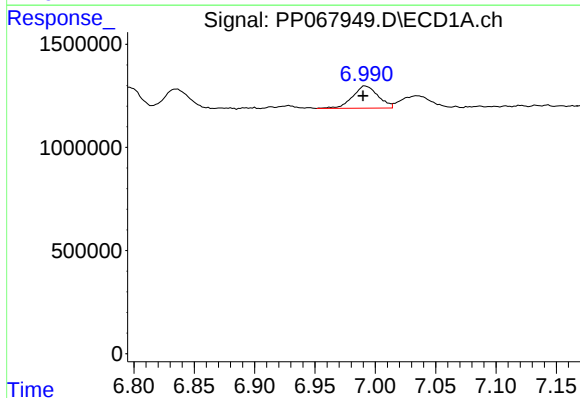


#27 AR-1254-2

R.T.: 6.992 min
Delta R.T.: 0.002 min
Response: 1579084
Conc: 23.89 ng/ml

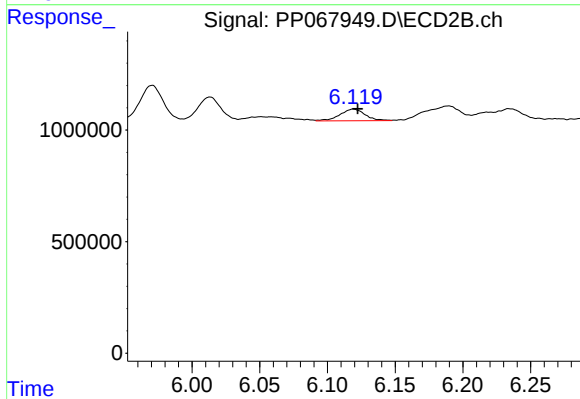

#27 AR-1254-2


R.T.: 6.119 min
Delta R.T.: -0.003 min
Response: 676923
Conc: 12.90 ng/ml

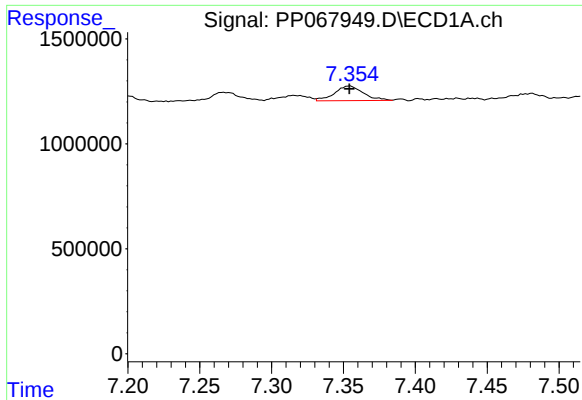

#28 AR-1254-3


R.T.: 7.354 min
Delta R.T.: 0.000 min
Response: 976905
Conc: 14.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

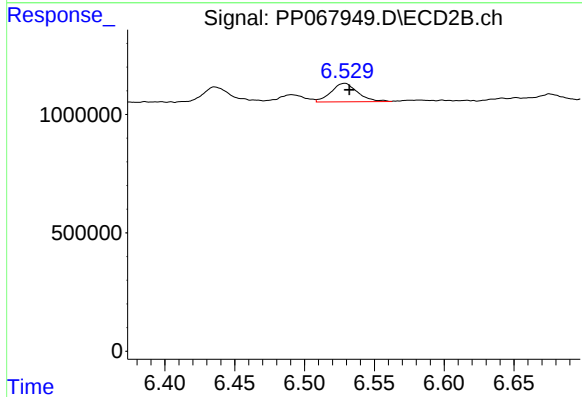


#28 AR-1254-3

R.T.: 6.529 min
Delta R.T.: -0.004 min
Response: 1034449
Conc: 12.43 ng/ml

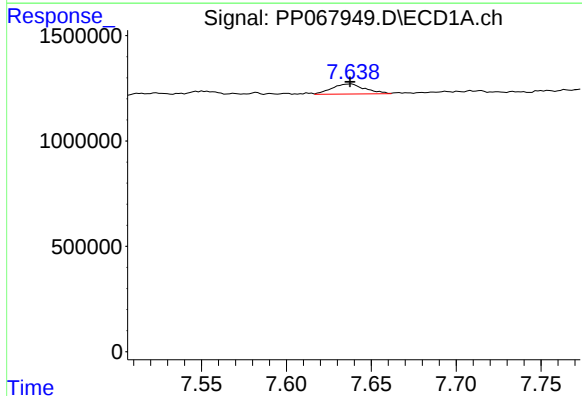


#29 AR-1254-4

R.T.: 7.638 min
Delta R.T.: 0.000 min
Response: 651877
Conc: 13.06 ng/ml

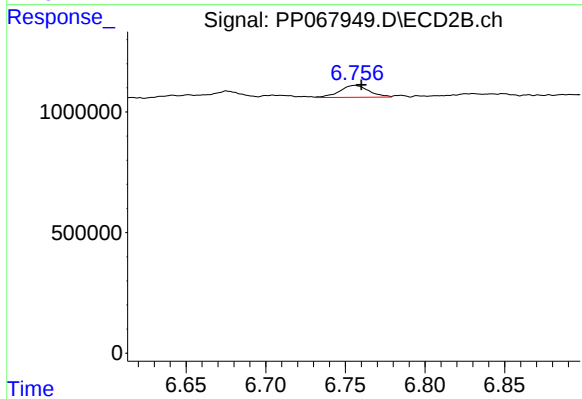

#29 AR-1254-4


R.T.: 6.756 min
Delta R.T.: -0.004 min
Response: 635743
Conc: 13.17 ng/ml

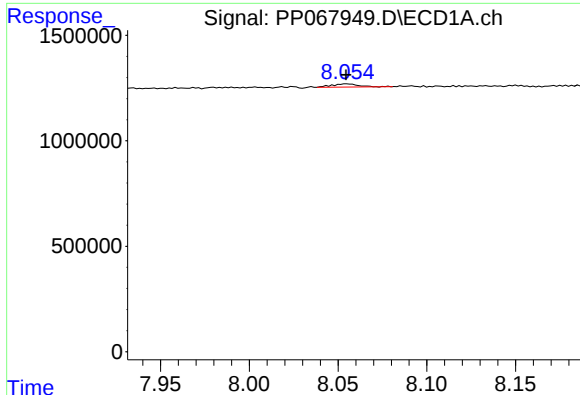

#30 AR-1254-5


R.T.: 8.055 min
Delta R.T.: 0.000 min
Response: 159442
Conc: 2.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

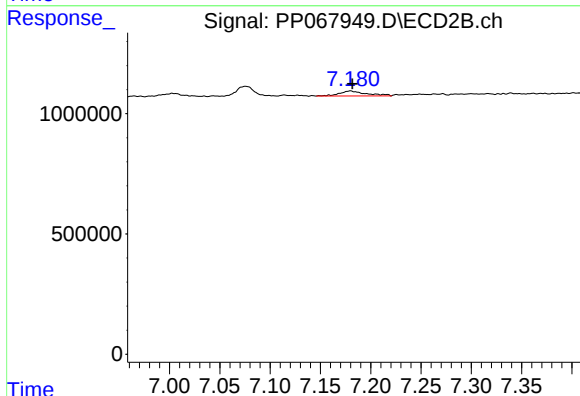


#30 AR-1254-5

R.T.: 7.180 min
Delta R.T.: -0.002 min
Response: 386732
Conc: 5.26 ng/ml

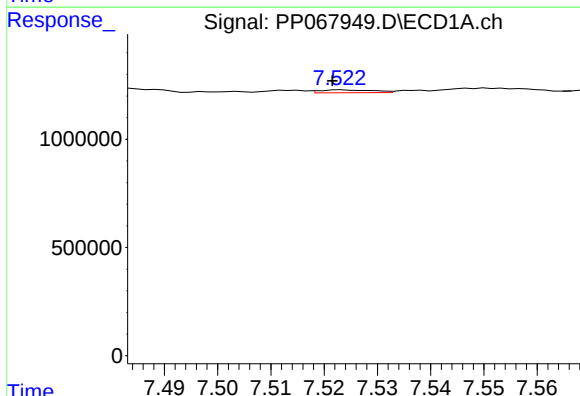


#31 AR-1260-1

R.T.: 7.523 min
Delta R.T.: 0.002 min
Response: 93043
Conc: 1.72 ng/ml

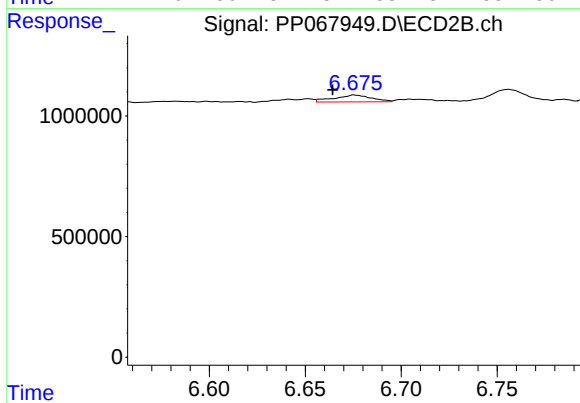

#31 AR-1260-1


R.T.: 6.676 min
Delta R.T.: 0.011 min
Response: 392587
Conc: 6.89 ng/ml

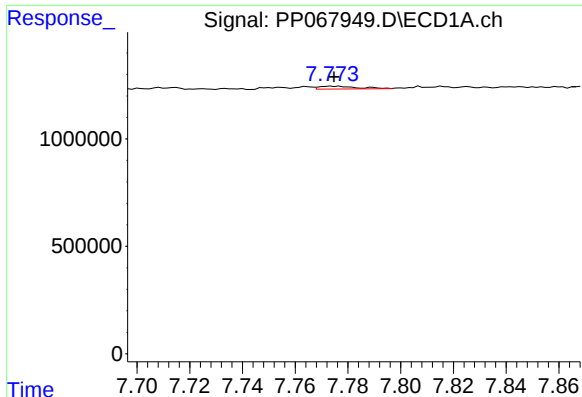

#32 AR-1260-2


R.T.: 7.774 min
Delta R.T.: 0.000 min
Response: 133878
Conc: 2.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

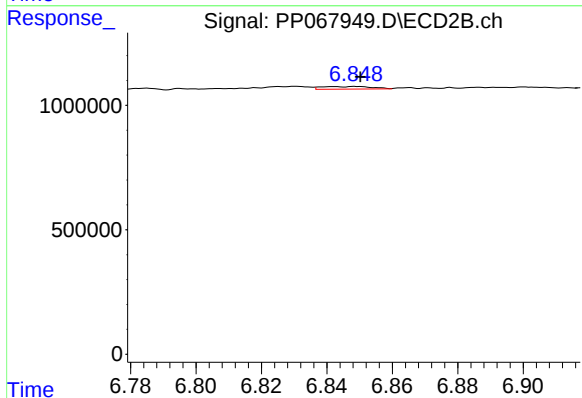


#32 AR-1260-2

R.T.: 6.849 min
Delta R.T.: -0.001 min
Response: 112600
Conc: 1.69 ng/ml

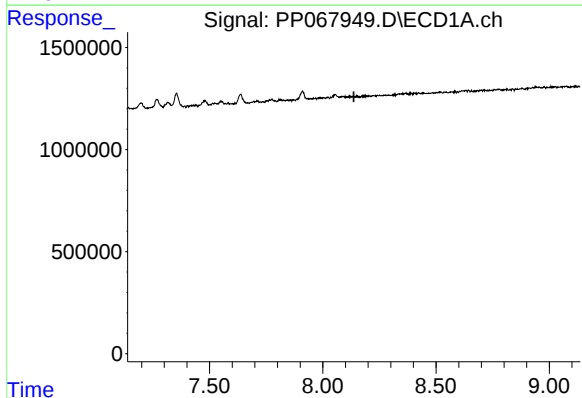


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.137 min
Response: 0
Conc: N.D.

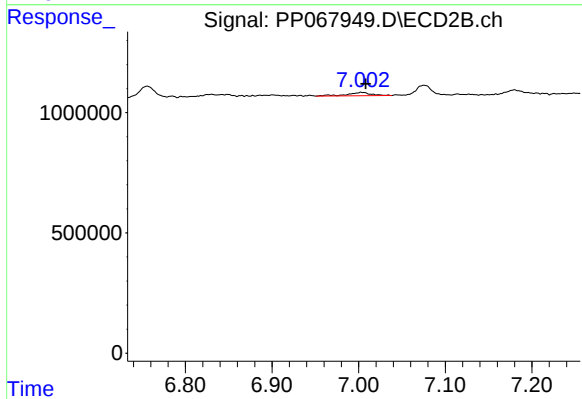

#33 AR-1260-3


R.T.: 7.003 min
Delta R.T.: -0.005 min
Response: 263938
Conc: 4.14 ng/ml

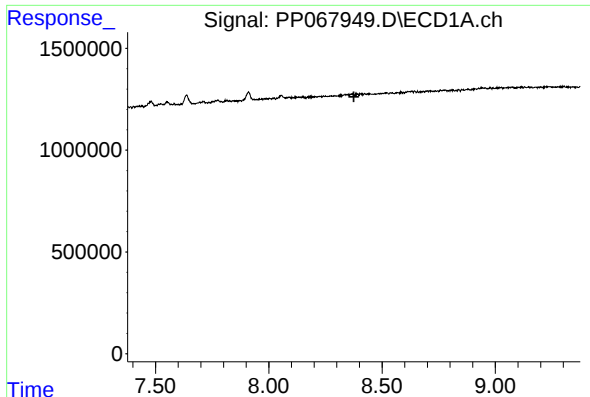

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

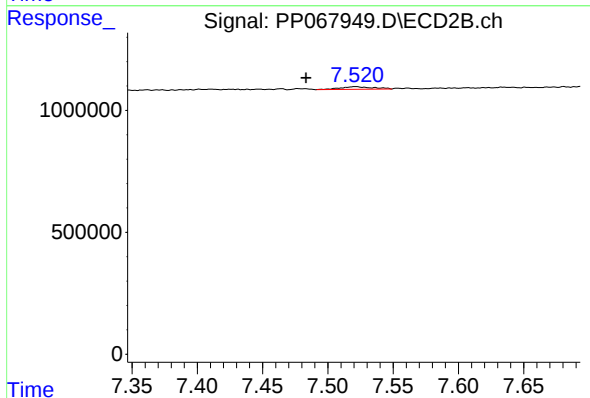


#34 AR-1260-4

R.T.: 7.521 min
Delta R.T.: 0.038 min
Response: 188636
Conc: 3.41 ng/ml

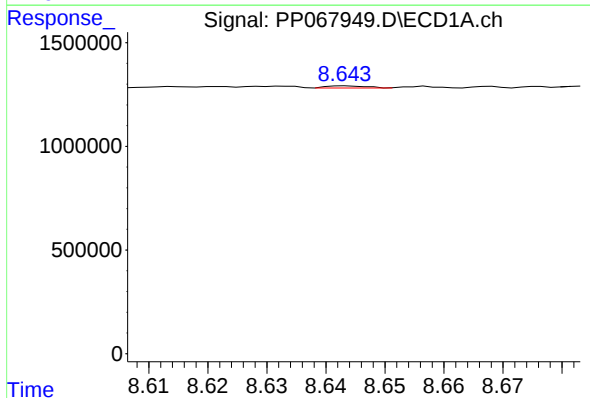


#35 AR-1260-5

R.T.: 8.643 min
Delta R.T.: -0.068 min
Response: 48428
Conc: 0.45 ng/ml

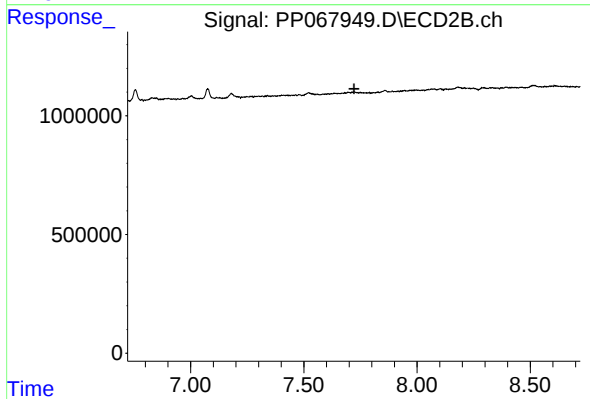

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 7.722 min
Response: 0
Conc: N.D.

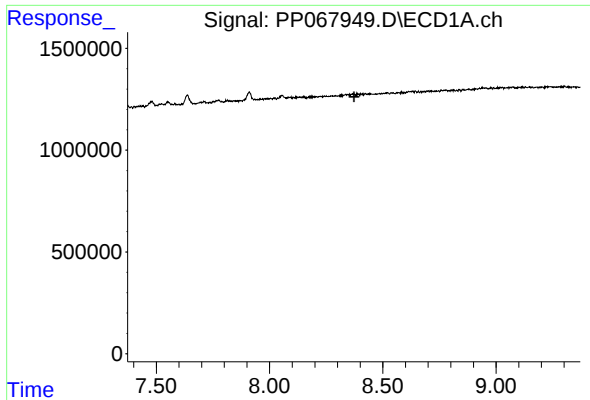

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 8.373 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

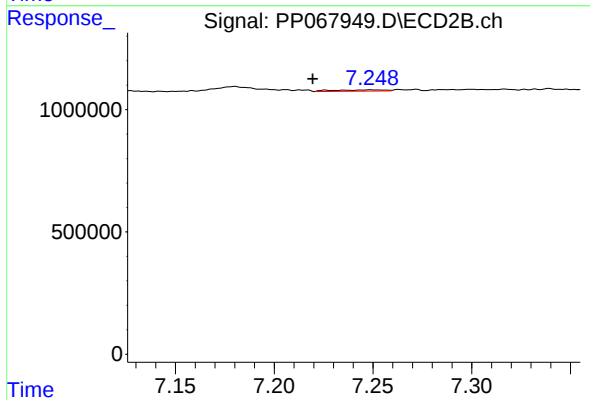


#36 AR-1262-1

R.T.: 7.249 min
Delta R.T.: 0.029 min
Response: 93031
Conc: 1.18 ng/ml

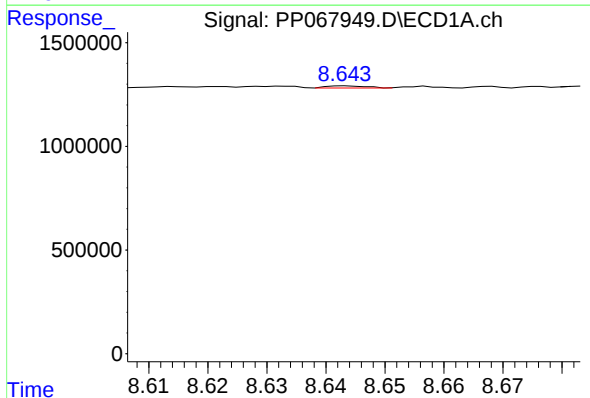


#37 AR-1262-2

R.T.: 8.643 min
Delta R.T.: -0.066 min
Response: 48428
Conc: 0.40 ng/ml

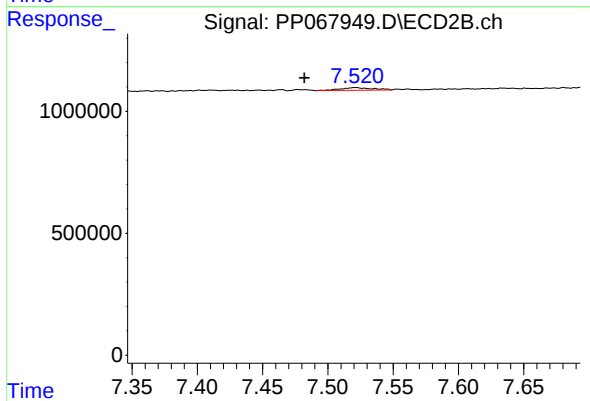

#37 AR-1262-2


R.T.: 7.521 min
Delta R.T.: 0.039 min
Response: 188636
Conc: 2.66 ng/ml

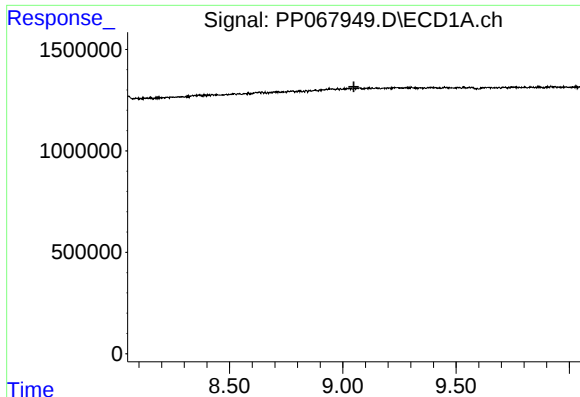

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

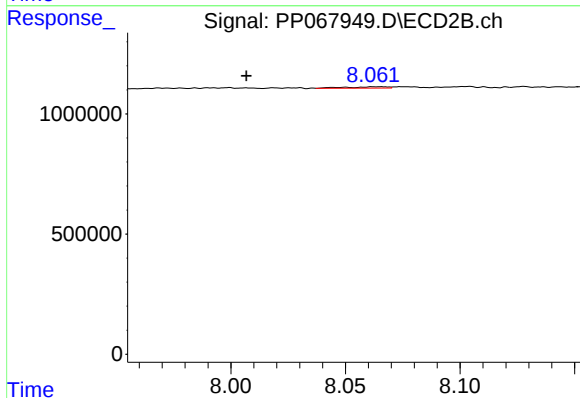


#38 AR-1262-3

R.T.: 8.066 min
Delta R.T.: 0.059 min
Response: 73191
Conc: 1.28 ng/ml

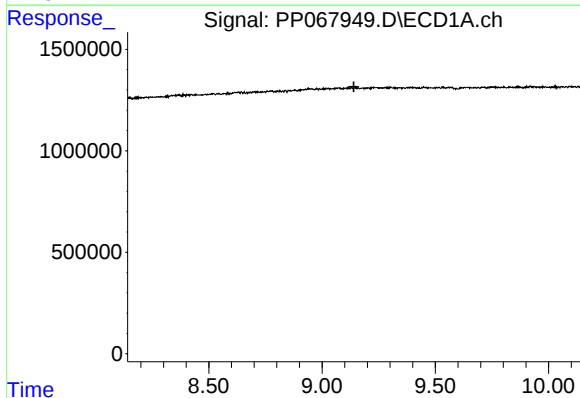


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 9.140 min
Response: 0
Conc: N.D.

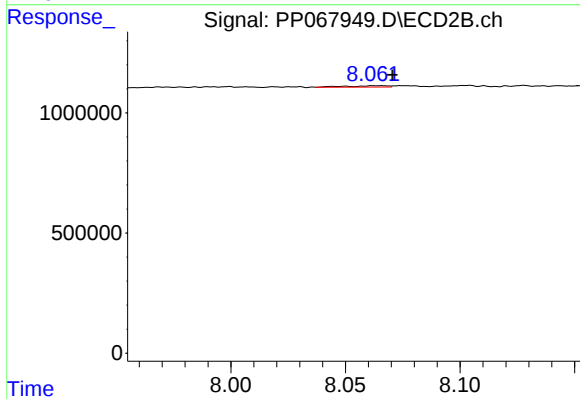

#39 AR-1262-4


R.T.: 8.066 min
Delta R.T.: -0.005 min
Response: 73191
Conc: 0.73 ng/ml

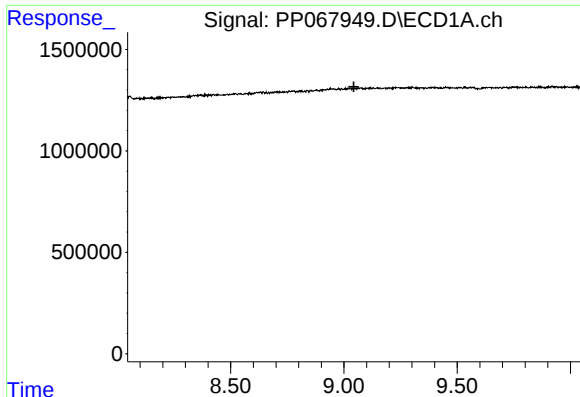

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 9.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

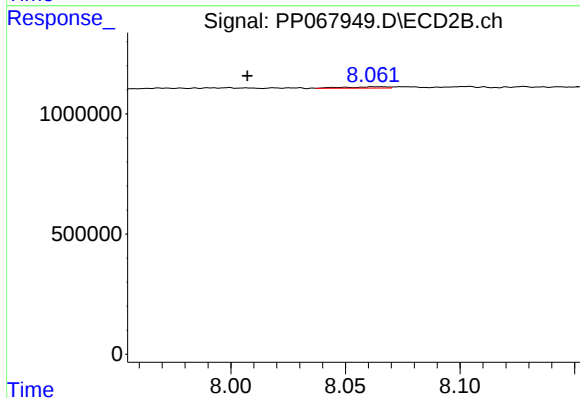


#41 AR-1268-1

R.T.: 8.066 min
Delta R.T.: 0.058 min
Response: 73191
Conc: 0.46 ng/ml

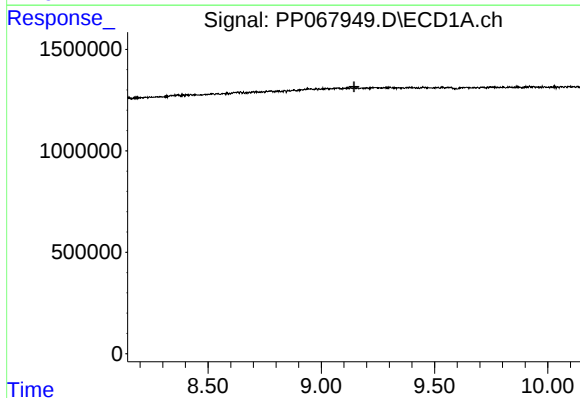


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 9.144 min
Response: 0
Conc: N.D.

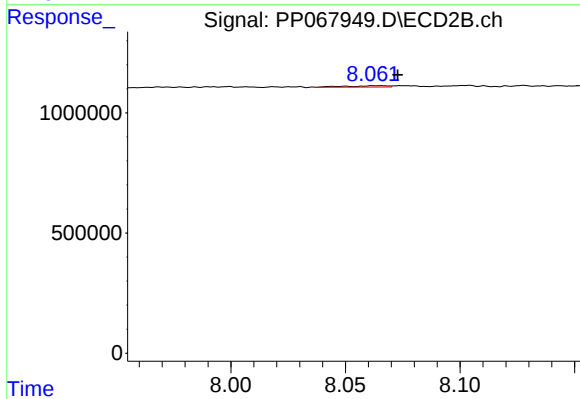

#42 AR-1268-2


R.T.: 8.066 min
Delta R.T.: -0.007 min
Response: 73191
Conc: 0.51 ng/ml

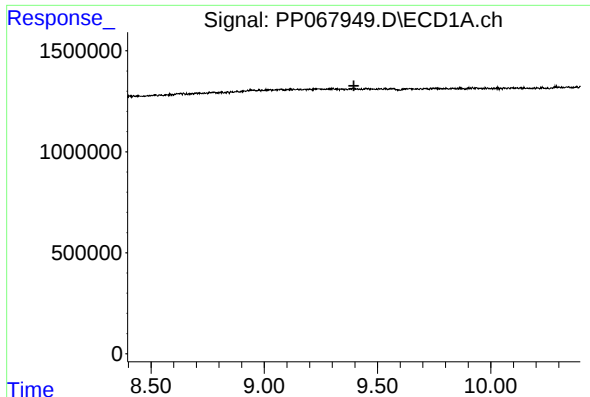

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

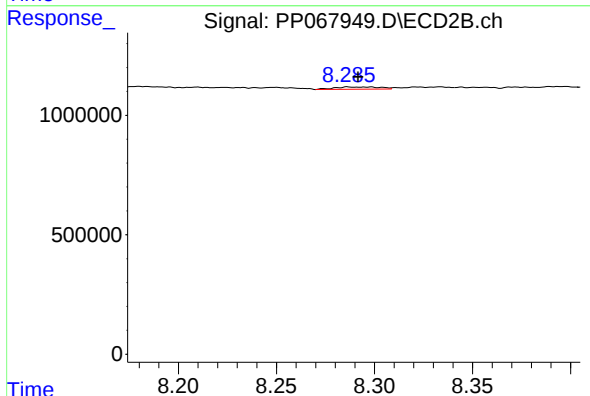


#43 AR-1268-3

R.T.: 8.298 min
Delta R.T.: 0.006 min
Response: 153825
Conc: 1.21 ng/ml

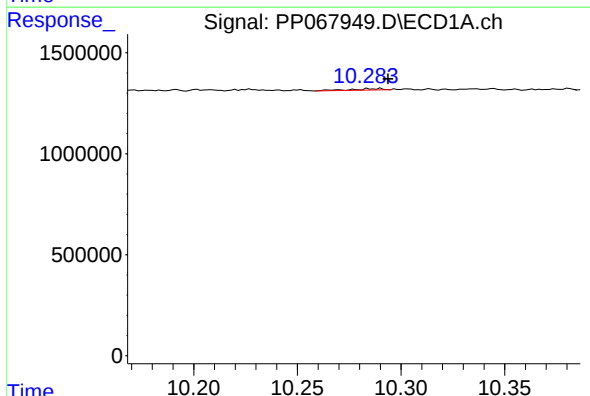

#45 AR-1268-5

R.T.: 10.290 min
Delta R.T.: -0.004 min
Response: 72457
Conc: 0.19 ng/ml

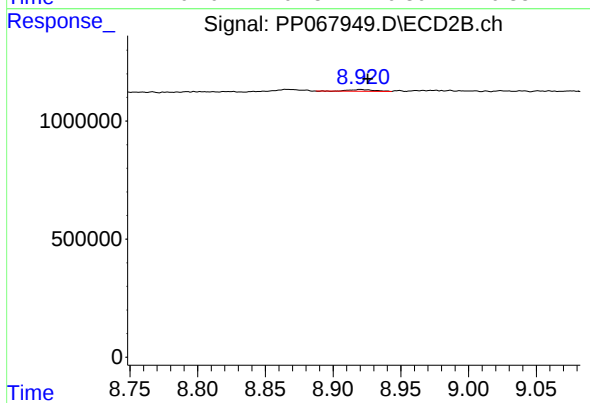

#45 AR-1268-5

R.T.: 8.920 min
Delta R.T.: -0.005 min
Response: 91819
Conc: 0.24 ng/ml