

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
 Data File : PP067951.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2024 01:50
 Operator : YP\AJ
 Sample : P4368-07
 Misc : AR1262 LOD 40 PPB
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 07:31:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.752	4.050	14375520	15213365	15.530	15.057
2)	SA Decachlor...	10.662	9.209	20440791	18603707	17.754	16.589
Target Compounds							
3)	L1 AR-1016-1	0.000	5.178	0	144738	N.D.	4.137 #
4)	L1 AR-1016-2	0.000	5.178	0	144738	N.D.	3.005 #
5)	L1 AR-1016-3	0.000	5.399f	0	98297	N.D.	3.649 #
6)	L1 AR-1016-4	0.000	5.399	0	98297	N.D.	4.081 #
7)	L1 AR-1016-5	6.394	5.614	78662	112302	2.906	3.693 #
9)	L2 AR-1221-2	5.061	4.359	269453	226309	28.482	22.719
10)	L2 AR-1221-3	5.061f	0.000	269453	0	9.321	N.D. #
11)	L3 AR-1232-1	5.061f	0.000	269453	0	11.787	N.D. #
12)	L3 AR-1232-2	0.000	5.178	0	144738	N.D.	6.472 #
13)	L3 AR-1232-3	0.000	5.399f	0	98297	N.D.	8.230 #
14)	L3 AR-1232-4	0.000	5.399f	0	98297	N.D.	8.524 #
15)	L3 AR-1232-5	0.000	5.614	0	112302	N.D.	8.349 #
16)	L4 AR-1242-1	0.000	5.178	0	144738	N.D.	4.978 #
17)	L4 AR-1242-2	0.000	5.178	0	144738	N.D.	3.605 #
18)	L4 AR-1242-3	0.000	5.399f	0	98297	N.D.	4.370 #
19)	L4 AR-1242-4	0.000	5.399f	0	98297	N.D.	4.141 #
20)	L4 AR-1242-5	6.774f	5.973	592915	640154	24.576	22.344
21)	L5 AR-1248-1	0.000	5.178	0	144738	N.D.	6.386 #
22)	L5 AR-1248-2	0.000	5.399	0	98297	N.D.	2.970 #
23)	L5 AR-1248-3	6.394	5.399f	78662	98297	2.148	2.851 #
24)	L5 AR-1248-4	6.774	5.614	592915	112302	14.658	2.742 #
25)	L5 AR-1248-5	6.774f	6.015	592915	63735	14.950	1.702 #
26)	L6 AR-1254-1	6.774	5.973	592915	640154	13.240	10.835
27)	L6 AR-1254-2	6.988	6.119	903530	661384	13.670	12.606
28)	L6 AR-1254-3	7.353	6.543	718917	2120221	10.351	25.481 #
29)	L6 AR-1254-4	7.635	6.756	637987	408761	12.784	8.467 #
30)	L6 AR-1254-5	8.051	7.177	2323646	1914149	39.189	26.025 #
31)	L7 AR-1260-1	7.518	6.659	1804861	1974351	33.409	34.661
32)	L7 AR-1260-2	7.770	6.846	2211900	2216520	34.959	33.229
33)	L7 AR-1260-3	8.132	7.006	2699156	2158869	52.058	33.891 #
34)	L7 AR-1260-4	8.370	7.478	2518675	2498396	41.842	45.185
35)	L7 AR-1260-5	8.706	7.716	4417697	4787916	41.014	39.149
36)	L8 AR-1262-1	8.370	7.215	2518675	2828355	35.093	35.951
37)	L8 AR-1262-2	8.706	7.478	4417697	2498396	36.336	35.208
38)	L8 AR-1262-3	9.045	8.002	3090479	2026646	34.915	35.493
39)	L8 AR-1262-4	9.136	8.067	2323741	3576279	33.222	35.607
40)	L8 AR-1262-5	9.839	8.593	1525854	1731720	32.610	34.622
41)	L9 AR-1268-1	9.045	8.002	3090479	2026646	20.246	12.735 #
42)	L9 AR-1268-2	9.136	8.067	2323741	3576279	17.012	24.976 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
Data File : PP067951.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 01:50
Operator : YP\AJ
Sample : P4368-07
Misc : AR1262 LOD 40 PPB
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:31:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	8.287	0	206695	N.D.	1.621 #
44) L9	AR-1268-4	9.839	8.593	1525854	1731720	30.025	30.663
45) L9	AR-1268-5	10.286	8.920	801777	659351	2.147	1.744



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
Data File : PP067951.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 01:50
Operator : YP\AJ
Sample : P4368-07
Misc : AR1262 LOD 40 PPB
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:31:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

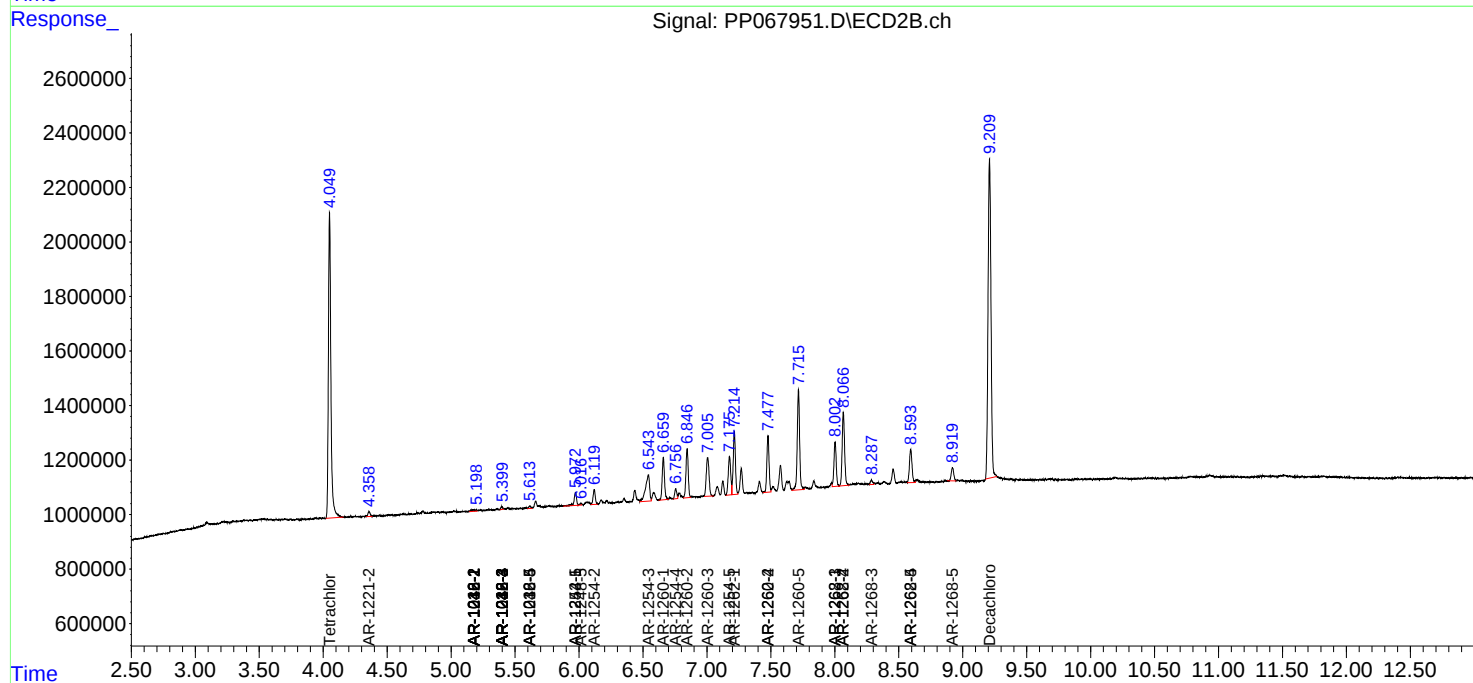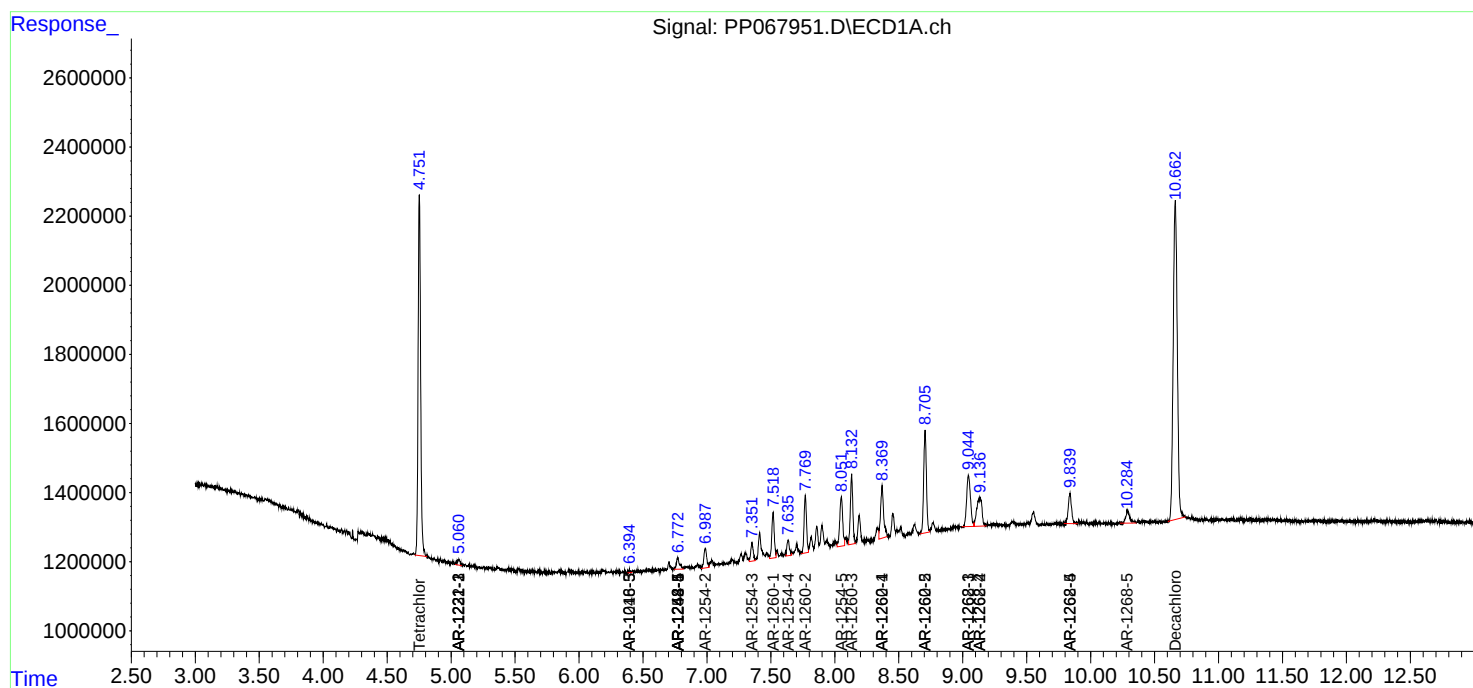


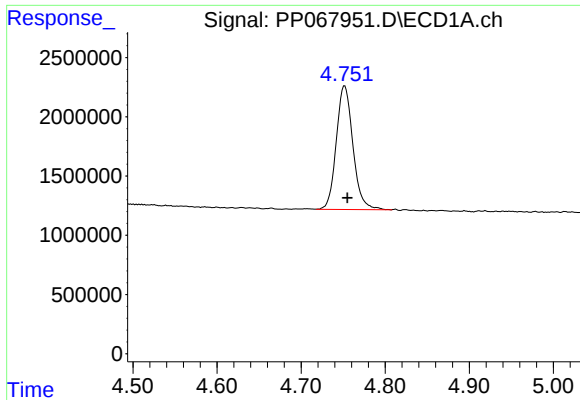

#1 Tetrachloro-m-xylene


R.T.: 4.752 min
Delta R.T.: -0.003 min
Response: 14375520
Conc: 15.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

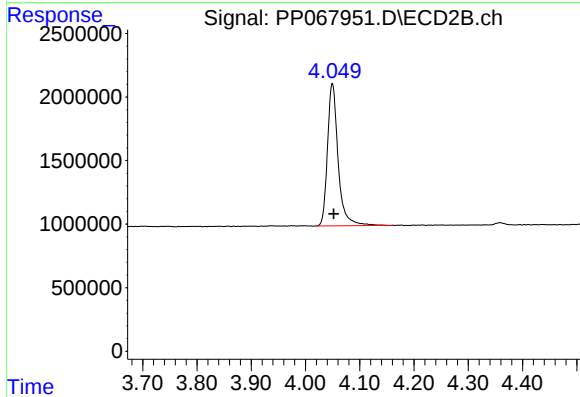


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 15213365
Conc: 15.06 ng/ml

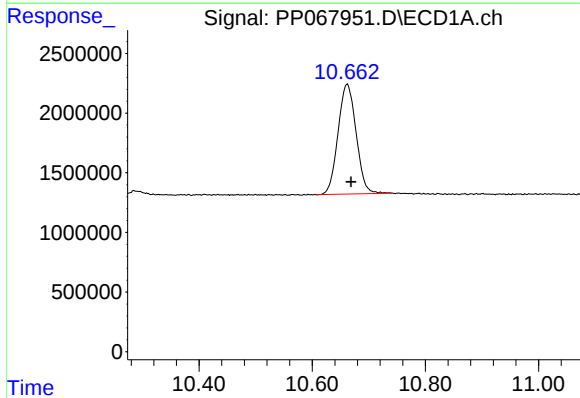


#2 Decachlorobiphenyl

R.T.: 10.662 min
Delta R.T.: -0.007 min
Response: 20440791
Conc: 17.75 ng/ml

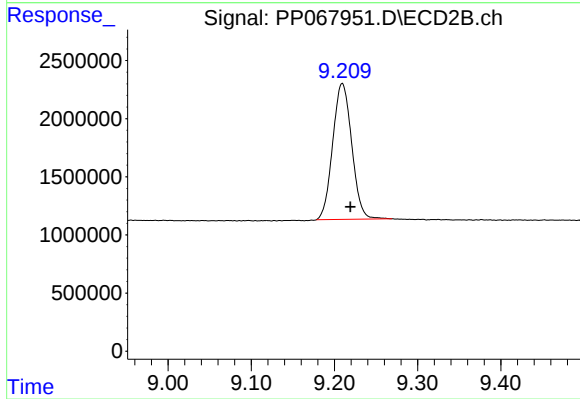

#2 Decachlorobiphenyl


R.T.: 9.209 min
Delta R.T.: -0.010 min
Response: 18603707
Conc: 16.59 ng/ml

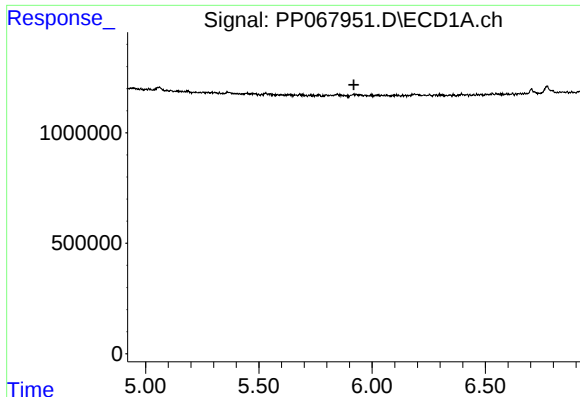

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.919 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

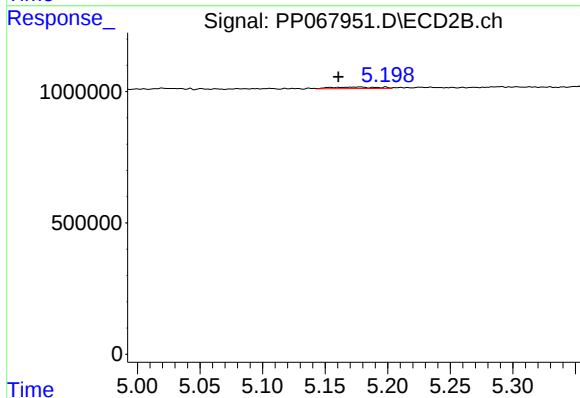


#3 AR-1016-1

R.T.: 5.178 min
Delta R.T.: 0.018 min
Response: 144738
Conc: 4.14 ng/ml

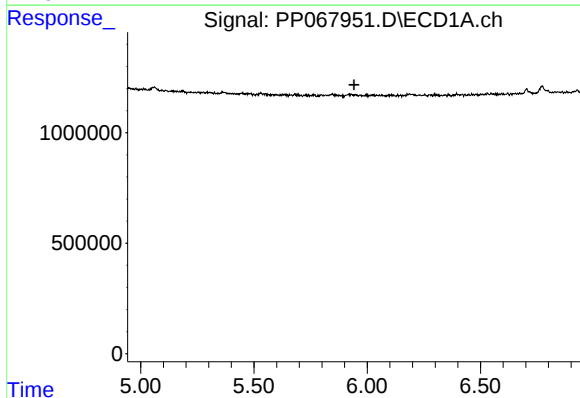


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.942 min
Response: 0
Conc: N.D.

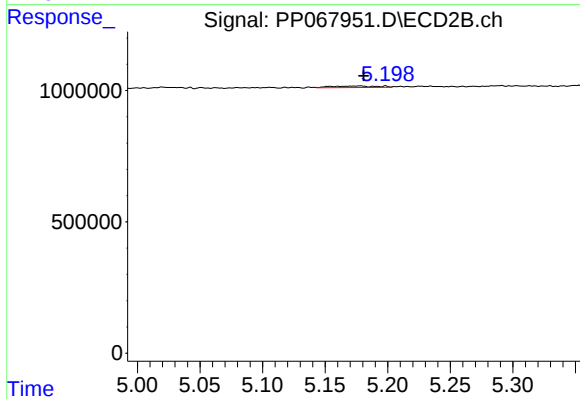

#4 AR-1016-2


R.T.: 5.178 min
Delta R.T.: -0.003 min
Response: 144738
Conc: 3.00 ng/ml

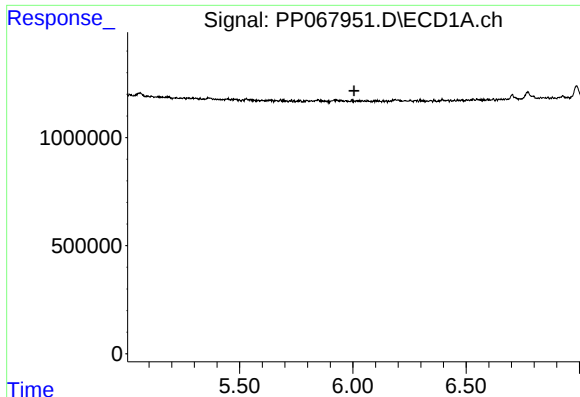

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 6.005 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

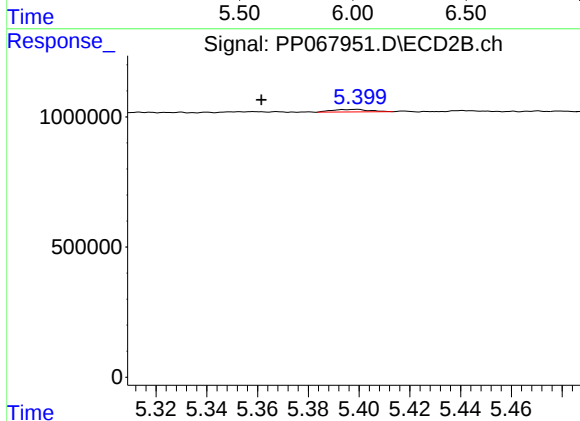


#5 AR-1016-3

R.T.: 5.399 min
Delta R.T.: 0.037 min
Response: 98297
Conc: 3.65 ng/ml

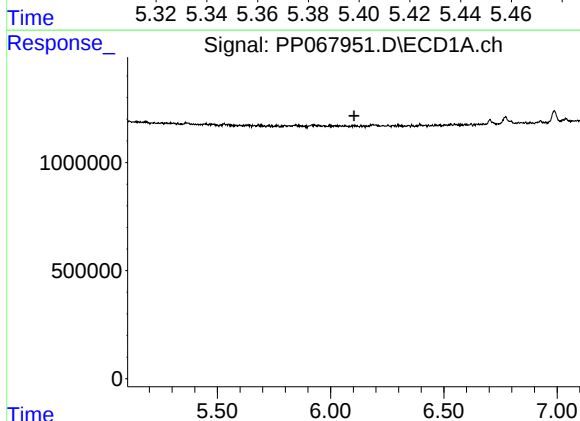


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 6.103 min
Response: 0
Conc: N.D.

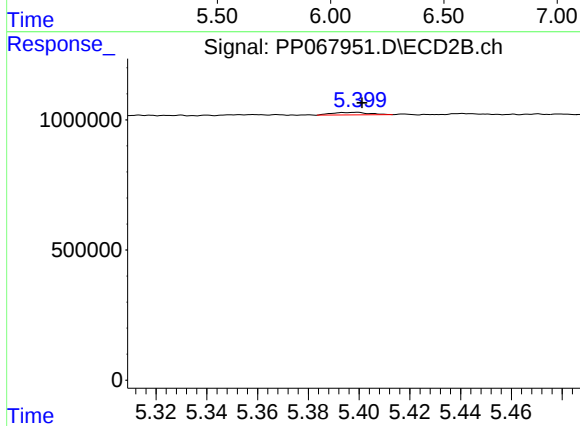

#6 AR-1016-4


R.T.: 5.399 min
Delta R.T.: -0.002 min
Response: 98297
Conc: 4.08 ng/ml

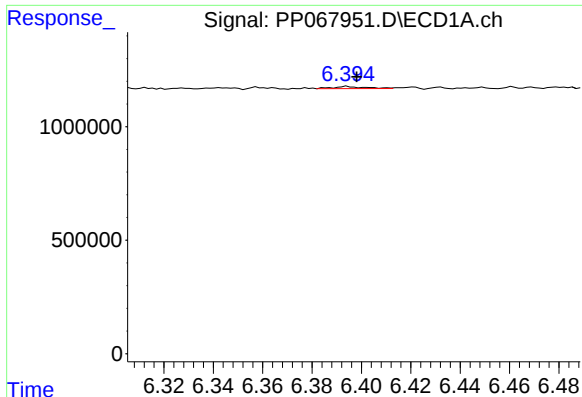

#7 AR-1016-5


R.T.: 6.394 min
Delta R.T.: -0.004 min
Response: 78662
Conc: 2.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

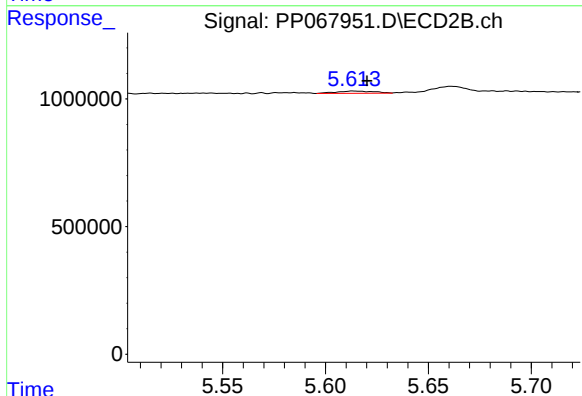


#7 AR-1016-5

R.T.: 5.614 min
Delta R.T.: -0.006 min
Response: 112302
Conc: 3.69 ng/ml

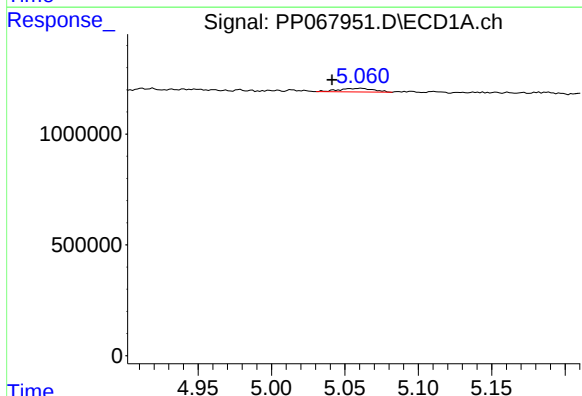


#9 AR-1221-2

R.T.: 5.061 min
Delta R.T.: 0.020 min
Response: 269453
Conc: 28.48 ng/ml

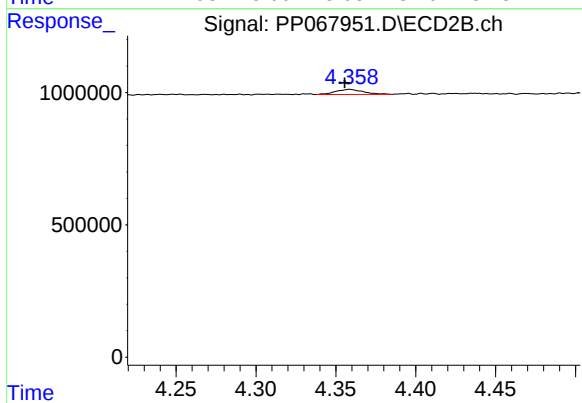

#9 AR-1221-2


R.T.: 4.359 min
Delta R.T.: 0.003 min
Response: 226309
Conc: 22.72 ng/ml

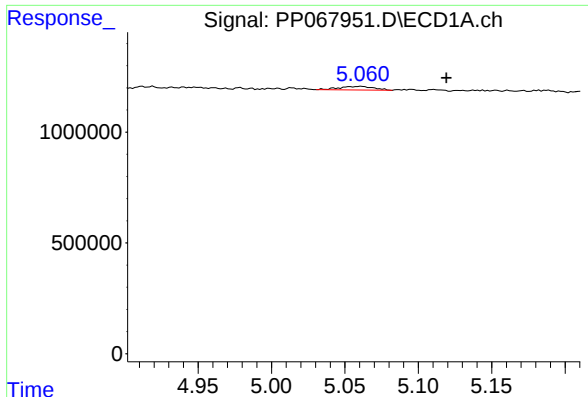

#10 AR-1221-3


R.T.: 5.061 min
Delta R.T.: -0.058 min
Response: 269453
Conc: 9.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

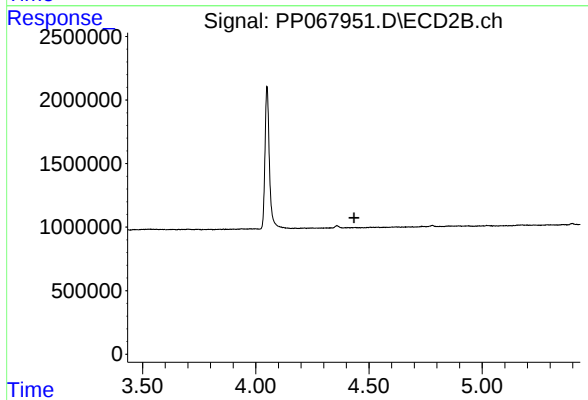


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.434 min
Response: 0
Conc: N.D.

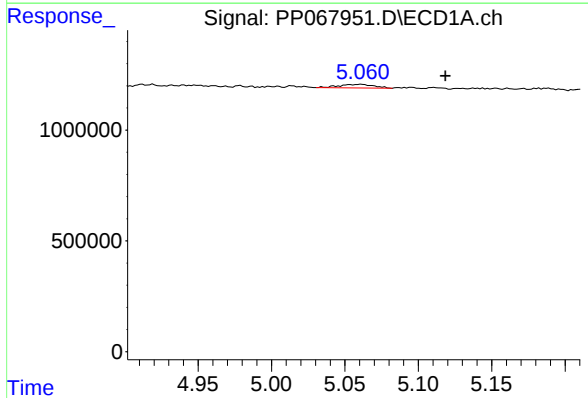


#11 AR-1232-1

R.T.: 5.061 min
Delta R.T.: -0.057 min
Response: 269453
Conc: 11.79 ng/ml

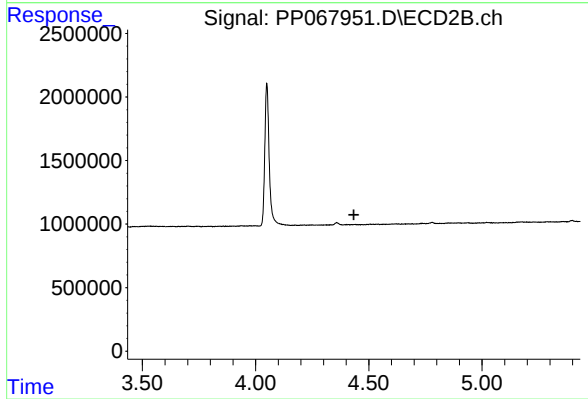

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.434 min
Response: 0
Conc: N.D.

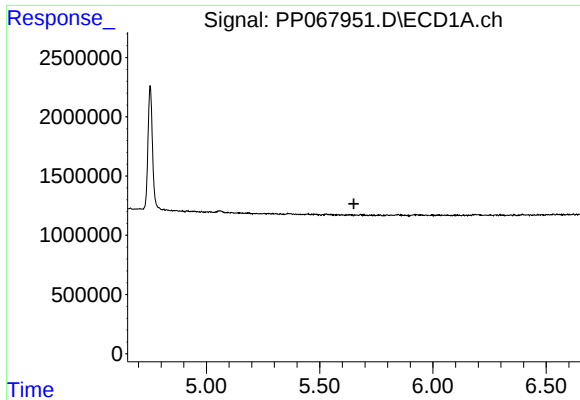

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 5.651 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

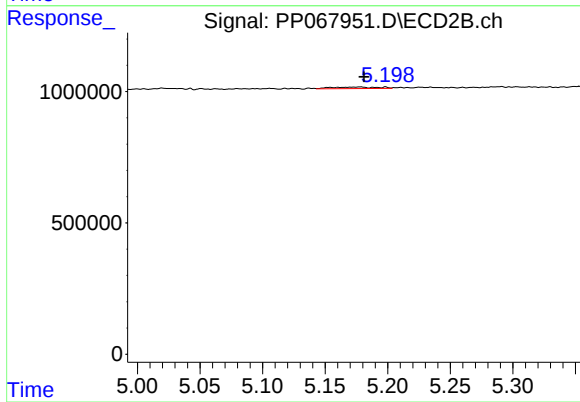


#12 AR-1232-2

R.T.: 5.178 min
Delta R.T.: -0.003 min
Response: 144738
Conc: 6.47 ng/ml

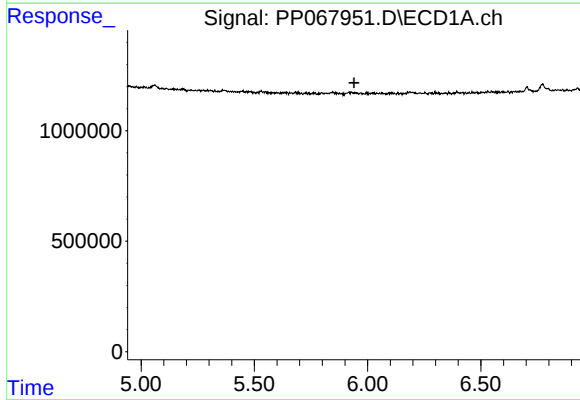


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T.: 5.940 min
Response: 0
Conc: N.D.

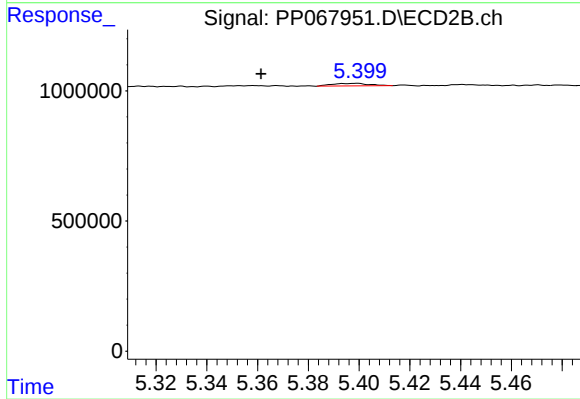

#13 AR-1232-3


R.T.: 5.399 min
Delta R.T.: 0.038 min
Response: 98297
Conc: 8.23 ng/ml

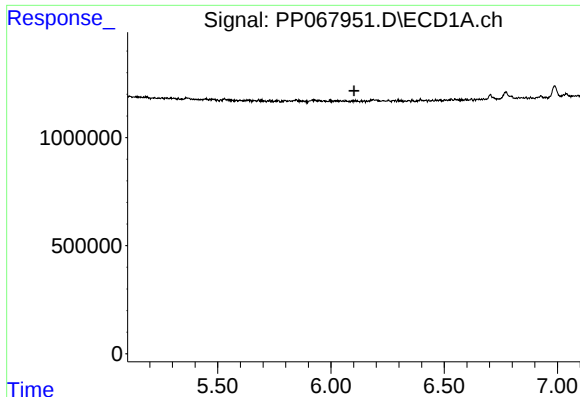

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T.: 6.101 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

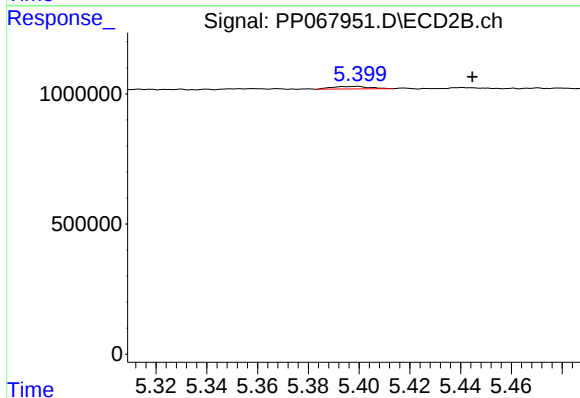


#14 AR-1232-4

R.T.: 5.399 min
Delta R.T.: -0.046 min
Response: 98297
Conc: 8.52 ng/ml

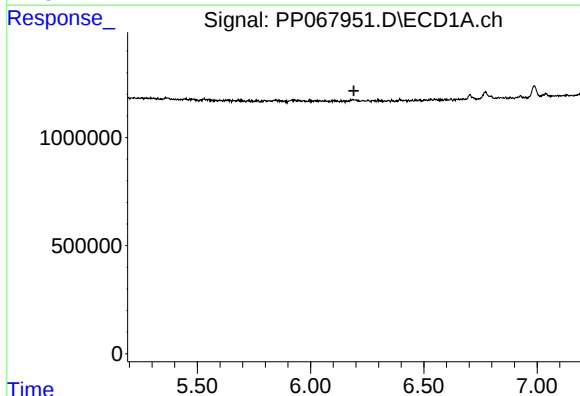


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

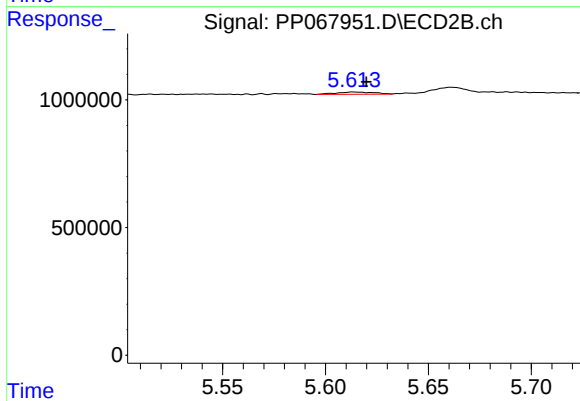

#15 AR-1232-5


R.T.: 5.614 min
Delta R.T.: -0.006 min
Response: 112302
Conc: 8.35 ng/ml

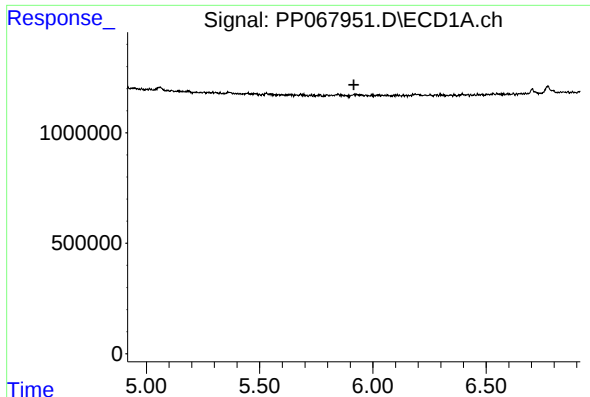

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T.: 5.916 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

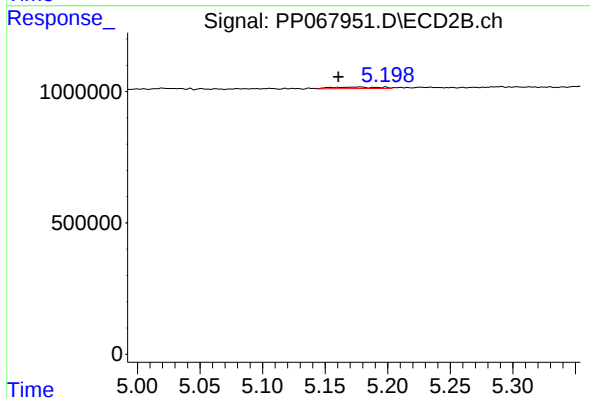


#16 AR-1242-1

R.T.: 5.178 min
Delta R.T.: 0.018 min
Response: 144738
Conc: 4.98 ng/ml

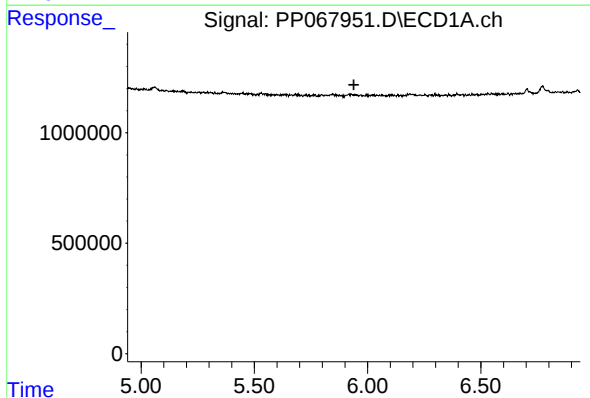


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T.: 5.939 min
Response: 0
Conc: N.D.

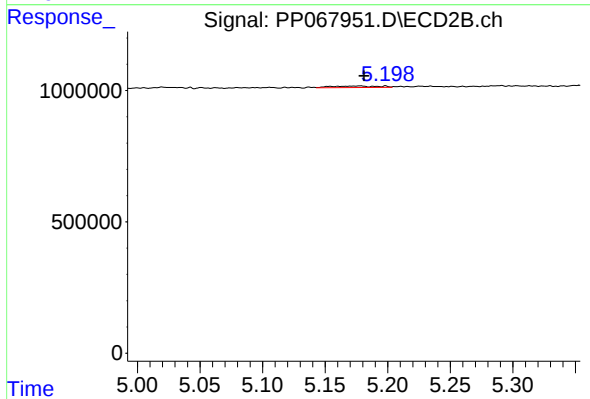

#17 AR-1242-2


R.T.: 5.178 min
Delta R.T.: -0.003 min
Response: 144738
Conc: 3.61 ng/ml

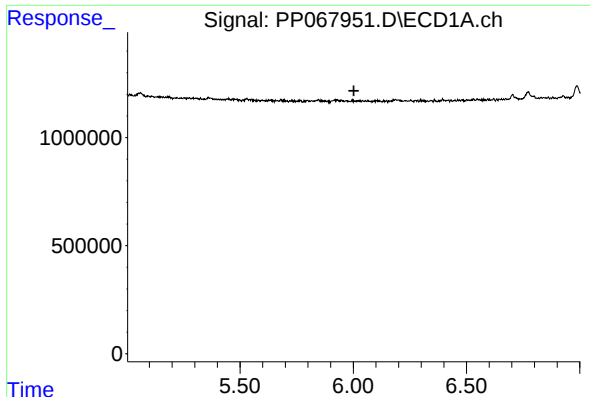

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 6.002 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

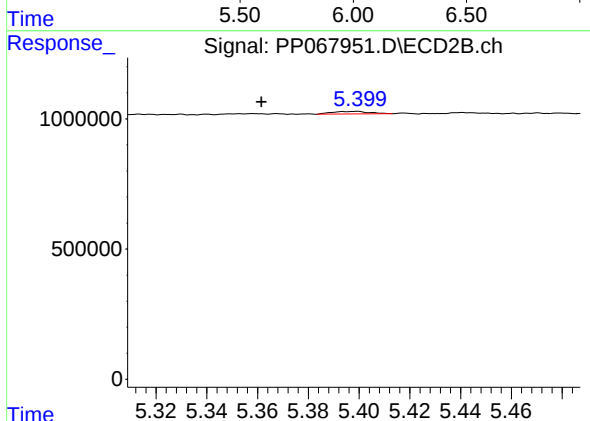


#18 AR-1242-3

R.T.: 5.399 min
Delta R.T.: 0.037 min
Response: 98297
Conc: 4.37 ng/ml

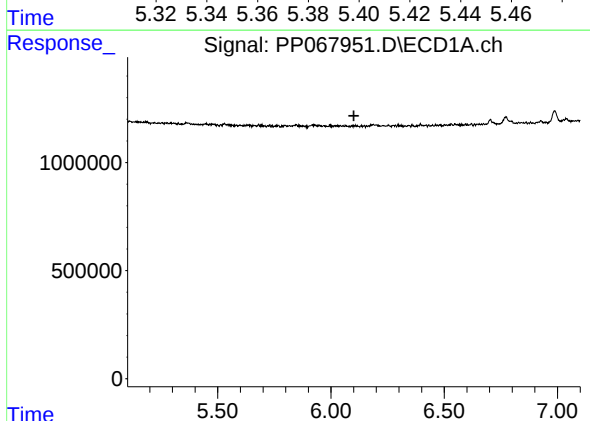


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T.: 6.101 min
Response: 0
Conc: N.D.

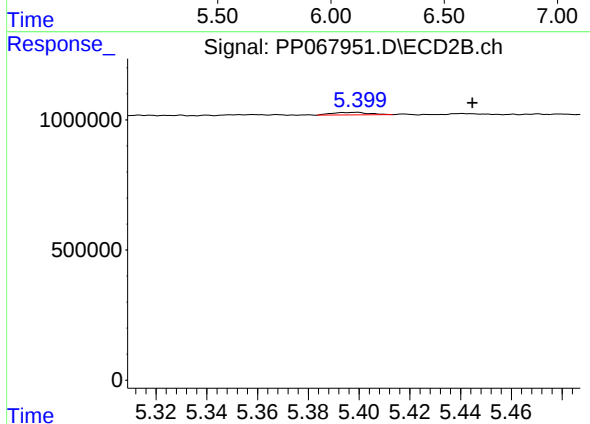

#19 AR-1242-4


R.T.: 5.399 min
Delta R.T.: -0.046 min
Response: 98297
Conc: 4.14 ng/ml

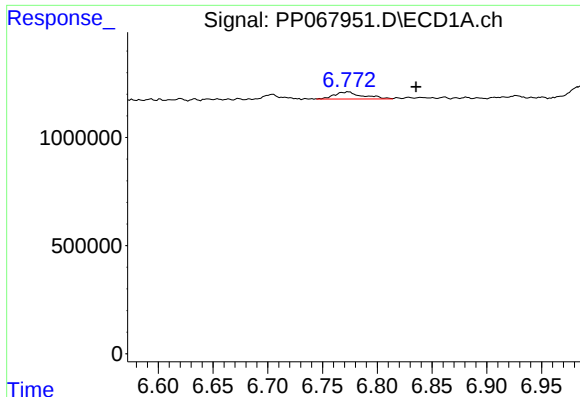

#20 AR-1242-5


R.T.: 6.774 min
Delta R.T.: -0.061 min
Response: 592915
Conc: 24.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

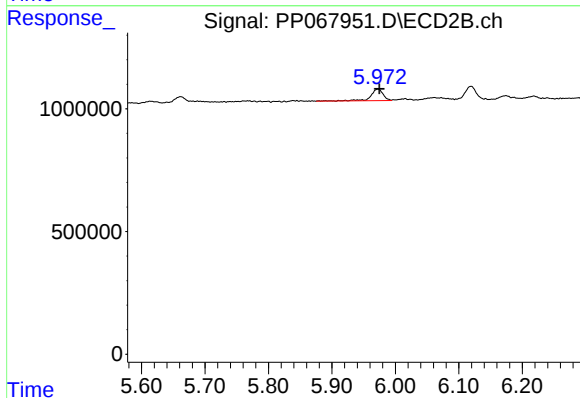


#20 AR-1242-5

R.T.: 5.973 min
Delta R.T.: -0.002 min
Response: 640154
Conc: 22.34 ng/ml

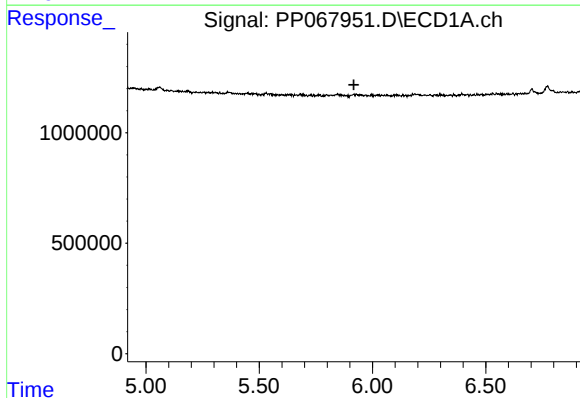


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 5.917 min
Response: 0
Conc: N.D.

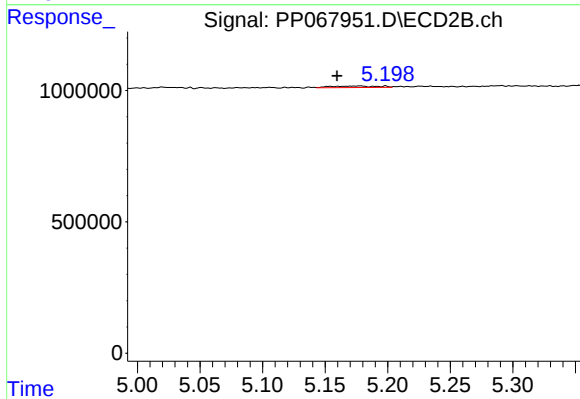

#21 AR-1248-1


R.T.: 5.178 min
Delta R.T.: 0.019 min
Response: 144738
Conc: 6.39 ng/ml

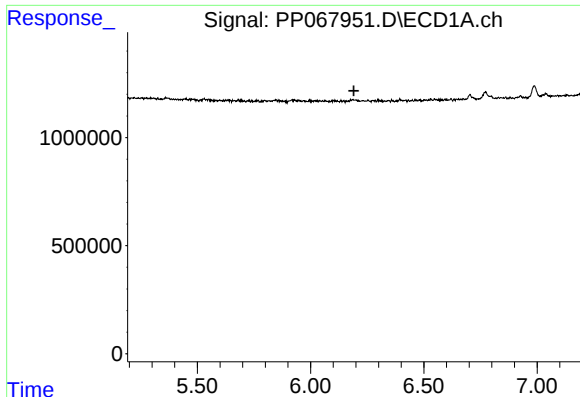

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

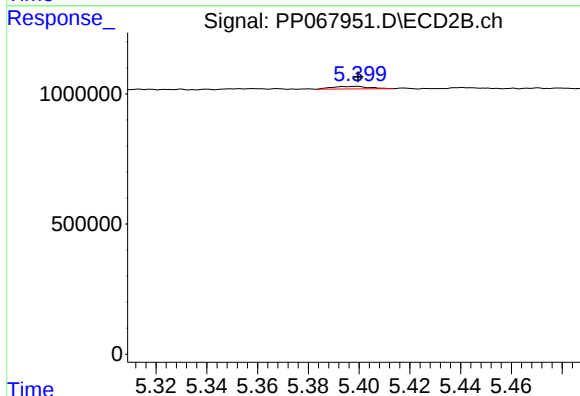


#22 AR-1248-2

R.T.: 5.399 min
Delta R.T.: 0.000 min
Response: 98297
Conc: 2.97 ng/ml

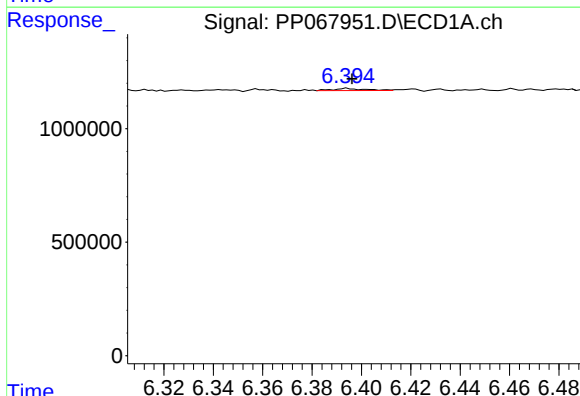


#23 AR-1248-3

R.T.: 6.394 min
Delta R.T.: -0.002 min
Response: 78662
Conc: 2.15 ng/ml

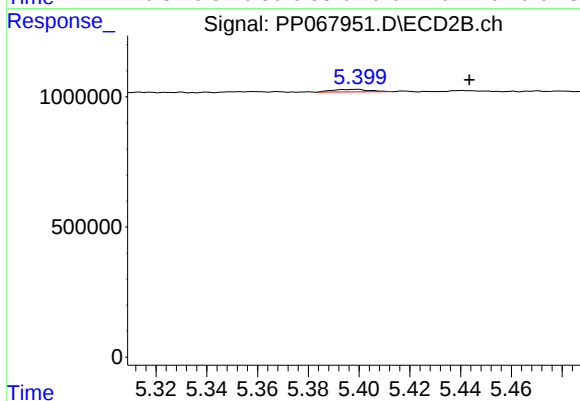

#23 AR-1248-3


R.T.: 5.399 min
Delta R.T.: -0.045 min
Response: 98297
Conc: 2.85 ng/ml

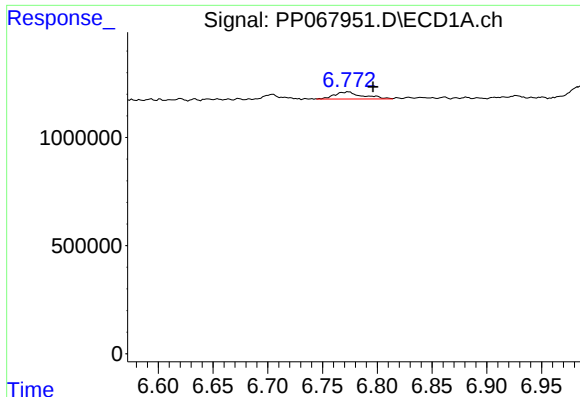

#24 AR-1248-4


R.T.: 6.774 min
Delta R.T.: -0.022 min
Response: 592915
Conc: 14.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

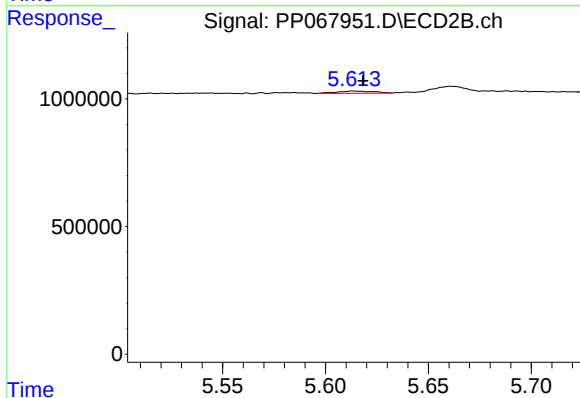


#24 AR-1248-4

R.T.: 5.614 min
Delta R.T.: -0.004 min
Response: 112302
Conc: 2.74 ng/ml

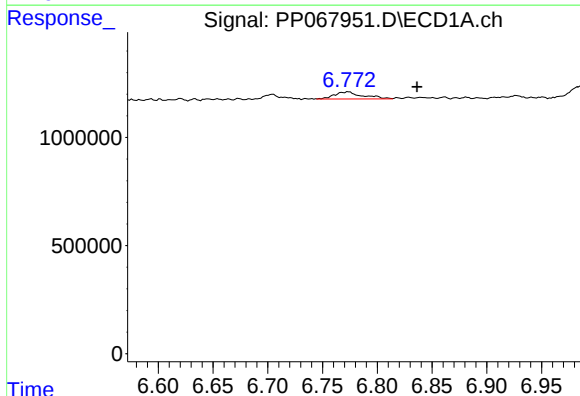


#25 AR-1248-5

R.T.: 6.774 min
Delta R.T.: -0.062 min
Response: 592915
Conc: 14.95 ng/ml

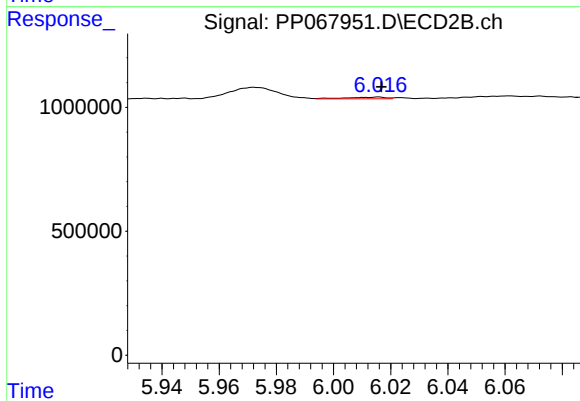

#25 AR-1248-5


R.T.: 6.015 min
Delta R.T.: -0.001 min
Response: 63735
Conc: 1.70 ng/ml

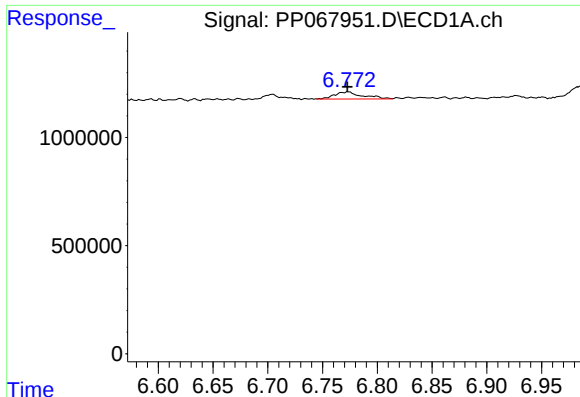

#26 AR-1254-1


R.T.: 6.774 min
Delta R.T.: 0.000 min
Response: 592915
Conc: 13.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

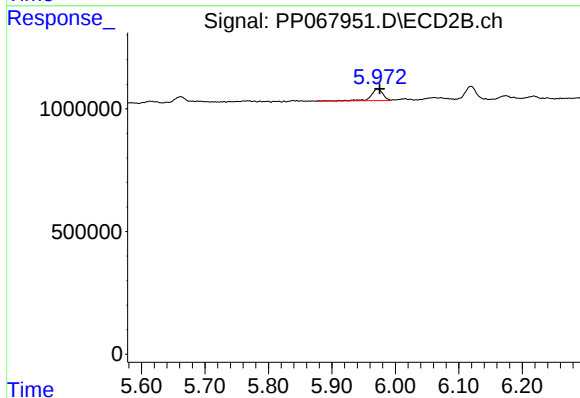


#26 AR-1254-1

R.T.: 5.973 min
Delta R.T.: -0.003 min
Response: 640154
Conc: 10.83 ng/ml

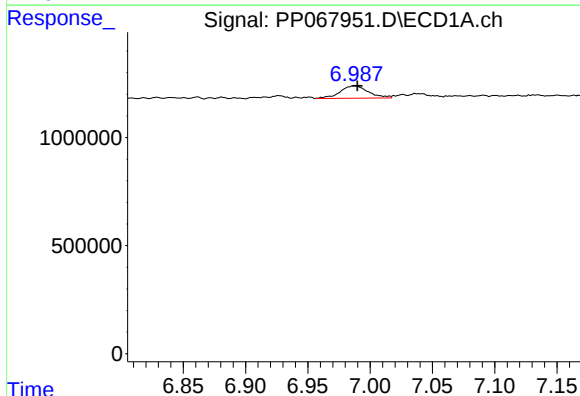


#27 AR-1254-2

R.T.: 6.988 min
Delta R.T.: -0.002 min
Response: 903530
Conc: 13.67 ng/ml

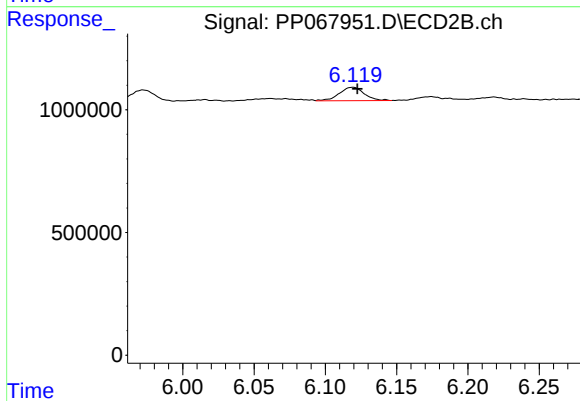

#27 AR-1254-2


R.T.: 6.119 min
Delta R.T.: -0.003 min
Response: 661384
Conc: 12.61 ng/ml

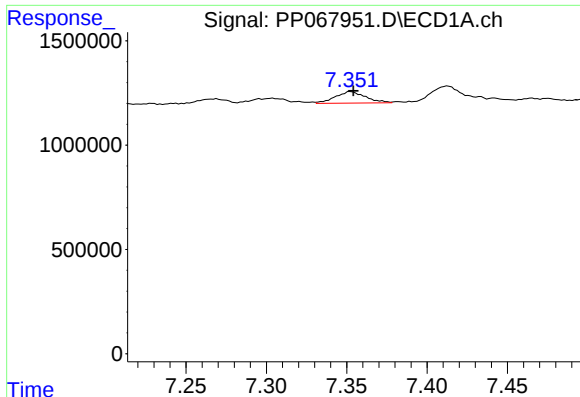

#28 AR-1254-3


R.T.: 7.353 min
Delta R.T.: -0.001 min
Response: 718917
Conc: 10.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

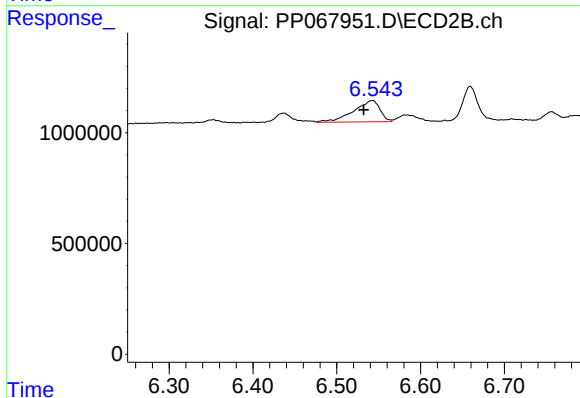


#28 AR-1254-3

R.T.: 6.543 min
Delta R.T.: 0.010 min
Response: 2120221
Conc: 25.48 ng/ml

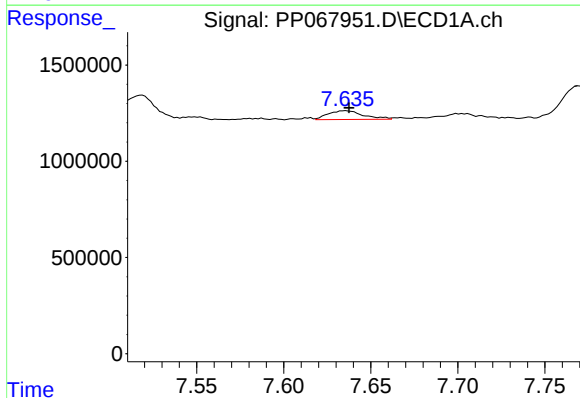


#29 AR-1254-4

R.T.: 7.635 min
Delta R.T.: -0.002 min
Response: 637987
Conc: 12.78 ng/ml

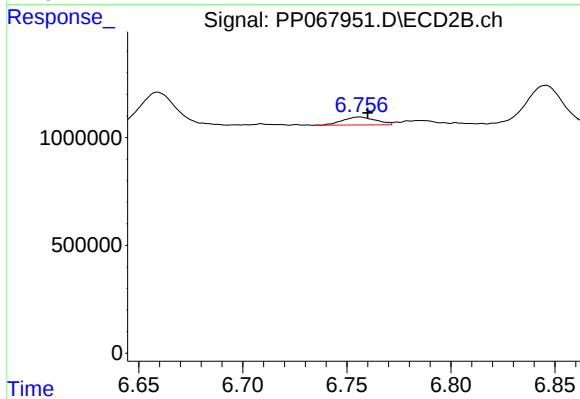

#29 AR-1254-4


R.T.: 6.756 min
Delta R.T.: -0.004 min
Response: 408761
Conc: 8.47 ng/ml

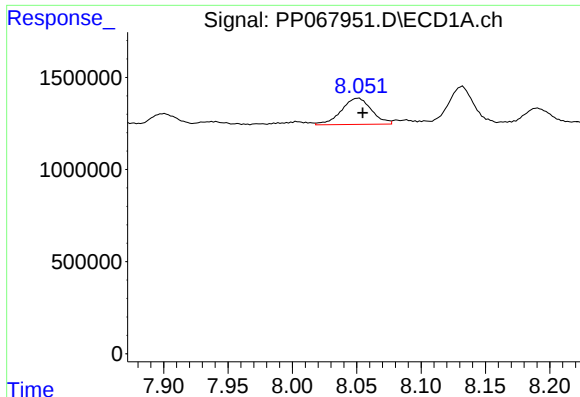

#30 AR-1254-5


R.T.: 8.051 min
Delta R.T.: -0.003 min
Response: 2323646
Conc: 39.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

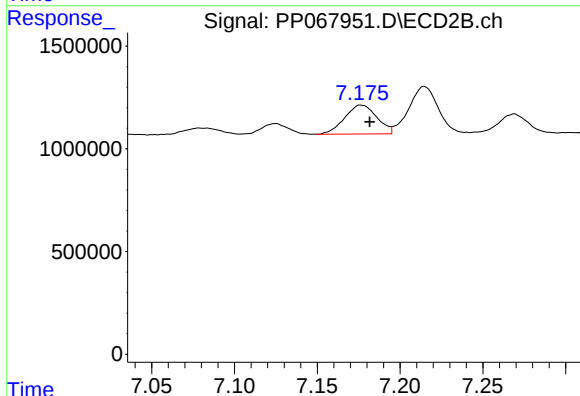


#30 AR-1254-5

R.T.: 7.177 min
Delta R.T.: -0.005 min
Response: 1914149
Conc: 26.02 ng/ml

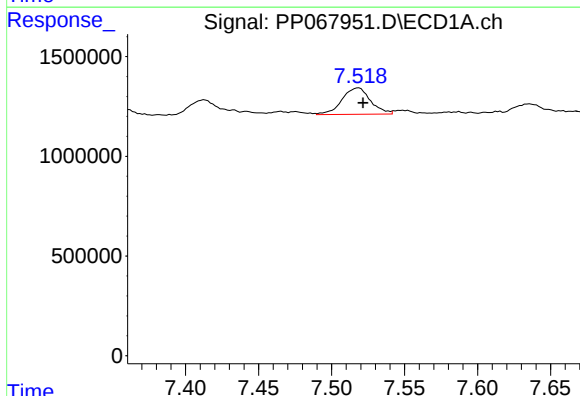


#31 AR-1260-1

R.T.: 7.518 min
Delta R.T.: -0.003 min
Response: 1804861
Conc: 33.41 ng/ml

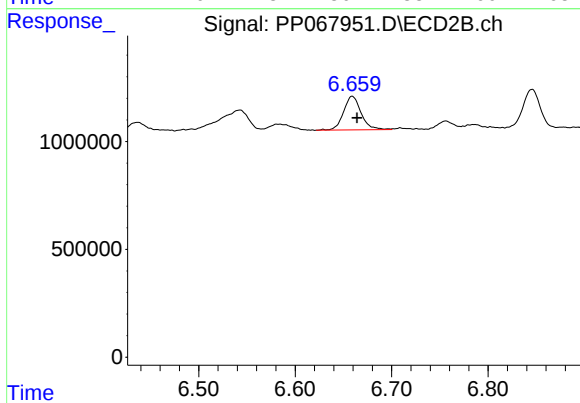

#31 AR-1260-1


R.T.: 6.659 min
Delta R.T.: -0.005 min
Response: 1974351
Conc: 34.66 ng/ml

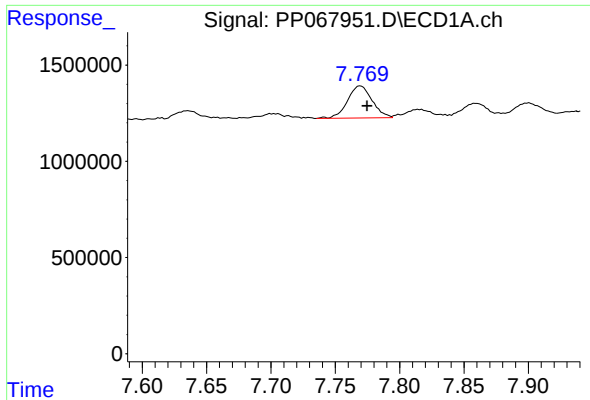

#32 AR-1260-2


R.T.: 7.770 min
Delta R.T.: -0.005 min
Response: 2211900
Conc: 34.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

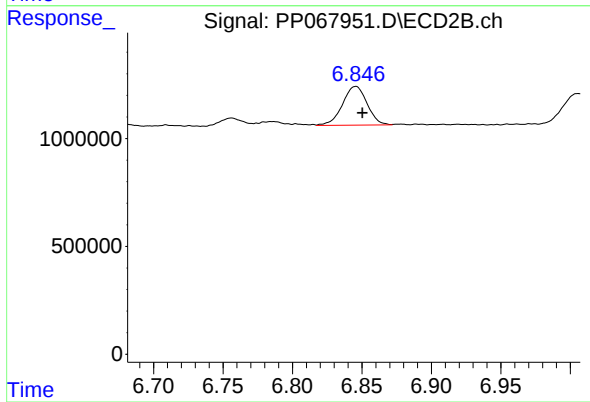


#32 AR-1260-2

R.T.: 6.846 min
Delta R.T.: -0.005 min
Response: 2216520
Conc: 33.23 ng/ml

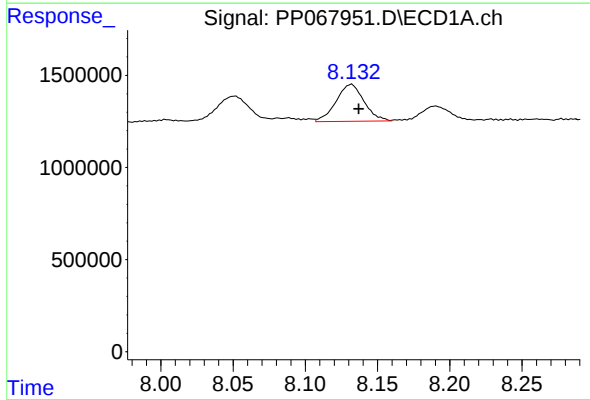


#33 AR-1260-3

R.T.: 8.132 min
Delta R.T.: -0.005 min
Response: 2699156
Conc: 52.06 ng/ml

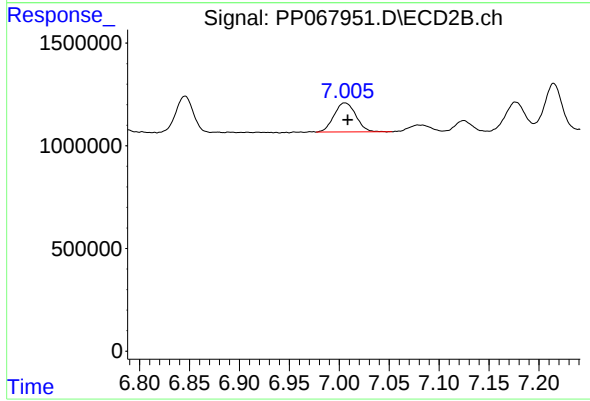

#33 AR-1260-3


R.T.: 7.006 min
Delta R.T.: -0.003 min
Response: 2158869
Conc: 33.89 ng/ml

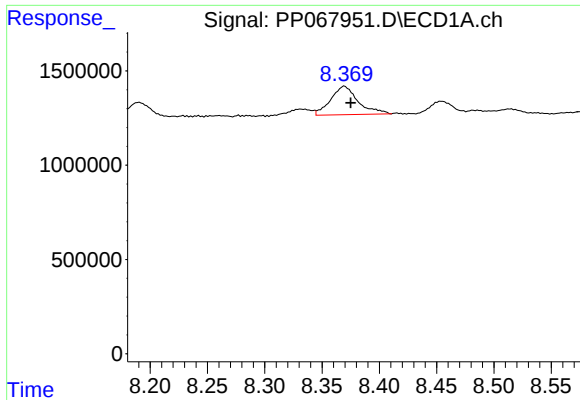

#34 AR-1260-4


R.T.: 8.370 min
Delta R.T.: -0.005 min
Response: 2518675
Conc: 41.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

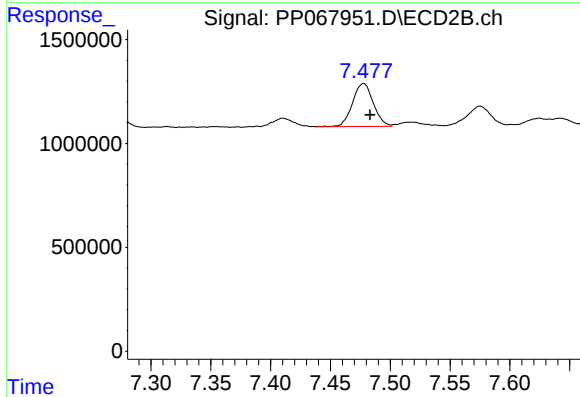


#34 AR-1260-4

R.T.: 7.478 min
Delta R.T.: -0.005 min
Response: 2498396
Conc: 45.18 ng/ml

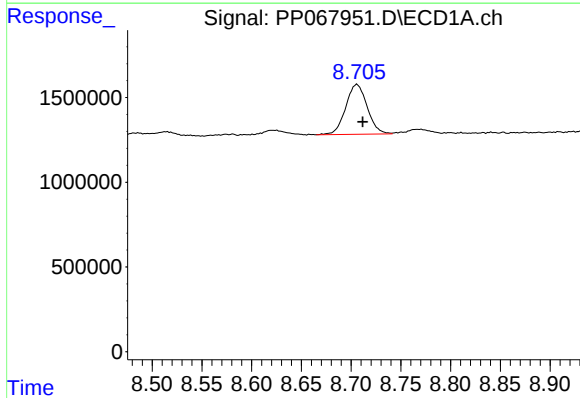


#35 AR-1260-5

R.T.: 8.706 min
Delta R.T.: -0.006 min
Response: 4417697
Conc: 41.01 ng/ml

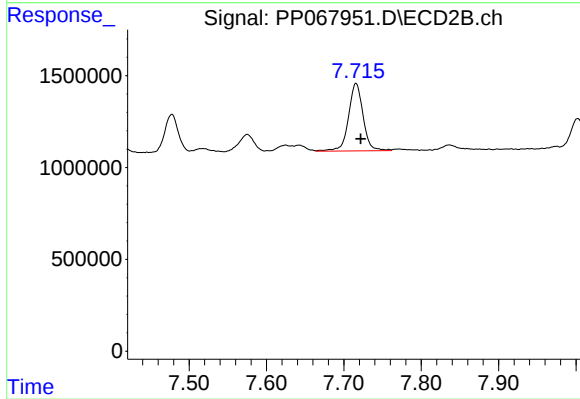

#35 AR-1260-5


R.T.: 7.716 min
Delta R.T.: -0.006 min
Response: 4787916
Conc: 39.15 ng/ml

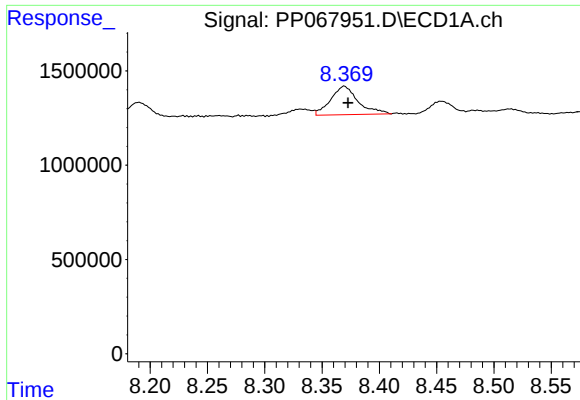

#36 AR-1262-1


R.T.: 8.370 min
Delta R.T.: -0.003 min
Response: 2518675
Conc: 35.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

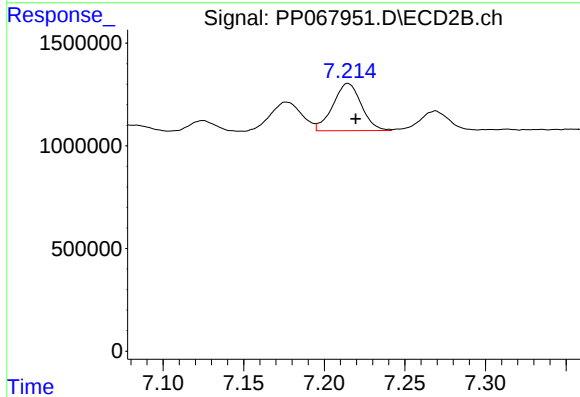


#36 AR-1262-1

R.T.: 7.215 min
Delta R.T.: -0.005 min
Response: 2828355
Conc: 35.95 ng/ml

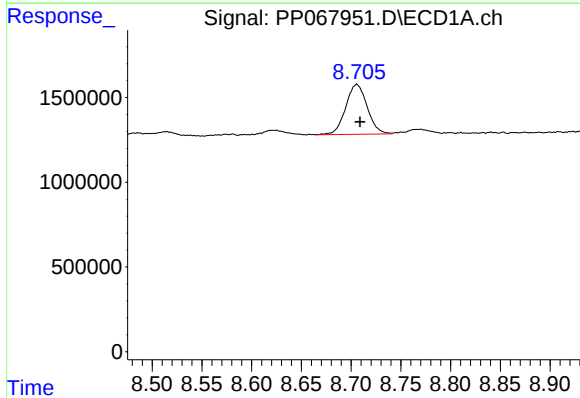


#37 AR-1262-2

R.T.: 8.706 min
Delta R.T.: -0.003 min
Response: 4417697
Conc: 36.34 ng/ml

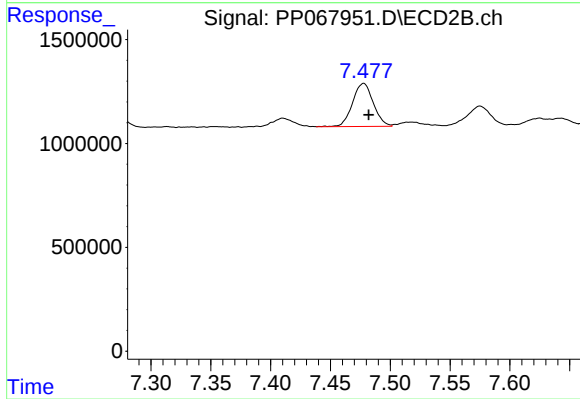

#37 AR-1262-2


R.T.: 7.478 min
Delta R.T.: -0.004 min
Response: 2498396
Conc: 35.21 ng/ml

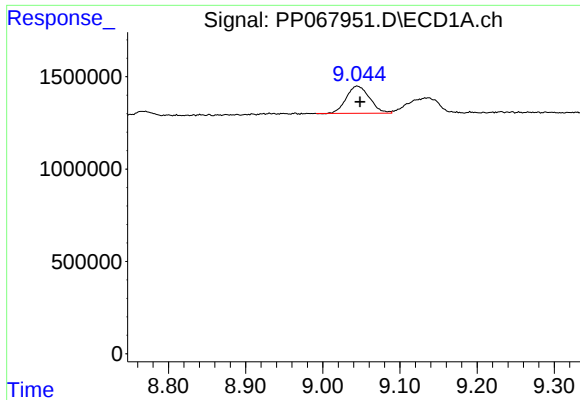

#38 AR-1262-3


R.T.: 9.045 min
Delta R.T.: -0.004 min
Response: 3090479
Conc: 34.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

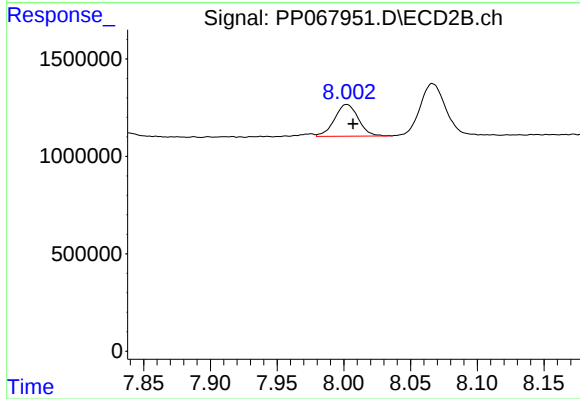


#38 AR-1262-3

R.T.: 8.002 min
Delta R.T.: -0.005 min
Response: 2026646
Conc: 35.49 ng/ml

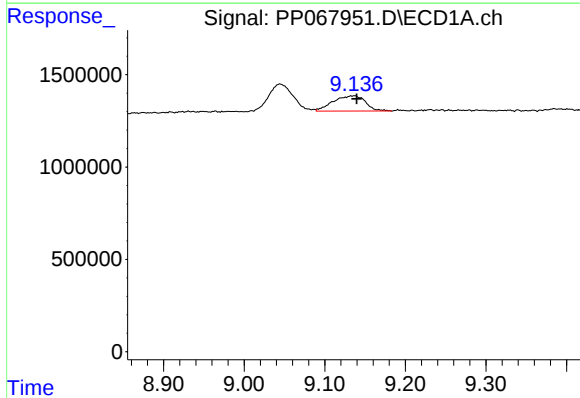


#39 AR-1262-4

R.T.: 9.136 min
Delta R.T.: -0.004 min
Response: 2323741
Conc: 33.22 ng/ml

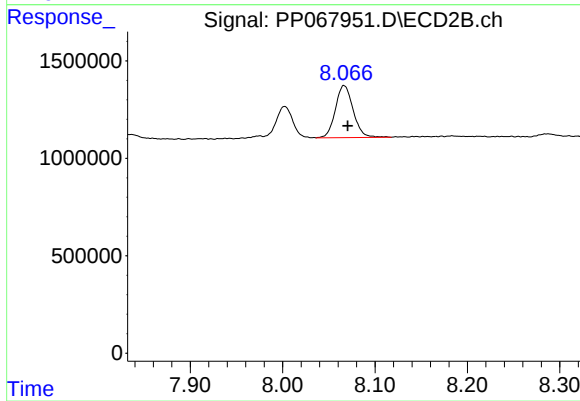

#39 AR-1262-4


R.T.: 8.067 min
Delta R.T.: -0.004 min
Response: 3576279
Conc: 35.61 ng/ml

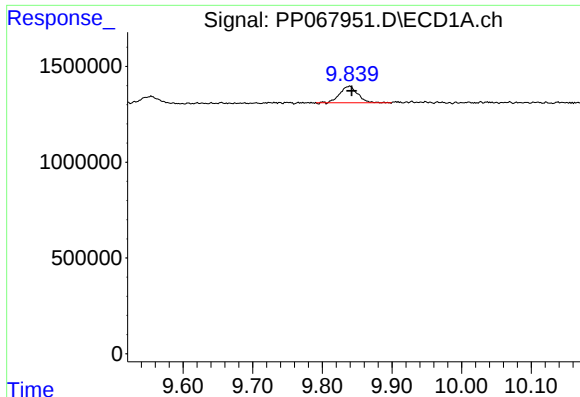

#40 AR-1262-5


R.T.: 9.839 min
Delta R.T.: -0.003 min
Response: 1525854
Conc: 32.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

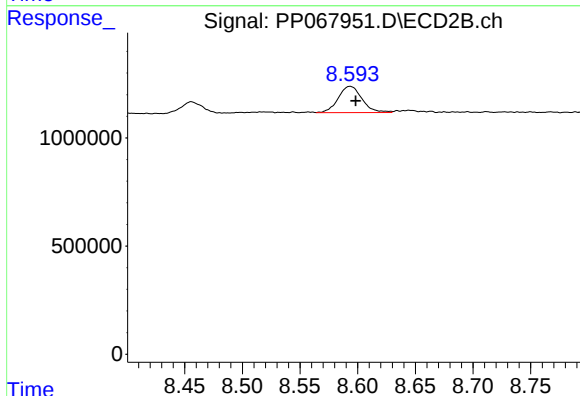


#40 AR-1262-5

R.T.: 8.593 min
Delta R.T.: -0.005 min
Response: 1731720
Conc: 34.62 ng/ml

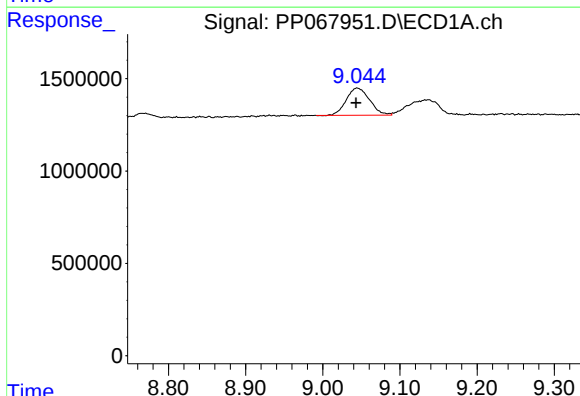


#41 AR-1268-1

R.T.: 9.045 min
Delta R.T.: 0.001 min
Response: 3090479
Conc: 20.25 ng/ml

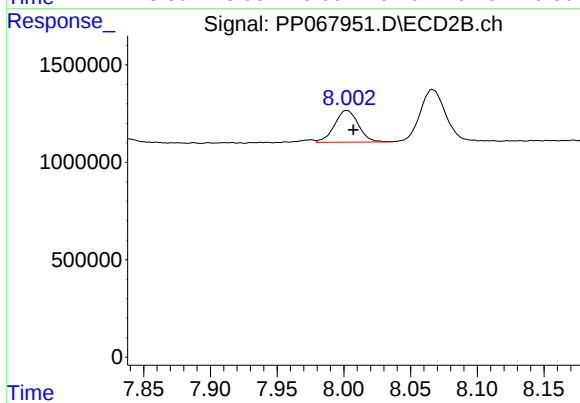

#41 AR-1268-1


R.T.: 8.002 min
Delta R.T.: -0.005 min
Response: 2026646
Conc: 12.73 ng/ml

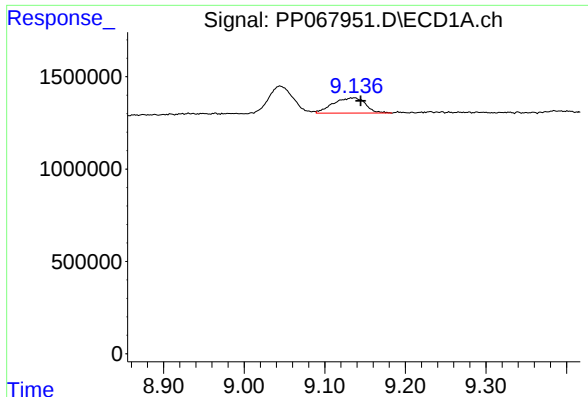

#42 AR-1268-2


R.T.: 9.136 min
Delta R.T.: -0.008 min
Response: 2323741
Conc: 17.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

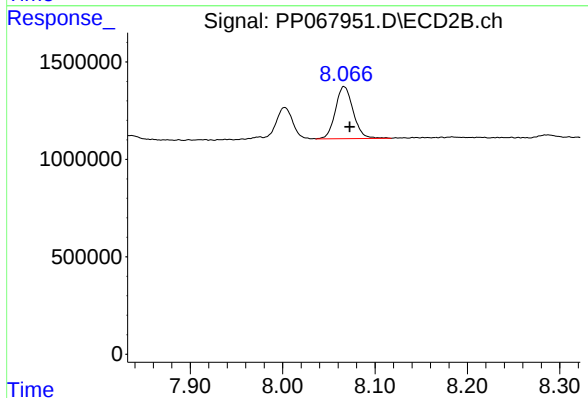


#42 AR-1268-2

R.T.: 8.067 min
Delta R.T.: -0.006 min
Response: 3576279
Conc: 24.98 ng/ml

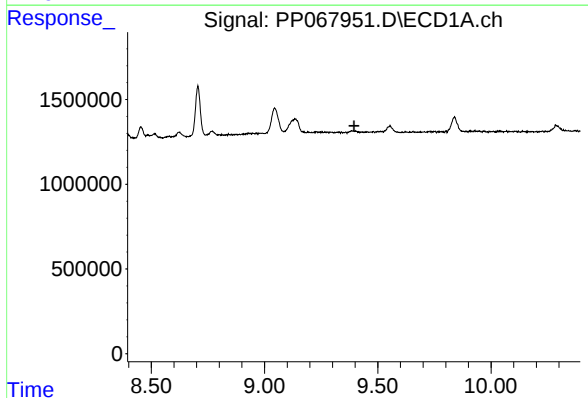


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 9.395 min
Response: 0
Conc: N.D.

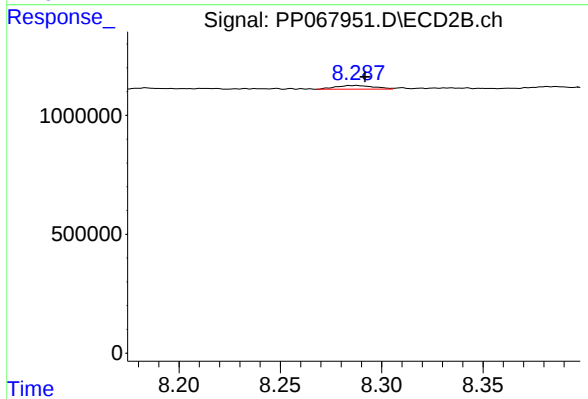

#43 AR-1268-3


R.T.: 8.287 min
Delta R.T.: -0.005 min
Response: 206695
Conc: 1.62 ng/ml

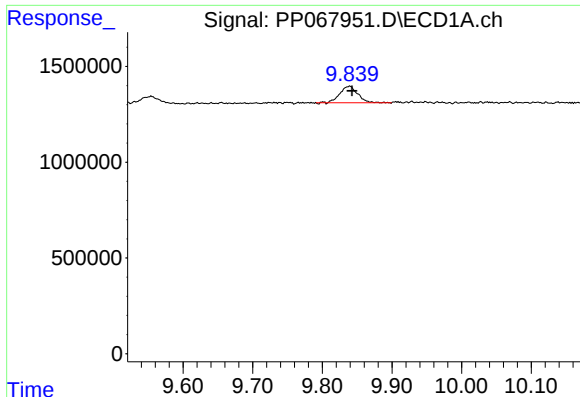

#44 AR-1268-4


R.T.: 9.839 min
Delta R.T.: -0.004 min
Response: 1525854
Conc: 30.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

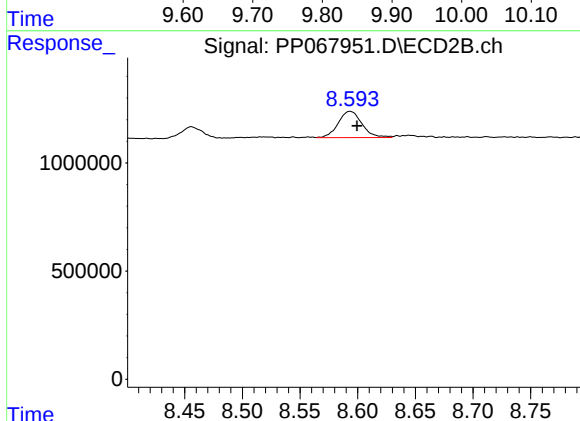


#44 AR-1268-4

R.T.: 8.593 min
Delta R.T.: -0.006 min
Response: 1731720
Conc: 30.66 ng/ml

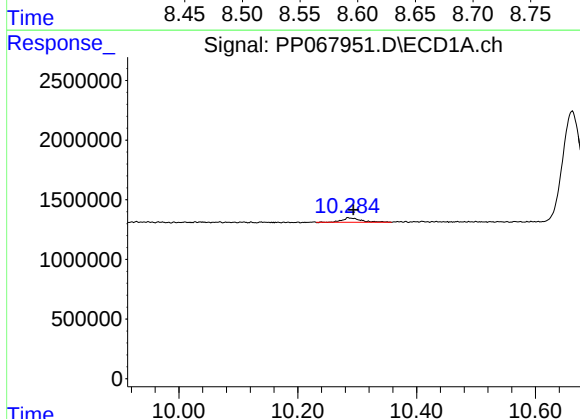

#45 AR-1268-5

R.T.: 10.286 min
Delta R.T.: -0.008 min
Response: 801777
Conc: 2.15 ng/ml

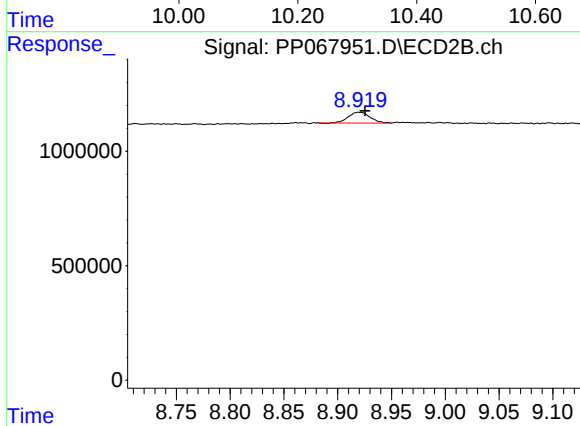

#45 AR-1268-5

R.T.: 8.920 min
Delta R.T.: -0.005 min
Response: 659351
Conc: 1.74 ng/ml