

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
 Data File : PP067952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2024 02:07
 Operator : YP\AJ
 Sample : P4368-07
 Misc : AR1268 LOD 40 PPB
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 07:31:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.753	4.050	14510873	15367224	15.677	15.209
2)	SA Decachlor...	10.662	9.210	23058239	20528838	20.028	18.305
Target Compounds							
3)	L1 AR-1016-1	0.000	5.202f	0	83385	N.D.	2.383 #
4)	L1 AR-1016-2	0.000	5.202	0	83385	N.D.	1.731 #
5)	L1 AR-1016-3	0.000	5.343	0	57241	N.D.	2.125 #
6)	L1 AR-1016-4	0.000	5.400	0	36277	N.D.	1.506 #
7)	L1 AR-1016-5	0.000	5.616	0	63084	N.D.	2.074 #
9)	L2 AR-1221-2	5.060	4.360	158515	274649	16.755	27.572 #
10)	L2 AR-1221-3	5.060f	0.000	158515	0	5.483	N.D. #
11)	L3 AR-1232-1	5.060f	0.000	158515	0	6.934	N.D. #
12)	L3 AR-1232-2	0.000	5.202	0	83385	N.D.	3.728 #
13)	L3 AR-1232-3	0.000	5.343	0	57241	N.D.	4.793 #
14)	L3 AR-1232-4	0.000	5.400f	0	36277	N.D.	3.146 #
15)	L3 AR-1232-5	0.000	5.616	0	63084	N.D.	4.690 #
16)	L4 AR-1242-1	5.848f	5.202f	267852	83385	9.588	2.868 #
17)	L4 AR-1242-2	0.000	5.202	0	83385	N.D.	2.077 #
18)	L4 AR-1242-3	0.000	5.343	0	57241	N.D.	2.545 #
19)	L4 AR-1242-4	0.000	5.400f	0	36277	N.D.	1.528 #
20)	L4 AR-1242-5	6.769f	5.971	245011	306190	10.156	10.687
21)	L5 AR-1248-1	5.848f	5.202f	267852	83385	12.503	3.679 #
22)	L5 AR-1248-2	0.000	5.400	0	36277	N.D.	1.096 #
23)	L5 AR-1248-3	0.000	5.400f	0	36277	N.D.	1.052 #
24)	L5 AR-1248-4	6.769	5.616	245011	63084	6.057	1.540 #
25)	L5 AR-1248-5	6.769f	6.018	245011	90750	6.178	2.424 #
26)	L6 AR-1254-1	6.769	5.971	245011	306190	5.471	5.182
27)	L6 AR-1254-2	6.988	6.119	496108	352653	7.506	6.722
28)	L6 AR-1254-3	7.354	6.530	690108	602446	9.936	7.240 #
29)	L6 AR-1254-4	7.637	6.758	526368	404180	10.547	8.373
30)	L6 AR-1254-5	8.056	7.179	562631	572263	9.489	7.780
31)	L7 AR-1260-1	7.515	6.661	217712	319944	4.030	5.617 #
32)	L7 AR-1260-2	7.775	6.847	489293	425908	7.733	6.385
33)	L7 AR-1260-3	8.133	7.004	997504	393873	19.239	6.183 #
34)	L7 AR-1260-4	8.360	7.478	362510	1432097	6.022	25.900 #
35)	L7 AR-1260-5	8.708	7.716	635039	864257	5.896	7.067
36)	L8 AR-1262-1	8.360	7.216	362510	1096642	5.051	13.939 #
37)	L8 AR-1262-2	8.708	7.478	635039	1432097	5.223	20.181 #
38)	L8 AR-1262-3	9.043	8.003	5435260	5466953	61.405	95.745 #
39)	L8 AR-1262-4	9.142	8.068	4642317	4874537	66.371	48.534 #
40)	L8 AR-1262-5	9.838	8.594	1721639	1777433	36.794	35.536
41)	L9 AR-1268-1	9.043	8.003	5435260	5466953	35.606	34.353
42)	L9 AR-1268-2	9.142	8.068	4642317	4874537	33.986	34.043

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
Data File : PP067952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 02:07
Operator : YP\AJ
Sample : P4368-07
Misc : AR1268 LOD 40 PPB
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:31:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43)	L9 AR-1268-3	9.393	8.286	4354560	4211869	36.013	33.032
44)	L9 AR-1268-4	9.838	8.594	1721639	1777433	33.877	31.472
45)	L9 AR-1268-5	10.291	8.920	13368709	12621167	35.796	33.386



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
Data File : PP067952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 02:07
Operator : YP\AJ
Sample : P4368-07
Misc : AR1268 LOD 40 PPB
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:31:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

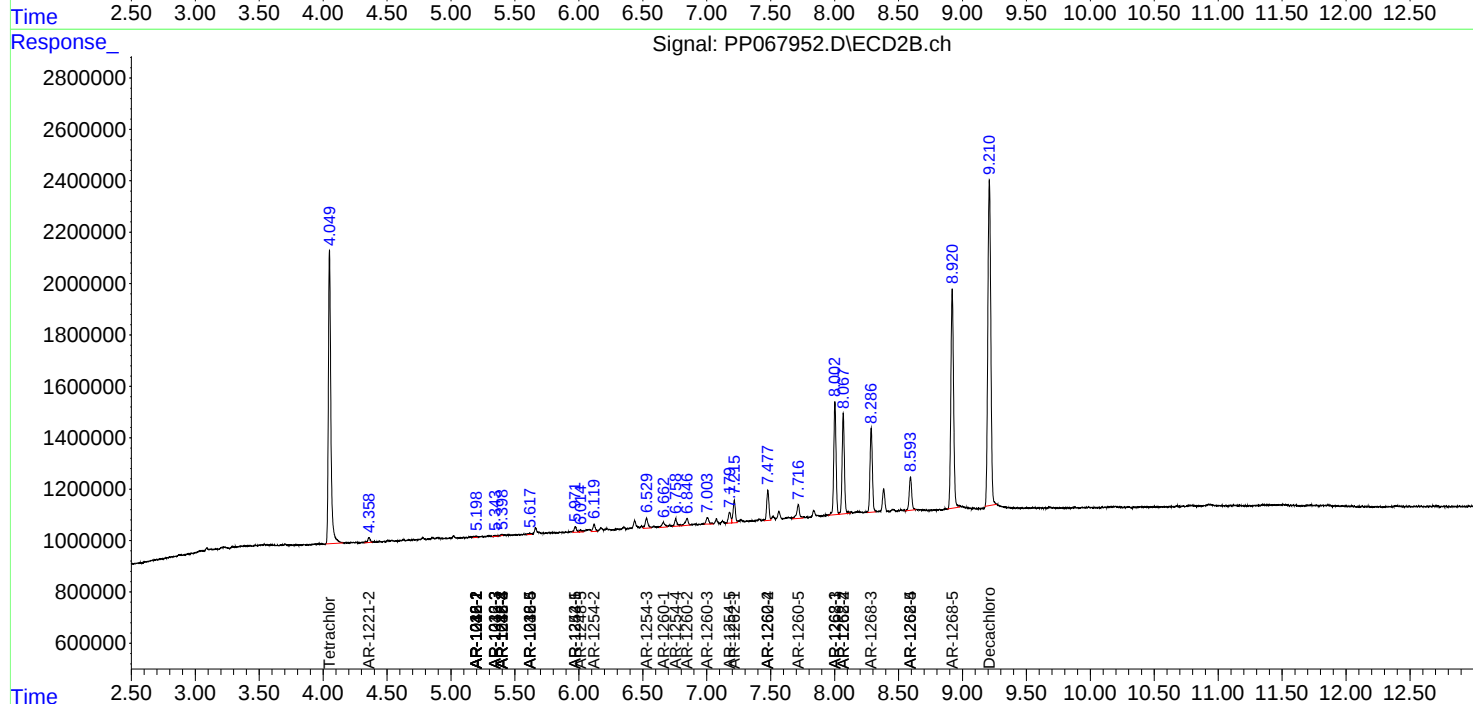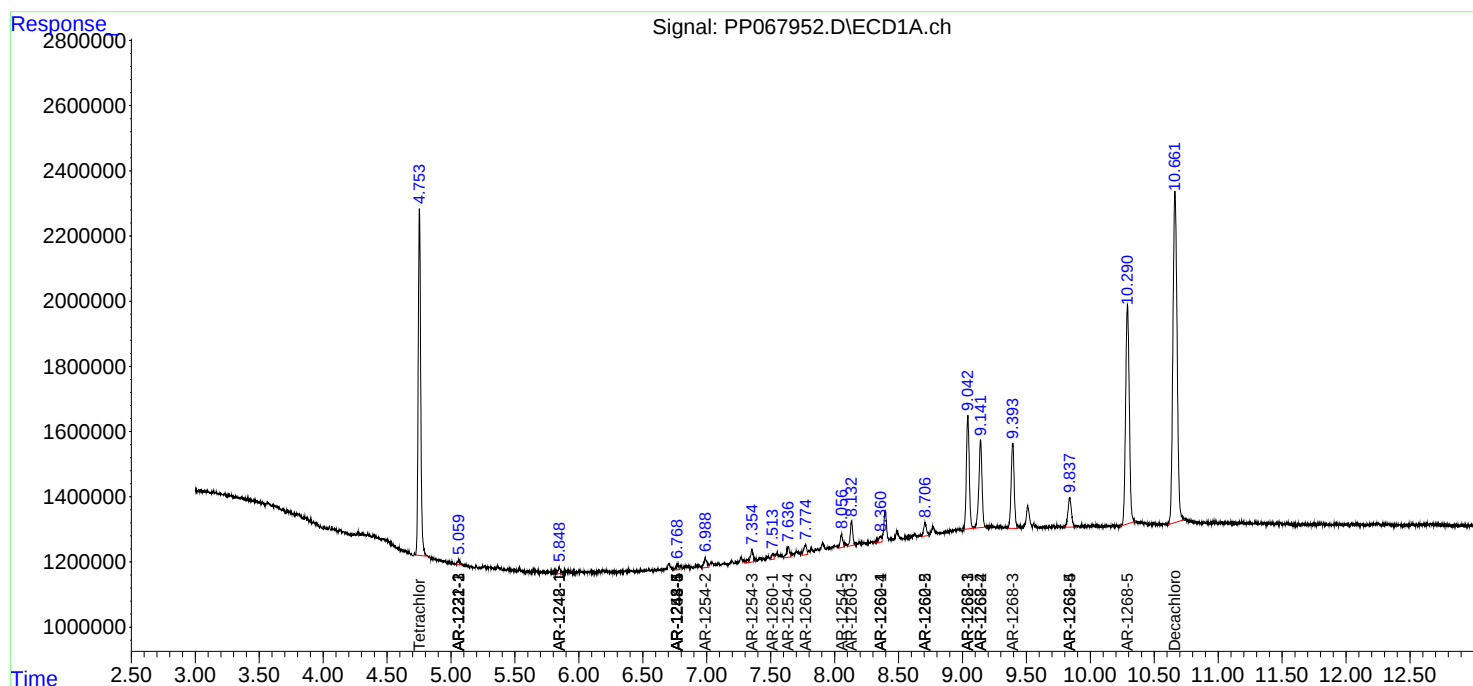


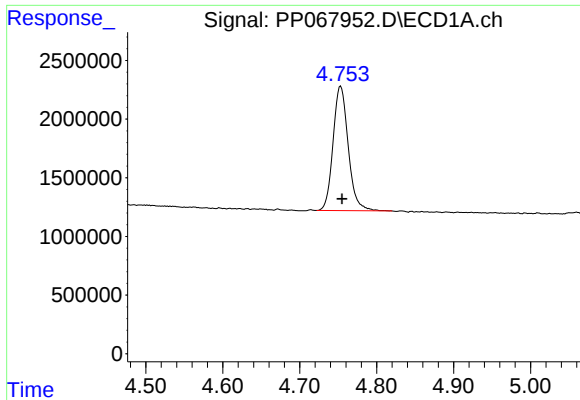

#1 Tetrachloro-m-xylene


R.T.: 4.753 min
Delta R.T.: -0.002 min
Response: 14510873
Conc: 15.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

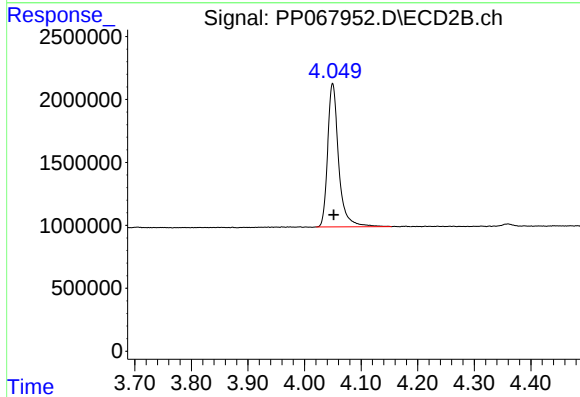


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 15367224
Conc: 15.21 ng/ml

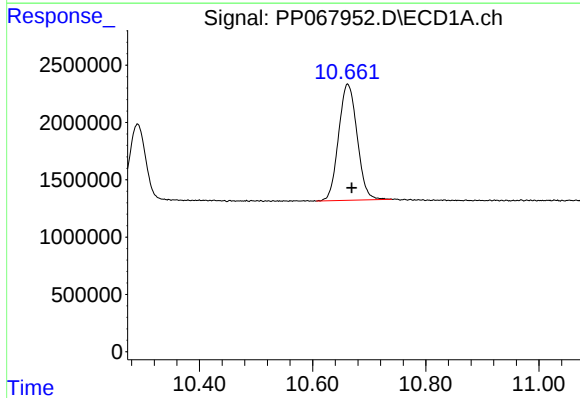


#2 Decachlorobiphenyl

R.T.: 10.662 min
Delta R.T.: -0.007 min
Response: 23058239
Conc: 20.03 ng/ml

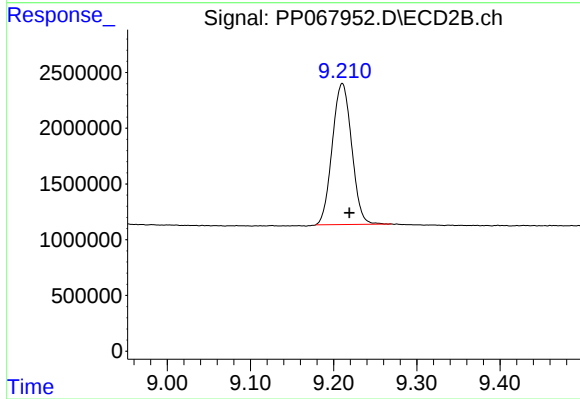

#2 Decachlorobiphenyl


R.T.: 9.210 min
Delta R.T.: -0.009 min
Response: 20528838
Conc: 18.31 ng/ml

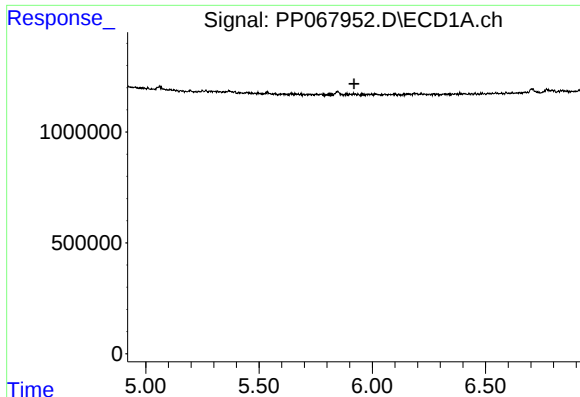

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.919 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

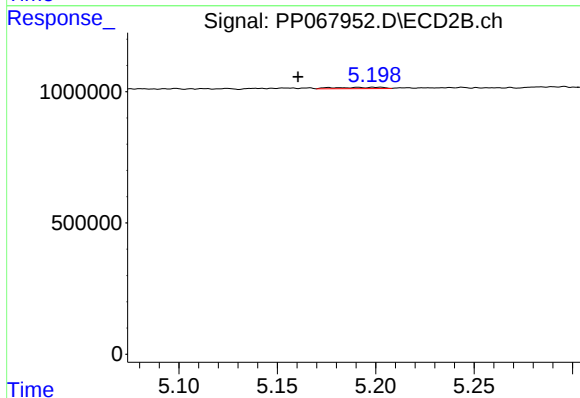


#3 AR-1016-1

R.T.: 5.202 min
Delta R.T.: 0.041 min
Response: 83385
Conc: 2.38 ng/ml

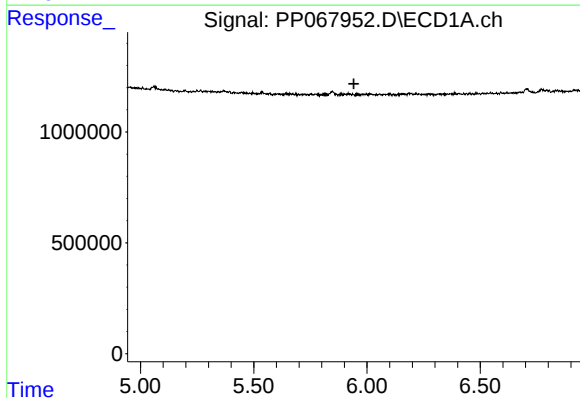


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.942 min
Response: 0
Conc: N.D.

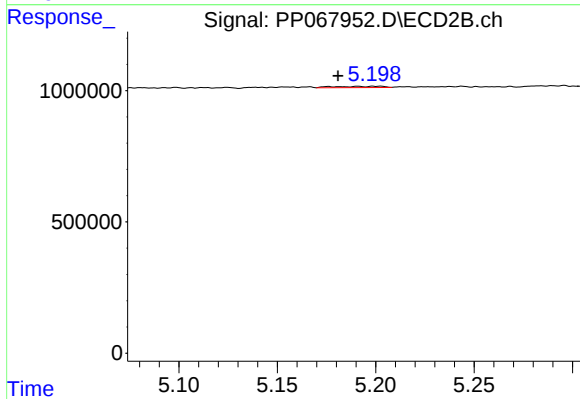

#4 AR-1016-2


R.T.: 5.202 min
Delta R.T.: 0.021 min
Response: 83385
Conc: 1.73 ng/ml

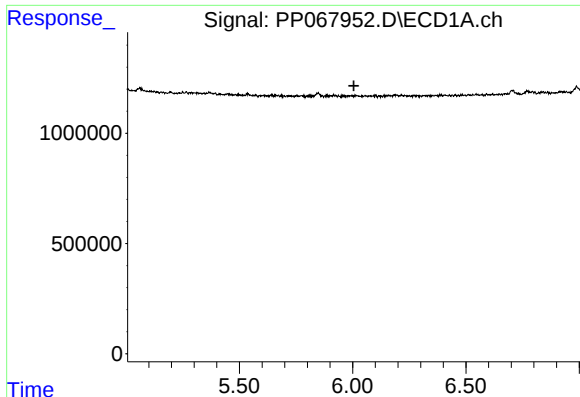

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 6.005 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

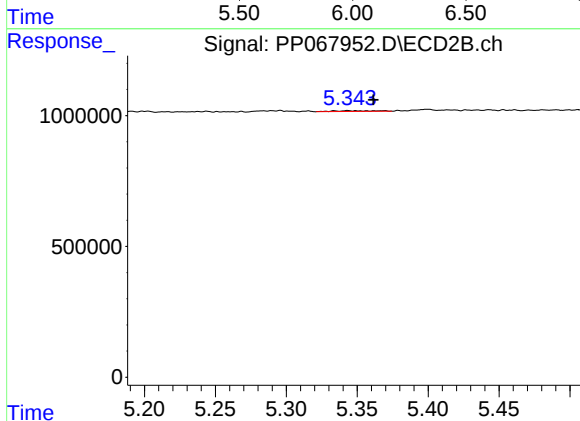


#5 AR-1016-3

R.T.: 5.343 min
Delta R.T.: -0.018 min
Response: 57241
Conc: 2.12 ng/ml

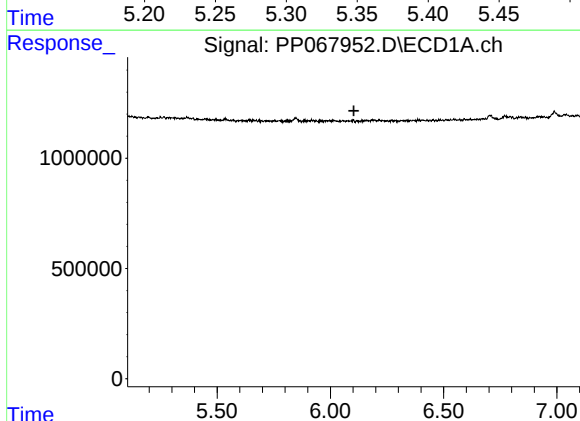


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 6.103 min
Response: 0
Conc: N.D.

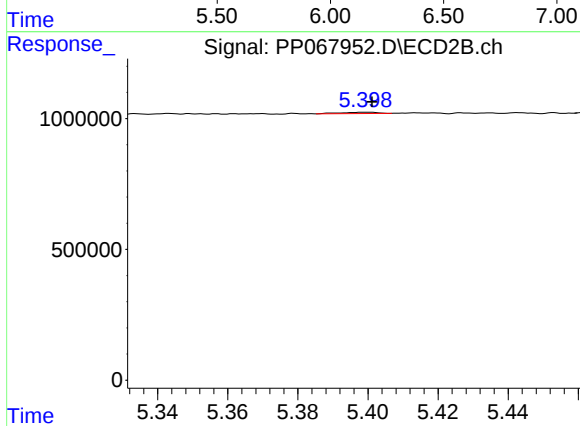

#6 AR-1016-4


R.T.: 5.400 min
Delta R.T.: -0.002 min
Response: 36277
Conc: 1.51 ng/ml

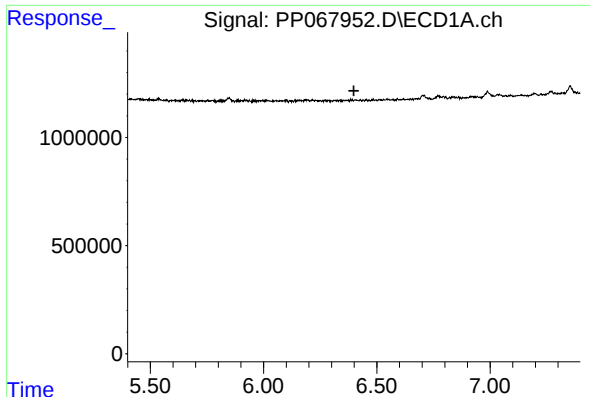

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

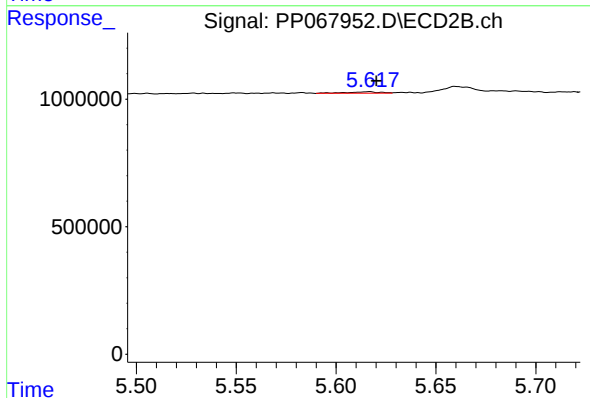


#7 AR-1016-5

R.T.: 5.616 min
Delta R.T.: -0.004 min
Response: 63084
Conc: 2.07 ng/ml

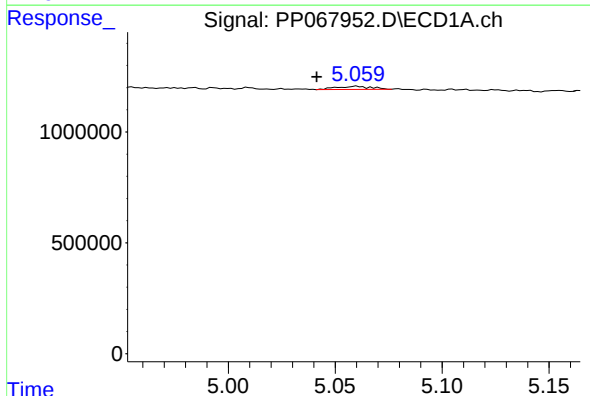


#9 AR-1221-2

R.T.: 5.060 min
Delta R.T.: 0.019 min
Response: 158515
Conc: 16.76 ng/ml

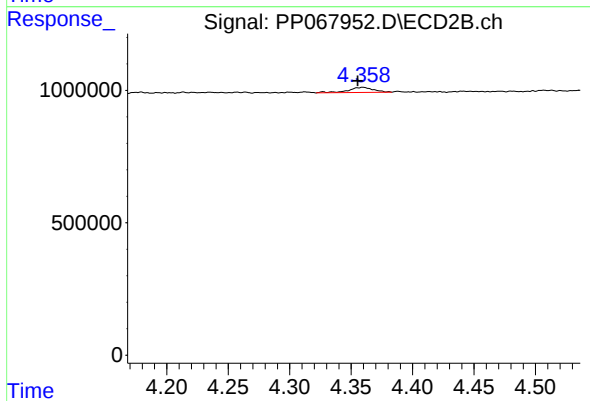

#9 AR-1221-2


R.T.: 4.360 min
Delta R.T.: 0.004 min
Response: 274649
Conc: 27.57 ng/ml

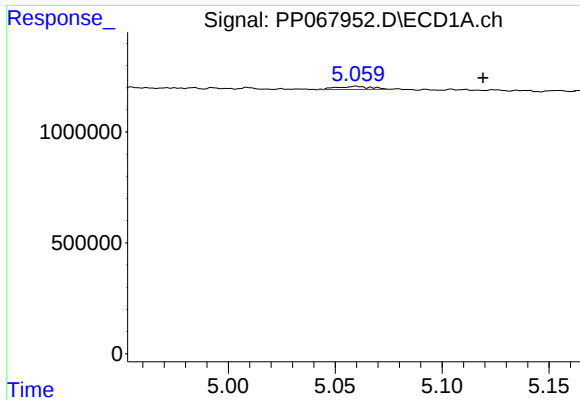

#10 AR-1221-3


R.T.: 5.060 min
Delta R.T.: -0.059 min
Response: 158515
Conc: 5.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

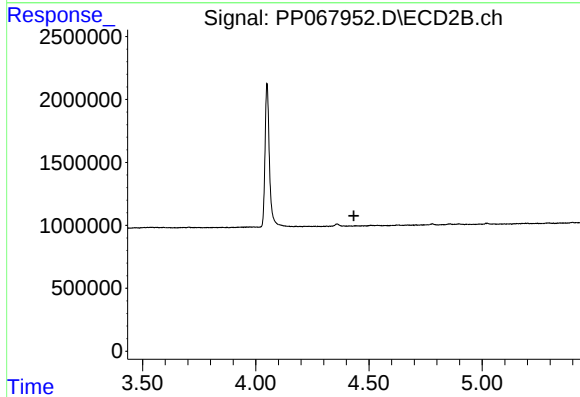


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.434 min
Response: 0
Conc: N.D.

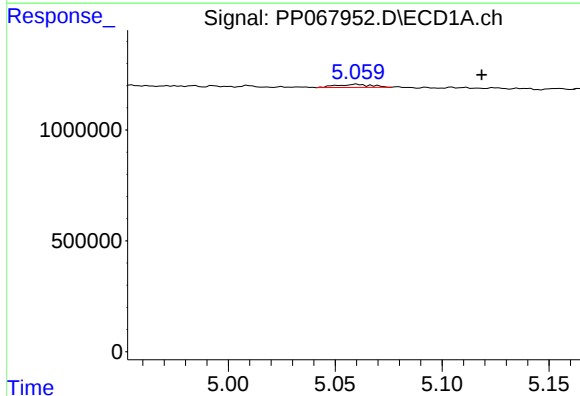


#11 AR-1232-1

R.T.: 5.060 min
Delta R.T.: -0.058 min
Response: 158515
Conc: 6.93 ng/ml

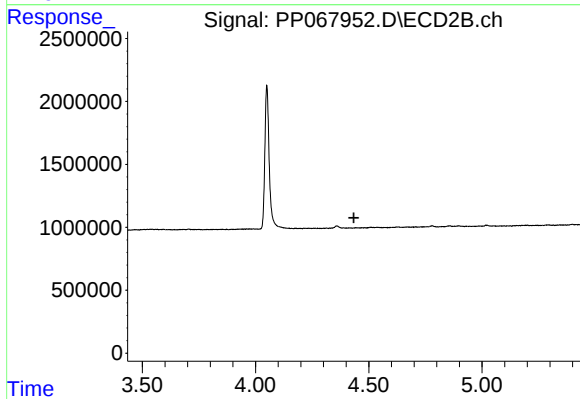

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.434 min
Response: 0
Conc: N.D.

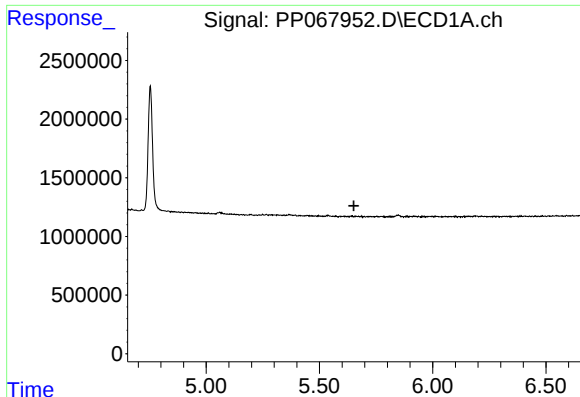

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 5.651 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

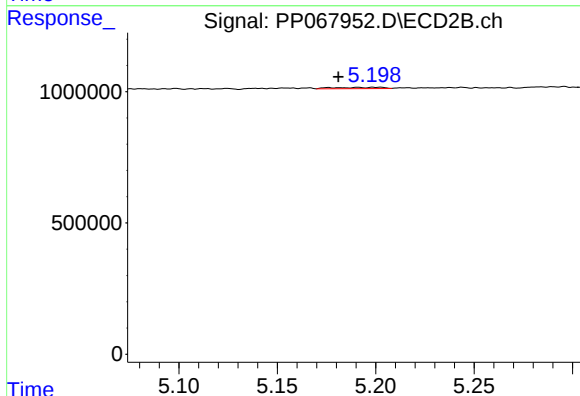


#12 AR-1232-2

R.T.: 5.202 min
Delta R.T.: 0.021 min
Response: 83385
Conc: 3.73 ng/ml

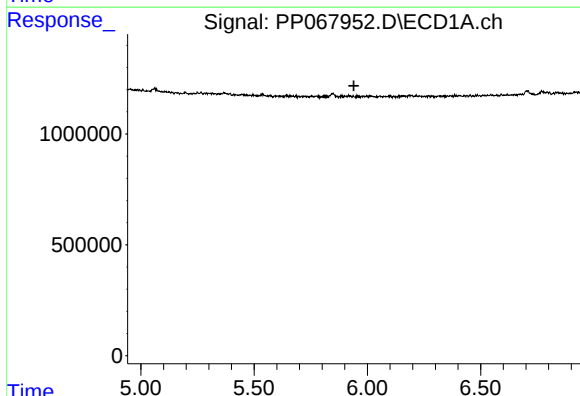


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T.: 5.940 min
Response: 0
Conc: N.D.

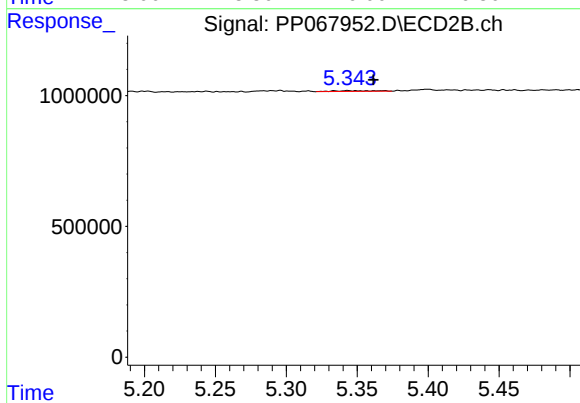

#13 AR-1232-3


R.T.: 5.343 min
Delta R.T.: -0.018 min
Response: 57241
Conc: 4.79 ng/ml

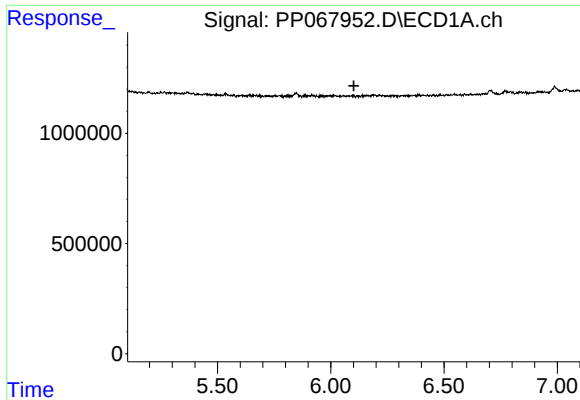

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T.: 6.101 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

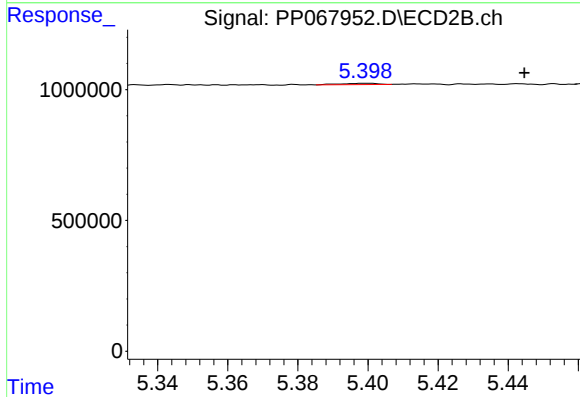


#14 AR-1232-4

R.T.: 5.400 min
Delta R.T.: -0.045 min
Response: 36277
Conc: 3.15 ng/ml

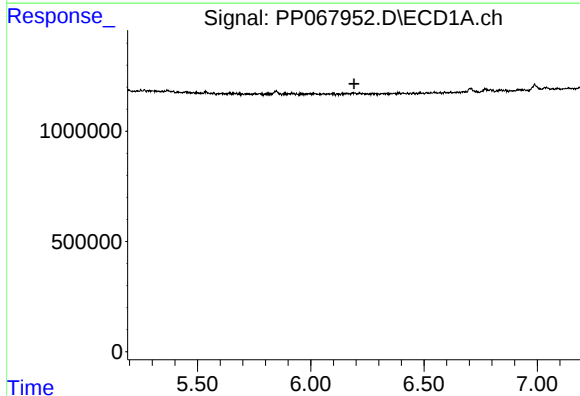


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

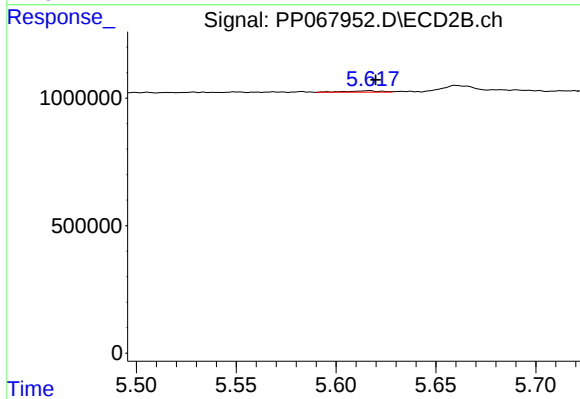

#15 AR-1232-5


R.T.: 5.616 min
Delta R.T.: -0.003 min
Response: 63084
Conc: 4.69 ng/ml

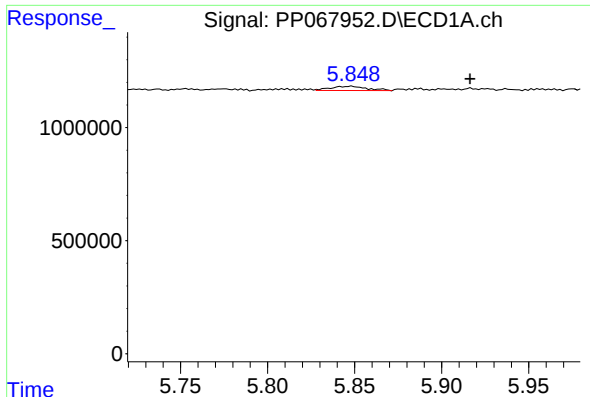

#16 AR-1242-1


R.T.: 5.848 min
Delta R.T.: -0.068 min
Response: 267852
Conc: 9.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

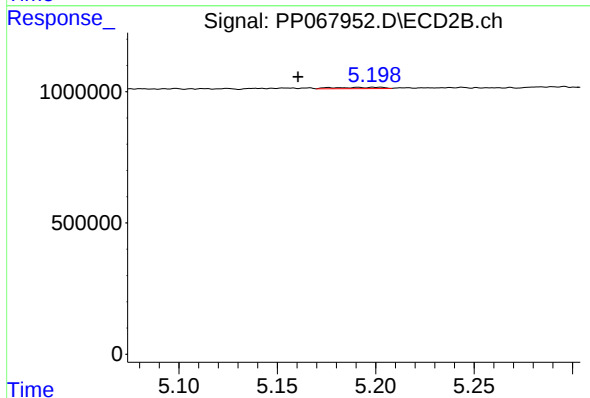


#16 AR-1242-1

R.T.: 5.202 min
Delta R.T.: 0.041 min
Response: 83385
Conc: 2.87 ng/ml

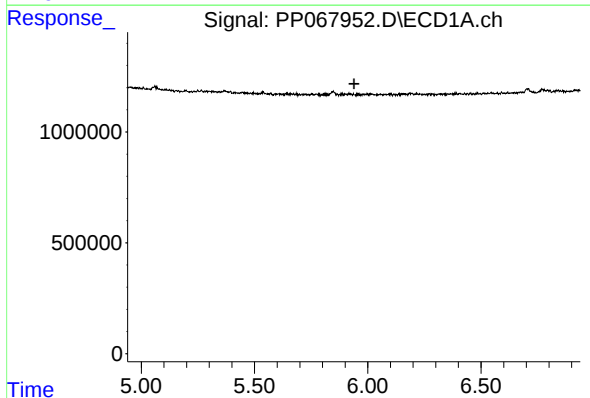


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 5.939 min
Response: 0
Conc: N.D.

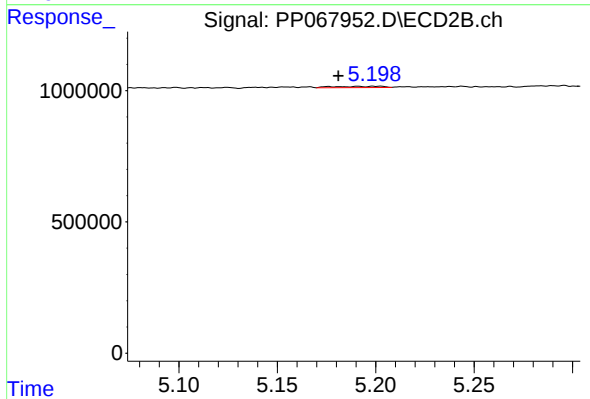

#17 AR-1242-2


R.T.: 5.202 min
Delta R.T.: 0.021 min
Response: 83385
Conc: 2.08 ng/ml

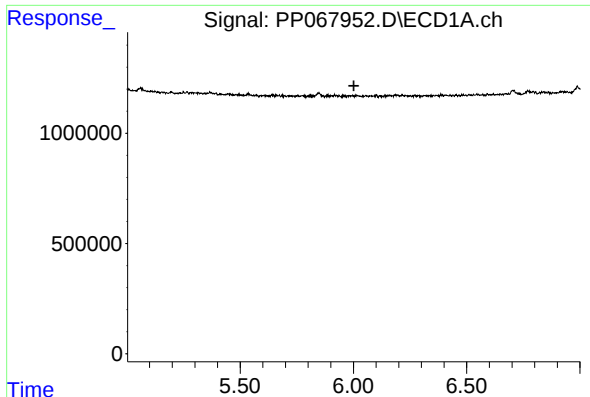

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 6.002 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

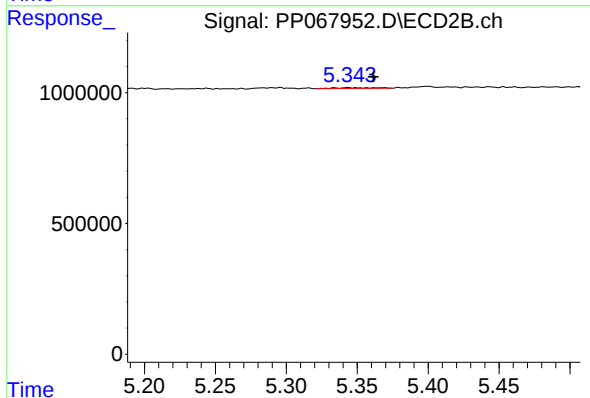


#18 AR-1242-3

R.T.: 5.343 min
Delta R.T.: -0.018 min
Response: 57241
Conc: 2.54 ng/ml

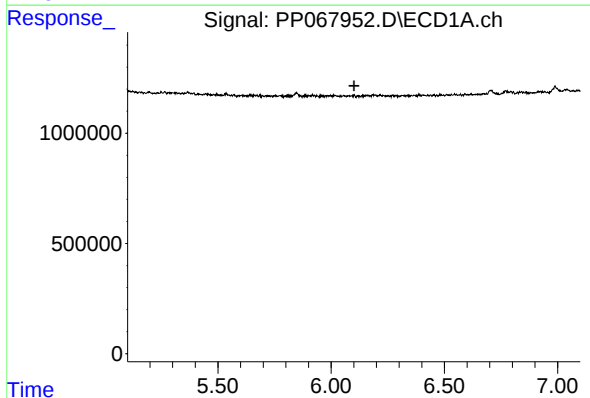


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T.: 6.101 min
Response: 0
Conc: N.D.

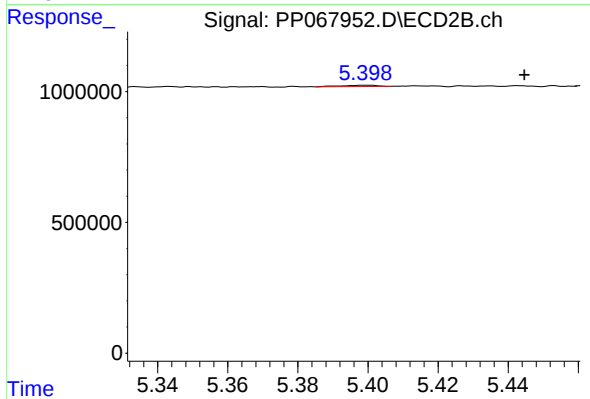

#19 AR-1242-4


R.T.: 5.400 min
Delta R.T.: -0.045 min
Response: 36277
Conc: 1.53 ng/ml

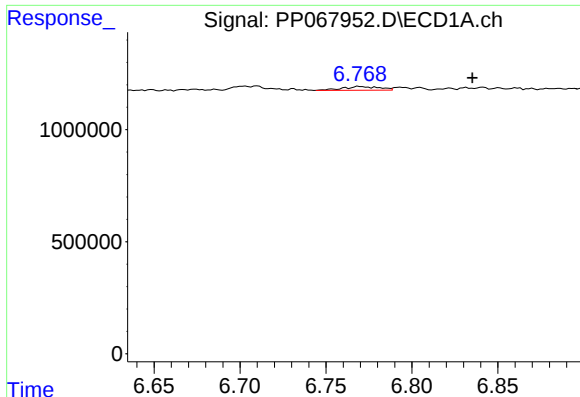

#20 AR-1242-5


R.T.: 6.769 min
Delta R.T.: -0.066 min
Response: 245011
Conc: 10.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

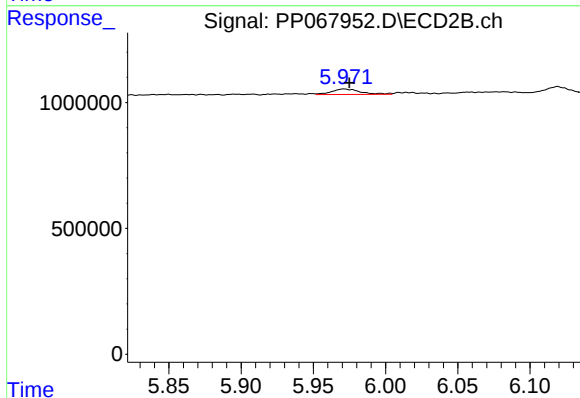


#20 AR-1242-5

R.T.: 5.971 min
Delta R.T.: -0.004 min
Response: 306190
Conc: 10.69 ng/ml

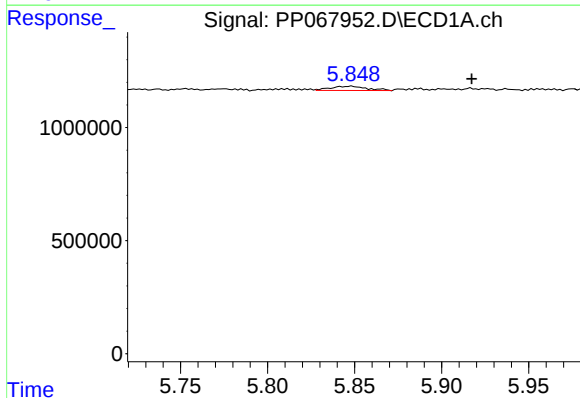


#21 AR-1248-1

R.T.: 5.848 min
Delta R.T.: -0.069 min
Response: 267852
Conc: 12.50 ng/ml

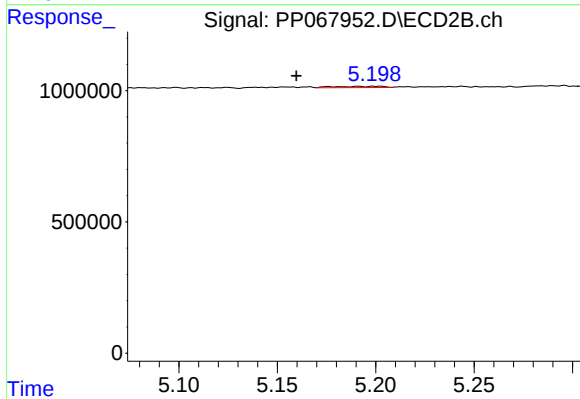

#21 AR-1248-1


R.T.: 5.202 min
Delta R.T.: 0.042 min
Response: 83385
Conc: 3.68 ng/ml

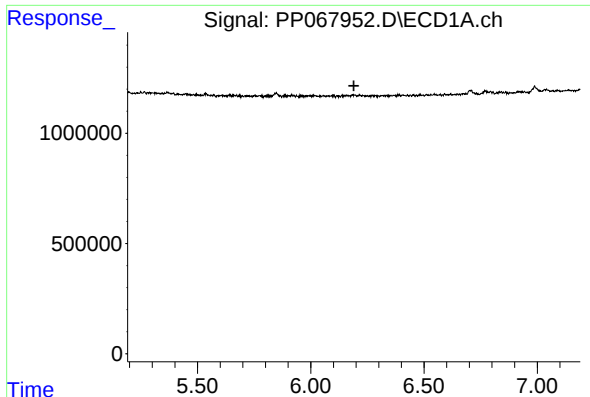

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

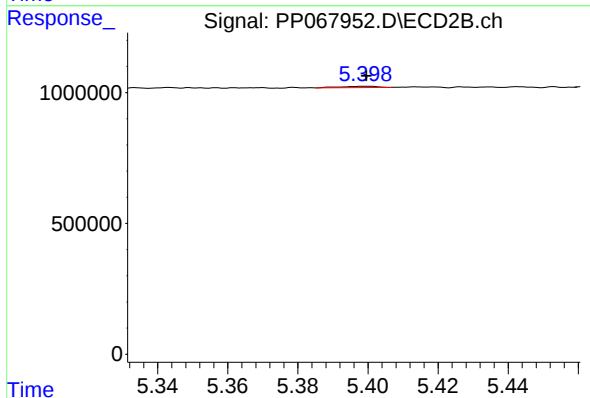


#22 AR-1248-2

R.T.: 5.400 min
Delta R.T.: 0.000 min
Response: 36277
Conc: 1.10 ng/ml

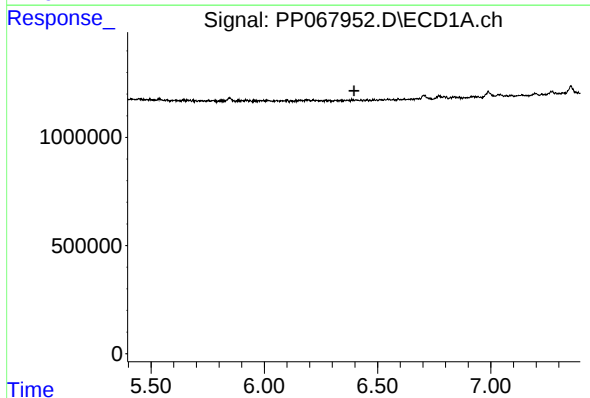


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

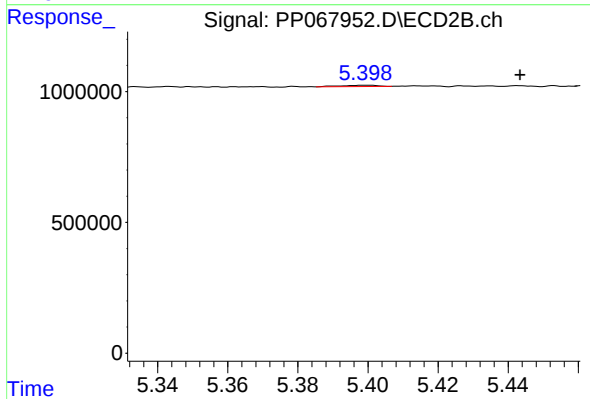

#23 AR-1248-3


R.T.: 5.400 min
Delta R.T.: -0.044 min
Response: 36277
Conc: 1.05 ng/ml

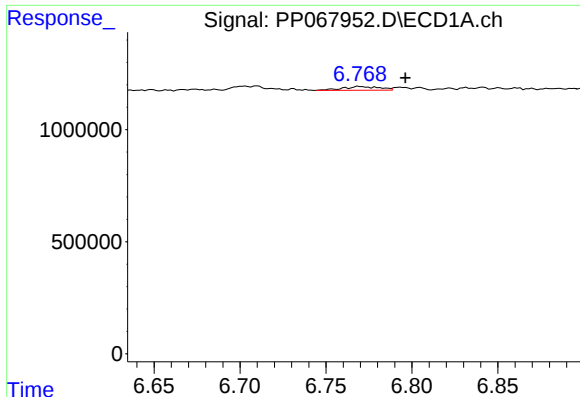

#24 AR-1248-4


R.T.: 6.769 min
Delta R.T.: -0.027 min
Response: 245011
Conc: 6.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

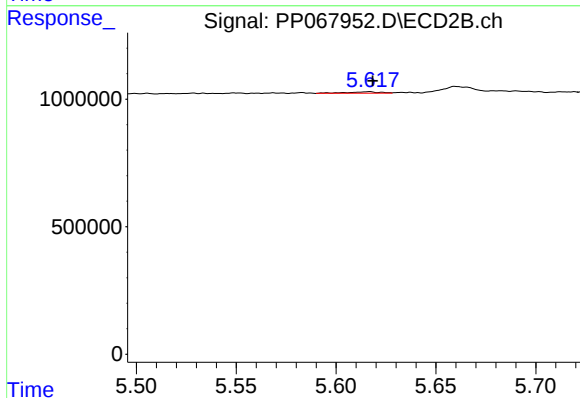


#24 AR-1248-4

R.T.: 5.616 min
Delta R.T.: -0.002 min
Response: 63084
Conc: 1.54 ng/ml

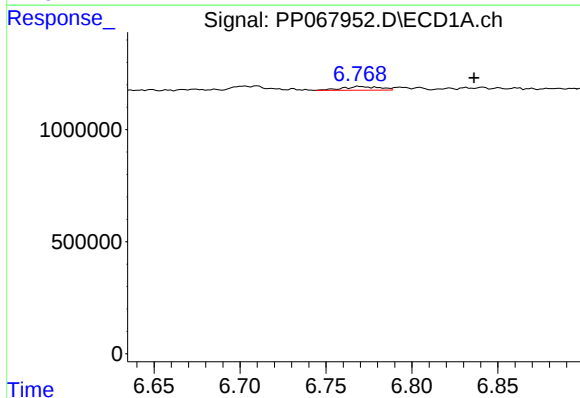


#25 AR-1248-5

R.T.: 6.769 min
Delta R.T.: -0.067 min
Response: 245011
Conc: 6.18 ng/ml

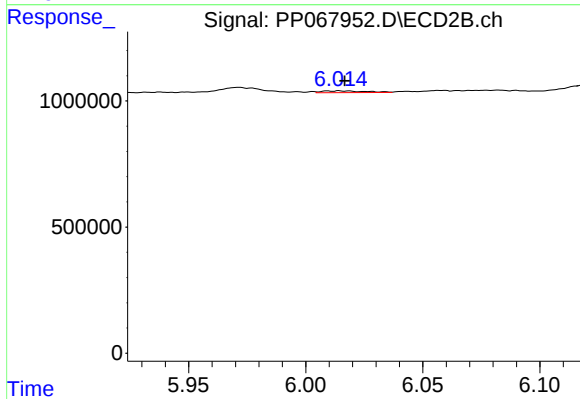

#25 AR-1248-5


R.T.: 6.018 min
Delta R.T.: 0.001 min
Response: 90750
Conc: 2.42 ng/ml

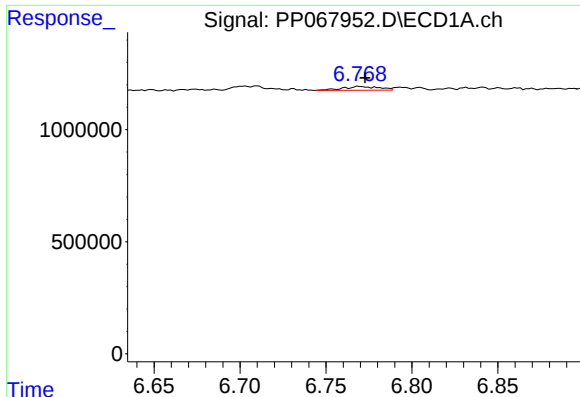

#26 AR-1254-1


R.T.: 6.769 min
Delta R.T.: -0.003 min
Response: 245011
Conc: 5.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

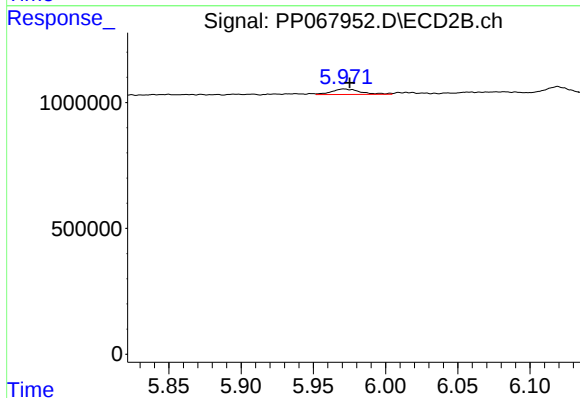


#26 AR-1254-1

R.T.: 5.971 min
Delta R.T.: -0.004 min
Response: 306190
Conc: 5.18 ng/ml

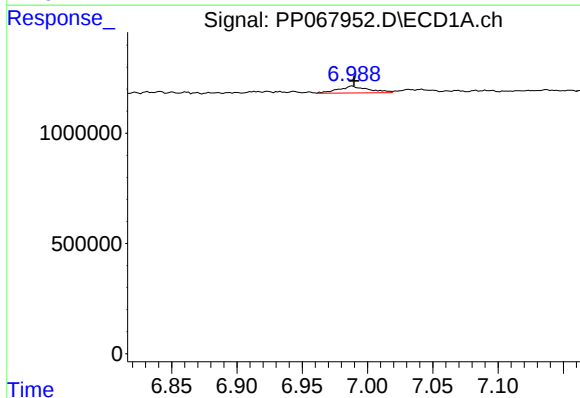


#27 AR-1254-2

R.T.: 6.988 min
Delta R.T.: -0.002 min
Response: 496108
Conc: 7.51 ng/ml

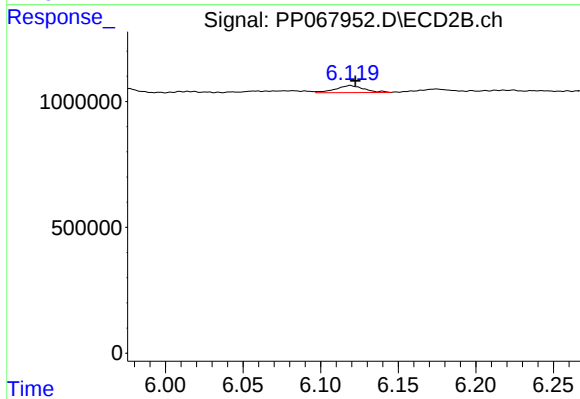

#27 AR-1254-2


R.T.: 6.119 min
Delta R.T.: -0.003 min
Response: 352653
Conc: 6.72 ng/ml

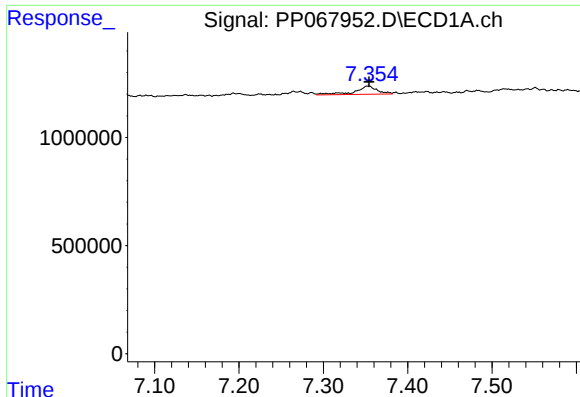

#28 AR-1254-3


R.T.: 7.354 min
Delta R.T.: 0.000 min
Response: 690108
Conc: 9.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

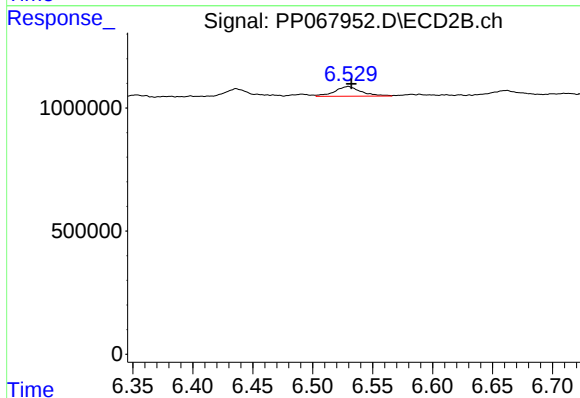


#28 AR-1254-3

R.T.: 6.530 min
Delta R.T.: -0.003 min
Response: 602446
Conc: 7.24 ng/ml

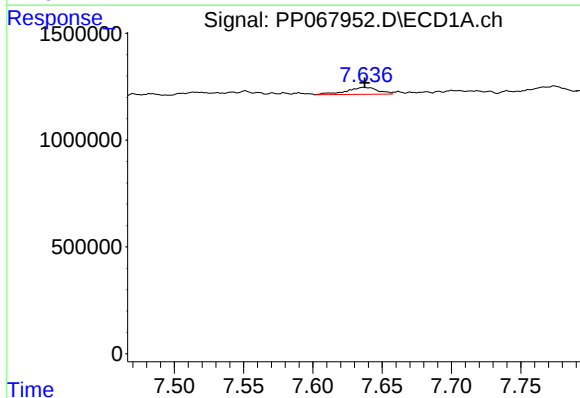


#29 AR-1254-4

R.T.: 7.637 min
Delta R.T.: 0.000 min
Response: 526368
Conc: 10.55 ng/ml

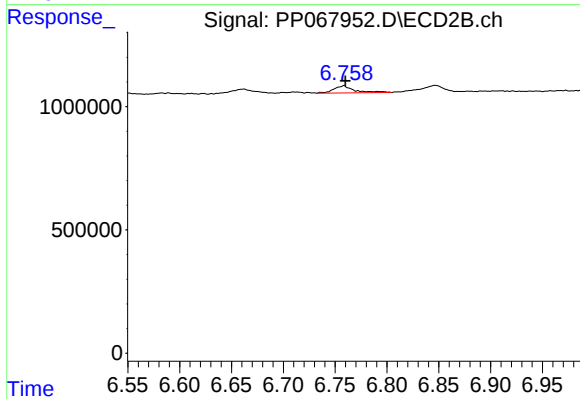

#29 AR-1254-4


R.T.: 6.758 min
Delta R.T.: -0.002 min
Response: 404180
Conc: 8.37 ng/ml

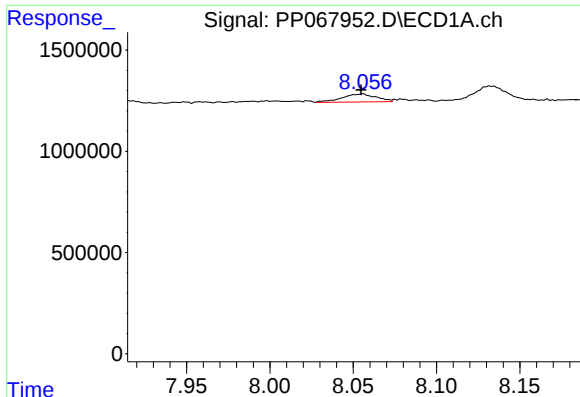

#30 AR-1254-5


R.T.: 8.056 min
Delta R.T.: 0.001 min
Response: 562631
Conc: 9.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

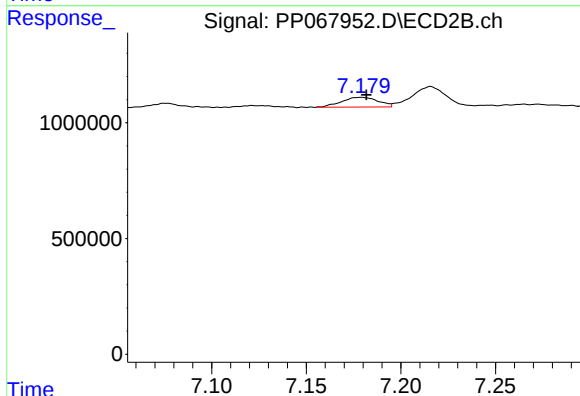


#30 AR-1254-5

R.T.: 7.179 min
Delta R.T.: -0.003 min
Response: 572263
Conc: 7.78 ng/ml

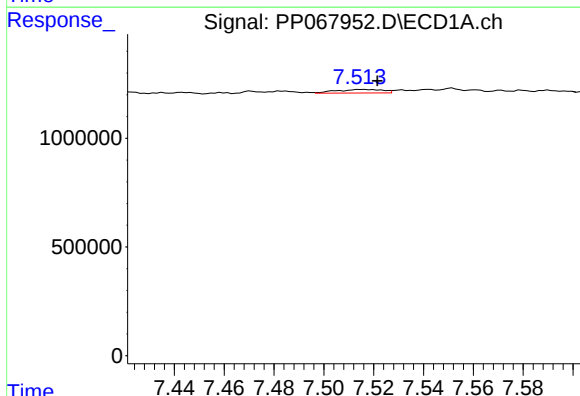


#31 AR-1260-1

R.T.: 7.515 min
Delta R.T.: -0.006 min
Response: 217712
Conc: 4.03 ng/ml

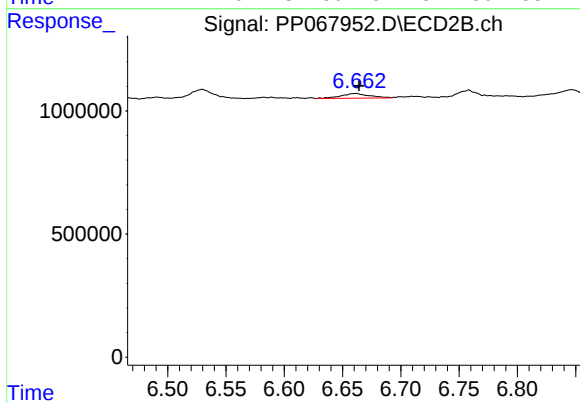

#31 AR-1260-1


R.T.: 6.661 min
Delta R.T.: -0.003 min
Response: 319944
Conc: 5.62 ng/ml

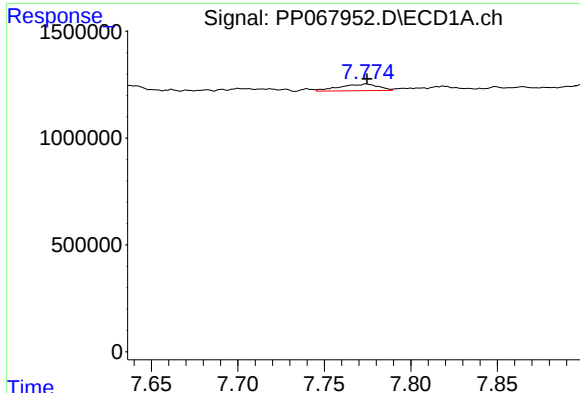

#32 AR-1260-2


R.T.: 7.775 min
Delta R.T.: 0.000 min
Response: 489293
Conc: 7.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

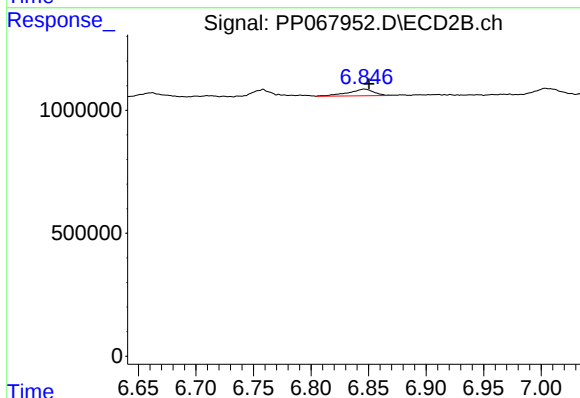


#32 AR-1260-2

R.T.: 6.847 min
Delta R.T.: -0.004 min
Response: 425908
Conc: 6.39 ng/ml

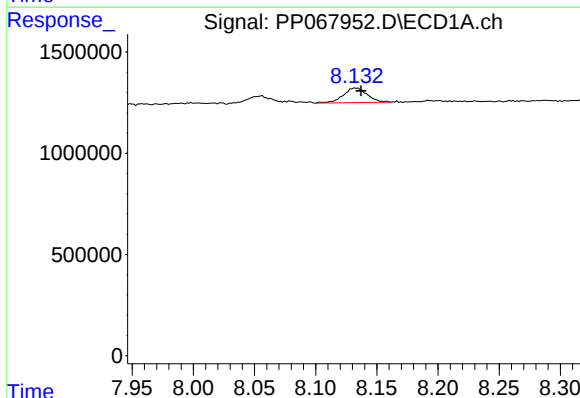


#33 AR-1260-3

R.T.: 8.133 min
Delta R.T.: -0.004 min
Response: 997504
Conc: 19.24 ng/ml

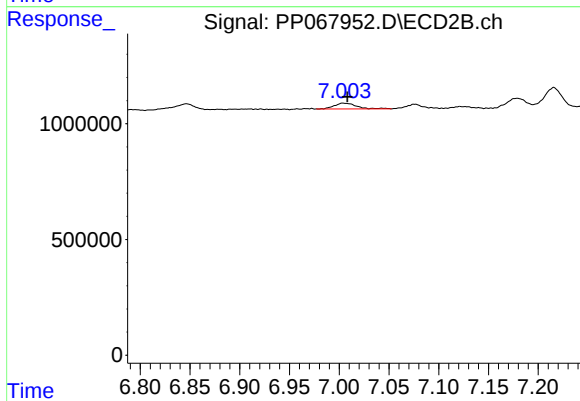

#33 AR-1260-3


R.T.: 7.004 min
Delta R.T.: -0.004 min
Response: 393873
Conc: 6.18 ng/ml

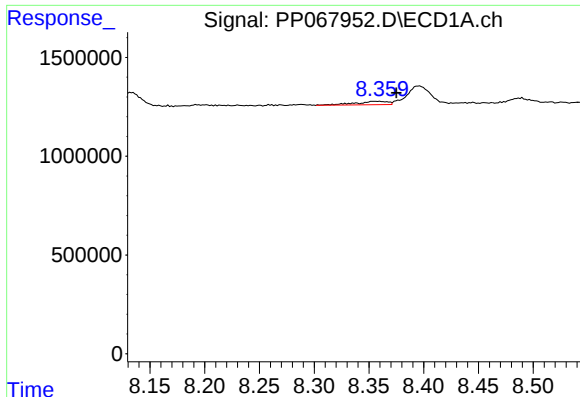

#34 AR-1260-4


R.T.: 8.360 min
Delta R.T.: -0.015 min
Response: 362510
Conc: 6.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

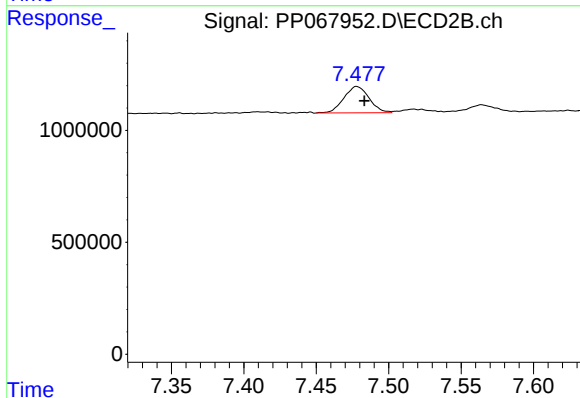


#34 AR-1260-4

R.T.: 7.478 min
Delta R.T.: -0.005 min
Response: 1432097
Conc: 25.90 ng/ml

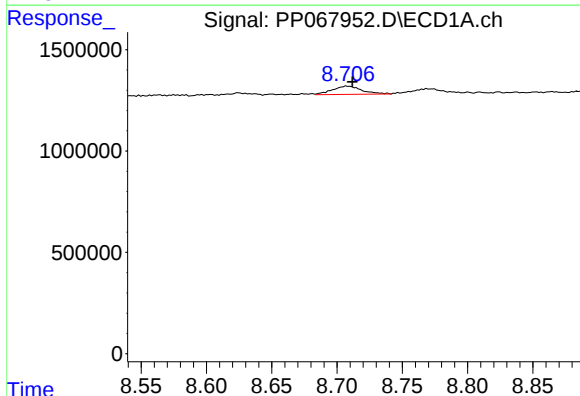


#35 AR-1260-5

R.T.: 8.708 min
Delta R.T.: -0.004 min
Response: 635039
Conc: 5.90 ng/ml

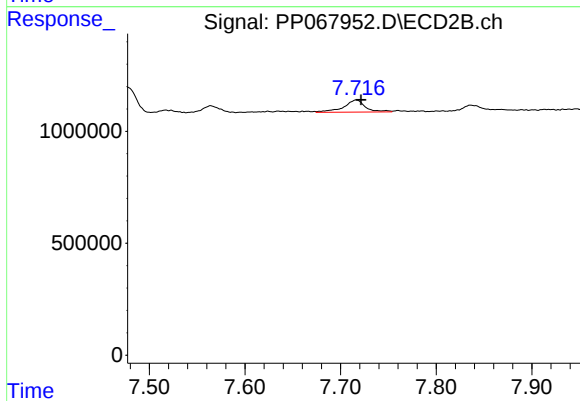

#35 AR-1260-5


R.T.: 7.716 min
Delta R.T.: -0.005 min
Response: 864257
Conc: 7.07 ng/ml

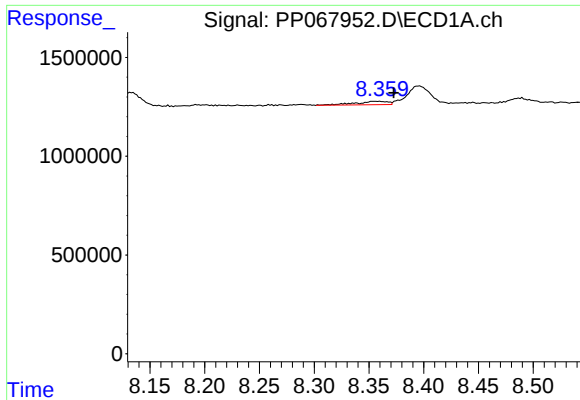

#36 AR-1262-1


R.T.: 8.360 min
Delta R.T.: -0.013 min
Response: 362510
Conc: 5.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

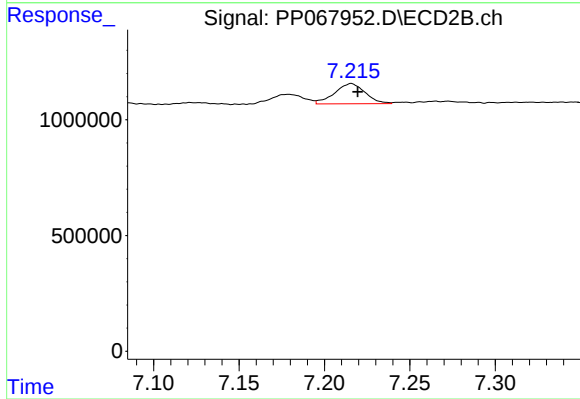


#36 AR-1262-1

R.T.: 7.216 min
Delta R.T.: -0.004 min
Response: 1096642
Conc: 13.94 ng/ml

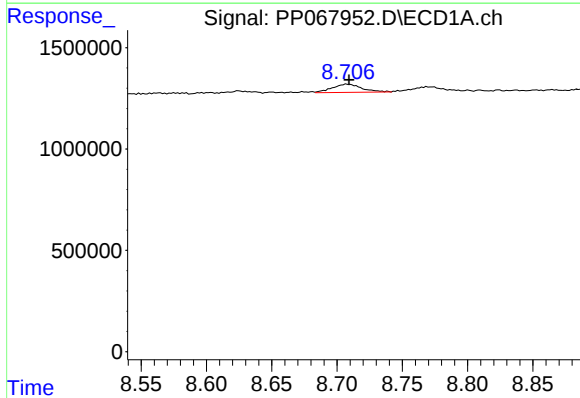


#37 AR-1262-2

R.T.: 8.708 min
Delta R.T.: -0.001 min
Response: 635039
Conc: 5.22 ng/ml

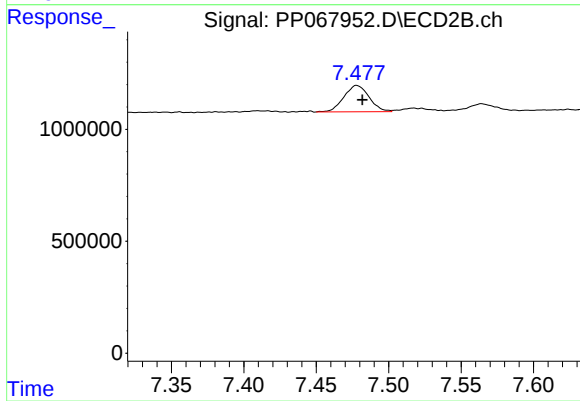

#37 AR-1262-2


R.T.: 7.478 min
Delta R.T.: -0.004 min
Response: 1432097
Conc: 20.18 ng/ml

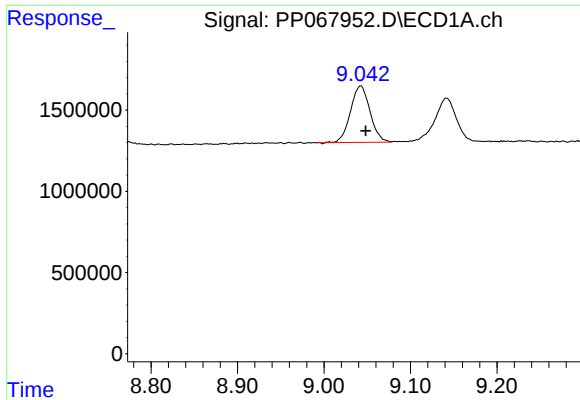

#38 AR-1262-3


R.T.: 9.043 min
Delta R.T.: -0.005 min
Response: 5435260
Conc: 61.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

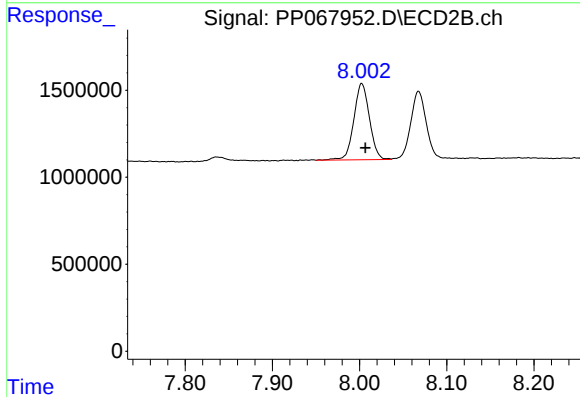


#38 AR-1262-3

R.T.: 8.003 min
Delta R.T.: -0.004 min
Response: 5466953
Conc: 95.74 ng/ml

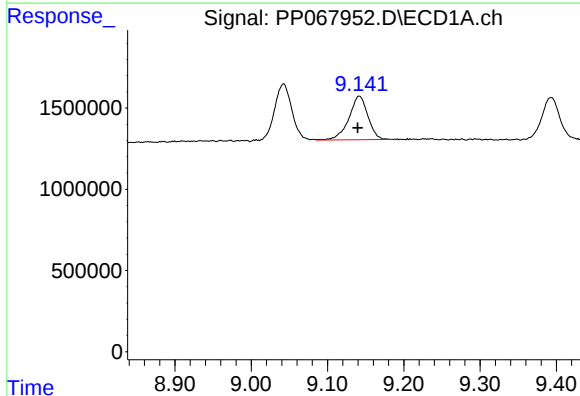


#39 AR-1262-4

R.T.: 9.142 min
Delta R.T.: 0.002 min
Response: 4642317
Conc: 66.37 ng/ml

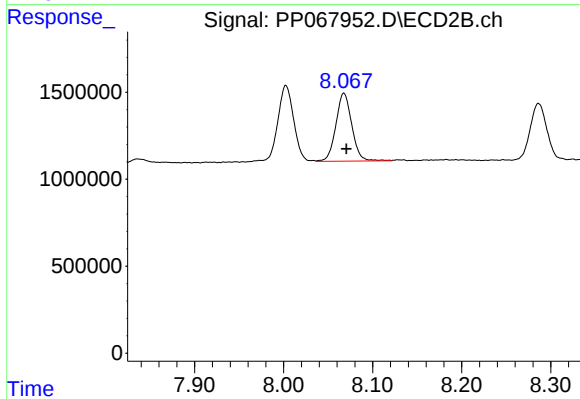

#39 AR-1262-4


R.T.: 8.068 min
Delta R.T.: -0.003 min
Response: 4874537
Conc: 48.53 ng/ml

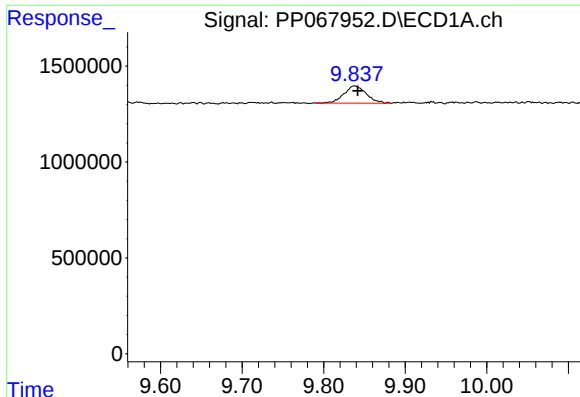

#40 AR-1262-5


R.T.: 9.838 min
Delta R.T.: -0.004 min
Response: 1721639
Conc: 36.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

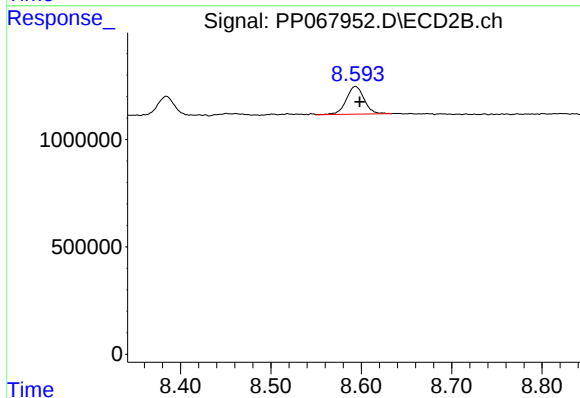


#40 AR-1262-5

R.T.: 8.594 min
Delta R.T.: -0.005 min
Response: 1777433
Conc: 35.54 ng/ml

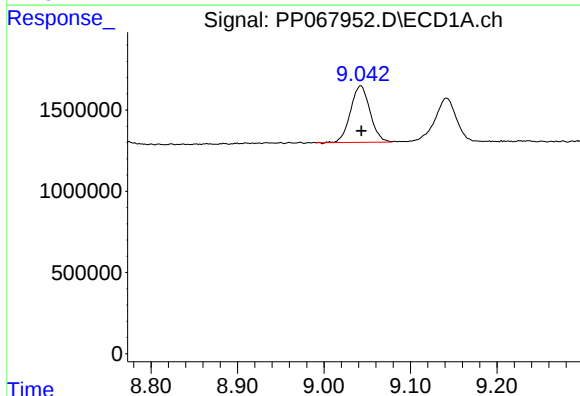


#41 AR-1268-1

R.T.: 9.043 min
Delta R.T.: 0.000 min
Response: 5435260
Conc: 35.61 ng/ml

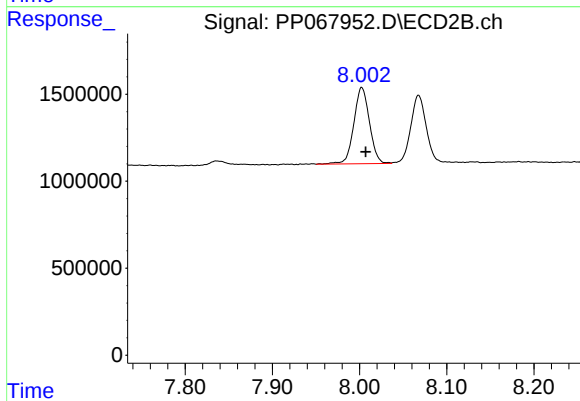

#41 AR-1268-1


R.T.: 8.003 min
Delta R.T.: -0.005 min
Response: 5466953
Conc: 34.35 ng/ml

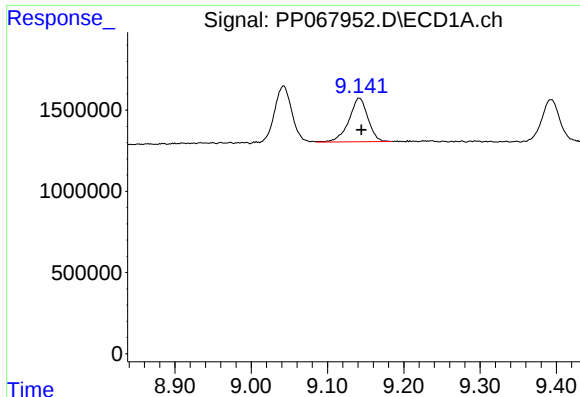

#42 AR-1268-2


R.T.: 9.142 min
Delta R.T.: -0.003 min
Response: 4642317
Conc: 33.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

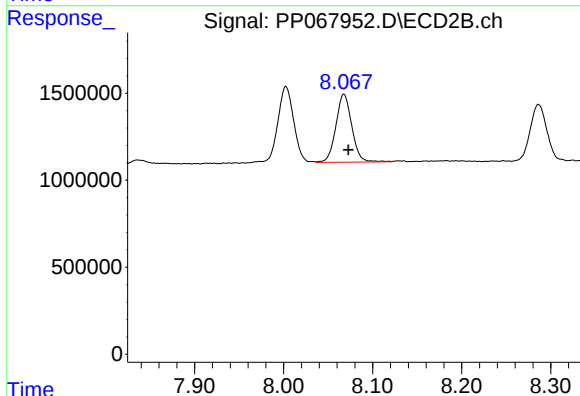


#42 AR-1268-2

R.T.: 8.068 min
Delta R.T.: -0.005 min
Response: 4874537
Conc: 34.04 ng/ml

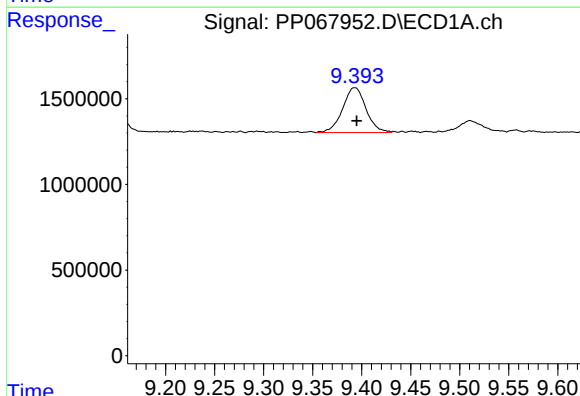


#43 AR-1268-3

R.T.: 9.393 min
Delta R.T.: -0.002 min
Response: 4354560
Conc: 36.01 ng/ml

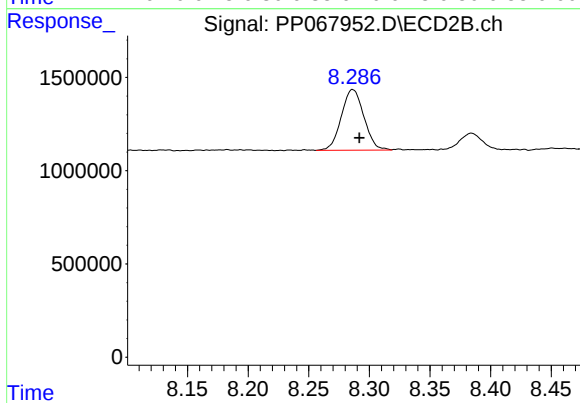

#43 AR-1268-3


R.T.: 8.286 min
Delta R.T.: -0.005 min
Response: 4211869
Conc: 33.03 ng/ml

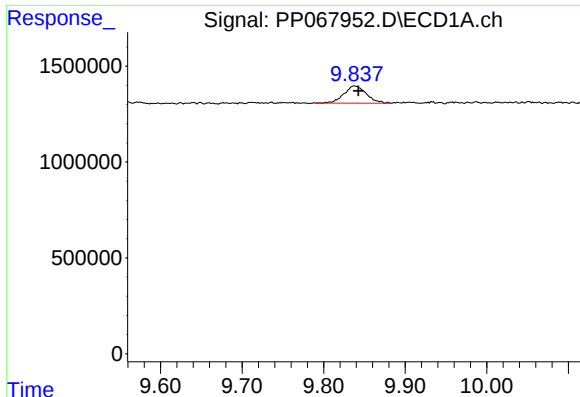

#44 AR-1268-4


R.T.: 9.838 min
Delta R.T.: -0.005 min
Response: 1721639
Conc: 33.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2024

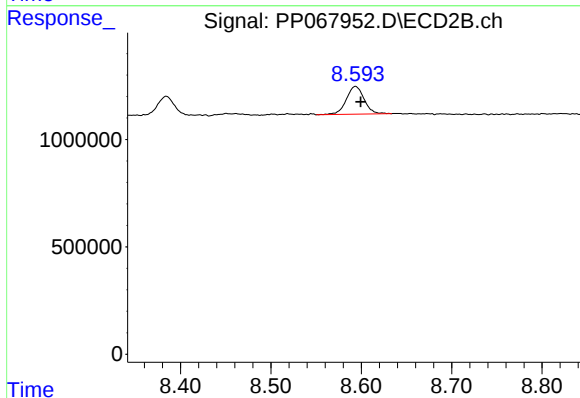


#44 AR-1268-4

R.T.: 8.594 min
Delta R.T.: -0.006 min
Response: 1777433
Conc: 31.47 ng/ml

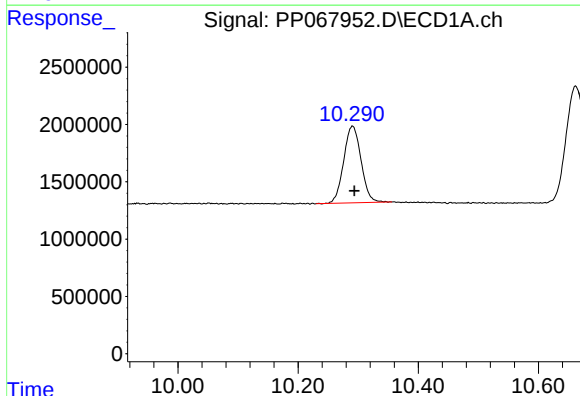

#45 AR-1268-5

R.T.: 10.291 min
Delta R.T.: -0.003 min
Response: 13368709
Conc: 35.80 ng/ml

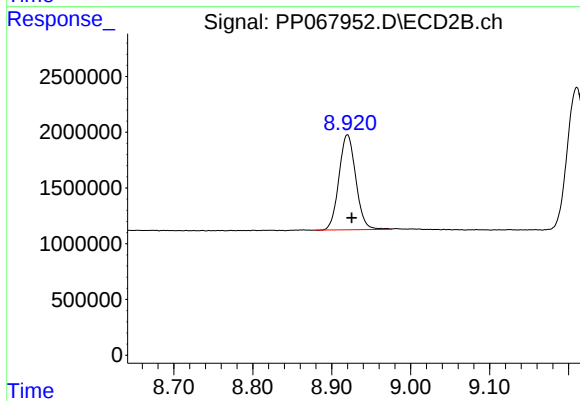

#45 AR-1268-5

R.T.: 8.920 min
Delta R.T.: -0.006 min
Response: 12621167
Conc: 33.39 ng/ml