

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
 Data File : PP067965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2024 05:36
 Operator : YP\AJ
 Sample : P4368-09
 Misc : AR1660 MDL 25 PPB
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT4-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 07:39:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.751	4.049	16359822	17049244	17.674	16.874
2)	SA Decachlor...	10.661	9.209	23007673	20463028	19.984	18.247
Target Compounds							
3)	L1 AR-1016-1	5.914	5.156	851071	919259	25.738	26.274
4)	L1 AR-1016-2	5.939	5.177	1444626	1295258	29.621	26.890
5)	L1 AR-1016-3	6.001	5.357	927983	664920	29.449	24.684
6)	L1 AR-1016-4	6.099	5.396	744967	639396	28.938	26.547
7)	L1 AR-1016-5	6.393	5.616	720842	761257	26.632	25.033
8)	L2 AR-1221-1	0.000	4.260	0	111211	N.D.	8.444 #
9)	L2 AR-1221-2	5.062	4.357	385655	442151	40.764	44.387
10)	L2 AR-1221-3	5.116	4.432	574606	616327	19.877	19.798
11)	L3 AR-1232-1	5.116	4.432	574606	616327	25.136	25.329
12)	L3 AR-1232-2	5.651	5.177	686042	1295258	58.223	57.915
13)	L3 AR-1232-3	5.939	5.357	1444626	664920	64.854	55.671
14)	L3 AR-1232-4	6.099	5.441	744967	739989	66.000	64.172
15)	L3 AR-1232-5	6.188	5.616	771031	761257	84.541	56.598 #
16)	L4 AR-1242-1	5.914	5.156	851071	919259	30.464	31.615
17)	L4 AR-1242-2	5.939	5.177	1444626	1295258	35.552	32.262
18)	L4 AR-1242-3	6.001	5.357	927983	664920	34.415	29.559
19)	L4 AR-1242-4	6.099	5.441	744967	739989	34.730	31.174
20)	L4 AR-1242-5	6.828	5.972	162870	870282	6.751	30.377 #
21)	L5 AR-1248-1	5.914	5.156	851071	919259	39.727	40.561
22)	L5 AR-1248-2	6.188	5.396	771031	639396	22.936	19.320
23)	L5 AR-1248-3	6.393	5.441	720842	739989	19.681	21.465
24)	L5 AR-1248-4	6.794	5.616	332295	761257	8.215	18.587 #
25)	L5 AR-1248-5	6.828	6.012	162870	203957	4.107	5.447 #
26)	L6 AR-1254-1	6.770	5.972	882657	870282	19.710	14.730 #
27)	L6 AR-1254-2	6.987	6.119	609703	688204	9.224	13.118 #
28)	L6 AR-1254-3	7.353	6.543	546670	1576524	7.871	18.947 #
29)	L6 AR-1254-4	7.637	6.757	442910	204926	8.875	4.245 #
30)	L6 AR-1254-5	8.051	7.176	2497050	2214985	42.114	30.115 #
31)	L7 AR-1260-1	7.517	6.659	1549666	1759157	28.685	30.883
32)	L7 AR-1260-2	7.770	6.845	1863670	2060834	29.455	30.895
33)	L7 AR-1260-3	8.131	7.004	1474442	1899730	28.437	29.823
34)	L7 AR-1260-4	8.370	7.477	2023384	1529544	33.614	27.663
35)	L7 AR-1260-5	8.706	7.715	2995495	3301450	27.810	26.995
36)	L8 AR-1262-1	8.370	7.214	2023384	1642733	28.192	20.880 #
37)	L8 AR-1262-2	8.706	7.477	2995495	1529544	24.638	21.554
38)	L8 AR-1262-3	9.052	8.002	1764071	746993	19.930	13.082 #
39)	L8 AR-1262-4	9.137	8.066	969960	2428475	13.867	24.179 #
40)	L8 AR-1262-5	9.837	8.592	888181	880168	18.982	17.597
41)	L9 AR-1268-1	9.052	8.002	1764071	746993	11.556	4.694 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
Data File : PP067965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 05:36
Operator : YP\AJ
Sample : P4368-09
Misc : AR1660 MDL 25 PPB
ALS Vial : 67 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:39:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm


	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	9.137	8.066	969960	2428475	7.101	16.960 #
43) L9	AR-1268-3	0.000	8.287	0	138845	N.D.	1.089 #
44) L9	AR-1268-4	9.837	8.592	888181	880168	17.477	15.585
45) L9	AR-1268-5	10.293	8.921	329223	262652	0.882	0.695

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-OT4-2024

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

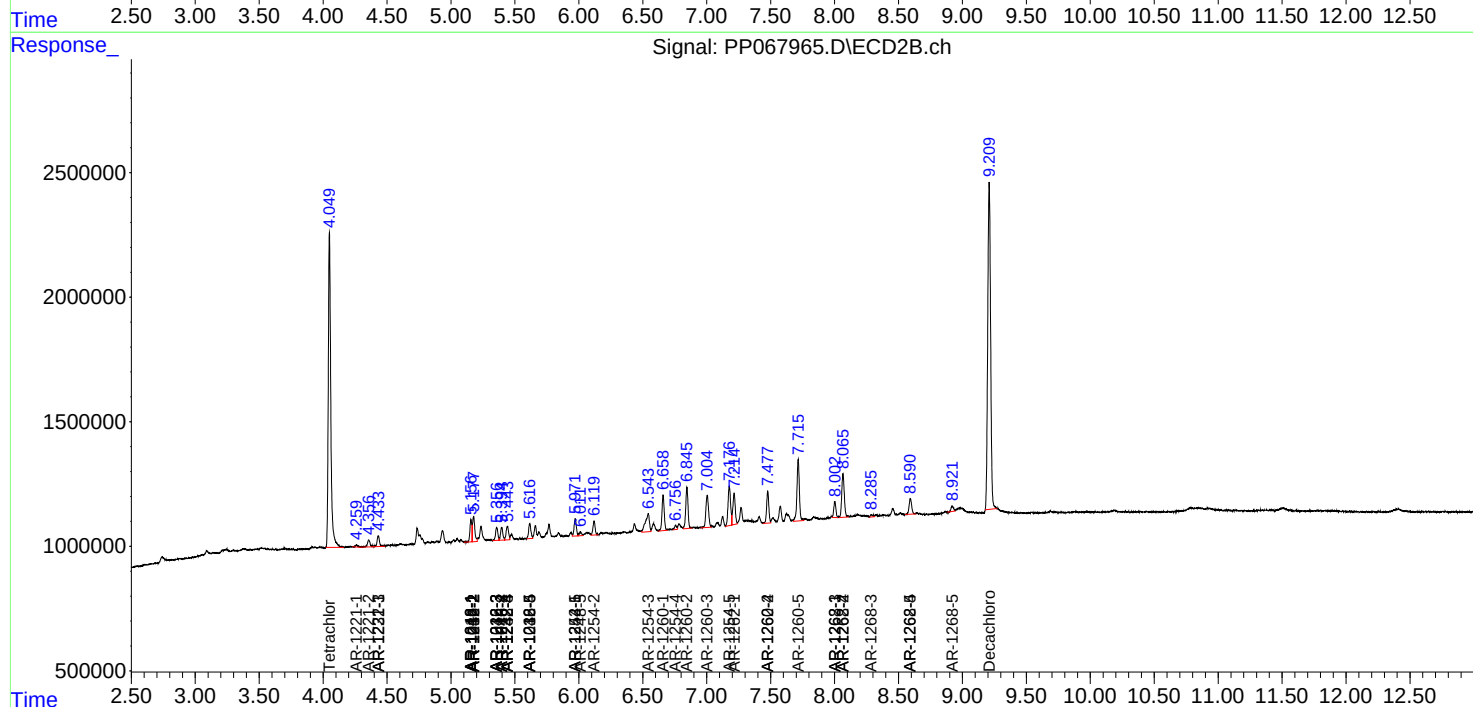


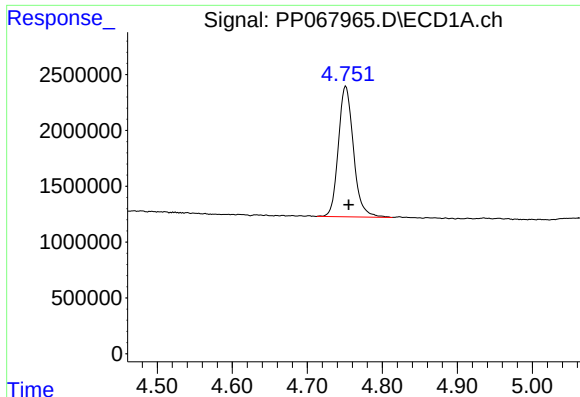

#1 Tetrachloro-m-xylene


R.T.: 4.751 min
Delta R.T.: -0.004 min
Response: 16359822
Conc: 17.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

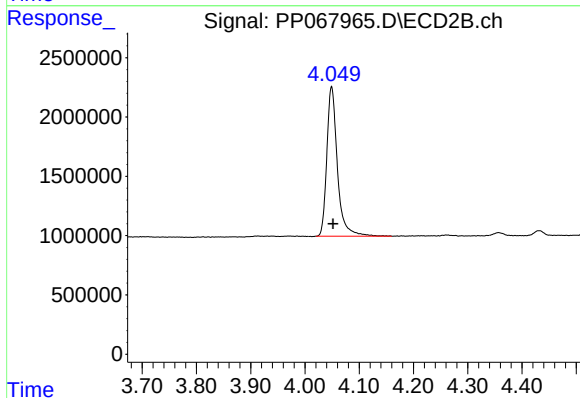


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: -0.003 min
Response: 17049244
Conc: 16.87 ng/ml

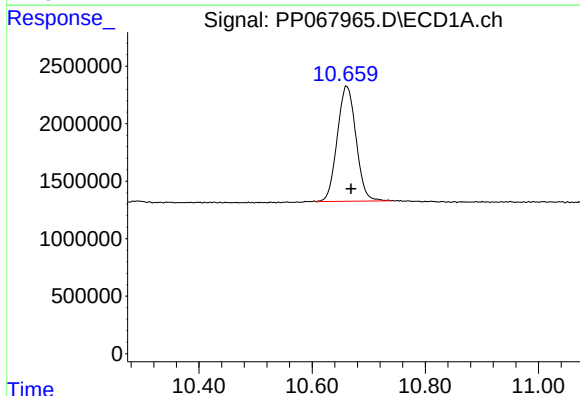


#2 Decachlorobiphenyl

R.T.: 10.661 min
Delta R.T.: -0.008 min
Response: 23007673
Conc: 19.98 ng/ml

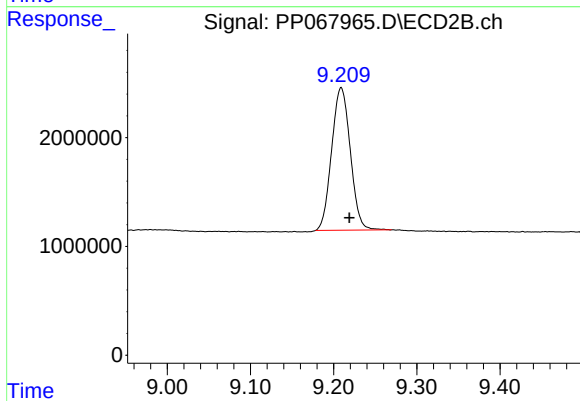

#2 Decachlorobiphenyl


R.T.: 9.209 min
Delta R.T.: -0.010 min
Response: 20463028
Conc: 18.25 ng/ml

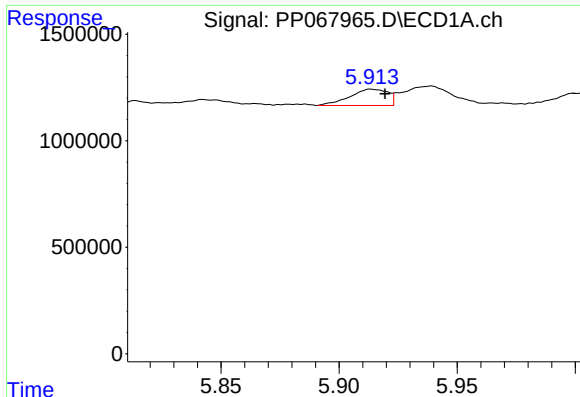

#3 AR-1016-1


R.T.: 5.914 min
Delta R.T.: -0.006 min
Response: 851071
Conc: 25.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

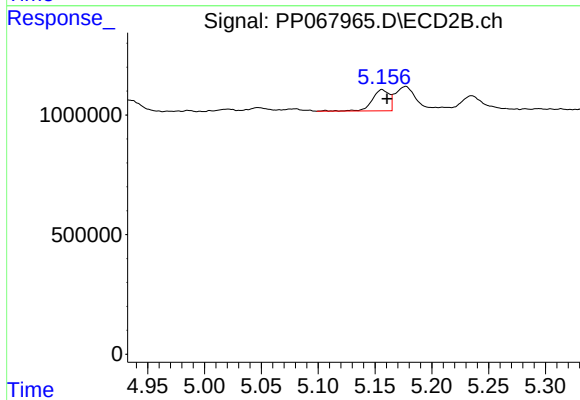


#3 AR-1016-1

R.T.: 5.156 min
Delta R.T.: -0.004 min
Response: 919259
Conc: 26.27 ng/ml

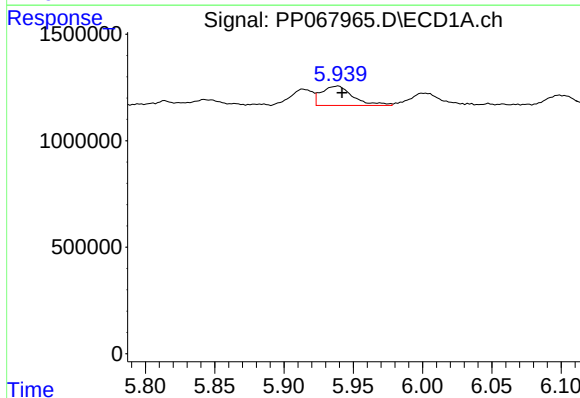


#4 AR-1016-2

R.T.: 5.939 min
Delta R.T.: -0.003 min
Response: 1444626
Conc: 29.62 ng/ml

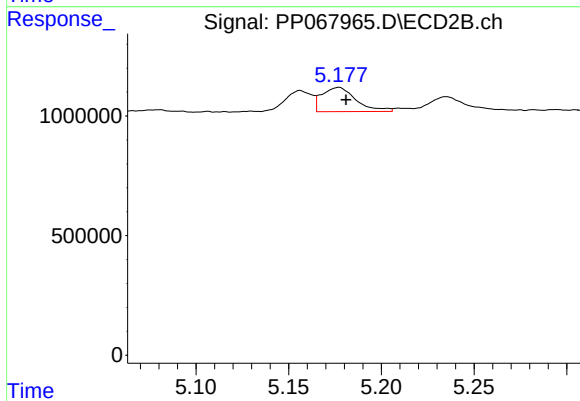

#4 AR-1016-2


R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 1295258
Conc: 26.89 ng/ml

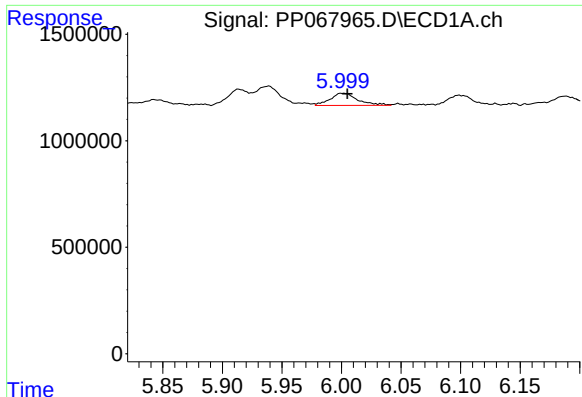

#5 AR-1016-3


R.T.: 6.001 min
Delta R.T.: -0.004 min
Response: 927983
Conc: 29.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

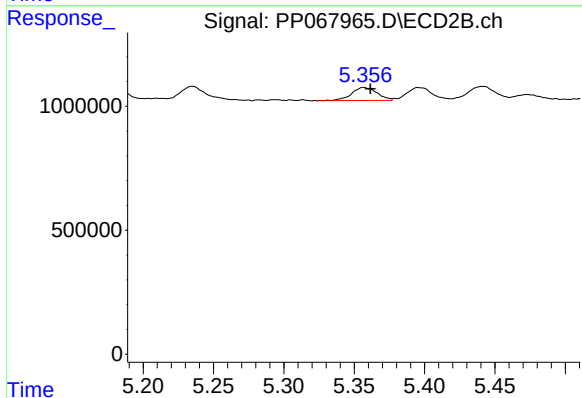


#5 AR-1016-3

R.T.: 5.357 min
Delta R.T.: -0.005 min
Response: 664920
Conc: 24.68 ng/ml

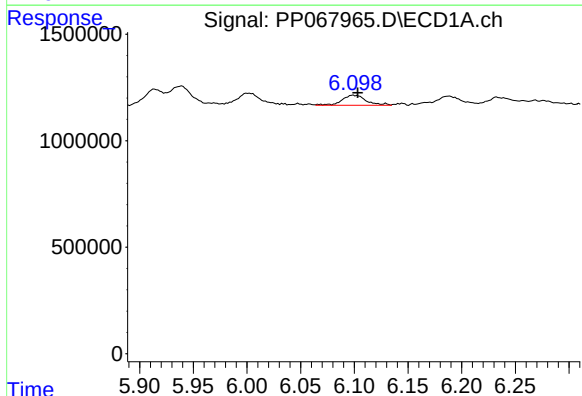


#6 AR-1016-4

R.T.: 6.099 min
Delta R.T.: -0.005 min
Response: 744967
Conc: 28.94 ng/ml

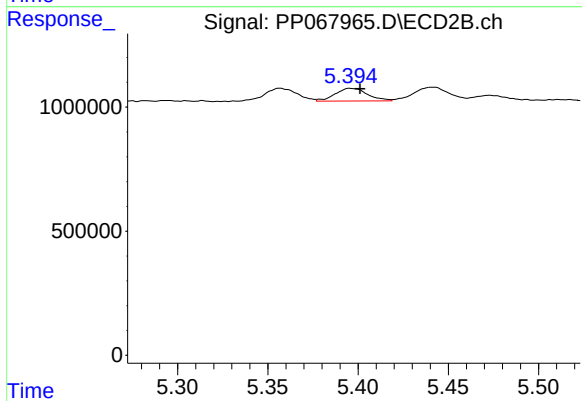

#6 AR-1016-4


R.T.: 5.396 min
Delta R.T.: -0.005 min
Response: 639396
Conc: 26.55 ng/ml

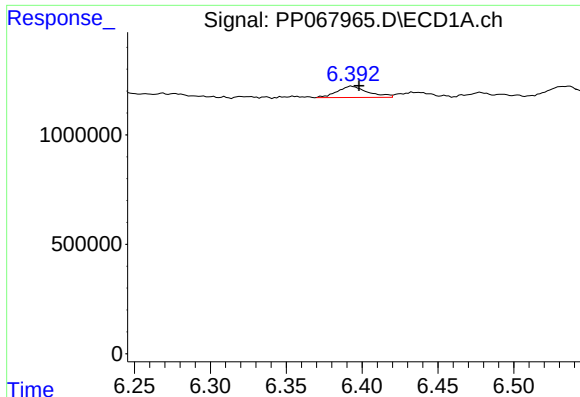

#7 AR-1016-5


R.T.: 6.393 min
Delta R.T.: -0.005 min
Response: 720842
Conc: 26.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

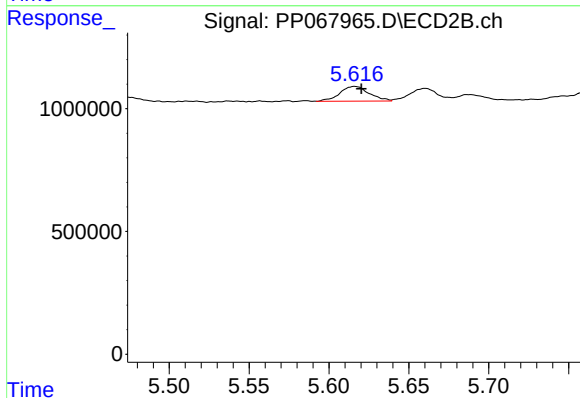


#7 AR-1016-5

R.T.: 5.616 min
Delta R.T.: -0.004 min
Response: 761257
Conc: 25.03 ng/ml

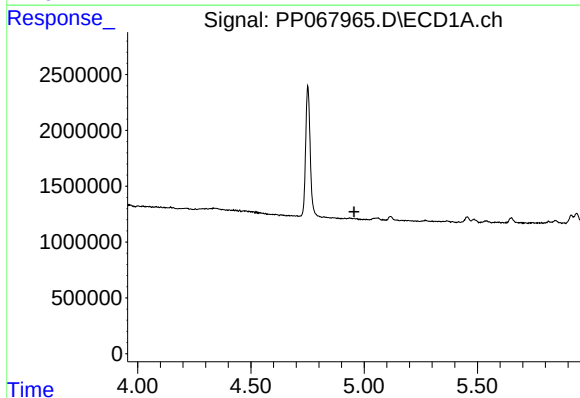


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.955 min
Response: 0
Conc: N.D.

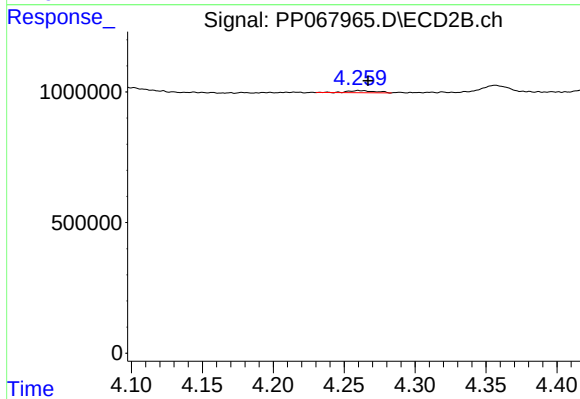

#8 AR-1221-1


R.T.: 4.260 min
Delta R.T.: -0.006 min
Response: 111211
Conc: 8.44 ng/ml

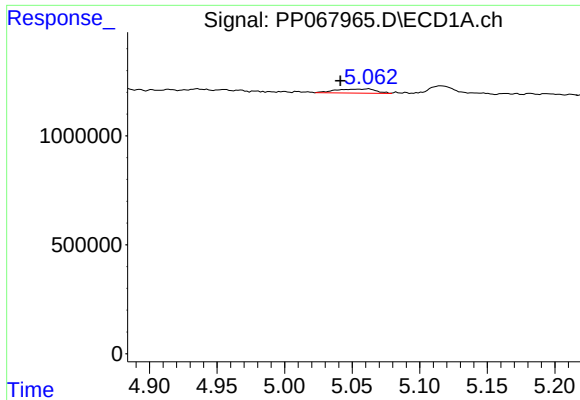

#9 AR-1221-2


R.T.: 5.062 min
Delta R.T.: 0.021 min
Response: 385655
Conc: 40.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

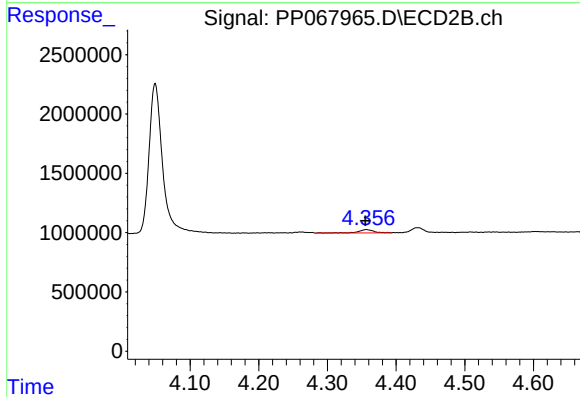


#9 AR-1221-2

R.T.: 4.357 min
Delta R.T.: 0.001 min
Response: 442151
Conc: 44.39 ng/ml

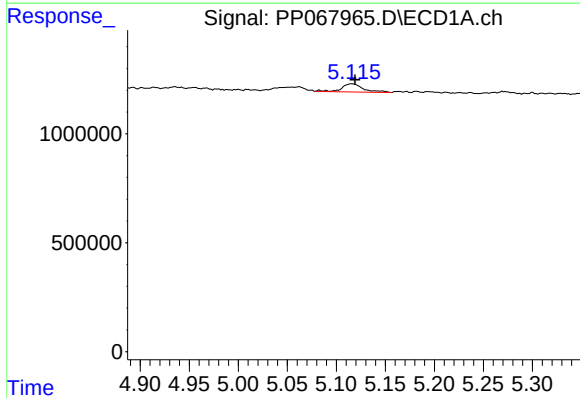


#10 AR-1221-3

R.T.: 5.116 min
Delta R.T.: -0.003 min
Response: 574606
Conc: 19.88 ng/ml

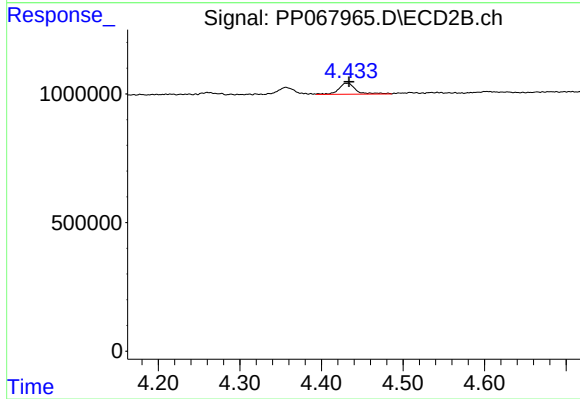

#10 AR-1221-3


R.T.: 4.432 min
Delta R.T.: -0.002 min
Response: 616327
Conc: 19.80 ng/ml

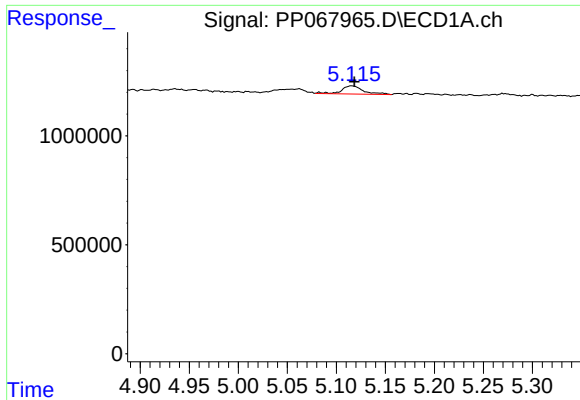

#11 AR-1232-1


R.T.: 5.116 min
Delta R.T.: -0.002 min
Response: 574606
Conc: 25.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

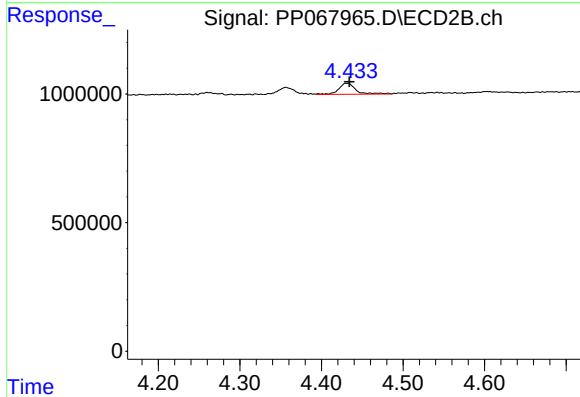


#11 AR-1232-1

R.T.: 4.432 min
Delta R.T.: -0.003 min
Response: 616327
Conc: 25.33 ng/ml

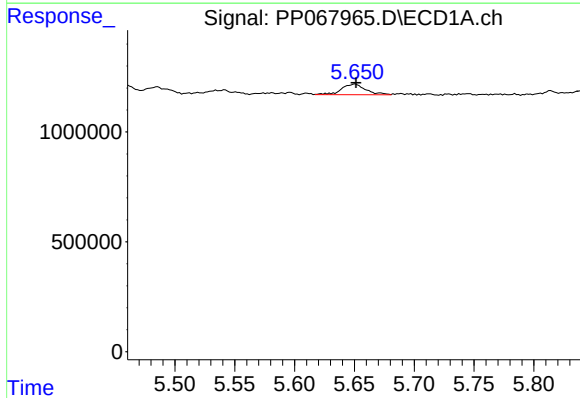


#12 AR-1232-2

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 686042
Conc: 58.22 ng/ml

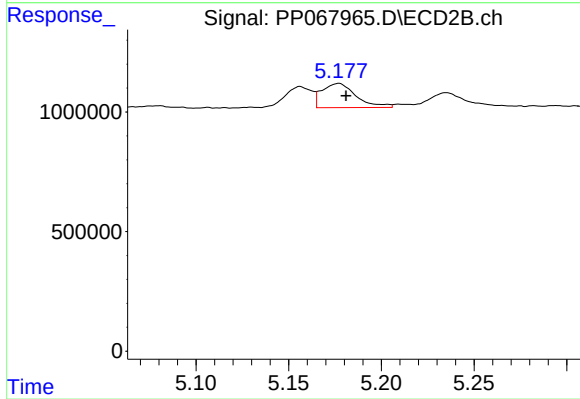

#12 AR-1232-2


R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 1295258
Conc: 57.91 ng/ml

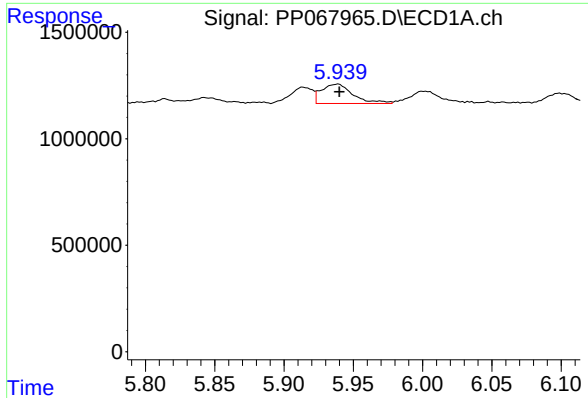

#13 AR-1232-3


R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 1444626
Conc: 64.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

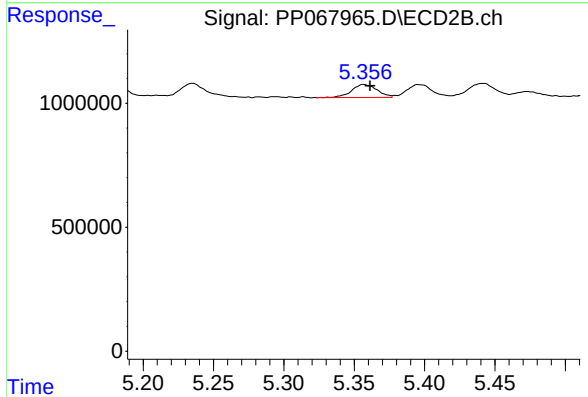


#13 AR-1232-3

R.T.: 5.357 min
Delta R.T.: -0.005 min
Response: 664920
Conc: 55.67 ng/ml

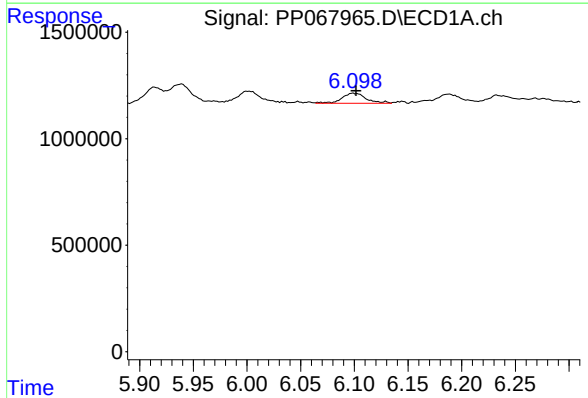


#14 AR-1232-4

R.T.: 6.099 min
Delta R.T.: -0.003 min
Response: 744967
Conc: 66.00 ng/ml

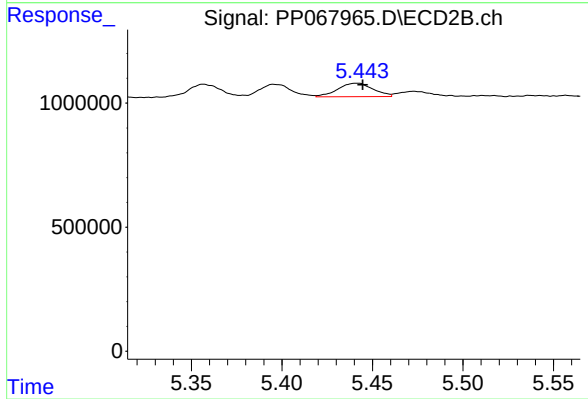

#14 AR-1232-4


R.T.: 5.441 min
Delta R.T.: -0.003 min
Response: 739989
Conc: 64.17 ng/ml

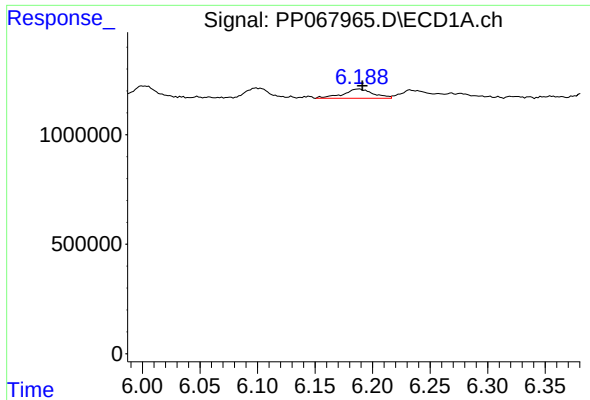

#15 AR-1232-5


R.T.: 6.188 min
Delta R.T.: -0.003 min
Response: 771031
Conc: 84.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

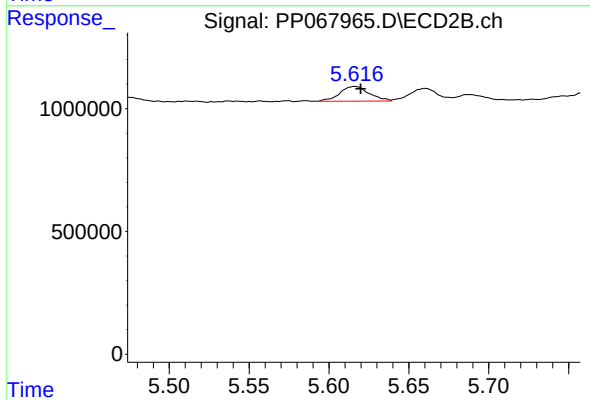


#15 AR-1232-5

R.T.: 5.616 min
Delta R.T.: -0.004 min
Response: 761257
Conc: 56.60 ng/ml

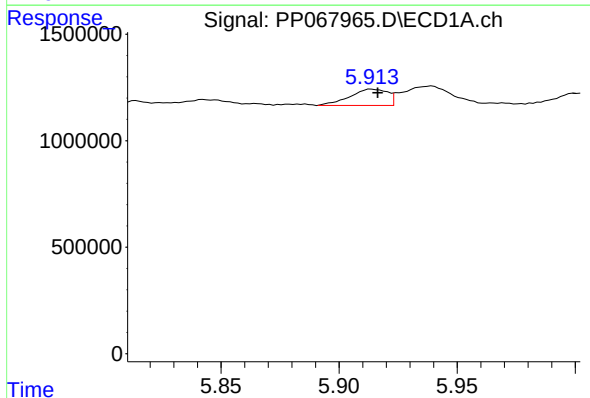


#16 AR-1242-1

R.T.: 5.914 min
Delta R.T.: -0.003 min
Response: 851071
Conc: 30.46 ng/ml

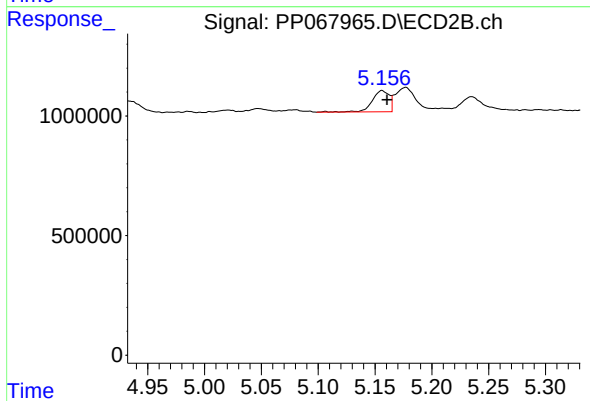

#16 AR-1242-1


R.T.: 5.156 min
Delta R.T.: -0.004 min
Response: 919259
Conc: 31.62 ng/ml

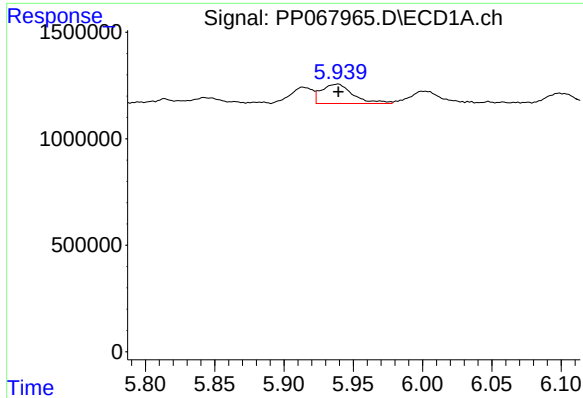

#17 AR-1242-2


R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 1444626
Conc: 35.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

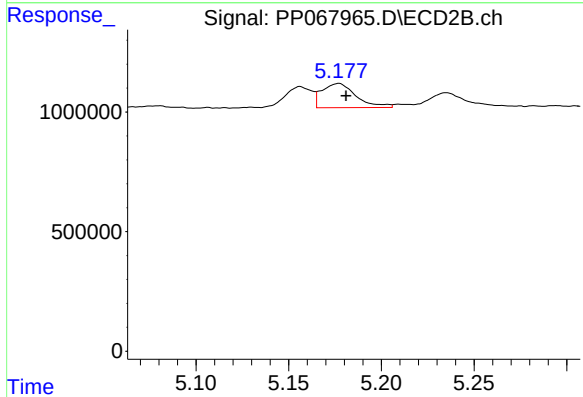


#17 AR-1242-2

R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 1295258
Conc: 32.26 ng/ml

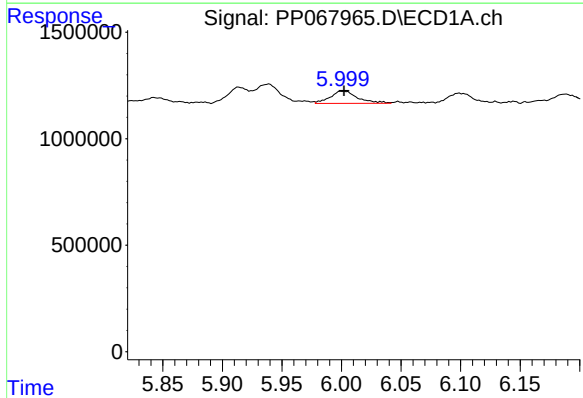


#18 AR-1242-3

R.T.: 6.001 min
Delta R.T.: -0.001 min
Response: 927983
Conc: 34.41 ng/ml

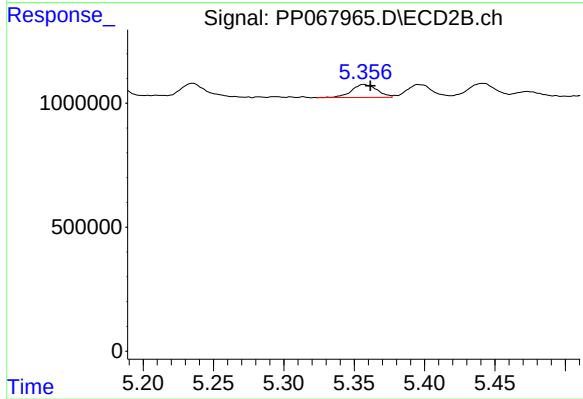

#18 AR-1242-3


R.T.: 5.357 min
Delta R.T.: -0.005 min
Response: 664920
Conc: 29.56 ng/ml

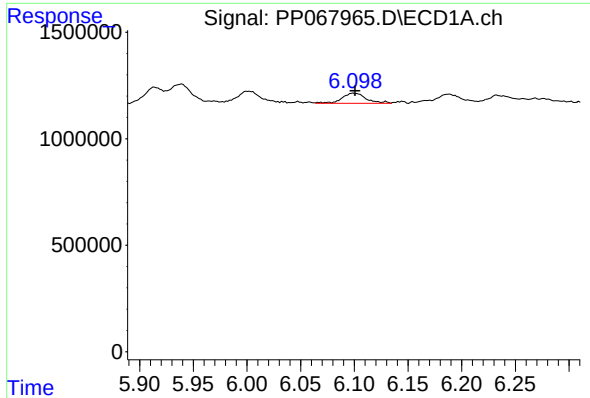

#19 AR-1242-4


R.T.: 6.099 min
Delta R.T.: -0.002 min
Response: 744967
Conc: 34.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

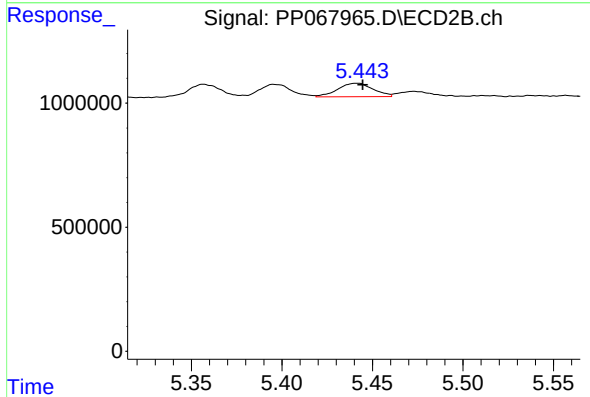


#19 AR-1242-4

R.T.: 5.441 min
Delta R.T.: -0.003 min
Response: 739989
Conc: 31.17 ng/ml

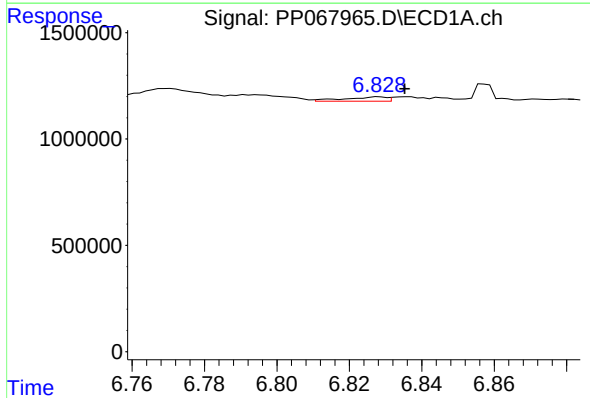


#20 AR-1242-5

R.T.: 6.828 min
Delta R.T.: -0.007 min
Response: 162870
Conc: 6.75 ng/ml

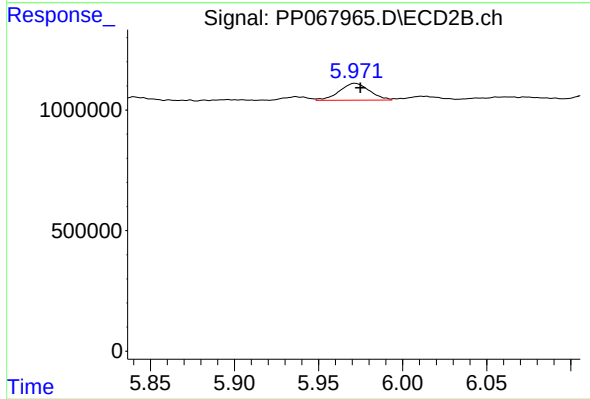

#20 AR-1242-5


R.T.: 5.972 min
Delta R.T.: -0.003 min
Response: 870282
Conc: 30.38 ng/ml

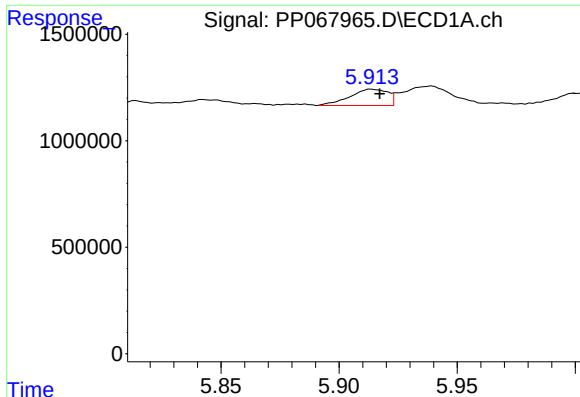

#21 AR-1248-1


R.T.: 5.914 min
Delta R.T.: -0.003 min
Response: 851071
Conc: 39.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

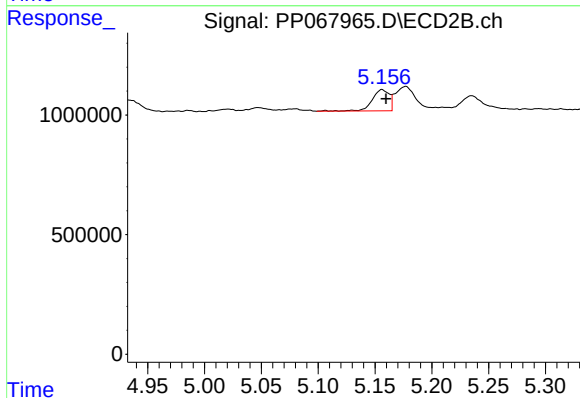


#21 AR-1248-1

R.T.: 5.156 min
Delta R.T.: -0.003 min
Response: 919259
Conc: 40.56 ng/ml

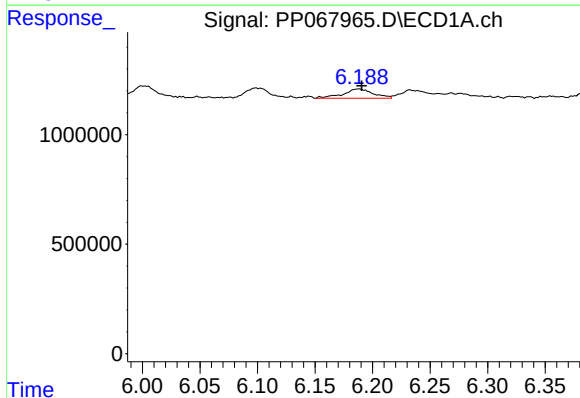


#22 AR-1248-2

R.T.: 6.188 min
Delta R.T.: -0.002 min
Response: 771031
Conc: 22.94 ng/ml

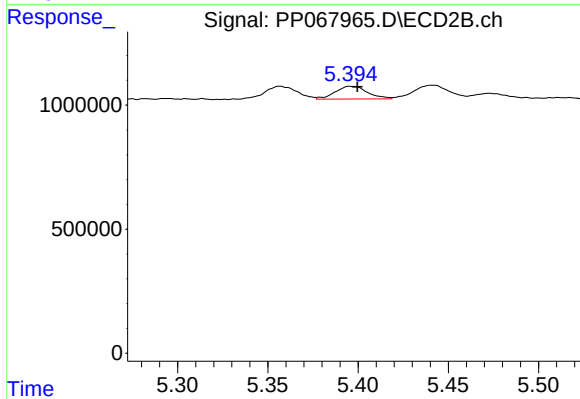

#22 AR-1248-2


R.T.: 5.396 min
Delta R.T.: -0.004 min
Response: 639396
Conc: 19.32 ng/ml

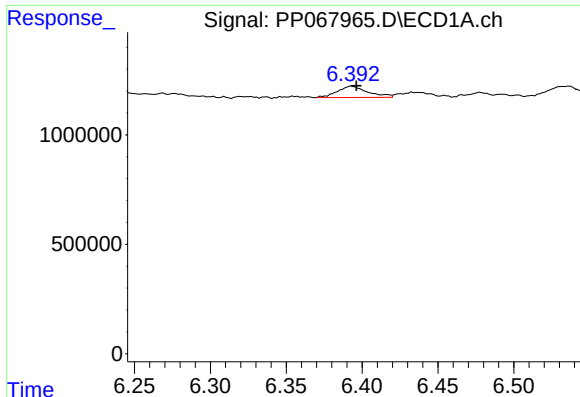

#23 AR-1248-3


R.T.: 6.393 min
Delta R.T.: -0.003 min
Response: 720842
Conc: 19.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

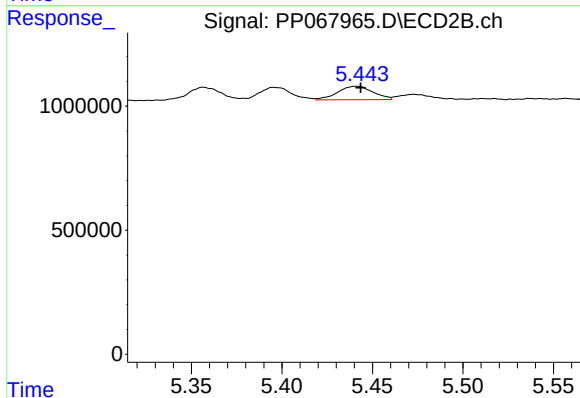


#23 AR-1248-3

R.T.: 5.441 min
Delta R.T.: -0.002 min
Response: 739989
Conc: 21.46 ng/ml

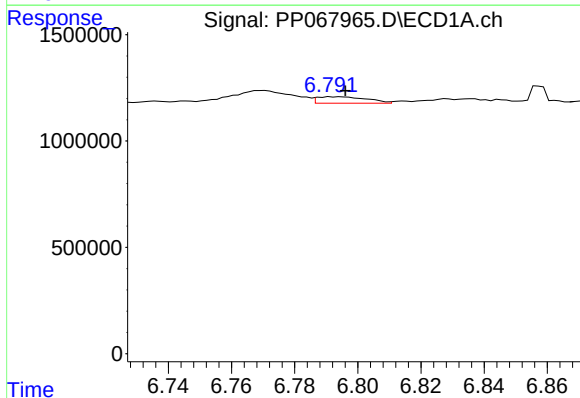


#24 AR-1248-4

R.T.: 6.794 min
Delta R.T.: -0.002 min
Response: 332295
Conc: 8.21 ng/ml

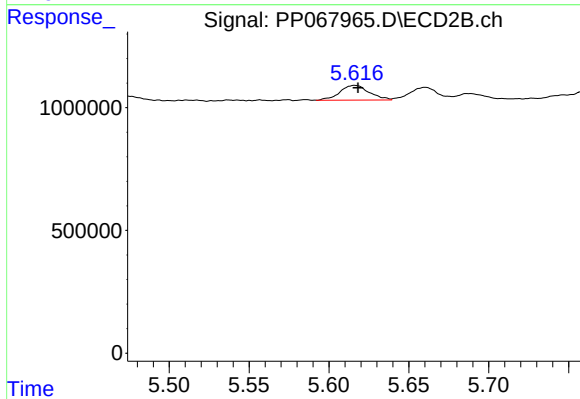

#24 AR-1248-4


R.T.: 5.616 min
Delta R.T.: -0.002 min
Response: 761257
Conc: 18.59 ng/ml

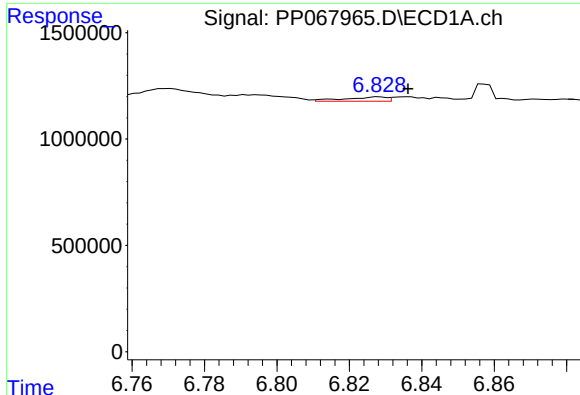

#25 AR-1248-5


R.T.: 6.828 min
Delta R.T.: -0.008 min
Response: 162870
Conc: 4.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

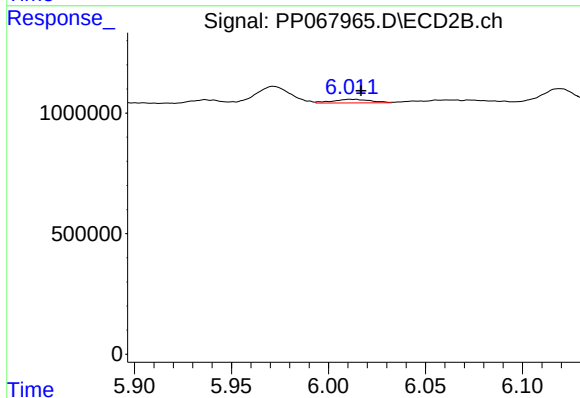


#25 AR-1248-5

R.T.: 6.012 min
Delta R.T.: -0.004 min
Response: 203957
Conc: 5.45 ng/ml

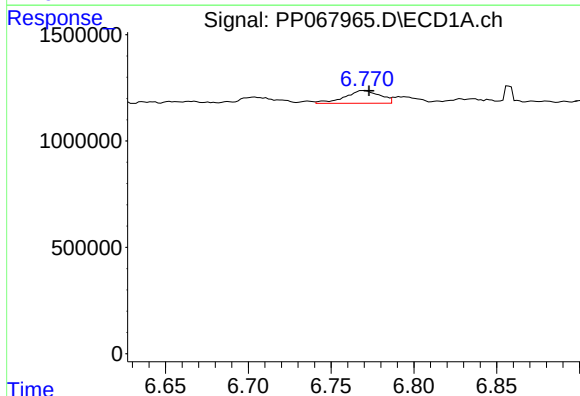


#26 AR-1254-1

R.T.: 6.770 min
Delta R.T.: -0.003 min
Response: 882657
Conc: 19.71 ng/ml

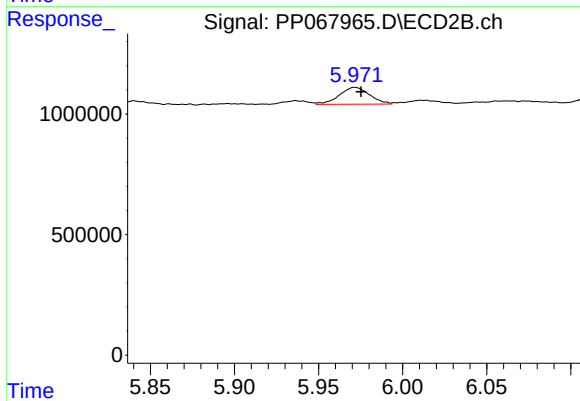

#26 AR-1254-1


R.T.: 5.972 min
Delta R.T.: -0.004 min
Response: 870282
Conc: 14.73 ng/ml

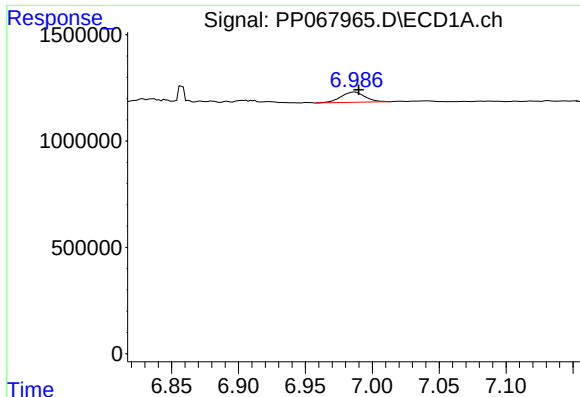

#27 AR-1254-2


R.T.: 6.987 min
Delta R.T.: -0.003 min
Response: 609703
Conc: 9.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

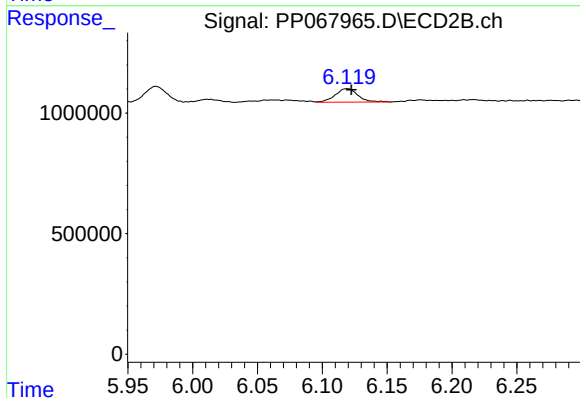


#27 AR-1254-2

R.T.: 6.119 min
Delta R.T.: -0.003 min
Response: 688204
Conc: 13.12 ng/ml

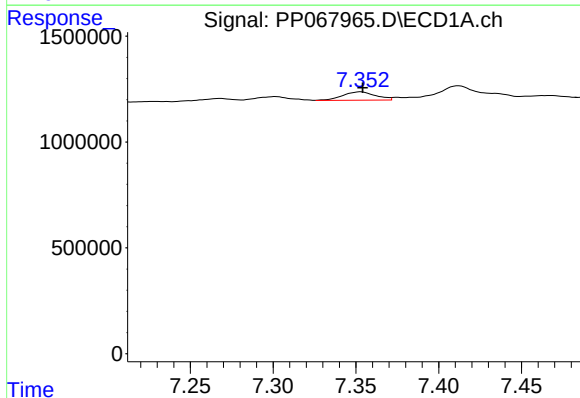


#28 AR-1254-3

R.T.: 7.353 min
Delta R.T.: -0.001 min
Response: 546670
Conc: 7.87 ng/ml

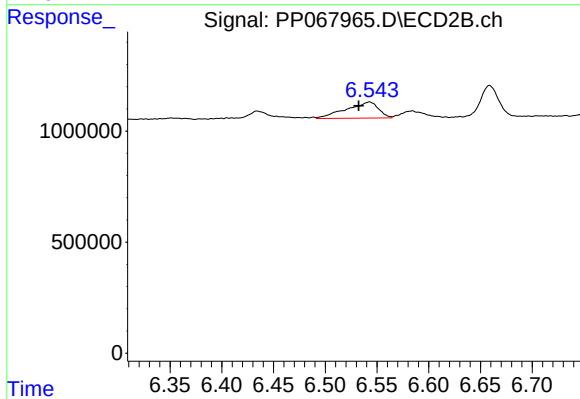

#28 AR-1254-3


R.T.: 6.543 min
Delta R.T.: 0.011 min
Response: 1576524
Conc: 18.95 ng/ml

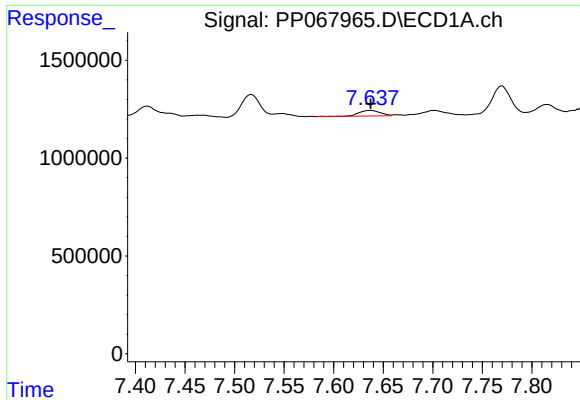

#29 AR-1254-4


R.T.: 7.637 min
Delta R.T.: 0.000 min
Response: 442910
Conc: 8.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

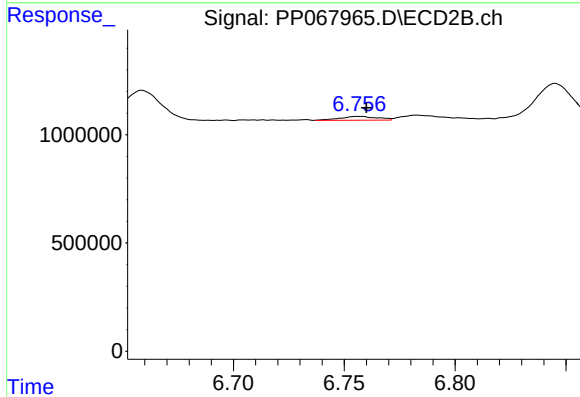


#29 AR-1254-4

R.T.: 6.757 min
Delta R.T.: -0.003 min
Response: 204926
Conc: 4.25 ng/ml

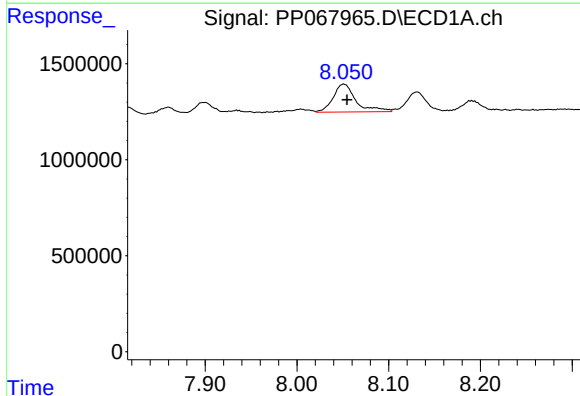


#30 AR-1254-5

R.T.: 8.051 min
Delta R.T.: -0.003 min
Response: 2497050
Conc: 42.11 ng/ml

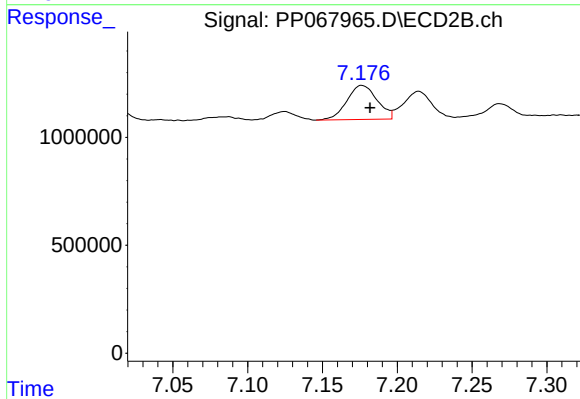

#30 AR-1254-5


R.T.: 7.176 min
Delta R.T.: -0.005 min
Response: 2214985
Conc: 30.11 ng/ml

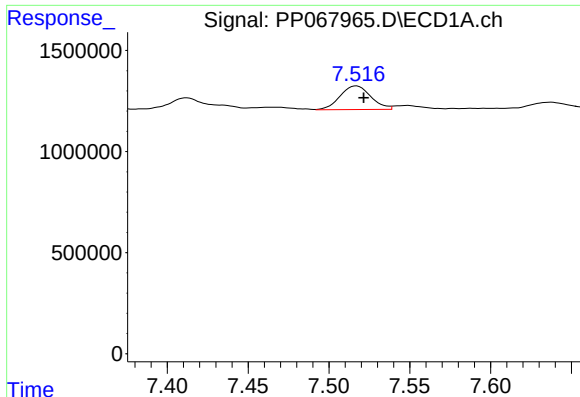

#31 AR-1260-1


R.T.: 7.517 min
Delta R.T.: -0.004 min
Response: 1549666
Conc: 28.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

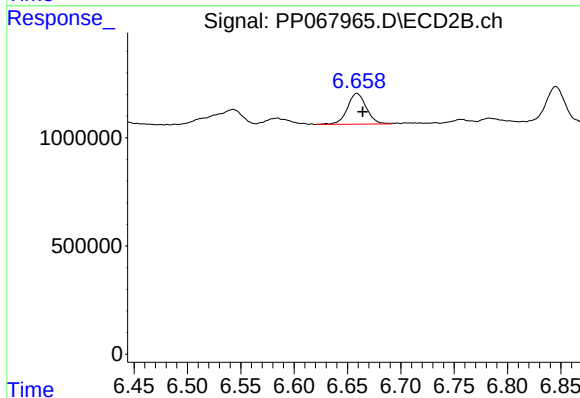


#31 AR-1260-1

R.T.: 6.659 min
Delta R.T.: -0.005 min
Response: 1759157
Conc: 30.88 ng/ml

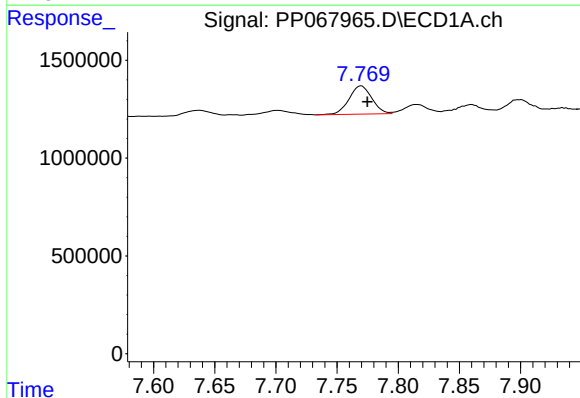


#32 AR-1260-2

R.T.: 7.770 min
Delta R.T.: -0.005 min
Response: 1863670
Conc: 29.46 ng/ml

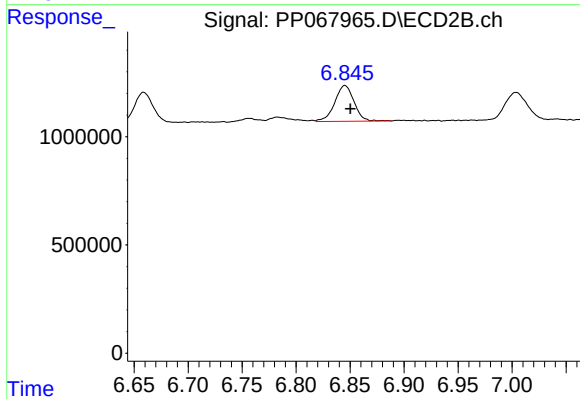

#32 AR-1260-2


R.T.: 6.845 min
Delta R.T.: -0.005 min
Response: 2060834
Conc: 30.90 ng/ml

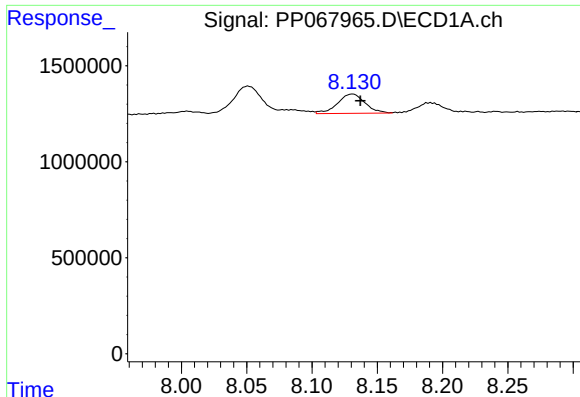

#33 AR-1260-3


R.T.: 8.131 min
Delta R.T.: -0.006 min
Response: 1474442
Conc: 28.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

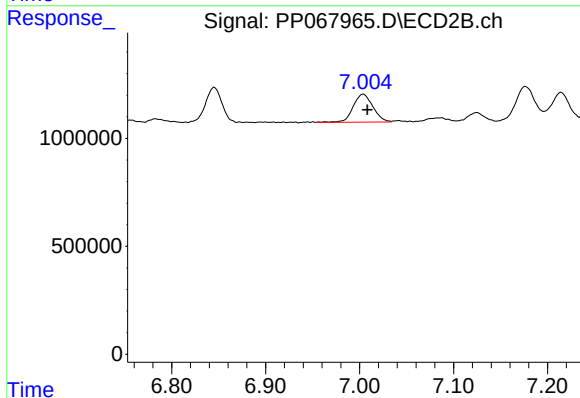


#33 AR-1260-3

R.T.: 7.004 min
Delta R.T.: -0.005 min
Response: 1899730
Conc: 29.82 ng/ml

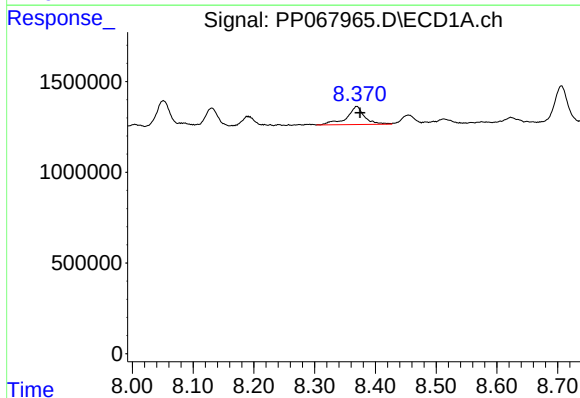


#34 AR-1260-4

R.T.: 8.370 min
Delta R.T.: -0.005 min
Response: 2023384
Conc: 33.61 ng/ml

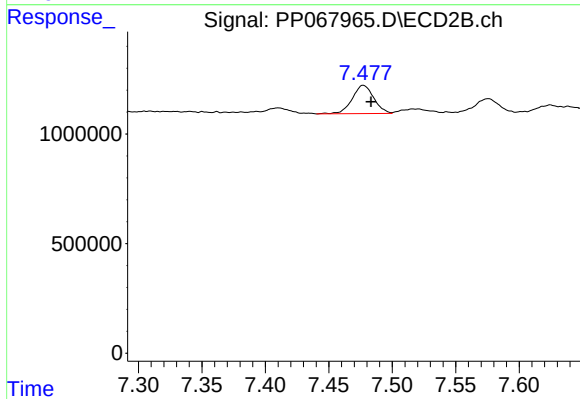

#34 AR-1260-4


R.T.: 7.477 min
Delta R.T.: -0.006 min
Response: 1529544
Conc: 27.66 ng/ml

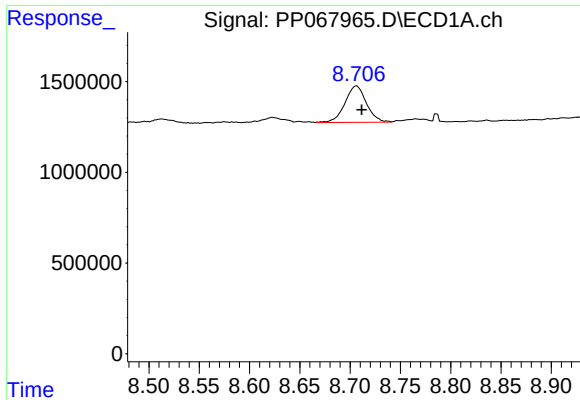

#35 AR-1260-5


R.T.: 8.706 min
Delta R.T.: -0.005 min
Response: 2995495
Conc: 27.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

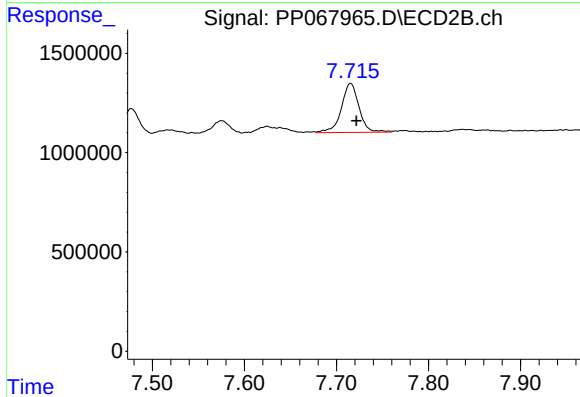


#35 AR-1260-5

R.T.: 7.715 min
Delta R.T.: -0.006 min
Response: 3301450
Conc: 27.00 ng/ml

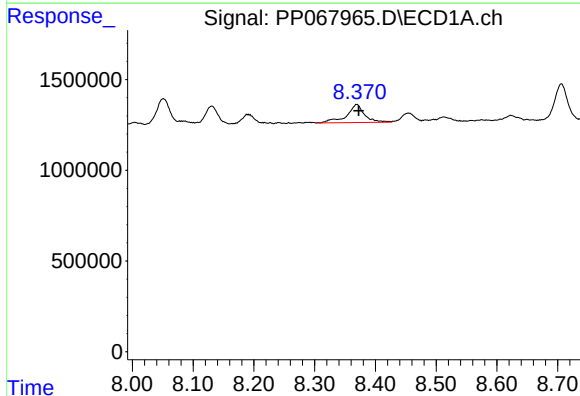


#36 AR-1262-1

R.T.: 8.370 min
Delta R.T.: -0.003 min
Response: 2023384
Conc: 28.19 ng/ml

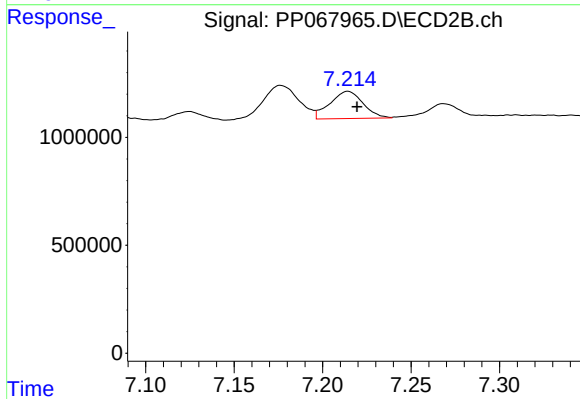

#36 AR-1262-1


R.T.: 7.214 min
Delta R.T.: -0.005 min
Response: 1642733
Conc: 20.88 ng/ml

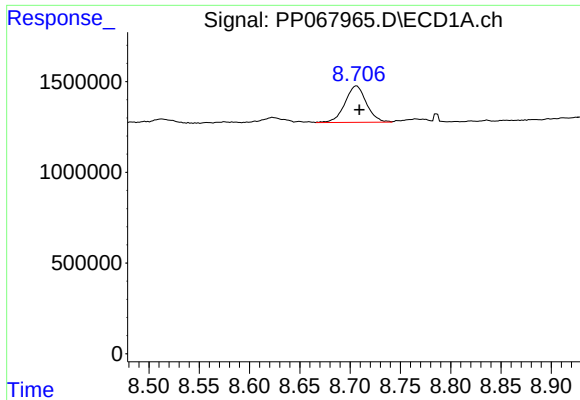

#37 AR-1262-2


R.T.: 8.706 min
Delta R.T.: -0.003 min
Response: 2995495
Conc: 24.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

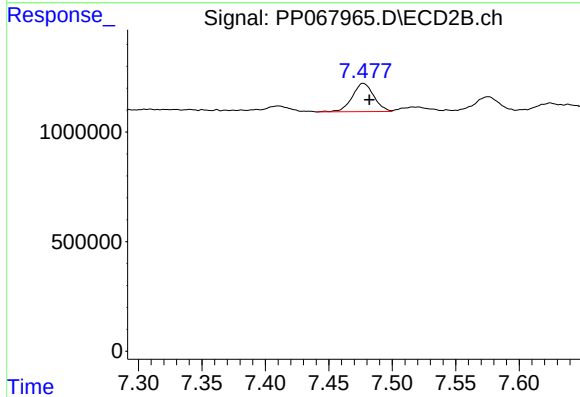


#37 AR-1262-2

R.T.: 7.477 min
Delta R.T.: -0.005 min
Response: 1529544
Conc: 21.55 ng/ml

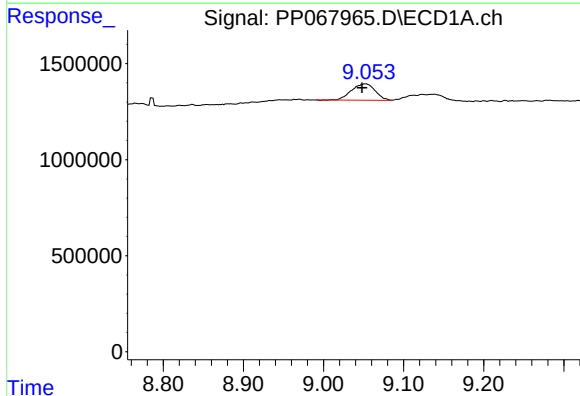


#38 AR-1262-3

R.T.: 9.052 min
Delta R.T.: 0.004 min
Response: 1764071
Conc: 19.93 ng/ml

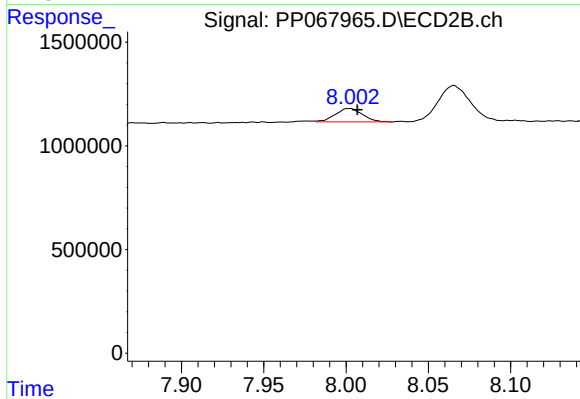

#38 AR-1262-3


R.T.: 8.002 min
Delta R.T.: -0.005 min
Response: 746993
Conc: 13.08 ng/ml

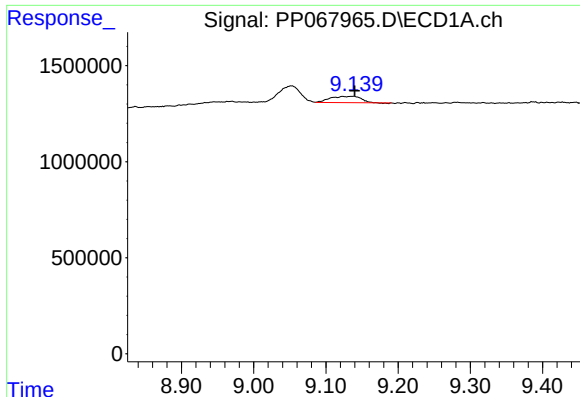

#39 AR-1262-4


R.T.: 9.137 min
Delta R.T.: -0.003 min
Response: 969960
Conc: 13.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

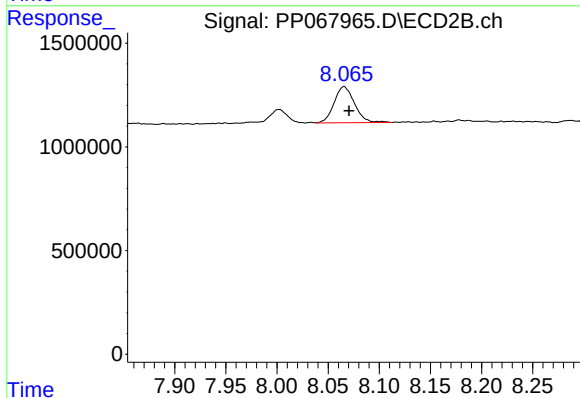


#39 AR-1262-4

R.T.: 8.066 min
Delta R.T.: -0.005 min
Response: 2428475
Conc: 24.18 ng/ml

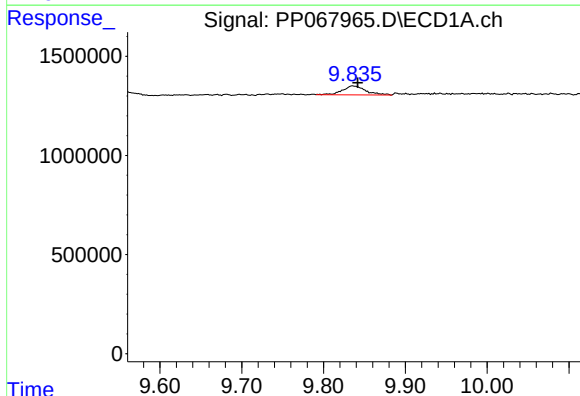


#40 AR-1262-5

R.T.: 9.837 min
Delta R.T.: -0.005 min
Response: 888181
Conc: 18.98 ng/ml

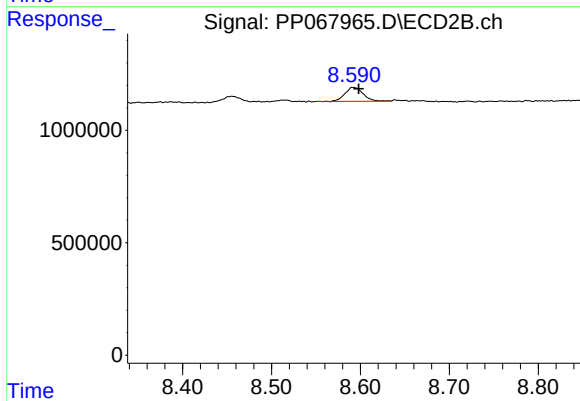

#40 AR-1262-5


R.T.: 8.592 min
Delta R.T.: -0.006 min
Response: 880168
Conc: 17.60 ng/ml

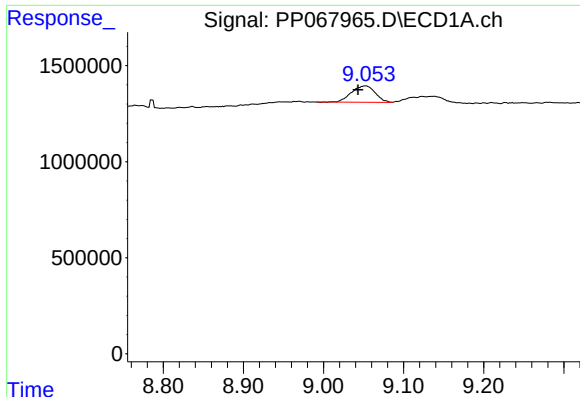

#41 AR-1268-1


R.T.: 9.052 min
Delta R.T.: 0.009 min
Response: 1764071
Conc: 11.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

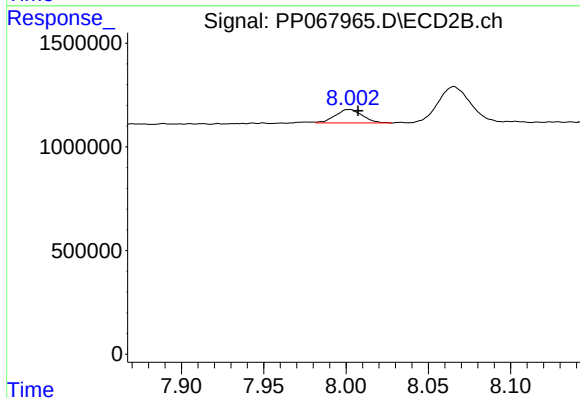


#41 AR-1268-1

R.T.: 8.002 min
Delta R.T.: -0.005 min
Response: 746993
Conc: 4.69 ng/ml

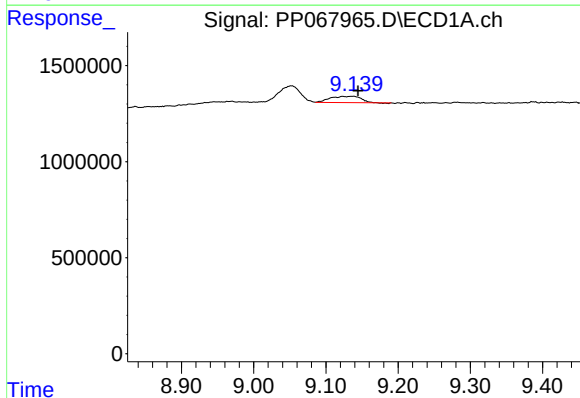


#42 AR-1268-2

R.T.: 9.137 min
Delta R.T.: -0.007 min
Response: 969960
Conc: 7.10 ng/ml

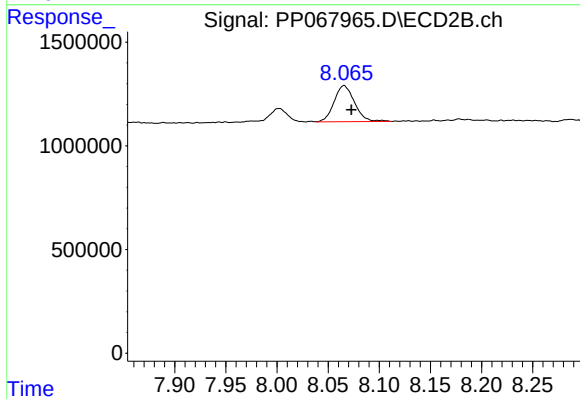

#42 AR-1268-2


R.T.: 8.066 min
Delta R.T.: -0.007 min
Response: 2428475
Conc: 16.96 ng/ml

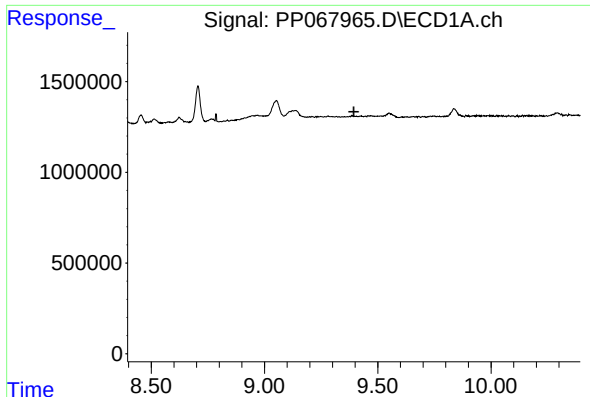

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

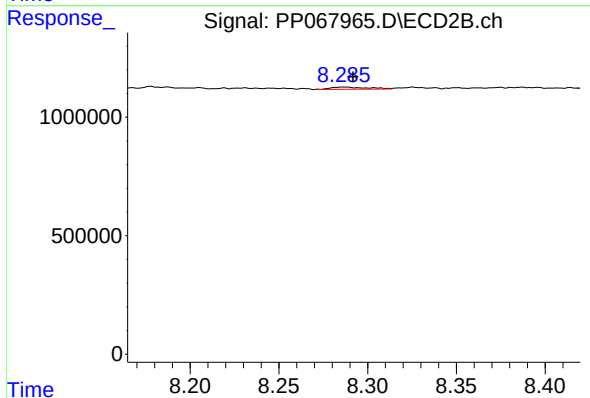


#43 AR-1268-3

R.T.: 8.287 min
Delta R.T.: -0.005 min
Response: 138845
Conc: 1.09 ng/ml

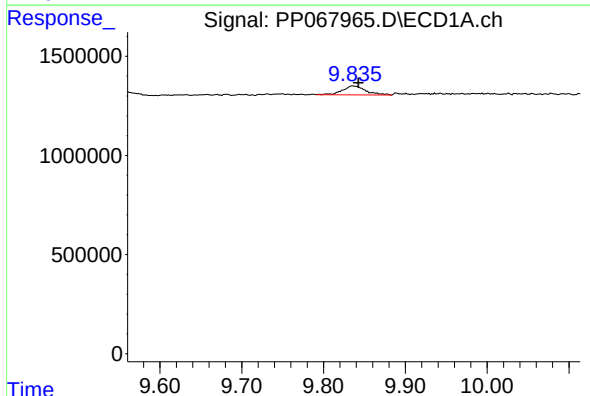


#44 AR-1268-4

R.T.: 9.837 min
Delta R.T.: -0.006 min
Response: 888181
Conc: 17.48 ng/ml

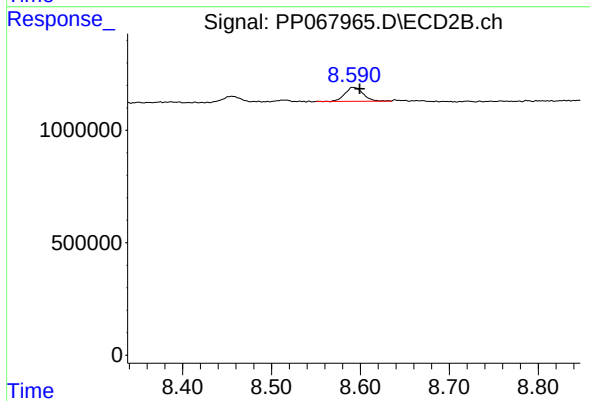

#44 AR-1268-4


R.T.: 8.592 min
Delta R.T.: -0.007 min
Response: 880168
Conc: 15.58 ng/ml

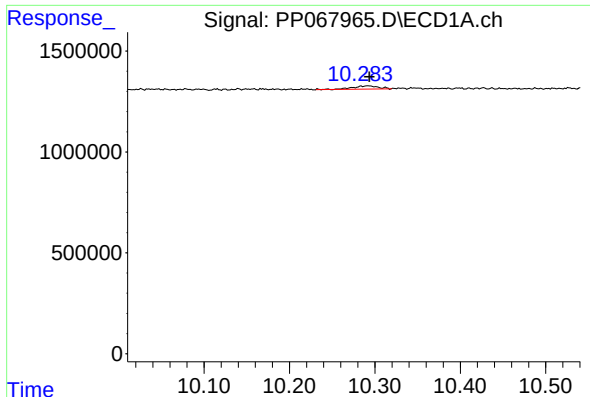

#45 AR-1268-5

R.T.: 10.293 min
Delta R.T.: -0.001 min
Response: 329223
Conc: 0.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

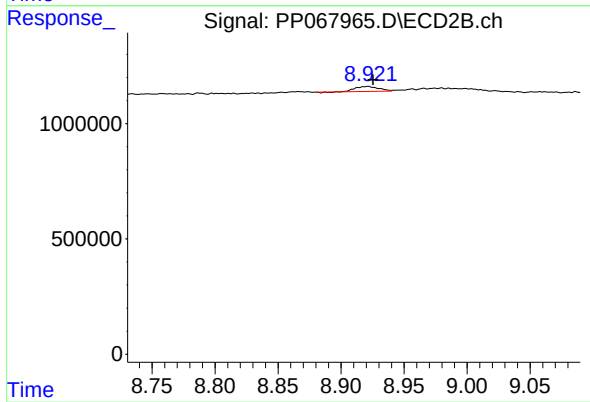

#45 AR-1268-5

R.T.: 8.921 min
Delta R.T.: -0.004 min
Response: 262652
Conc: 0.69 ng/ml