

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
 Data File : PP067967.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2024 06:08
 Operator : YP\AJ
 Sample : P4368-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT4-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 07:40:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.753	4.049	14718143	15874247	15.900	15.711
2)	SA Decachlor...	10.663	9.209	20739530	19598818	18.014	17.476
Target Compounds							
3)	L1 AR-1016-1	5.915	5.157	425226	373934	12.860	10.688
4)	L1 AR-1016-2	5.939	5.177	496357	596979	10.177	12.394
5)	L1 AR-1016-3	6.000	5.355	462057	343192	14.663	12.740
6)	L1 AR-1016-4	6.100	5.396	281230	238671	10.924	9.909
7)	L1 AR-1016-5	6.392	5.616	323136	285347	11.938	9.383
8)	L2 AR-1221-1	0.000	4.264	0	228860	N.D.	17.377 #
9)	L2 AR-1221-2	5.060	4.357	273368	397814	28.896	39.936 #
10)	L2 AR-1221-3	5.117	4.431	431196	529356	14.916	17.004
11)	L3 AR-1232-1	5.117	4.431	431196	529356	18.863	21.755
12)	L3 AR-1232-2	5.649	5.177	249586	596979	21.182	26.693 #
13)	L3 AR-1232-3	5.939	5.355	496357	343192	22.283	28.734 #
14)	L3 AR-1232-4	6.100	5.439	281230	312712	24.915	27.118
15)	L3 AR-1232-5	6.190	5.616	223629	285347	24.520	21.215
16)	L4 AR-1242-1	5.915	5.157	425226	373934	15.221	12.860
17)	L4 AR-1242-2	5.939	5.177	496357	596979	12.215	14.870
18)	L4 AR-1242-3	6.000	5.355	462057	343192	17.136	15.256
19)	L4 AR-1242-4	6.100	5.439	281230	312712	13.111	13.174
20)	L4 AR-1242-5	6.836	5.971	280128	322838	11.611	11.269
21)	L5 AR-1248-1	5.915	5.157	425226	373934	19.849	16.499
22)	L5 AR-1248-2	6.190	5.396	223629	238671	6.652	7.212
23)	L5 AR-1248-3	6.392	5.439	323136	312712	8.823	9.071
24)	L5 AR-1248-4	6.796	5.616	297143	285347	7.346	6.967
25)	L5 AR-1248-5	6.836	6.012	280128	265653	7.063	7.095
26)	L6 AR-1254-1	6.771	5.971	300717	322838	6.715	5.464
27)	L6 AR-1254-2	6.994	6.119	382152	114951	5.782	2.191 #
28)	L6 AR-1254-3	7.353	6.527	283382	214989	4.080	2.584 #
29)	L6 AR-1254-4	7.634	6.760	327398	92504	6.560	1.916 #
30)	L6 AR-1254-5	8.055	7.181	627767	219415	10.588	2.983 #
31)	L7 AR-1260-1	7.549	6.665	277006	191094	5.127	3.355 #
32)	L7 AR-1260-2	7.771	6.824	287790	193530	4.549	2.901 #
33)	L7 AR-1260-3	8.138	7.004	545429	222754	10.520	3.497 #
34)	L7 AR-1260-4	0.000	7.521f	0	65654	N.D.	1.187 #
35)	L7 AR-1260-5	8.769f	7.712	151573	125120	1.407	1.023 #
36)	L8 AR-1262-1	0.000	7.250	0	52109	N.D.	0.662 #
37)	L8 AR-1262-2	8.769f	7.521f	151573	65654	1.247	0.925 #
38)	L8 AR-1262-3	0.000	8.043f	0	33641	N.D.	0.589 #
39)	L8 AR-1262-4	0.000	8.043	0	33641	N.D.	0.335 #
41)	L9 AR-1268-1	0.000	8.043f	0	33641	N.D.	0.211 #
42)	L9 AR-1268-2	0.000	8.100	0	71724	N.D.	0.501 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
Data File : PP067967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 06:08
Operator : YP\AJ
Sample : P4368-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 69 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:40:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	8.290	0	130751	N.D.	1.025 #
45) L9	AR-1268-5	0.000	8.921	0	114035	N.D.	0.302 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
Data File : PP067967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 06:08
Operator : YP\AJ
Sample : P4368-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 69 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:40:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

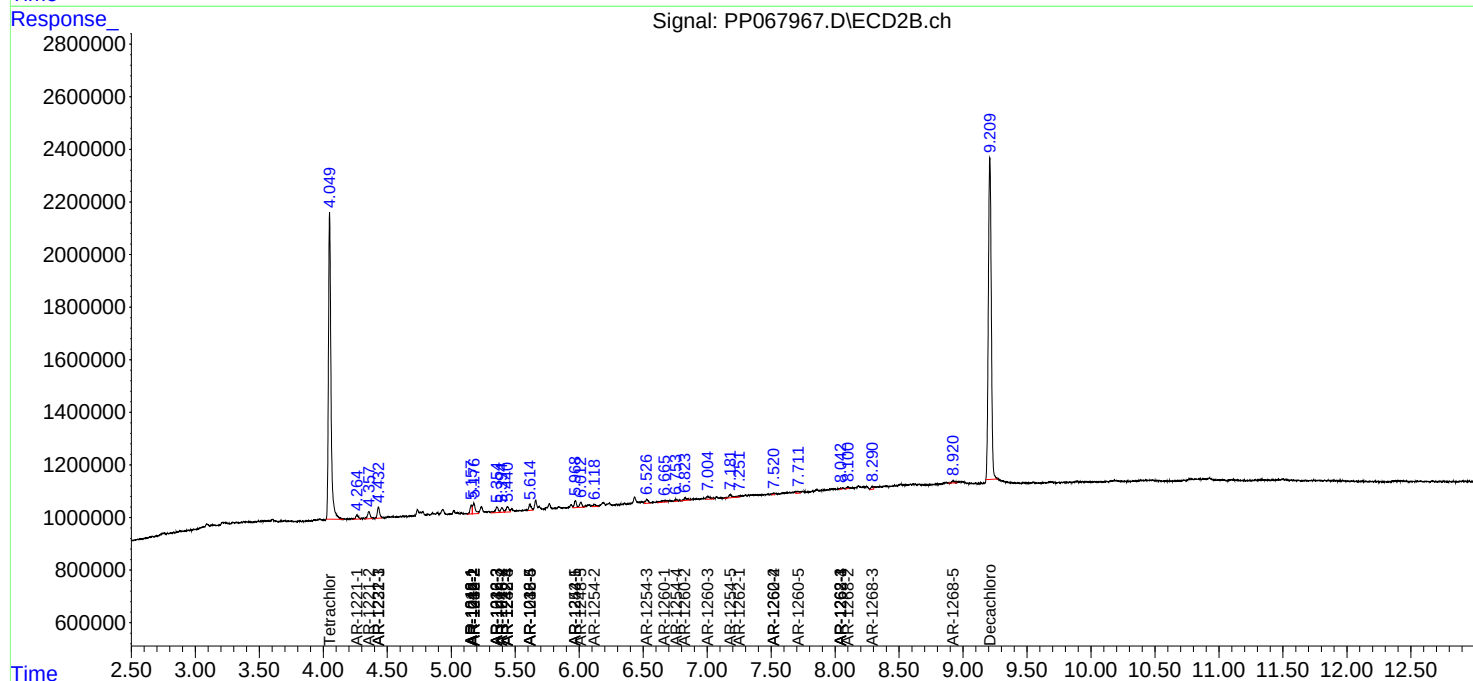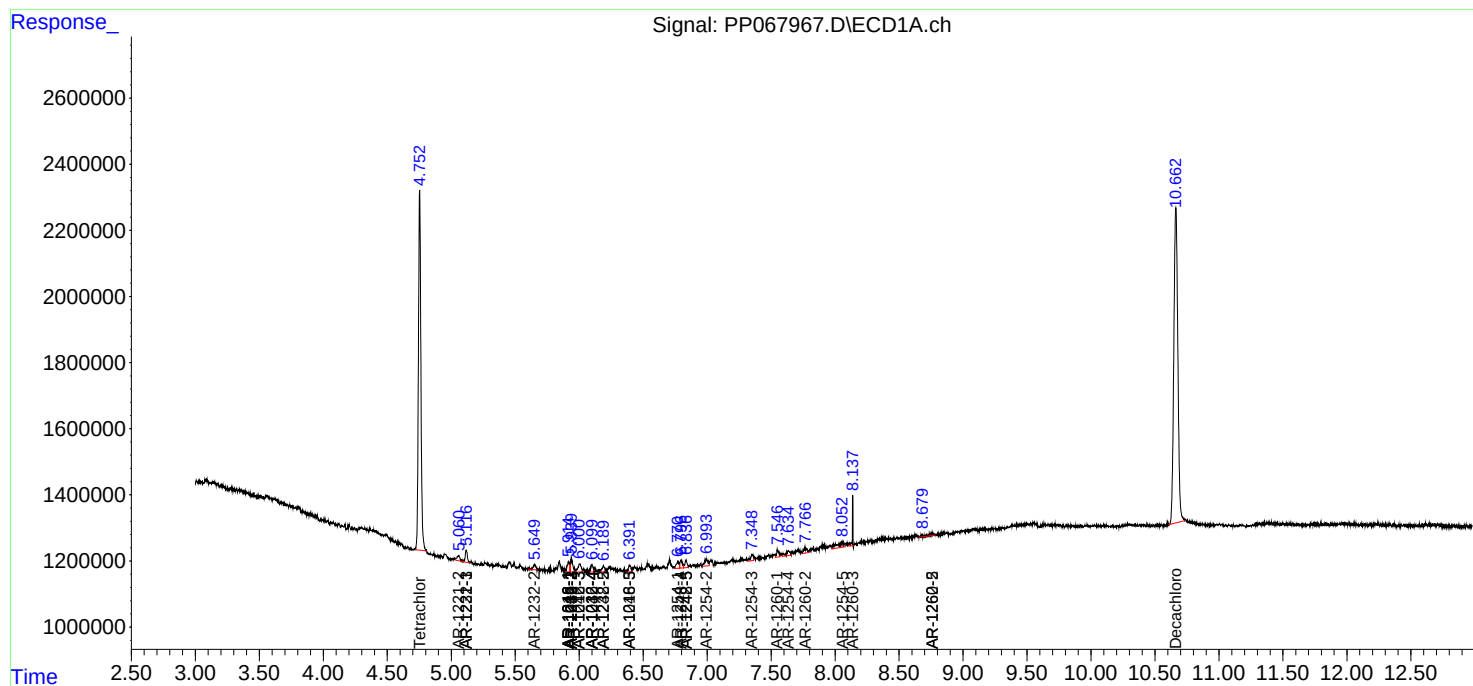


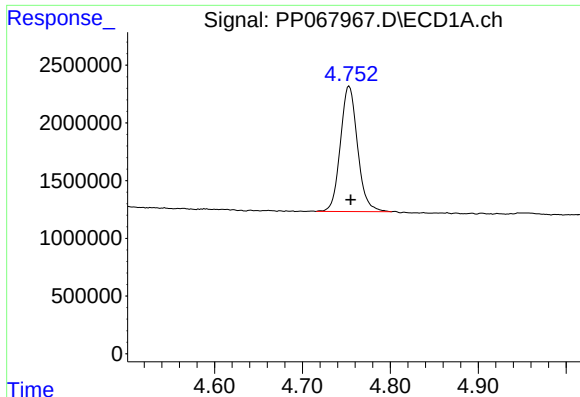

#1 Tetrachloro-m-xylene


R.T.: 4.753 min
Delta R.T.: -0.002 min
Response: 14718143
Conc: 15.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

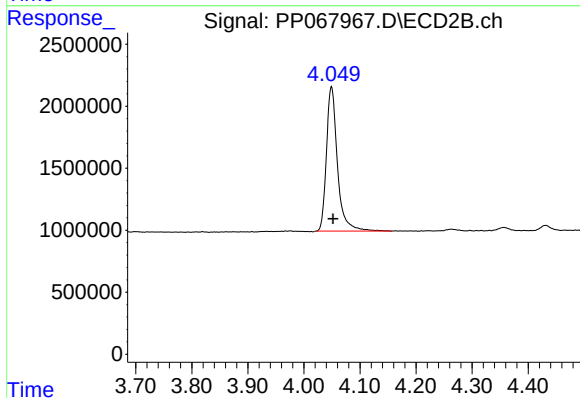


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: -0.003 min
Response: 15874247
Conc: 15.71 ng/ml

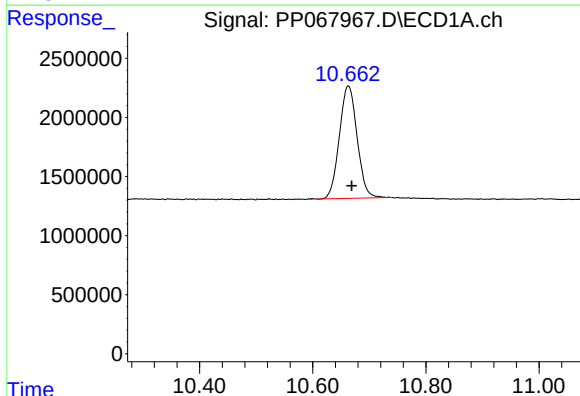


#2 Decachlorobiphenyl

R.T.: 10.663 min
Delta R.T.: -0.006 min
Response: 20739530
Conc: 18.01 ng/ml

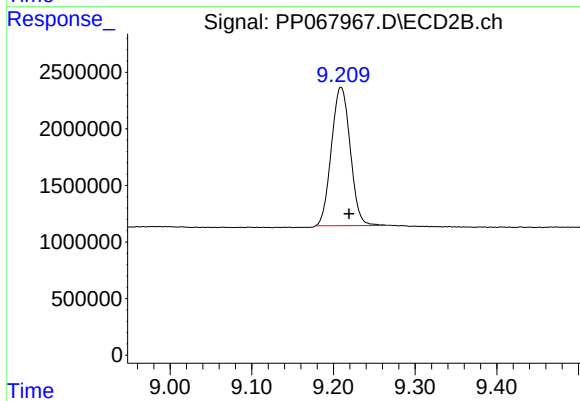

#2 Decachlorobiphenyl


R.T.: 9.209 min
Delta R.T.: -0.010 min
Response: 19598818
Conc: 17.48 ng/ml

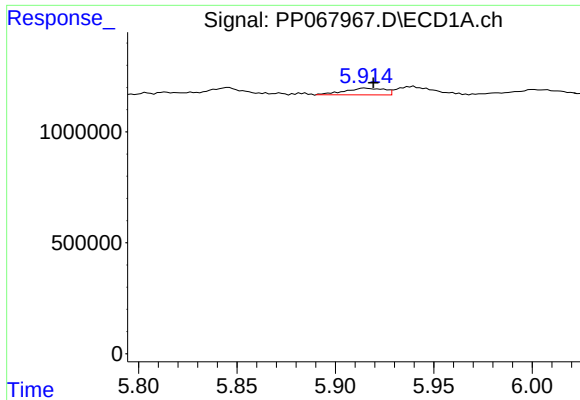

#3 AR-1016-1


R.T.: 5.915 min
Delta R.T.: -0.004 min
Response: 425226
Conc: 12.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

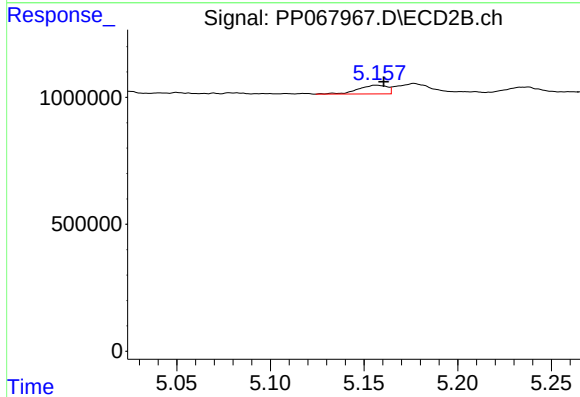


#3 AR-1016-1

R.T.: 5.157 min
Delta R.T.: -0.004 min
Response: 373934
Conc: 10.69 ng/ml

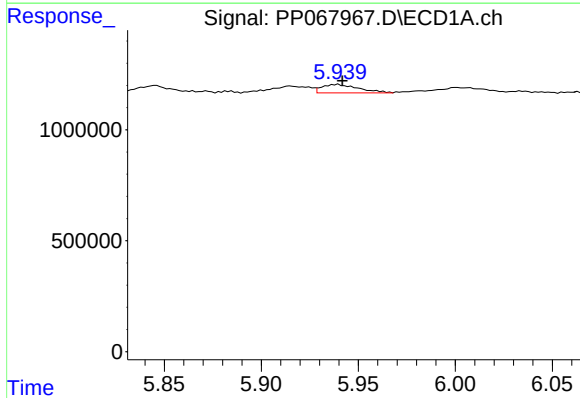


#4 AR-1016-2

R.T.: 5.939 min
Delta R.T.: -0.003 min
Response: 496357
Conc: 10.18 ng/ml

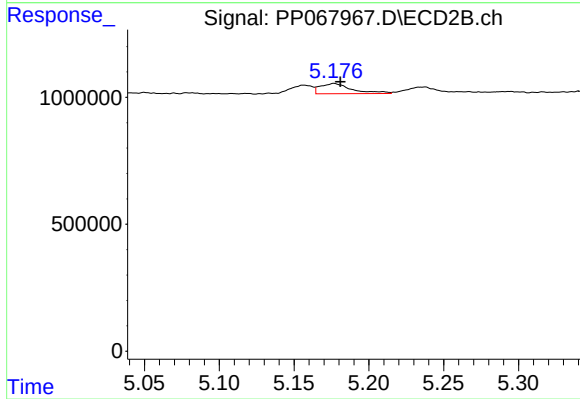

#4 AR-1016-2


R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 596979
Conc: 12.39 ng/ml

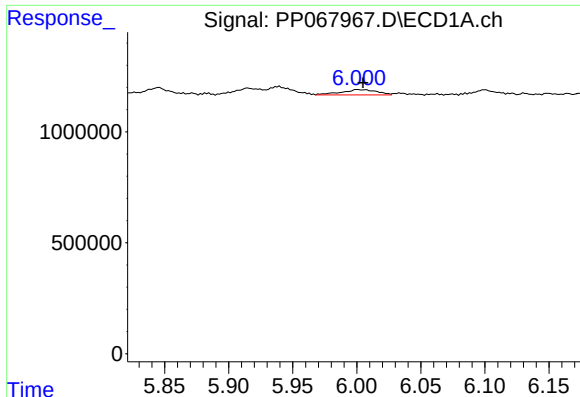

#5 AR-1016-3


R.T.: 6.000 min
Delta R.T.: -0.005 min
Response: 462057
Conc: 14.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

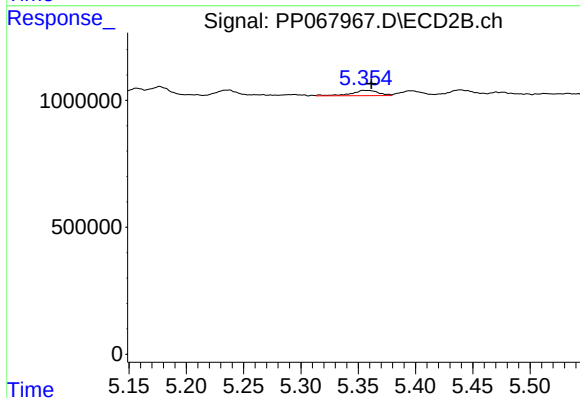


#5 AR-1016-3

R.T.: 5.355 min
Delta R.T.: -0.006 min
Response: 343192
Conc: 12.74 ng/ml

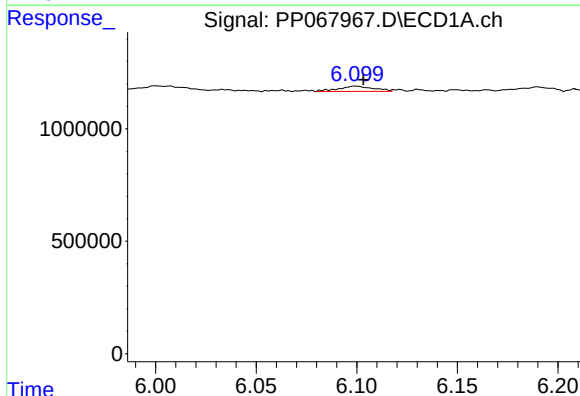


#6 AR-1016-4

R.T.: 6.100 min
Delta R.T.: -0.003 min
Response: 281230
Conc: 10.92 ng/ml

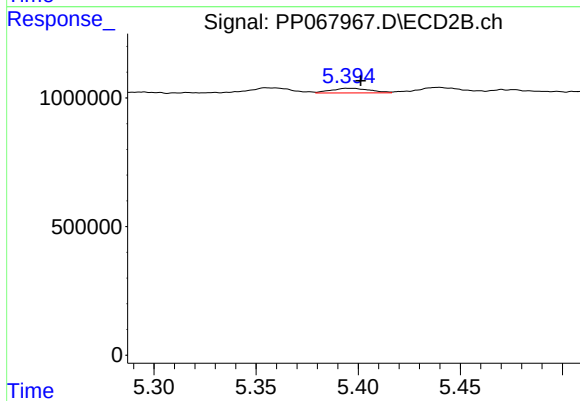

#6 AR-1016-4


R.T.: 5.396 min
Delta R.T.: -0.005 min
Response: 238671
Conc: 9.91 ng/ml

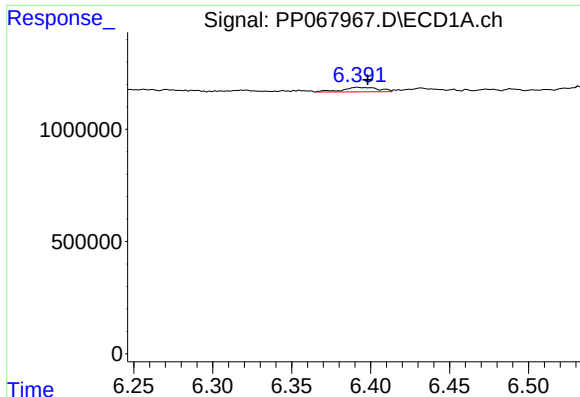

#7 AR-1016-5


R.T.: 6.392 min
Delta R.T.: -0.006 min
Response: 323136
Conc: 11.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

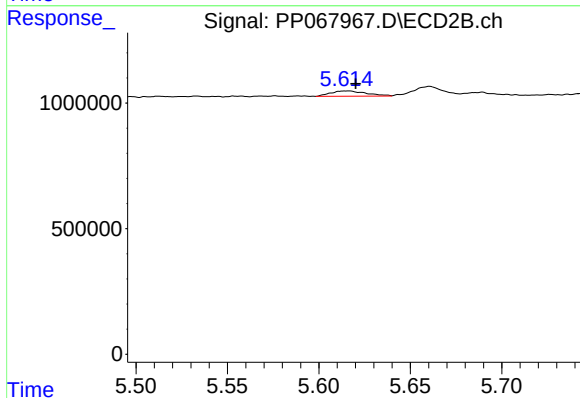


#7 AR-1016-5

R.T.: 5.616 min
Delta R.T.: -0.004 min
Response: 285347
Conc: 9.38 ng/ml

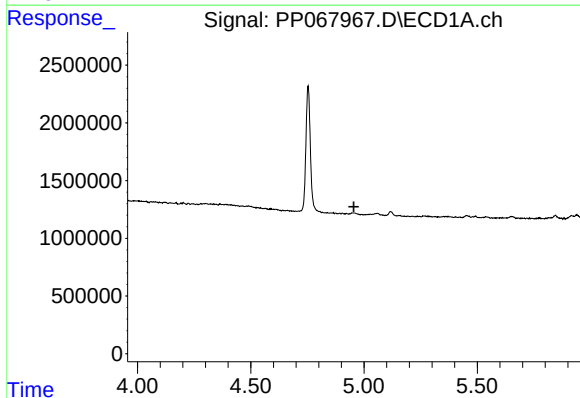


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.955 min
Response: 0
Conc: N.D.

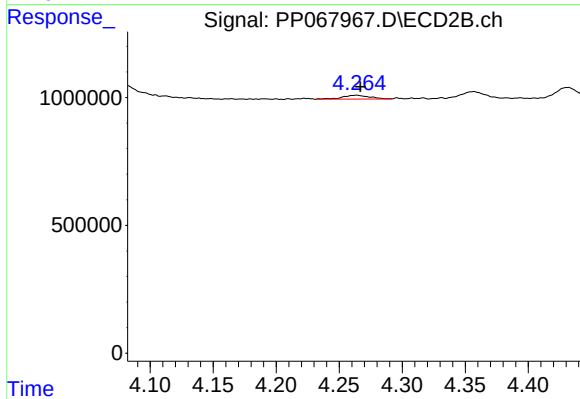

#8 AR-1221-1


R.T.: 4.264 min
Delta R.T.: -0.003 min
Response: 228860
Conc: 17.38 ng/ml

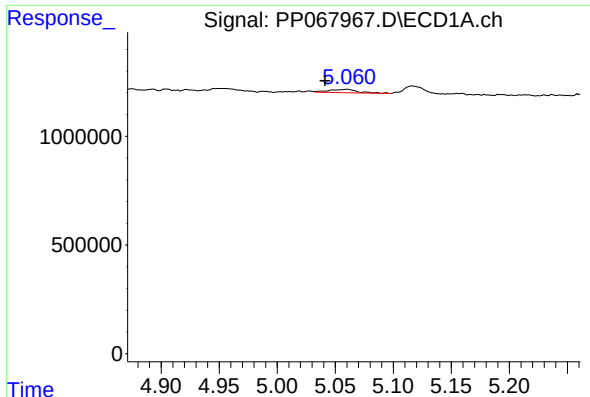

#9 AR-1221-2


R.T.: 5.060 min
Delta R.T.: 0.019 min
Response: 273368
Conc: 28.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

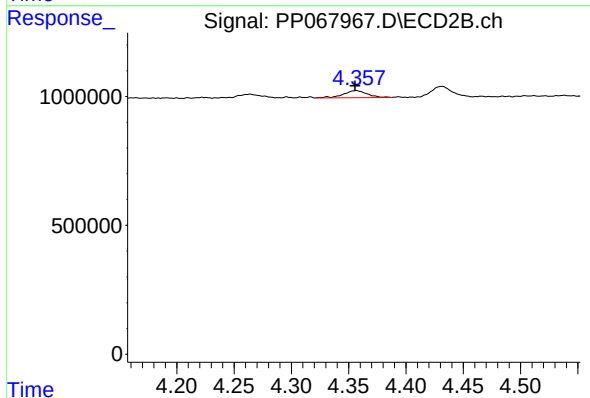


#9 AR-1221-2

R.T.: 4.357 min
Delta R.T.: 0.001 min
Response: 397814
Conc: 39.94 ng/ml

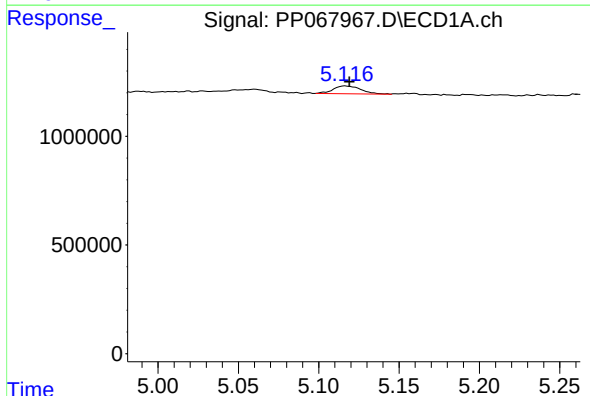


#10 AR-1221-3

R.T.: 5.117 min
Delta R.T.: -0.003 min
Response: 431196
Conc: 14.92 ng/ml

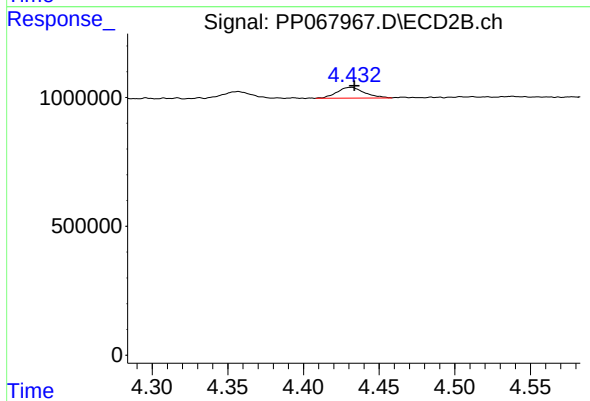

#10 AR-1221-3


R.T.: 4.431 min
Delta R.T.: -0.002 min
Response: 529356
Conc: 17.00 ng/ml

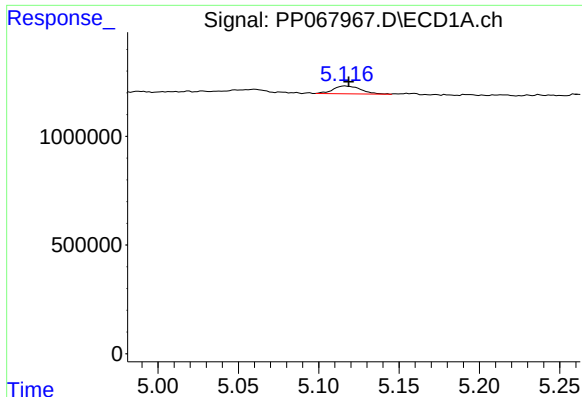

#11 AR-1232-1


R.T.: 5.117 min
Delta R.T.: -0.002 min
Response: 431196
Conc: 18.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

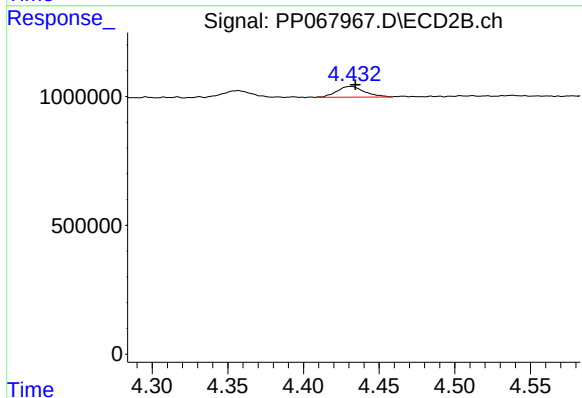


#11 AR-1232-1

R.T.: 4.431 min
Delta R.T.: -0.003 min
Response: 529356
Conc: 21.75 ng/ml

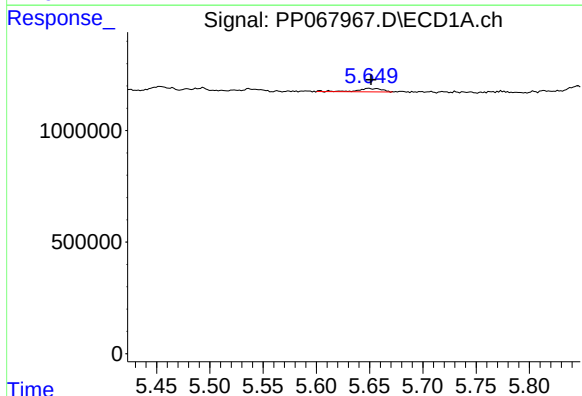


#12 AR-1232-2

R.T.: 5.649 min
Delta R.T.: -0.002 min
Response: 249586
Conc: 21.18 ng/ml

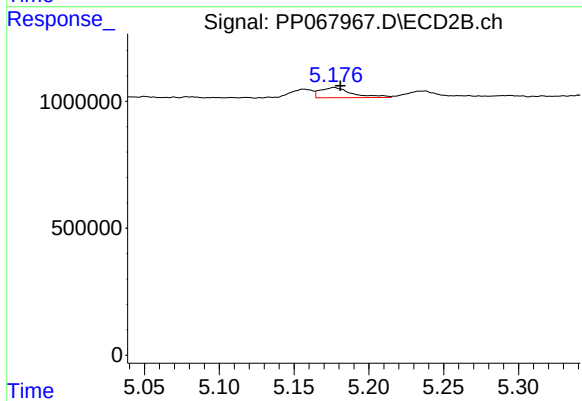

#12 AR-1232-2


R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 596979
Conc: 26.69 ng/ml

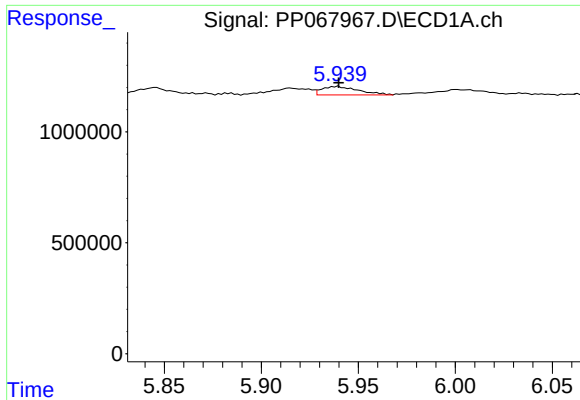

#13 AR-1232-3


R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 496357
Conc: 22.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

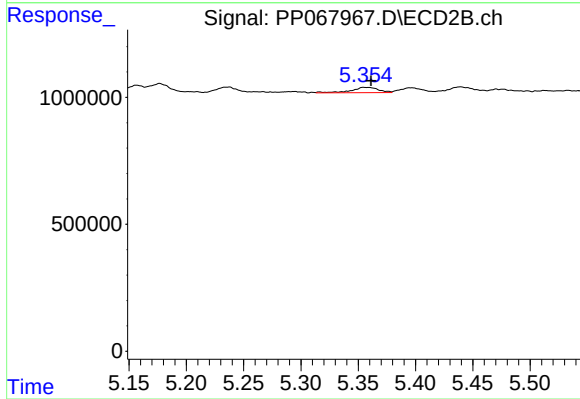


#13 AR-1232-3

R.T.: 5.355 min
Delta R.T.: -0.006 min
Response: 343192
Conc: 28.73 ng/ml

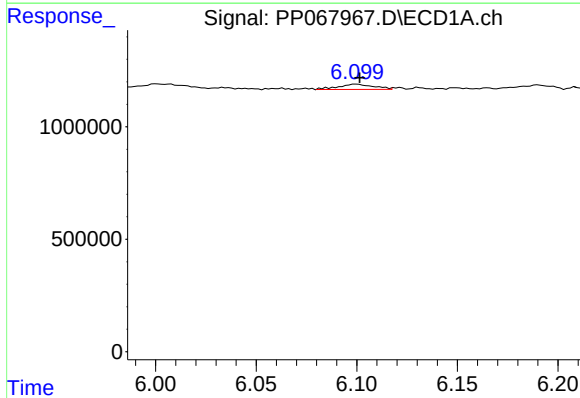


#14 AR-1232-4

R.T.: 6.100 min
Delta R.T.: -0.002 min
Response: 281230
Conc: 24.92 ng/ml

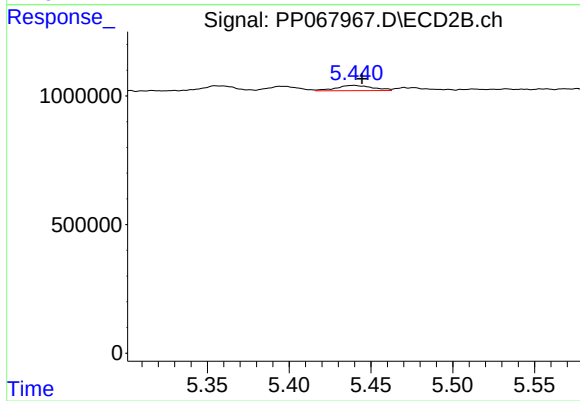

#14 AR-1232-4


R.T.: 5.439 min
Delta R.T.: -0.005 min
Response: 312712
Conc: 27.12 ng/ml

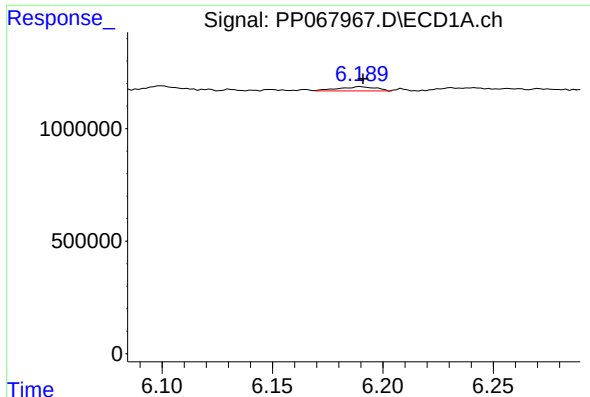

#15 AR-1232-5


R.T.: 6.190 min
Delta R.T.: 0.000 min
Response: 223629
Conc: 24.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

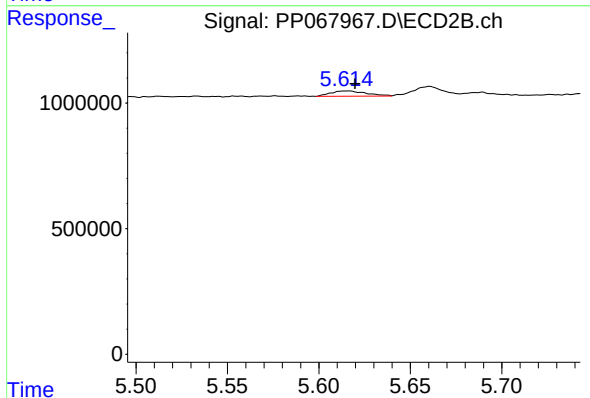


#15 AR-1232-5

R.T.: 5.616 min
Delta R.T.: -0.004 min
Response: 285347
Conc: 21.21 ng/ml

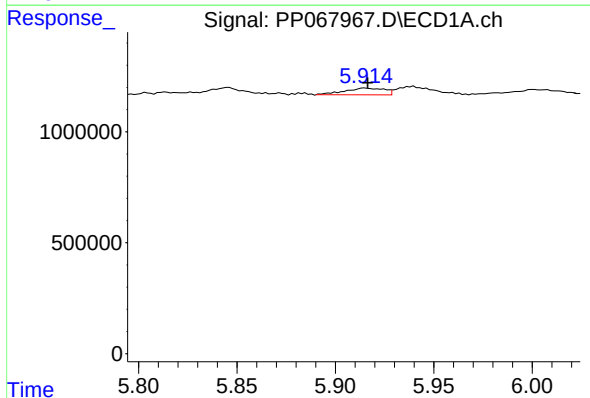


#16 AR-1242-1

R.T.: 5.915 min
Delta R.T.: -0.001 min
Response: 425226
Conc: 15.22 ng/ml

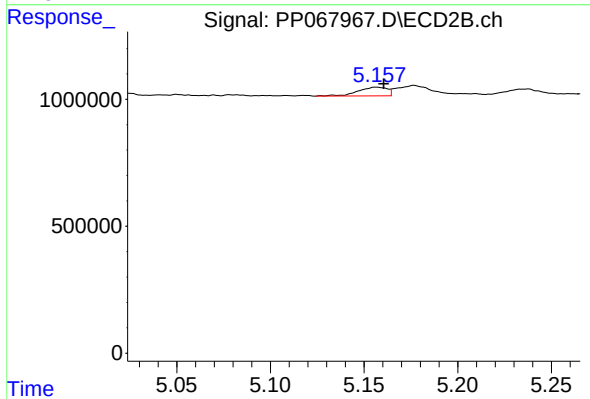

#16 AR-1242-1


R.T.: 5.157 min
Delta R.T.: -0.004 min
Response: 373934
Conc: 12.86 ng/ml

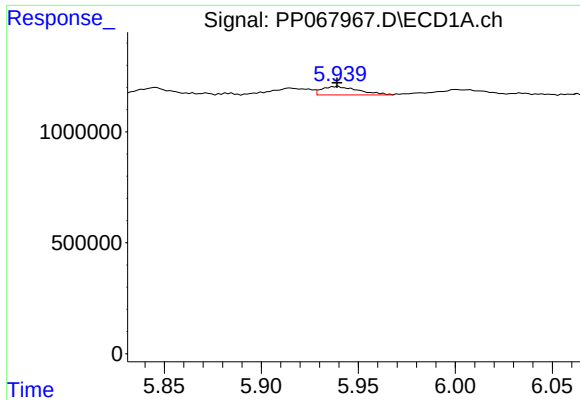

#17 AR-1242-2


R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 496357
Conc: 12.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

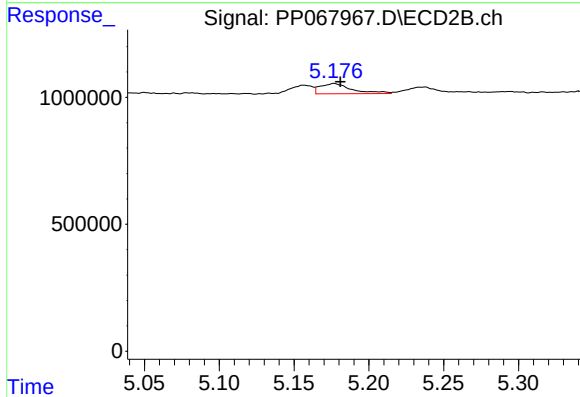


#17 AR-1242-2

R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 596979
Conc: 14.87 ng/ml

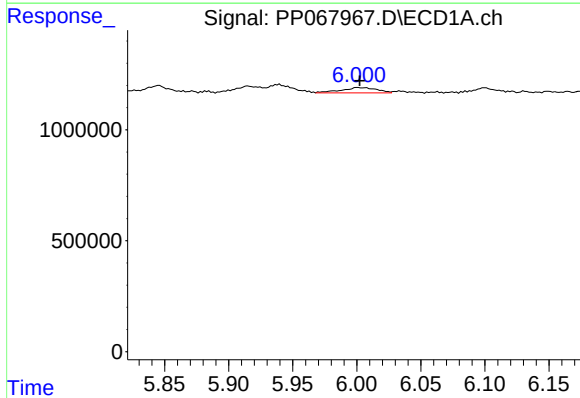


#18 AR-1242-3

R.T.: 6.000 min
Delta R.T.: -0.002 min
Response: 462057
Conc: 17.14 ng/ml

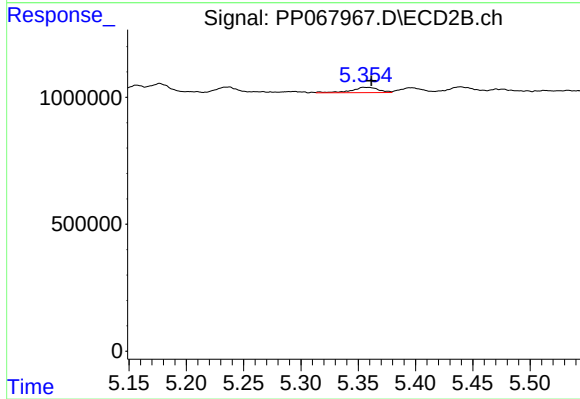

#18 AR-1242-3


R.T.: 5.355 min
Delta R.T.: -0.006 min
Response: 343192
Conc: 15.26 ng/ml

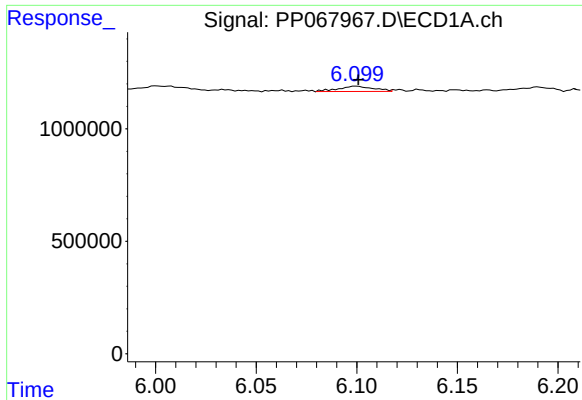

#19 AR-1242-4


R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 281230
Conc: 13.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

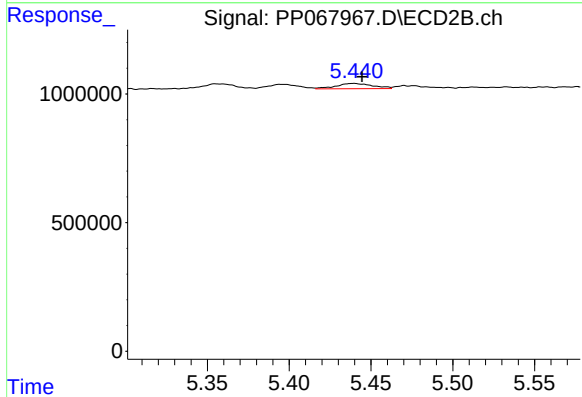


#19 AR-1242-4

R.T.: 5.439 min
Delta R.T.: -0.005 min
Response: 312712
Conc: 13.17 ng/ml

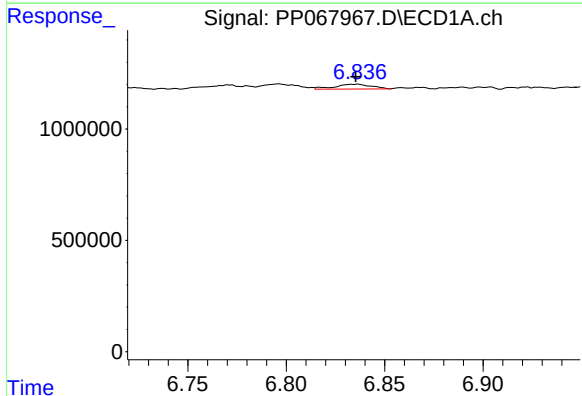


#20 AR-1242-5

R.T.: 6.836 min
Delta R.T.: 0.001 min
Response: 280128
Conc: 11.61 ng/ml

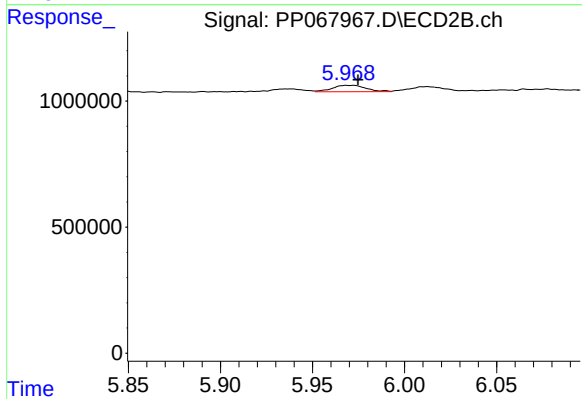

#20 AR-1242-5


R.T.: 5.971 min
Delta R.T.: -0.004 min
Response: 322838
Conc: 11.27 ng/ml

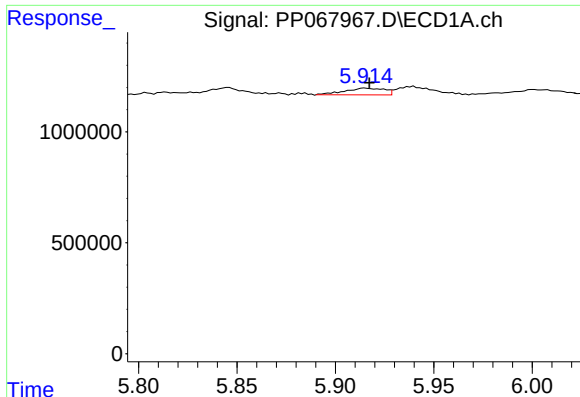

#21 AR-1248-1


R.T.: 5.915 min
Delta R.T.: -0.002 min
Response: 425226
Conc: 19.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

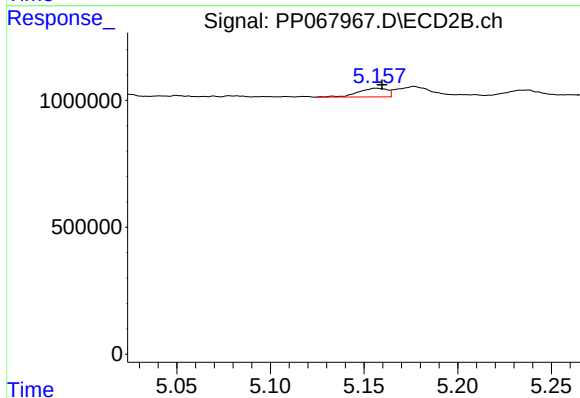


#21 AR-1248-1

R.T.: 5.157 min
Delta R.T.: -0.003 min
Response: 373934
Conc: 16.50 ng/ml

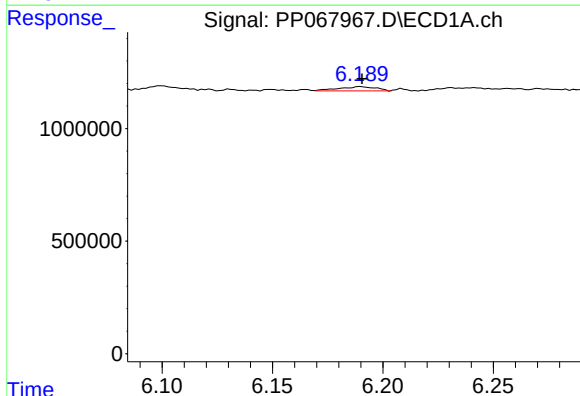


#22 AR-1248-2

R.T.: 6.190 min
Delta R.T.: 0.000 min
Response: 223629
Conc: 6.65 ng/ml

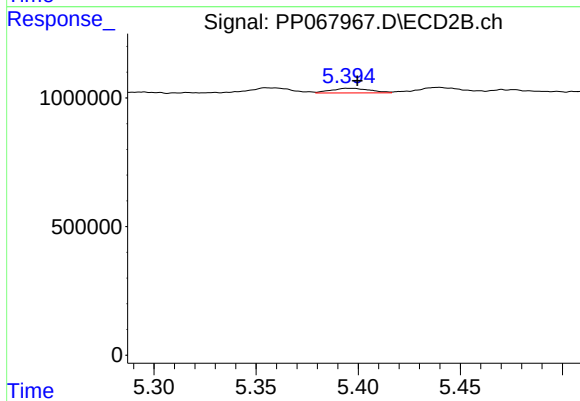

#22 AR-1248-2


R.T.: 5.396 min
Delta R.T.: -0.004 min
Response: 238671
Conc: 7.21 ng/ml

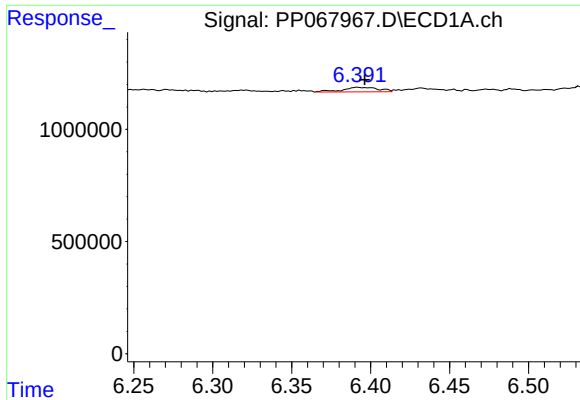

#23 AR-1248-3


R.T.: 6.392 min
Delta R.T.: -0.004 min
Response: 323136
Conc: 8.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

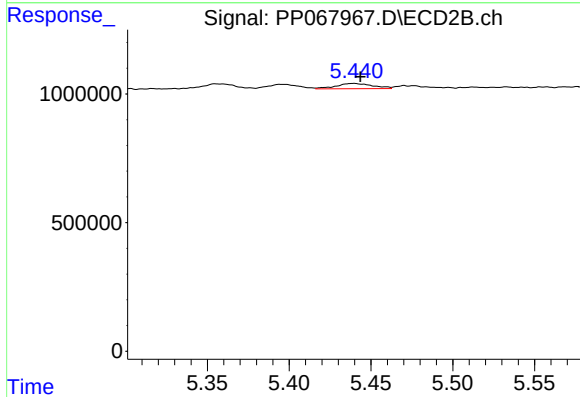


#23 AR-1248-3

R.T.: 5.439 min
Delta R.T.: -0.004 min
Response: 312712
Conc: 9.07 ng/ml

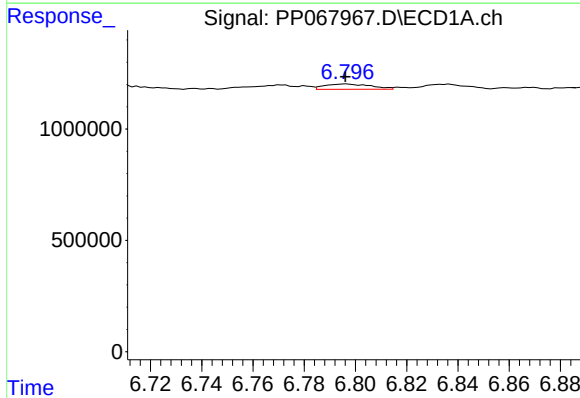


#24 AR-1248-4

R.T.: 6.796 min
Delta R.T.: 0.000 min
Response: 297143
Conc: 7.35 ng/ml

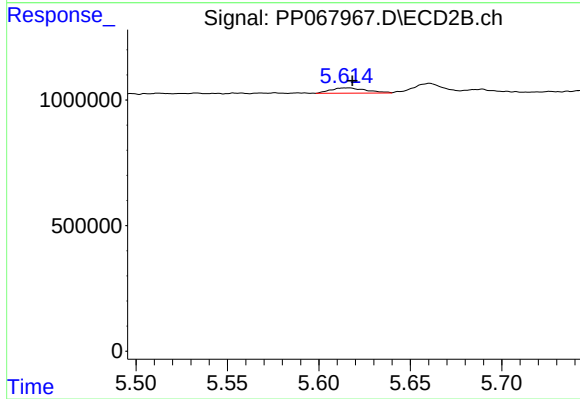

#24 AR-1248-4


R.T.: 5.616 min
Delta R.T.: -0.002 min
Response: 285347
Conc: 6.97 ng/ml

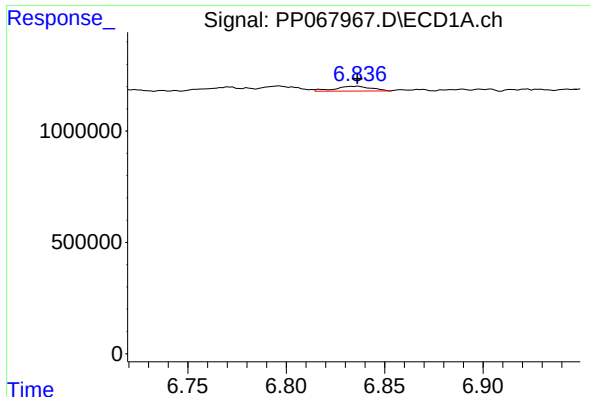

#25 AR-1248-5


R.T.: 6.836 min
Delta R.T.: 0.000 min
Response: 280128
Conc: 7.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

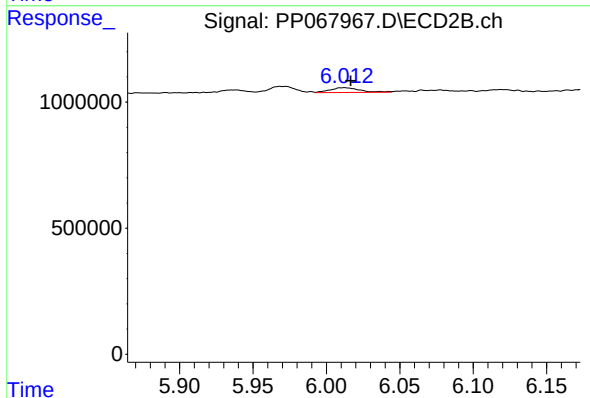


#25 AR-1248-5

R.T.: 6.012 min
Delta R.T.: -0.005 min
Response: 265653
Conc: 7.09 ng/ml

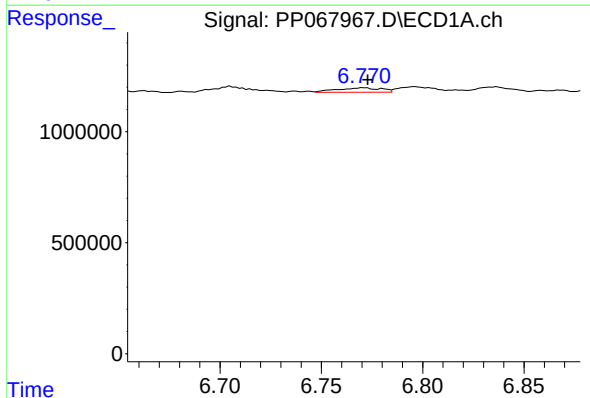


#26 AR-1254-1

R.T.: 6.771 min
Delta R.T.: -0.002 min
Response: 300717
Conc: 6.72 ng/ml

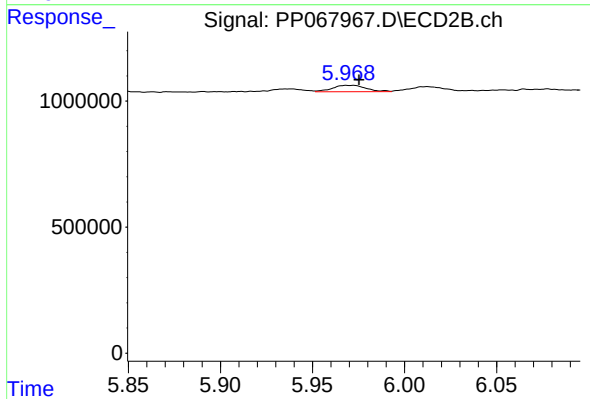

#26 AR-1254-1


R.T.: 5.971 min
Delta R.T.: -0.005 min
Response: 322838
Conc: 5.46 ng/ml

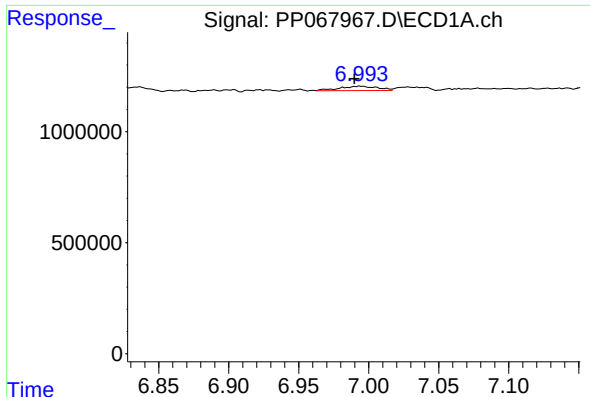

#27 AR-1254-2


R.T.: 6.994 min
Delta R.T.: 0.005 min
Response: 382152
Conc: 5.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

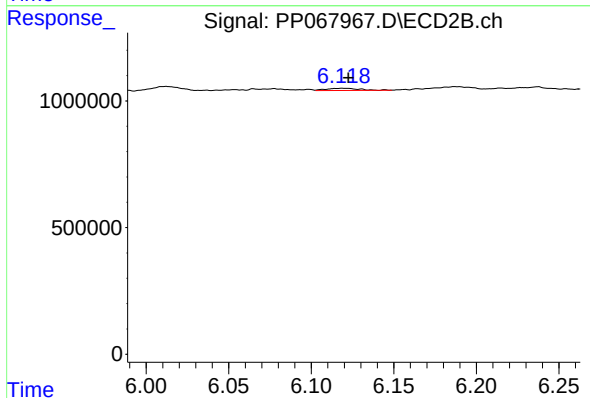


#27 AR-1254-2

R.T.: 6.119 min
Delta R.T.: -0.003 min
Response: 114951
Conc: 2.19 ng/ml

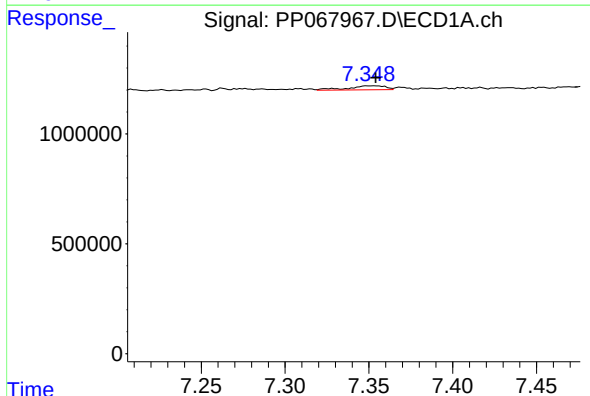


#28 AR-1254-3

R.T.: 7.353 min
Delta R.T.: -0.001 min
Response: 283382
Conc: 4.08 ng/ml

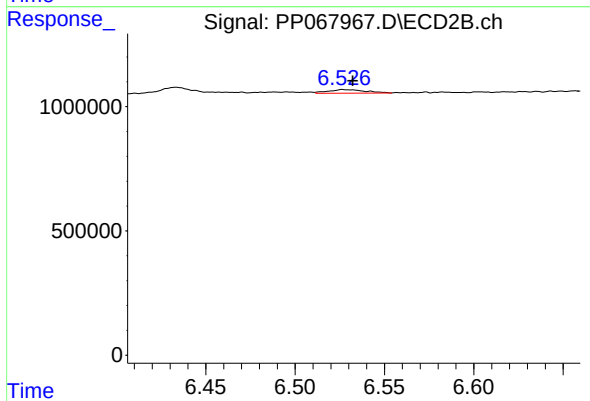

#28 AR-1254-3


R.T.: 6.527 min
Delta R.T.: -0.005 min
Response: 214989
Conc: 2.58 ng/ml

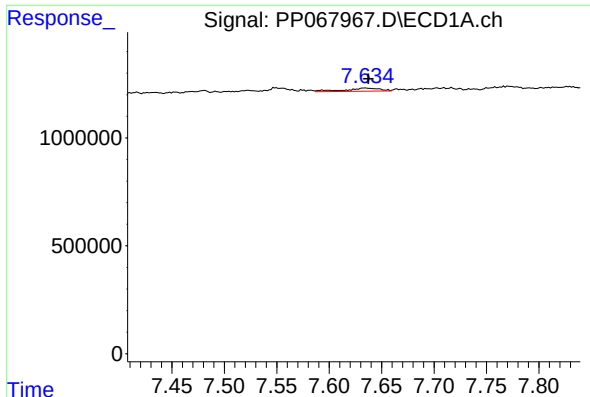

#29 AR-1254-4


R.T.: 7.634 min
Delta R.T.: -0.003 min
Response: 327398
Conc: 6.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

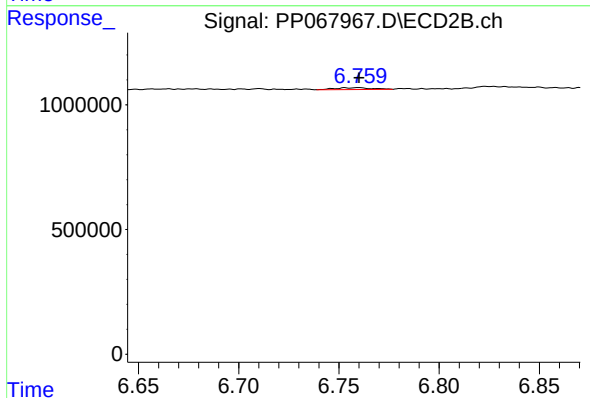


#29 AR-1254-4

R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 92504
Conc: 1.92 ng/ml

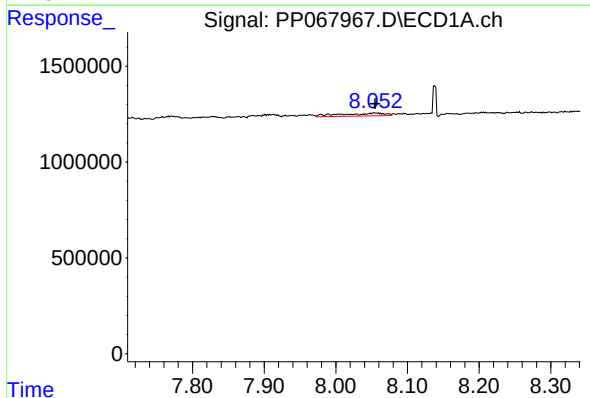


#30 AR-1254-5

R.T.: 8.055 min
Delta R.T.: 0.000 min
Response: 627767
Conc: 10.59 ng/ml

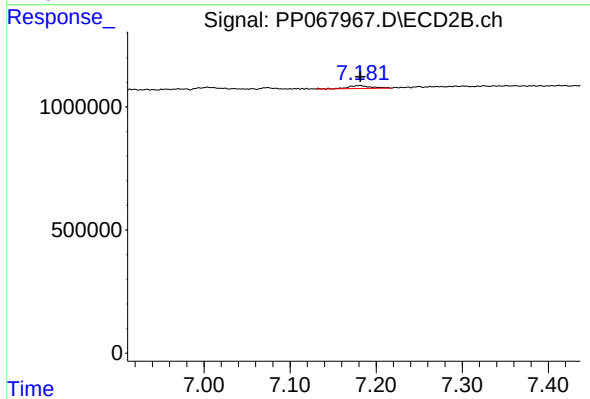

#30 AR-1254-5


R.T.: 7.181 min
Delta R.T.: 0.000 min
Response: 219415
Conc: 2.98 ng/ml

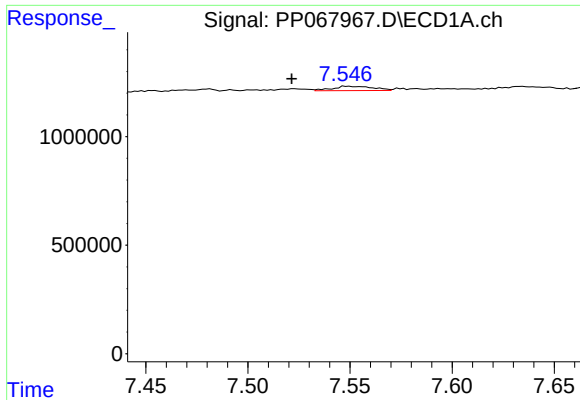

#31 AR-1260-1


R.T.: 7.549 min
Delta R.T.: 0.027 min
Response: 277006
Conc: 5.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

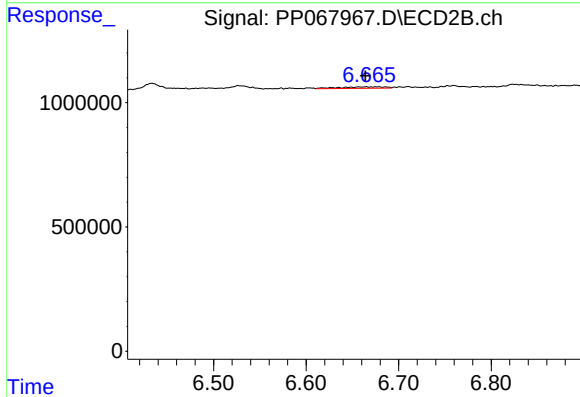


#31 AR-1260-1

R.T.: 6.665 min
Delta R.T.: 0.000 min
Response: 191094
Conc: 3.35 ng/ml

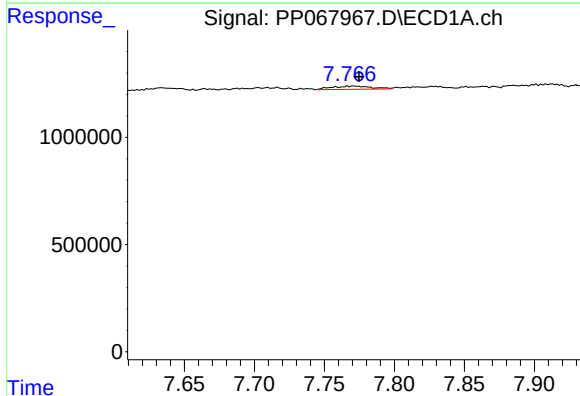


#32 AR-1260-2

R.T.: 7.771 min
Delta R.T.: -0.004 min
Response: 287790
Conc: 4.55 ng/ml

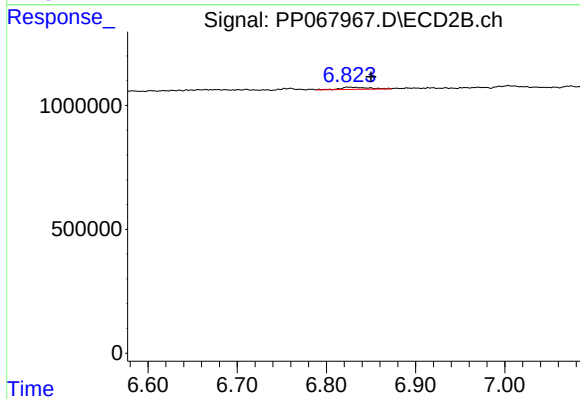

#32 AR-1260-2


R.T.: 6.824 min
Delta R.T.: -0.027 min
Response: 193530
Conc: 2.90 ng/ml

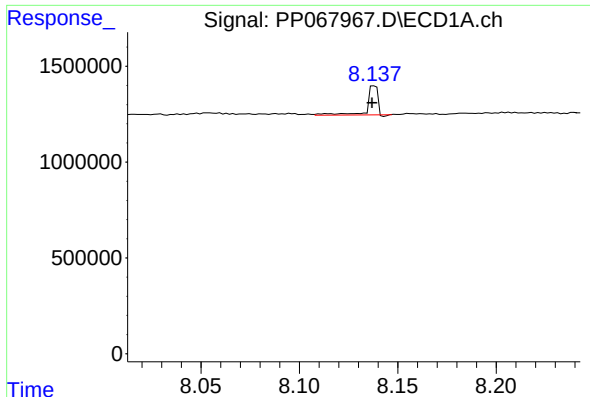

#33 AR-1260-3


R.T.: 8.138 min
Delta R.T.: 0.001 min
Response: 545429
Conc: 10.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

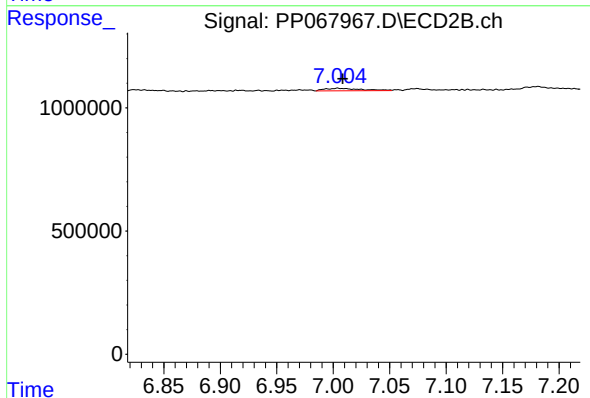


#33 AR-1260-3

R.T.: 7.004 min
Delta R.T.: -0.004 min
Response: 222754
Conc: 3.50 ng/ml

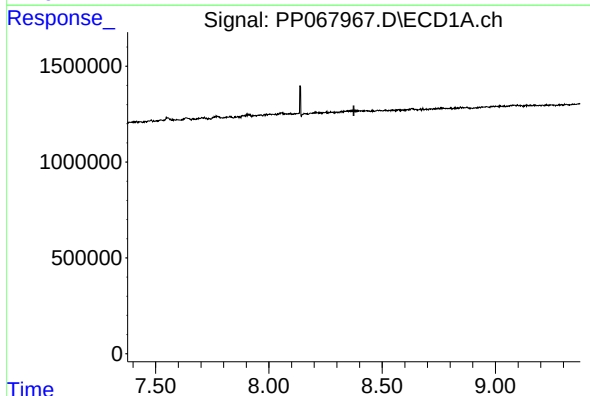


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

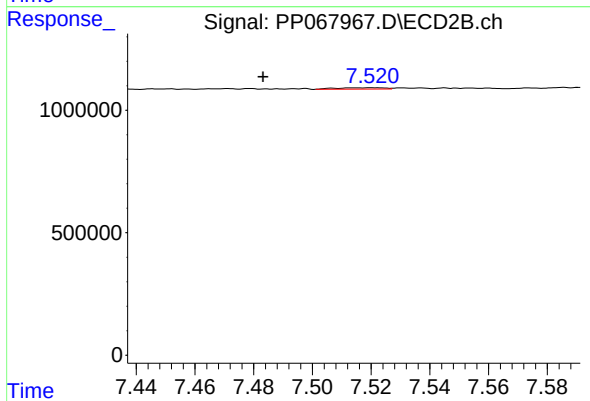

#34 AR-1260-4


R.T.: 7.521 min
Delta R.T.: 0.037 min
Response: 65654
Conc: 1.19 ng/ml

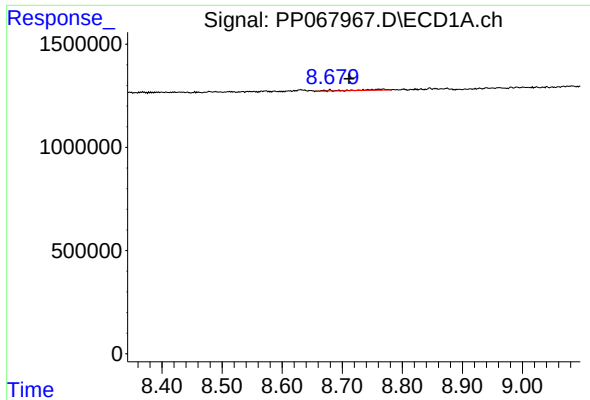

#35 AR-1260-5


R.T.: 8.769 min
Delta R.T.: 0.057 min
Response: 151573
Conc: 1.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

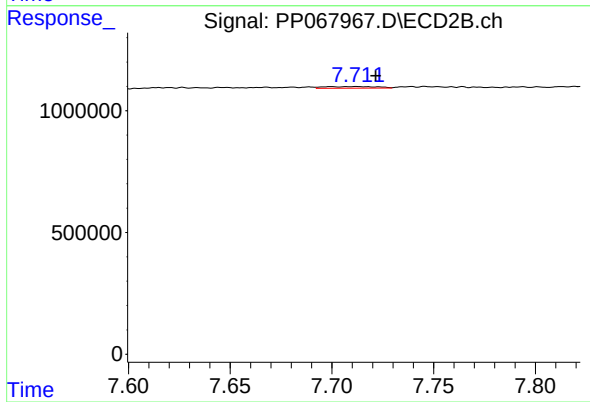


#35 AR-1260-5

R.T.: 7.712 min
Delta R.T.: -0.009 min
Response: 125120
Conc: 1.02 ng/ml

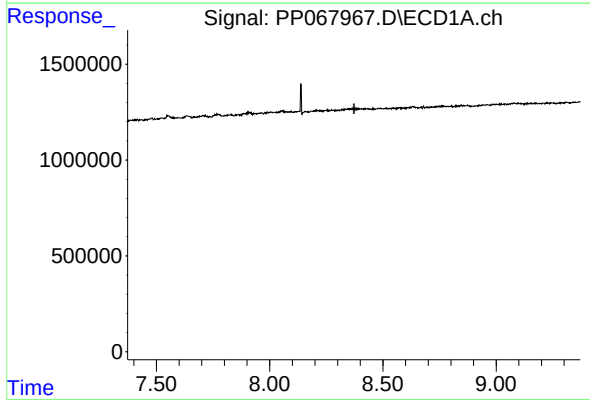


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 8.373 min
Response: 0
Conc: N.D.

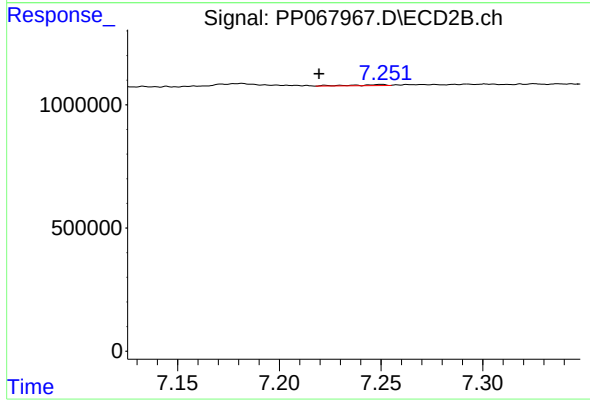

#36 AR-1262-1


R.T.: 7.250 min
Delta R.T.: 0.030 min
Response: 52109
Conc: 0.66 ng/ml

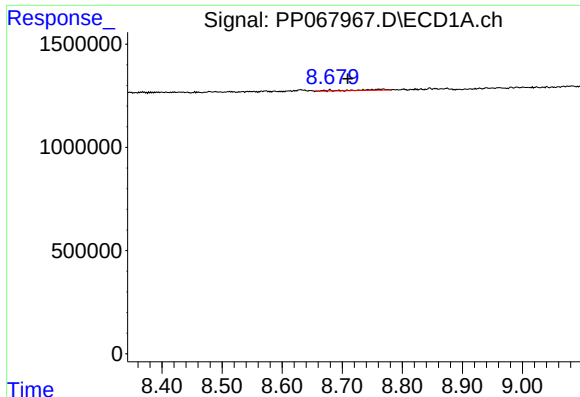

#37 AR-1262-2


R.T.: 8.769 min
Delta R.T.: 0.060 min
Response: 151573
Conc: 1.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

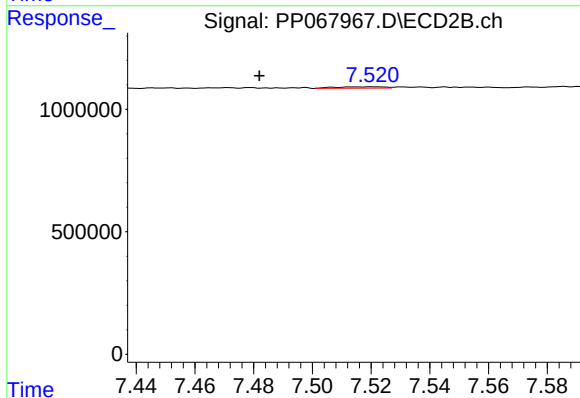


#37 AR-1262-2

R.T.: 7.521 min
Delta R.T.: 0.039 min
Response: 65654
Conc: 0.93 ng/ml

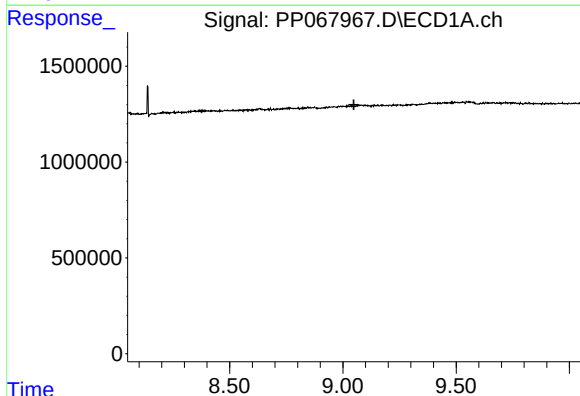


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.048 min
Response: 0
Conc: N.D.

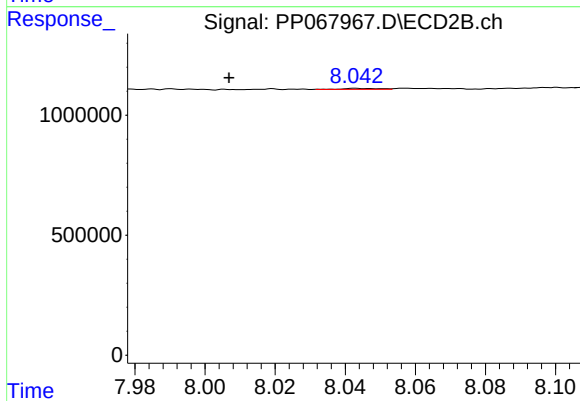

#38 AR-1262-3


R.T.: 8.043 min
Delta R.T.: 0.036 min
Response: 33641
Conc: 0.59 ng/ml

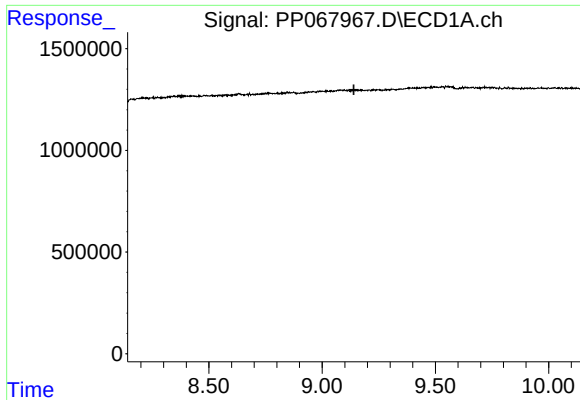

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 9.140 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

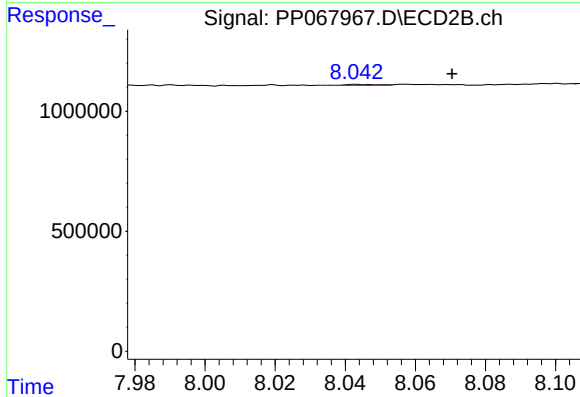


#39 AR-1262-4

R.T.: 8.043 min
Delta R.T.: -0.027 min
Response: 33641
Conc: 0.33 ng/ml

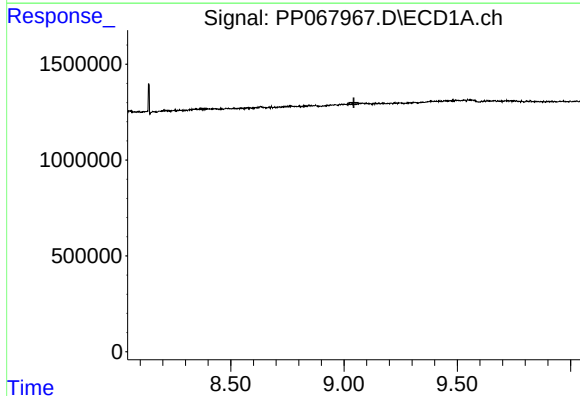


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.043 min
Response: 0
Conc: N.D.

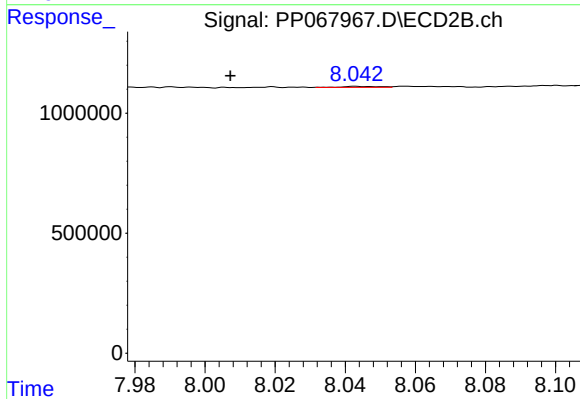

#41 AR-1268-1


R.T.: 8.043 min
Delta R.T.: 0.036 min
Response: 33641
Conc: 0.21 ng/ml

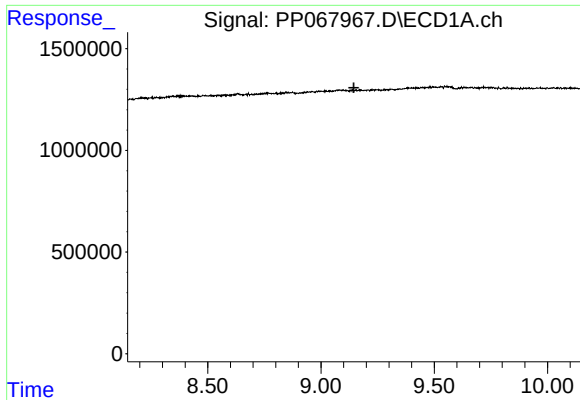

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 9.144 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

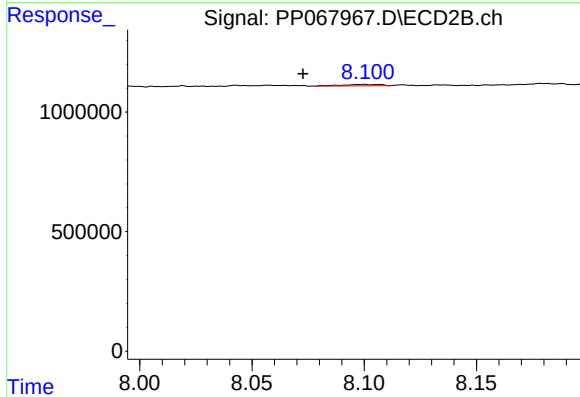


#42 AR-1268-2

R.T.: 8.100 min
Delta R.T.: 0.027 min
Response: 71724
Conc: 0.50 ng/ml

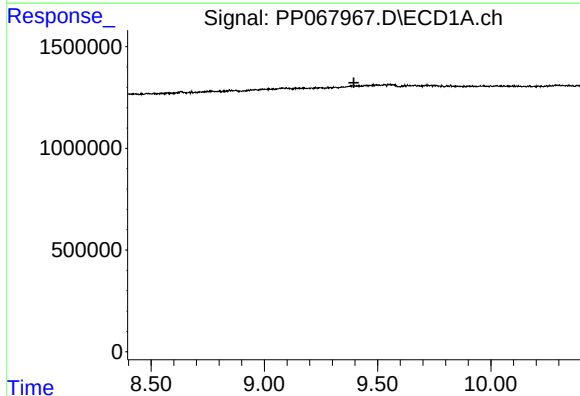


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.395 min
Response: 0
Conc: N.D.

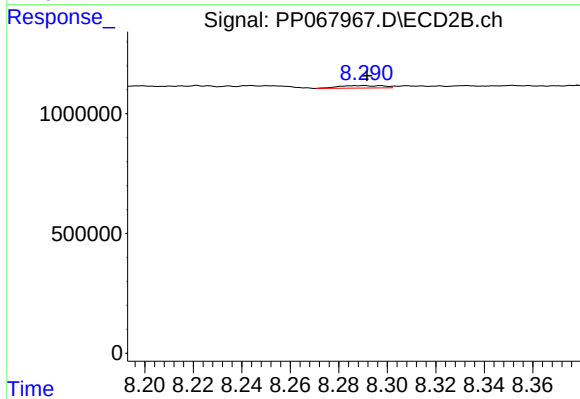

#43 AR-1268-3


R.T.: 8.290 min
Delta R.T.: -0.002 min
Response: 130751
Conc: 1.03 ng/ml

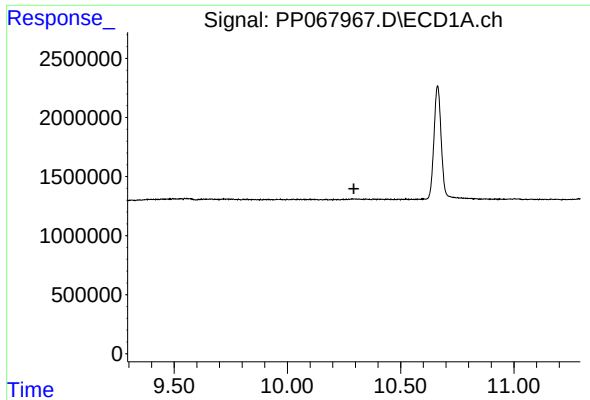

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.294 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

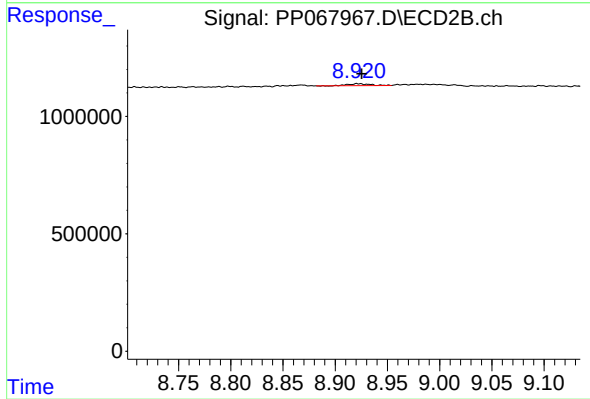

#45 AR-1268-5

R.T.: 8.921 min
Delta R.T.: -0.004 min
Response: 114035
Conc: 0.30 ng/ml