

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP101624\  
 Data File : PP067968.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 17 Oct 2024 06:24  
 Operator : YP\AJ  
 Sample : P4368-09  
 Misc : AR1242 MDL 25 PPB  
 ALS Vial : 70 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 MDL-WATER-03-QT4-2024

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 17 07:41:32 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP100824.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Oct 09 05:48:32 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound        | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml  | ng/ml    |
|-----------------------------|-----------------|--------|--------|----------|----------|--------|----------|
| -----                       |                 |        |        |          |          |        |          |
| System Monitoring Compounds |                 |        |        |          |          |        |          |
| 1)                          | SA Tetrachlo... | 4.752  | 4.050  | 16205728 | 16898393 | 17.508 | 16.724   |
| 2)                          | SA Decachlor... | 10.663 | 9.211  | 22351683 | 20702453 | 19.414 | 18.460   |
| Target Compounds            |                 |        |        |          |          |        |          |
| 3)                          | L1 AR-1016-1    | 5.915  | 5.159  | 732002   | 765014   | 22.137 | 21.866   |
| 4)                          | L1 AR-1016-2    | 5.939  | 5.178  | 1024499  | 941602   | 21.006 | 19.548   |
| 5)                          | L1 AR-1016-3    | 6.001  | 5.359  | 706722   | 542314   | 22.427 | 20.132   |
| 6)                          | L1 AR-1016-4    | 6.101  | 5.398  | 594987   | 546951   | 23.112 | 22.709   |
| 7)                          | L1 AR-1016-5    | 6.394  | 5.617  | 489934   | 634642   | 18.101 | 20.870   |
| 8)                          | L2 AR-1221-1    | 0.000  | 4.261  | 0        | 137542   | N.D.   | 10.443 # |
| 9)                          | L2 AR-1221-2    | 5.053  | 4.357  | 175715   | 387947   | 18.573 | 38.946 # |
| 10)                         | L2 AR-1221-3    | 5.119  | 4.432  | 343959   | 440657   | 11.898 | 14.155   |
| 11)                         | L3 AR-1232-1    | 5.119  | 4.432  | 343959   | 440657   | 15.046 | 18.109   |
| 12)                         | L3 AR-1232-2    | 5.649  | 5.178  | 626218   | 941602   | 53.146 | 42.102   |
| 13)                         | L3 AR-1232-3    | 5.939  | 5.359  | 1024499  | 542314   | 45.993 | 45.405   |
| 14)                         | L3 AR-1232-4    | 6.101  | 5.442  | 594987   | 604053   | 52.712 | 52.383   |
| 15)                         | L3 AR-1232-5    | 6.187  | 5.617  | 456349   | 634642   | 50.037 | 47.184   |
| 16)                         | L4 AR-1242-1    | 5.915  | 5.159  | 732002   | 765014   | 26.202 | 26.310   |
| 17)                         | L4 AR-1242-2    | 5.939  | 5.178  | 1024499  | 941602   | 25.212 | 23.453   |
| 18)                         | L4 AR-1242-3    | 6.001  | 5.359  | 706722   | 542314   | 26.209 | 24.108   |
| 19)                         | L4 AR-1242-4    | 6.101  | 5.442  | 594987   | 604053   | 27.738 | 25.447   |
| 20)                         | L4 AR-1242-5    | 6.834  | 5.972  | 608102   | 733805   | 25.205 | 25.613   |
| 21)                         | L5 AR-1248-1    | 5.915  | 5.159  | 732002   | 765014   | 34.169 | 33.755   |
| 22)                         | L5 AR-1248-2    | 6.187  | 5.398  | 456349   | 546951   | 13.575 | 16.526   |
| 23)                         | L5 AR-1248-3    | 6.394  | 5.442  | 489934   | 604053   | 13.377 | 17.522 # |
| 24)                         | L5 AR-1248-4    | 6.796  | 5.617  | 593286   | 634642   | 14.667 | 15.496   |
| 25)                         | L5 AR-1248-5    | 6.834  | 6.014  | 608102   | 589973   | 15.332 | 15.757   |
| 26)                         | L6 AR-1254-1    | 6.772  | 5.972  | 569045   | 733805   | 12.707 | 12.420   |
| 27)                         | L6 AR-1254-2    | 6.992  | 6.118  | 664627   | 278194   | 10.055 | 5.303 #  |
| 28)                         | L6 AR-1254-3    | 7.353  | 6.530  | 417576   | 423299   | 6.012  | 5.087    |
| 29)                         | L6 AR-1254-4    | 7.635  | 6.757  | 373056   | 247352   | 7.475  | 5.124 #  |
| 30)                         | L6 AR-1254-5    | 8.053  | 7.181  | 163952   | 340283   | 2.765  | 4.626 #  |
| 31)                         | L7 AR-1260-1    | 7.550  | 6.662  | 481521   | 49923    | 8.913  | 0.876 #  |
| 32)                         | L7 AR-1260-2    | 7.776  | 6.852  | 165269   | 31076    | 2.612  | 0.466 #  |
| 33)                         | L7 AR-1260-3    | 0.000  | 7.004  | 0        | 216269   | N.D.   | 3.395 #  |
| 34)                         | L7 AR-1260-4    | 0.000  | 7.470  | 0        | 79362    | N.D.   | 1.435 #  |
| 35)                         | L7 AR-1260-5    | 0.000  | 7.720  | 0        | 100188   | N.D.   | 0.819 #  |
| 36)                         | L8 AR-1262-1    | 0.000  | 7.222  | 0        | 37112    | N.D.   | 0.472 #  |
| 37)                         | L8 AR-1262-2    | 0.000  | 7.470  | 0        | 79362    | N.D.   | 1.118 #  |
| 38)                         | L8 AR-1262-3    | 9.063  | 8.049f | 156045   | 44502    | 1.763  | 0.779 #  |
| 39)                         | L8 AR-1262-4    | 0.000  | 8.063  | 0        | 51402    | N.D.   | 0.512 #  |
| 41)                         | L9 AR-1268-1    | 9.063  | 8.049f | 156045   | 44502    | 1.022  | 0.280 #  |
| 42)                         | L9 AR-1268-2    | 0.000  | 8.063  | 0        | 51402    | N.D.   | 0.359 #  |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP101624\  
Data File : PP067968.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 17 Oct 2024 06:24  
Operator : YP\AJ  
Sample : P4368-09  
Misc : AR1242 MDL 25 PPB  
ALS Vial : 70 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 17 07:41:32 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP100824.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Oct 09 05:48:32 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|        | Compound  | RT#1  | RT#2  | Resp#1 | Resp#2 | ng/ml | ng/ml   |
|--------|-----------|-------|-------|--------|--------|-------|---------|
| 43) L9 | AR-1268-3 | 0.000 | 8.302 | 0      | 99021  | N.D.  | 0.777 # |
| 45) L9 | AR-1268-5 | 0.000 | 8.922 | 0      | 71670  | N.D.  | 0.190 # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP101624\  
Data File : PP067968.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 17 Oct 2024 06:24  
Operator : YP\AJ  
Sample : P4368-09  
Misc : AR1242 MDL 25 PPB  
ALS Vial : 70 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 17 07:41:32 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP100824.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Oct 09 05:48:32 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

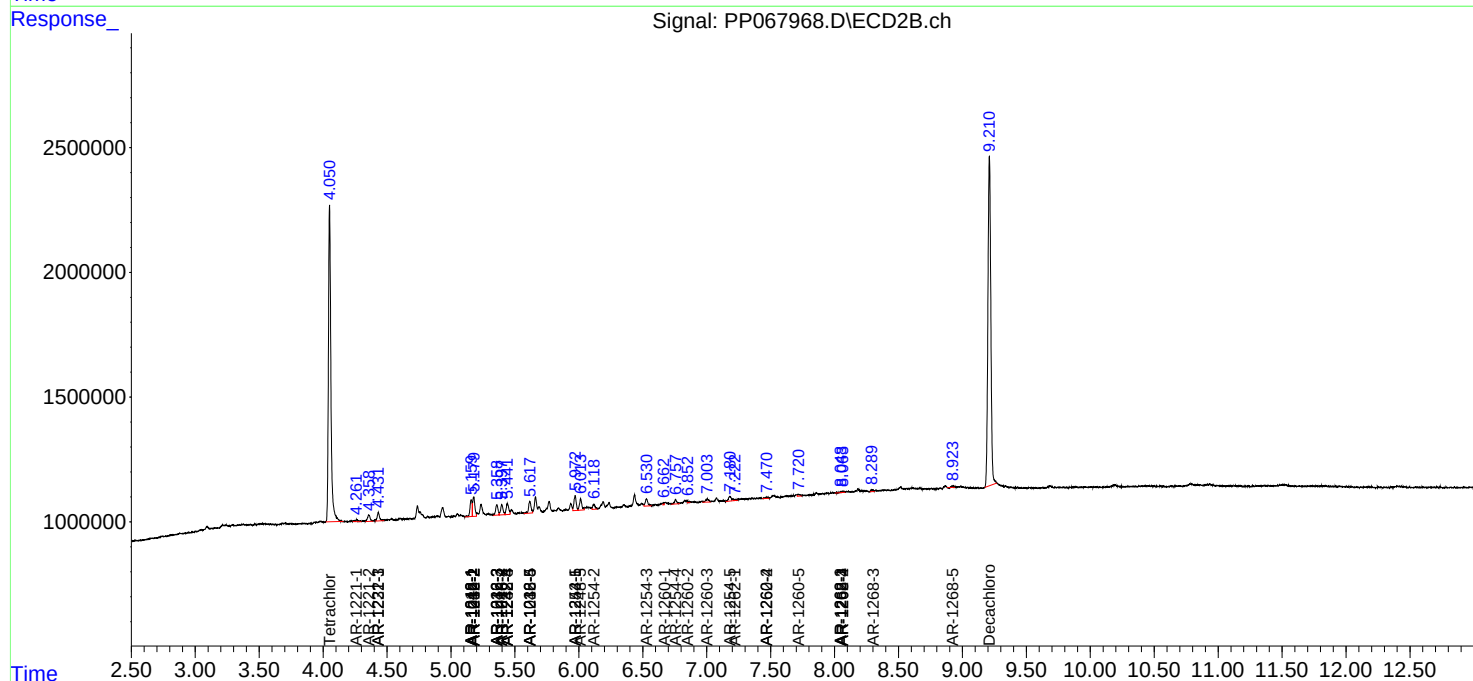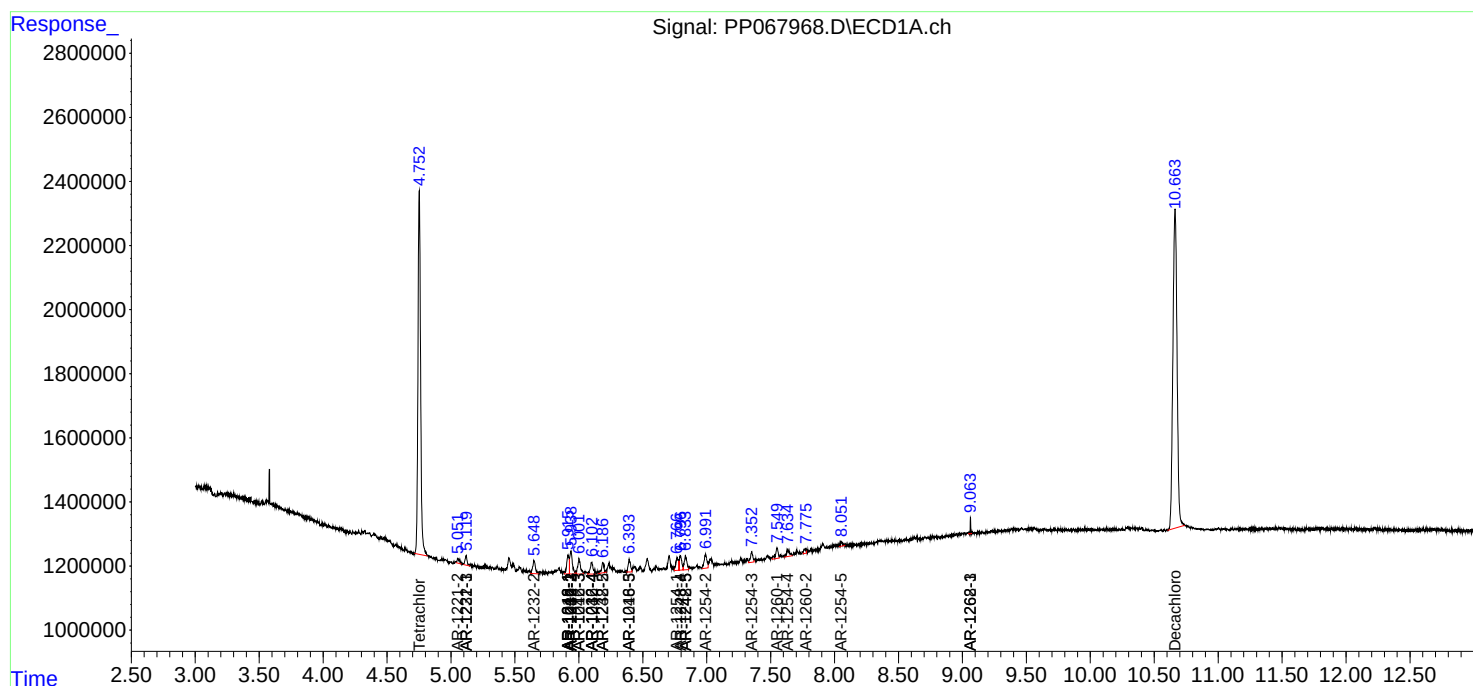


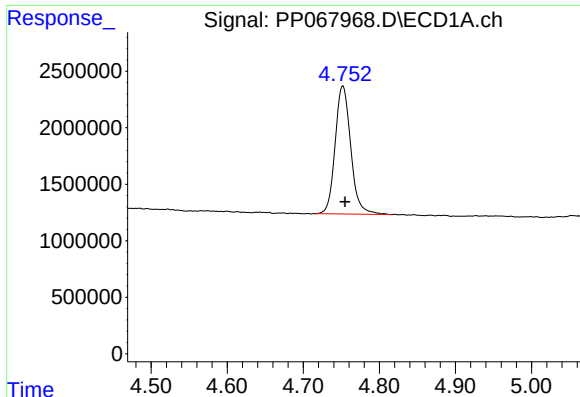

#1 Tetrachloro-m-xylene


R.T.: 4.752 min  
Delta R.T.: -0.003 min  
Response: 16205728  
Conc: 17.51 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

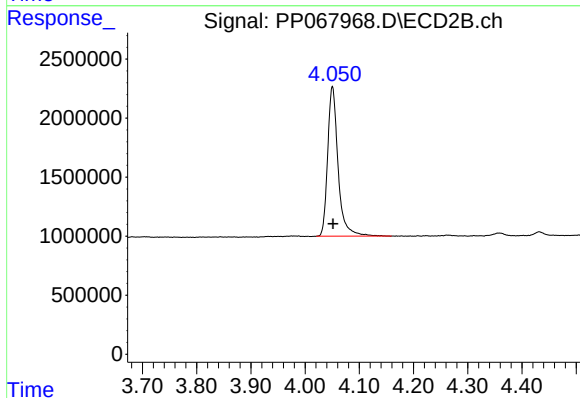


#1 Tetrachloro-m-xylene

R.T.: 4.050 min  
Delta R.T.: -0.002 min  
Response: 16898393  
Conc: 16.72 ng/ml

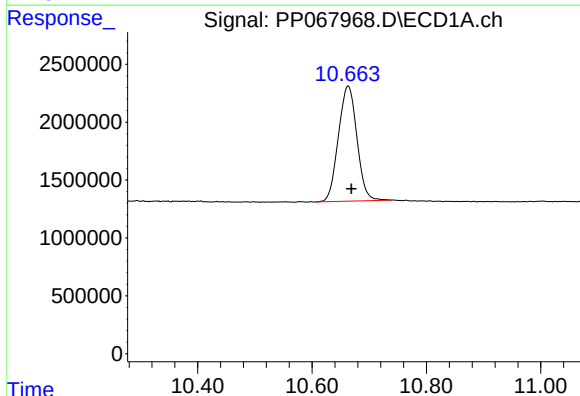


#2 Decachlorobiphenyl

R.T.: 10.663 min  
Delta R.T.: -0.006 min  
Response: 22351683  
Conc: 19.41 ng/ml

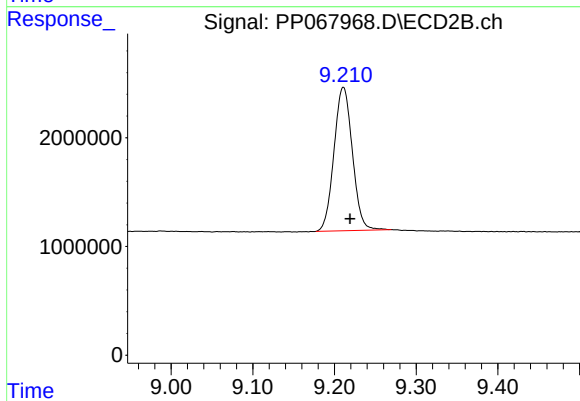

#2 Decachlorobiphenyl


R.T.: 9.211 min  
Delta R.T.: -0.008 min  
Response: 20702453  
Conc: 18.46 ng/ml

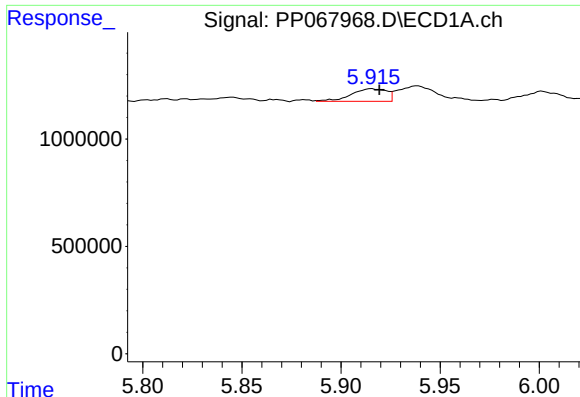

#3 AR-1016-1


R.T.: 5.915 min  
Delta R.T.: -0.004 min  
Response: 732002  
Conc: 22.14 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

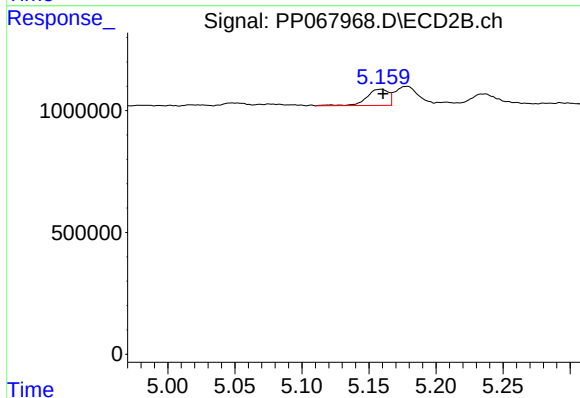


#3 AR-1016-1

R.T.: 5.159 min  
Delta R.T.: -0.002 min  
Response: 765014  
Conc: 21.87 ng/ml

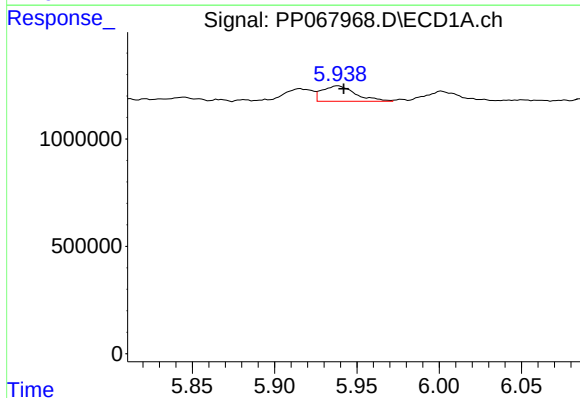


#4 AR-1016-2

R.T.: 5.939 min  
Delta R.T.: -0.003 min  
Response: 1024499  
Conc: 21.01 ng/ml

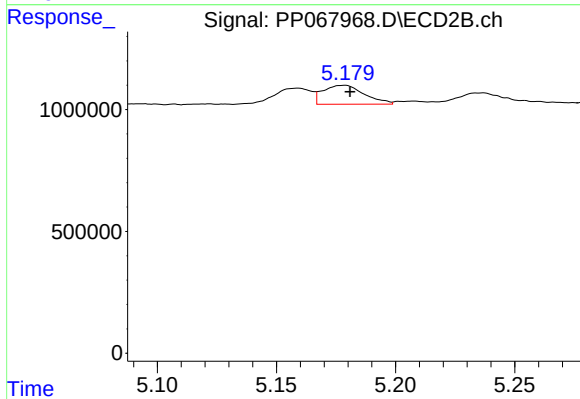

#4 AR-1016-2


R.T.: 5.178 min  
Delta R.T.: -0.003 min  
Response: 941602  
Conc: 19.55 ng/ml

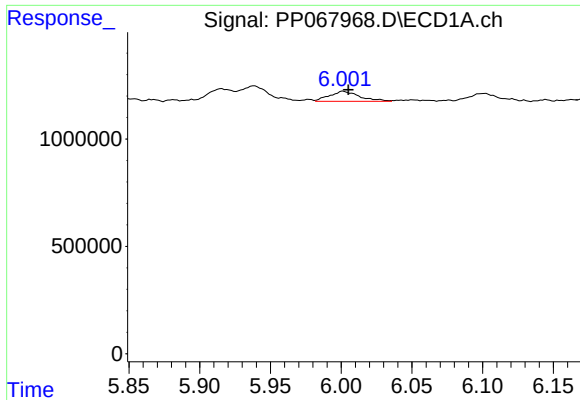

#5 AR-1016-3


R.T.: 6.001 min  
Delta R.T.: -0.004 min  
Response: 706722  
Conc: 22.43 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

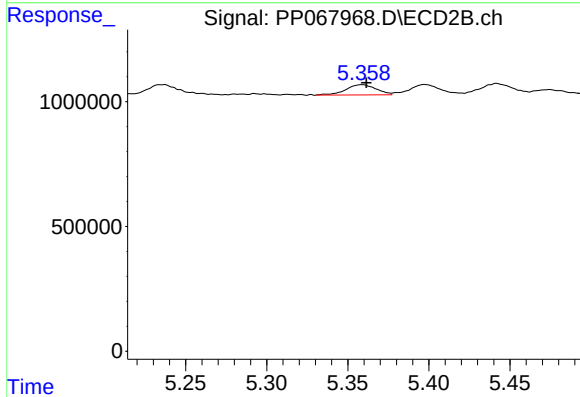


#5 AR-1016-3

R.T.: 5.359 min  
Delta R.T.: -0.003 min  
Response: 542314  
Conc: 20.13 ng/ml

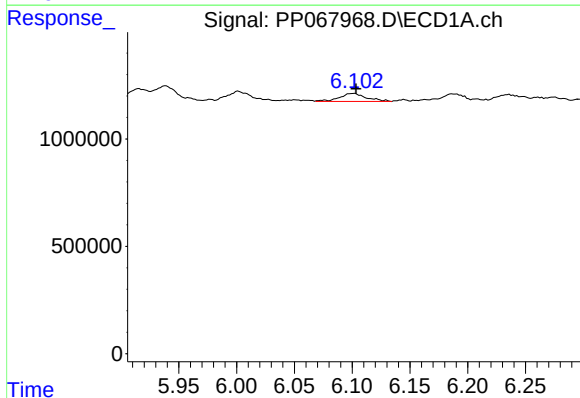


#6 AR-1016-4

R.T.: 6.101 min  
Delta R.T.: -0.002 min  
Response: 594987  
Conc: 23.11 ng/ml

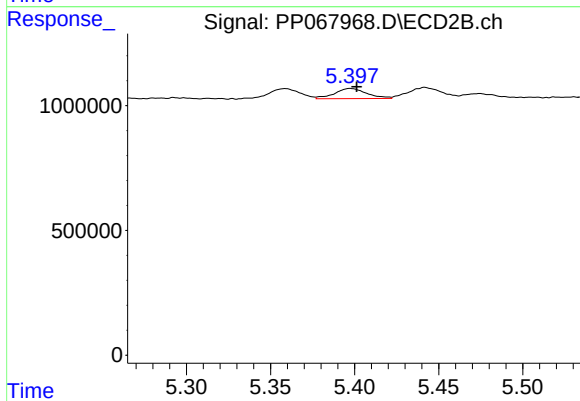

#6 AR-1016-4


R.T.: 5.398 min  
Delta R.T.: -0.004 min  
Response: 546951  
Conc: 22.71 ng/ml

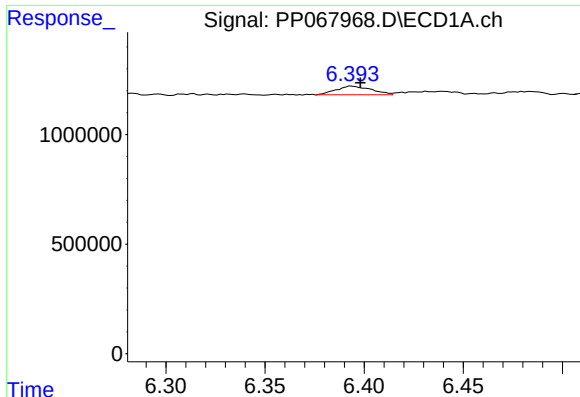

#7 AR-1016-5


R.T.: 6.394 min  
Delta R.T.: -0.004 min  
Response: 489934  
Conc: 18.10 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

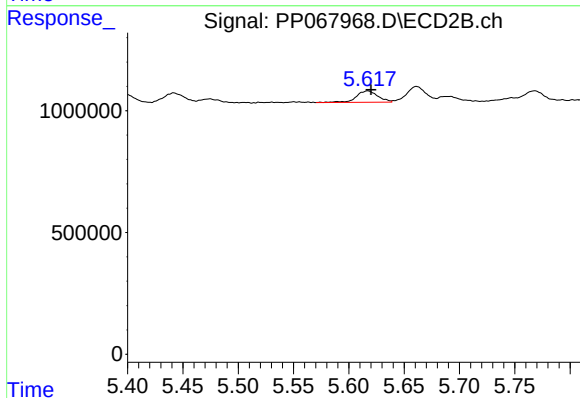


#7 AR-1016-5

R.T.: 5.617 min  
Delta R.T.: -0.003 min  
Response: 634642  
Conc: 20.87 ng/ml

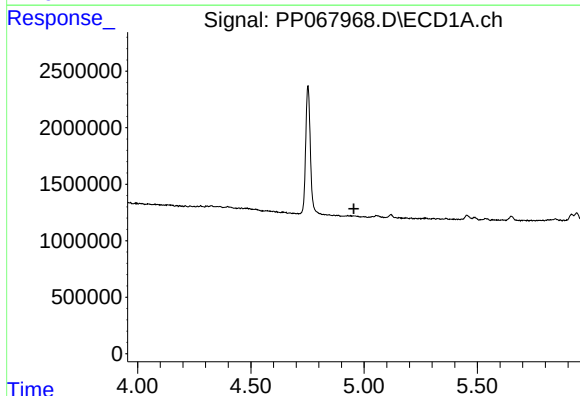


#8 AR-1221-1

R.T.: 0.000 min  
Exp R.T. : 4.955 min  
Response: 0  
Conc: N.D.

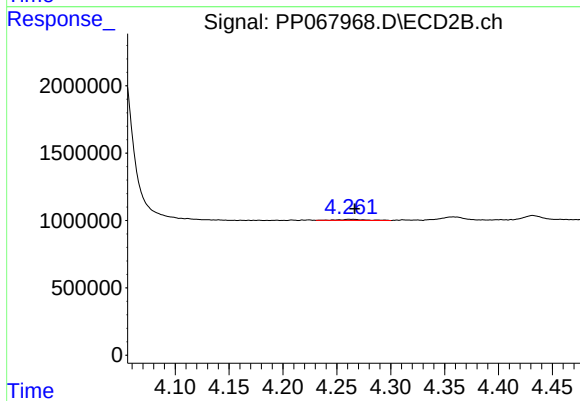

#8 AR-1221-1


R.T.: 4.261 min  
Delta R.T.: -0.005 min  
Response: 137542  
Conc: 10.44 ng/ml

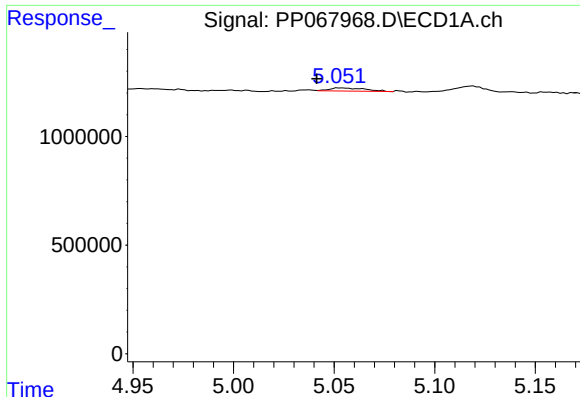

#9 AR-1221-2


R.T.: 5.053 min  
Delta R.T.: 0.012 min  
Response: 175715  
Conc: 18.57 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

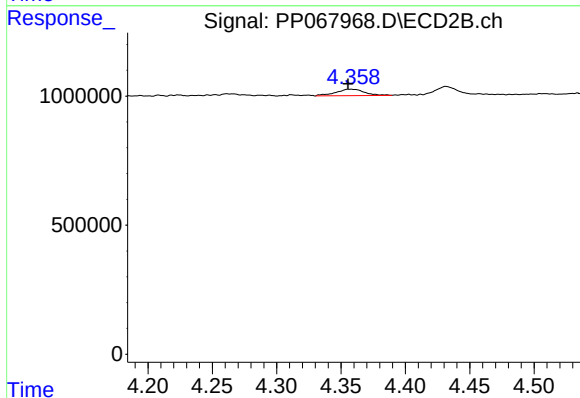


#9 AR-1221-2

R.T.: 4.357 min  
Delta R.T.: 0.002 min  
Response: 387947  
Conc: 38.95 ng/ml

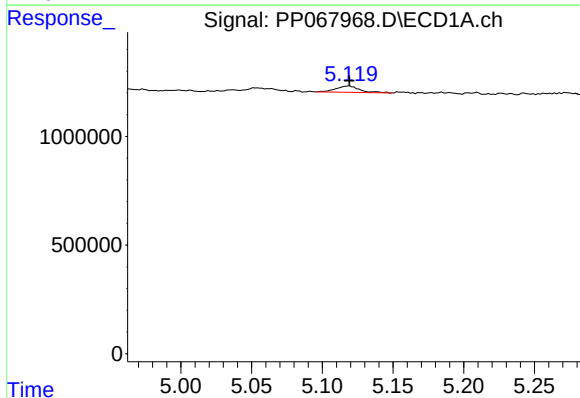

#10 AR-1221-3


R.T.: 5.119 min  
Delta R.T.: 0.000 min  
Response: 343959  
Conc: 11.90 ng/ml

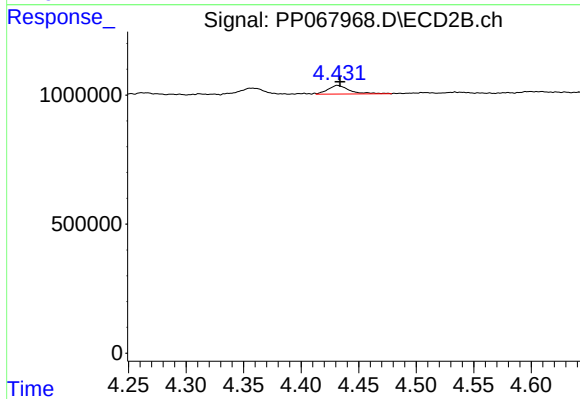

#10 AR-1221-3

R.T.: 4.432 min  
Delta R.T.: -0.002 min  
Response: 440657  
Conc: 14.15 ng/ml




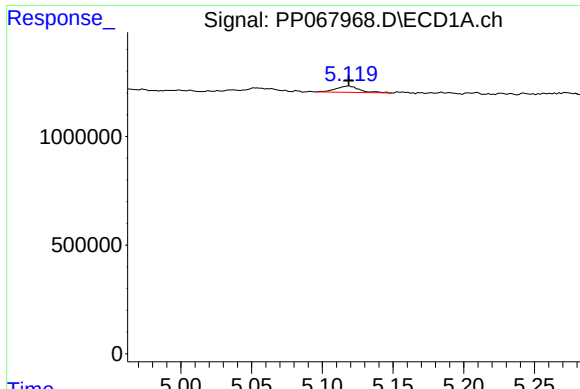

#11 AR-1232-1


R.T.: 5.119 min  
Delta R.T.: 0.000 min  
Response: 343959  
Conc: 15.05 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

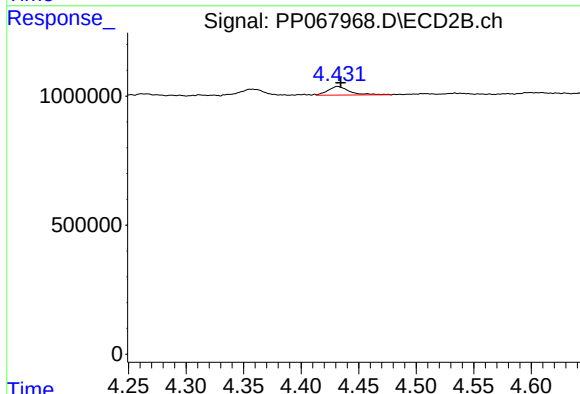


#11 AR-1232-1

R.T.: 4.432 min  
Delta R.T.: -0.003 min  
Response: 440657  
Conc: 18.11 ng/ml

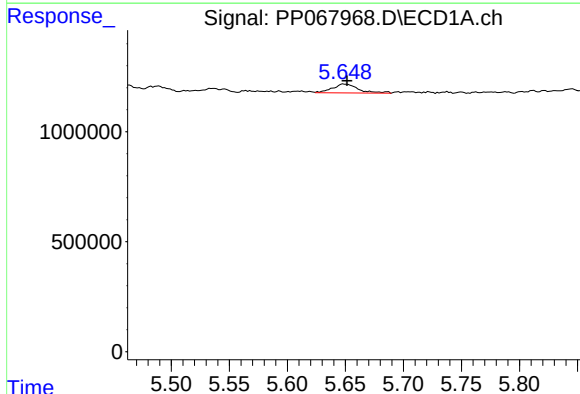


#12 AR-1232-2

R.T.: 5.649 min  
Delta R.T.: -0.003 min  
Response: 626218  
Conc: 53.15 ng/ml

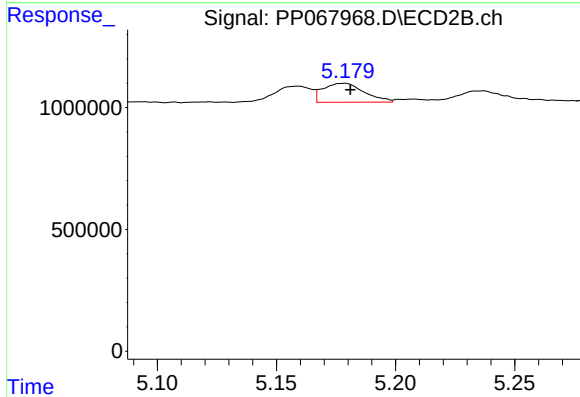

#12 AR-1232-2


R.T.: 5.178 min  
Delta R.T.: -0.003 min  
Response: 941602  
Conc: 42.10 ng/ml

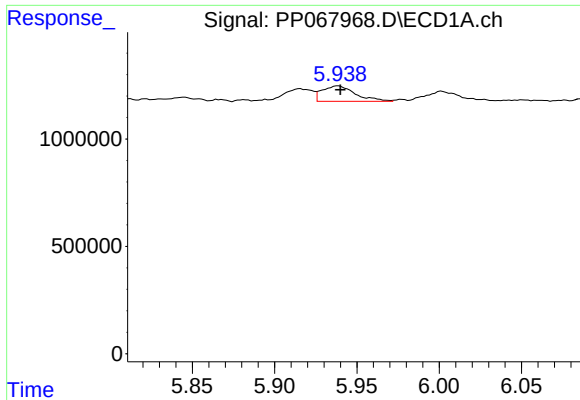

#13 AR-1232-3


R.T.: 5.939 min  
Delta R.T.: -0.001 min  
Response: 1024499  
Conc: 45.99 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

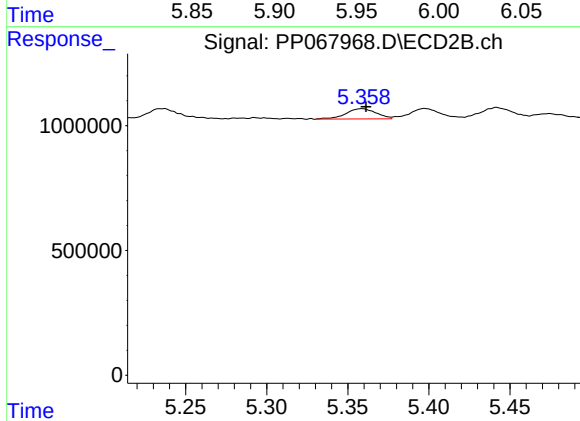


#13 AR-1232-3

R.T.: 5.359 min  
Delta R.T.: -0.003 min  
Response: 542314  
Conc: 45.41 ng/ml

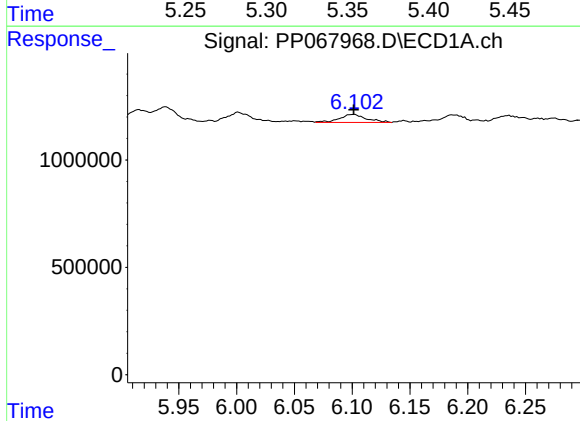


#14 AR-1232-4

R.T.: 6.101 min  
Delta R.T.: 0.000 min  
Response: 594987  
Conc: 52.71 ng/ml

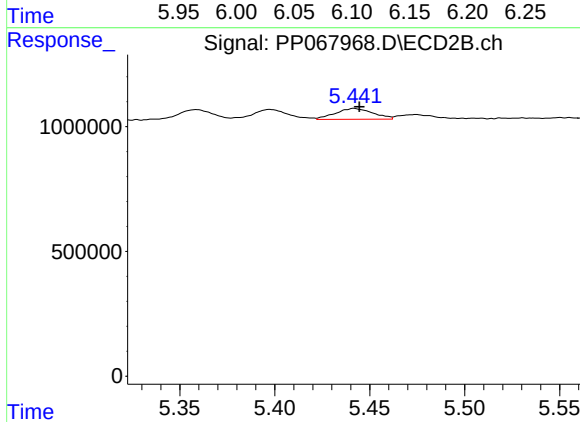

#14 AR-1232-4


R.T.: 5.442 min  
Delta R.T.: -0.003 min  
Response: 604053  
Conc: 52.38 ng/ml

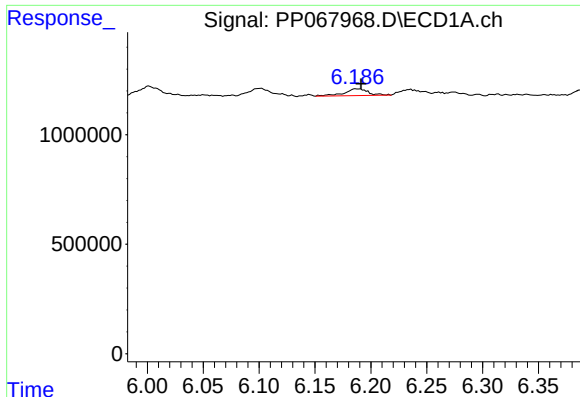

#15 AR-1232-5


R.T.: 6.187 min  
Delta R.T.: -0.004 min  
Response: 456349  
Conc: 50.04 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

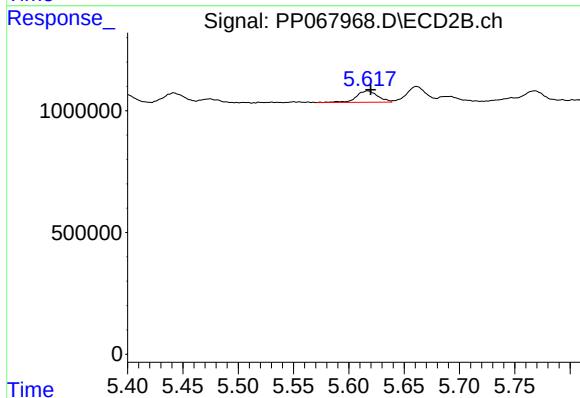


#15 AR-1232-5

R.T.: 5.617 min  
Delta R.T.: -0.003 min  
Response: 634642  
Conc: 47.18 ng/ml

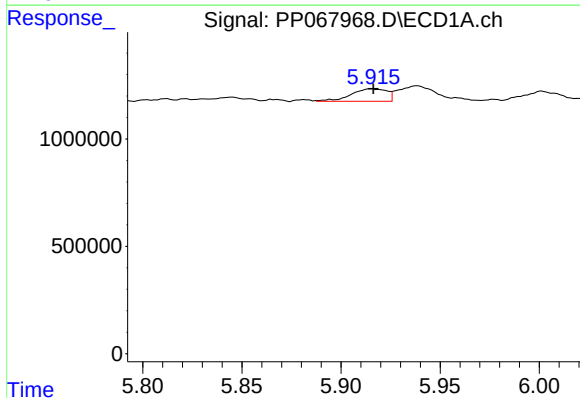


#16 AR-1242-1

R.T.: 5.915 min  
Delta R.T.: -0.001 min  
Response: 732002  
Conc: 26.20 ng/ml

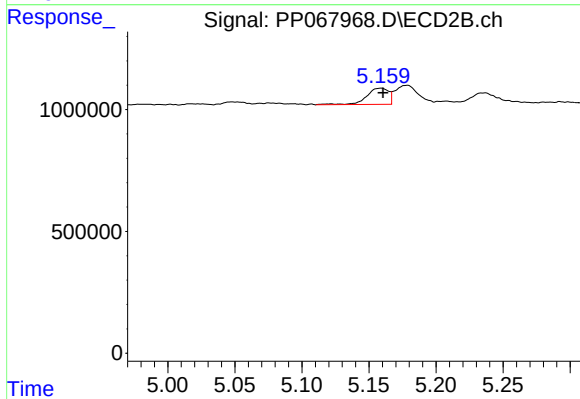

#16 AR-1242-1


R.T.: 5.159 min  
Delta R.T.: -0.002 min  
Response: 765014  
Conc: 26.31 ng/ml

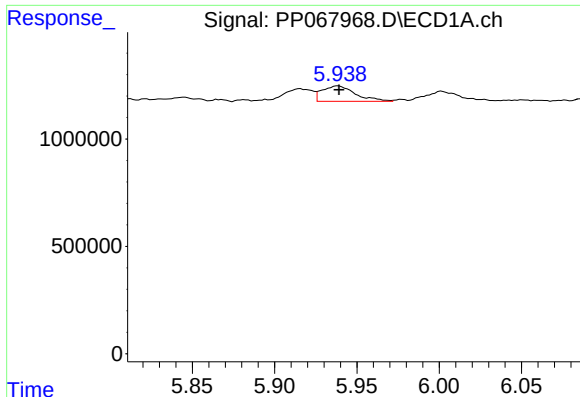

#17 AR-1242-2


R.T.: 5.939 min  
Delta R.T.: 0.000 min  
Response: 1024499  
Conc: 25.21 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

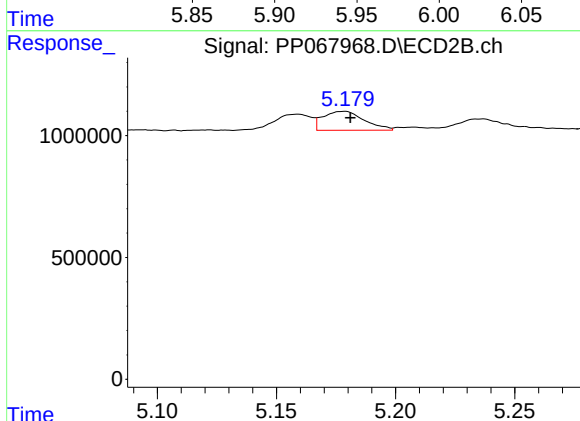


#17 AR-1242-2

R.T.: 5.178 min  
Delta R.T.: -0.003 min  
Response: 941602  
Conc: 23.45 ng/ml

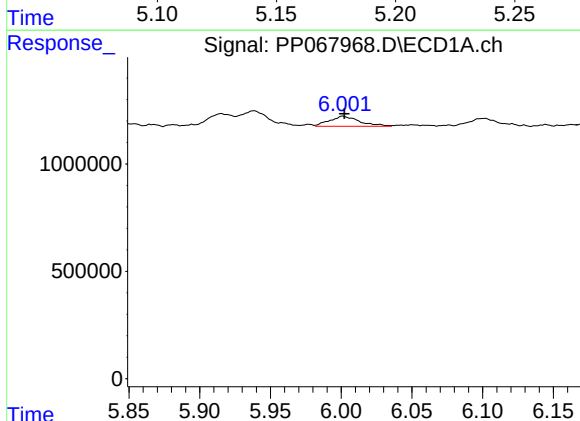


#18 AR-1242-3

R.T.: 6.001 min  
Delta R.T.: 0.000 min  
Response: 706722  
Conc: 26.21 ng/ml

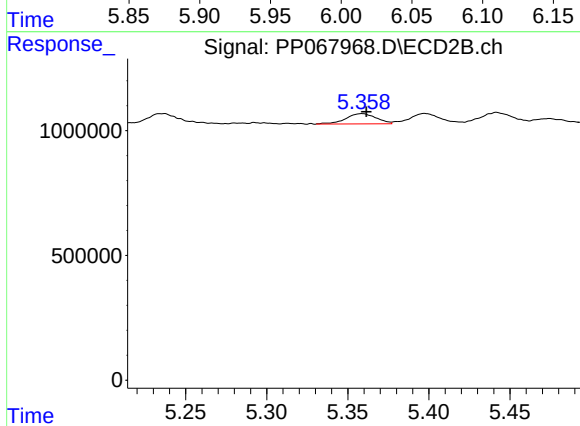

#18 AR-1242-3


R.T.: 5.359 min  
Delta R.T.: -0.003 min  
Response: 542314  
Conc: 24.11 ng/ml

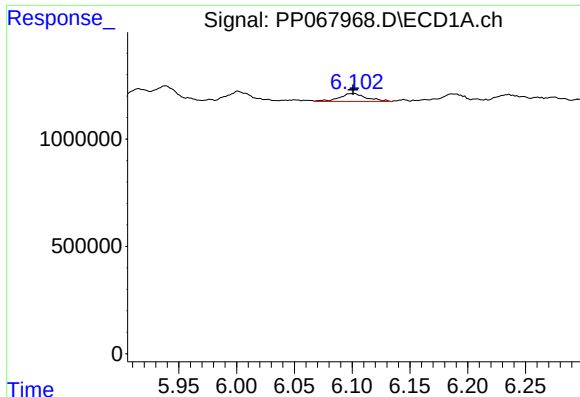

#19 AR-1242-4


R.T.: 6.101 min  
Delta R.T.: 0.000 min  
Response: 594987  
Conc: 27.74 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

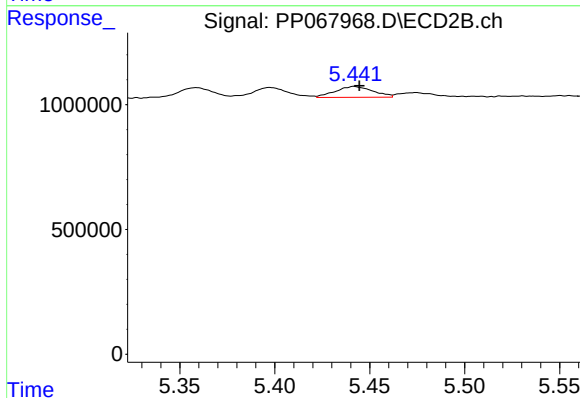


#19 AR-1242-4

R.T.: 5.442 min  
Delta R.T.: -0.003 min  
Response: 604053  
Conc: 25.45 ng/ml

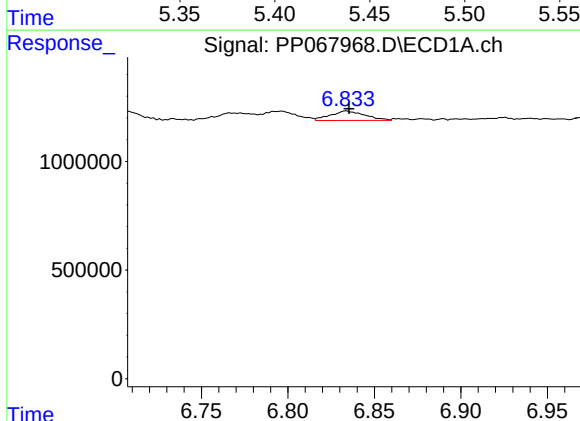


#20 AR-1242-5

R.T.: 6.834 min  
Delta R.T.: -0.001 min  
Response: 608102  
Conc: 25.21 ng/ml

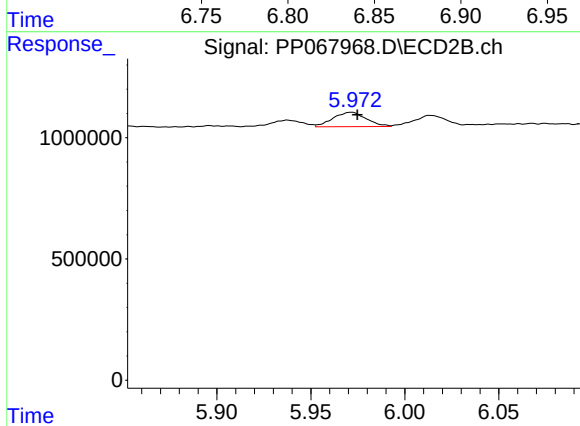

#20 AR-1242-5


R.T.: 5.972 min  
Delta R.T.: -0.003 min  
Response: 733805  
Conc: 25.61 ng/ml

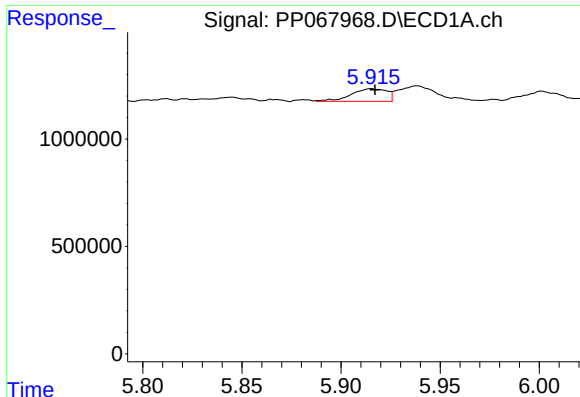

#21 AR-1248-1


R.T.: 5.915 min  
Delta R.T.: -0.002 min  
Response: 732002  
Conc: 34.17 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

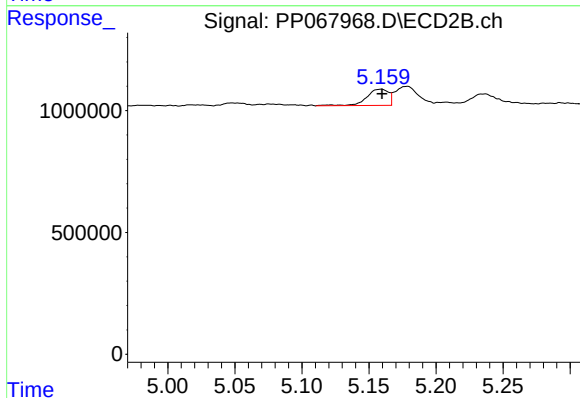


#21 AR-1248-1

R.T.: 5.159 min  
Delta R.T.: -0.001 min  
Response: 765014  
Conc: 33.75 ng/ml

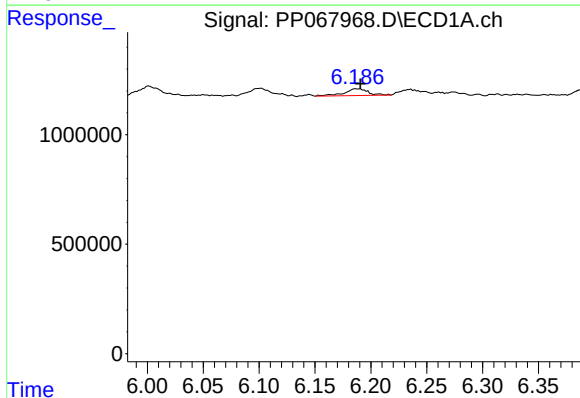


#22 AR-1248-2

R.T.: 6.187 min  
Delta R.T.: -0.004 min  
Response: 456349  
Conc: 13.58 ng/ml

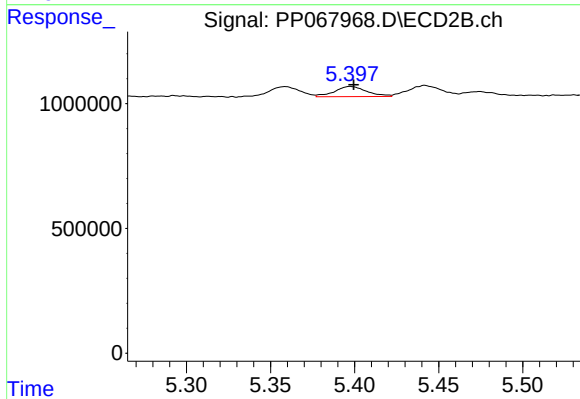

#22 AR-1248-2


R.T.: 5.398 min  
Delta R.T.: -0.002 min  
Response: 546951  
Conc: 16.53 ng/ml

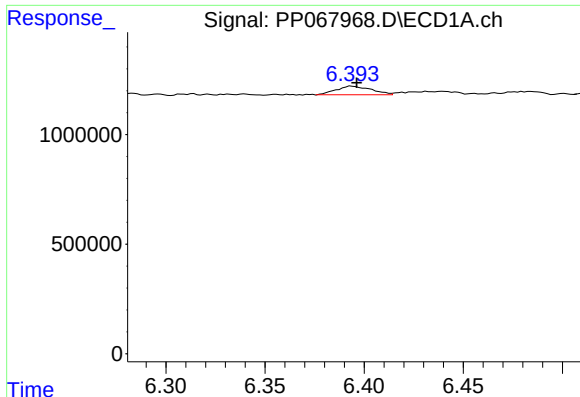

#23 AR-1248-3


R.T.: 6.394 min  
Delta R.T.: -0.002 min  
Response: 489934  
Conc: 13.38 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

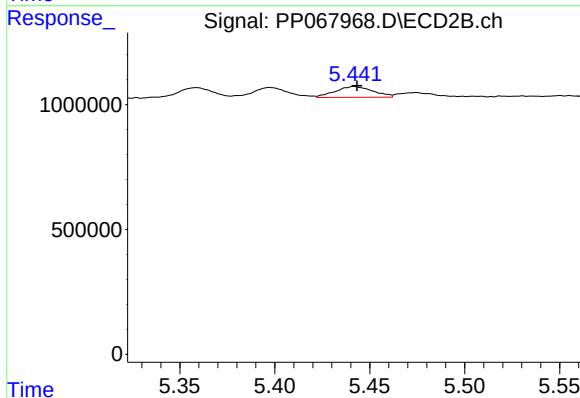


#23 AR-1248-3

R.T.: 5.442 min  
Delta R.T.: -0.002 min  
Response: 604053  
Conc: 17.52 ng/ml

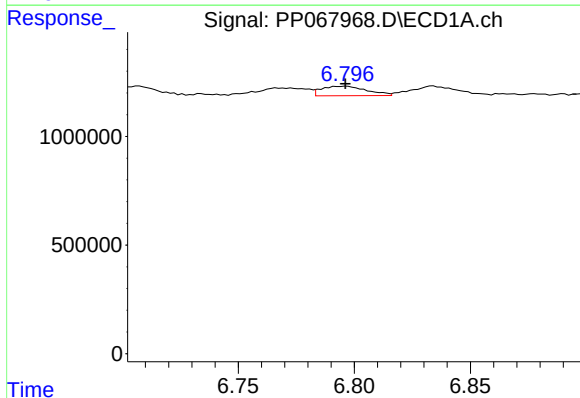


#24 AR-1248-4

R.T.: 6.796 min  
Delta R.T.: 0.000 min  
Response: 593286  
Conc: 14.67 ng/ml

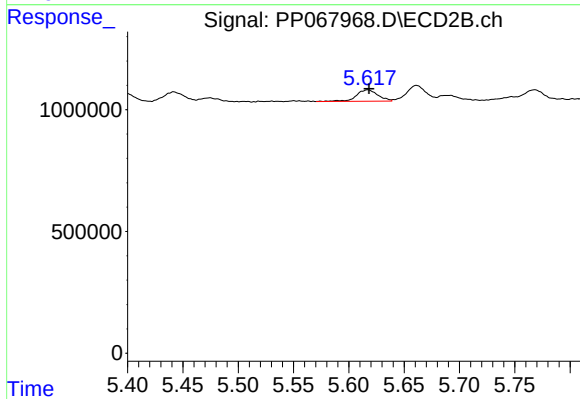

#24 AR-1248-4


R.T.: 5.617 min  
Delta R.T.: -0.001 min  
Response: 634642  
Conc: 15.50 ng/ml

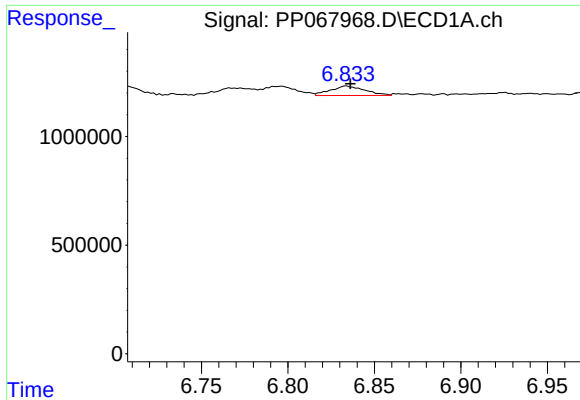

#25 AR-1248-5


R.T.: 6.834 min  
Delta R.T.: -0.002 min  
Response: 608102  
Conc: 15.33 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

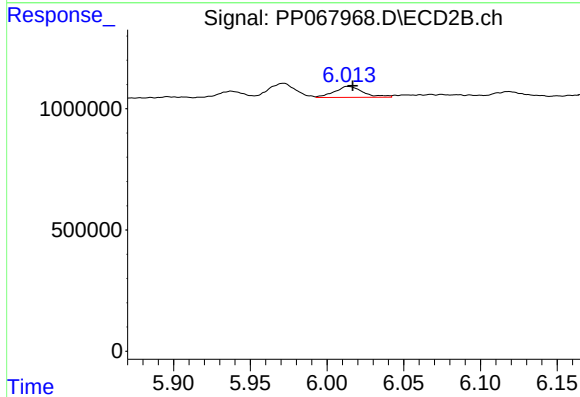


#25 AR-1248-5

R.T.: 6.014 min  
Delta R.T.: -0.003 min  
Response: 589973  
Conc: 15.76 ng/ml

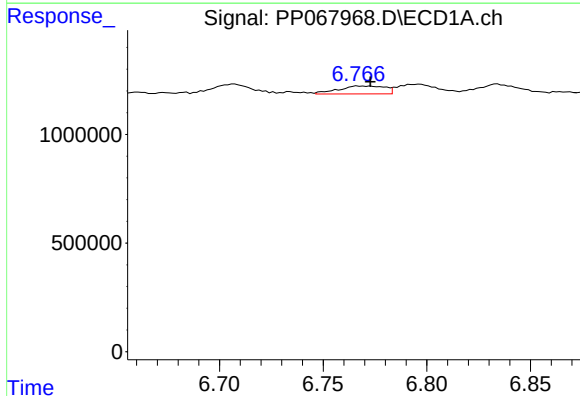

#26 AR-1254-1


R.T.: 6.772 min  
Delta R.T.: 0.000 min  
Response: 569045  
Conc: 12.71 ng/ml

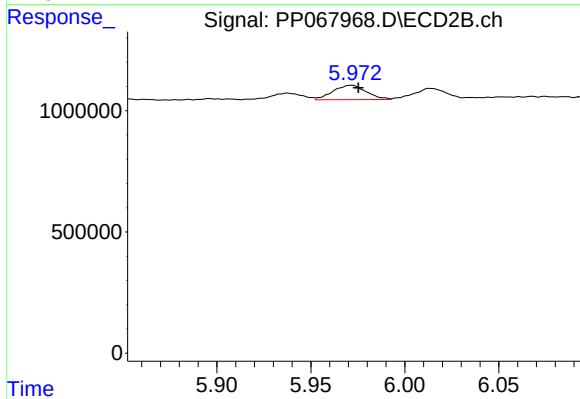

#26 AR-1254-1

R.T.: 5.972 min  
Delta R.T.: -0.004 min  
Response: 733805  
Conc: 12.42 ng/ml




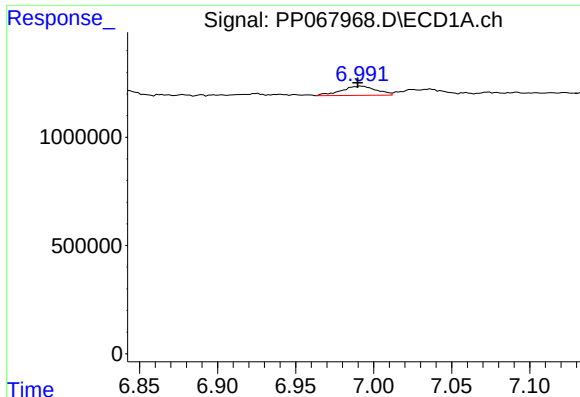

#27 AR-1254-2


R.T.: 6.992 min  
Delta R.T.: 0.002 min  
Response: 664627  
Conc: 10.06 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

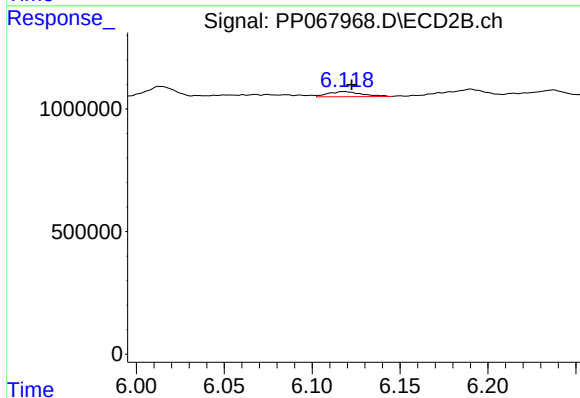


#27 AR-1254-2

R.T.: 6.118 min  
Delta R.T.: -0.004 min  
Response: 278194  
Conc: 5.30 ng/ml

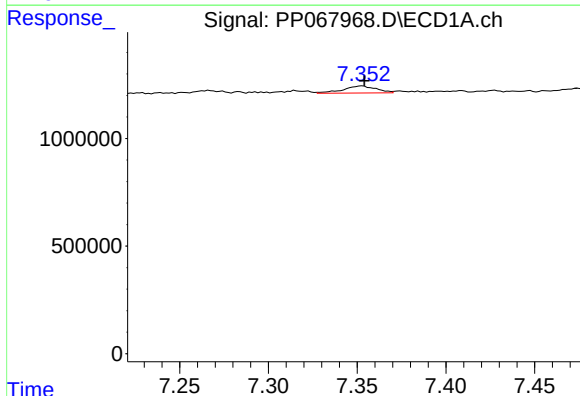


#28 AR-1254-3

R.T.: 7.353 min  
Delta R.T.: -0.001 min  
Response: 417576  
Conc: 6.01 ng/ml

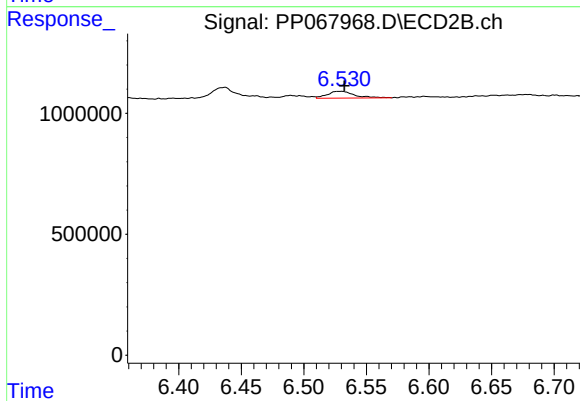

#28 AR-1254-3


R.T.: 6.530 min  
Delta R.T.: -0.003 min  
Response: 423299  
Conc: 5.09 ng/ml

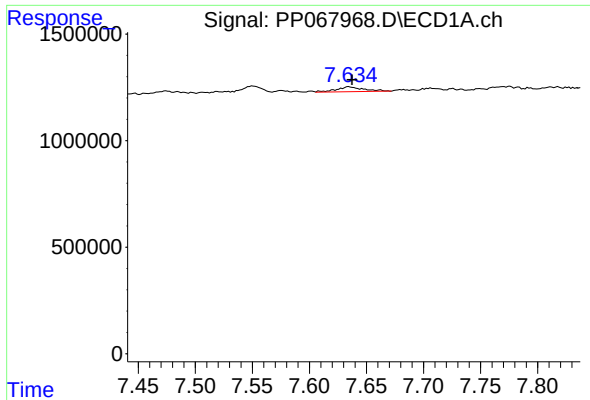

#29 AR-1254-4


R.T.: 7.635 min  
Delta R.T.: -0.003 min  
Response: 373056  
Conc: 7.48 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

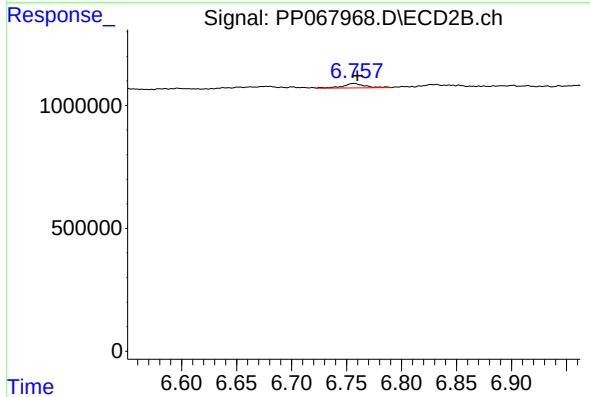


#29 AR-1254-4

R.T.: 6.757 min  
Delta R.T.: -0.003 min  
Response: 247352  
Conc: 5.12 ng/ml

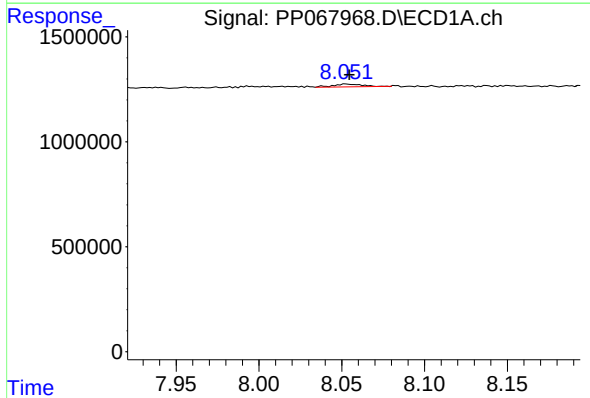


#30 AR-1254-5

R.T.: 8.053 min  
Delta R.T.: -0.002 min  
Response: 163952  
Conc: 2.77 ng/ml

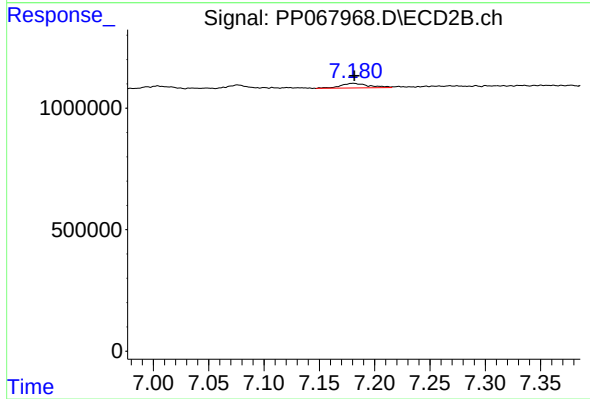

#30 AR-1254-5


R.T.: 7.181 min  
Delta R.T.: -0.001 min  
Response: 340283  
Conc: 4.63 ng/ml

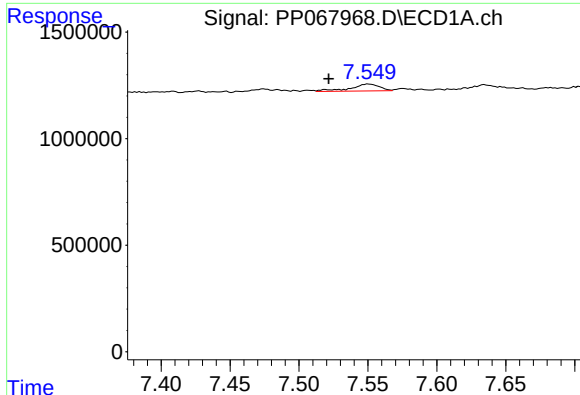

#31 AR-1260-1


R.T.: 7.550 min  
Delta R.T.: 0.029 min  
Response: 481521  
Conc: 8.91 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

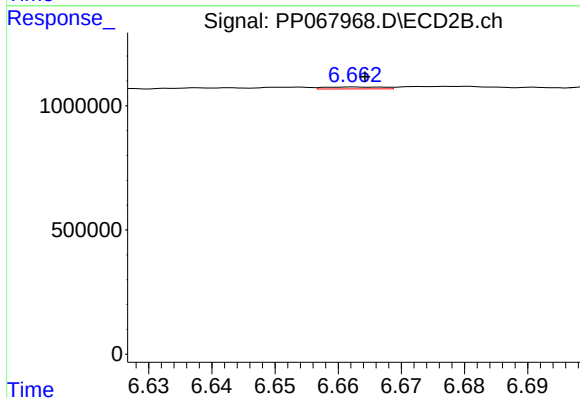


#31 AR-1260-1

R.T.: 6.662 min  
Delta R.T.: -0.002 min  
Response: 49923  
Conc: 0.88 ng/ml

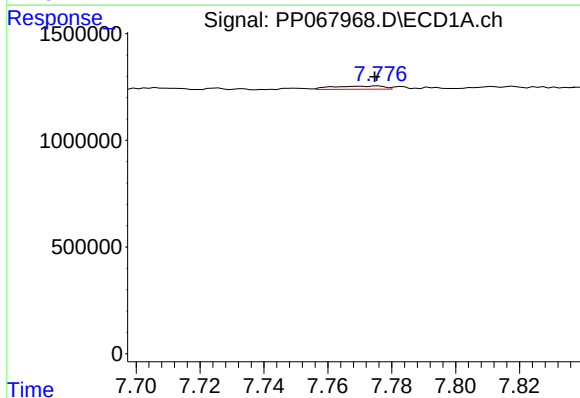


#32 AR-1260-2

R.T.: 7.776 min  
Delta R.T.: 0.000 min  
Response: 165269  
Conc: 2.61 ng/ml

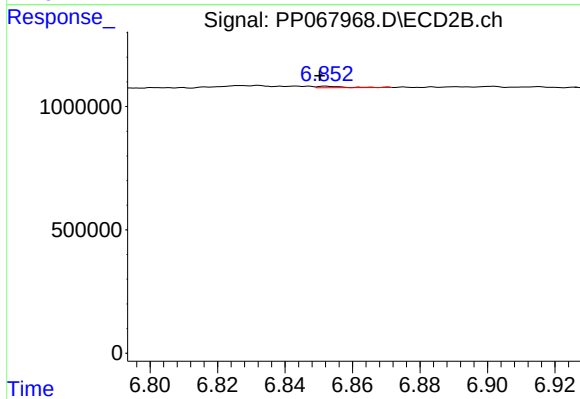

#32 AR-1260-2


R.T.: 6.852 min  
Delta R.T.: 0.002 min  
Response: 31076  
Conc: 0.47 ng/ml

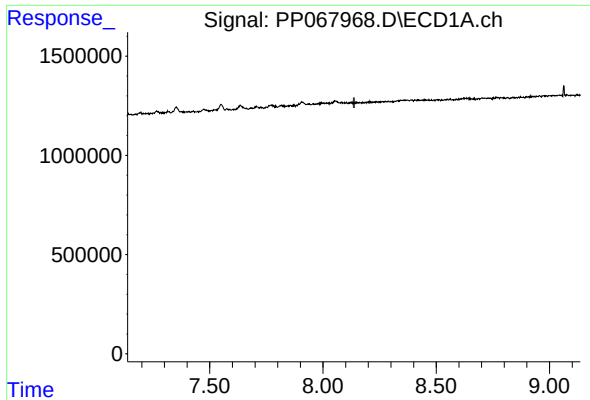

#33 AR-1260-3


R.T.: 0.000 min  
Exp R.T.: 8.137 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

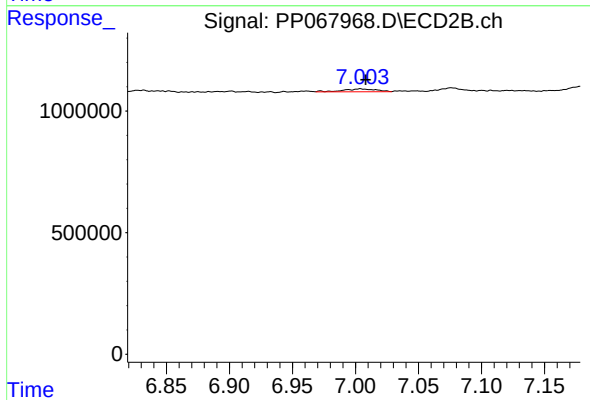


#33 AR-1260-3

R.T.: 7.004 min  
Delta R.T.: -0.005 min  
Response: 216269  
Conc: 3.40 ng/ml

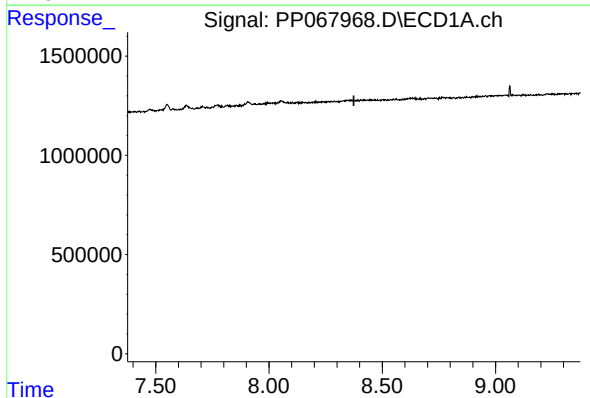


#34 AR-1260-4

R.T.: 0.000 min  
Exp R.T.: 8.375 min  
Response: 0  
Conc: N.D.

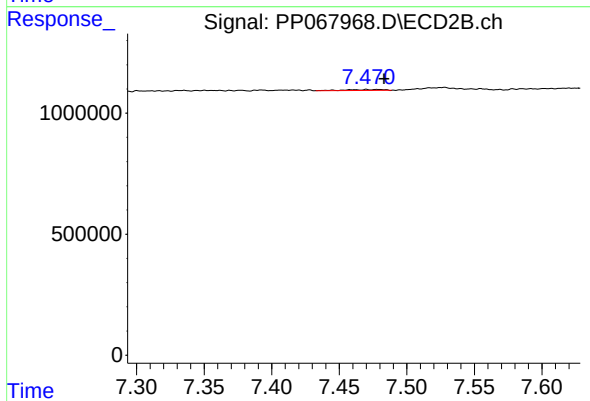

#34 AR-1260-4


R.T.: 7.470 min  
Delta R.T.: -0.013 min  
Response: 79362  
Conc: 1.44 ng/ml

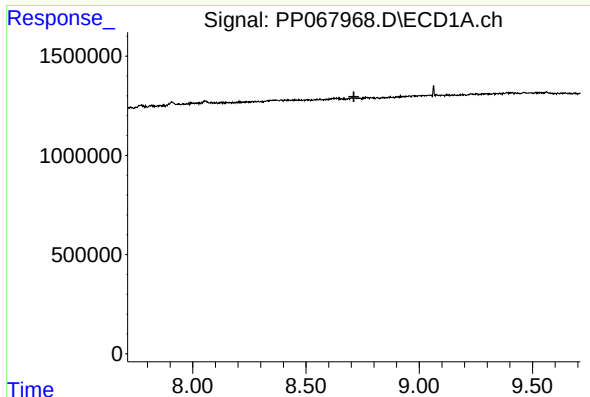

#35 AR-1260-5


R.T.: 0.000 min  
Exp R.T.: 8.712 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

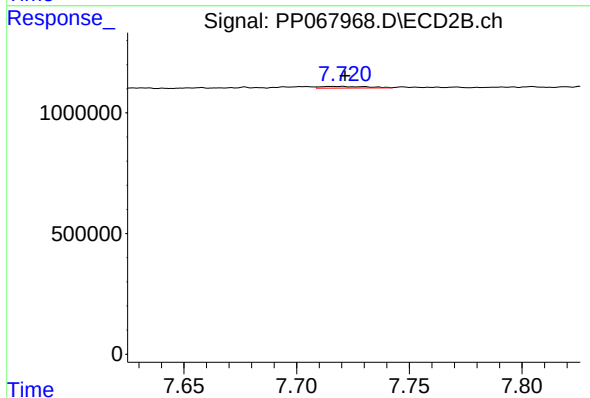


#35 AR-1260-5

R.T.: 7.720 min  
Delta R.T.: -0.002 min  
Response: 100188  
Conc: 0.82 ng/ml

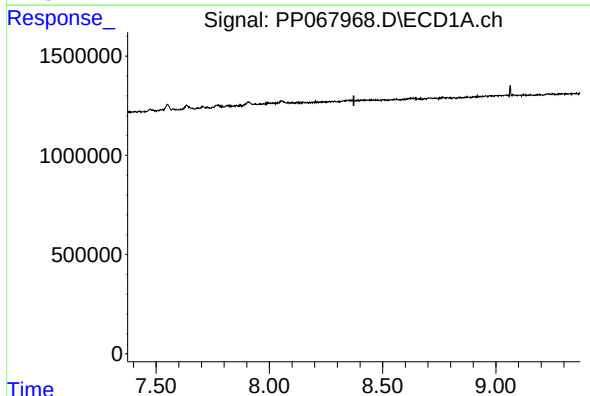


#36 AR-1262-1

R.T.: 0.000 min  
Exp R.T.: 8.373 min  
Response: 0  
Conc: N.D.

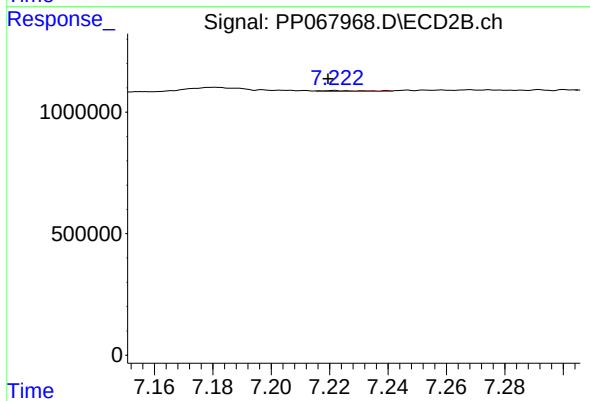

#36 AR-1262-1


R.T.: 7.222 min  
Delta R.T.: 0.002 min  
Response: 37112  
Conc: 0.47 ng/ml

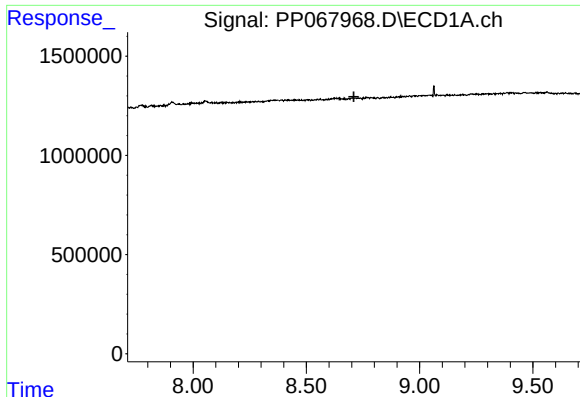

#37 AR-1262-2


R.T.: 0.000 min  
Exp R.T.: 8.709 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

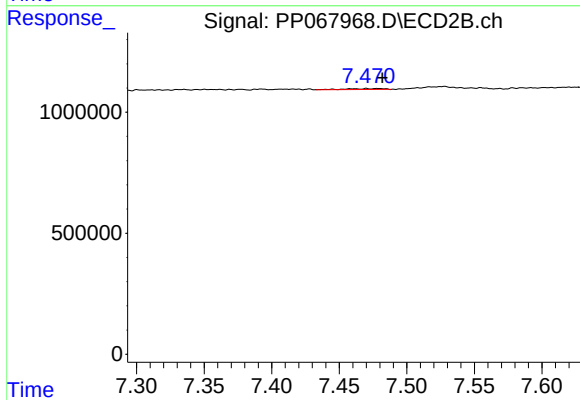


#37 AR-1262-2

R.T.: 7.470 min  
Delta R.T.: -0.012 min  
Response: 79362  
Conc: 1.12 ng/ml

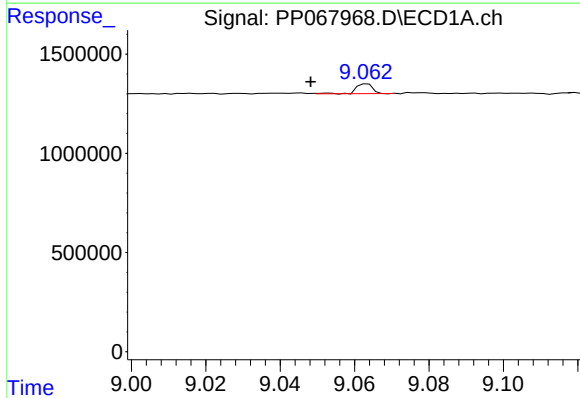


#38 AR-1262-3

R.T.: 9.063 min  
Delta R.T.: 0.015 min  
Response: 156045  
Conc: 1.76 ng/ml

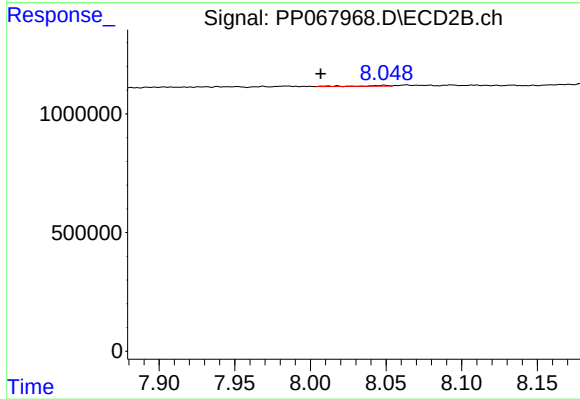

#38 AR-1262-3


R.T.: 8.049 min  
Delta R.T.: 0.042 min  
Response: 44502  
Conc: 0.78 ng/ml

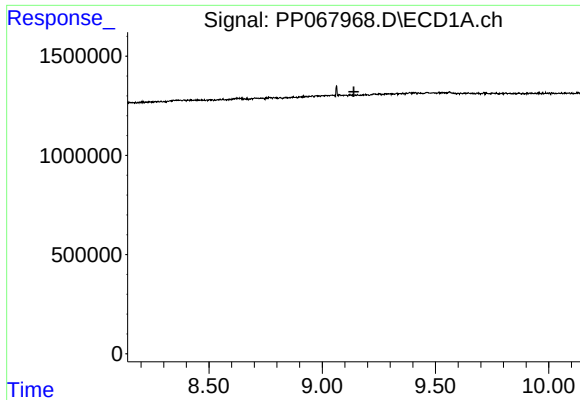

#39 AR-1262-4


R.T.: 0.000 min  
Exp R.T.: 9.140 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

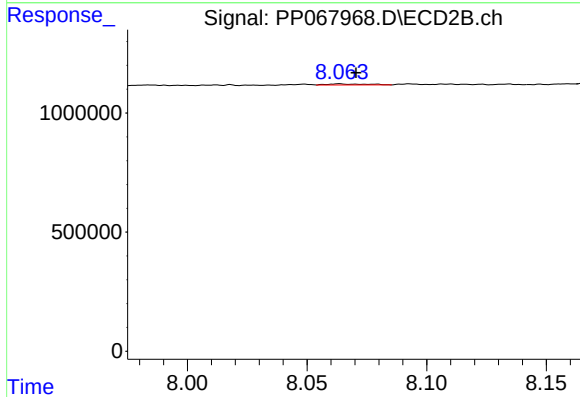


#39 AR-1262-4

R.T.: 8.063 min  
Delta R.T.: -0.007 min  
Response: 51402  
Conc: 0.51 ng/ml

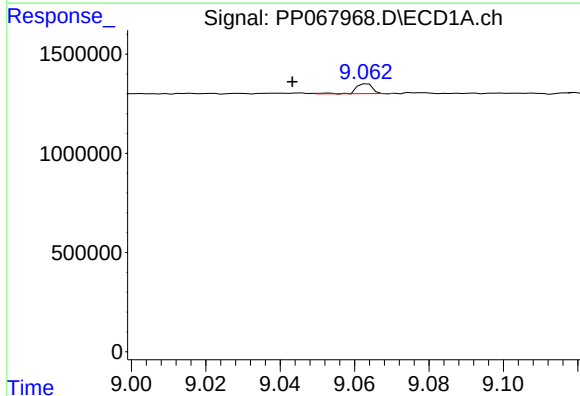


#41 AR-1268-1

R.T.: 9.063 min  
Delta R.T.: 0.020 min  
Response: 156045  
Conc: 1.02 ng/ml

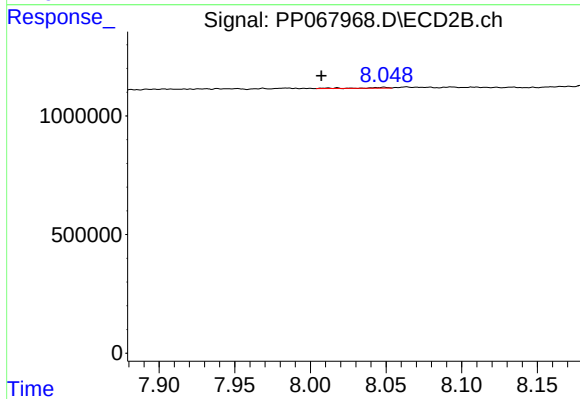

#41 AR-1268-1


R.T.: 8.049 min  
Delta R.T.: 0.041 min  
Response: 44502  
Conc: 0.28 ng/ml

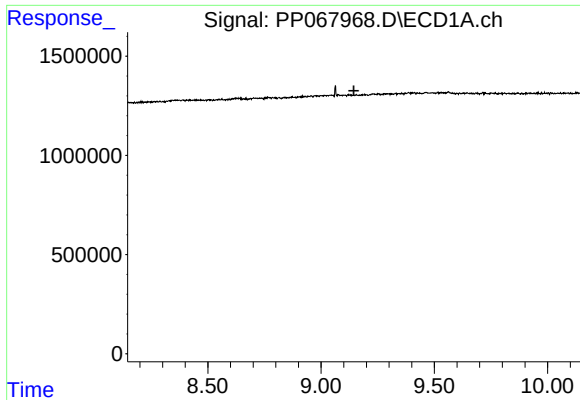

#42 AR-1268-2


R.T.: 0.000 min  
Exp R.T.: 9.144 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

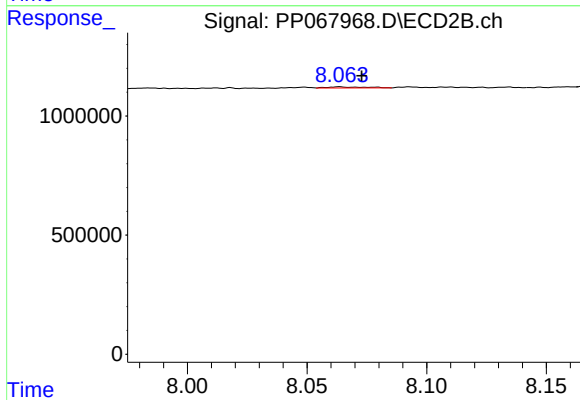


#42 AR-1268-2

R.T.: 8.063 min  
Delta R.T.: -0.009 min  
Response: 51402  
Conc: 0.36 ng/ml

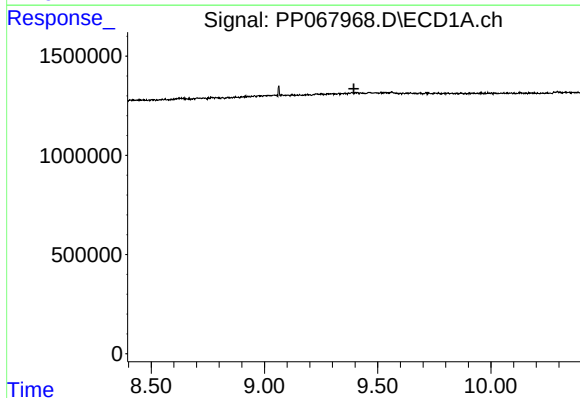

#43 AR-1268-3


R.T.: 0.000 min  
Exp R.T.: 9.395 min  
Response: 0  
Conc: N.D.

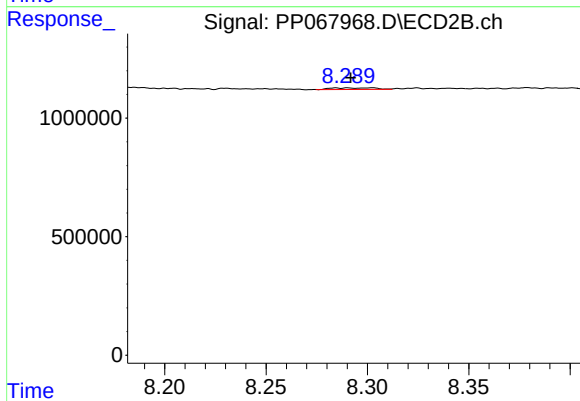

#43 AR-1268-3

R.T.: 8.302 min  
Delta R.T.: 0.010 min  
Response: 99021  
Conc: 0.78 ng/ml




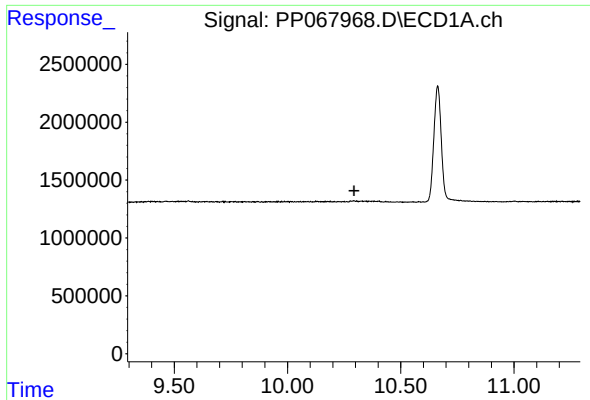

#45 AR-1268-5

R.T.: 0.000 min  
Exp R.T.: 10.294 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-WATER-03-QT4-2024

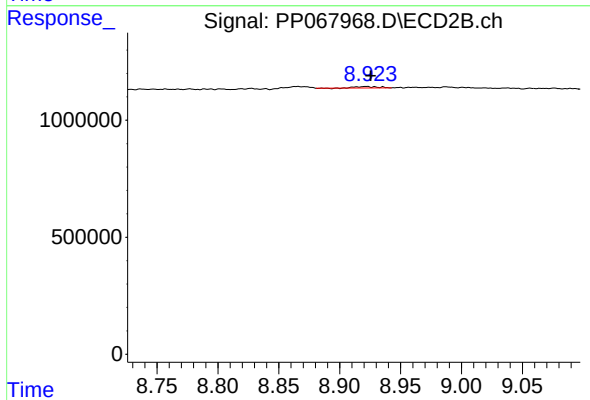

#45 AR-1268-5

R.T.: 8.922 min  
Delta R.T.: -0.004 min  
Response: 71670  
Conc: 0.19 ng/ml