

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
 Data File : PP067972.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2024 07:28
 Operator : YP\AJ
 Sample : P4368-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT4-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 08:31:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.753	4.049	15196741	15952539	16.418	15.788
2)	SA Decachlor...	10.661	9.210	23148520	21271154	20.106	18.967
Target Compounds							
3)	L1 AR-1016-1	0.000	5.199f	0	48124	N.D.	1.375 #
4)	L1 AR-1016-2	0.000	5.199	0	48124	N.D.	0.999 #
5)	L1 AR-1016-3	0.000	5.354	0	32453	N.D.	1.205 #
6)	L1 AR-1016-4	6.153f	5.354f	74289	32453	2.886	1.347 #
7)	L1 AR-1016-5	0.000	5.661f	0	597645	N.D.	19.653 #
9)	L2 AR-1221-2	5.059	4.359	258434	270757	27.317	27.181
10)	L2 AR-1221-3	5.059f	0.000	258434	0	8.940	N.D. #
11)	L3 AR-1232-1	5.059f	0.000	258434	0	11.305	N.D. #
12)	L3 AR-1232-2	0.000	5.199	0	48124	N.D.	2.152 #
13)	L3 AR-1232-3	0.000	5.354	0	32453	N.D.	2.717 #
14)	L3 AR-1232-4	6.153f	0.000	74289	0	6.582	N.D. #
15)	L3 AR-1232-5	6.180	5.661f	85251	597645	9.348	44.434 #
16)	L4 AR-1242-1	0.000	5.199f	0	48124	N.D.	1.655 #
17)	L4 AR-1242-2	0.000	5.199	0	48124	N.D.	1.199 #
18)	L4 AR-1242-3	0.000	5.354	0	32453	N.D.	1.443 #
19)	L4 AR-1242-4	6.153f	0.000	74289	0	3.463	N.D. #
20)	L4 AR-1242-5	0.000	5.968	0	63423	N.D.	2.214 #
21)	L5 AR-1248-1	0.000	5.199f	0	48124	N.D.	2.123 #
22)	L5 AR-1248-2	6.180	5.354f	85251	32453	2.536	0.981 #
24)	L5 AR-1248-4	0.000	5.661f	0	597645	N.D.	14.592 #
25)	L5 AR-1248-5	0.000	6.045	0	69105	N.D.	1.846 #
26)	L6 AR-1254-1	6.706f	5.968	494702	63423	11.047	1.073 #
27)	L6 AR-1254-2	0.000	6.081f	0	60965	N.D.	1.162 #
28)	L6 AR-1254-3	0.000	6.528	0	150013	N.D.	1.803 #
29)	L6 AR-1254-4	0.000	6.708f	0	73636	N.D.	1.525 #
30)	L6 AR-1254-5	0.000	7.216	0	803568	N.D.	10.925 #
31)	L7 AR-1260-1	7.550	6.655	356134	67283	6.592	1.181 #
32)	L7 AR-1260-2	7.767	6.826	38156	183944	0.603	2.758 #
33)	L7 AR-1260-3	8.132	7.007	707844	168181	13.652	2.640 #
34)	L7 AR-1260-4	8.394	7.477	990437	1046776	16.454	18.932
35)	L7 AR-1260-5	8.708	7.716	361385	503642	3.355	4.118
36)	L8 AR-1262-1	8.394	7.216	990437	803568	13.800	10.214 #
37)	L8 AR-1262-2	8.708	7.477	361385	1046776	2.972	14.751 #
38)	L8 AR-1262-3	9.042	8.002	3638154	3728138	41.102	65.292 #
39)	L8 AR-1262-4	9.141	8.067	3059698	3260422	43.744	32.463 #
40)	L8 AR-1262-5	9.839	8.593	1113806	1249947	23.804	24.990
41)	L9 AR-1268-1	9.042	8.002	3638154	3728138	23.834	23.427
42)	L9 AR-1268-2	9.141	8.067	3059698	3260422	22.400	22.771
43)	L9 AR-1268-3	9.392	8.287	3075797	2905069	25.437	22.783

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
Data File : PP067972.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 07:28
Operator : YP\AJ
Sample : P4368-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 74 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 08:31:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44)	L9 AR-1268-4	9.839	8.593	1113806	1249947	21.917	22.132
45)	L9 AR-1268-5	10.290	8.920	9219060	9037360	24.685	23.906



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
Data File : PP067972.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 07:28
Operator : YP\AJ
Sample : P4368-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 74 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 08:31:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

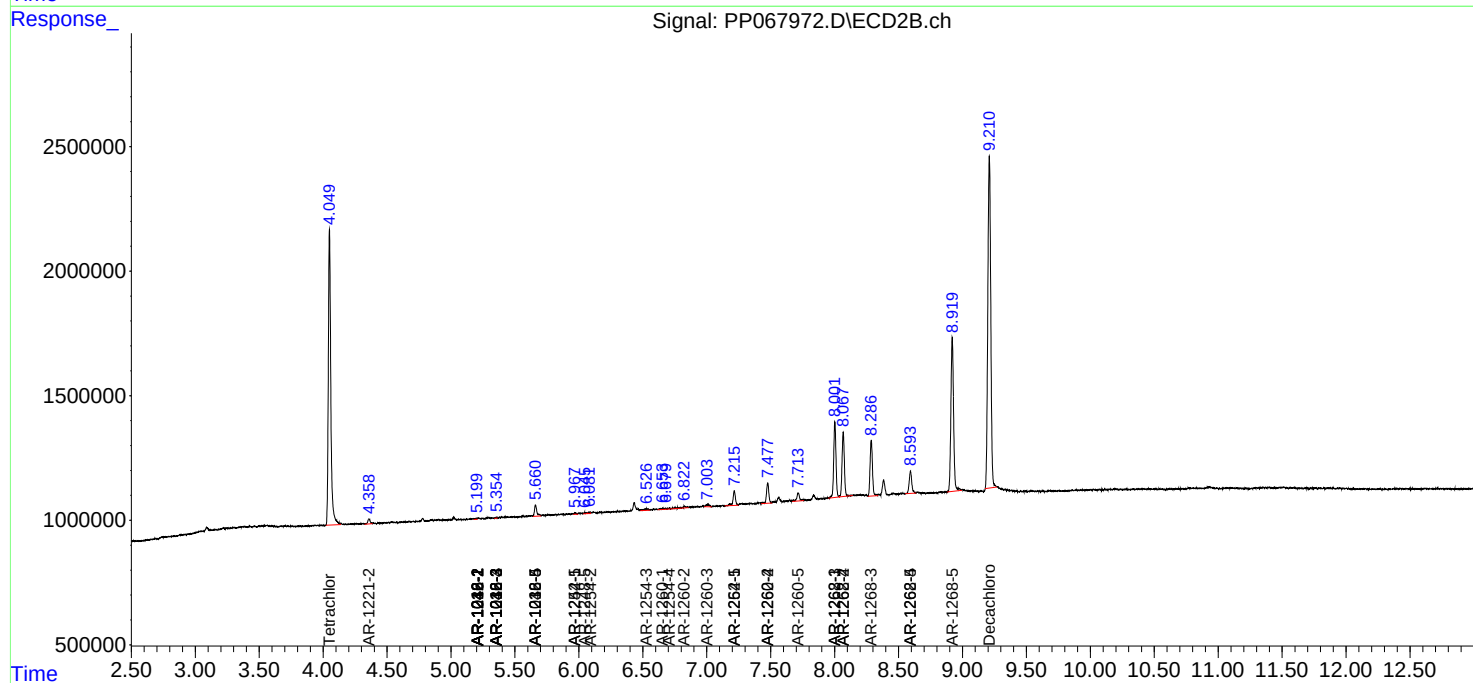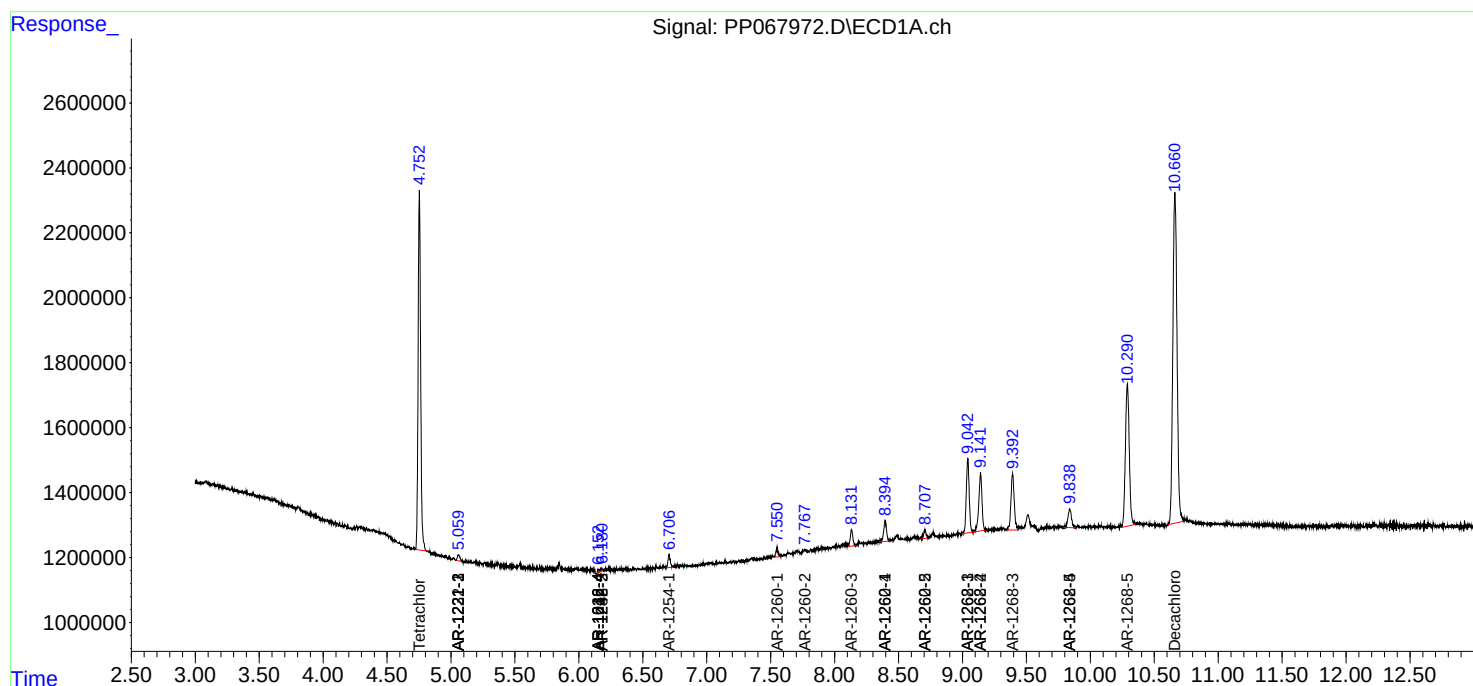


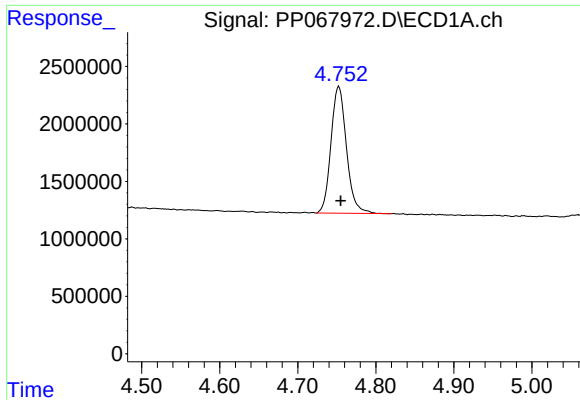

#1 Tetrachloro-m-xylene


R.T.: 4.753 min
Delta R.T.: -0.002 min
Response: 15196741
Conc: 16.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

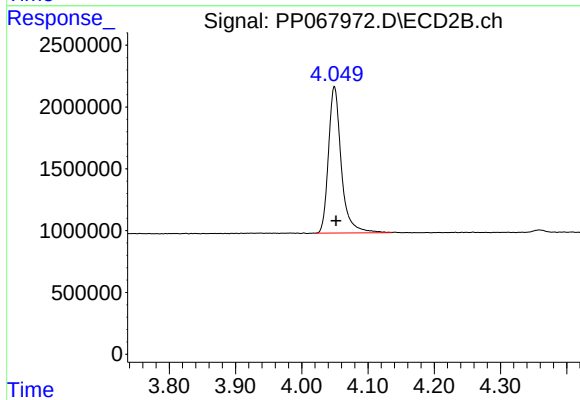


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: -0.003 min
Response: 15952539
Conc: 15.79 ng/ml

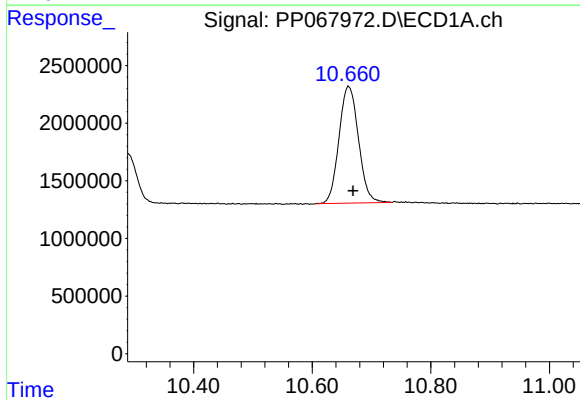


#2 Decachlorobiphenyl

R.T.: 10.661 min
Delta R.T.: -0.008 min
Response: 23148520
Conc: 20.11 ng/ml

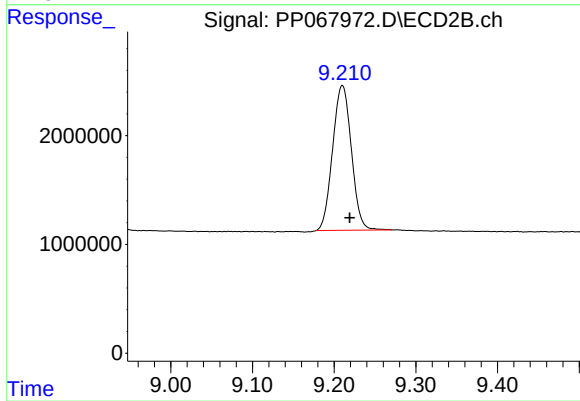

#2 Decachlorobiphenyl


R.T.: 9.210 min
Delta R.T.: -0.009 min
Response: 21271154
Conc: 18.97 ng/ml

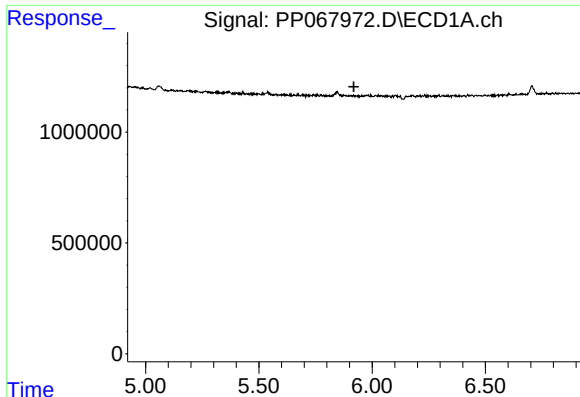

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.919 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

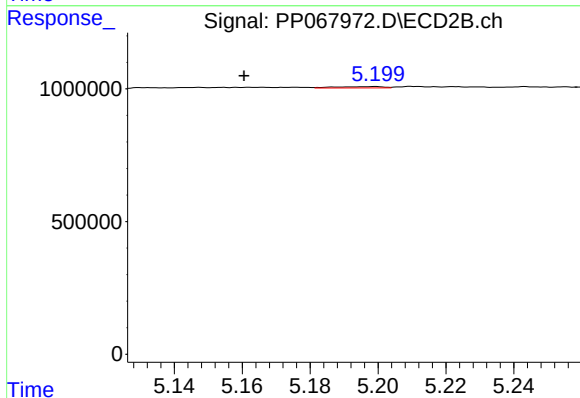


#3 AR-1016-1

R.T.: 5.199 min
Delta R.T.: 0.038 min
Response: 48124
Conc: 1.38 ng/ml

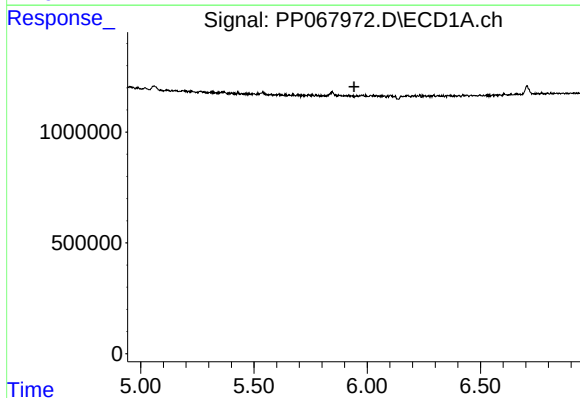


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.942 min
Response: 0
Conc: N.D.

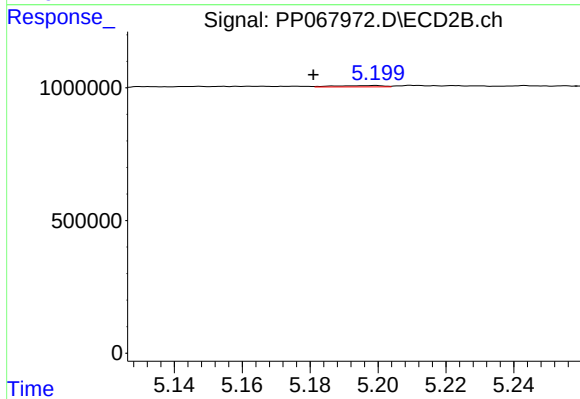

#4 AR-1016-2


R.T.: 5.199 min
Delta R.T.: 0.018 min
Response: 48124
Conc: 1.00 ng/ml

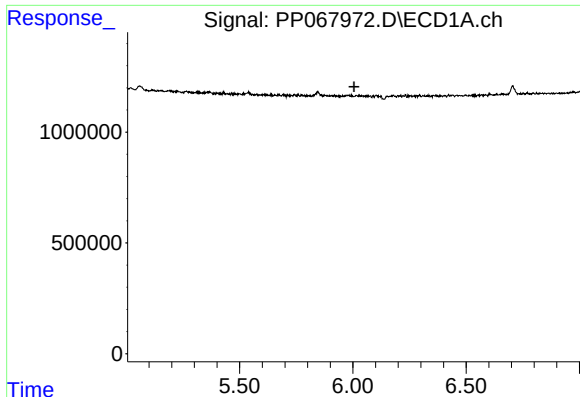

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 6.005 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

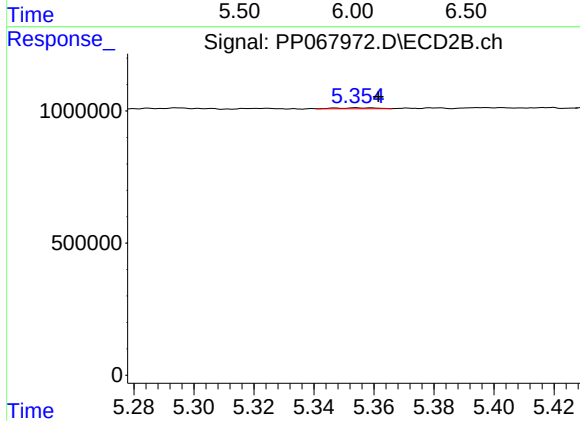


#5 AR-1016-3

R.T.: 5.354 min
Delta R.T.: -0.007 min
Response: 32453
Conc: 1.20 ng/ml

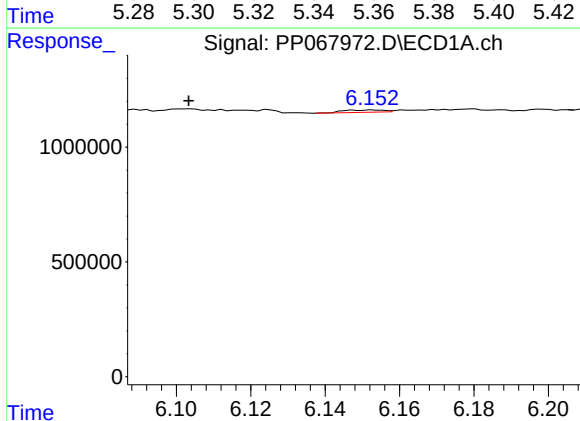


#6 AR-1016-4

R.T.: 6.153 min
Delta R.T.: 0.050 min
Response: 74289
Conc: 2.89 ng/ml

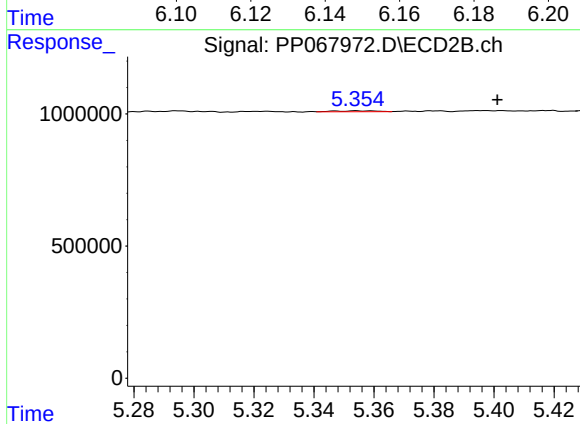

#6 AR-1016-4


R.T.: 5.354 min
Delta R.T.: -0.047 min
Response: 32453
Conc: 1.35 ng/ml

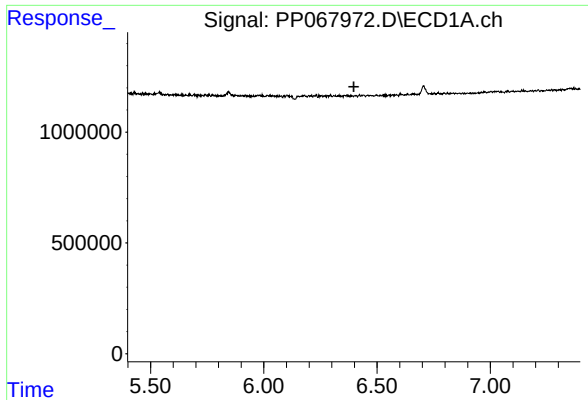

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

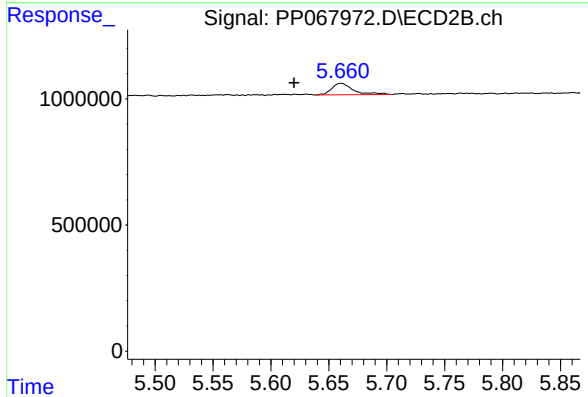


#7 AR-1016-5

R.T.: 5.661 min
Delta R.T.: 0.040 min
Response: 597645
Conc: 19.65 ng/ml

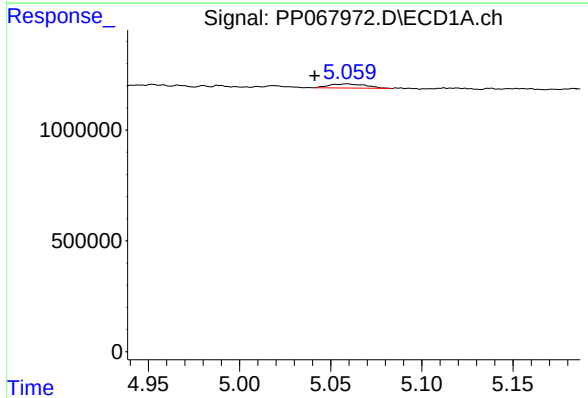


#9 AR-1221-2

R.T.: 5.059 min
Delta R.T.: 0.018 min
Response: 258434
Conc: 27.32 ng/ml

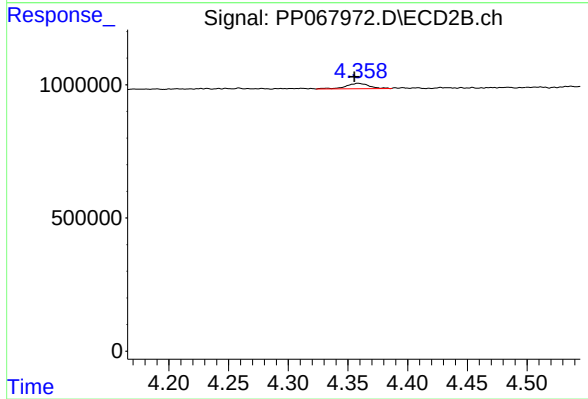

#9 AR-1221-2


R.T.: 4.359 min
Delta R.T.: 0.003 min
Response: 270757
Conc: 27.18 ng/ml

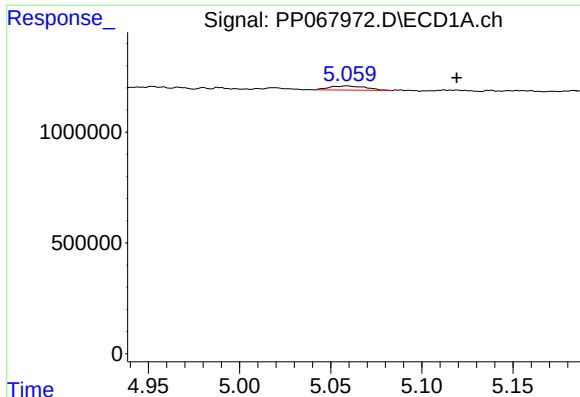

#10 AR-1221-3


R.T.: 5.059 min
Delta R.T.: -0.060 min
Response: 258434
Conc: 8.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

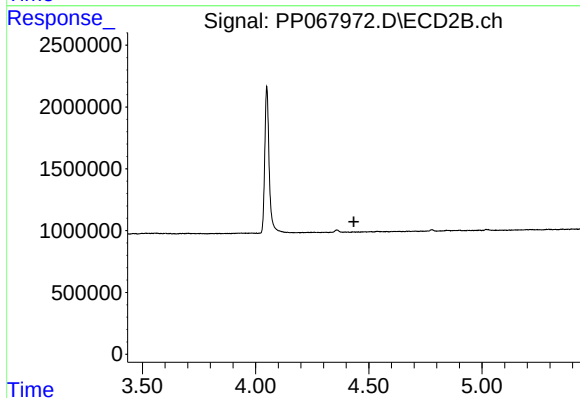


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.434 min
Response: 0
Conc: N.D.

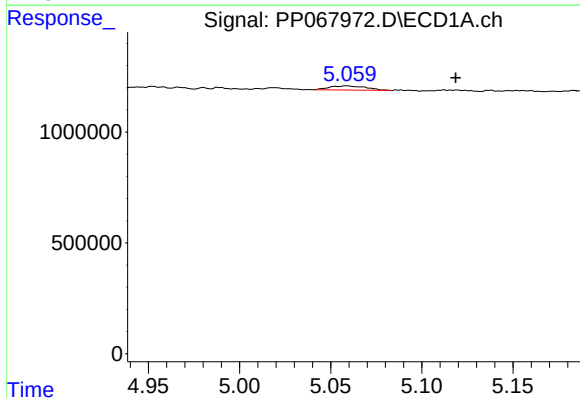


#11 AR-1232-1

R.T.: 5.059 min
Delta R.T.: -0.059 min
Response: 258434
Conc: 11.31 ng/ml

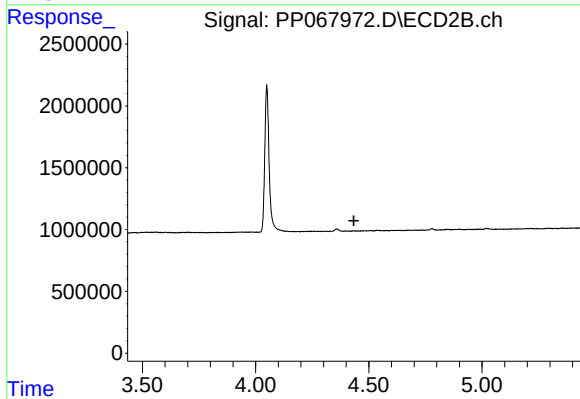

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.434 min
Response: 0
Conc: N.D.

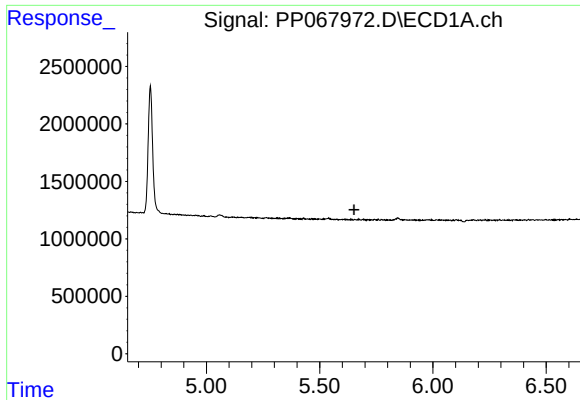

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 5.651 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

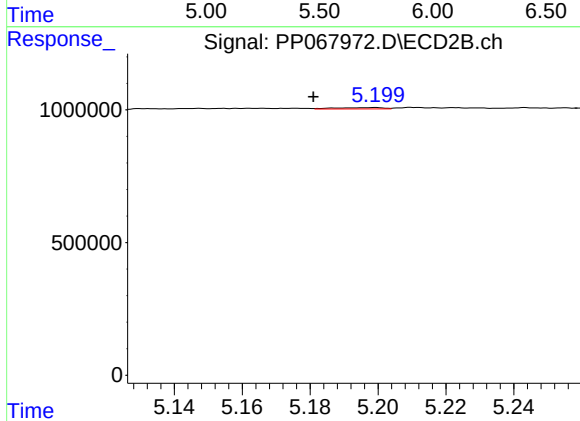


#12 AR-1232-2

R.T.: 5.199 min
Delta R.T.: 0.018 min
Response: 48124
Conc: 2.15 ng/ml

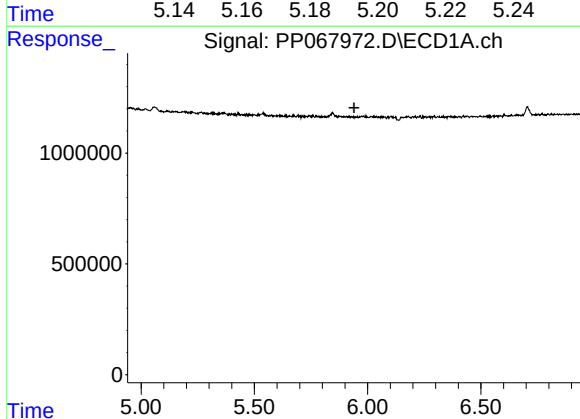


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T.: 5.940 min
Response: 0
Conc: N.D.

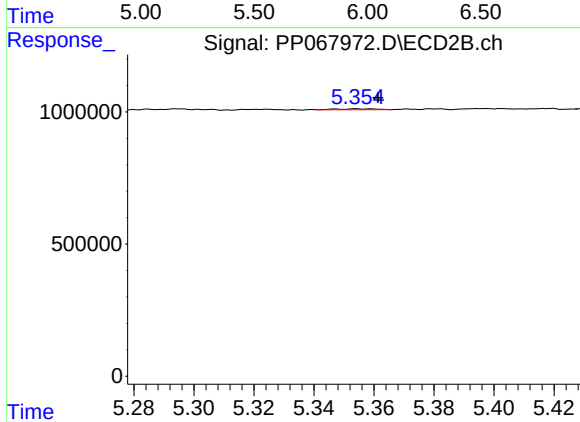

#13 AR-1232-3


R.T.: 5.354 min
Delta R.T.: -0.007 min
Response: 32453
Conc: 2.72 ng/ml

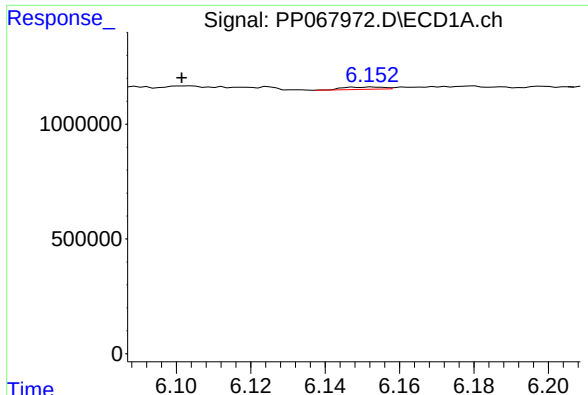

#14 AR-1232-4


R.T.: 6.153 min
Delta R.T.: 0.051 min
Response: 74289
Conc: 6.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

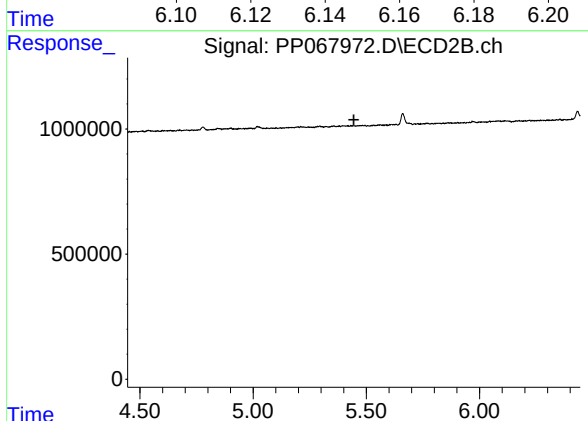


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.445 min
Response: 0
Conc: N.D.

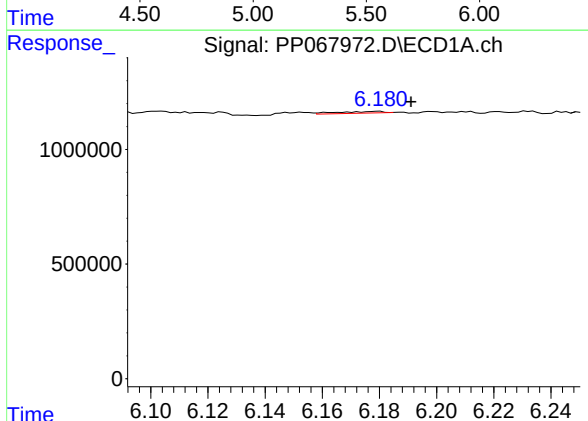


#15 AR-1232-5

R.T.: 6.180 min
Delta R.T.: -0.011 min
Response: 85251
Conc: 9.35 ng/ml

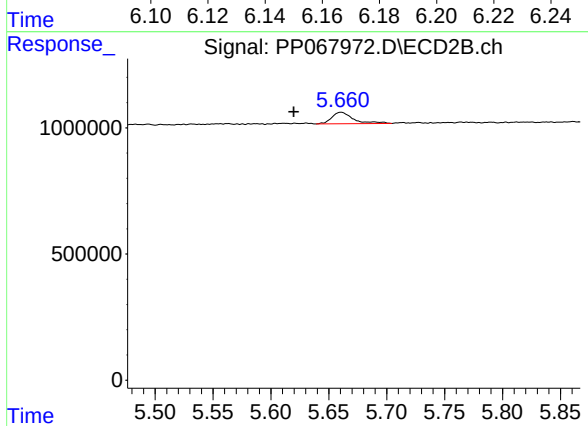

#15 AR-1232-5


R.T.: 5.661 min
Delta R.T.: 0.041 min
Response: 597645
Conc: 44.43 ng/ml

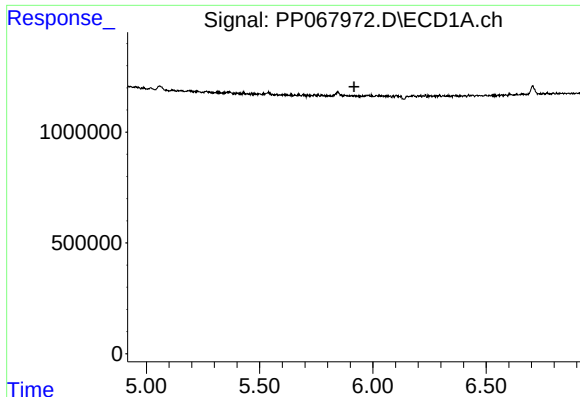

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T.: 5.916 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

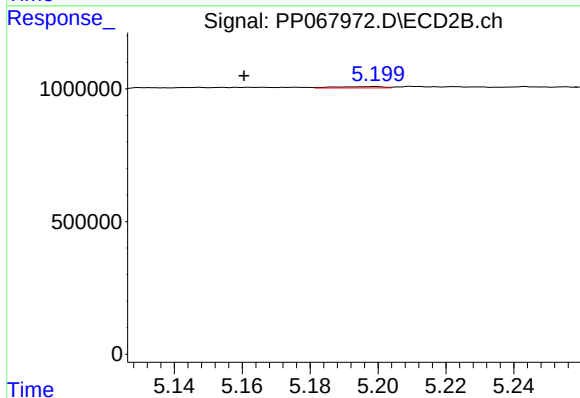


#16 AR-1242-1

R.T.: 5.199 min
Delta R.T.: 0.038 min
Response: 48124
Conc: 1.66 ng/ml

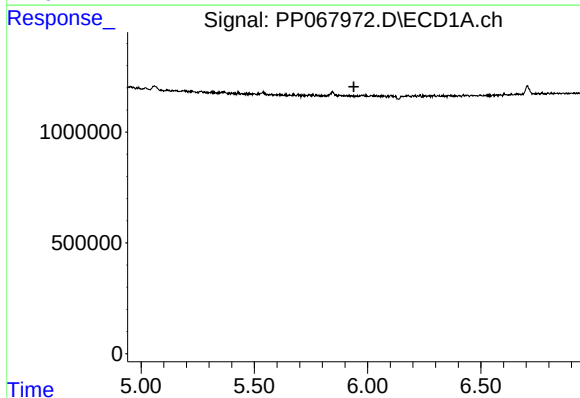


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T.: 5.939 min
Response: 0
Conc: N.D.

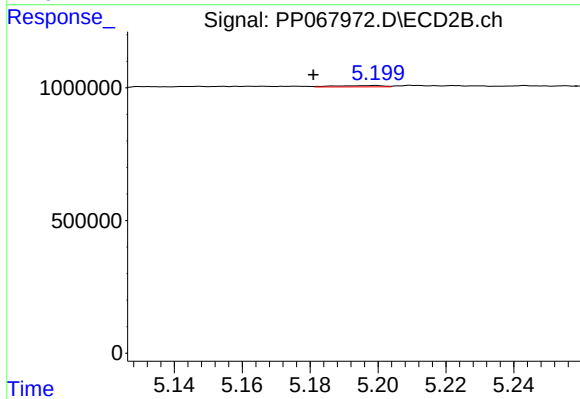

#17 AR-1242-2


R.T.: 5.199 min
Delta R.T.: 0.018 min
Response: 48124
Conc: 1.20 ng/ml

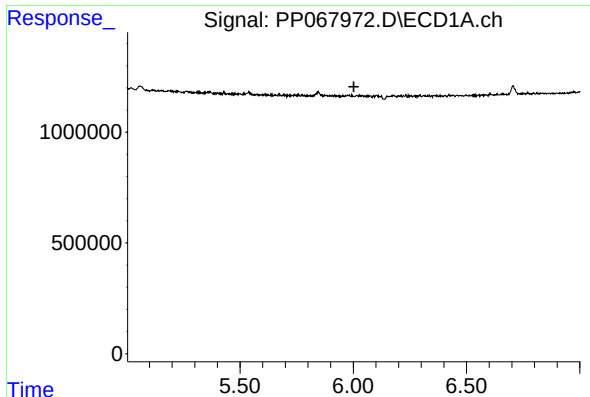

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 6.002 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

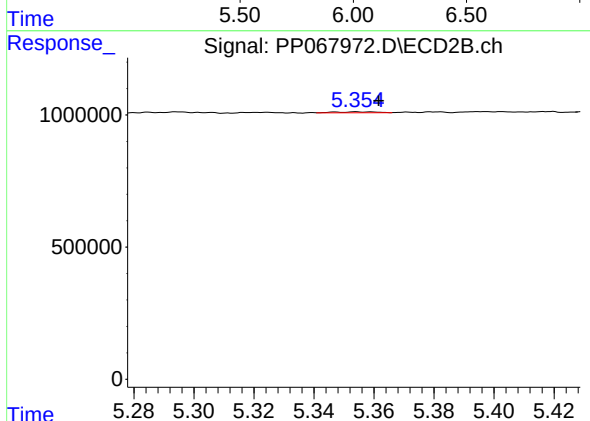


#18 AR-1242-3

R.T.: 5.354 min
Delta R.T.: -0.007 min
Response: 32453
Conc: 1.44 ng/ml

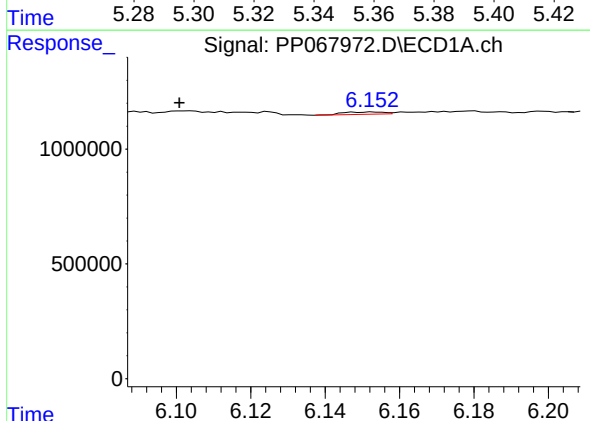


#19 AR-1242-4

R.T.: 6.153 min
Delta R.T.: 0.052 min
Response: 74289
Conc: 3.46 ng/ml

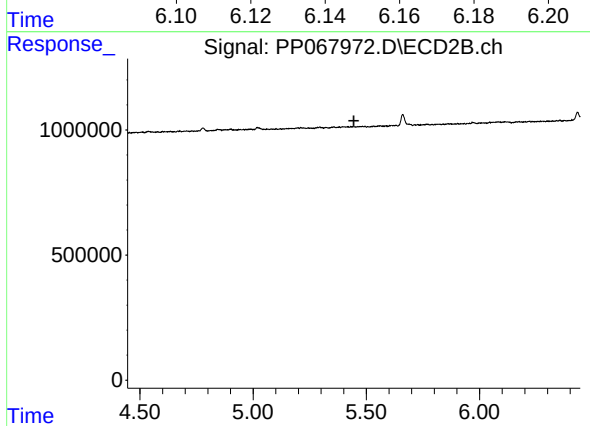

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.445 min
Response: 0
Conc: N.D.

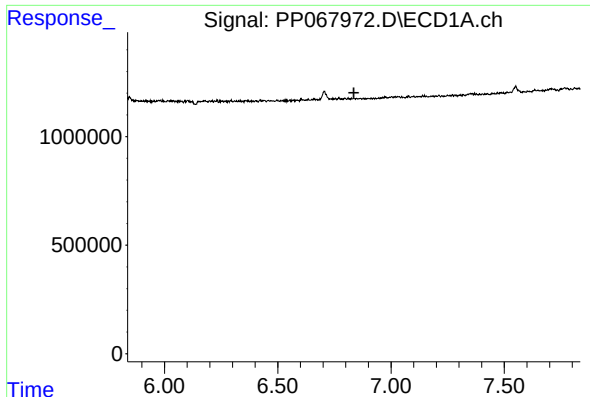

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.835 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

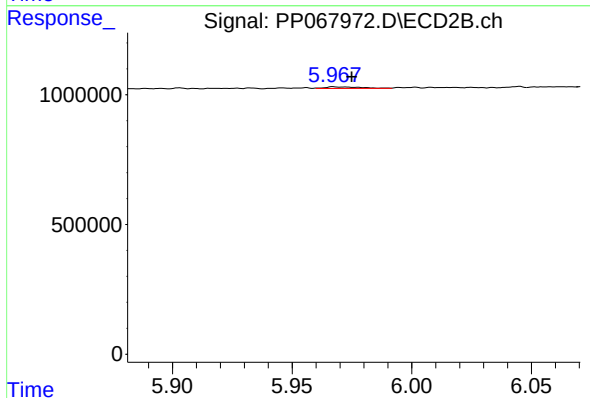


#20 AR-1242-5

R.T.: 5.968 min
Delta R.T.: -0.007 min
Response: 63423
Conc: 2.21 ng/ml

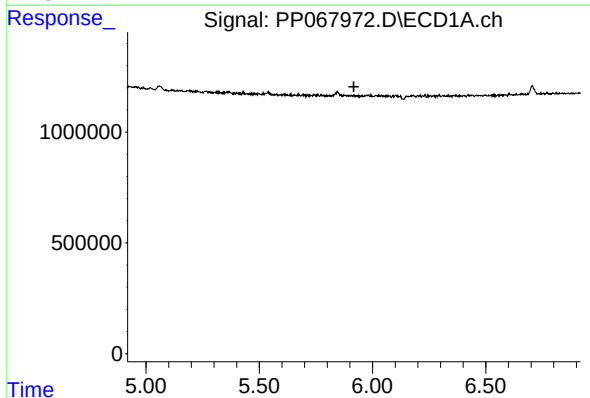


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T.: 5.917 min
Response: 0
Conc: N.D.

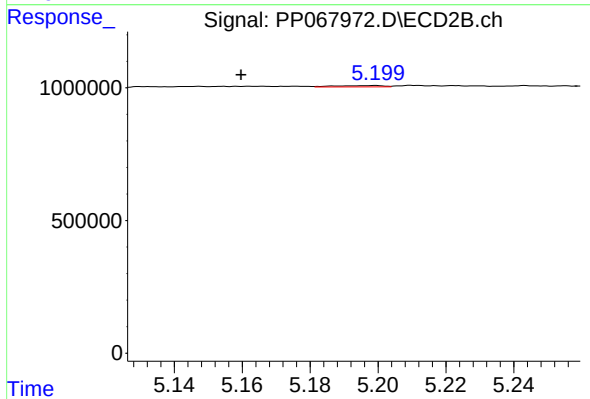

#21 AR-1248-1


R.T.: 5.199 min
Delta R.T.: 0.039 min
Response: 48124
Conc: 2.12 ng/ml

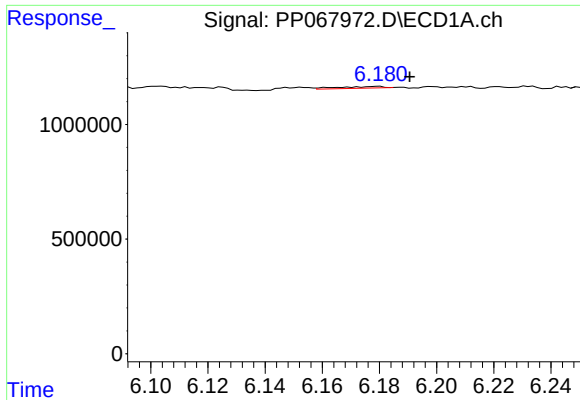

#22 AR-1248-2


R.T.: 6.180 min
Delta R.T.: -0.011 min
Response: 85251
Conc: 2.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

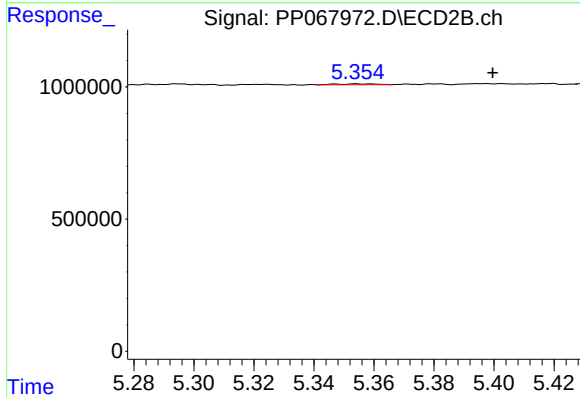


#22 AR-1248-2

R.T.: 5.354 min
Delta R.T.: -0.046 min
Response: 32453
Conc: 0.98 ng/ml

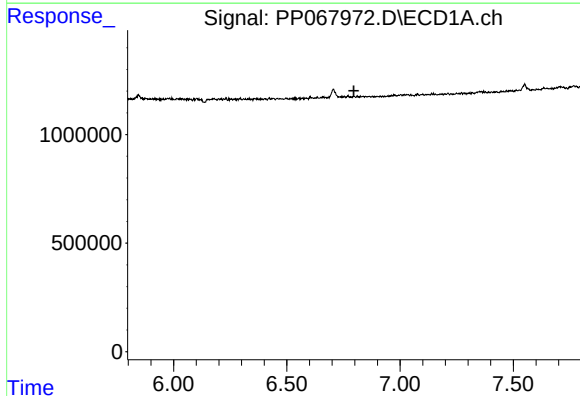


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 6.796 min
Response: 0
Conc: N.D.

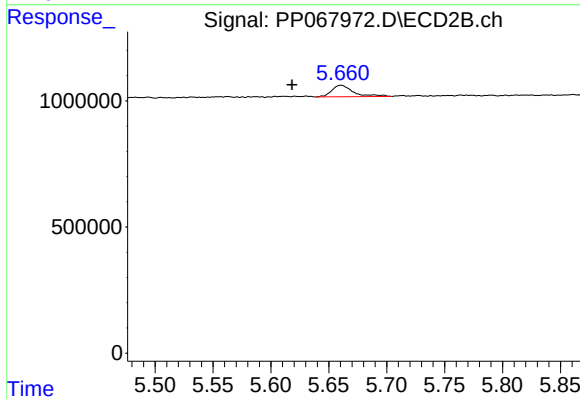

#24 AR-1248-4


R.T.: 5.661 min
Delta R.T.: 0.042 min
Response: 597645
Conc: 14.59 ng/ml

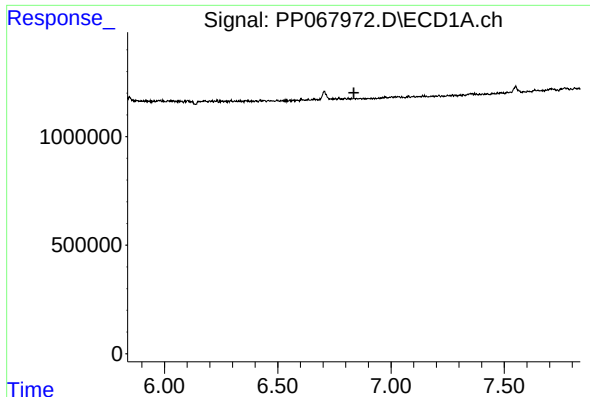

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.836 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

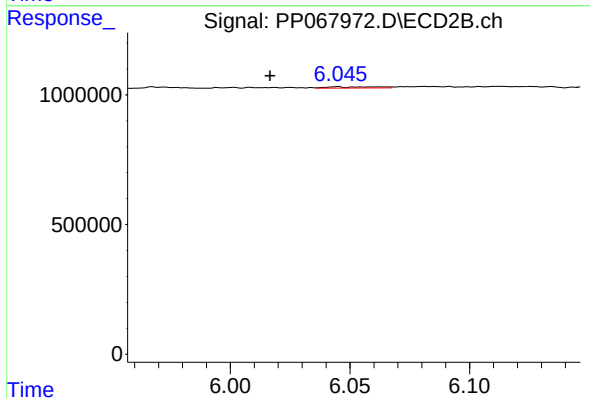


#25 AR-1248-5

R.T.: 6.045 min
Delta R.T.: 0.028 min
Response: 69105
Conc: 1.85 ng/ml

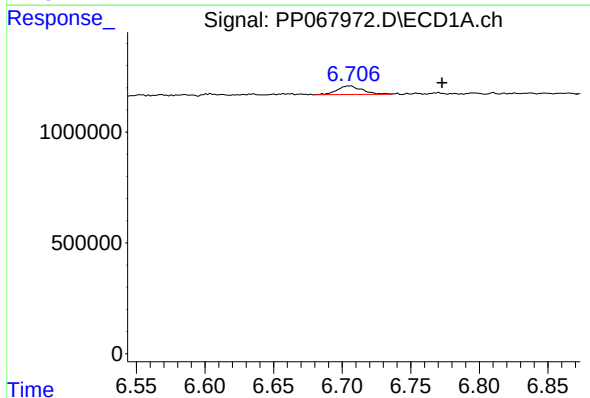


#26 AR-1254-1

R.T.: 6.706 min
Delta R.T.: -0.067 min
Response: 494702
Conc: 11.05 ng/ml

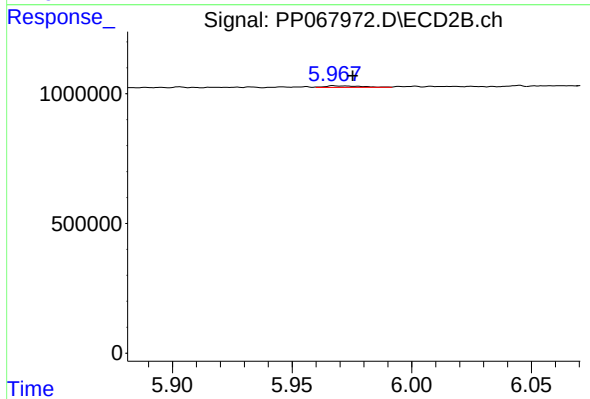

#26 AR-1254-1


R.T.: 5.968 min
Delta R.T.: -0.008 min
Response: 63423
Conc: 1.07 ng/ml

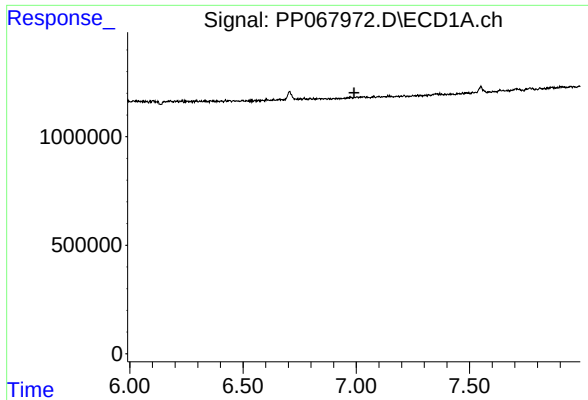

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.990 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

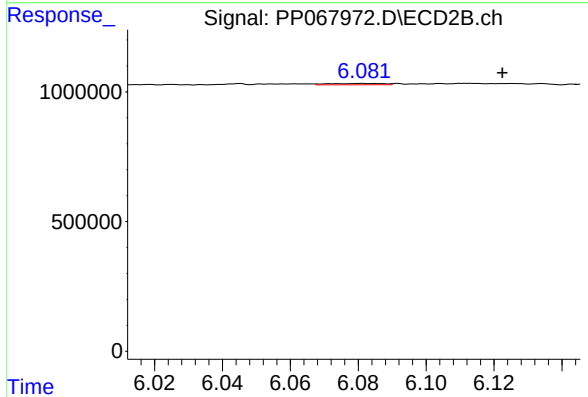


#27 AR-1254-2

R.T.: 6.081 min
Delta R.T.: -0.041 min
Response: 60965
Conc: 1.16 ng/ml

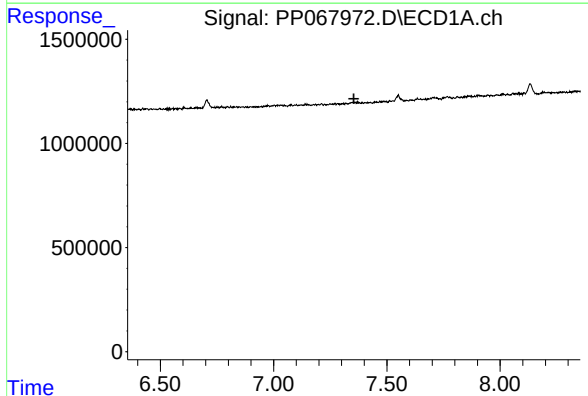


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 7.354 min
Response: 0
Conc: N.D.

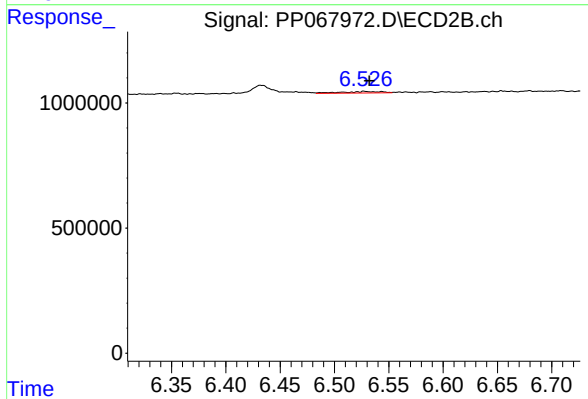

#28 AR-1254-3


R.T.: 6.528 min
Delta R.T.: -0.005 min
Response: 150013
Conc: 1.80 ng/ml

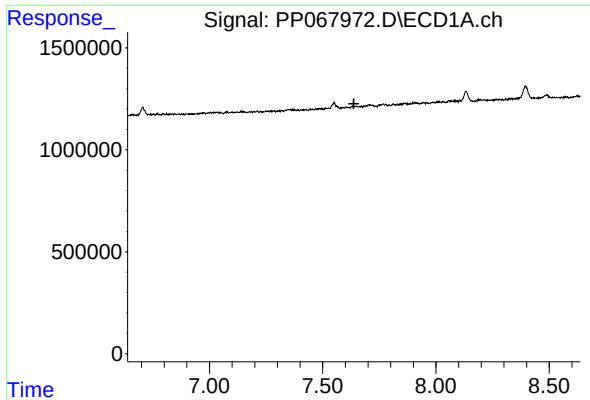

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.637 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

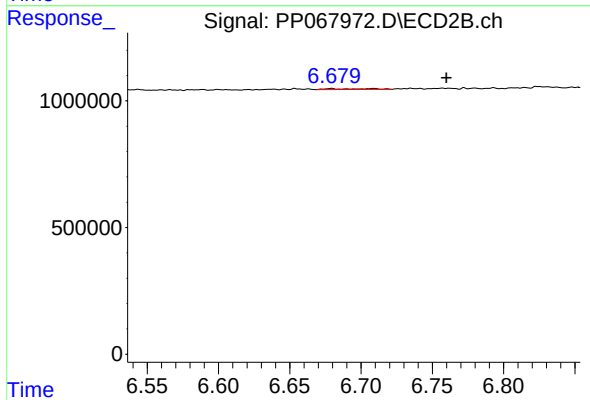


#29 AR-1254-4

R.T.: 6.708 min
Delta R.T.: -0.052 min
Response: 73636
Conc: 1.53 ng/ml

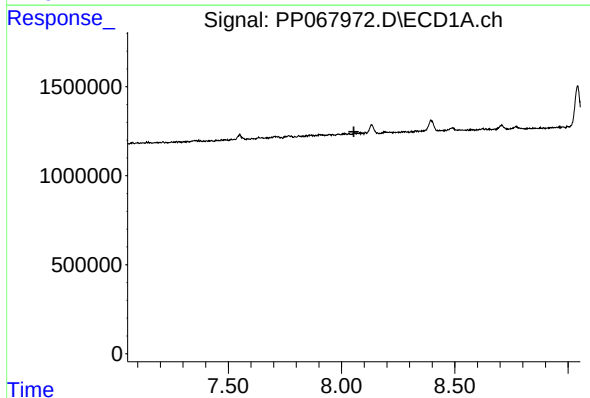


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 8.055 min
Response: 0
Conc: N.D.

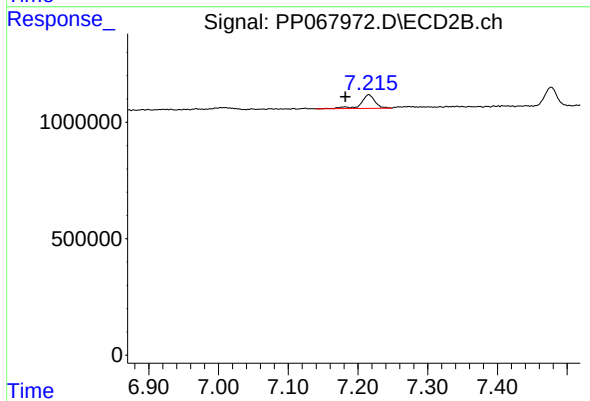

#30 AR-1254-5


R.T.: 7.216 min
Delta R.T.: 0.034 min
Response: 803568
Conc: 10.93 ng/ml

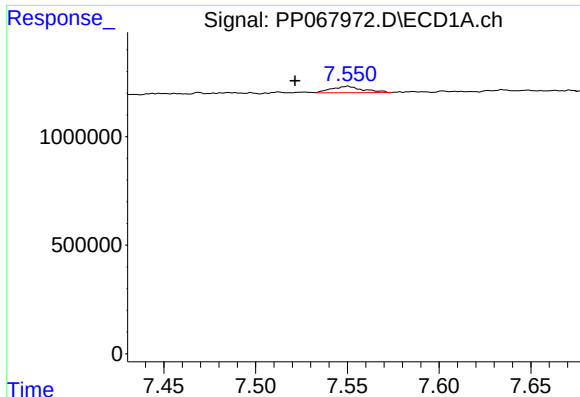

#31 AR-1260-1


R.T.: 7.550 min
Delta R.T.: 0.029 min
Response: 356134
Conc: 6.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

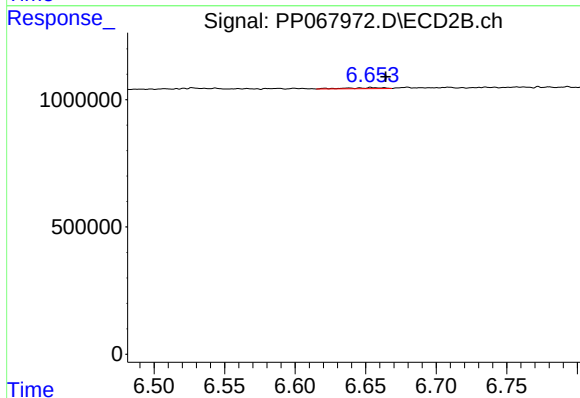


#31 AR-1260-1

R.T.: 6.655 min
Delta R.T.: -0.009 min
Response: 67283
Conc: 1.18 ng/ml

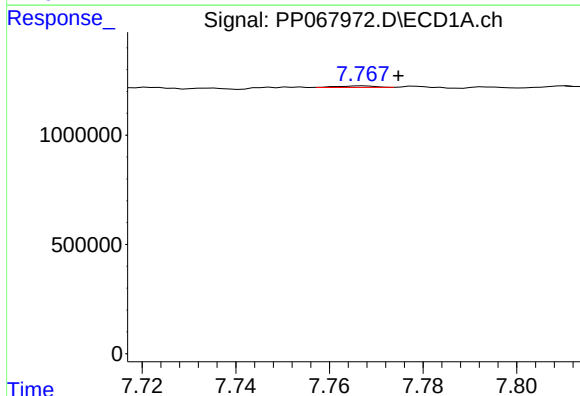


#32 AR-1260-2

R.T.: 7.767 min
Delta R.T.: -0.008 min
Response: 38156
Conc: 0.60 ng/ml

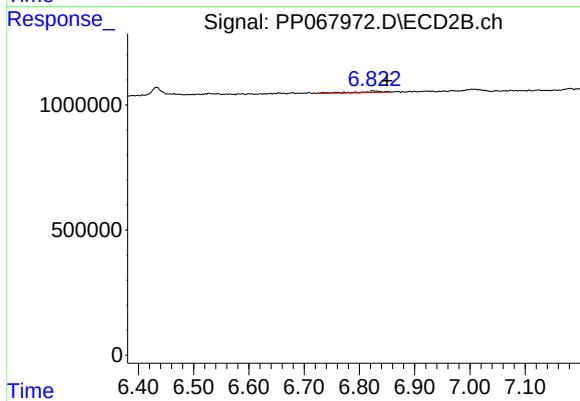

#32 AR-1260-2


R.T.: 6.826 min
Delta R.T.: -0.024 min
Response: 183944
Conc: 2.76 ng/ml

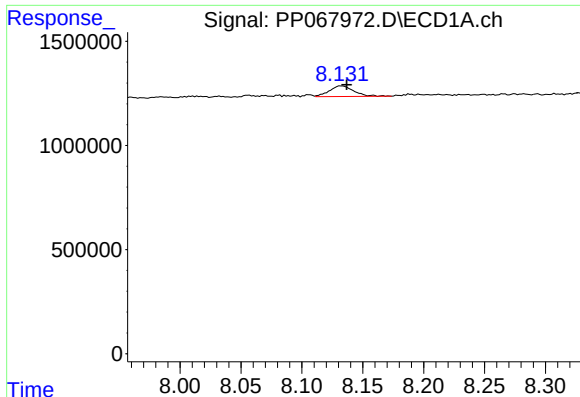

#33 AR-1260-3


R.T.: 8.132 min
Delta R.T.: -0.005 min
Response: 707844
Conc: 13.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

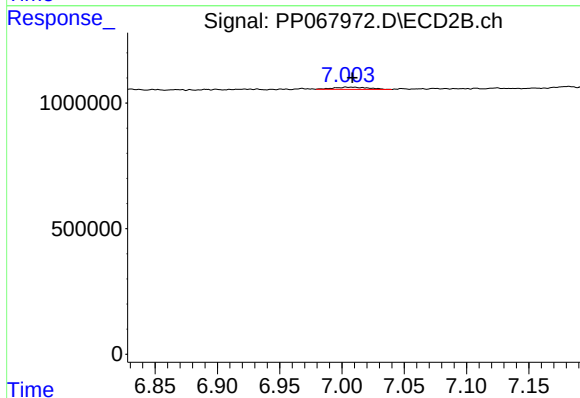


#33 AR-1260-3

R.T.: 7.007 min
Delta R.T.: -0.002 min
Response: 168181
Conc: 2.64 ng/ml

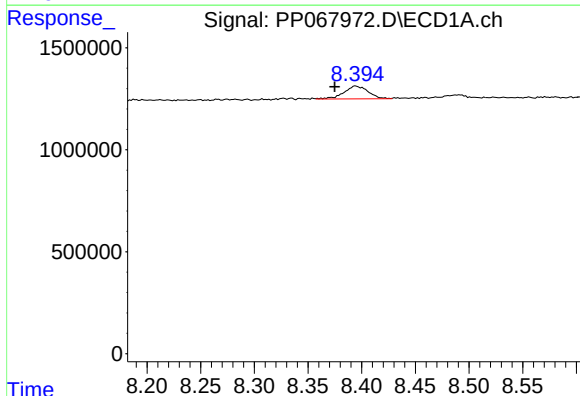


#34 AR-1260-4

R.T.: 8.394 min
Delta R.T.: 0.019 min
Response: 990437
Conc: 16.45 ng/ml

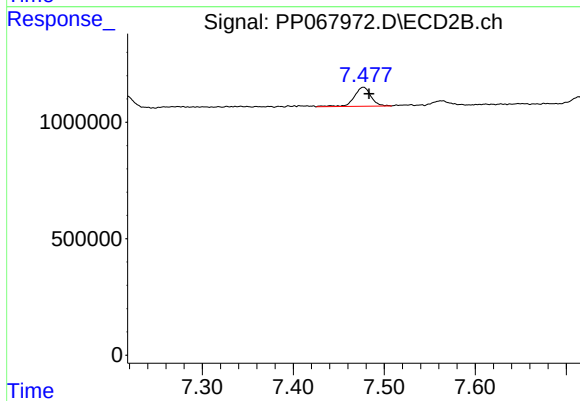

#34 AR-1260-4


R.T.: 7.477 min
Delta R.T.: -0.006 min
Response: 1046776
Conc: 18.93 ng/ml

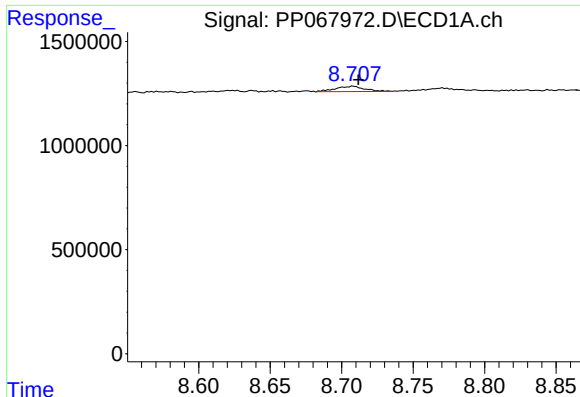

#35 AR-1260-5


R.T.: 8.708 min
Delta R.T.: -0.003 min
Response: 361385
Conc: 3.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

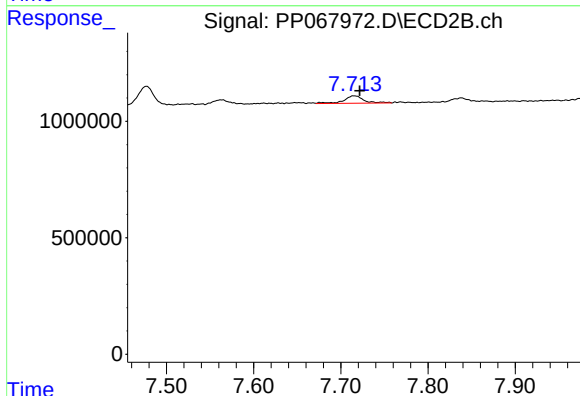


#35 AR-1260-5

R.T.: 7.716 min
Delta R.T.: -0.006 min
Response: 503642
Conc: 4.12 ng/ml

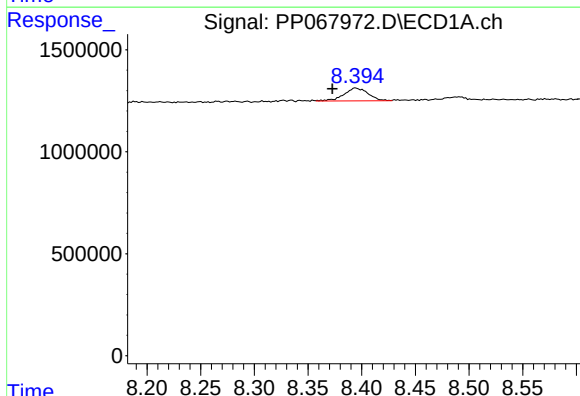


#36 AR-1262-1

R.T.: 8.394 min
Delta R.T.: 0.022 min
Response: 990437
Conc: 13.80 ng/ml

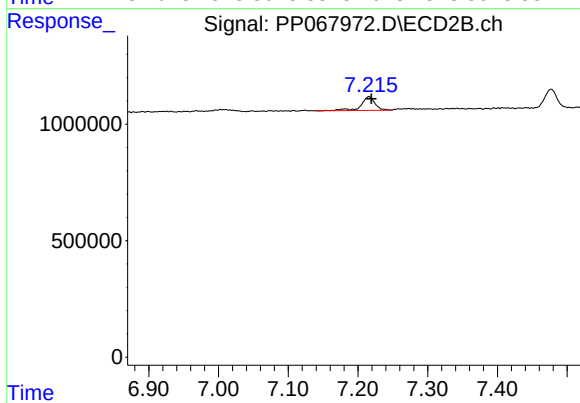

#36 AR-1262-1


R.T.: 7.216 min
Delta R.T.: -0.004 min
Response: 803568
Conc: 10.21 ng/ml

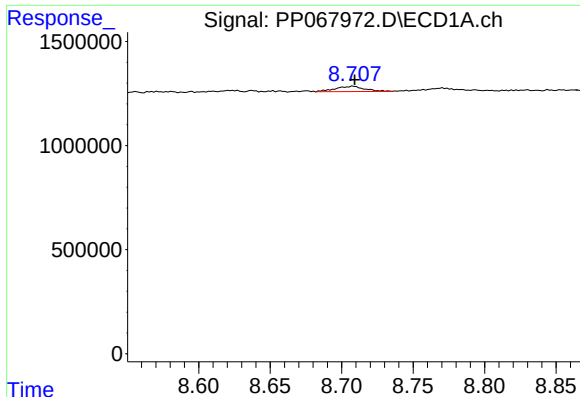

#37 AR-1262-2


R.T.: 8.708 min
Delta R.T.: 0.000 min
Response: 361385
Conc: 2.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

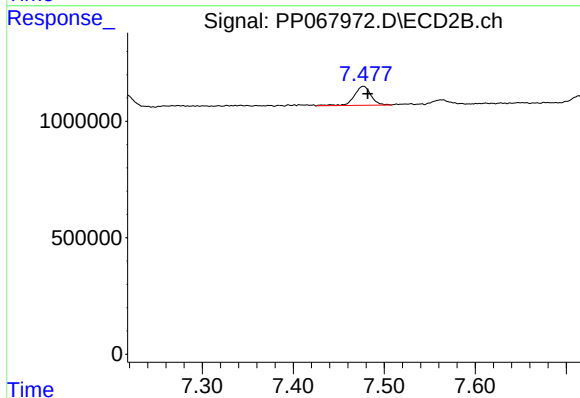


#37 AR-1262-2

R.T.: 7.477 min
Delta R.T.: -0.005 min
Response: 1046776
Conc: 14.75 ng/ml

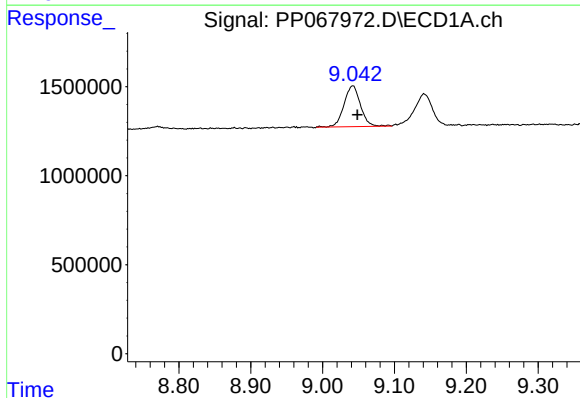


#38 AR-1262-3

R.T.: 9.042 min
Delta R.T.: -0.006 min
Response: 3638154
Conc: 41.10 ng/ml

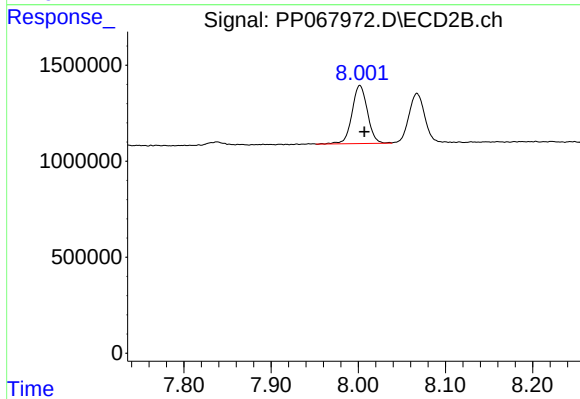

#38 AR-1262-3


R.T.: 8.002 min
Delta R.T.: -0.005 min
Response: 3728138
Conc: 65.29 ng/ml

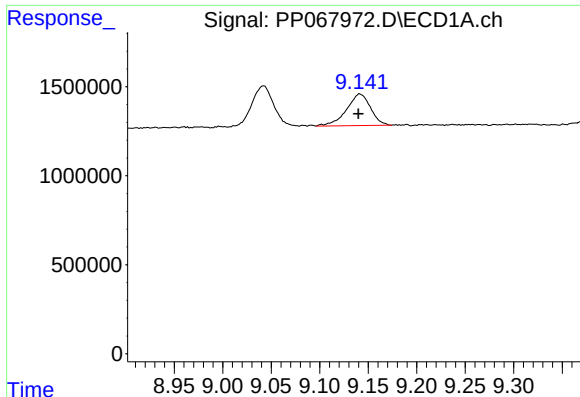

#39 AR-1262-4


R.T.: 9.141 min
Delta R.T.: 0.002 min
Response: 3059698
Conc: 43.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

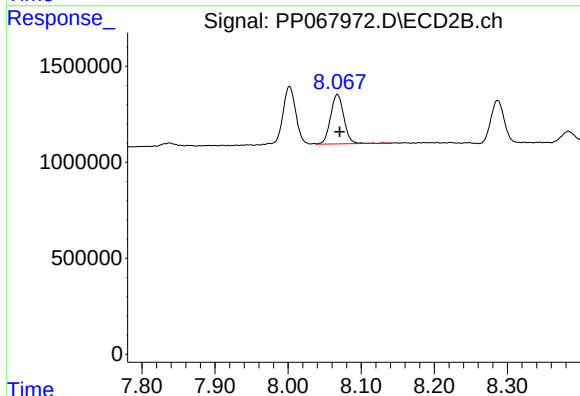


#39 AR-1262-4

R.T.: 8.067 min
Delta R.T.: -0.003 min
Response: 3260422
Conc: 32.46 ng/ml

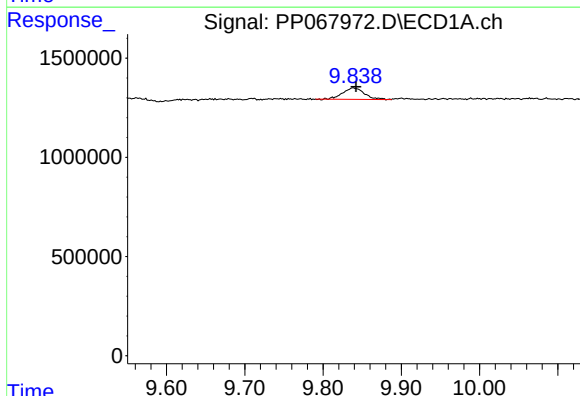


#40 AR-1262-5

R.T.: 9.839 min
Delta R.T.: -0.003 min
Response: 1113806
Conc: 23.80 ng/ml

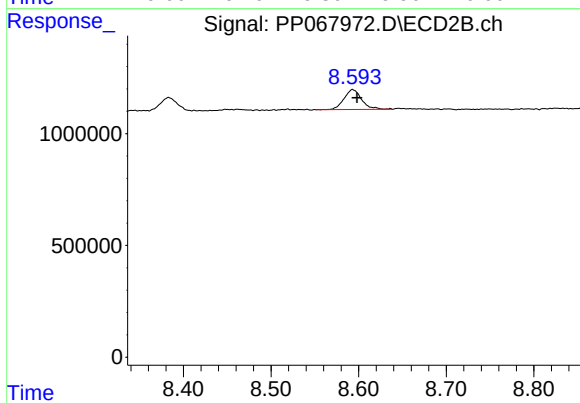

#40 AR-1262-5


R.T.: 8.593 min
Delta R.T.: -0.005 min
Response: 1249947
Conc: 24.99 ng/ml

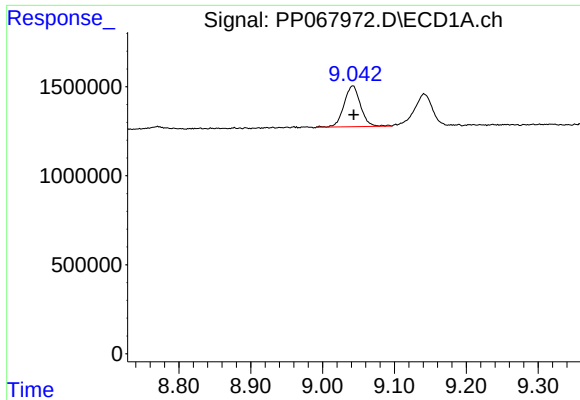

#41 AR-1268-1


R.T.: 9.042 min
Delta R.T.: 0.000 min
Response: 3638154
Conc: 23.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

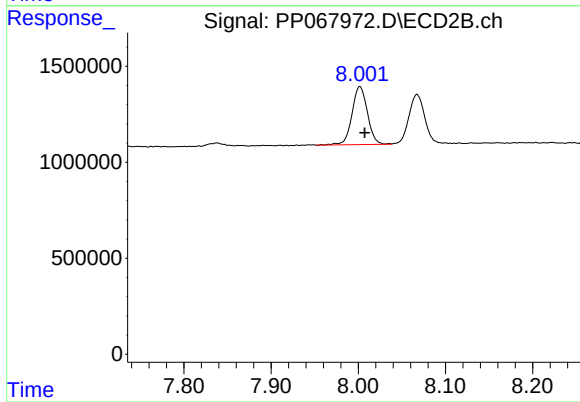


#41 AR-1268-1

R.T.: 8.002 min
Delta R.T.: -0.005 min
Response: 3728138
Conc: 23.43 ng/ml

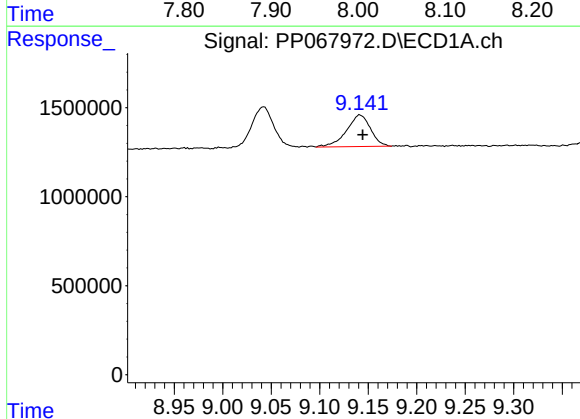


#42 AR-1268-2

R.T.: 9.141 min
Delta R.T.: -0.003 min
Response: 3059698
Conc: 22.40 ng/ml

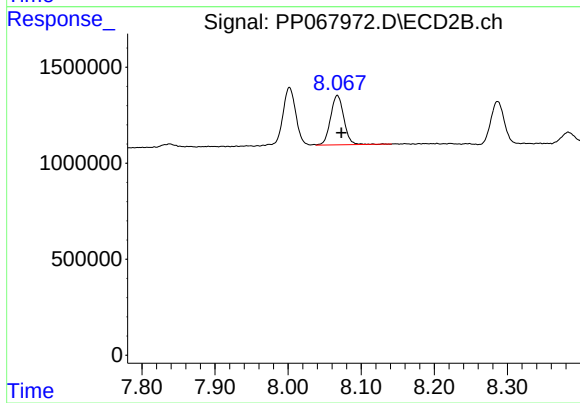

#42 AR-1268-2


R.T.: 8.067 min
Delta R.T.: -0.005 min
Response: 3260422
Conc: 22.77 ng/ml

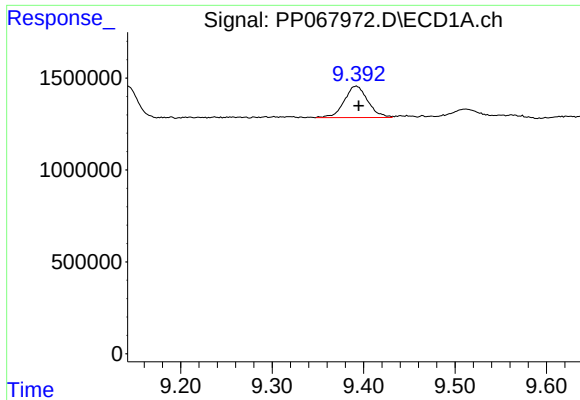

#43 AR-1268-3


R.T.: 9.392 min
Delta R.T.: -0.003 min
Response: 3075797
Conc: 25.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

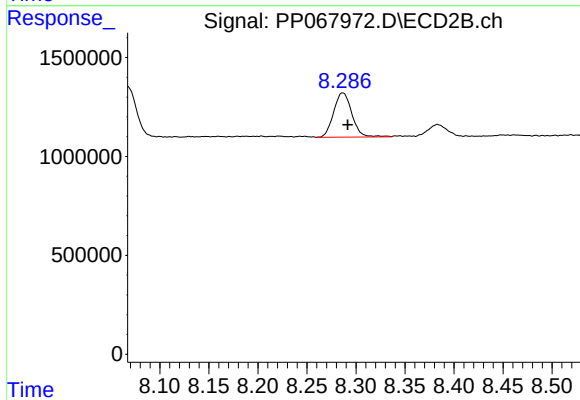


#43 AR-1268-3

R.T.: 8.287 min
Delta R.T.: -0.005 min
Response: 2905069
Conc: 22.78 ng/ml

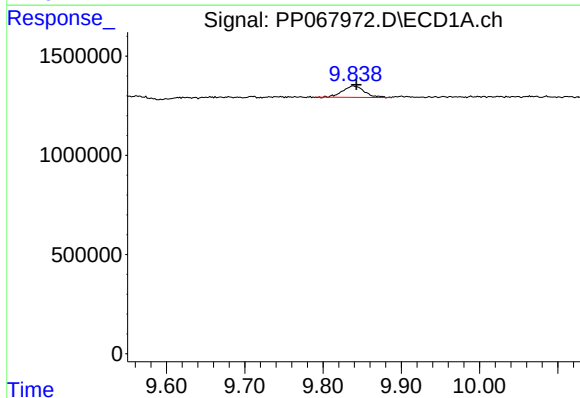


#44 AR-1268-4

R.T.: 9.839 min
Delta R.T.: -0.004 min
Response: 1113806
Conc: 21.92 ng/ml

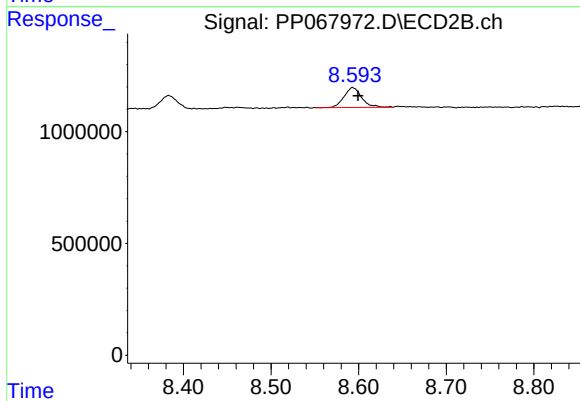

#44 AR-1268-4


R.T.: 8.593 min
Delta R.T.: -0.006 min
Response: 1249947
Conc: 22.13 ng/ml

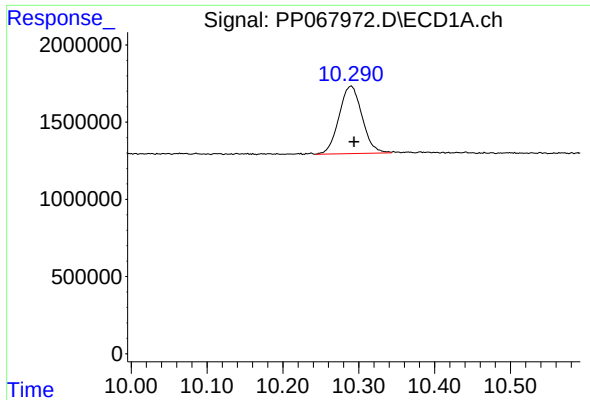

#45 AR-1268-5

R.T.: 10.290 min
Delta R.T.: -0.004 min
Response: 9219060
Conc: 24.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

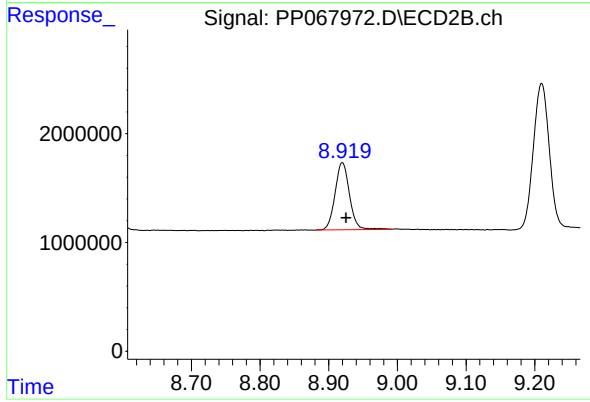

#45 AR-1268-5

R.T.: 8.920 min
Delta R.T.: -0.006 min
Response: 9037360
Conc: 23.91 ng/ml