

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
 Data File : PP067967.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2024 06:08
 Operator : YP\AJ
 Sample : P4368-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT4-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 07:40:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.753	4.049	14718143	15874247	15.900	15.711
2) SA Decachlor...	10.663	9.209	20739530	19598818	18.014	17.476
Target Compounds						
11) L3 AR-1232-1	5.117	4.431	431196	529356	18.863	21.755
12) L3 AR-1232-2	5.649	5.177	249586	596979	21.182	26.693 #
13) L3 AR-1232-3	5.939	5.355	496357	343192	22.283	28.734 #
14) L3 AR-1232-4	6.100	5.439	281230	312712	24.915	27.118
15) L3 AR-1232-5	6.190	5.616	223629	285347	24.520	21.215



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101624\
Data File : PP067967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 06:08
Operator : YP\AJ
Sample : P4368-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 69 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:40:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

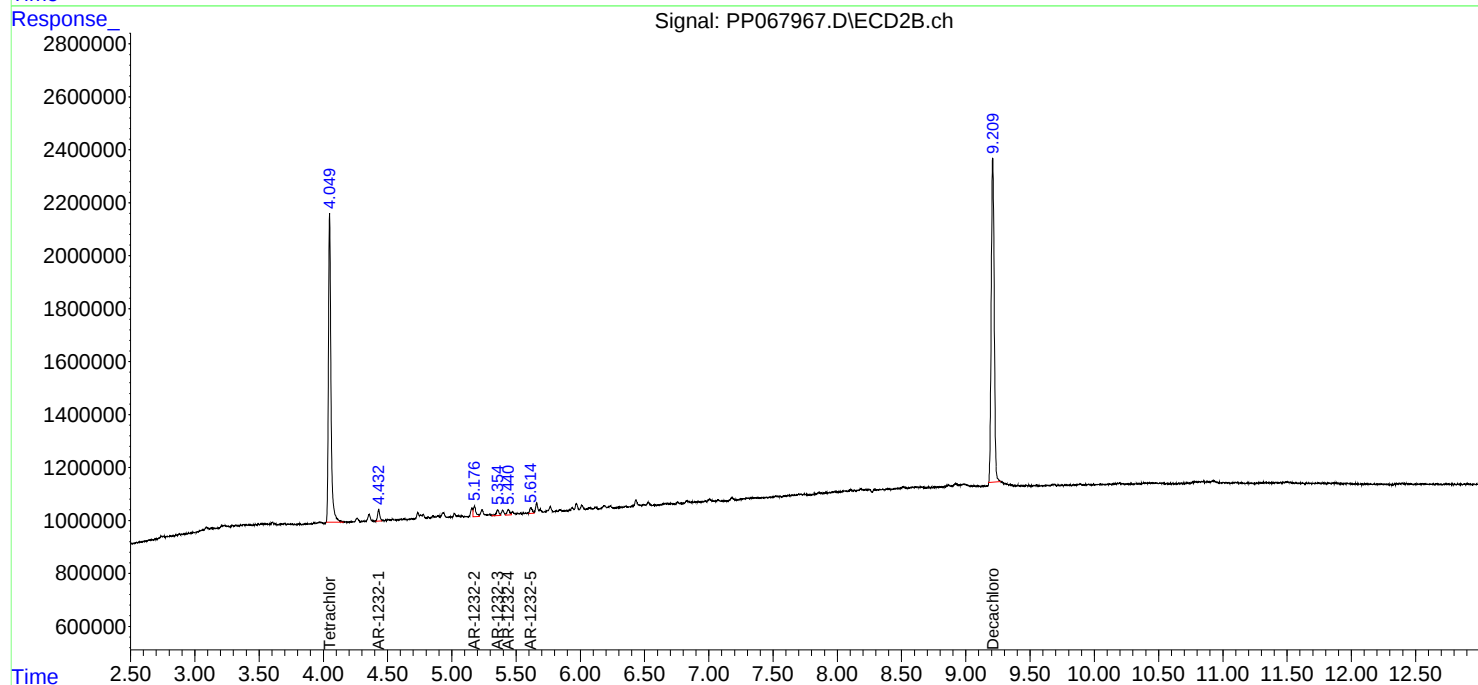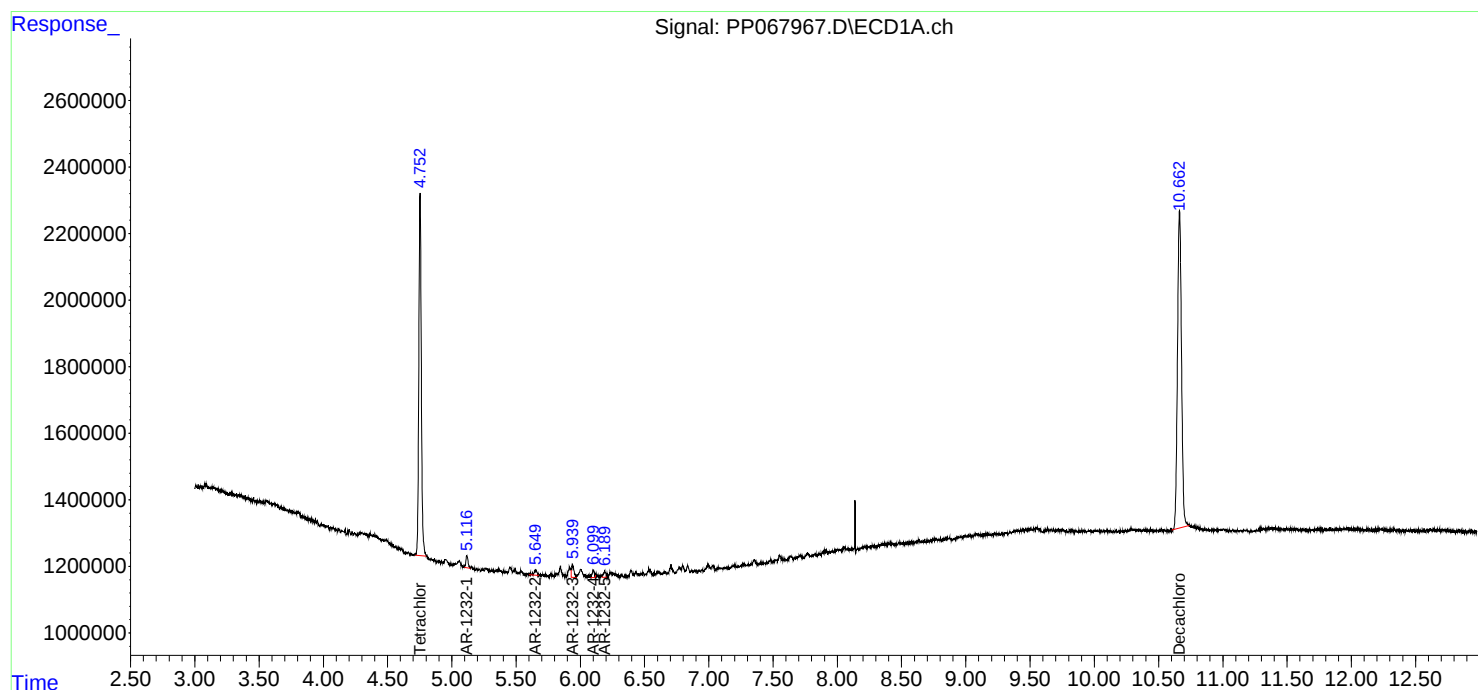


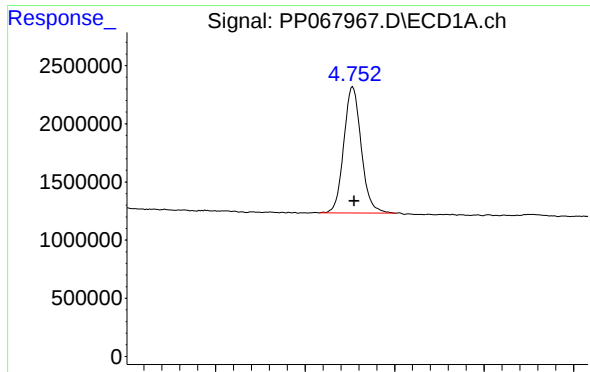

#1 Tetrachloro-m-xylene


R.T.: 4.753 min
Delta R.T.: -0.002 min
Response: 14718143
Conc: 15.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

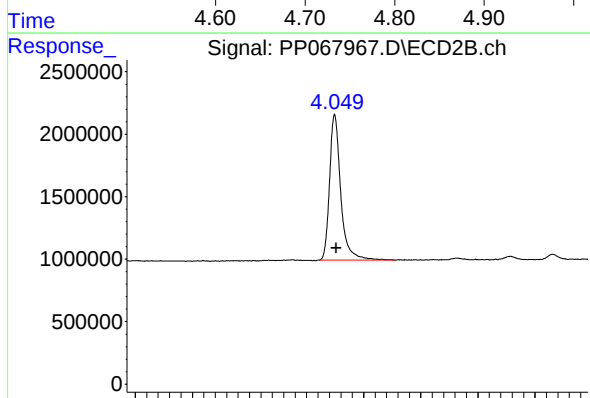


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: -0.003 min
Response: 15874247
Conc: 15.71 ng/ml

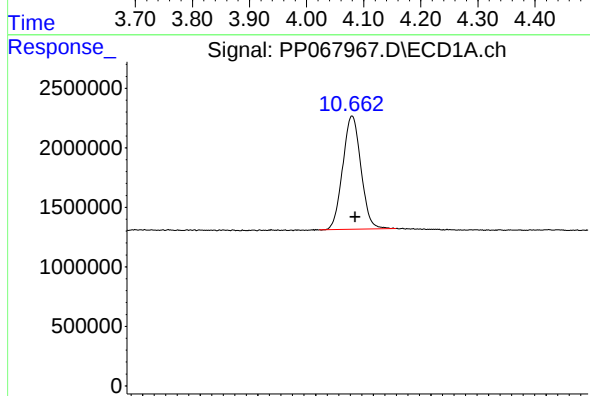


#2 Decachlorobiphenyl

R.T.: 10.663 min
Delta R.T.: -0.006 min
Response: 20739530
Conc: 18.01 ng/ml

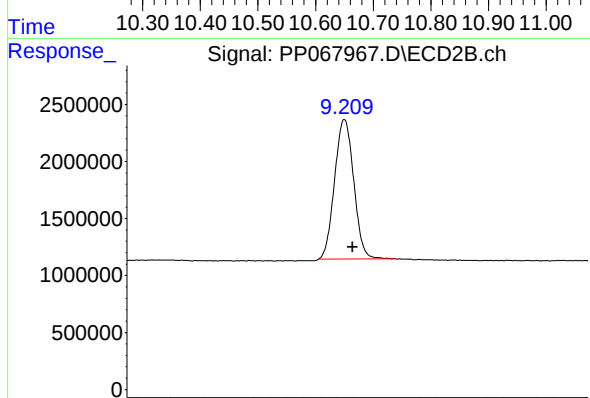

#2 Decachlorobiphenyl


R.T.: 9.209 min
Delta R.T.: -0.010 min
Response: 19598818
Conc: 17.48 ng/ml

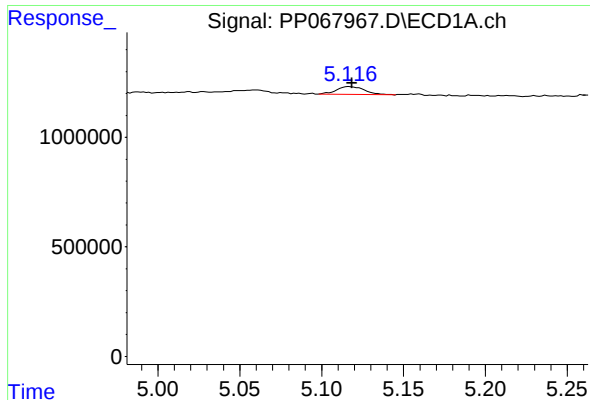

#11 AR-1232-1


R.T.: 5.117 min
Delta R.T.: -0.002 min
Response: 431196
Conc: 18.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

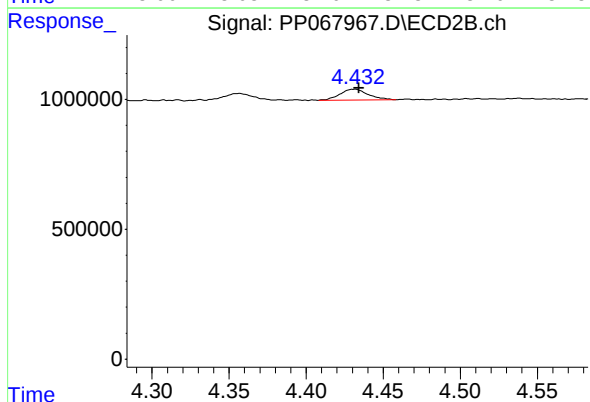


#11 AR-1232-1

R.T.: 4.431 min
Delta R.T.: -0.003 min
Response: 529356
Conc: 21.75 ng/ml

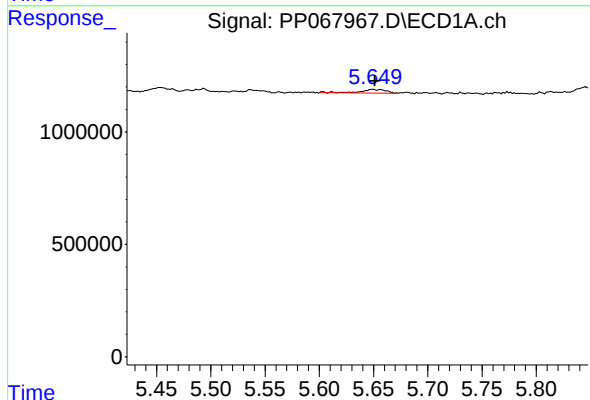


#12 AR-1232-2

R.T.: 5.649 min
Delta R.T.: -0.002 min
Response: 249586
Conc: 21.18 ng/ml

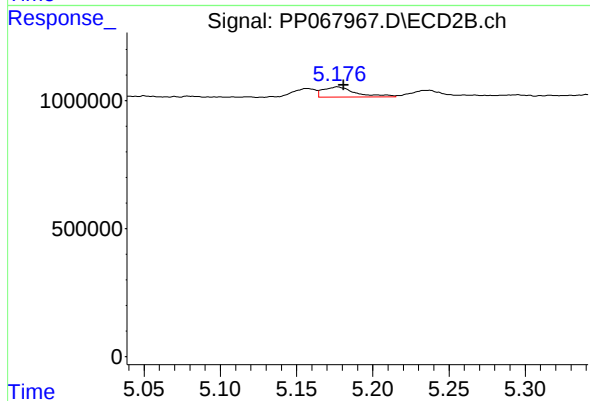

#12 AR-1232-2


R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 596979
Conc: 26.69 ng/ml

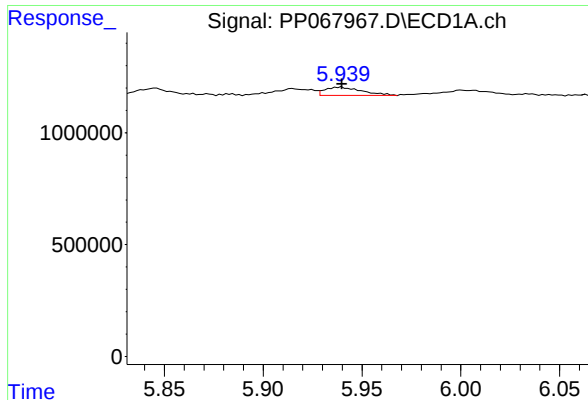

#13 AR-1232-3


R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 496357
Conc: 22.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

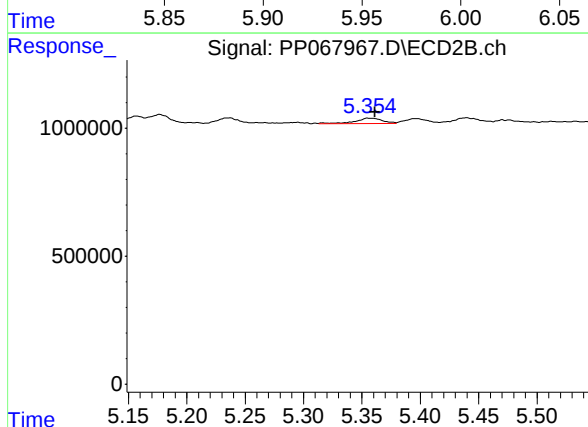


#13 AR-1232-3

R.T.: 5.355 min
Delta R.T.: -0.006 min
Response: 343192
Conc: 28.73 ng/ml

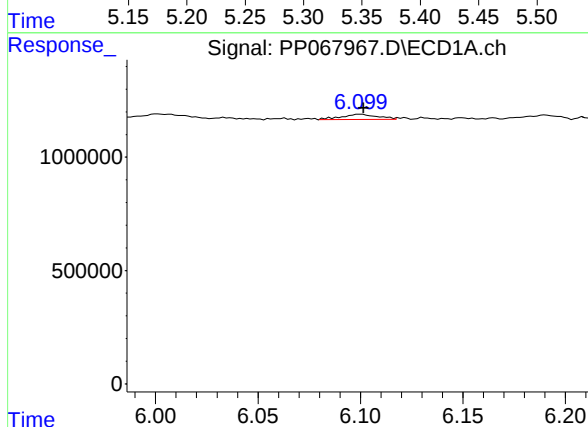


#14 AR-1232-4

R.T.: 6.100 min
Delta R.T.: -0.002 min
Response: 281230
Conc: 24.92 ng/ml

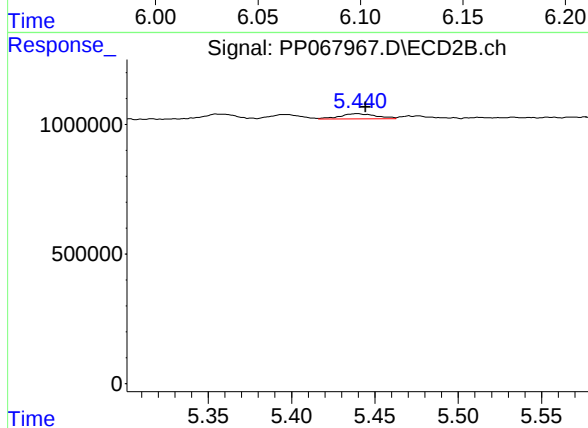

#14 AR-1232-4


R.T.: 5.439 min
Delta R.T.: -0.005 min
Response: 312712
Conc: 27.12 ng/ml

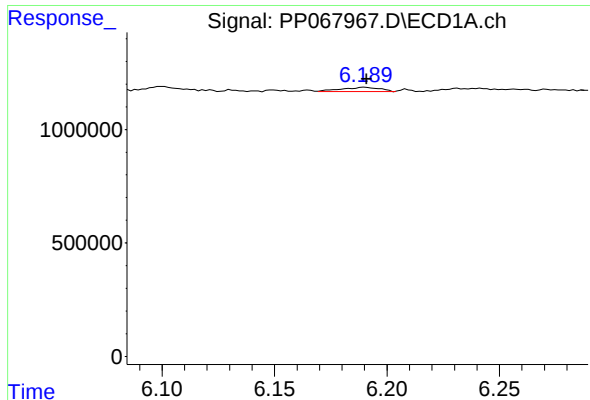

#15 AR-1232-5

R.T.: 6.190 min
Delta R.T.: 0.000 min
Response: 223629
Conc: 24.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2024

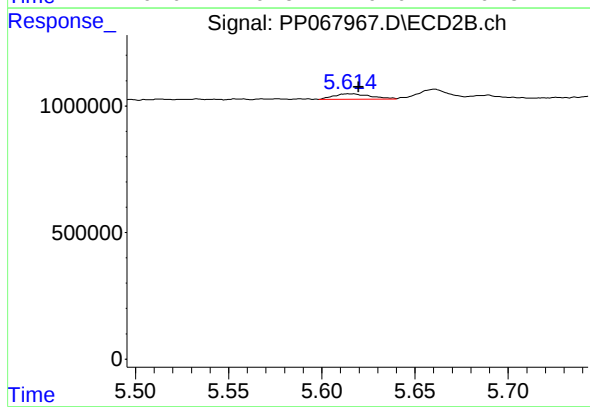

#15 AR-1232-5

R.T.: 5.616 min
Delta R.T.: -0.004 min
Response: 285347
Conc: 21.21 ng/ml