

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101722\
 Data File : PP052387.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2022 19:07
 Operator : YP\AJ
 Sample : N5160-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HD-1-101422

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/18/2022
 Supervised By :Ankita Jodhani 10/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 00:07:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 12 05:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.423	3.674	24958116	18124905	15.878m	15.821
2) SA Decachlor...	10.243	8.768	23612661	17611950	17.014	15.762

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101722\
Data File : PP052387.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2022 19:07
Operator : YP\AJ
Sample : N5160-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HD-1-101422


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/18/2022
Supervised By :Ankita Jodhani 10/19/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 00:07:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

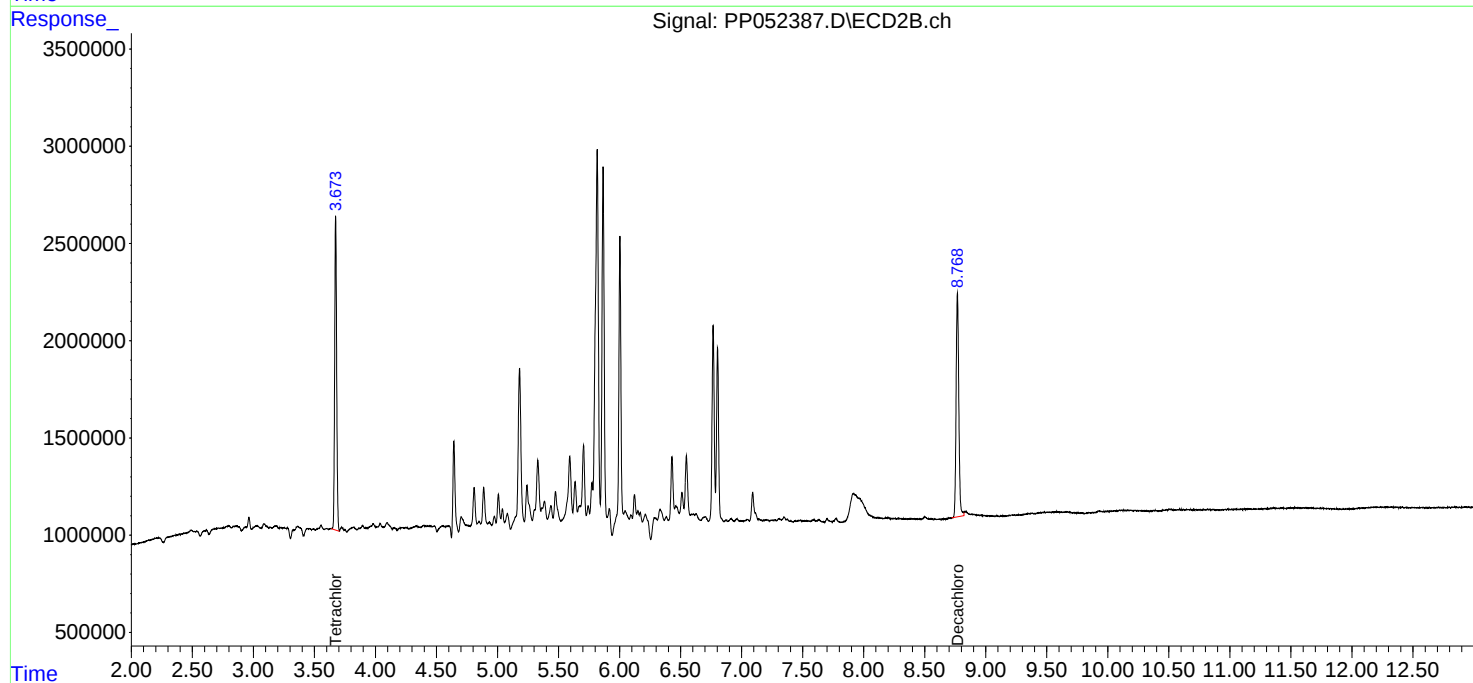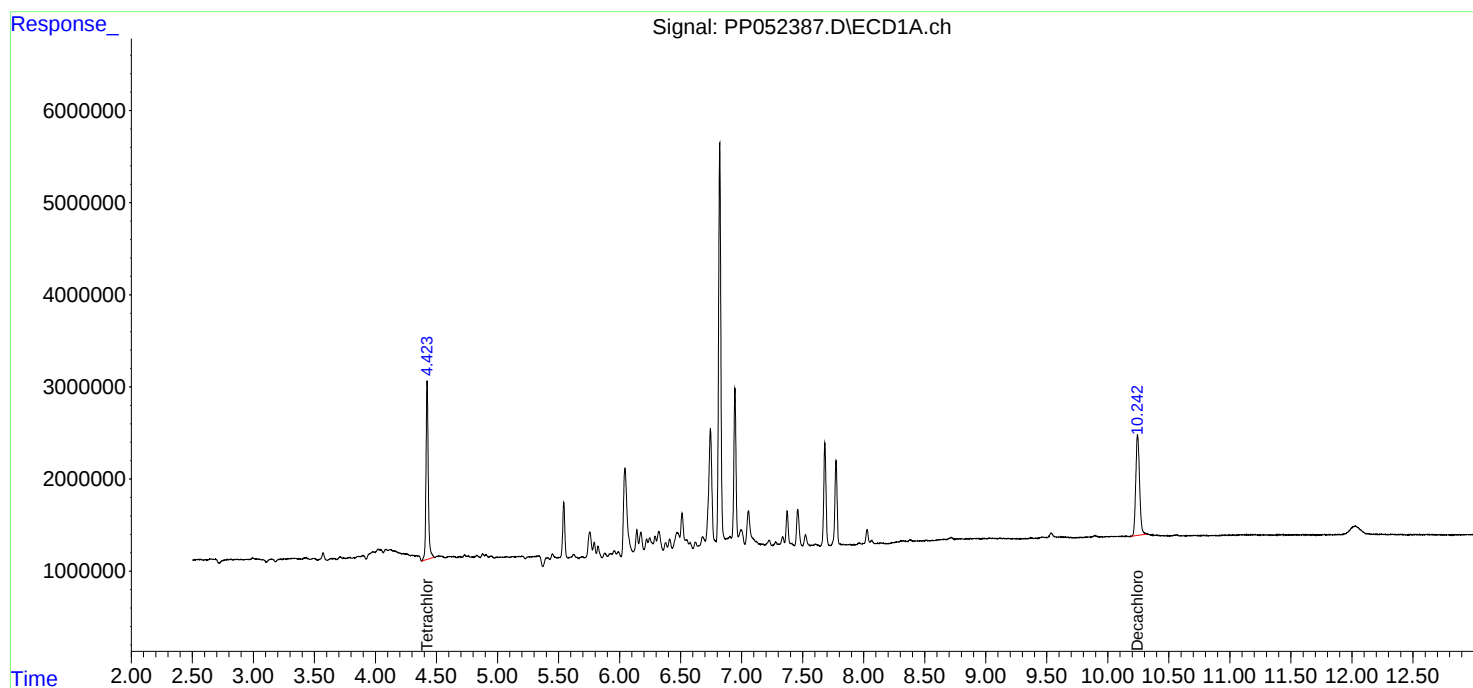

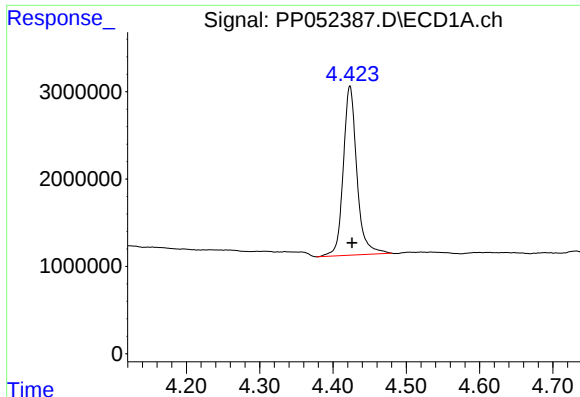


#1 Tetrachloro-m-xylene

R.T.: 4.423 min
Delta R.T.: -0.003 min
Response: 24958116
Conc: 15.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
HD-1-101422


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/18/2022
Supervised By :Ankita Jodhani 10/19/2022

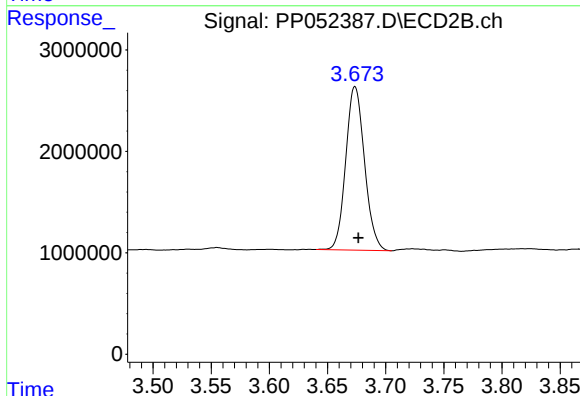


#1 Tetrachloro-m-xylene

R.T.: 3.674 min
Delta R.T.: -0.003 min
Response: 18124905
Conc: 15.82 ng/ml

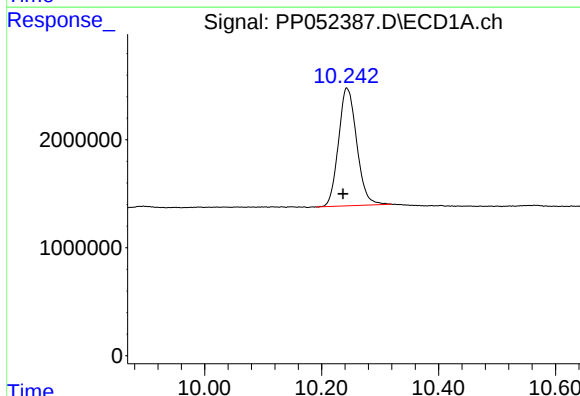

#2 Decachlorobiphenyl

R.T.: 10.243 min
Delta R.T.: 0.007 min
Response: 23612661
Conc: 17.01 ng/ml

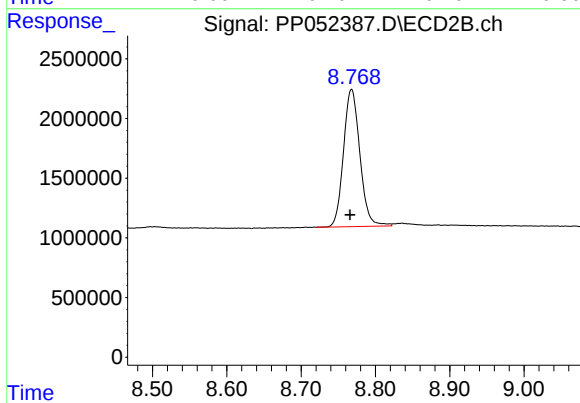

#2 Decachlorobiphenyl

R.T.: 8.768 min
Delta R.T.: 0.002 min
Response: 17611950
Conc: 15.76 ng/ml