

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101723\
 Data File : PP061010.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2023 13:48
 Operator : YP\AJ
 Sample : 04905-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LSS-B4-COMP-101323

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 15:35:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 14 13:32:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.551	3.686	49221207	30140739	22.390	22.293
2) SA Decachlor...	10.507	8.753	28353965	24285920	18.106	16.153

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101723\
Data File : PP061010.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2023 13:48
Operator : YP\AJ
Sample : 04905-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LSS-B4-COMP-101323

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 15:35:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 14 13:32:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

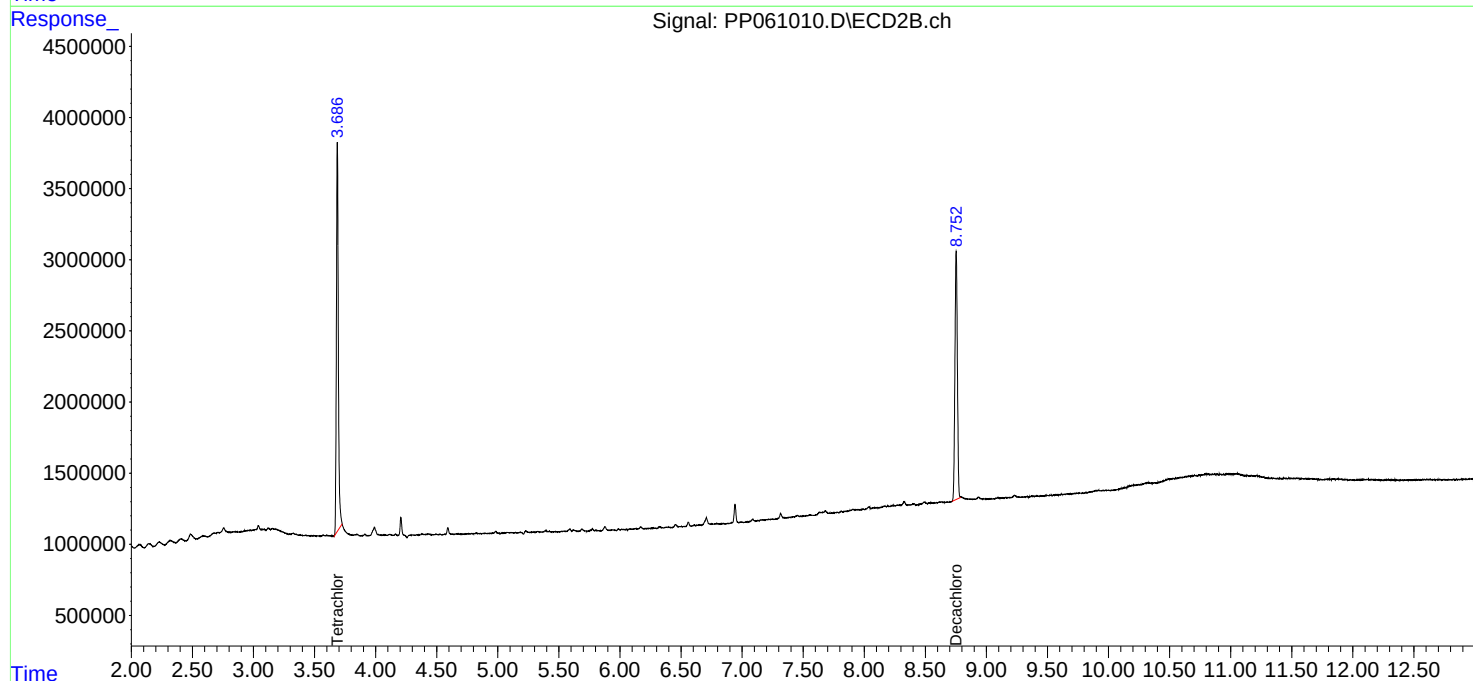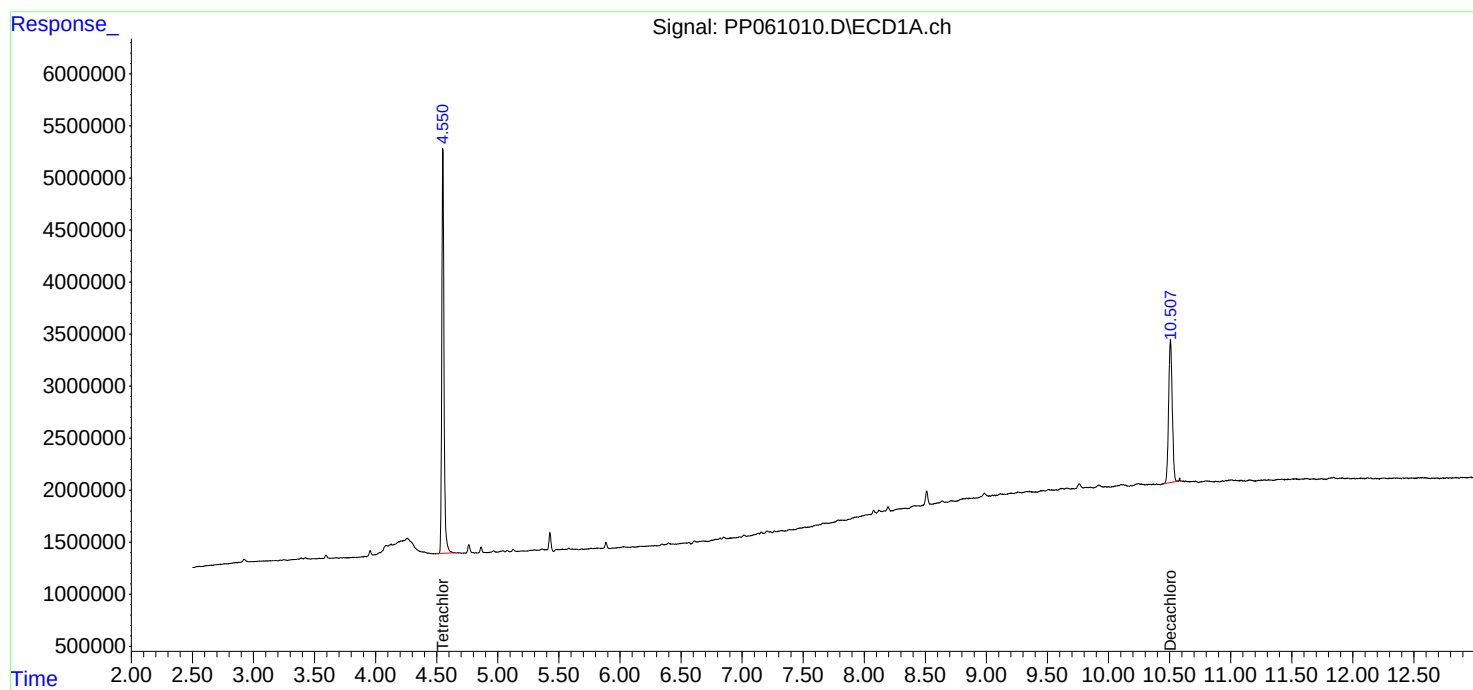


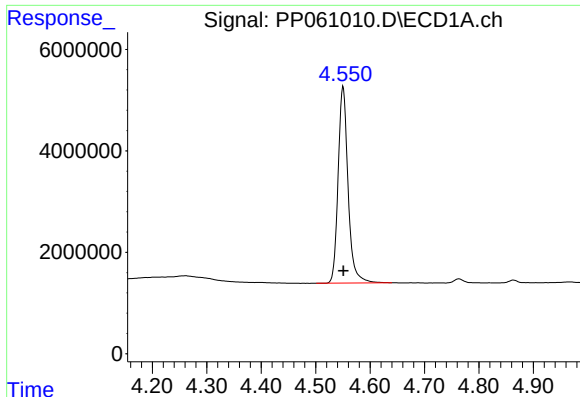

#1 Tetrachloro-m-xylene


R.T.: 4.551 min
Delta R.T.: 0.000 min
Response: 49221207
Conc: 22.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
LSS-B4-COMP-101323

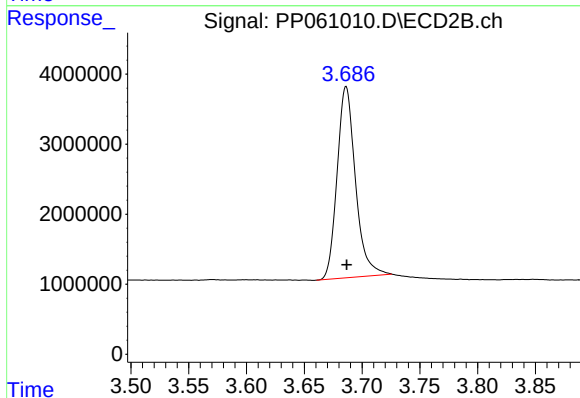


#1 Tetrachloro-m-xylene

R.T.: 3.686 min
Delta R.T.: 0.000 min
Response: 30140739
Conc: 22.29 ng/ml

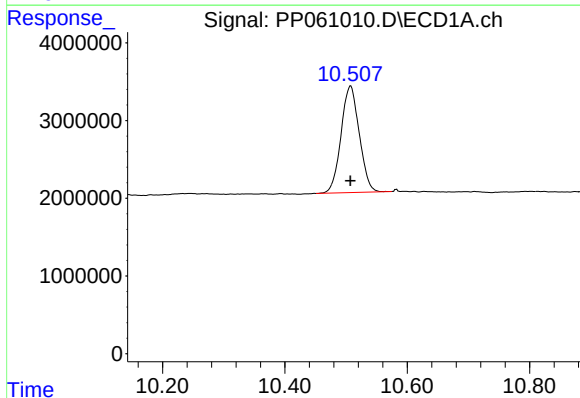

#2 Decachlorobiphenyl

R.T.: 10.507 min
Delta R.T.: 0.000 min
Response: 28353965
Conc: 18.11 ng/ml

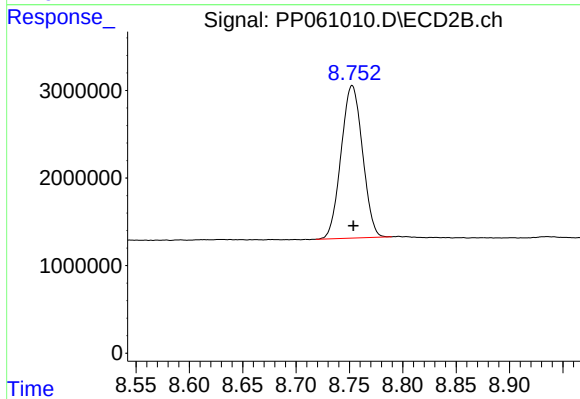

#2 Decachlorobiphenyl

R.T.: 8.753 min
Delta R.T.: -0.001 min
Response: 24285920
Conc: 16.15 ng/ml