

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101724\
 Data File : PP068011.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2024 03:14
 Operator : YP\AJ
 Sample : P4426-37
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WALL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/18/2024
 Supervised By :Ankita Jodhani 10/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 05:20:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.753	4.049	18997086	20120836	20.523	19.914
2) SA Decachlor...	10.662	9.208	23865793	22569440	20.729	20.125m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101724\
Data File : PP068011.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2024 03:14
Operator : YP\AJ
Sample : P4426-37
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WALL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/18/2024
Supervised By :Ankita Jodhani 10/18/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 05:20:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

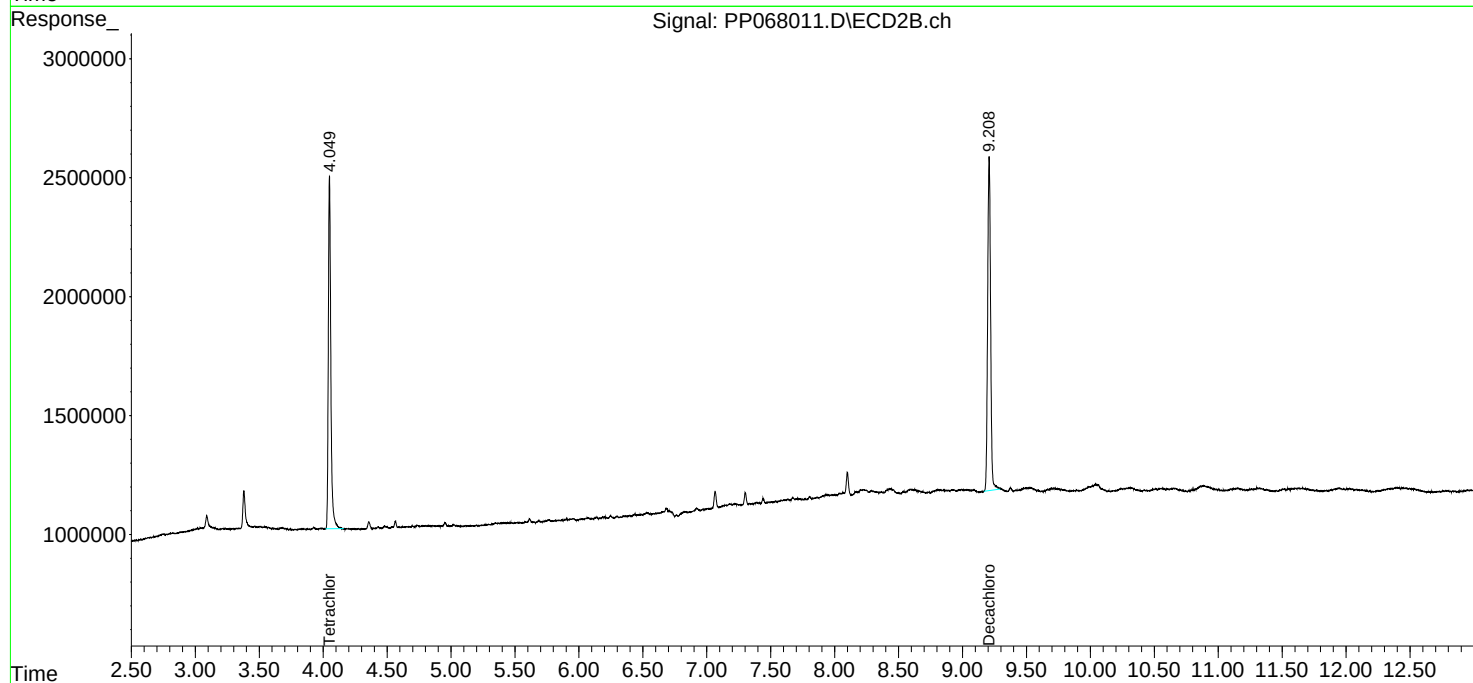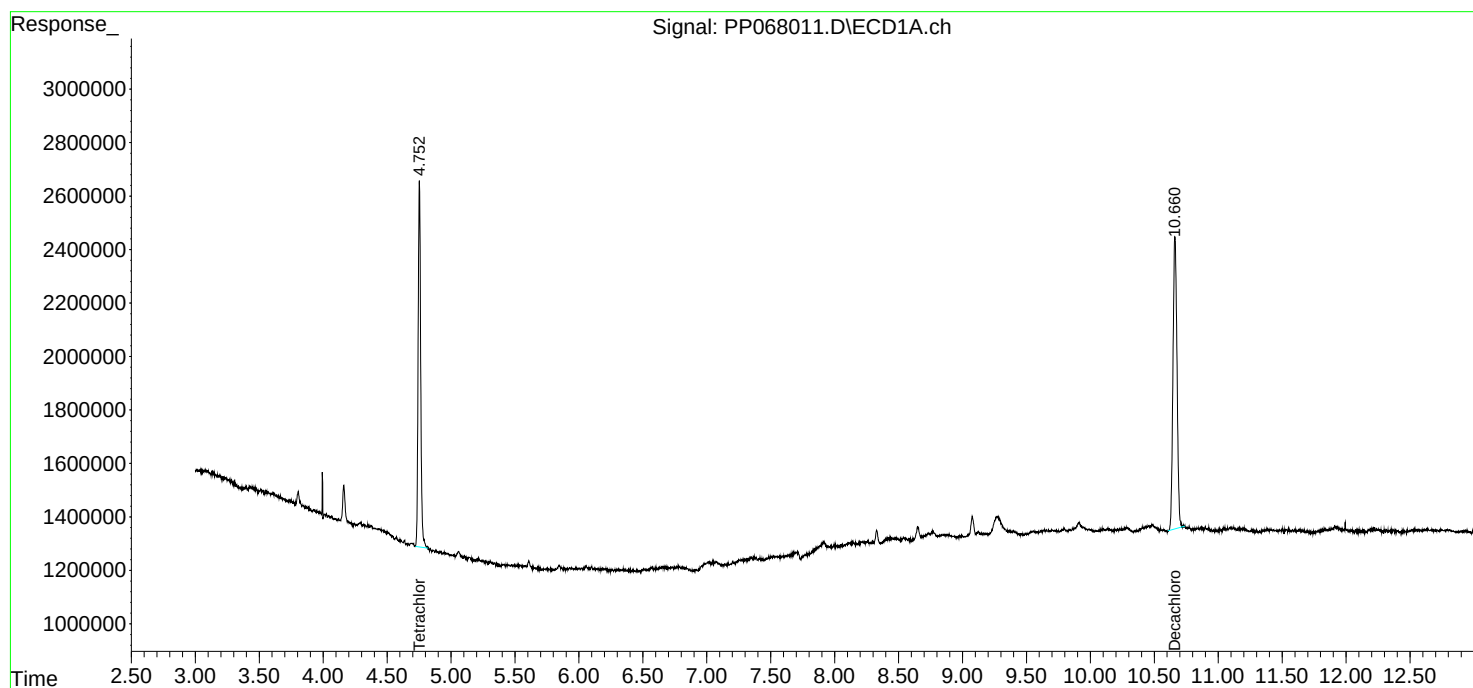

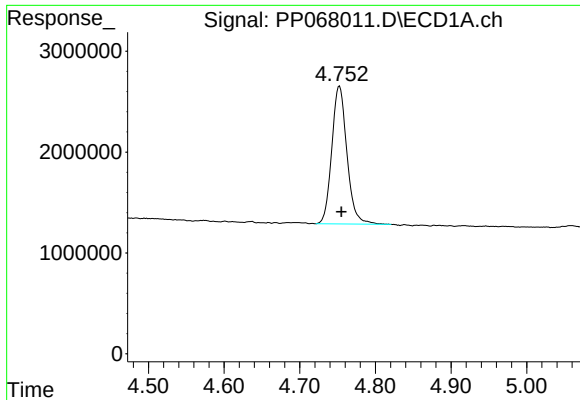


#1 Tetrachloro-m-xylene

R.T.: 4.753 min
Delta R.T.: -0.002 min
Response: 18997086
Conc: 20.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
WALL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/18/2024
Supervised By :Ankita Jodhani 10/18/2024

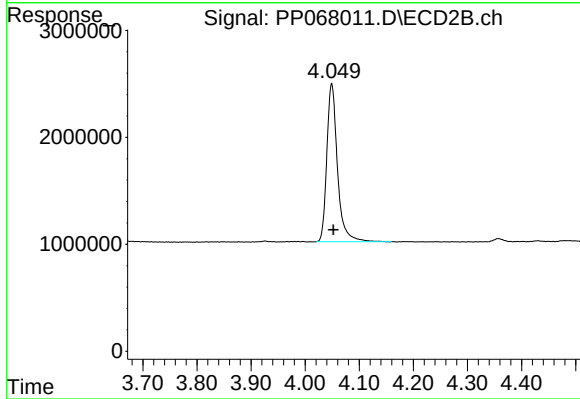


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: -0.003 min
Response: 20120836
Conc: 19.91 ng/ml

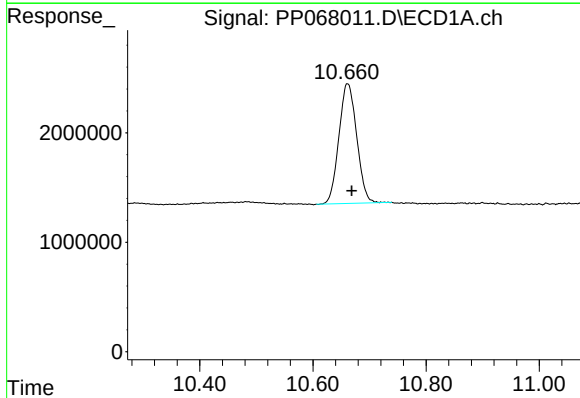

#2 Decachlorobiphenyl

R.T.: 10.662 min
Delta R.T.: -0.007 min
Response: 23865793
Conc: 20.73 ng/ml

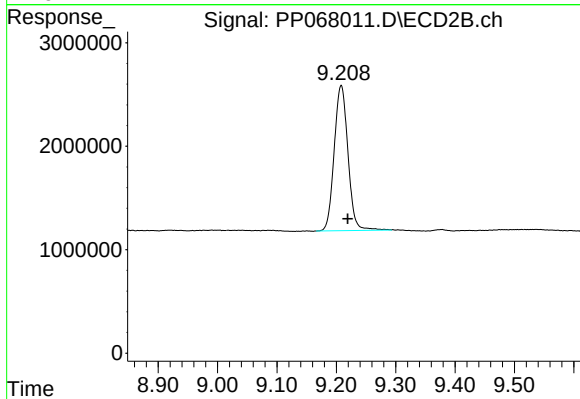

#2 Decachlorobiphenyl

R.T.: 9.208 min
Delta R.T.: -0.011 min
Response: 22569440
Conc: 20.13 ng/ml m