

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101724\
 Data File : PP068027.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2024 08:51
 Operator : YP\AJ
 Sample : PB164231BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB164231BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/18/2024
 Supervised By :Ankita Jodhani 10/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 13:18:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.752	4.049	17556502	17871338	18.967	17.687
2) SA Decachlor...	10.659	9.206	23757334	22118402	20.635	19.723m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101724\
Data File : PP068027.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2024 08:51
Operator : YP\AJ
Sample : PB164231BL
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB164231BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/18/2024
Supervised By :Ankita Jodhani 10/18/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 13:18:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

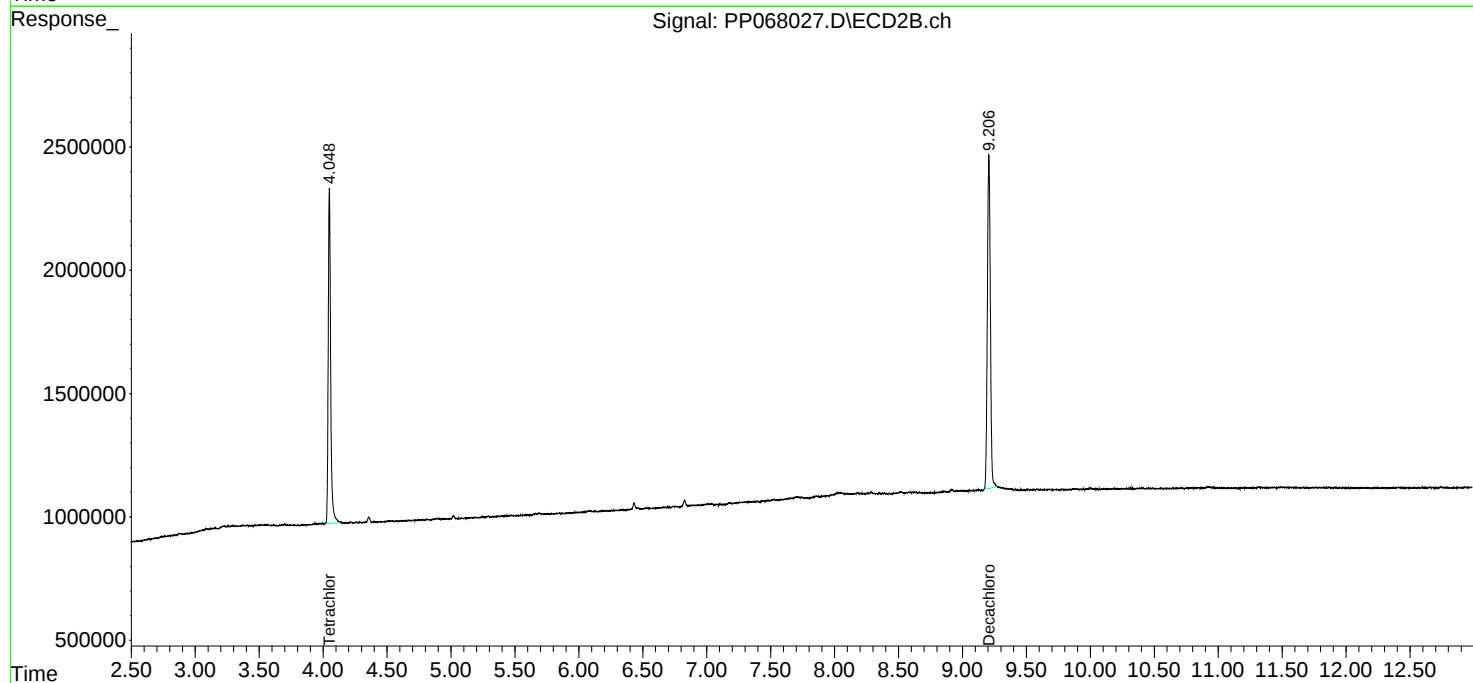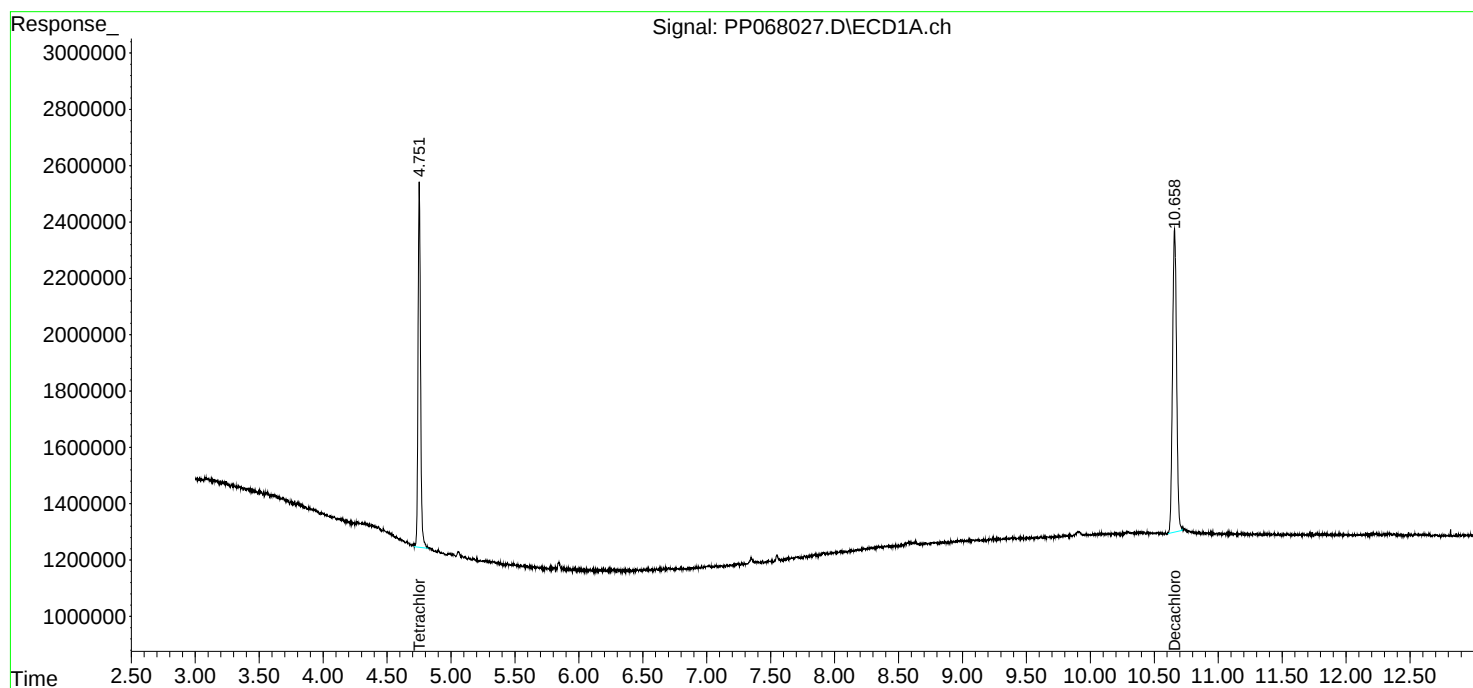

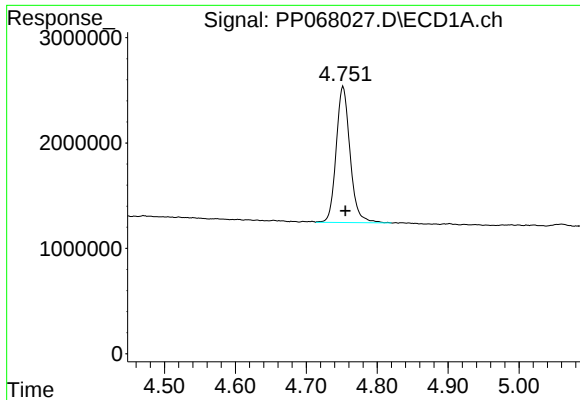

#1 Tetrachloro-m-xylene

R.T.: 4.752 min
Delta R.T.: -0.003 min
Response: 17556502
Conc: 18.97 ng/ml

Instrument :

ECD_P

ClientSampleId :


PB164231BL

Manual Integrations

APPROVED


Reviewed By :Yogesh Patel 10/18/2024

Supervised By :Ankita Jodhani 10/18/2024

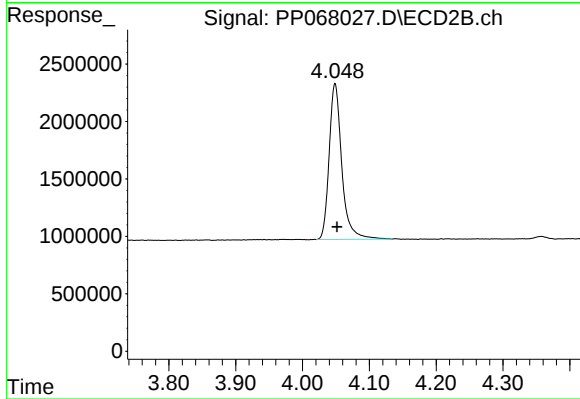


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: -0.003 min
Response: 17871338
Conc: 17.69 ng/ml

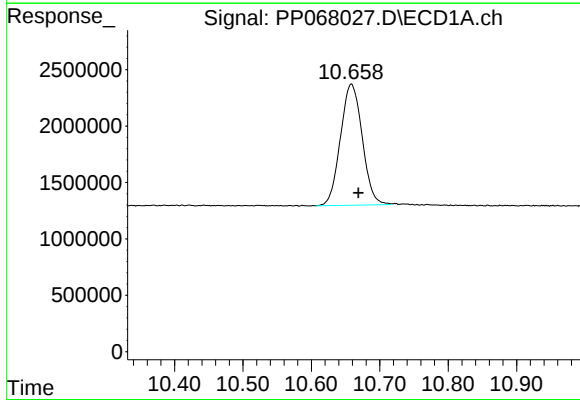

#2 Decachlorobiphenyl

R.T.: 10.659 min
Delta R.T.: -0.010 min
Response: 23757334
Conc: 20.64 ng/ml

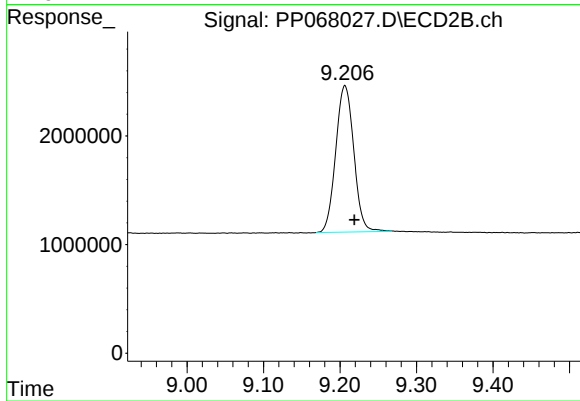

#2 Decachlorobiphenyl

R.T.: 9.206 min
Delta R.T.: -0.013 min
Response: 22118402
Conc: 19.72 ng/ml m