

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101818\
 Data File : PP027728.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Oct 2018 23:08
 Operator : EI\MA
 Sample : J5202-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 03:27:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100918.M
 Quant Title : 8080.M
 QLast Update : Thu Oct 11 18:41:33 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.045	12.160	72847065	104.4E6	294.456	248.168
Target Compounds							
1) T	Dalapon	3.273	2.945	150.4E6	202.3E6	250.144	378.660 #
3) T	4-Nitroph...	0.000	11.301	0	3111596	N.D.	17.342 #
6) T	MCP	12.726	0.000	25069326	0	58.082	N.D. #
7) T	MCPA	0.000	12.984	0	29707358	N.D.	22.829 #
8) T	DICHLORPROP	13.543	13.599	6733962	15605210	19.005	38.355 #
10) T	Pentachlo...	0.000	14.680	0	2353164	N.D.	0.359 #
12) T	2,4,5-T	15.592	15.896	1535143	10543905	0.696	6.417 #
15) T	Picloram	0.000	18.280	0	16591851	N.D.	161.096 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101818\
Data File : PP027728.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Oct 2018 23:08
Operator : EI\MA
Sample : J5202-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 03:27:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100918.M
Quant Title : 8080.M
QLast Update : Thu Oct 11 18:41:33 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

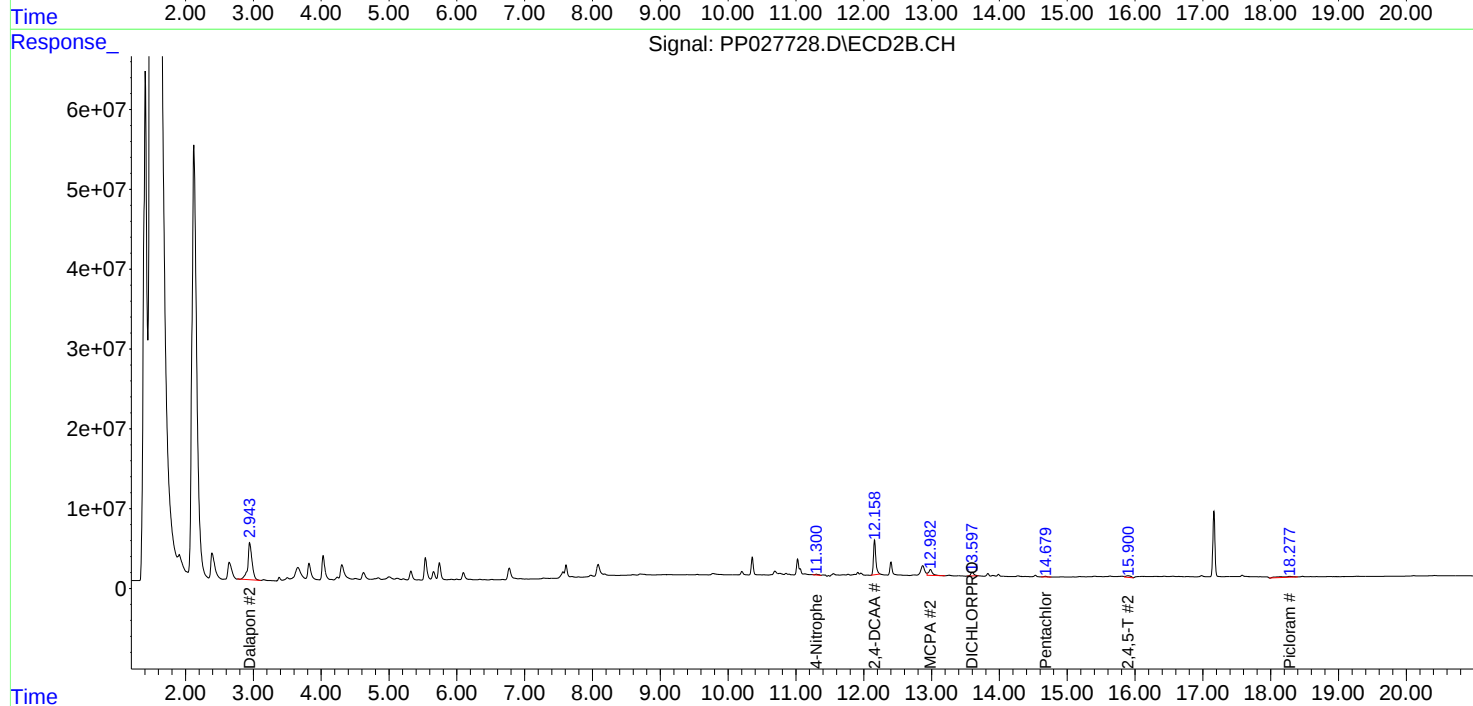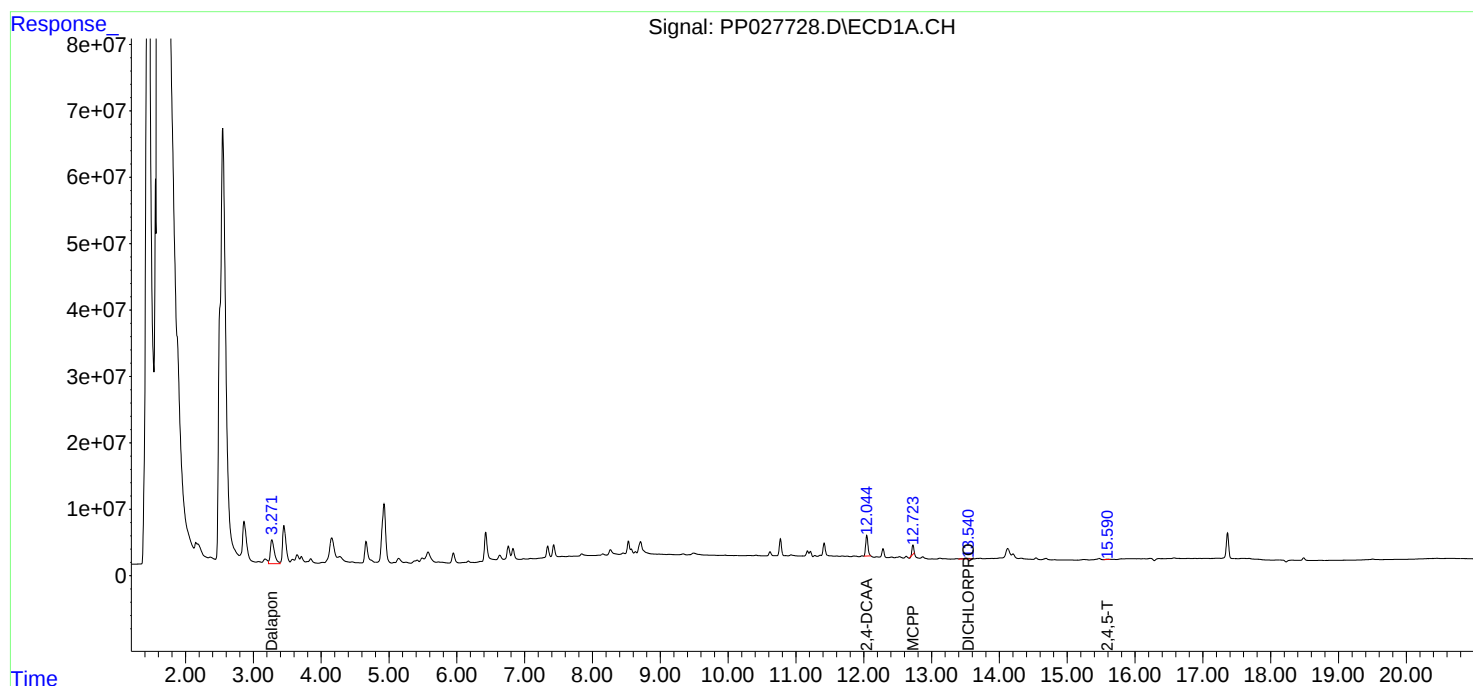


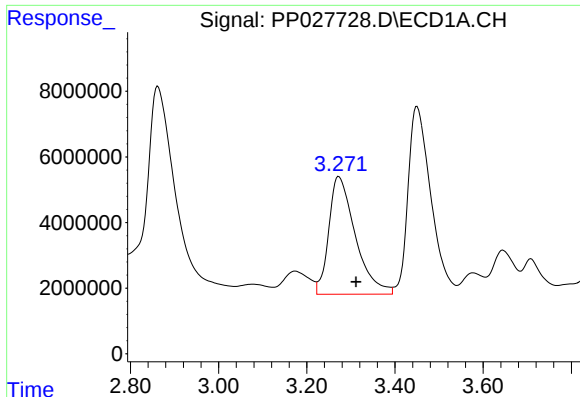

#1 Dalapon


R.T.: 3.273 min
Delta R.T.: -0.039 min
Response: 150365309
Conc: 250.14 ng/ml

Instrument :
ECD_P
ClientSampleId :

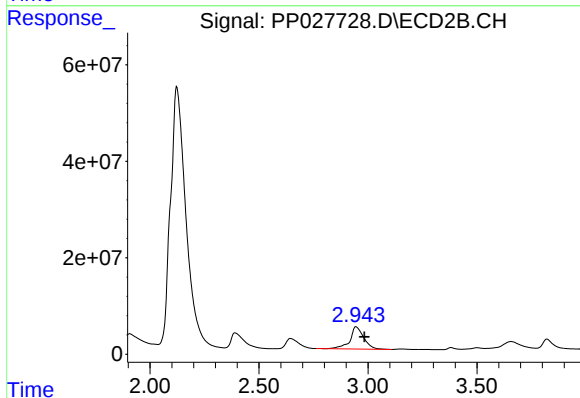


#1 Dalapon

R.T.: 2.945 min
Delta R.T.: -0.038 min
Response: 202336277
Conc: 378.66 ng/ml

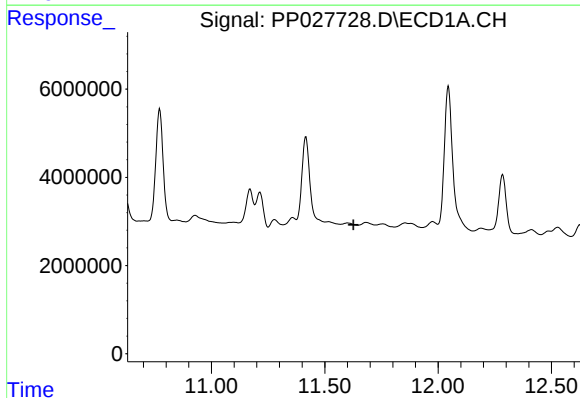


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 11.627 min
Response: 0
Conc: N.D.

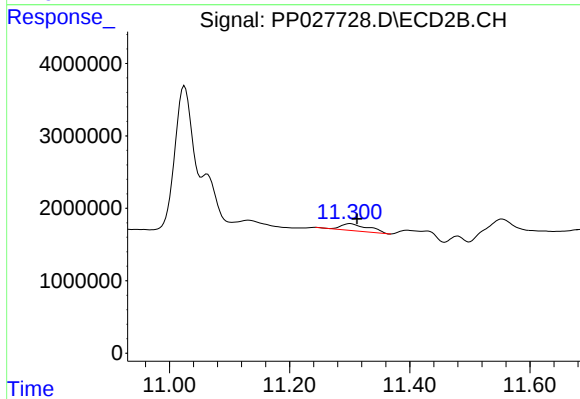

#3 4-Nitrophenol


R.T.: 11.301 min
Delta R.T.: -0.011 min
Response: 3111596
Conc: 17.34 ng/ml

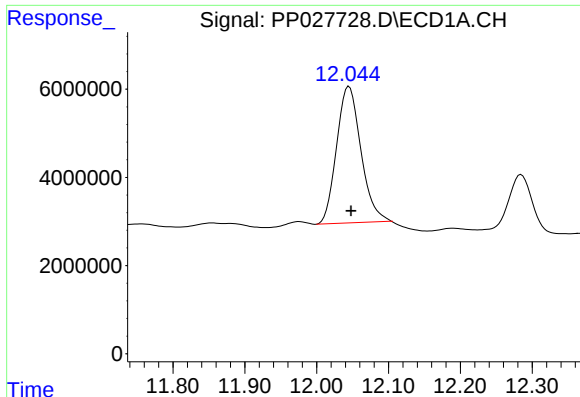

#4 2,4-DCAA


R.T.: 12.045 min
Delta R.T.: -0.003 min
Response: 72847065
Conc: 294.46 ng/ml

Instrument :
ECD_P
ClientSampleId :

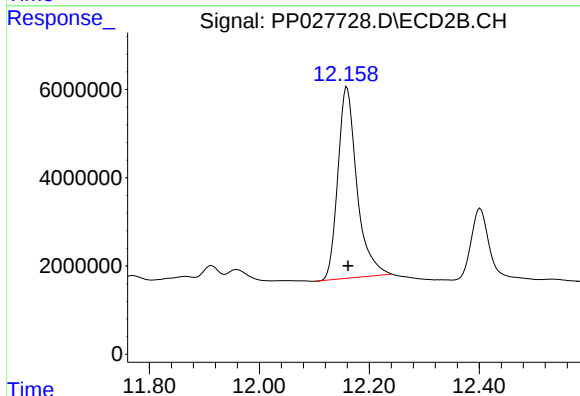


#4 2,4-DCAA

R.T.: 12.160 min
Delta R.T.: -0.002 min
Response: 104427583
Conc: 248.17 ng/ml

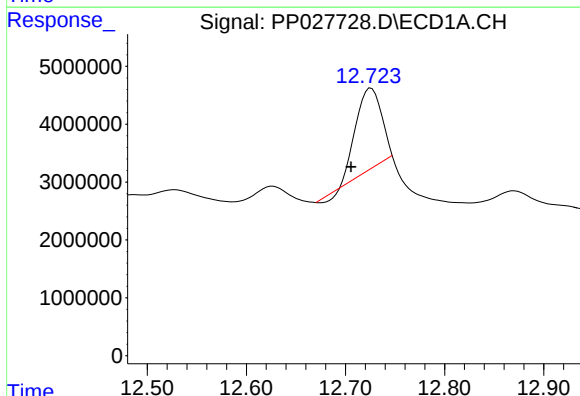


#6 MCPP

R.T.: 12.726 min
Delta R.T.: 0.020 min
Response: 25069326
Conc: 58.08 ug/ml

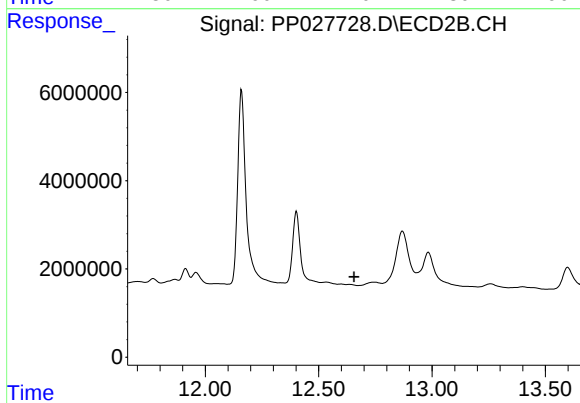

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 12.656 min
Response: 0
Conc: N.D.

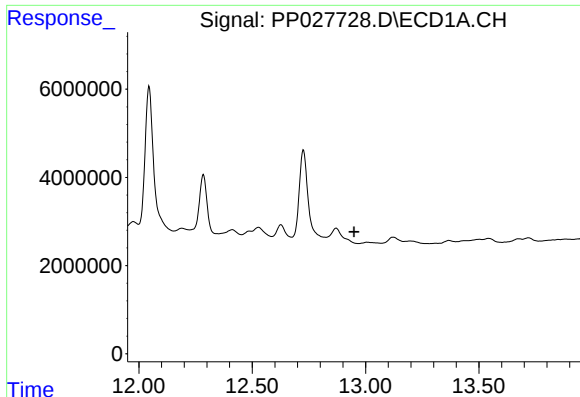

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.950 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

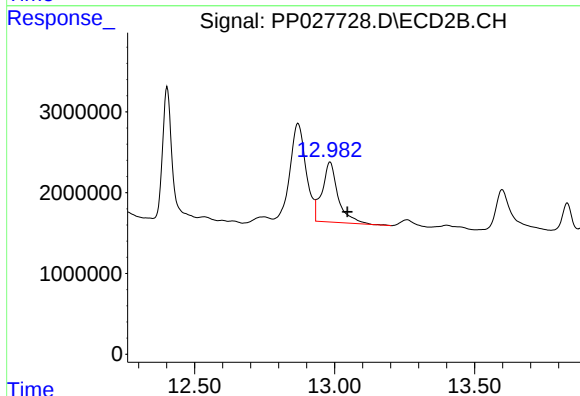


#7 MCPA

R.T.: 12.984 min
Delta R.T.: -0.061 min
Response: 29707358
Conc: 22.83 ug/ml

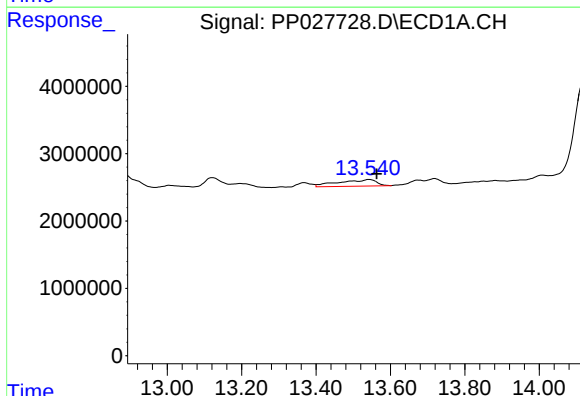


#8 DICHLORPROP

R.T.: 13.543 min
Delta R.T.: -0.021 min
Response: 6733962
Conc: 19.00 ng/ml

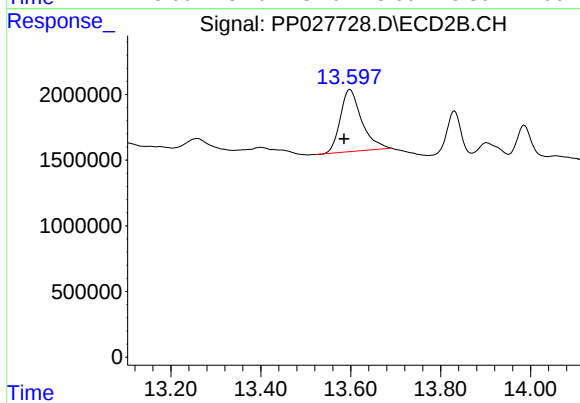

#8 DICHLORPROP


R.T.: 13.599 min
Delta R.T.: 0.013 min
Response: 15605210
Conc: 38.35 ng/ml

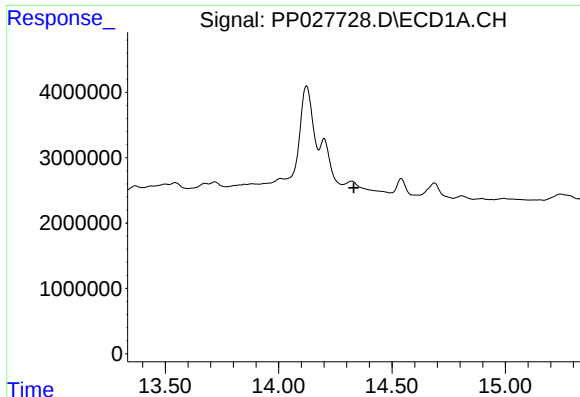

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 14.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

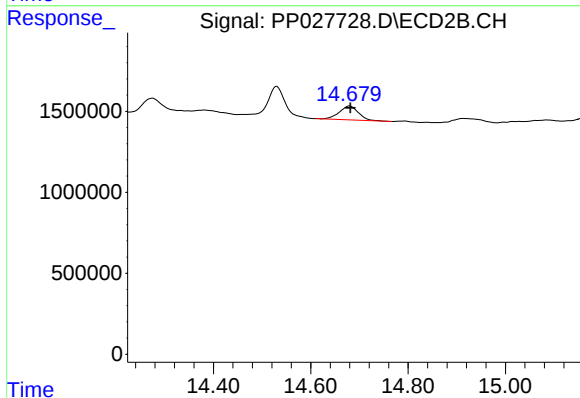


#10 Pentachlorophenol

R.T.: 14.680 min
Delta R.T.: -0.001 min
Response: 2353164
Conc: 0.36 ng/ml

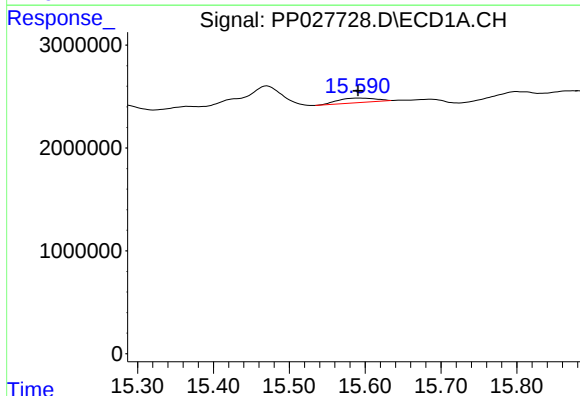


#12 2,4,5-T

R.T.: 15.592 min
Delta R.T.: 0.001 min
Response: 1535143
Conc: 0.70 ng/ml

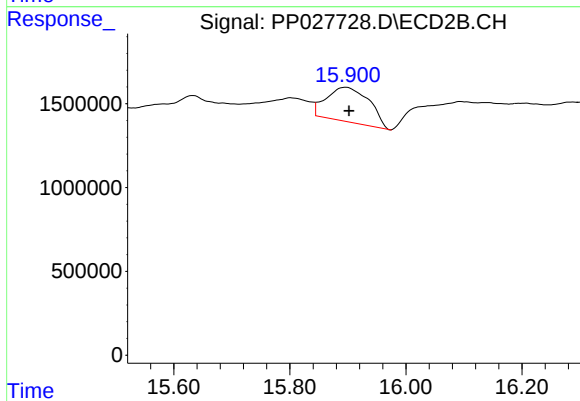

#12 2,4,5-T


R.T.: 15.896 min
Delta R.T.: -0.006 min
Response: 10543905
Conc: 6.42 ng/ml

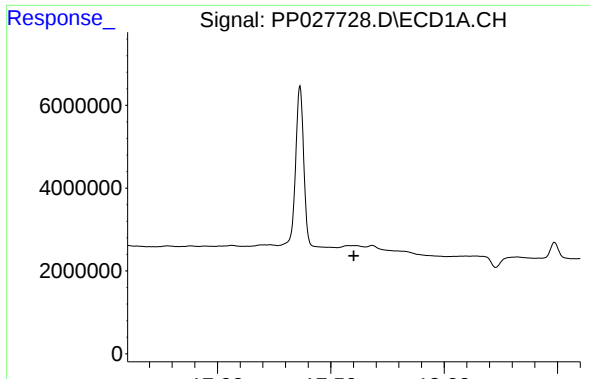

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.602 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

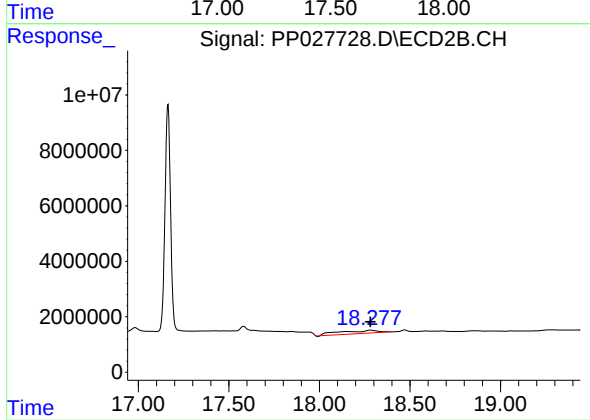

#15 Picloram

R.T.: 18.280 min
Delta R.T.: -0.002 min
Response: 16591851
Conc: 161.10 ng/ml