

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101821\
 Data File : PP040176.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Oct 2021 23:38
 Operator : AJ\MA
 Sample : M4259-07
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-1-BD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 02:22:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.893	3.980	663905	381029	21.862	22.538
2) SA Decachlor...	10.912	9.308	534879	451639	21.640	21.281
Target Compounds						
8) L2 AR-1221-1	5.145	0.000	48247	0	138.539	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101821\
Data File : PP040176.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Oct 2021 23:38
Operator : AJ\MA
Sample : M4259-07
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
WC-1-BD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 02:22:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

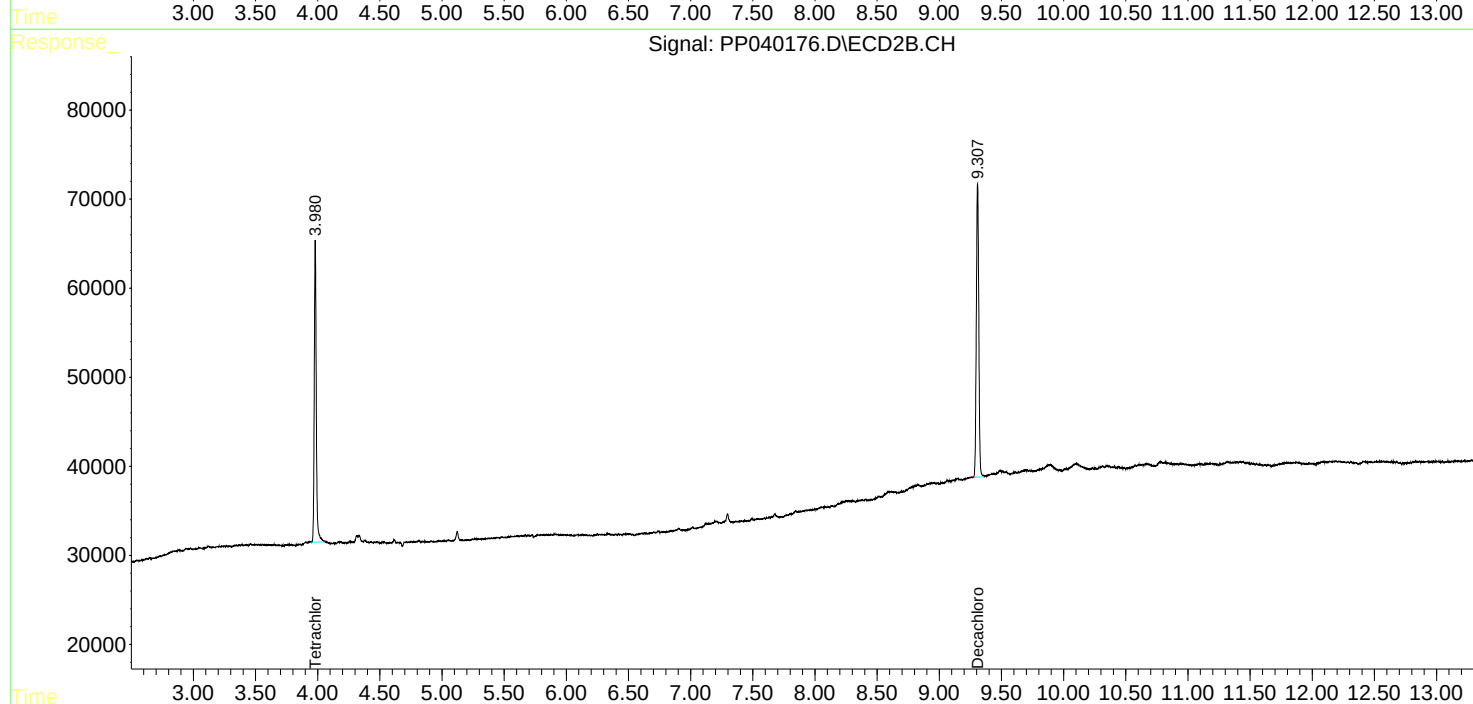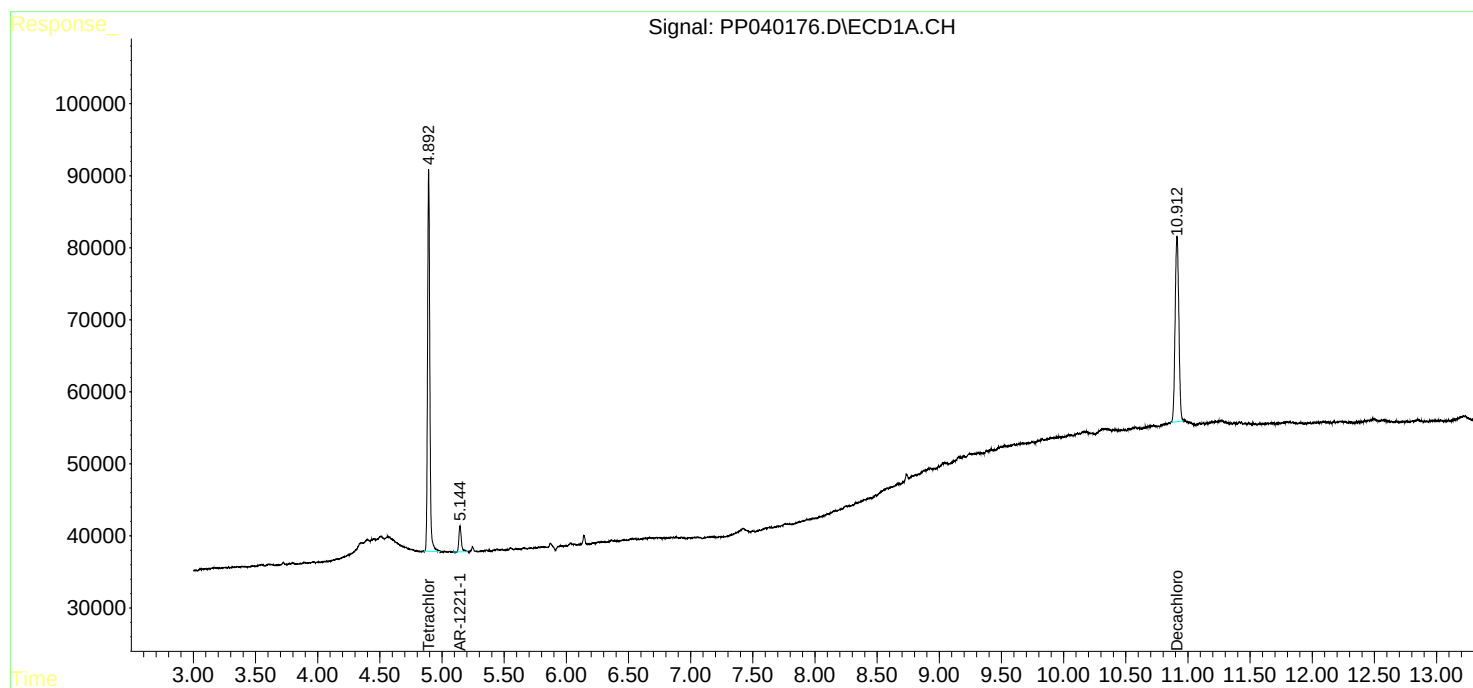


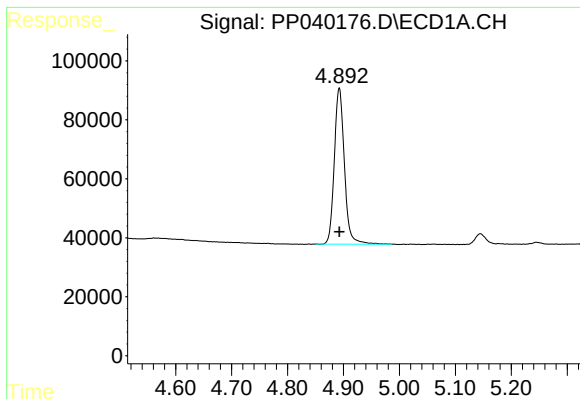

#1 Tetrachloro-m-xylene


R.T.: 4.893 min
Delta R.T.: 0.000 min
Response: 663905
Conc: 21.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-1-BD

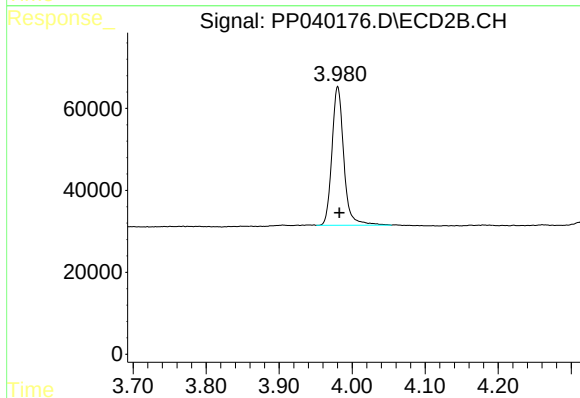


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 381029
Conc: 22.54 ng/ml

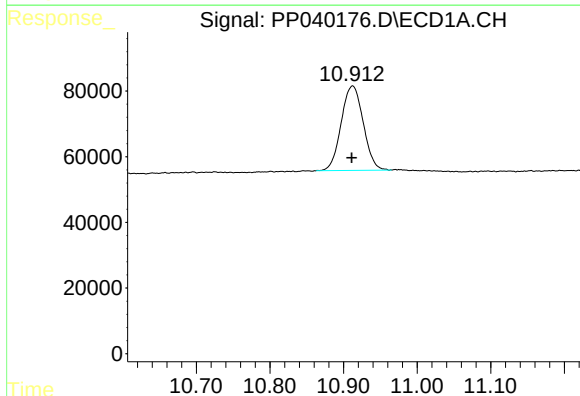


#2 Decachlorobiphenyl

R.T.: 10.912 min
Delta R.T.: 0.000 min
Response: 534879
Conc: 21.64 ng/ml

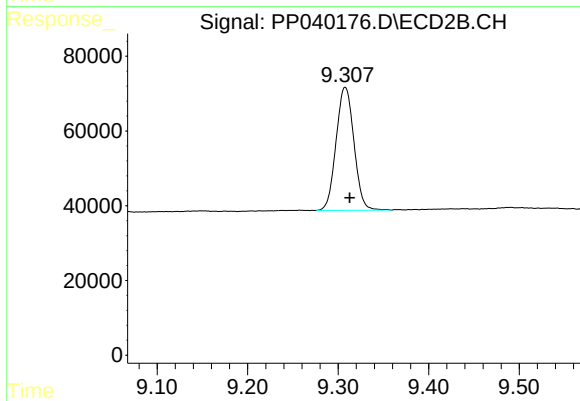

#2 Decachlorobiphenyl


R.T.: 9.308 min
Delta R.T.: -0.005 min
Response: 451639
Conc: 21.28 ng/ml

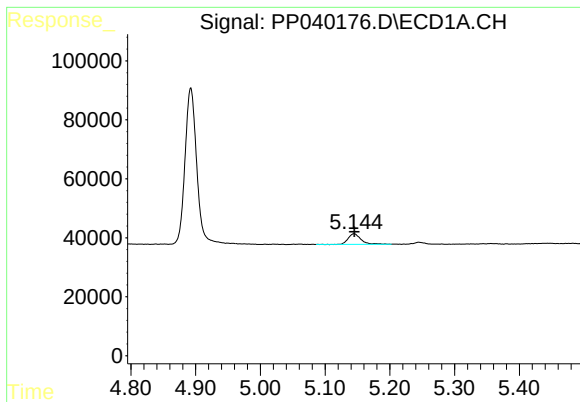

#8 AR-1221-1

R.T.: 5.145 min
Delta R.T.: 0.000 min
Response: 48247
Conc: 138.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-1-BD

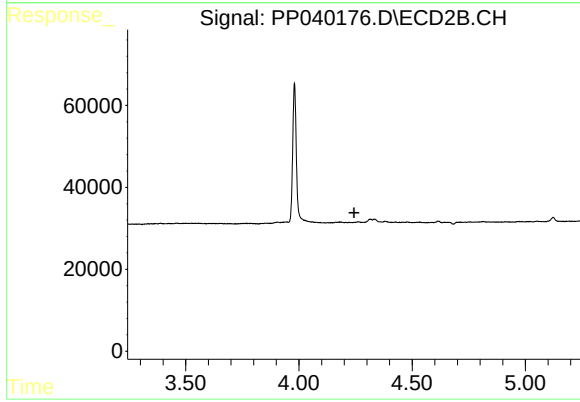

#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.243 min
Response: 0
Conc: N.D.