

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101821\
 Data File : PP040183.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2021 2:03
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 02:13:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.893	3.981	695973	395171	22.918	23.375
2)	SA Decachlor...	10.912	9.307	603052	528657	24.399	24.910
Target Compounds							
10)	L2 AR-1221-3	0.000	4.420	0	8381	N.D.	15.477 #
11)	L3 AR-1232-1	0.000	4.420	0	8381	N.D.	20.636 #
20)	L4 AR-1242-5	0.000	6.148f	0	13873	N.D.	29.086 #
25)	L5 AR-1248-5	0.000	6.148f	0	13873	N.D.	22.238 #
26)	L6 AR-1254-1	0.000	6.148f	0	13873	N.D.	14.481 #
28)	L6 AR-1254-3	7.759f	0.000	22982	0	16.132	N.D. #
32)	L7 AR-1260-2	8.194f	7.015f	38423	13944	28.112	11.776 #
33)	L7 AR-1260-3	0.000	7.188	0	10541	N.D.	8.922 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101821\
Data File : PP040183.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2021 2:03
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 02:13:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

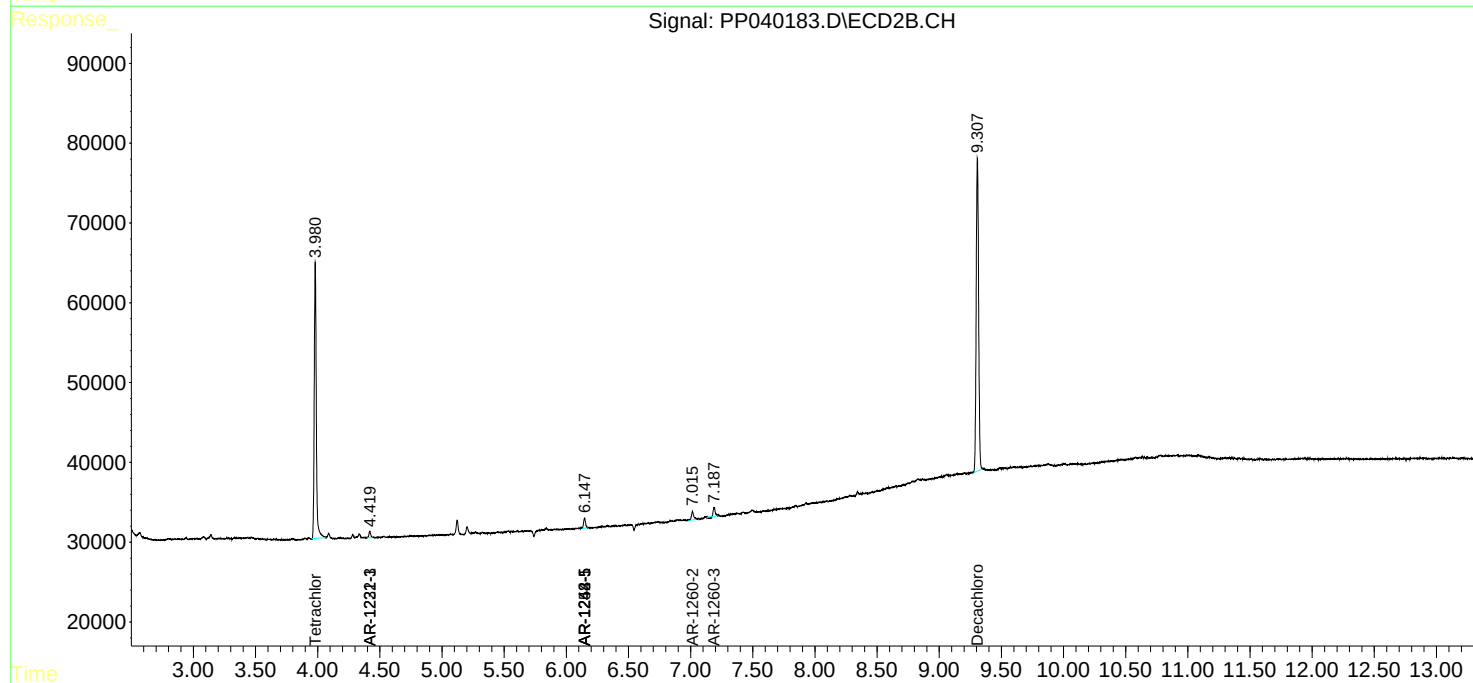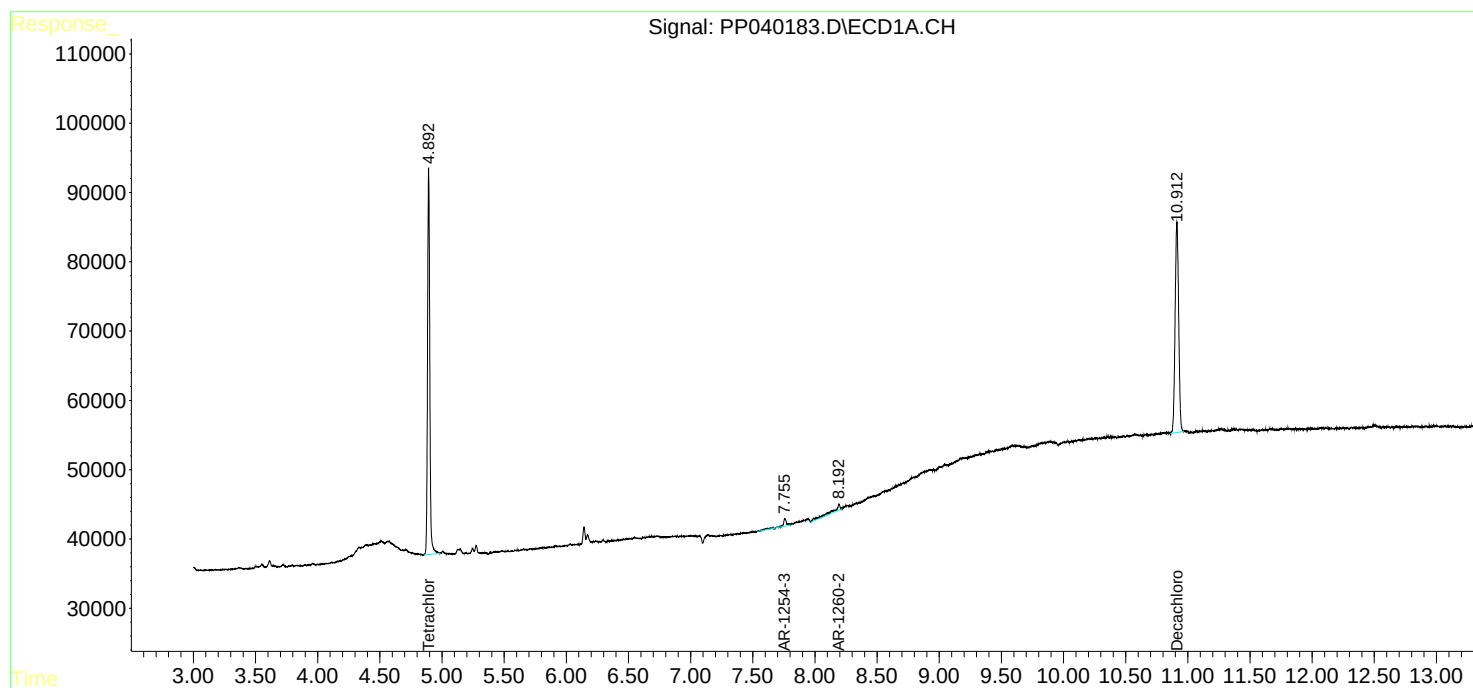


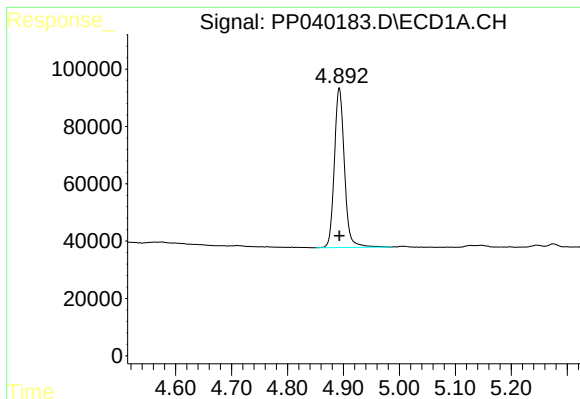

#1 Tetrachloro-m-xylene


R.T.: 4.893 min
Delta R.T.: 0.000 min
Response: 695973
Conc: 22.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

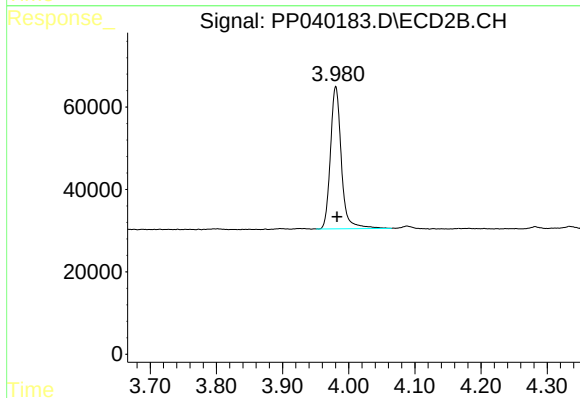


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: -0.002 min
Response: 395171
Conc: 23.37 ng/ml

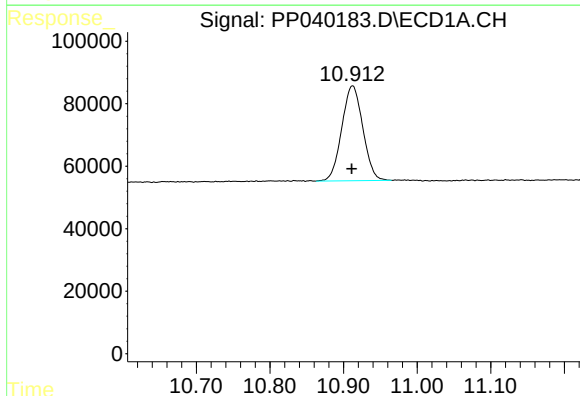


#2 Decachlorobiphenyl

R.T.: 10.912 min
Delta R.T.: 0.000 min
Response: 603052
Conc: 24.40 ng/ml

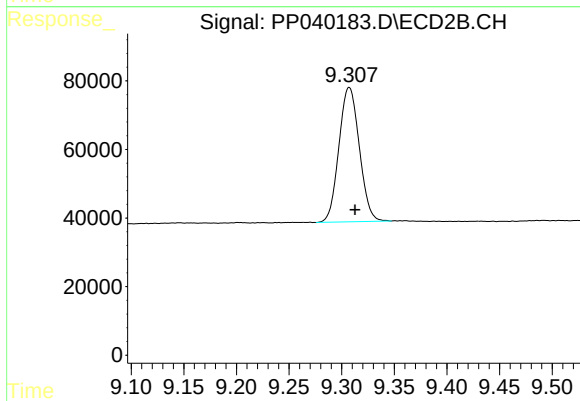

#2 Decachlorobiphenyl


R.T.: 9.307 min
Delta R.T.: -0.006 min
Response: 528657
Conc: 24.91 ng/ml

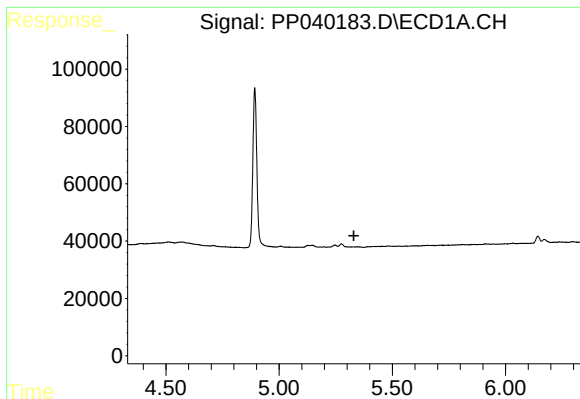

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 5.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

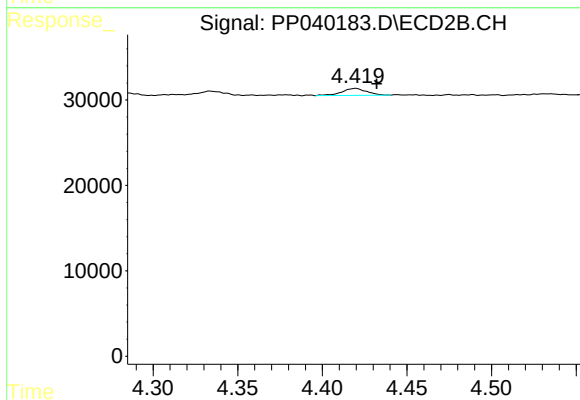


#10 AR-1221-3

R.T.: 4.420 min
Delta R.T.: -0.012 min
Response: 8381
Conc: 15.48 ng/ml

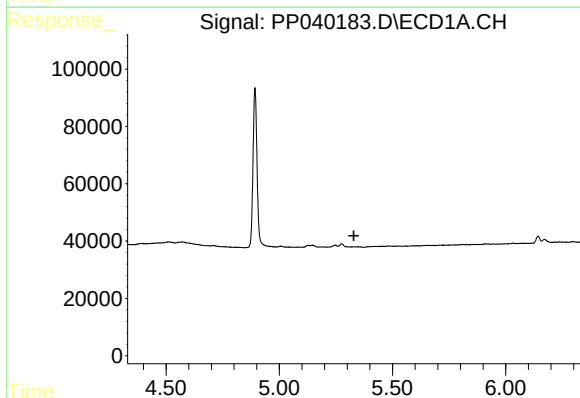


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 5.330 min
Response: 0
Conc: N.D.

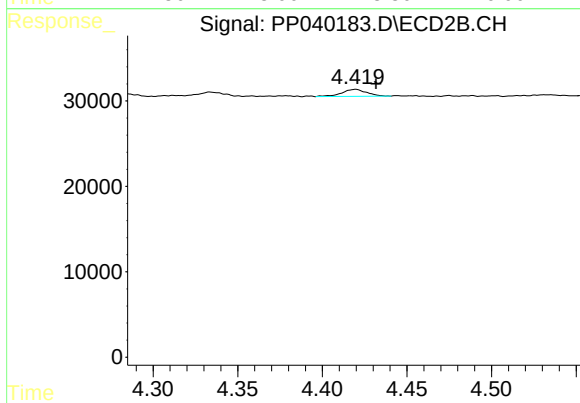

#11 AR-1232-1


R.T.: 4.420 min
Delta R.T.: -0.012 min
Response: 8381
Conc: 20.64 ng/ml

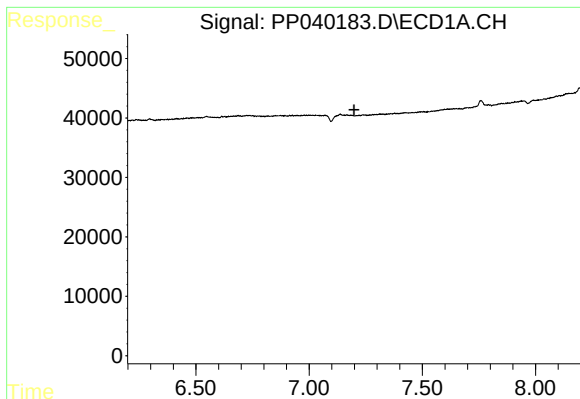

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.198 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

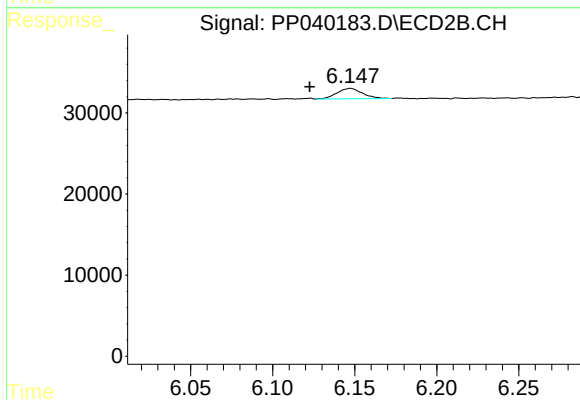


#20 AR-1242-5

R.T.: 6.148 min
Delta R.T.: 0.025 min
Response: 13873
Conc: 29.09 ng/ml

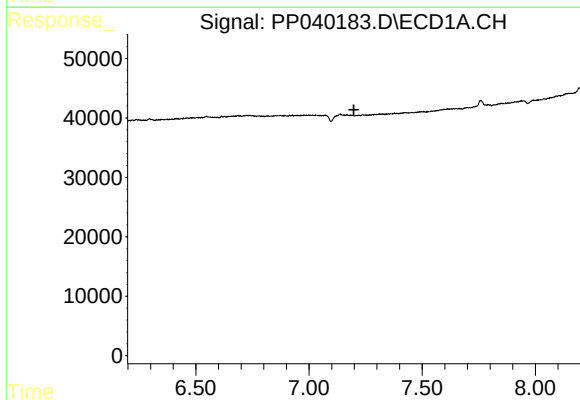


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 7.198 min
Response: 0
Conc: N.D.

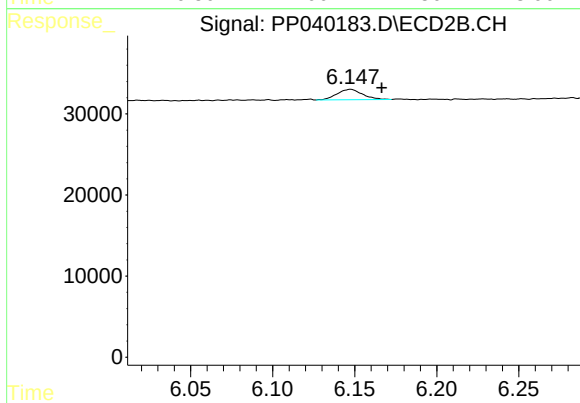

#25 AR-1248-5


R.T.: 6.148 min
Delta R.T.: -0.019 min
Response: 13873
Conc: 22.24 ng/ml

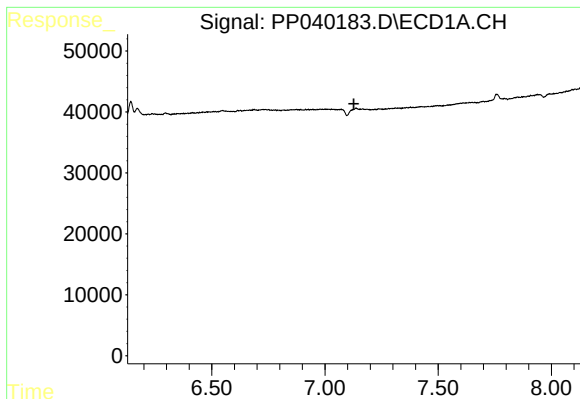

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 7.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

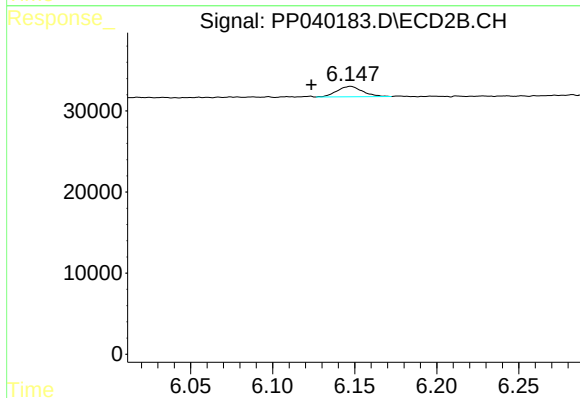


#26 AR-1254-1

R.T.: 6.148 min
Delta R.T.: 0.024 min
Response: 13873
Conc: 14.48 ng/ml

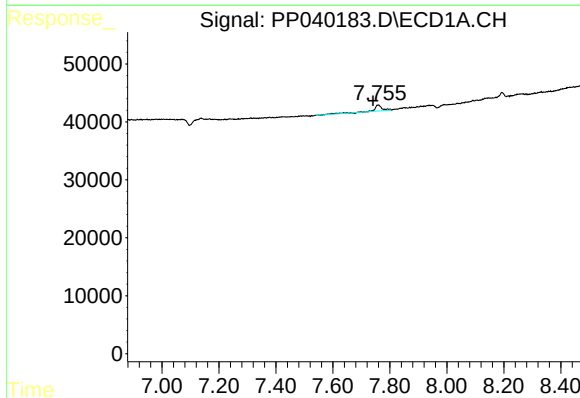


#28 AR-1254-3

R.T.: 7.759 min
Delta R.T.: 0.018 min
Response: 22982
Conc: 16.13 ng/ml

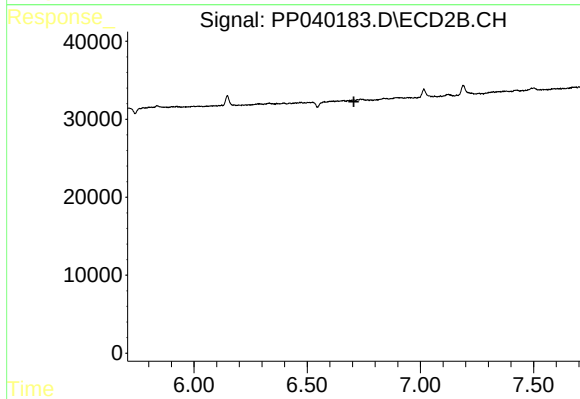

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.706 min
Response: 0
Conc: N.D.

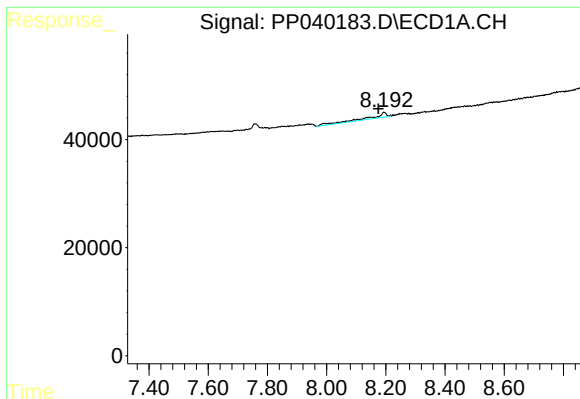

#32 AR-1260-2


R.T.: 8.194 min
Delta R.T.: 0.019 min
Response: 38423
Conc: 28.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

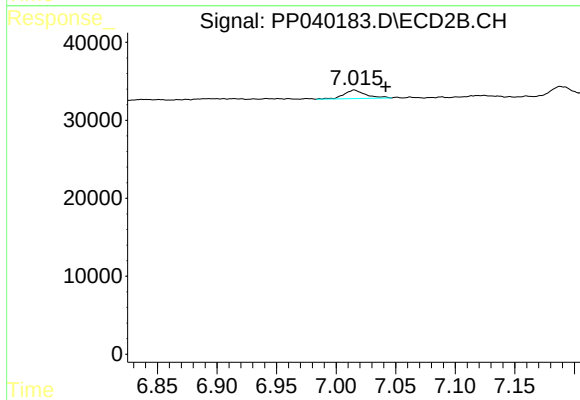


#32 AR-1260-2

R.T.: 7.015 min
Delta R.T.: -0.026 min
Response: 13944
Conc: 11.78 ng/ml

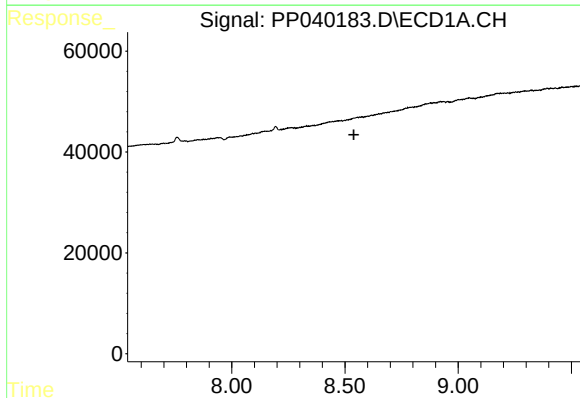

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.540 min
Response: 0
Conc: N.D.

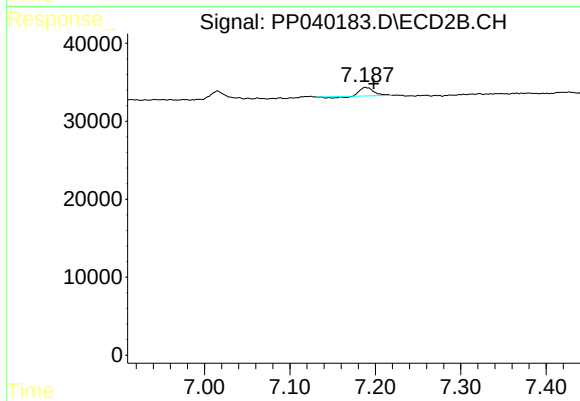

#33 AR-1260-3

R.T.: 7.188 min
Delta R.T.: -0.010 min
Response: 10541
Conc: 8.92 ng/ml