

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101821\
 Data File : PP040184.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2021 2:19
 Operator : AJ\MA
 Sample : M4261-02
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S-819-N-SO-1-1.5-093021-FD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 07:41:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.891	3.979	660089	380800	21.736	22.525
2)	SA Decachlor...	10.909	9.305	512865	457842	20.750	21.573

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101821\
Data File : PP040184.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2021 2:19
Operator : AJ\MA
Sample : M4261-02
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
S-819-N-SO-1-1.5-093021-FD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 07:41:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

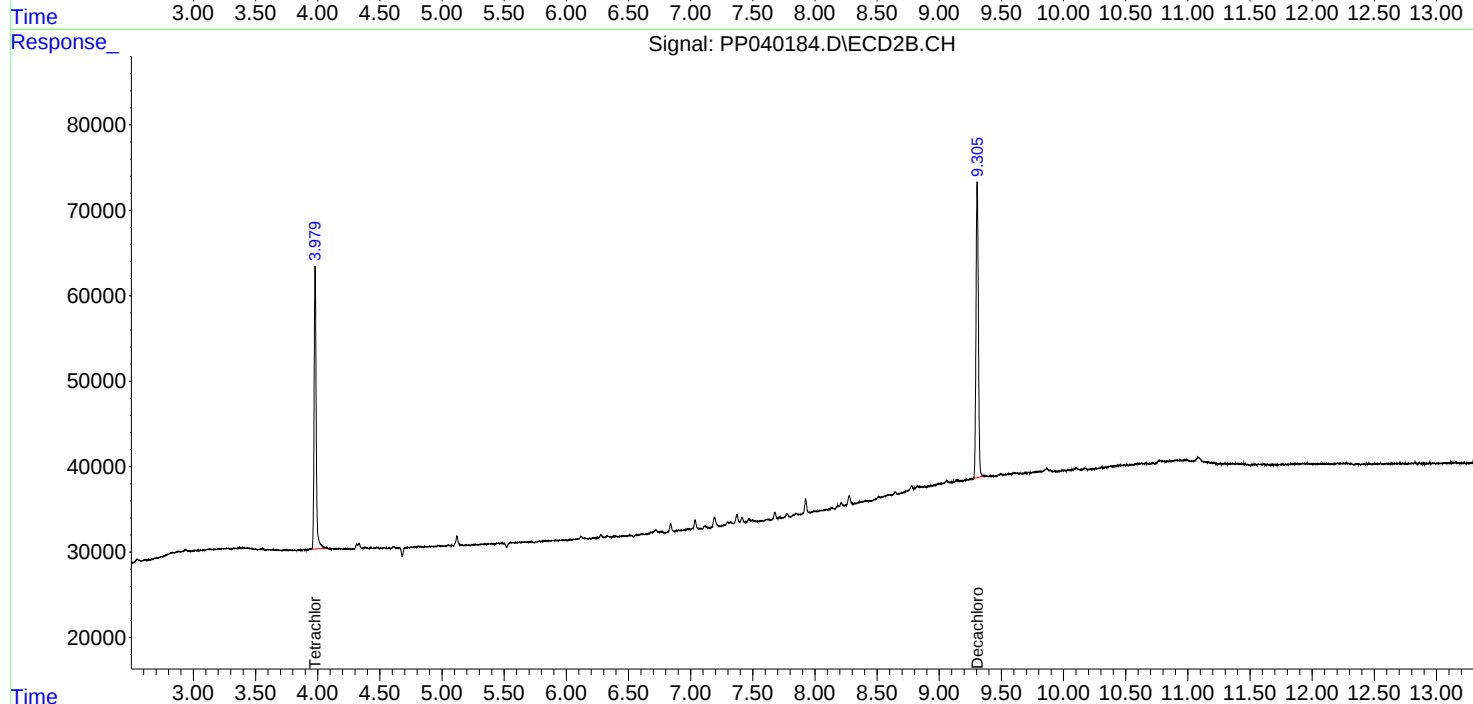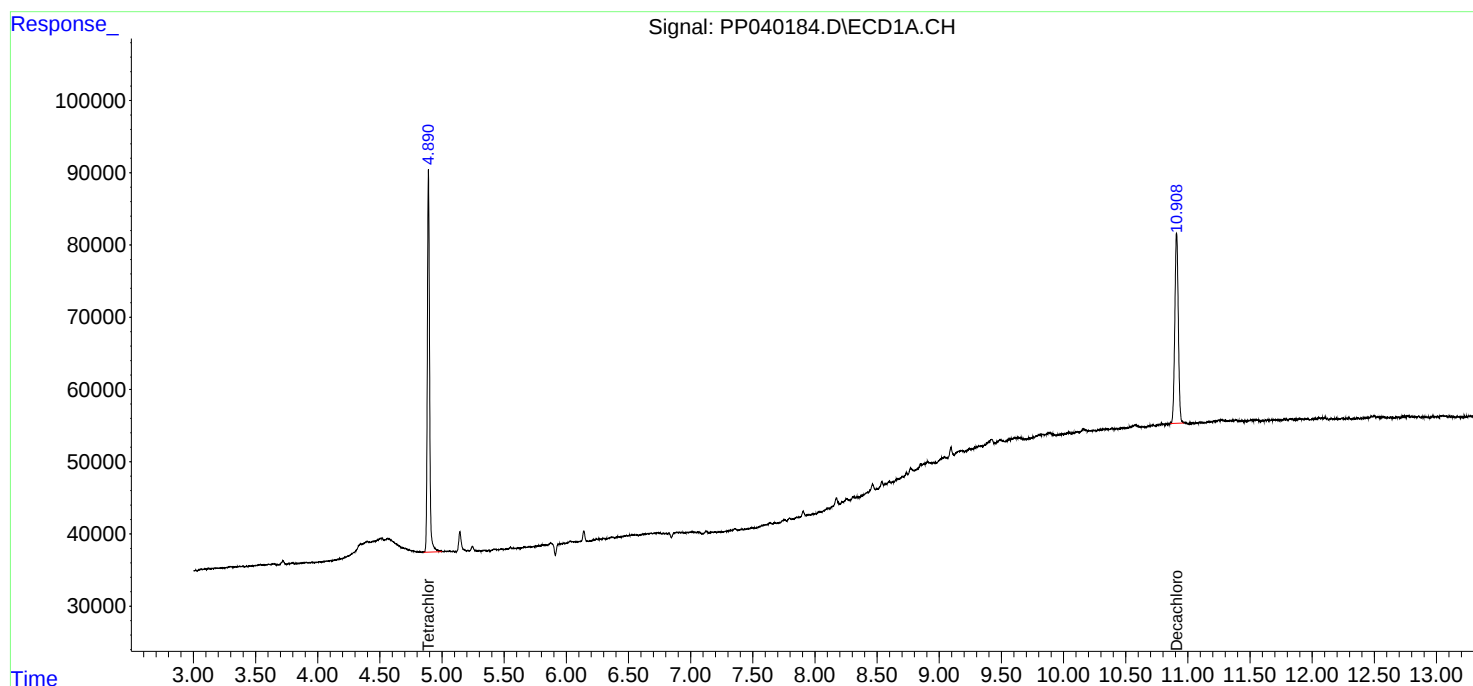


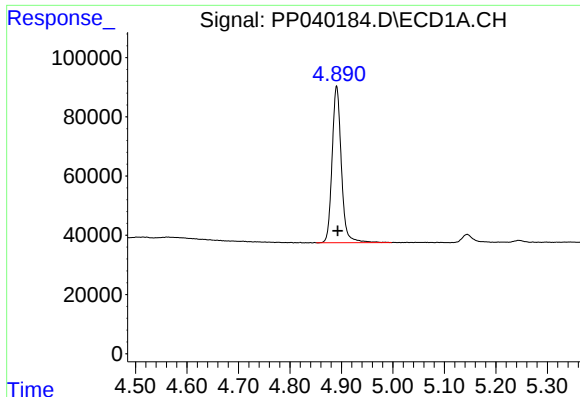

#1 Tetrachloro-m-xylene


R.T.: 4.891 min
Delta R.T.: -0.002 min
Response: 660089
Conc: 21.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
S-819-N-SO-1-1.5-093021-FD

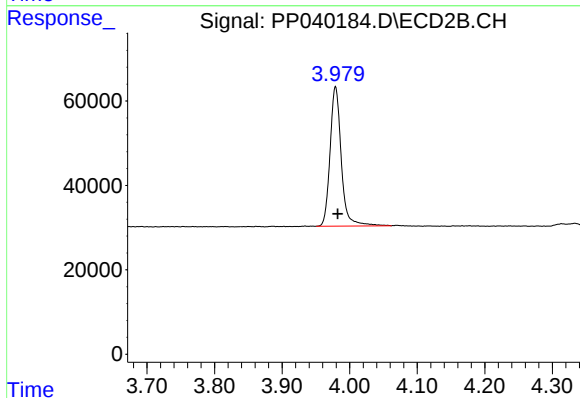


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.003 min
Response: 380800
Conc: 22.52 ng/ml

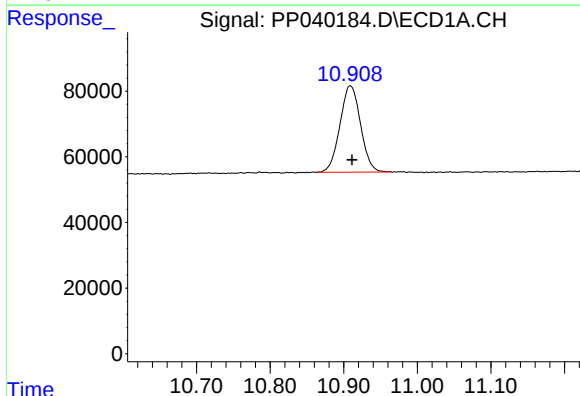

#2 Decachlorobiphenyl

R.T.: 10.909 min
Delta R.T.: -0.002 min
Response: 512865
Conc: 20.75 ng/ml

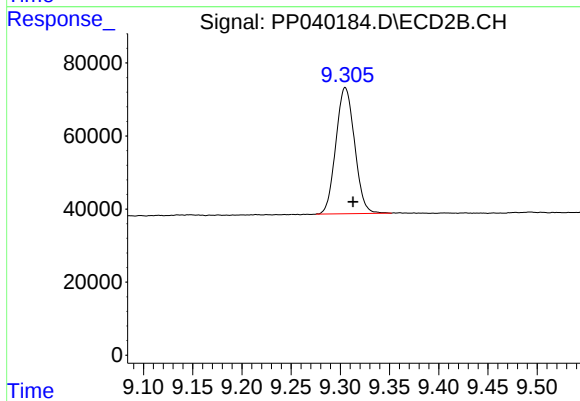

#2 Decachlorobiphenyl

R.T.: 9.305 min
Delta R.T.: -0.008 min
Response: 457842
Conc: 21.57 ng/ml