

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101821\
 Data File : PP040186.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2021 2:53
 Operator : AJ\MA
 Sample : M4261-04
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S-818-N-SO-3-3.5-100121

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 04:59:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.891	3.978	628019	352759	20.680	20.866
2)	SA Decachlor...	10.910	9.306	415788	378373	16.822	17.829

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101821\
Data File : PP040186.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2021 2:53
Operator : AJ\MA
Sample : M4261-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
S-818-N-SO-3-3.5-100121

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 04:59:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

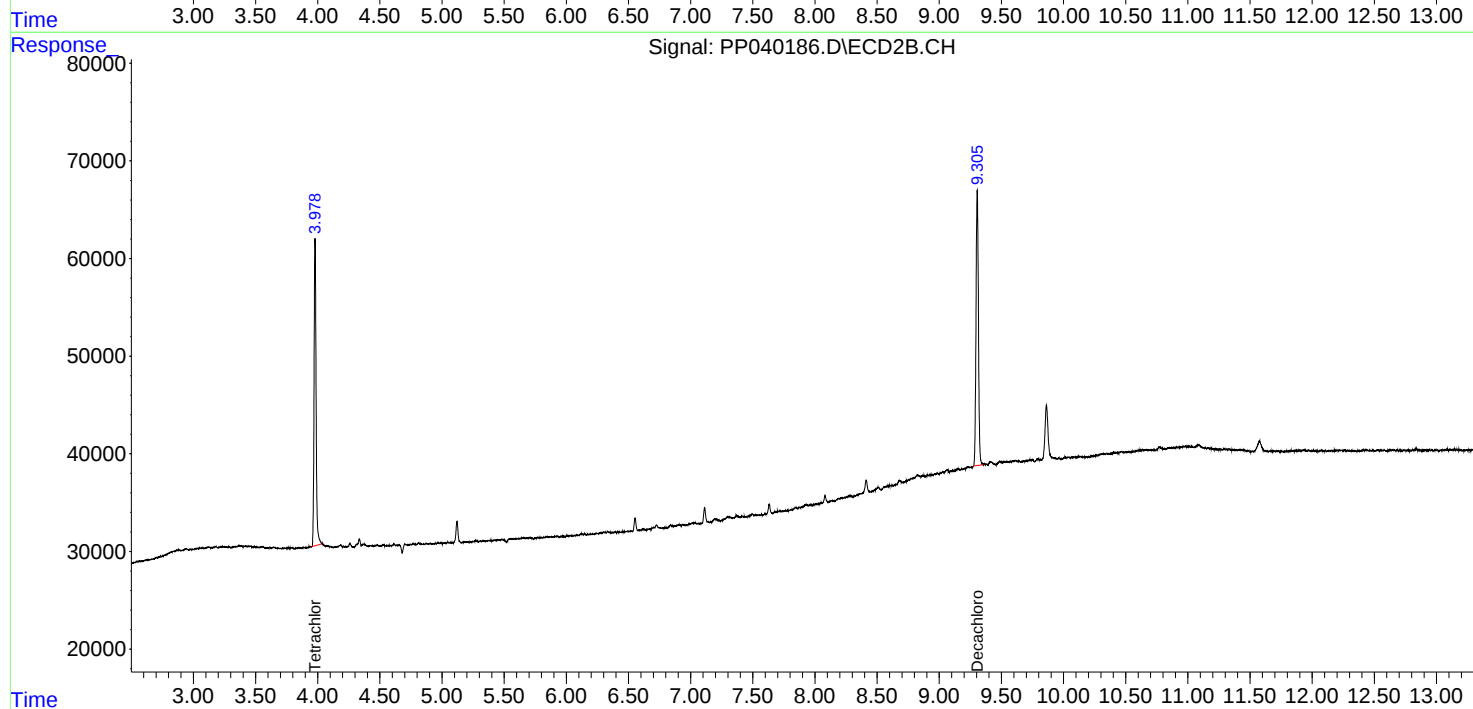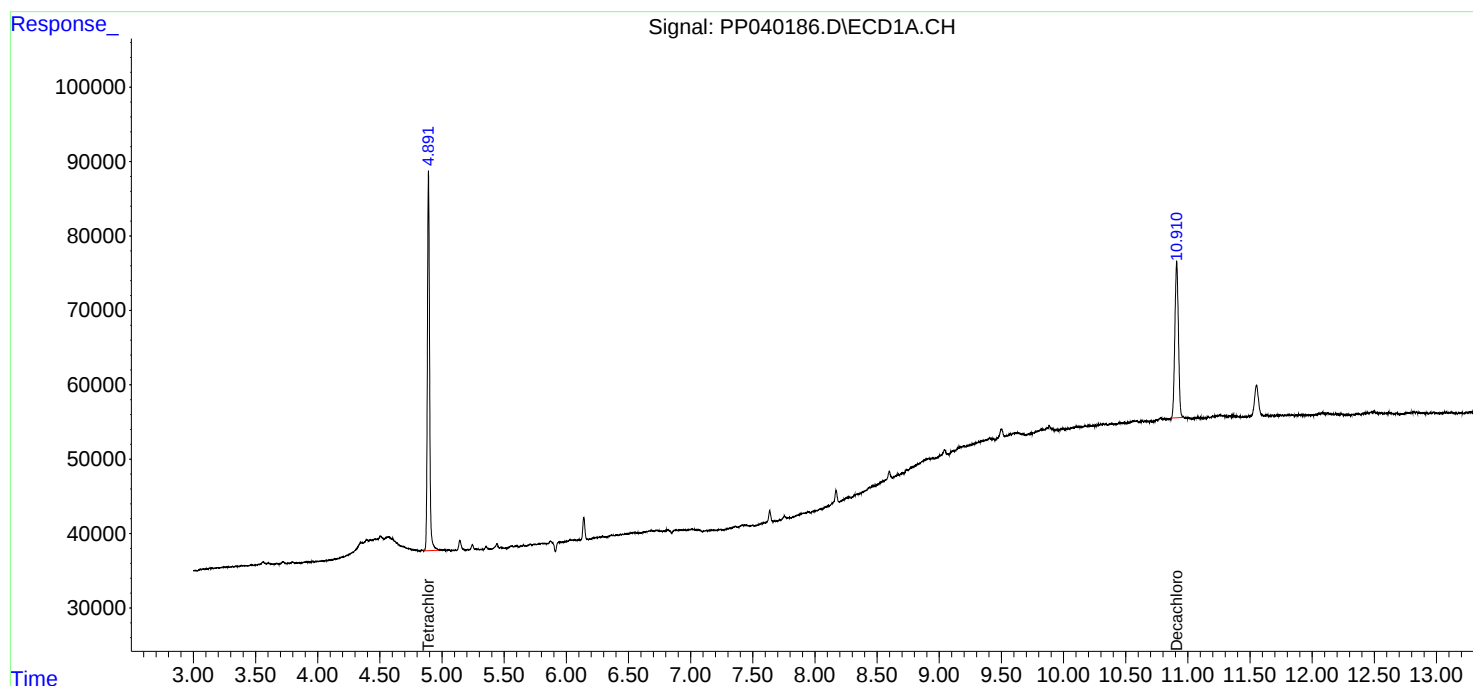


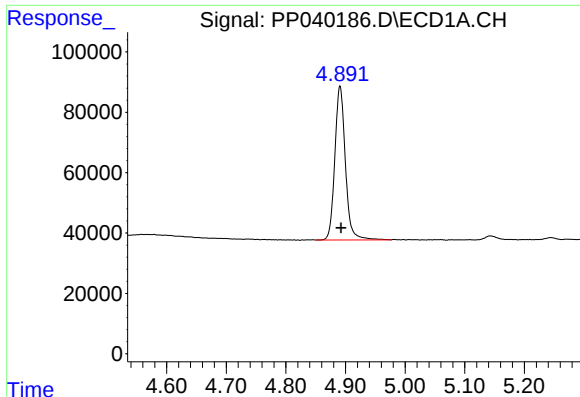

#1 Tetrachloro-m-xylene


R.T.: 4.891 min
Delta R.T.: -0.002 min
Response: 628019
Conc: 20.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
S-818-N-SO-3-3.5-100121

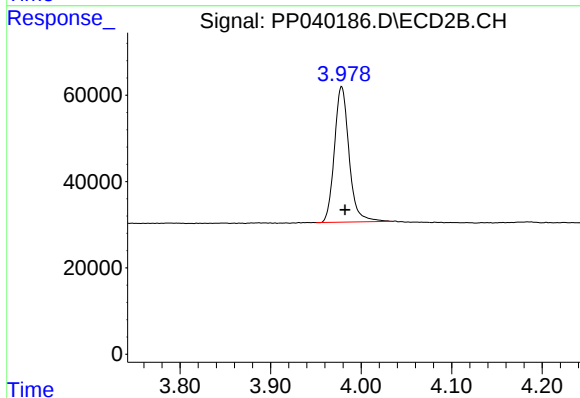


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.004 min
Response: 352759
Conc: 20.87 ng/ml

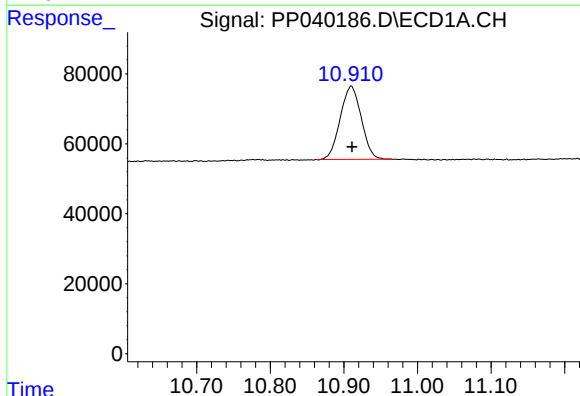

#2 Decachlorobiphenyl

R.T.: 10.910 min
Delta R.T.: -0.001 min
Response: 415788
Conc: 16.82 ng/ml

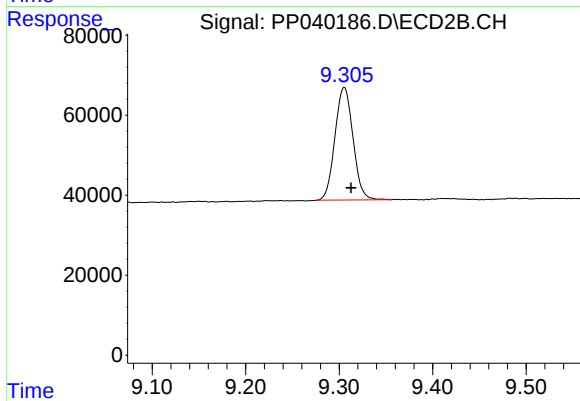

#2 Decachlorobiphenyl

R.T.: 9.306 min
Delta R.T.: -0.007 min
Response: 378373
Conc: 17.83 ng/ml