

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101822\
 Data File : PP052455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2022 03:08
 Operator : YP\AJ
 Sample : N5170-10
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP-TRE-1662-1667

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 04:59:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 12 05:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.420	3.671	13847085	10854824	8.809	9.475
2) SA Decachlor...	10.240	8.764	13826236	9334504	9.962	8.354

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101822\
Data File : PP052455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2022 03:08
Operator : YP\AJ
Sample : N5170-10
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
COMP-TRE-1662-1667

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 04:59:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

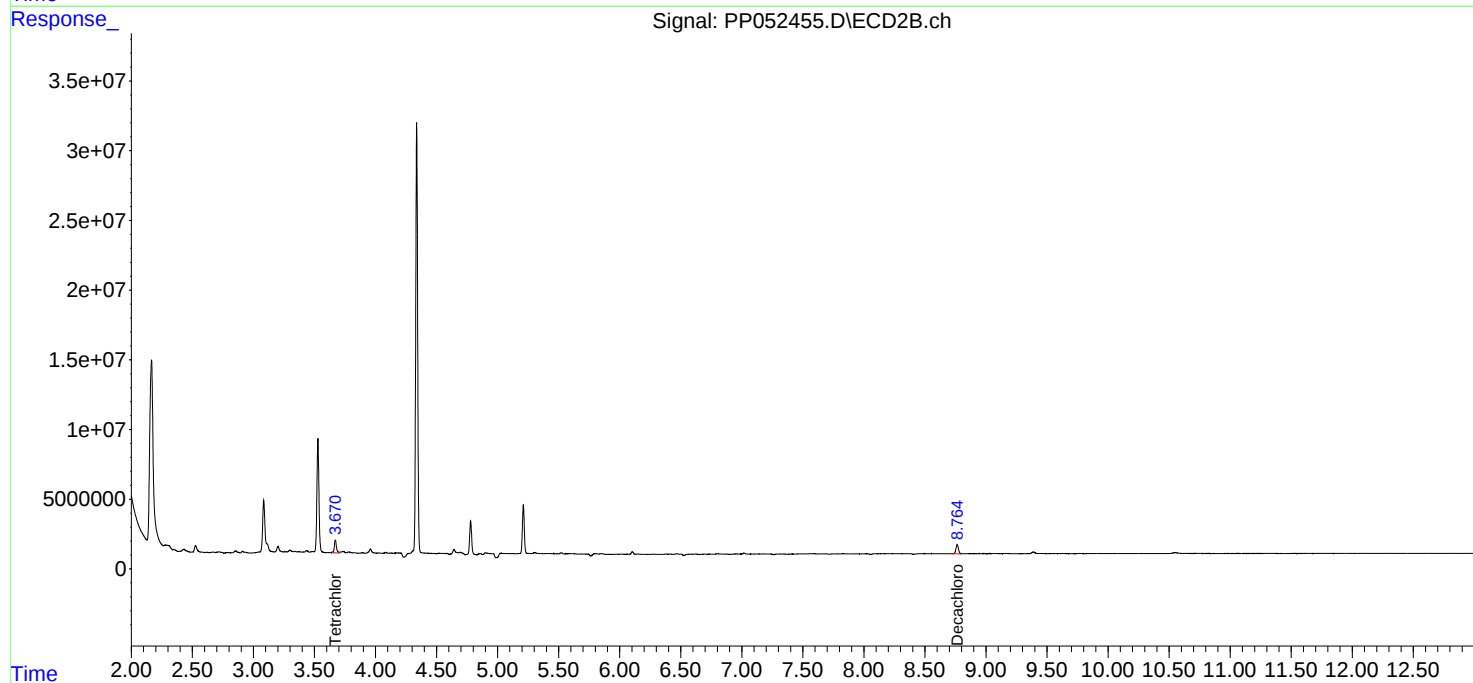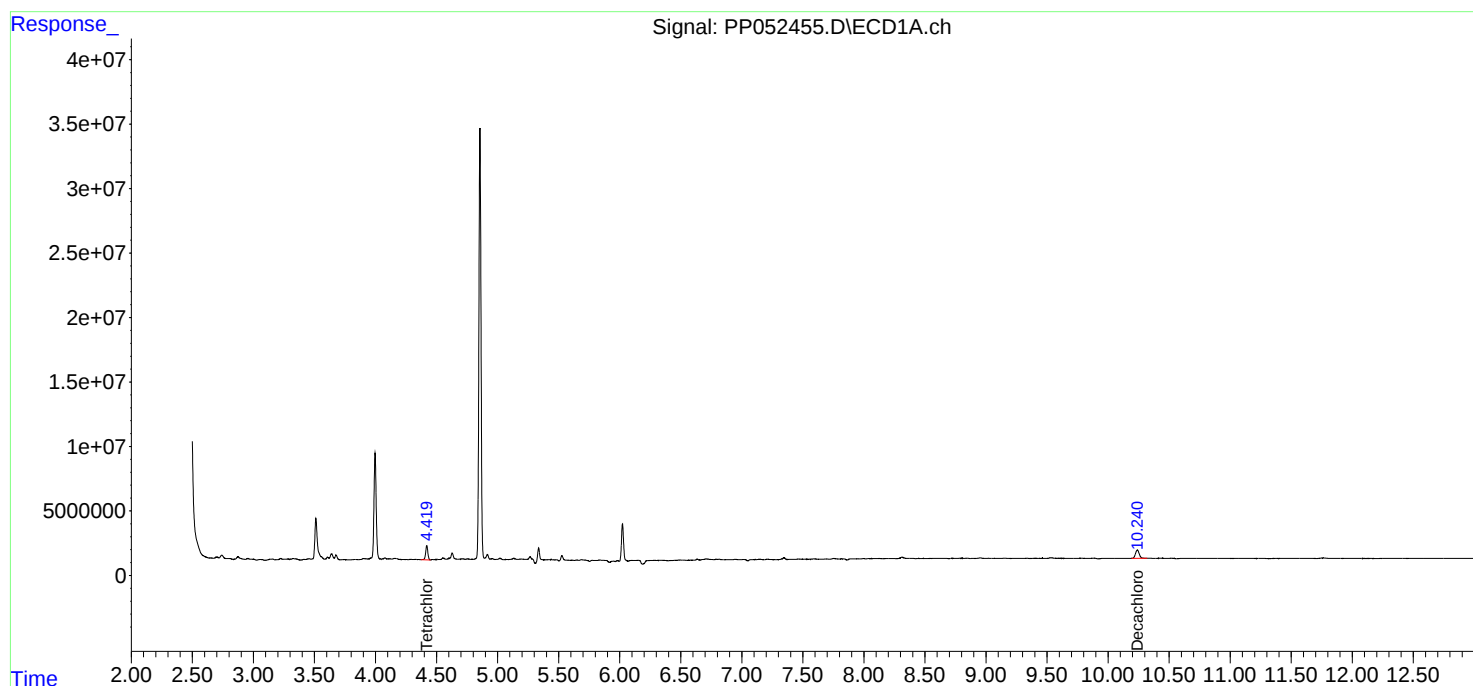


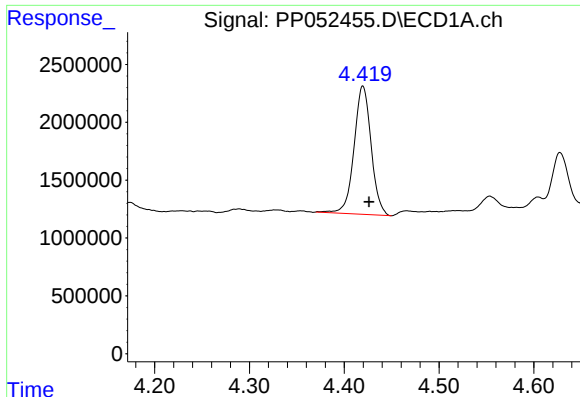

#1 Tetrachloro-m-xylene


R.T.: 4.420 min
Delta R.T.: -0.006 min
Response: 13847085
Conc: 8.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-TRE-1662-1667

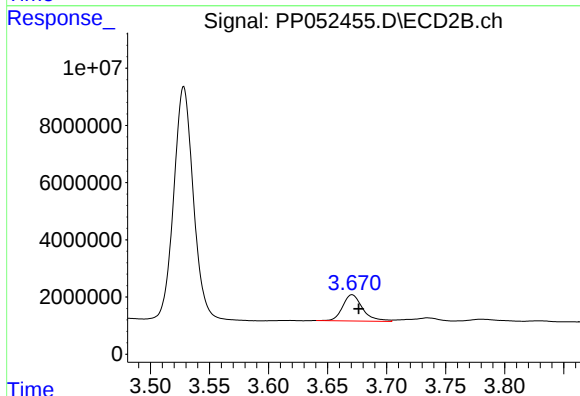


#1 Tetrachloro-m-xylene

R.T.: 3.671 min
Delta R.T.: -0.006 min
Response: 10854824
Conc: 9.47 ng/ml

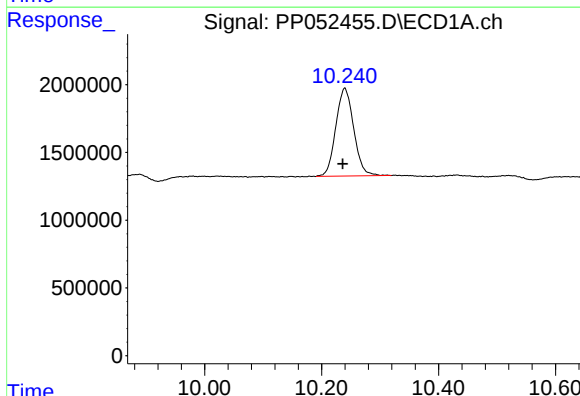

#2 Decachlorobiphenyl

R.T.: 10.240 min
Delta R.T.: 0.003 min
Response: 13826236
Conc: 9.96 ng/ml

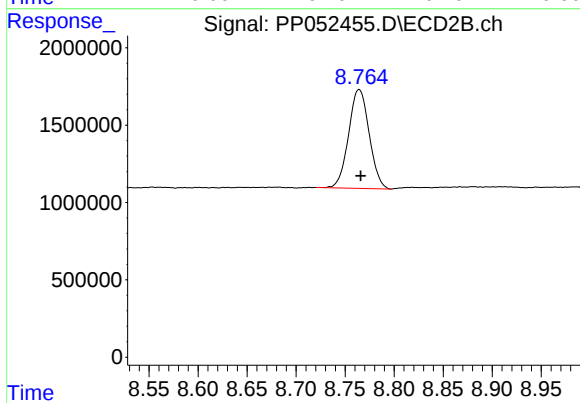

#2 Decachlorobiphenyl

R.T.: 8.764 min
Delta R.T.: -0.002 min
Response: 9334504
Conc: 8.35 ng/ml