

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101823\
 Data File : PP061079.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2023 05:37
 Operator : YP\AJ
 Sample : 04923-06 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 06:20:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 14 13:32:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.551	3.687	3389617	2714448	1.542	2.008 #
2)	SA Decachlor...	10.512	8.755	4006947	2528503	2.559	1.682 #
Target Compounds							
9)	L2 AR-1221-2	4.864	0.000	478546	0	23.041	N.D. #
28)	L6 AR-1254-3	7.210	0.000	1136581	0	9.290	N.D. #
29)	L6 AR-1254-4	7.489	0.000	655594	0	7.448	N.D. #
30)	L6 AR-1254-5	7.915	0.000	730751	0	7.359	N.D. #
31)	L7 AR-1260-1	7.373	0.000	39910	0	0.426	N.D. #
33)	L7 AR-1260-3	7.990	0.000	382536	0	5.504	N.D. #
36)	L8 AR-1262-1	7.990	0.000	382536	0	3.046	N.D. #
39)	L8 AR-1262-4	8.987	0.000	283481	0	2.506	N.D. #
42)	L9 AR-1268-2	8.987	0.000	283481	0	1.209	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101823\
Data File : PP061079.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2023 05:37
Operator : YP\AJ
Sample : 04923-06 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 06:20:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 14 13:32:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

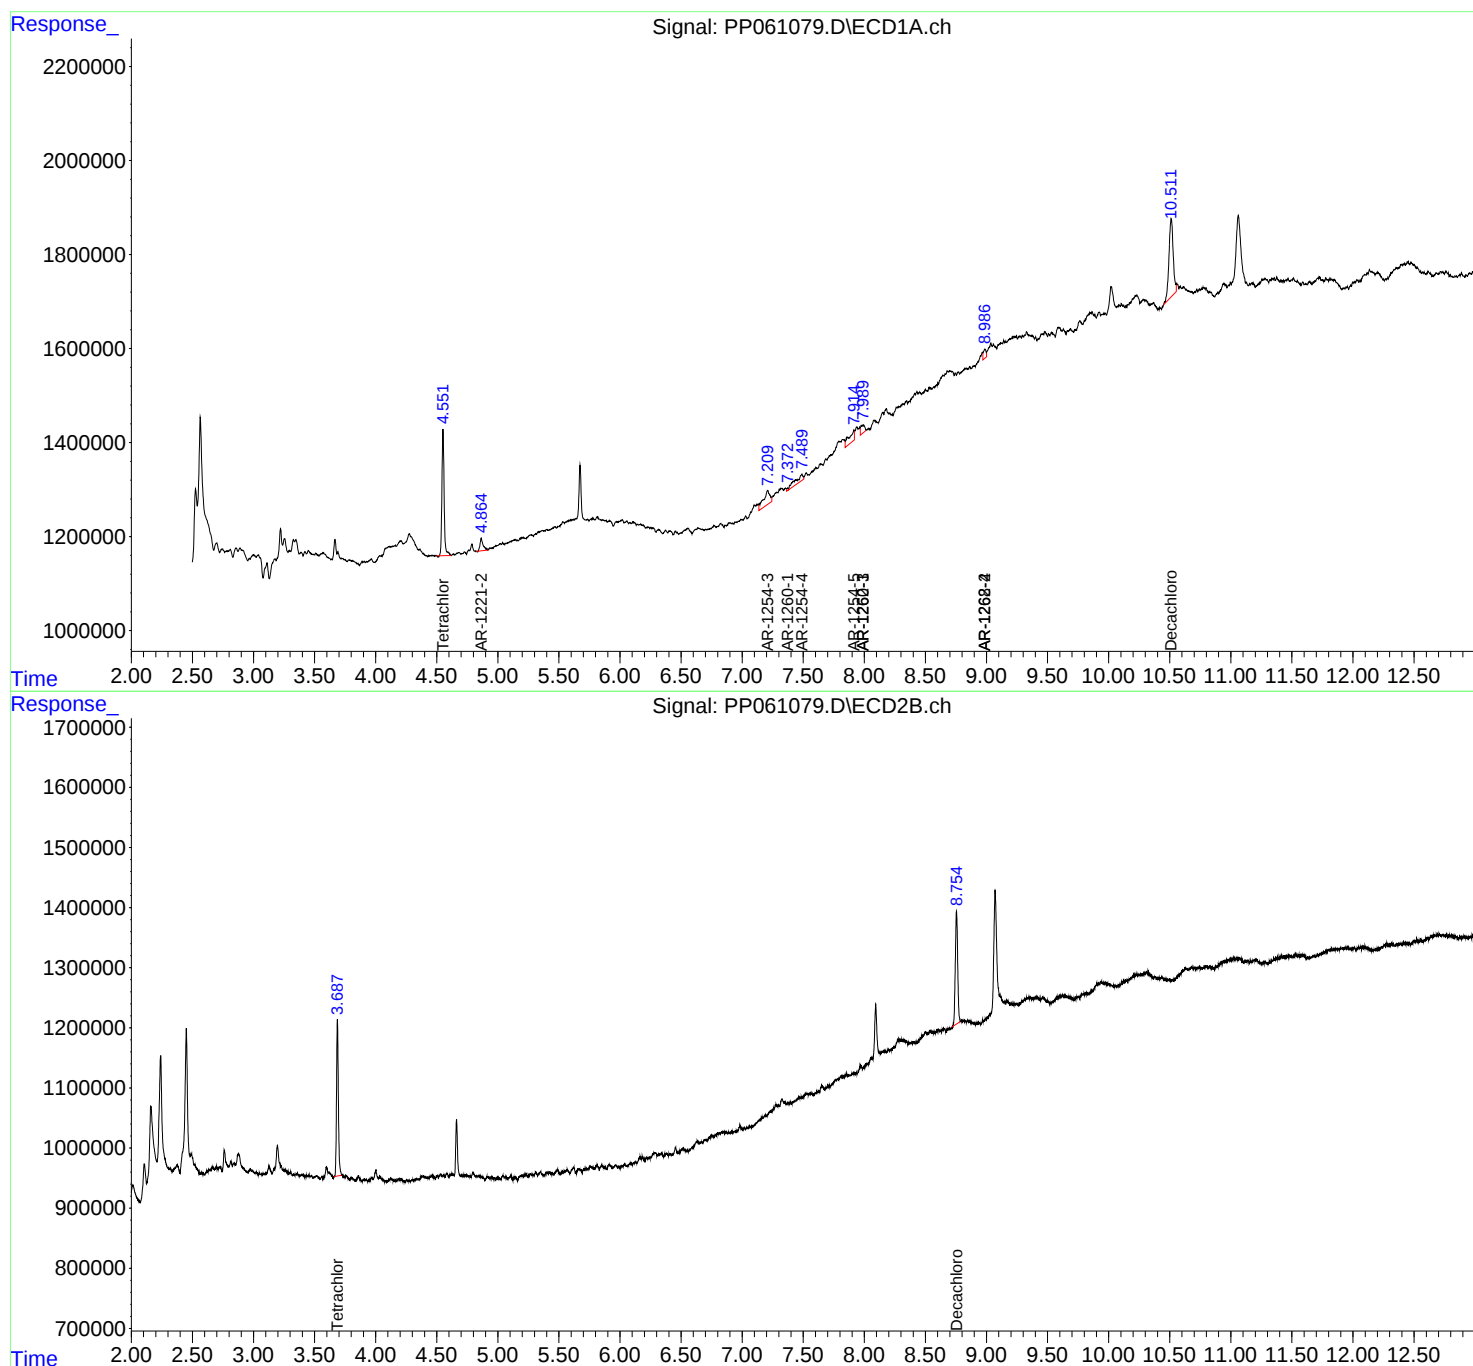


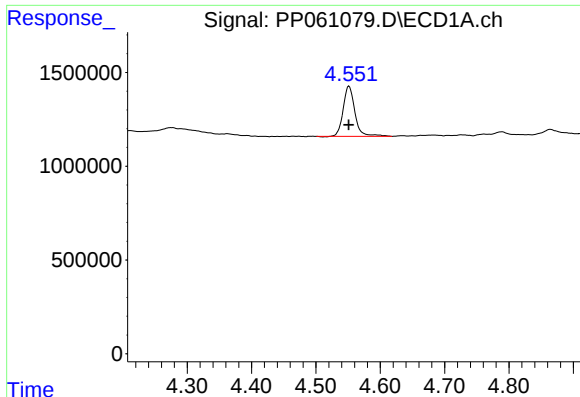

#1 Tetrachloro-m-xylene


R.T.: 4.551 min
Delta R.T.: 0.000 min
Response: 3389617
Conc: 1.54 ng/ml

Instrument :
ECD_P
ClientSampleId :

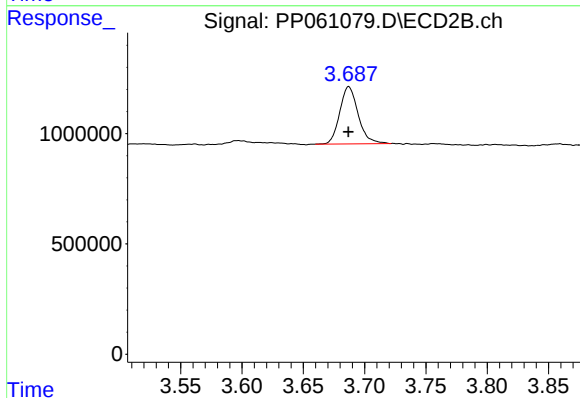


#1 Tetrachloro-m-xylene

R.T.: 3.687 min
Delta R.T.: 0.000 min
Response: 2714448
Conc: 2.01 ng/ml

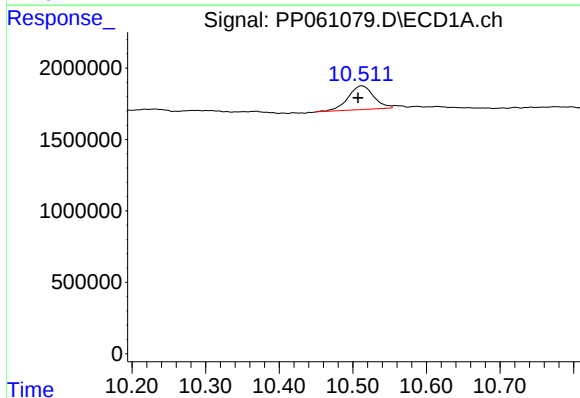


#2 Decachlorobiphenyl

R.T.: 10.512 min
Delta R.T.: 0.005 min
Response: 4006947
Conc: 2.56 ng/ml

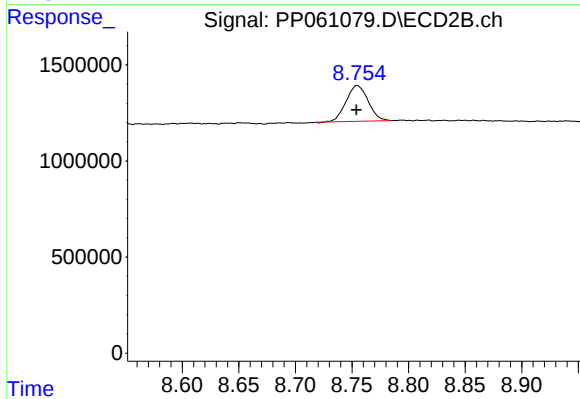

#2 Decachlorobiphenyl


R.T.: 8.755 min
Delta R.T.: 0.000 min
Response: 2528503
Conc: 1.68 ng/ml

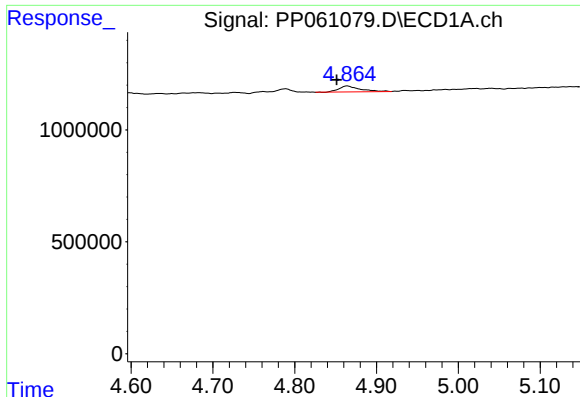

#9 AR-1221-2


R.T.: 4.864 min
Delta R.T.: 0.013 min
Response: 478546
Conc: 23.04 ng/ml

Instrument :
ECD_P
ClientSampleId :

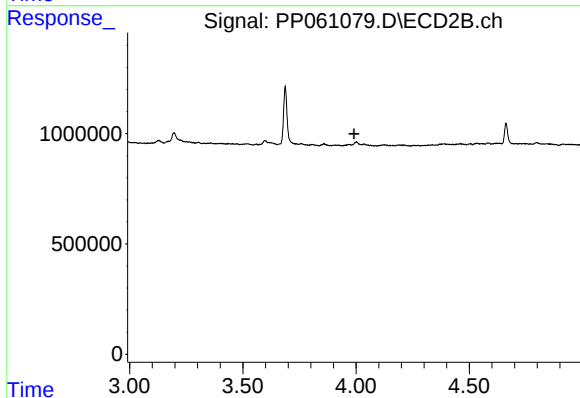


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.991 min
Response: 0
Conc: N.D.

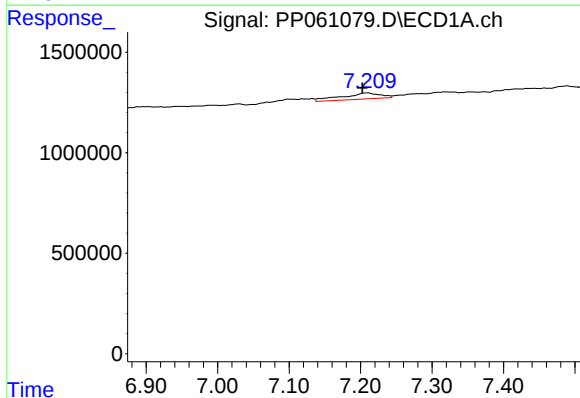


#28 AR-1254-3

R.T.: 7.210 min
Delta R.T.: 0.007 min
Response: 1136581
Conc: 9.29 ng/ml

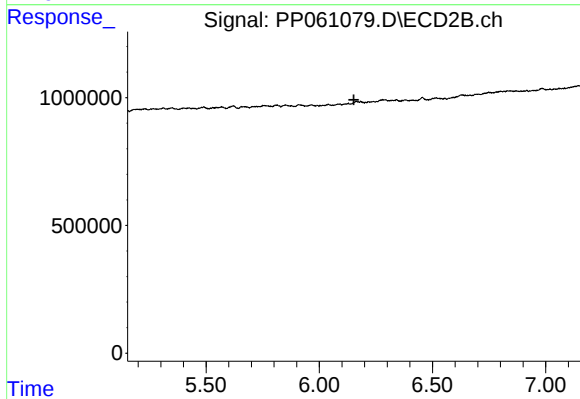

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.153 min
Response: 0
Conc: N.D.

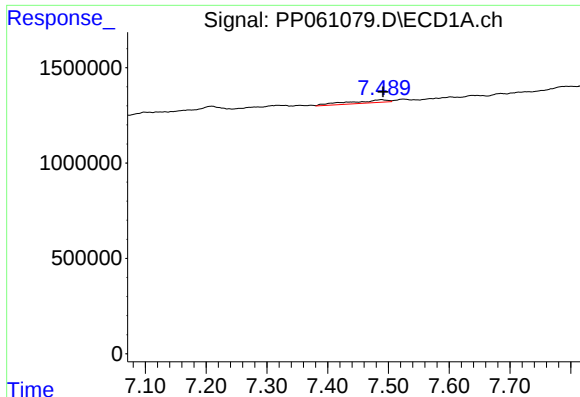

#29 AR-1254-4


R.T.: 7.489 min
Delta R.T.: -0.002 min
Response: 655594
Conc: 7.45 ng/ml

Instrument :
ECD_P
ClientSampleId :

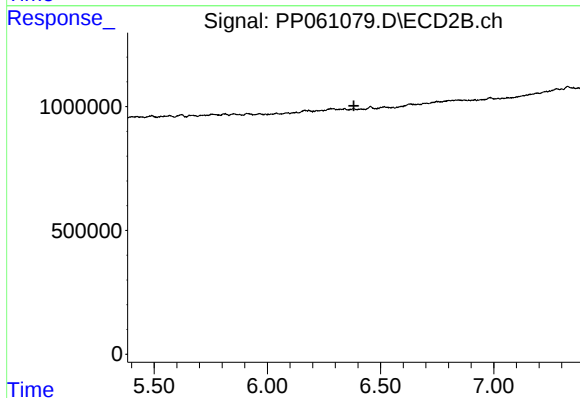


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.382 min
Response: 0
Conc: N.D.

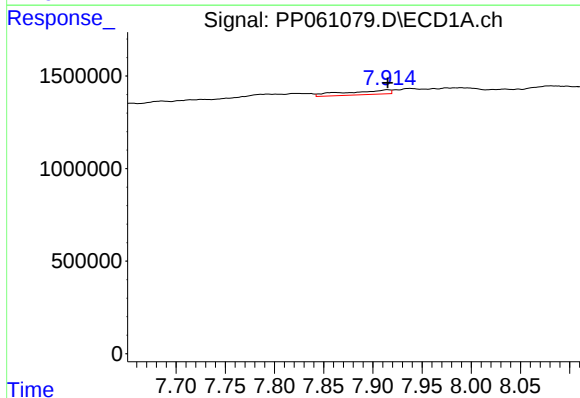


#30 AR-1254-5

R.T.: 7.915 min
Delta R.T.: 0.000 min
Response: 730751
Conc: 7.36 ng/ml

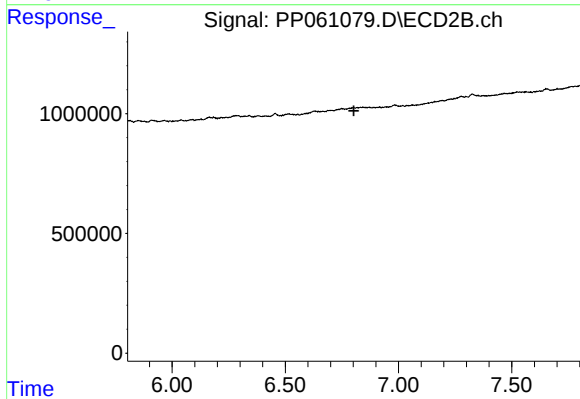

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.803 min
Response: 0
Conc: N.D.

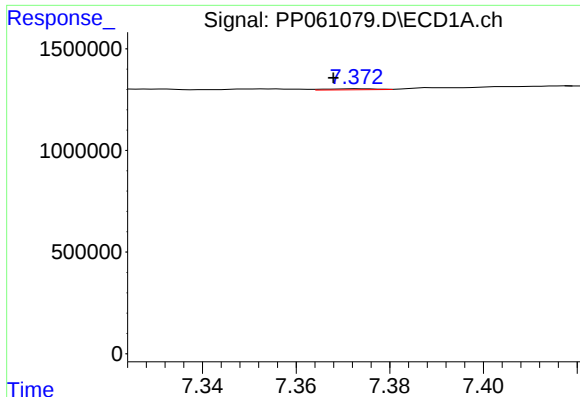

#31 AR-1260-1


R.T.: 7.373 min
Delta R.T.: 0.005 min
Response: 39910
Conc: 0.43 ng/ml

Instrument :
ECD_P
ClientSampleId :

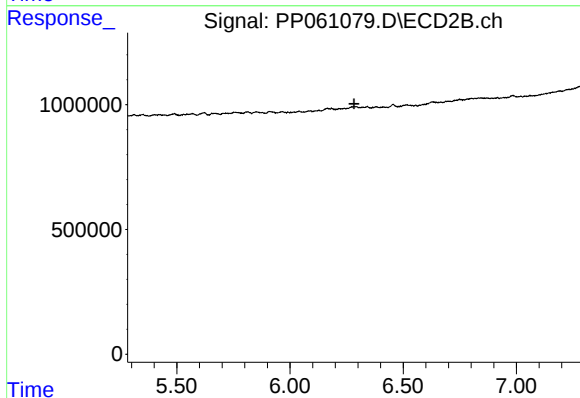


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.282 min
Response: 0
Conc: N.D.

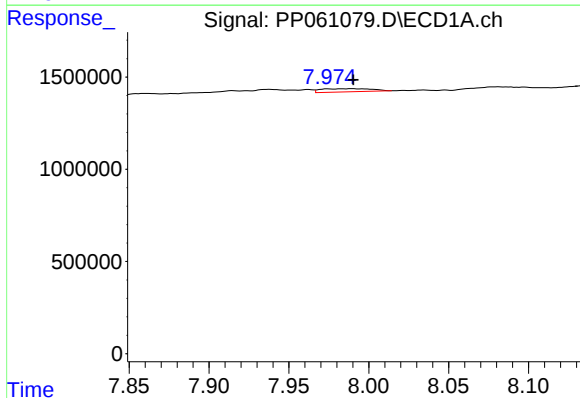


#33 AR-1260-3

R.T.: 7.990 min
Delta R.T.: 0.000 min
Response: 382536
Conc: 5.50 ng/ml

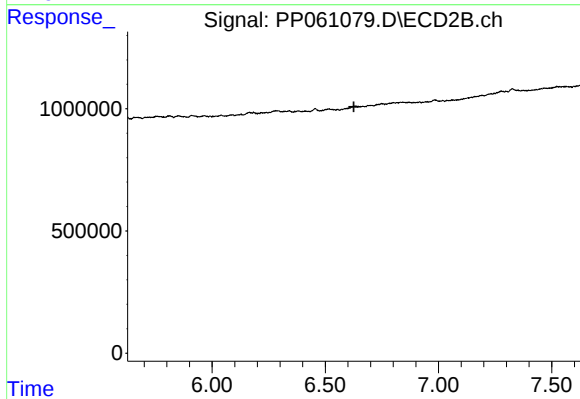

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 6.626 min
Response: 0
Conc: N.D.

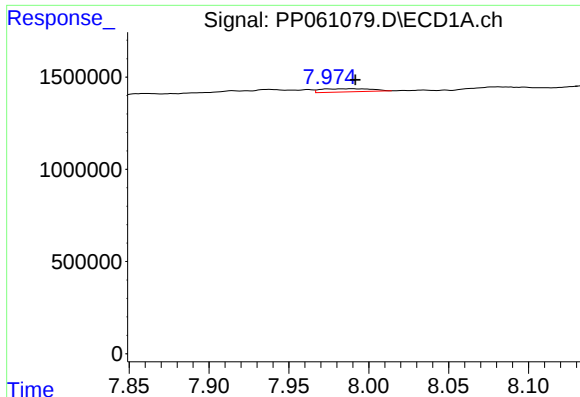

#36 AR-1262-1


R.T.: 7.990 min
Delta R.T.: -0.002 min
Response: 382536
Conc: 3.05 ng/ml

Instrument :
ECD_P
ClientSampleId :

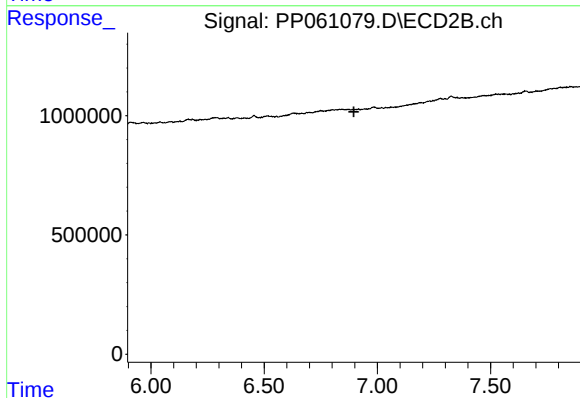


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 6.896 min
Response: 0
Conc: N.D.

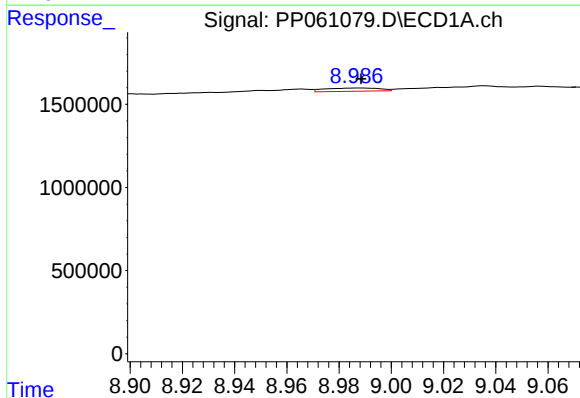


#39 AR-1262-4

R.T.: 8.987 min
Delta R.T.: -0.001 min
Response: 283481
Conc: 2.51 ng/ml

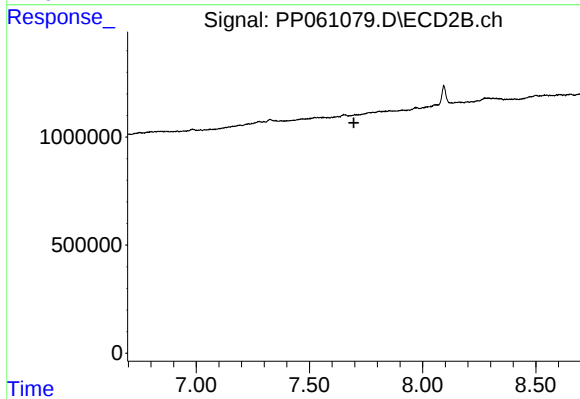

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 7.696 min
Response: 0
Conc: N.D.

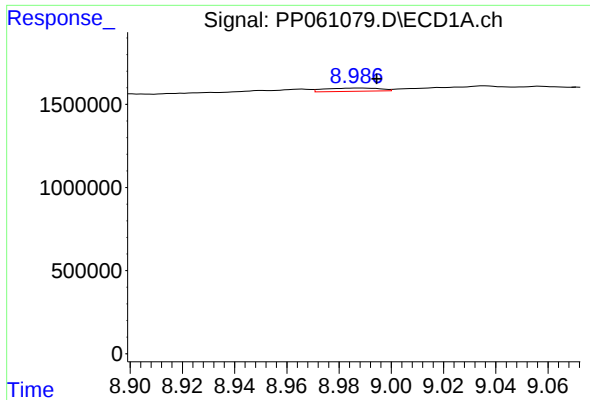

#42 AR-1268-2

R.T.: 8.987 min
Delta R.T.: -0.007 min
Response: 283481
Conc: 1.21 ng/ml

Instrument :
ECD_P
ClientSampleId :

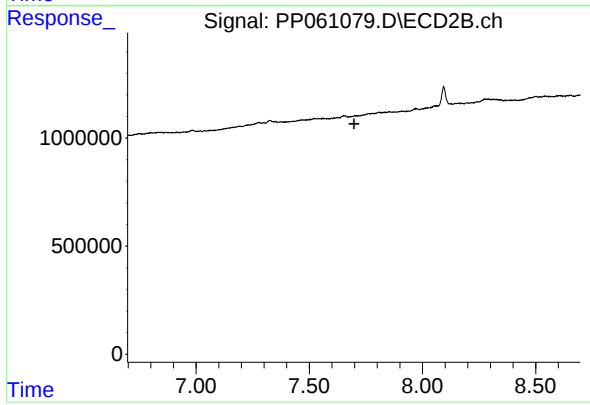

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.697 min
Response: 0
Conc: N.D.