

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP101823\  
 Data File : PP061029.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Oct 2023 13:59  
 Operator : YP\AJ  
 Sample : 04924-01  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 50129

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 18 15:04:17 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP101323.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Sat Oct 14 13:32:01 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound        | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|--------|-------|----------|----------|--------|--------|
| -----                       |                 |        |       |          |          |        |        |
| System Monitoring Compounds |                 |        |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 4.550  | 3.686 | 51813376 | 31808072 | 23.569 | 23.527 |
| 2)                          | SA Decachlor... | 10.509 | 8.752 | 41247311 | 33561343 | 26.339 | 22.322 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP101823\  
Data File : PP061029.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 18 Oct 2023 13:59  
Operator : YP\AJ  
Sample : 04924-01  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
50129

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 18 15:04:17 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP101323.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Sat Oct 14 13:32:01 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

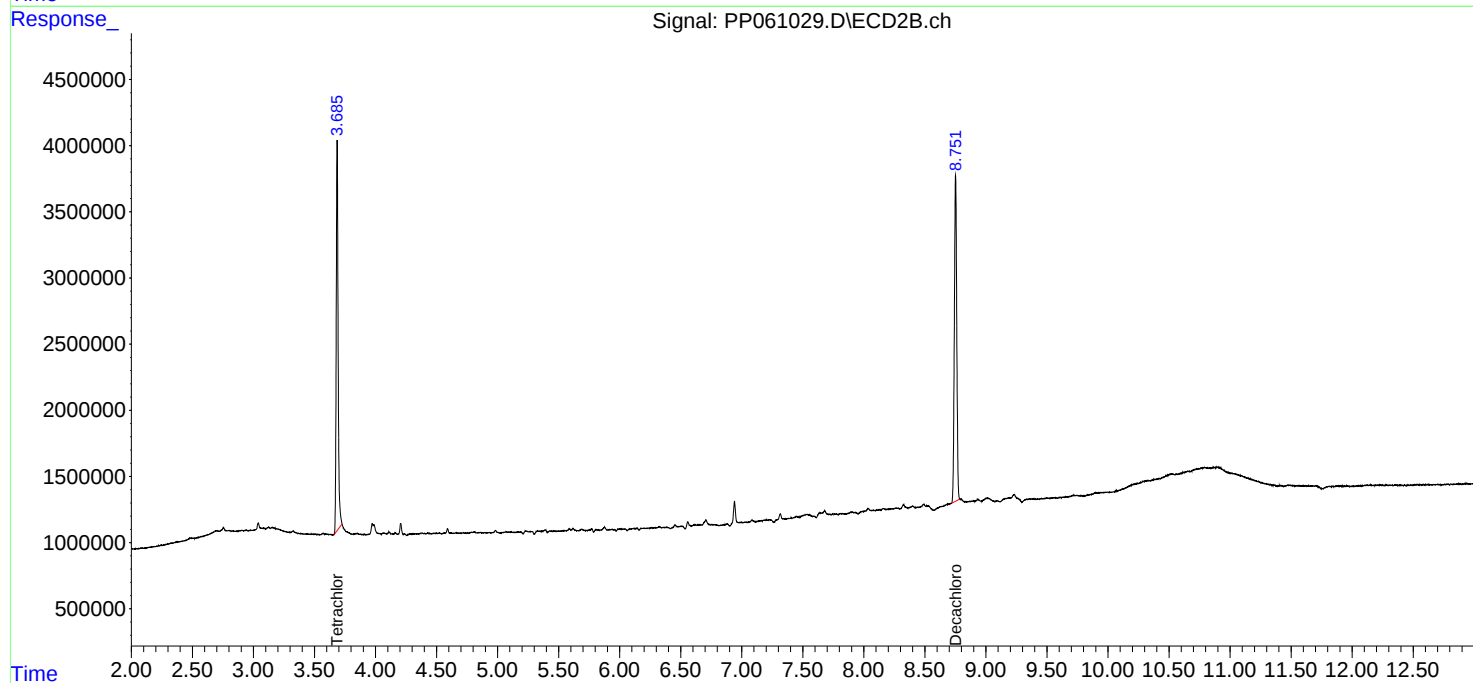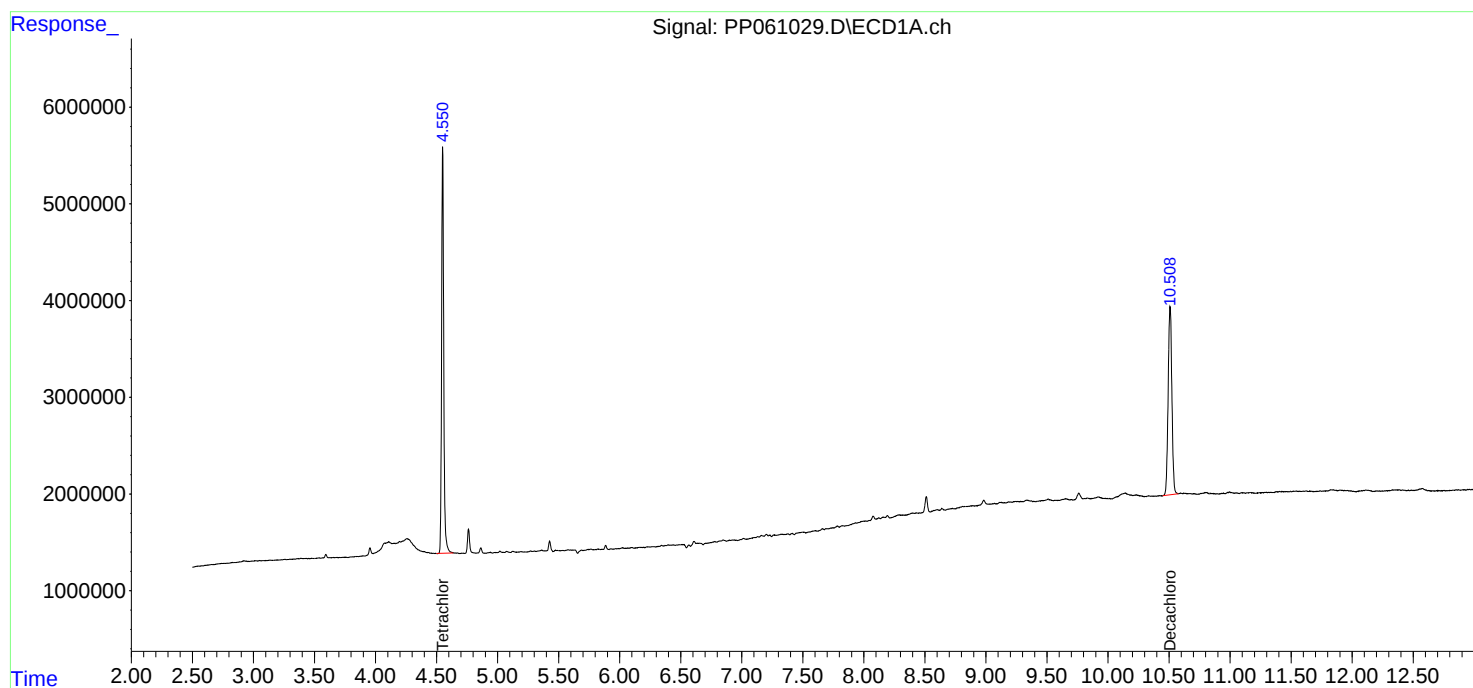


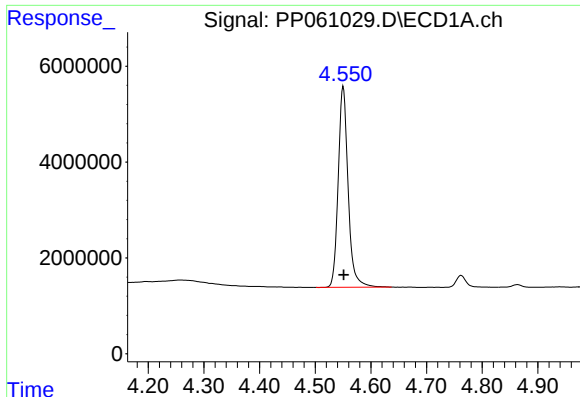

#1 Tetrachloro-m-xylene


R.T.: 4.550 min  
Delta R.T.: 0.000 min  
Response: 51813376  
Conc: 23.57 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
50129

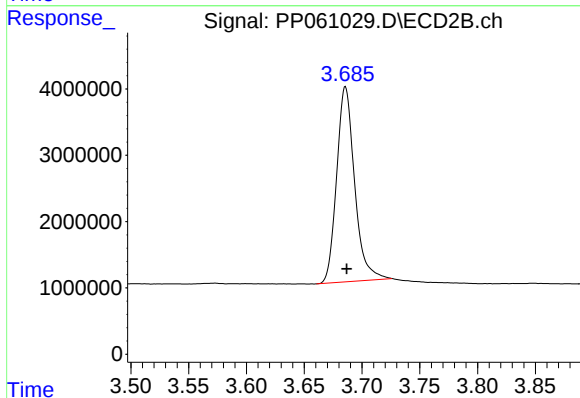


#1 Tetrachloro-m-xylene

R.T.: 3.686 min  
Delta R.T.: -0.001 min  
Response: 31808072  
Conc: 23.53 ng/ml

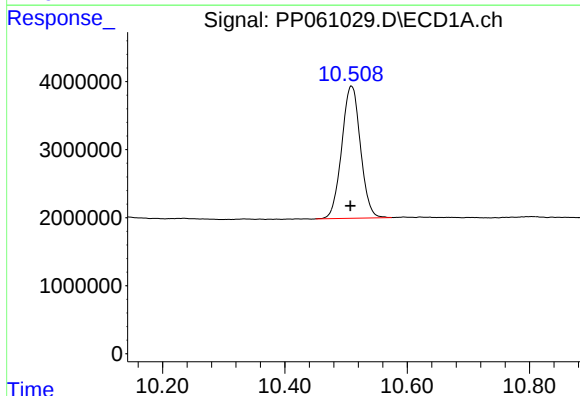

#2 Decachlorobiphenyl

R.T.: 10.509 min  
Delta R.T.: 0.002 min  
Response: 41247311  
Conc: 26.34 ng/ml

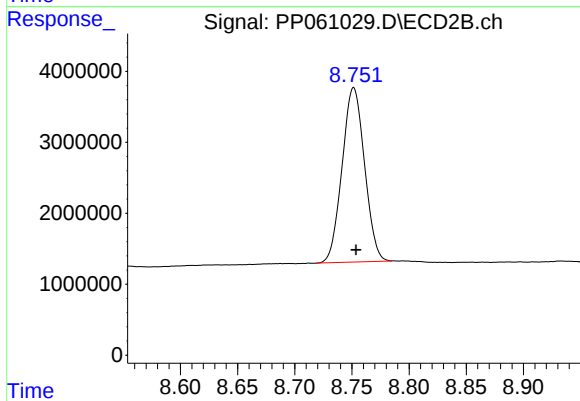

#2 Decachlorobiphenyl

R.T.: 8.752 min  
Delta R.T.: -0.002 min  
Response: 33561343  
Conc: 22.32 ng/ml